

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080721\
 Data File : BP006574.D
 Acq On : 07 Aug 2021 18:23
 Operator : CG/JU
 Sample : M3163-12
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGEZ0

Manual Integrations
 APPROVED

mohammad
 8/9/2021 12:16:45 PM

Quant Time: Aug 08 02:36:22 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 07 13:59:25 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.752	152	174913	20.000	ng/ul	0.00
20) Naphthalene-d8	10.534	136	732862	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.381	164	406246	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.134	188	807081	20.000	ng/ul	0.00
79) Chrysene-d12	21.227	240	838218	20.000	ng/ul	0.00
88) Perylene-d12	23.551	264	901957	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	17680	3.773	ng/uL	0.00
4) Pyridine-d5	3.681	84	137662	9.896	ng/ul	0.00
7) Phenol-d5	6.928	99	268648	16.353	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.093	67	185155	18.114	ng/ul	0.00
11) 2-Chlorophenol-d4	7.281	132	211371	17.319	ng/ul	0.00
15) 4-Methylphenol-d8	8.458	113	192723	14.918	ng/ul	0.00
21) Nitrobenzene-d5	8.905	128	104393	19.131	ng/ul	0.00
24) 2-Nitrophenol-d4	9.622	143	101657	19.511	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.157	165	158227	15.497	ng/ul	0.00
31) 4-Chloroaniline-d4	10.675	131	255298	15.188	ng/ul	0.00
46) Dimethylphthalate-d6	13.798	166	537283	18.582	ng/ul	0.00
49) Acenaphthylene-d8	14.069	160	647813	18.237	ng/ul	0.00
54) 4-Nitrophenol-d4	14.587	143	68268m	11.891	ng/ul	0.00
60) Fluorene-d10	15.375	176	440582	18.126	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.492	200	48866	10.861	ng/ul	0.00
73) Anthracene-d10	17.228	188	681541	18.707	ng/ul	0.00
81) Pyrene-d10	19.469	212	792193	18.375	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.398	264	802431	17.507	ng/ul	-0.01
Target Compounds						
					Qvalue	
8) Phenol	6.952	94	21083	1.256	ng/ul	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080721\
Data File : BP006574.D
Acq On : 07 Aug 2021 18:23
Operator : CG/JU
Sample : M3163-12
Misc :
ALS Vial : 16 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
BGEZ0

Manual Integrations
APPROVED

mohammad
8/9/2021 12:16:45 PM


Quant Time: Aug 08 02:36:22 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 07 13:59:25 2021
Response via : Initial Calibration

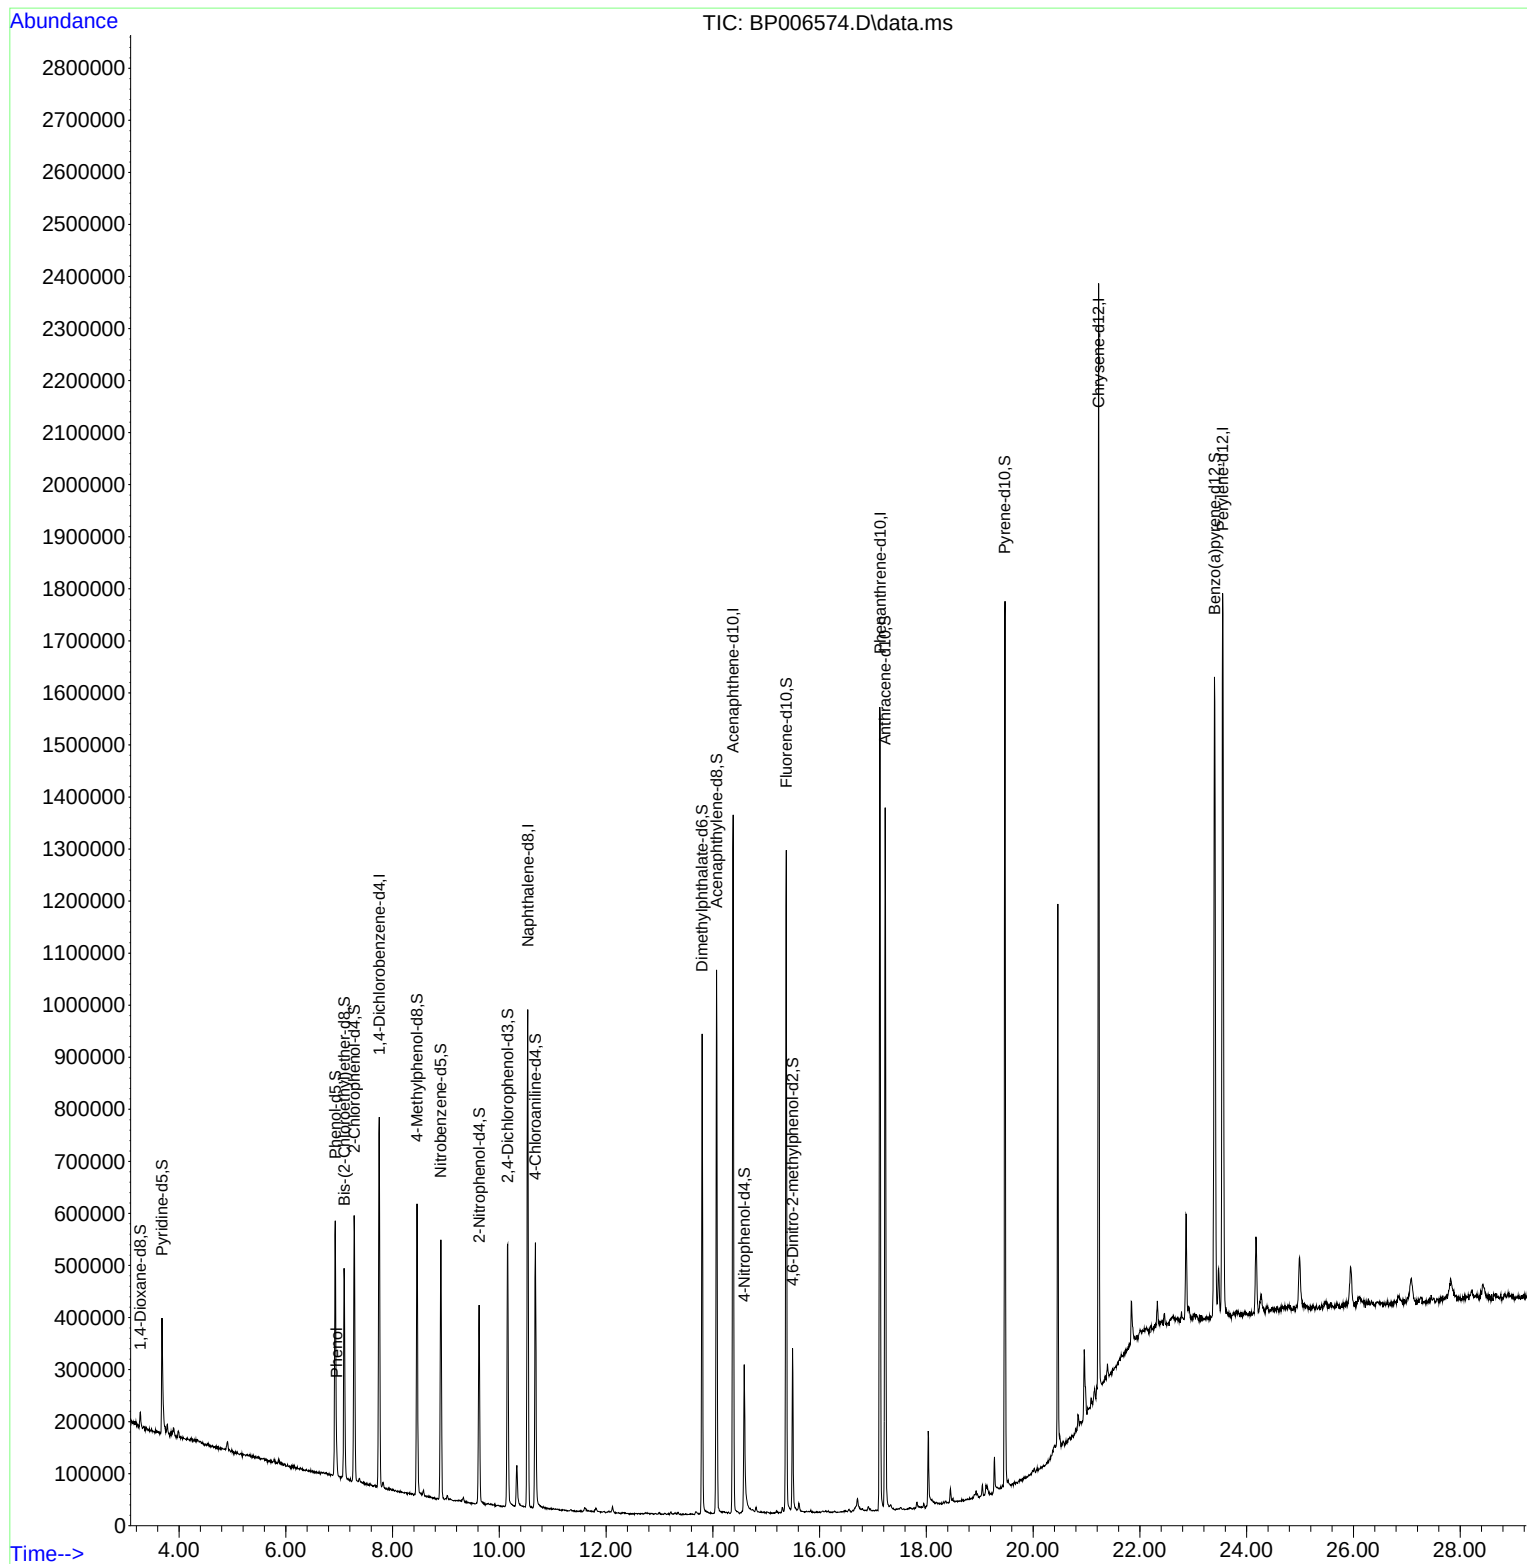

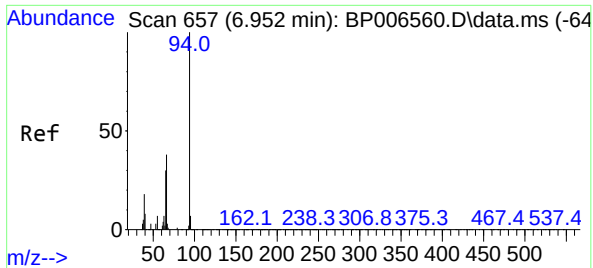

#8
Phenol
Concen: 1.256 ng/ul
RT: 6.952 min Scan# 657
Delta R.T. -0.000 min
Lab File: BP006574.D
Acq: 07 Aug 2021 18:23

Instrument :
BNA_P
ClientSampleId :
BGEZ0

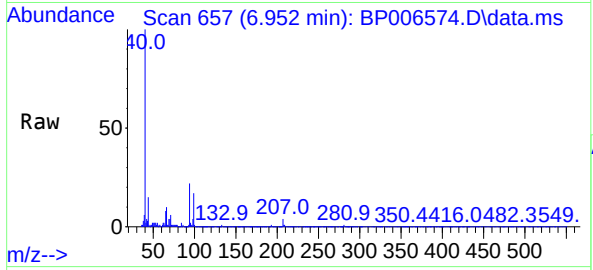

Tgt Ion: 94 Resp: 21083
Ion Ratio Lower Upper
94 100
65 35.1 23.8 35.8
66 45.7 30.9 46.3

Manual Integrations
APPROVED

mohammad
8/9/2021 12:16:45 PM

