

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080721\
 Data File : BP006582.D
 Acq On : 07 Aug 2021 23:30
 Operator : CG/JU
 Sample : M3163-16
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGEZ5

Quant Time: Aug 08 02:37:48 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 07 13:59:25 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.746	152	146905	20.000	ng/ul	0.00
20) Naphthalene-d8	10.528	136	641305	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.375	164	363538	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.128	188	735347	20.000	ng/ul	0.00
79) Chrysene-d12	21.227	240	733699	20.000	ng/ul	0.00
88) Perylene-d12	23.551	264	773266	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.269	96	22515	5.721	ng/uL	0.00
4) Pyridine-d5	3.675	84	314251	26.897	ng/ul	0.00
7) Phenol-d5	6.922	99	352159	25.524	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.093	67	241364	28.116	ng/ul	0.00
11) 2-Chlorophenol-d4	7.281	132	274705	26.799	ng/ul	0.00
15) 4-Methylphenol-d8	8.457	113	283167	26.098	ng/ul	0.00
21) Nitrobenzene-d5	8.904	128	136986	28.687	ng/ul	0.00
24) 2-Nitrophenol-d4	9.622	143	130978	28.727	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.151	165	216023	24.178	ng/ul	0.00
31) 4-Chloroaniline-d4	10.675	131	368595	25.059	ng/ul	0.00
46) Dimethylphthalate-d6	13.798	166	751598	29.049	ng/ul	0.00
49) Acenaphthylene-d8	14.069	160	912005	28.690	ng/ul	0.00
54) 4-Nitrophenol-d4	14.586	143	99909	19.447	ng/ul	0.00
60) Fluorene-d10	15.375	176	621301	28.564	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.492	200	70265	17.140	ng/ul	0.00
73) Anthracene-d10	17.228	188	976324	29.412	ng/ul	0.00
81) Pyrene-d10	19.469	212	1087370	28.814	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.398	264	1098849	27.964	ng/ul	-0.01
Target Compounds						
					Qvalue	
8) Phenol	6.952	94	31340	2.222	ng/ul#	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080721\
Data File : BP006582.D
Acq On : 07 Aug 2021 23:30
Operator : CG/JU
Sample : M3163-16
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGEZ5

Quant Time: Aug 08 02:37:48 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 07 13:59:25 2021
Response via : Initial Calibration

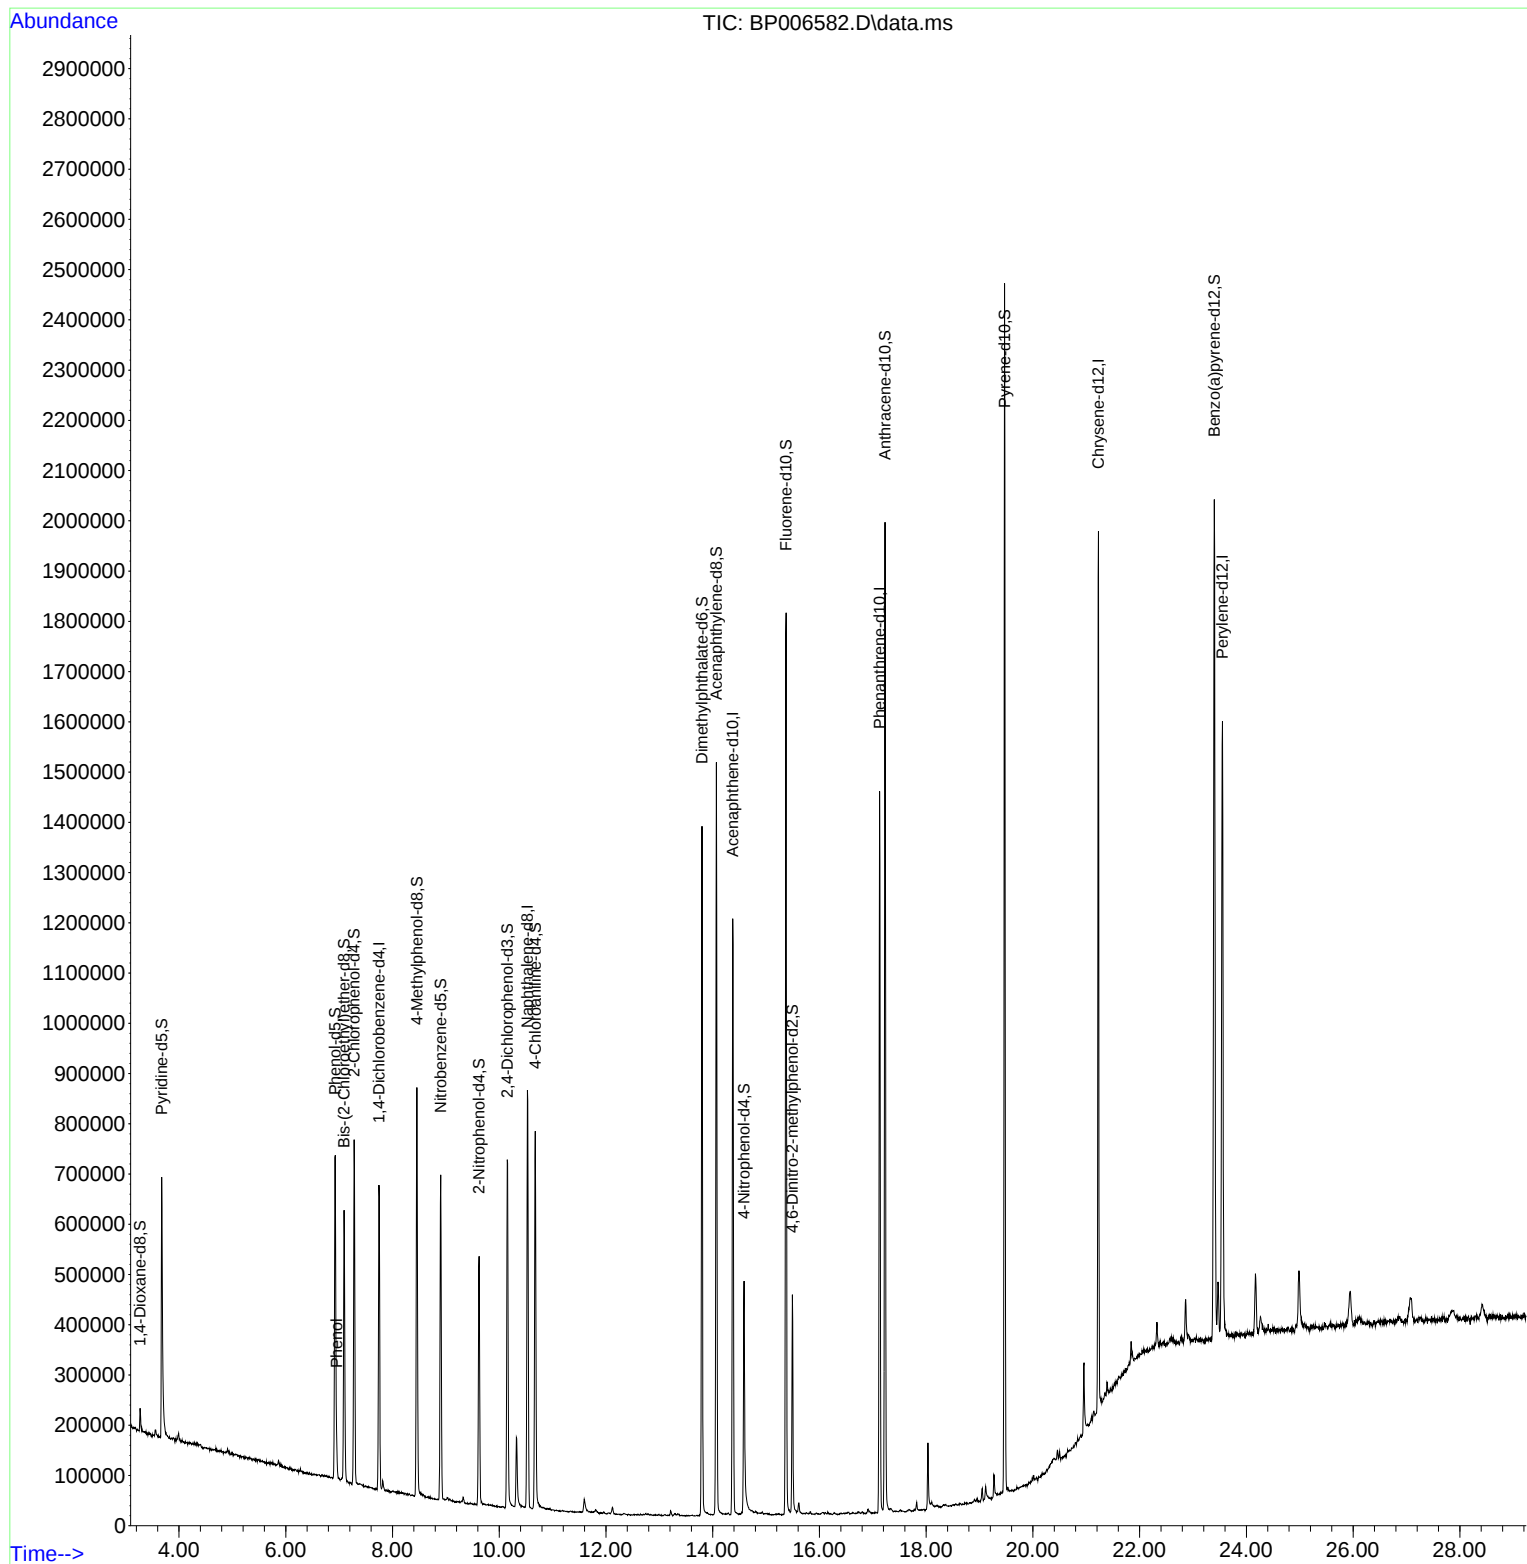

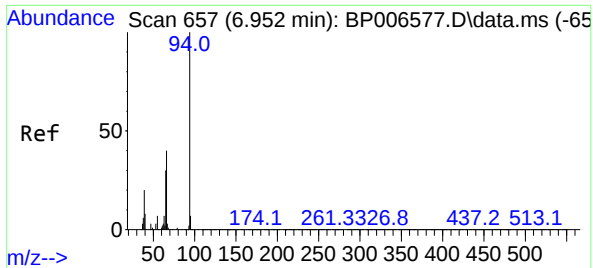

#8
Phenol
Concen: 2.222 ng/ul
RT: 6.952 min Scan# 657
Delta R.T. -0.000 min
Lab File: BP006582.D
Acq: 07 Aug 2021 23:30

Instrument :
BNA_P
ClientSampleId :
BGEZ5

Tgt Ion: 94 Resp: 31340

Ion	Ratio	Lower	Upper
94	100		
65	34.5	23.8	35.8
66	49.6	30.9	46.3

