

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080721\
 Data File : BP006583.D
 Acq On : 08 Aug 2021 00:04
 Operator : CG/JU
 Sample : M3163-08
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGEY6

Quant Time: Aug 08 02:37:59 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 07 13:59:25 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.752	152	163624	20.000	ng/ul	0.00
20) Naphthalene-d8	10.528	136	709574	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.375	164	403345	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.128	188	807775	20.000	ng/ul	0.00
79) Chrysene-d12	21.227	240	812780	20.000	ng/ul	0.00
88) Perylene-d12	23.551	264	870278	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.276	96	18268	4.167	ng/uL	0.00
4) Pyridine-d5	3.681	84	199928	15.364	ng/ul	0.00
7) Phenol-d5	6.922	99	313231	20.383	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.093	67	217913	22.790	ng/ul	0.00
11) 2-Chlorophenol-d4	7.281	132	248259	21.745	ng/ul	0.00
15) 4-Methylphenol-d8	8.458	113	243265	20.130	ng/ul	0.00
21) Nitrobenzene-d5	8.905	128	124567	23.577	ng/ul	0.00
24) 2-Nitrophenol-d4	9.622	143	117172	23.226	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.152	165	189140	19.133	ng/ul	0.00
31) 4-Chloroaniline-d4	10.675	131	308532	18.957	ng/ul	0.00
46) Dimethylphthalate-d6	13.798	166	678679	23.642	ng/ul	0.00
49) Acenaphthylene-d8	14.069	160	800160	22.687	ng/ul	0.00
54) 4-Nitrophenol-d4	14.587	143	98861	17.344	ng/ul	0.00
60) Fluorene-d10	15.375	176	562693	23.317	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.493	200	72168	16.026	ng/ul	0.00
73) Anthracene-d10	17.228	188	921065	25.259	ng/ul	0.00
81) Pyrene-d10	19.469	212	1052858	25.185	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.398	264	984141	22.253	ng/ul	-0.01
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.151	149	111273	3.240	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080721\
Data File : BP006583.D
Acq On : 08 Aug 2021 00:04
Operator : CG/JU
Sample : M3163-08
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGEY6

Quant Time: Aug 08 02:37:59 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 07 13:59:25 2021
Response via : Initial Calibration

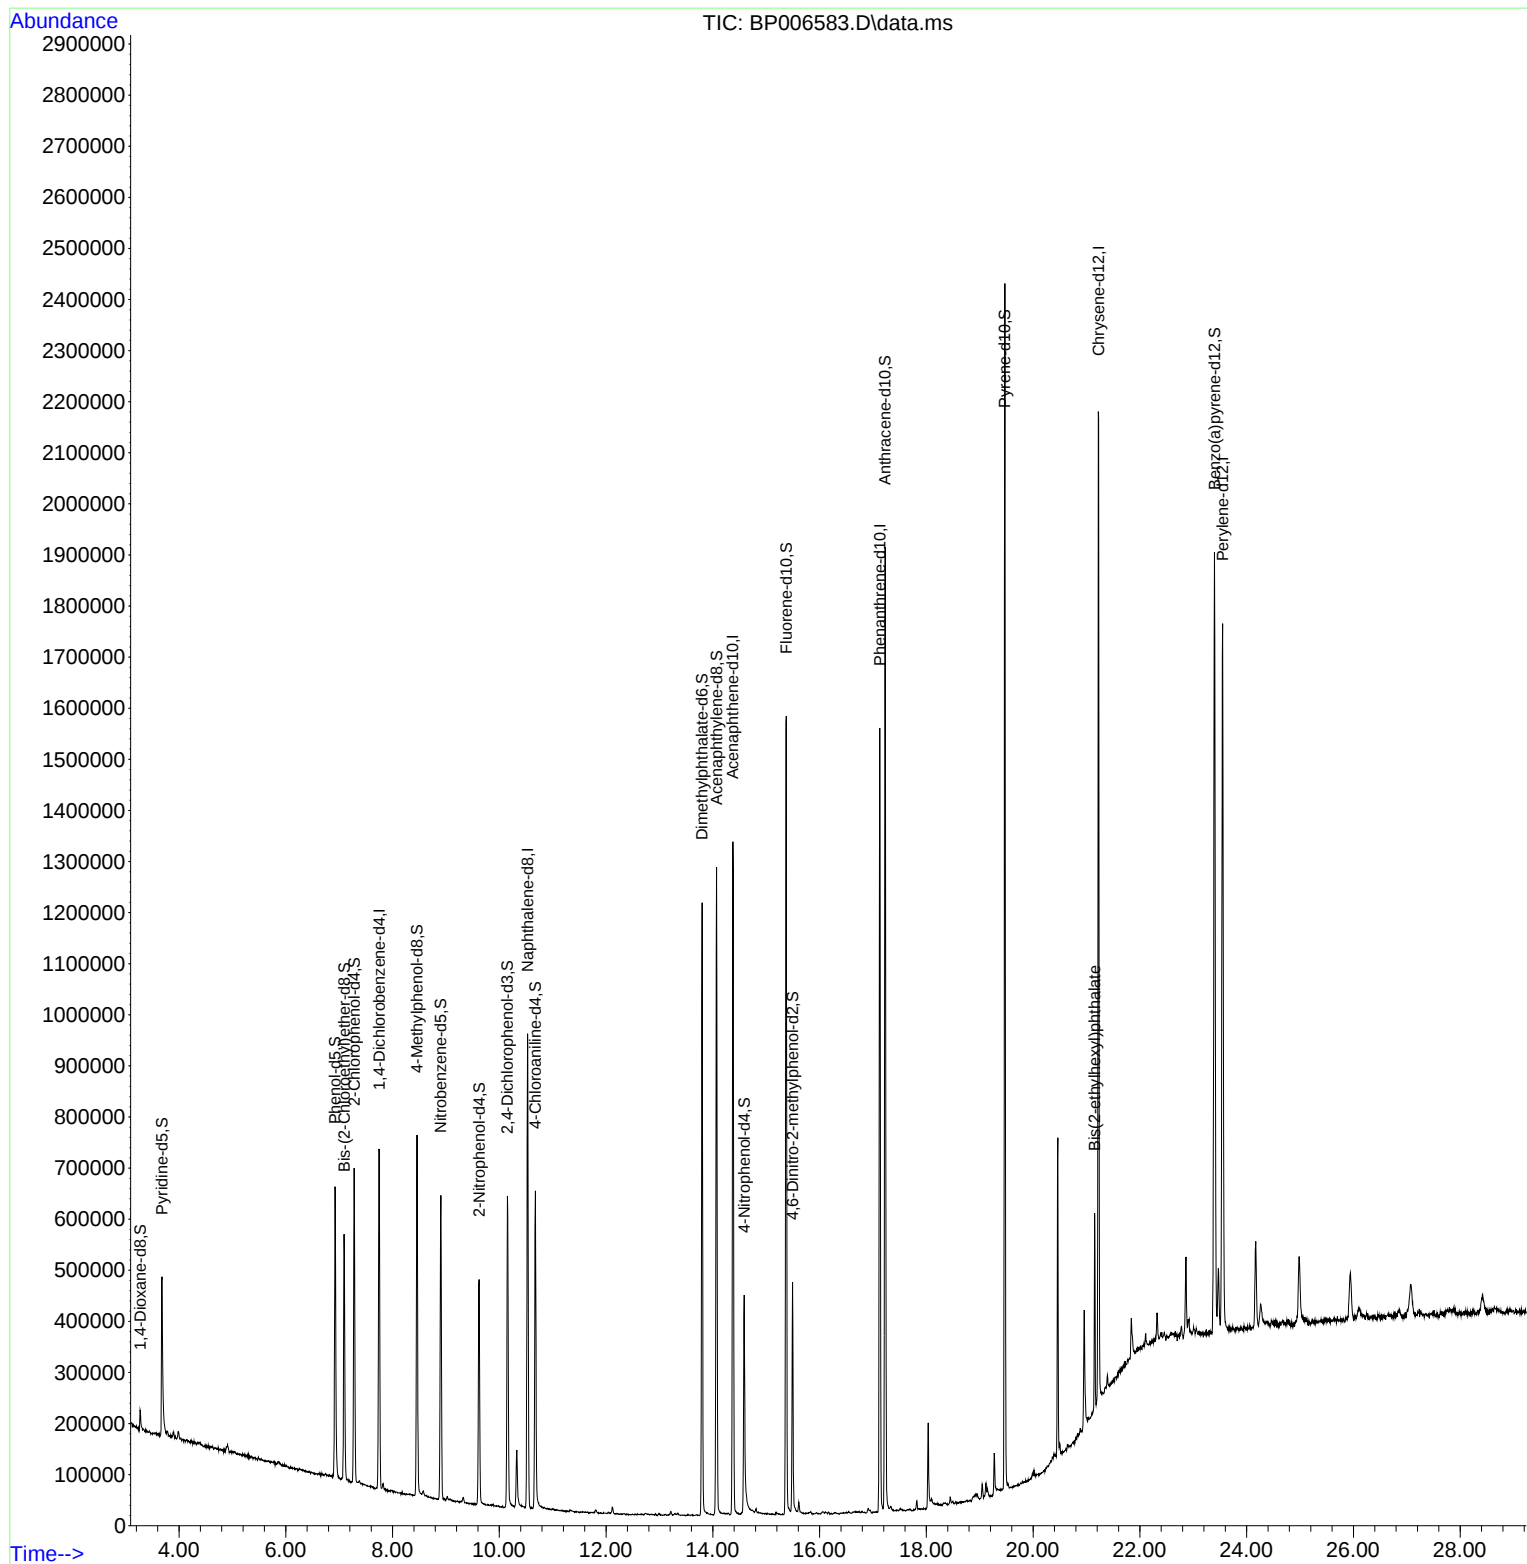

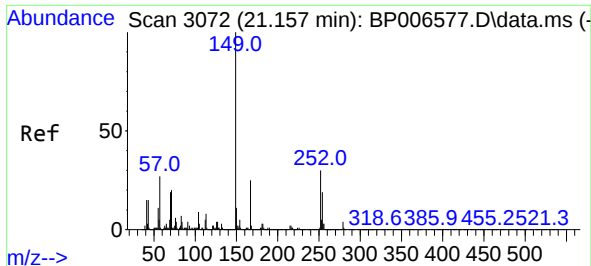

#86
Bis(2-ethylhexyl)phthalate
Concen: 3.240 ng/ul
RT: 21.151 min Scan# 3071
Delta R.T. -0.012 min
Lab File: BP006583.D
Acq: 08 Aug 2021 00:04

Instrument :
BNA_P
ClientSampleId :
BGEY6

Tgt Ion:149 Resp: 111273
Ion Ratio Lower Upper
149 100
167 24.9 19.6 29.4
279 3.7 3.0 4.4

