

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080721\
 Data File : BP006590.D
 Acq On : 08 Aug 2021 04:37
 Operator : CG/JU
 Sample : M3169-15
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C00B4

Quant Time: Aug 08 05:53:38 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Aug 08 03:08:02 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.752	152	207115	20.000	ng/ul	0.00
20) Naphthalene-d8	10.528	136	896060	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.375	164	498016	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.128	188	952527	20.000	ng/ul	0.00
79) Chrysene-d12	21.228	240	886508	20.000	ng/ul	0.00
88) Perylene-d12	23.545	264	915311	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.276	96	19572	3.527	ng/uL	0.00
4) Pyridine-d5	3.687	84	226855	13.772	ng/ul	0.01
7) Phenol-d5	6.928	99	522961	26.885	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.093	67	354248	29.269	ng/ul	0.00
11) 2-Chlorophenol-d4	7.281	132	414120	28.656	ng/ul	0.00
15) 4-Methylphenol-d8	8.458	113	365392	23.886	ng/ul	0.00
21) Nitrobenzene-d5	8.905	128	214786	32.192	ng/ul	0.00
24) 2-Nitrophenol-d4	9.622	143	220734	34.649	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.158	165	346074	27.722	ng/ul	0.00
31) 4-Chloroaniline-d4	10.675	131	476611	23.190	ng/ul	0.00
46) Dimethylphthalate-d6	13.799	166	1128290	31.832	ng/ul	0.00
49) Acenaphthylene-d8	14.069	160	1370382	31.469	ng/ul	0.00
54) 4-Nitrophenol-d4	14.587	143	168421	23.931	ng/ul	0.00
60) Fluorene-d10	15.375	176	924917	31.040	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.498	200	114663	21.593	ng/ul	0.00
73) Anthracene-d10	17.228	188	1402902	32.627	ng/ul	0.00
81) Pyrene-d10	19.469	212	1583706	34.732	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.404	264	1574649	33.854	ng/ul	0.00
Target Compounds						
					Qvalue	
80) Fluoranthene	19.145	202	58074	1.034	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080721\
Data File : BP006590.D
Acq On : 08 Aug 2021 04:37
Operator : CG/JU
Sample : M3169-15
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C00B4


Quant Time: Aug 08 05:53:38 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Aug 08 03:08:02 2021
Response via : Initial Calibration

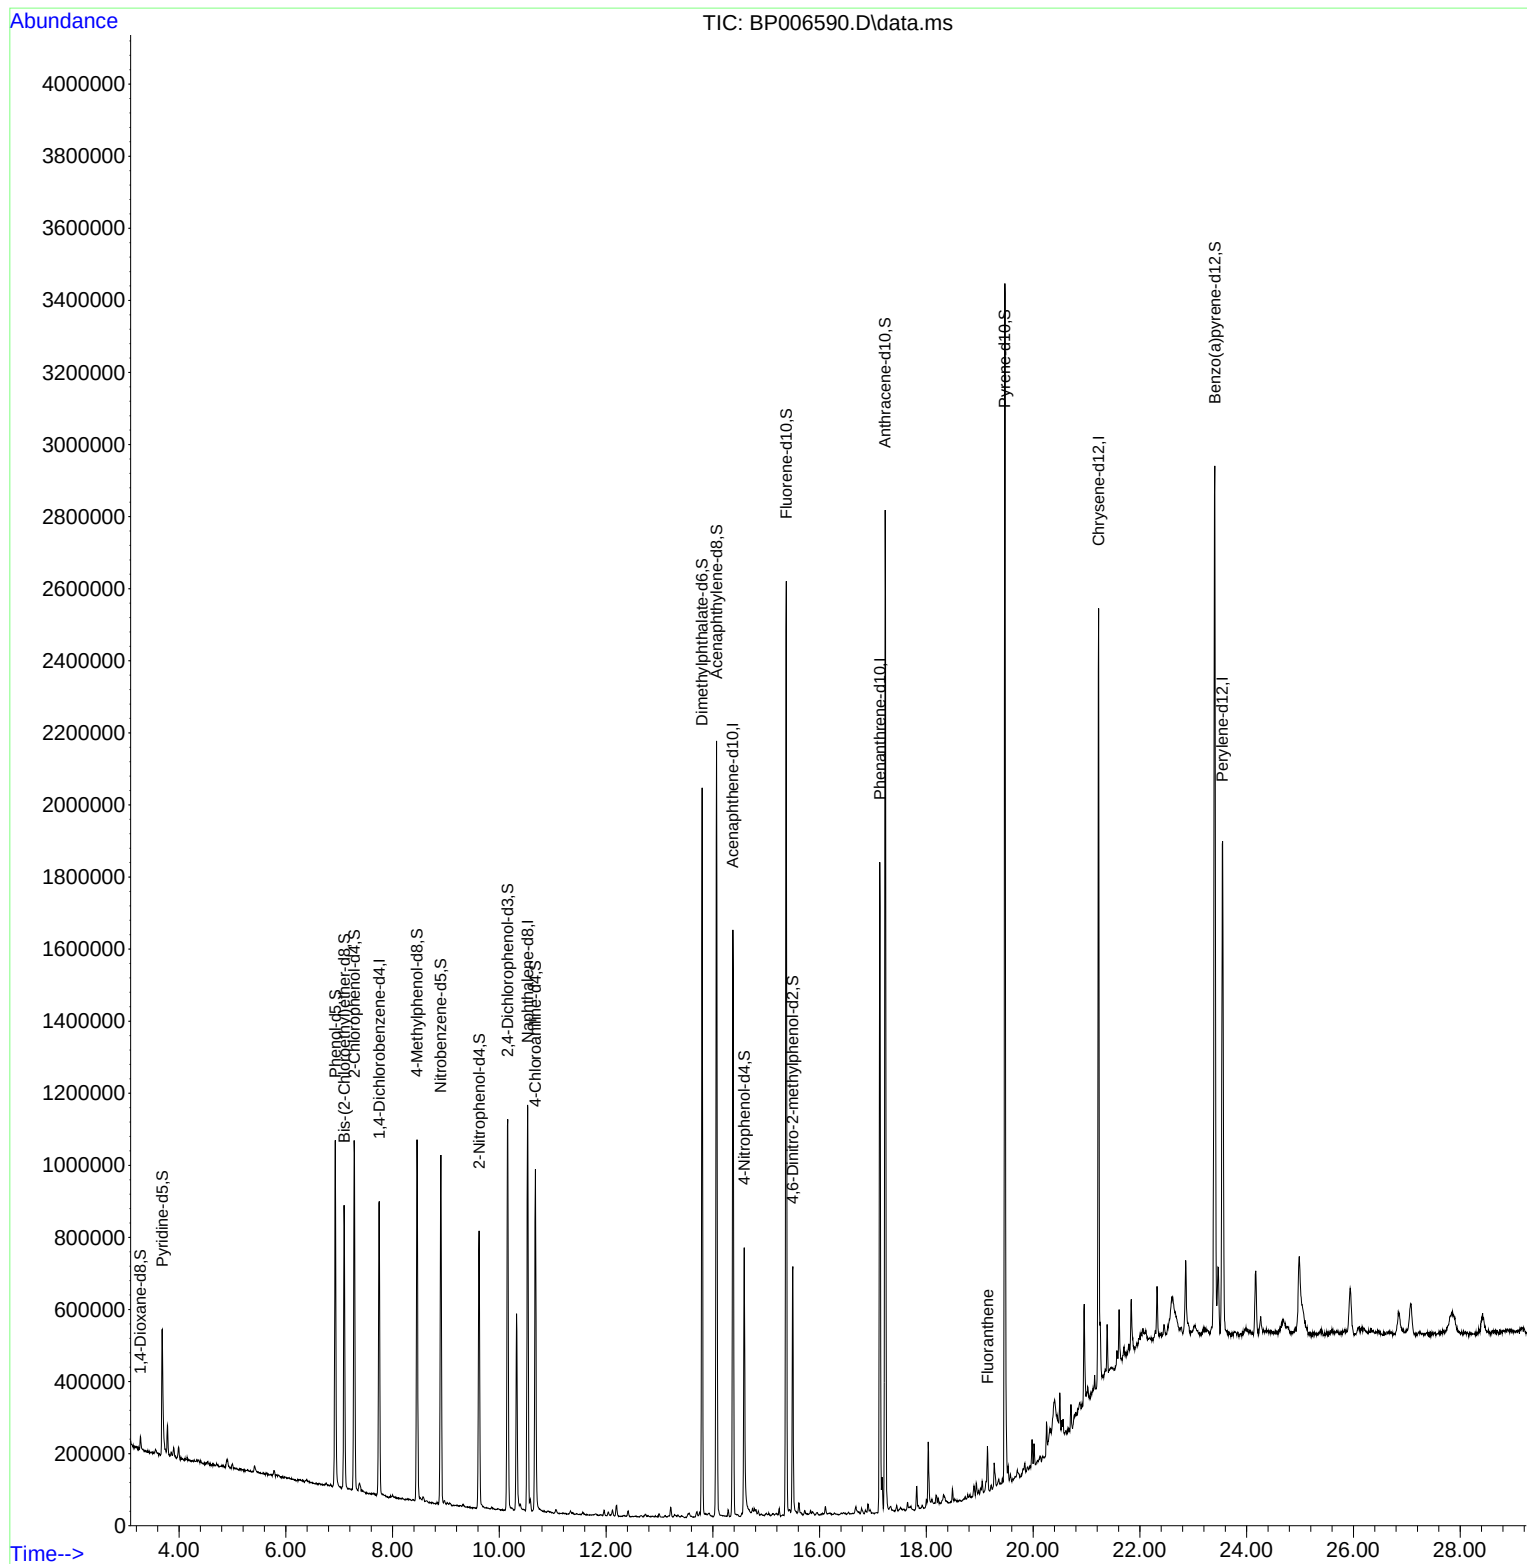

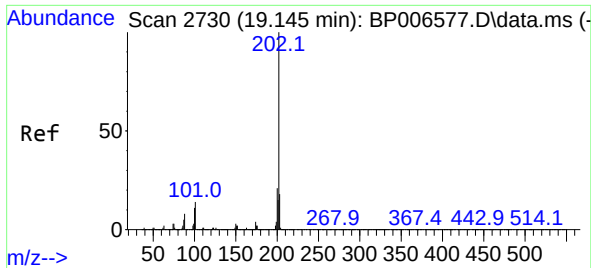

#80
Fluoranthene
Concen: 1.034 ng/ul
RT: 19.145 min Scan# 2730
Delta R.T. -0.006 min
Lab File: BP006590.D
Acq: 08 Aug 2021 04:37

Instrument :
BNA_P
ClientSampleId :
C00B4

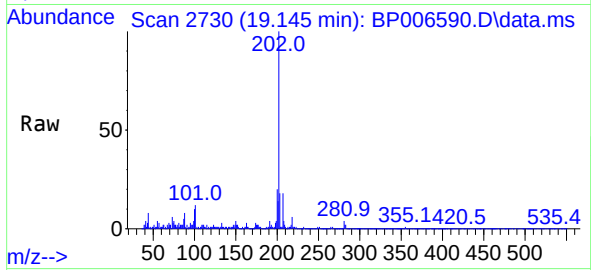

Tgt Ion:202 Resp: 58074
Ion Ratio Lower Upper
202 100
101 12.3 11.2 16.8
100 9.7 8.7 13.1

