

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080721\
 Data File : BP006578.D
 Acq On : 07 Aug 2021 21:13
 Operator : CG/JU
 Sample : PB138110BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK110

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Title : SVOA CALIBRATION

Signal : TIC: BP006578.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.276	28	32	40	rVB2	79805	114513	1.99%	0.181%
2	3.676	96	100	121	rBV	980483	1545966	26.93%	2.443%
3	6.928	647	653	663	rVB	1214166	1888397	32.89%	2.984%
4	7.093	676	681	691	rVB	944199	1491261	25.97%	2.356%
5	7.281	707	713	724	rVB	1260473	1956861	34.08%	3.092%
6	7.752	786	793	802	rVB	779337	1233800	21.49%	1.949%
7	8.458	906	913	928	rBV	1493655	2317123	40.36%	3.661%
8	8.905	982	989	998	rVB	1211219	1916917	33.39%	3.029%
9	9.622	1103	1111	1125	rBV	948791	1563105	27.23%	2.470%
10	10.152	1194	1201	1215	rBV	1328420	2224327	38.74%	3.514%
11	10.528	1258	1265	1274	rBV	1068995	1791722	31.21%	2.831%
12	10.675	1282	1290	1306	rBV	1414886	2415844	42.08%	3.817%
13	11.810	1476	1483	1491	rVB4	6043	16237	0.28%	0.026%
14	12.122	1530	1536	1543	rVB	25085	44819	0.78%	0.071%
15	12.334	1567	1572	1577	rVB9	4087	7664	0.13%	0.012%
16	13.346	1740	1744	1747	rBV5	5461	9216	0.16%	0.015%
17	13.799	1814	1821	1834	rBV	2576741	3418159	59.54%	5.400%
18	14.069	1859	1867	1876	rBV	2802836	3964696	69.06%	6.264%
19	14.375	1912	1919	1931	rBV	1570942	2262828	39.41%	3.575%
20	14.587	1948	1955	1975	rBV	1055482	1866655	32.51%	2.949%
21	15.375	2081	2089	2102	rBV	3216292	4713787	82.10%	7.447%
22	15.493	2102	2109	2122	rVV	1086879	1507150	26.25%	2.381%
23	15.610	2125	2129	2135	rVB	41796	65541	1.14%	0.104%
24	15.945	2182	2186	2191	rVB7	3571	5833	0.10%	0.009%
25	16.051	2198	2204	2212	rBV7	6685	16466	0.29%	0.026%
26	16.163	2217	2223	2228	rVB6	8160	13512	0.24%	0.021%
27	16.440	2264	2270	2275	rBV6	11011	19965	0.35%	0.032%
28	16.716	2311	2317	2320	rBV3	5171	8662	0.15%	0.014%
29	16.810	2329	2333	2337	rVB7	6531	8956	0.16%	0.014%
30	16.910	2346	2350	2356	rBV5	12129	20253	0.35%	0.032%
31	17.128	2379	2387	2397	rBV	1815032	2579940	44.94%	4.076%
32	17.228	2397	2404	2423	rVB2	3720752	5167146	90.00%	8.164%
33	17.510	2449	2452	2457	rVB5	5221	7082	0.12%	0.011%
34	17.810	2498	2503	2505	rBV5	6567	10490	0.18%	0.017%
35	18.034	2535	2541	2550	rBV4	36145	67774	1.18%	0.107%
36	18.322	2587	2590	2593	rBV4	8016	9463	0.16%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080721\
 Data File : BP006578.D
 Acq On : 07 Aug 2021 21:13
 Operator : CG/JU
 Sample : PB138110BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK110

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Title : SVOA CALIBRATION

37	18.775	2663	2667	2671	rBV6	9394	12655	0.22%	0.020%
38	19.045	2709	2713	2719	rBV4	24632	36486	0.64%	0.058%
39	19.116	2720	2725	2729	rBV	43816	60419	1.05%	0.095%
40	19.275	2749	2752	2755	rBV4	13214	15409	0.27%	0.024%
41	19.363	2764	2767	2770	rVB2	16410	18638	0.32%	0.029%
42	19.469	2779	2785	2793	rBV	4324381	5671701	98.79%	8.961%
43	21.228	3079	3084	3092	rBV	2146630	2702419	47.07%	4.270%
44	23.404	3446	3454	3462	rBV2	3076866	5741170	100.00%	9.071%
45	23.551	3472	3479	3489	rVB2	1450184	2762638	48.12%	4.365%


Sum of corrected areas: 63293665

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080721\
Data File : BP006578.D
Acq On : 07 Aug 2021 21:13
Operator : CG/JU
Sample : PB138110BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK110

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

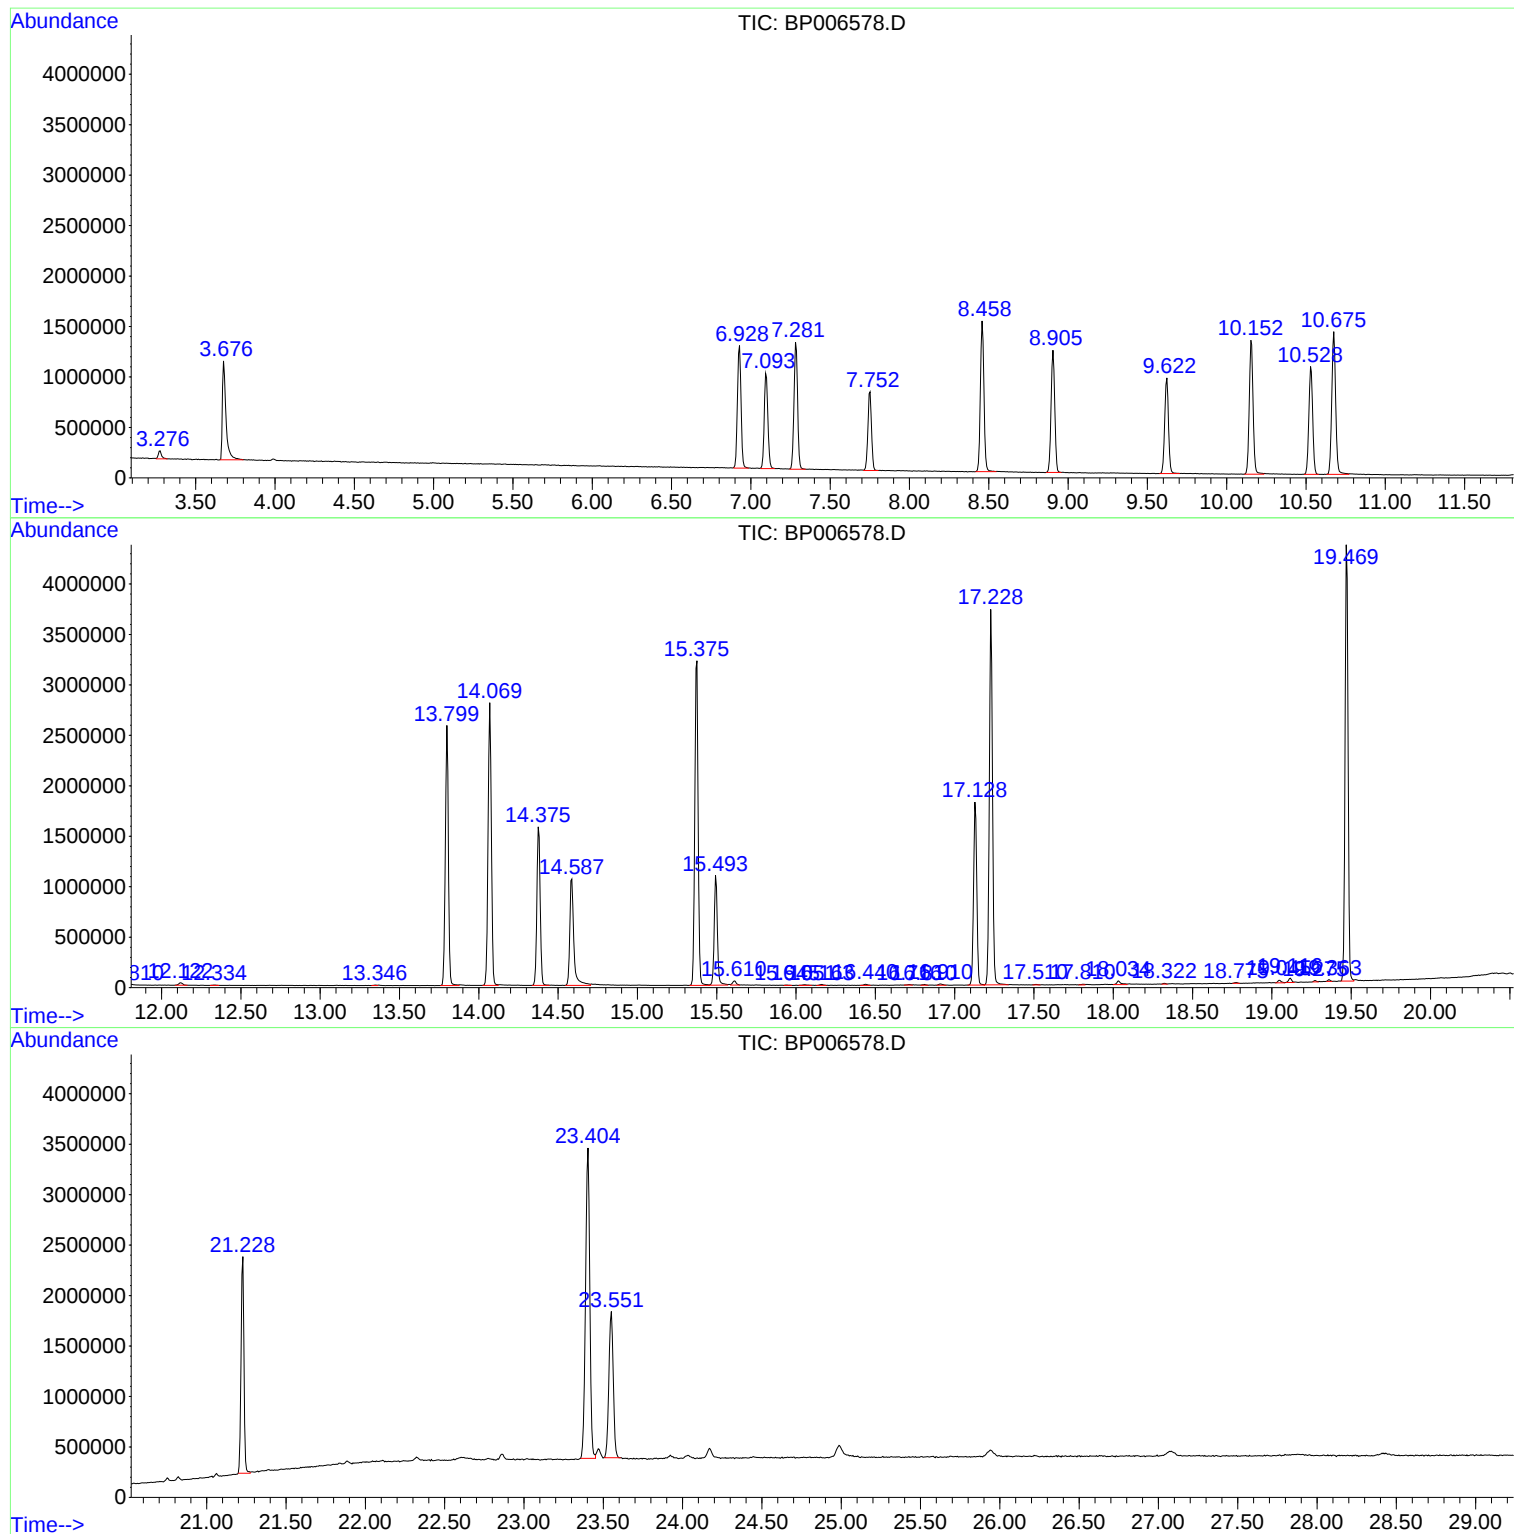

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080721\
Data File : BP006578.D
Acq On : 07 Aug 2021 21:13
Operator : CG/JU
Sample : PB138110BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK110

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080721\
Data File : BP006578.D
Acq On : 07 Aug 2021 21:13
Operator : CG/JU
Sample : PB138110BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK110

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
