

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080721\
 Data File : BP006581.D
 Acq On : 07 Aug 2021 22:56
 Operator : CG/JU
 Sample : M3163-14
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGEZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Title : SVOA CALIBRATION

Signal : TIC: BP006581.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.681	98	101	114	rBV	184730	311538	10.71%	1.001%
2	6.922	647	652	663	rVB	385685	642506	22.08%	2.064%
3	7.093	676	681	692	rVB	333699	526874	18.11%	1.693%
4	7.281	707	713	722	rVB	422950	642248	22.07%	2.063%
5	7.746	786	792	802	rVB	765411	1220892	41.96%	3.922%
6	8.458	907	913	920	rBV	402286	626950	21.55%	2.014%
7	8.905	982	989	996	rBV	415422	660528	22.70%	2.122%
8	9.322	1058	1060	1065	rVB2	9541	10899	0.37%	0.035%
9	9.622	1104	1111	1121	rBV	300640	496120	17.05%	1.594%
10	10.152	1195	1201	1209	rBV	404283	678757	23.33%	2.181%
11	10.328	1226	1231	1239	rBV	60204	101060	3.47%	0.325%
12	10.528	1258	1265	1276	rVB	1033288	1758499	60.43%	5.649%
13	10.675	1282	1290	1304	rBV	409627	733777	25.22%	2.357%
14	11.434	1416	1419	1425	rVB8	1742	3028	0.10%	0.010%
15	11.610	1443	1449	1458	rBV6	6381	15655	0.54%	0.050%
16	11.816	1476	1484	1488	rVB7	4677	11342	0.39%	0.036%
17	12.122	1531	1536	1540	rBV4	9365	15188	0.52%	0.049%
18	12.328	1568	1571	1574	rBV5	2517	3261	0.11%	0.010%
19	12.734	1639	1640	1644	rBV4	2266	3026	0.10%	0.010%
20	12.987	1680	1683	1688	rVB6	3476	5020	0.17%	0.016%
21	13.104	1699	1703	1710	rVB9	3725	5805	0.20%	0.019%
22	13.216	1715	1722	1726	rBV9	6397	11982	0.41%	0.038%
23	13.293	1731	1735	1737	rVV5	3501	4808	0.17%	0.015%
24	13.346	1740	1744	1752	rVB5	3856	6028	0.21%	0.019%
25	13.798	1815	1821	1837	rBV	829951	1166875	40.10%	3.749%
26	14.069	1858	1867	1879	rBV	910495	1302481	44.76%	4.184%
27	14.287	1900	1904	1907	rVB6	2929	3200	0.11%	0.010%
28	14.375	1909	1919	1933	rBV	1459477	2241330	77.03%	7.201%
29	14.540	1944	1947	1949	rBV4	3385	3685	0.13%	0.012%
30	14.587	1949	1955	1978	rVV	204821	435955	14.98%	1.401%
31	14.740	1978	1981	1982	rBV3	3720	3322	0.11%	0.011%
32	14.804	1988	1992	1998	rVB7	8767	14490	0.50%	0.047%
33	15.245	2065	2067	2072	rVB6	3167	3509	0.12%	0.011%
34	15.369	2082	2088	2104	rBV	1079188	1625497	55.86%	5.222%
35	15.492	2104	2109	2123	rVV	236169	354565	12.19%	1.139%
36	15.610	2126	2129	2135	rVB	14590	19554	0.67%	0.063%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080721\
 Data File : BP006581.D
 Acq On : 07 Aug 2021 22:56
 Operator : CG/JU
 Sample : M3163-14
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGEZ3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Title : SVOA CALIBRATION

37	15.934	2181	2184	2188	rVB6	2158	3209	0.11%	0.010%
38	16.051	2199	2204	2205	rBV5	2977	4372	0.15%	0.014%
39	16.110	2212	2214	2219	rVB6	3177	4284	0.15%	0.014%
40	16.475	2273	2276	2279	rVB5	2420	3075	0.11%	0.010%
41	16.622	2297	2301	2306	rBV8	2610	5283	0.18%	0.017%
42	16.681	2306	2311	2316	rBV5	10921	16936	0.58%	0.054%
43	16.804	2331	2332	2337	rVB5	2704	3290	0.11%	0.011%
44	16.910	2345	2350	2353	rBV3	9529	14741	0.51%	0.047%
45	17.128	2380	2387	2398	rBV	1839923	2567494	88.24%	8.248%
46	17.228	2398	2404	2418	rVV	1201846	1707277	58.67%	5.485%
47	17.328	2418	2421	2425	rVB6	4868	9227	0.32%	0.030%
48	17.686	2478	2482	2485	rBV6	3606	5951	0.20%	0.019%
49	17.816	2501	2504	2508	rBV5	8656	13328	0.46%	0.043%
50	18.034	2536	2541	2548	rBV	113036	165544	5.69%	0.532%
51	18.445	2608	2611	2616	rBV	18639	27341	0.94%	0.088%
52	18.481	2616	2617	2623	rVB6	5555	6785	0.23%	0.022%
53	18.933	2689	2694	2695	rBV5	6650	8956	0.31%	0.029%
54	19.045	2709	2713	2717	rBV4	17566	26095	0.90%	0.084%
55	19.116	2721	2725	2728	rBV2	16324	27972	0.96%	0.090%
56	19.269	2747	2751	2757	rBV	50627	73750	2.53%	0.237%
57	19.469	2779	2785	2792	rBV	1485757	1961034	67.40%	6.300%
58	20.457	2949	2953	2958	rBV	753372	819859	28.18%	2.634%
59	20.957	3034	3038	3045	rBV4	74571	151807	5.22%	0.488%
60	21.222	3078	3083	3093	rBV	2128590	2776084	95.41%	8.919%
61	23.392	3446	3452	3460	rBV2	1007993	1875754	64.46%	6.026%
62	23.545	3471	3478	3489	rVB2	1481349	2909751	100.00%	9.348%
63	24.168	3581	3584	3591	rVB2	154113	267452	9.19%	0.859%




Sum of corrected areas: 31126905

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080721\
Data File : BP006581.D
Acq On : 07 Aug 2021 22:56
Operator : CG/JU
Sample : M3163-14
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGEZ3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

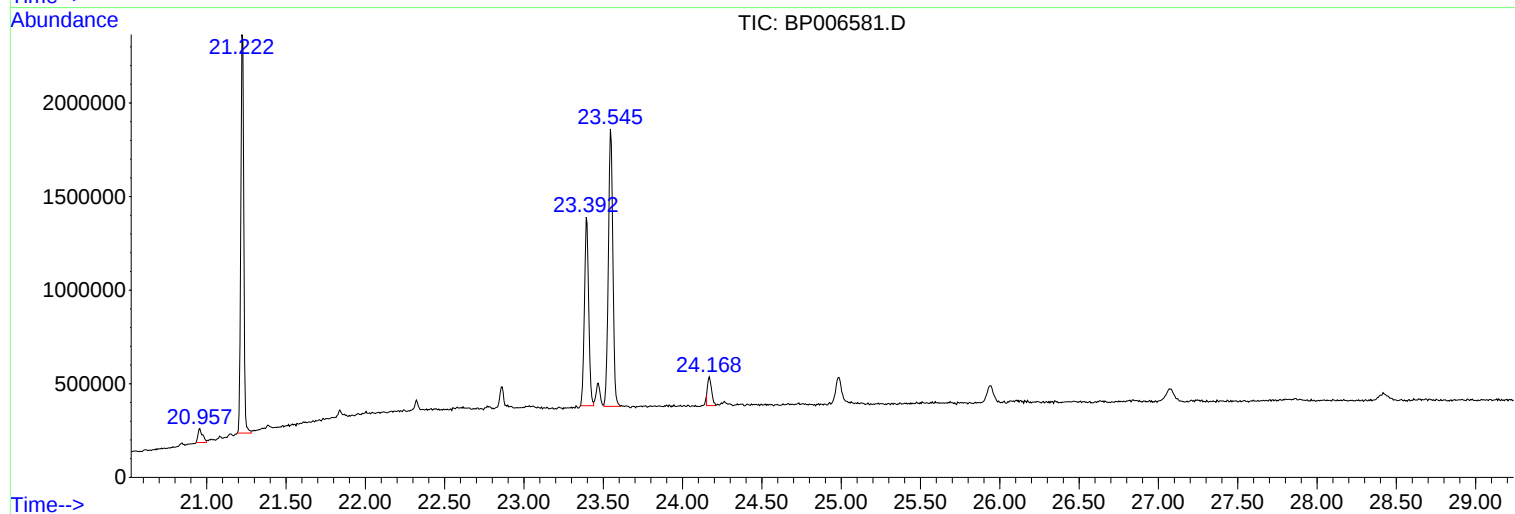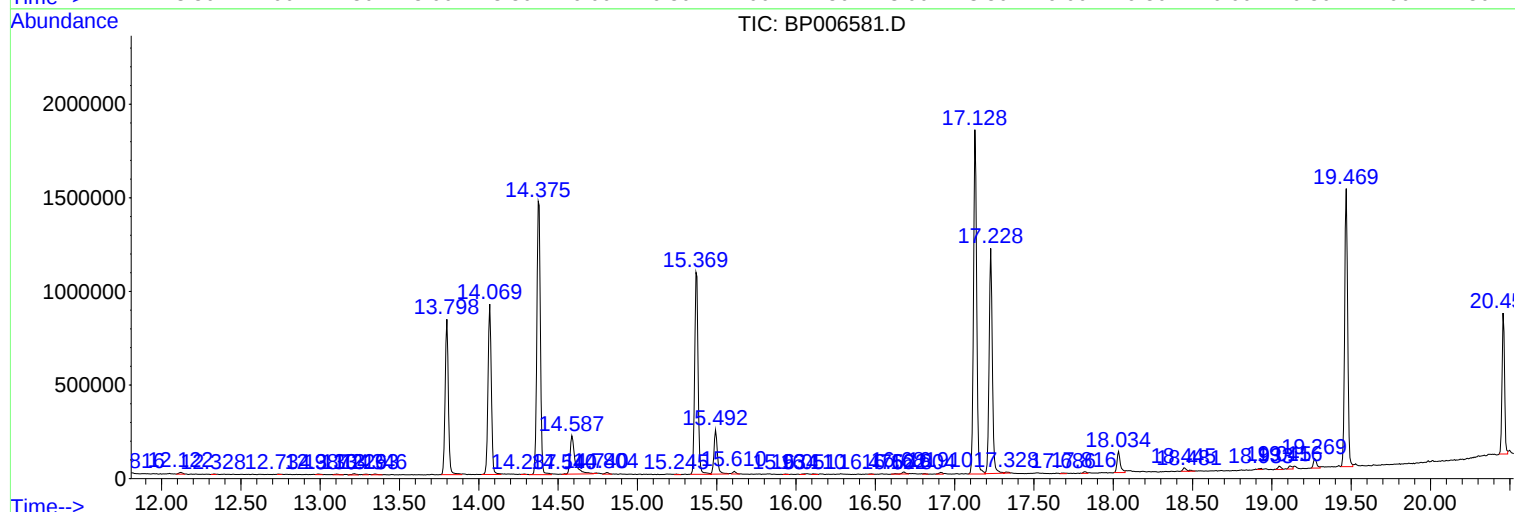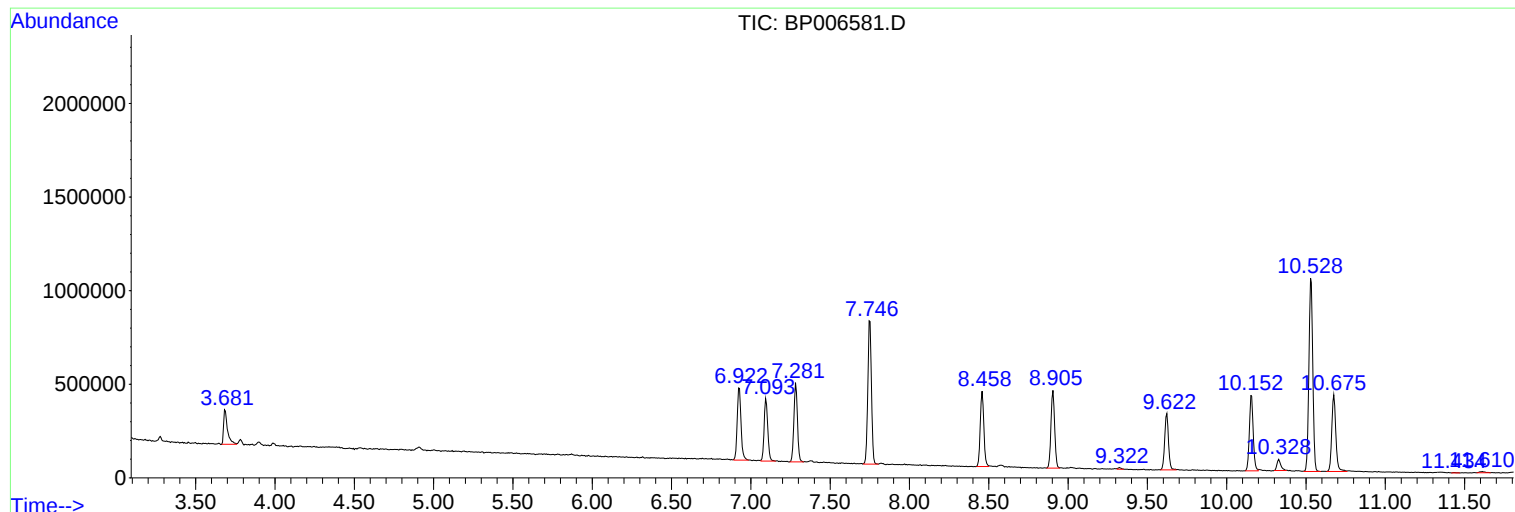

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080721\
Data File : BP006581.D
Acq On : 07 Aug 2021 22:56
Operator : CG/JU
Sample : M3163-14
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGEZ3










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Hexanedioic acid, dioctyl e... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.460	5.91 ng/ul	819859	Chrysene-d12	21.227

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Hexanedioic acid, dioctyl ester	370	C22H42O4	000123-79-5	96
2			Diisooctyl adipate	370	C22H42O4	001330-86-5	94
3			Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	92
4			Hexanedioic acid, dioctyl ester	370	C22H42O4	000123-79-5	90
5			Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	90

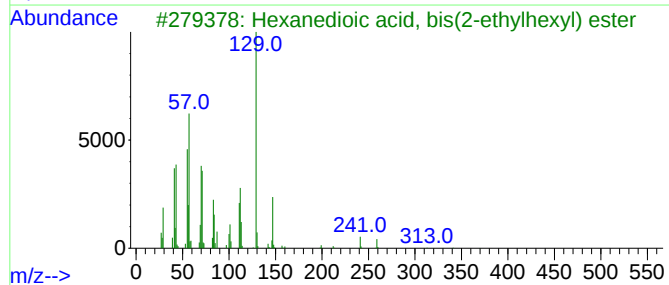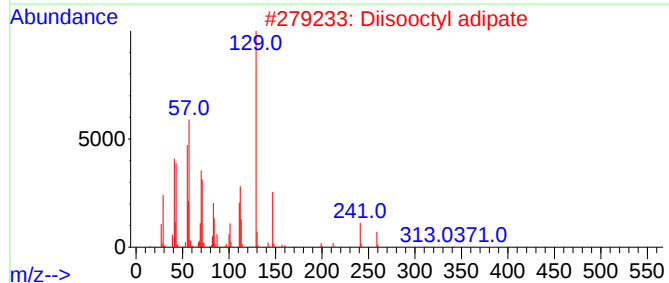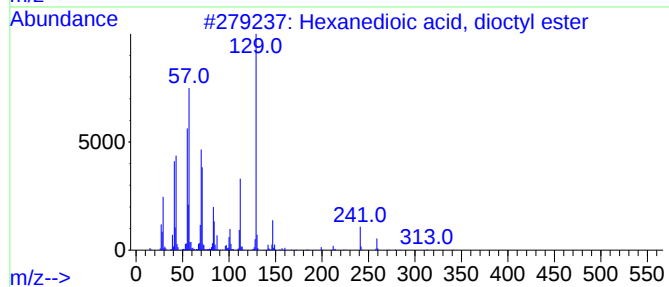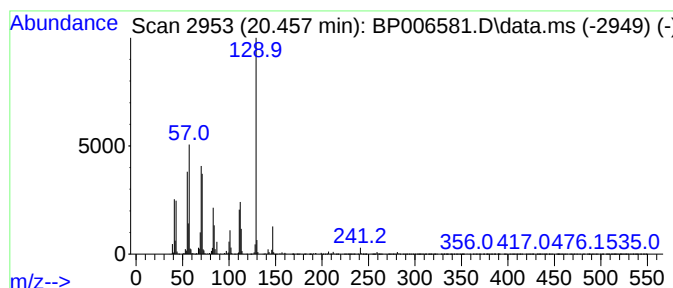

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080721\
Data File : BP006581.D
Acq On : 07 Aug 2021 22:56
Operator : CG/JU
Sample : M3163-14
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGEZ3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Hexanedioic aci...	20.460	5.9	ng/ul	819859	5	21.227	2776080	20.0