

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080721\
 Data File : BP006590.D
 Acq On : 08 Aug 2021 04:37
 Operator : CG/JU
 Sample : M3169-15
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C00B4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Title : SVOA CALIBRATION

Signal : TIC: BP006591.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.687	98	102	114	rBV	347660	603585	12.82%	1.081%
2	3.781	115	118	126	rVB	87038	124396	2.64%	0.223%
3	6.928	647	653	666	rVB	961975	1519024	32.26%	2.721%
4	7.093	676	681	692	rVB	787419	1214529	25.80%	2.175%
5	7.281	707	713	725	rVB	971477	1535980	32.62%	2.751%
6	7.752	786	793	802	rVB	814128	1305056	27.72%	2.338%
7	8.458	907	913	921	rBV	999853	1596436	33.91%	2.859%
8	8.905	982	989	997	rBV	967831	1551473	32.95%	2.779%
9	9.622	1104	1111	1123	rBV	767928	1276542	27.11%	2.286%
10	10.158	1194	1202	1213	rBV	1084368	1808107	38.40%	3.239%
11	10.322	1224	1230	1239	rBV	544533	881554	18.72%	1.579%
12	10.528	1258	1265	1271	rBV	1126958	1937848	41.16%	3.471%
13	10.581	1271	1274	1279	rVB	34271	50945	1.08%	0.091%
14	10.675	1283	1290	1306	rVV	945930	1606131	34.11%	2.877%
15	11.057	1349	1355	1363	rBV5	11356	22844	0.49%	0.041%
16	11.334	1397	1402	1406	rBV7	8795	14258	0.30%	0.026%
17	11.805	1477	1482	1486	rVB6	3490	7276	0.15%	0.013%
18	11.963	1505	1509	1517	rVB3	15508	22347	0.47%	0.040%
19	12.040	1518	1522	1528	rVV2	10611	18508	0.39%	0.033%
20	12.122	1530	1536	1542	rVB2	16937	29638	0.63%	0.053%
21	12.199	1542	1549	1554	rBV	30237	50608	1.07%	0.091%
22	12.416	1580	1586	1594	rVB2	16618	29680	0.63%	0.053%
23	12.657	1622	1627	1632	rBV9	4437	10731	0.23%	0.019%
24	12.734	1635	1640	1645	rVV7	7772	16512	0.35%	0.030%
25	12.869	1661	1663	1668	rVB6	2821	4952	0.11%	0.009%
26	12.993	1681	1684	1690	rVB3	9425	13750	0.29%	0.025%
27	13.110	1697	1704	1706	rBV7	5312	8879	0.19%	0.016%
28	13.169	1708	1714	1715	rVV6	3649	5785	0.12%	0.010%
29	13.210	1717	1721	1728	rVB4	27580	44111	0.94%	0.079%
30	13.281	1728	1733	1739	rBV7	7365	15846	0.34%	0.028%
31	13.346	1741	1744	1750	rVB7	5713	9084	0.19%	0.016%
32	13.540	1770	1777	1778	rBV6	11546	18459	0.39%	0.033%
33	13.557	1778	1780	1786	rVB5	9964	14035	0.30%	0.025%
34	13.704	1798	1805	1809	rBV3	15239	28518	0.61%	0.051%
35	13.751	1809	1813	1815	rVV4	10580	12870	0.27%	0.023%
36	13.799	1815	1821	1831	rVV	2018254	2624519	55.74%	4.701%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080721\
 Data File : BP006590.D
 Acq On : 08 Aug 2021 04:37
 Operator : CG/JU
 Sample : M3169-15
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C00B4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Title : SVOA CALIBRATION

37	13.916	1837	1841	1842	rBV4	4464	5462	0.12%	0.010%
38	14.069	1856	1867	1878	rBV	2153392	3227569	68.55%	5.781%
39	14.287	1901	1904	1909	rVB	19698	25641	0.54%	0.046%
40	14.375	1911	1919	1927	rBV	1627913	2360023	50.13%	4.227%
41	14.546	1944	1948	1949	rBV4	8770	10079	0.21%	0.018%
42	14.587	1949	1955	1976	rVV	745010	1298939	27.59%	2.327%
43	14.740	1978	1981	1985	rVV5	20297	37520	0.80%	0.067%
44	14.775	1985	1987	1990	rVV	21370	29303	0.62%	0.052%
45	14.804	1990	1992	1996	rVV4	17222	26259	0.56%	0.047%
46	14.851	1997	2000	2004	rVV4	12941	17599	0.37%	0.032%
47	14.910	2007	2010	2015	rVB7	4676	6644	0.14%	0.012%
48	15.046	2031	2033	2038	rVB6	7372	8036	0.17%	0.014%
49	15.116	2040	2045	2046	rBV5	5581	6343	0.13%	0.011%
50	15.246	2063	2067	2071	rVB2	21831	28458	0.60%	0.051%
51	15.310	2074	2078	2082	rBV7	3467	4764	0.10%	0.009%
52	15.375	2082	2089	2096	rBV	2592740	3758404	79.83%	6.732%
53	15.498	2103	2110	2124	rVB	684619	982509	20.87%	1.760%
54	15.610	2125	2129	2134	rVB	27656	36631	0.78%	0.066%
55	15.722	2143	2148	2151	rBV5	12241	18690	0.40%	0.033%
56	15.828	2163	2166	2170	rBV5	9149	9660	0.21%	0.017%
57	15.863	2170	2172	2180	rVB5	10256	21217	0.45%	0.038%
58	15.945	2180	2186	2187	rBV5	7043	10173	0.22%	0.018%
59	16.057	2200	2205	2206	rBV5	4583	5326	0.11%	0.010%
60	16.110	2210	2214	2221	rVB	20617	30881	0.66%	0.055%
61	16.404	2259	2264	2267	rBV7	4643	7770	0.17%	0.014%
62	16.451	2268	2272	2275	rVV6	5137	8415	0.18%	0.015%
63	16.540	2283	2287	2291	rVV6	5309	7350	0.16%	0.013%
64	16.681	2305	2311	2318	rBV5	19160	41136	0.87%	0.074%
65	16.787	2324	2329	2338	rBV7	16036	31522	0.67%	0.056%
66	16.857	2338	2341	2346	rBV7	10605	18840	0.40%	0.034%
67	16.904	2346	2349	2353	rBV4	22955	32553	0.69%	0.058%
68	17.128	2381	2387	2392	rBV	1804968	2585406	54.91%	4.631%
69	17.169	2392	2394	2398	rVV	95642	119455	2.54%	0.214%
70	17.228	2398	2404	2416	rVB2	2774569	3968467	84.29%	7.108%
71	17.445	2437	2441	2445	rVB4	16091	21711	0.46%	0.039%
72	17.645	2472	2475	2478	rBV3	19449	24479	0.52%	0.044%
73	17.822	2500	2505	2508	rBV	64346	87578	1.86%	0.157%
74	17.922	2520	2522	2527	rVB6	9122	11280	0.24%	0.020%
75	17.998	2532	2535	2537	rBV2	21973	25226	0.54%	0.045%
76	18.034	2537	2541	2550	rVV3	170884	248768	5.28%	0.446%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080721\
 Data File : BP006590.D
 Acq On : 08 Aug 2021 04:37
 Operator : CG/JU
 Sample : M3169-15
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C00B4

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Title : SVOA CALIBRATION

77	18.181	2563	2566	2570	rBV2	22126	33112	0.70%	0.059%
78	18.222	2570	2573	2576	rVB	15597	18180	0.39%	0.033%
79	18.322	2587	2590	2592	rBV2	14904	18193	0.39%	0.033%
80	18.487	2615	2618	2623	rBV	36775	45748	0.97%	0.082%
81	18.892	2683	2687	2691	rBV3	30041	45697	0.97%	0.082%
82	18.934	2691	2694	2699	rBV3	35051	48170	1.02%	0.086%
83	19.016	2706	2708	2710	rBV2	13104	13532	0.29%	0.024%
84	19.045	2711	2713	2717	rVB2	31940	35879	0.76%	0.064%
85	19.116	2722	2725	2726	rVV	27103	31068	0.66%	0.056%
86	19.145	2726	2730	2735	rVB	122770	173568	3.69%	0.311%
87	19.269	2748	2751	2759	rBV3	66890	108521	2.30%	0.194%
88	19.469	2780	2785	2794	rBV	3324883	4708219	100.00%	8.433%
89	19.981	2869	2872	2875	rVV4	68080	74590	1.58%	0.134%
90	20.016	2875	2878	2882	rVB2	58714	62162	1.32%	0.111%
91	20.251	2915	2918	2922	rBV3	92222	127424	2.71%	0.228%
92	20.498	2958	2960	2964	rVB	104670	104597	2.22%	0.187%
93	20.710	2993	2996	3001	rVB3	68037	83610	1.78%	0.150%
94	20.957	3034	3038	3044	rBV	282007	437820	9.30%	0.784%
95	21.228	3079	3084	3088	rBV	2138399	2781090	59.07%	4.981%
96	21.386	3108	3111	3115	rVB	133887	152922	3.25%	0.274%
97	21.610	3146	3149	3155	rVB	137665	175372	3.72%	0.314%
98	21.839	3185	3188	3196	rVB2	136437	205488	4.36%	0.368%
99	23.404	3447	3454	3460	rBV	2363997	4357100	92.54%	7.804%
100	23.551	3472	3479	3489	rVB2	1358331	2746906	58.34%	4.920%



Sum of corrected areas: 55829870

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080721\
Data File : BP006590.D
Acq On : 08 Aug 2021 04:37
Operator : CG/JU
Sample : M3169-15
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C00B4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

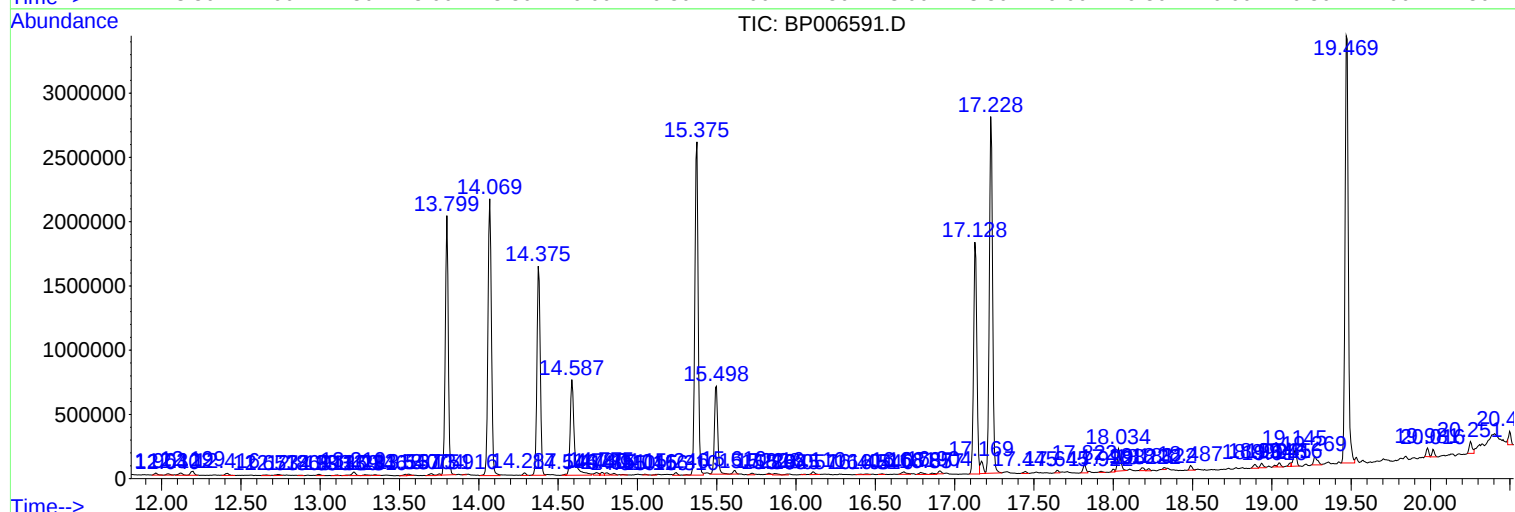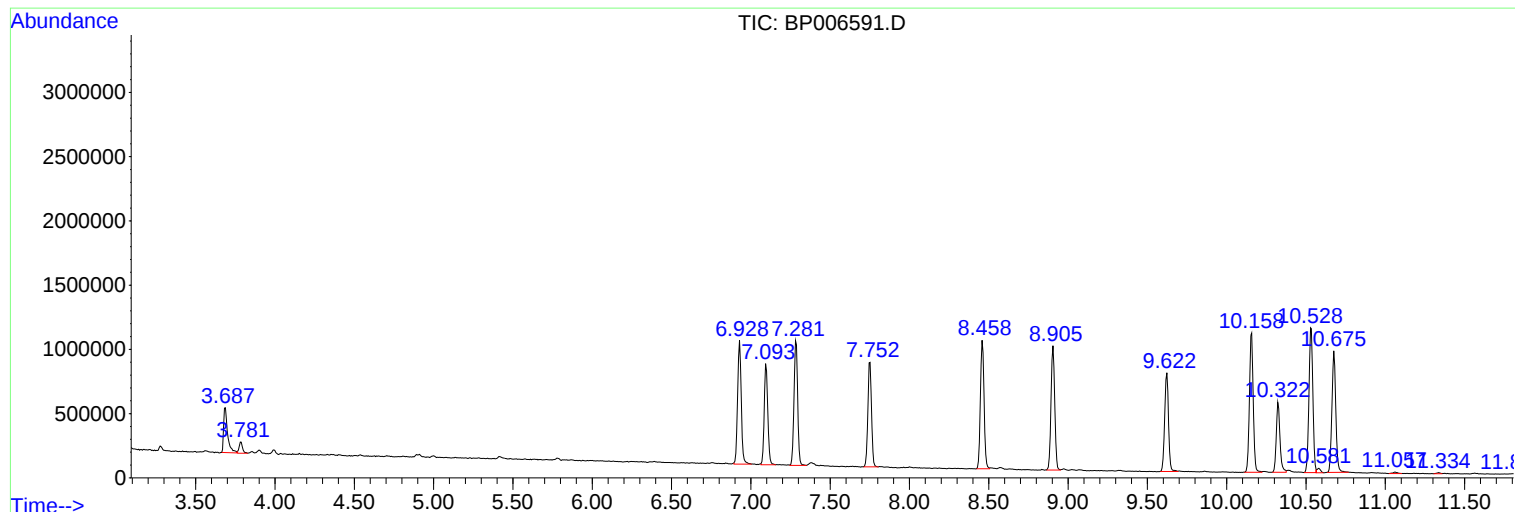

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080721\
Data File : BP006590.D
Acq On : 08 Aug 2021 04:37
Operator : CG/JU
Sample : M3169-15
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C00B4










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 1-(2-butoxyethoxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.320	9.10 ng/ul	881554	Naphthalene-d8	10.528

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 1-(2-butoxyethoxy)-	162	C8H18O3	054446-78-5	90
2			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
3			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
4			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	90
5			Ethanol, 2-(2-butoxyethoxy)-	162	C8H18O3	000112-34-5	72

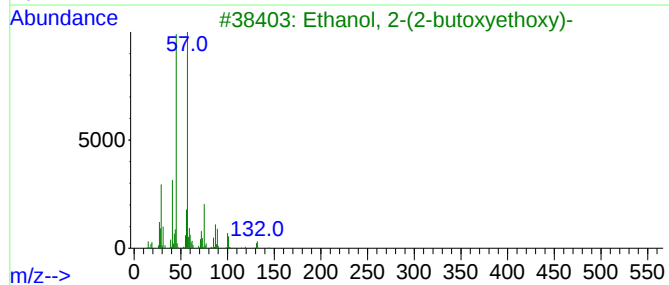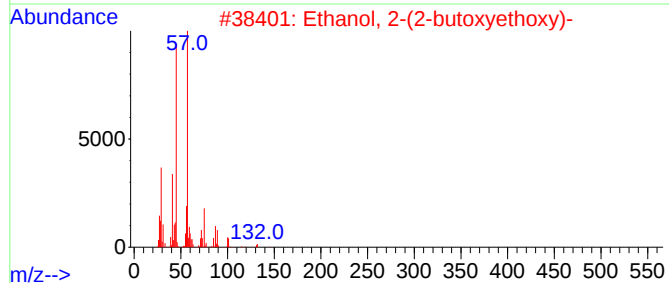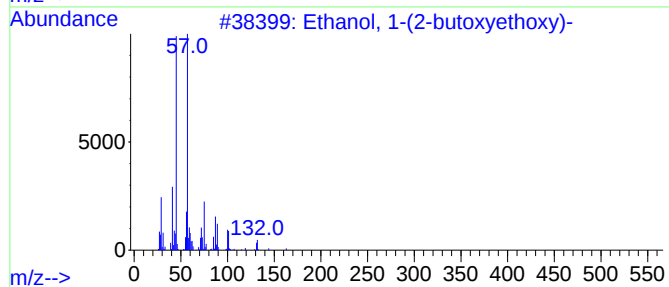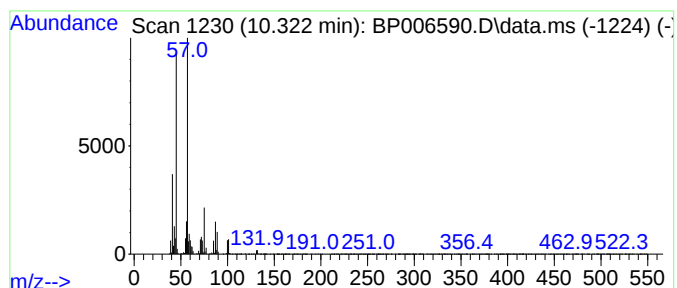

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080721\
Data File : BP006590.D
Acq On : 08 Aug 2021 04:37
Operator : CG/JU
Sample : M3169-15
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C00B4










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Hexadecane, 1,1'-[1,2-ethan... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.960	3.15 ng/ul	437820	Chrysene-d12	21.228

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Hexadecane, 1,1'-[1,2-ethanediyl...	511	C34H70O2	017367-09-8	93
2			Hexadecane	226	C16H34	000544-76-3	91
3			Hexadecane	226	C16H34	000544-76-3	90
4			Triacontyl acetate	480	C32H64O2	041755-58-2	90
5			Carbonic acid, octadecyl vinyl e...	340	C21H40O3	1000382-54-4	90

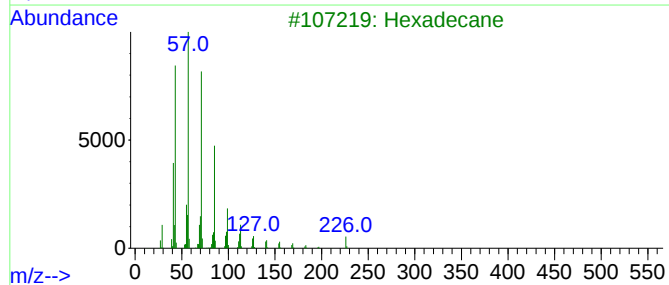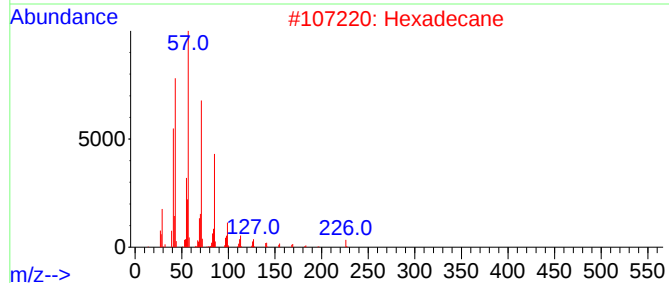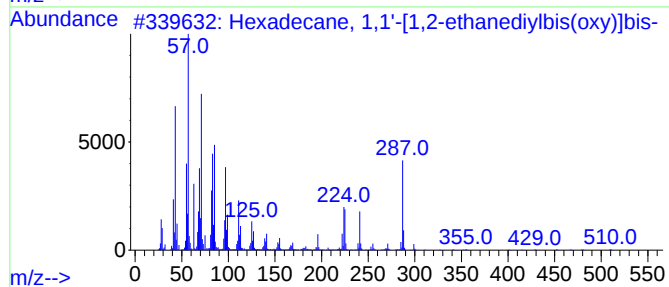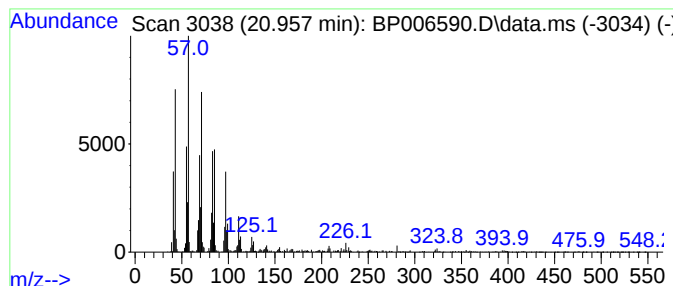

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080721\
Data File : BP006590.D
Acq On : 08 Aug 2021 04:37
Operator : CG/JU
Sample : M3169-15
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C00B4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 1-(2-b...	10.320	9.1	ng/ul	881554	2	10.528	1937850	20.0
Hexadecane, 1,1...	20.960	3.1	ng/ul	437820	5	21.228	2781090	20.0