

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080725\
 Data File : BP025312.D
 Acq On : 07 Aug 2025 13:47
 Operator : CG/JU
 Sample : Q2763-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 TP-2

Quant Time: Aug 07 14:41:17 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080525.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 06 06:41:44 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.802	152	212342	20.000	ng	0.00
21) Naphthalene-d8	10.572	136	839386	20.000	ng	0.00
39) Acenaphthene-d10	14.419	164	512353	20.000	ng	0.00
64) Phenanthrene-d10	17.219	188	988138	20.000	ng	0.00
76) Chrysene-d12	21.648	240	1150288	20.000	ng	-0.01
86) Perylene-d12	25.048	264	1281191	20.000	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.414	112	1522961	115.355	ng	0.00
7) Phenol-d6	6.966	99	1811520	104.258	ng	0.00
23) Nitrobenzene-d5	8.937	82	1271427	83.917	ng	0.00
42) 2,4,6-Tribromophenol	15.931	330	771562	150.952	ng	0.00
45) 2-Fluorobiphenyl	13.037	172	2555047	68.879	ng	0.00
79) Terphenyl-d14	19.948	244	4568357	75.013	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080725\
Data File : BP025312.D
Acq On : 07 Aug 2025 13:47
Operator : CG/JU
Sample : Q2763-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TP-2

Quant Time: Aug 07 14:41:17 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 06:41:44 2025
Response via : Initial Calibration




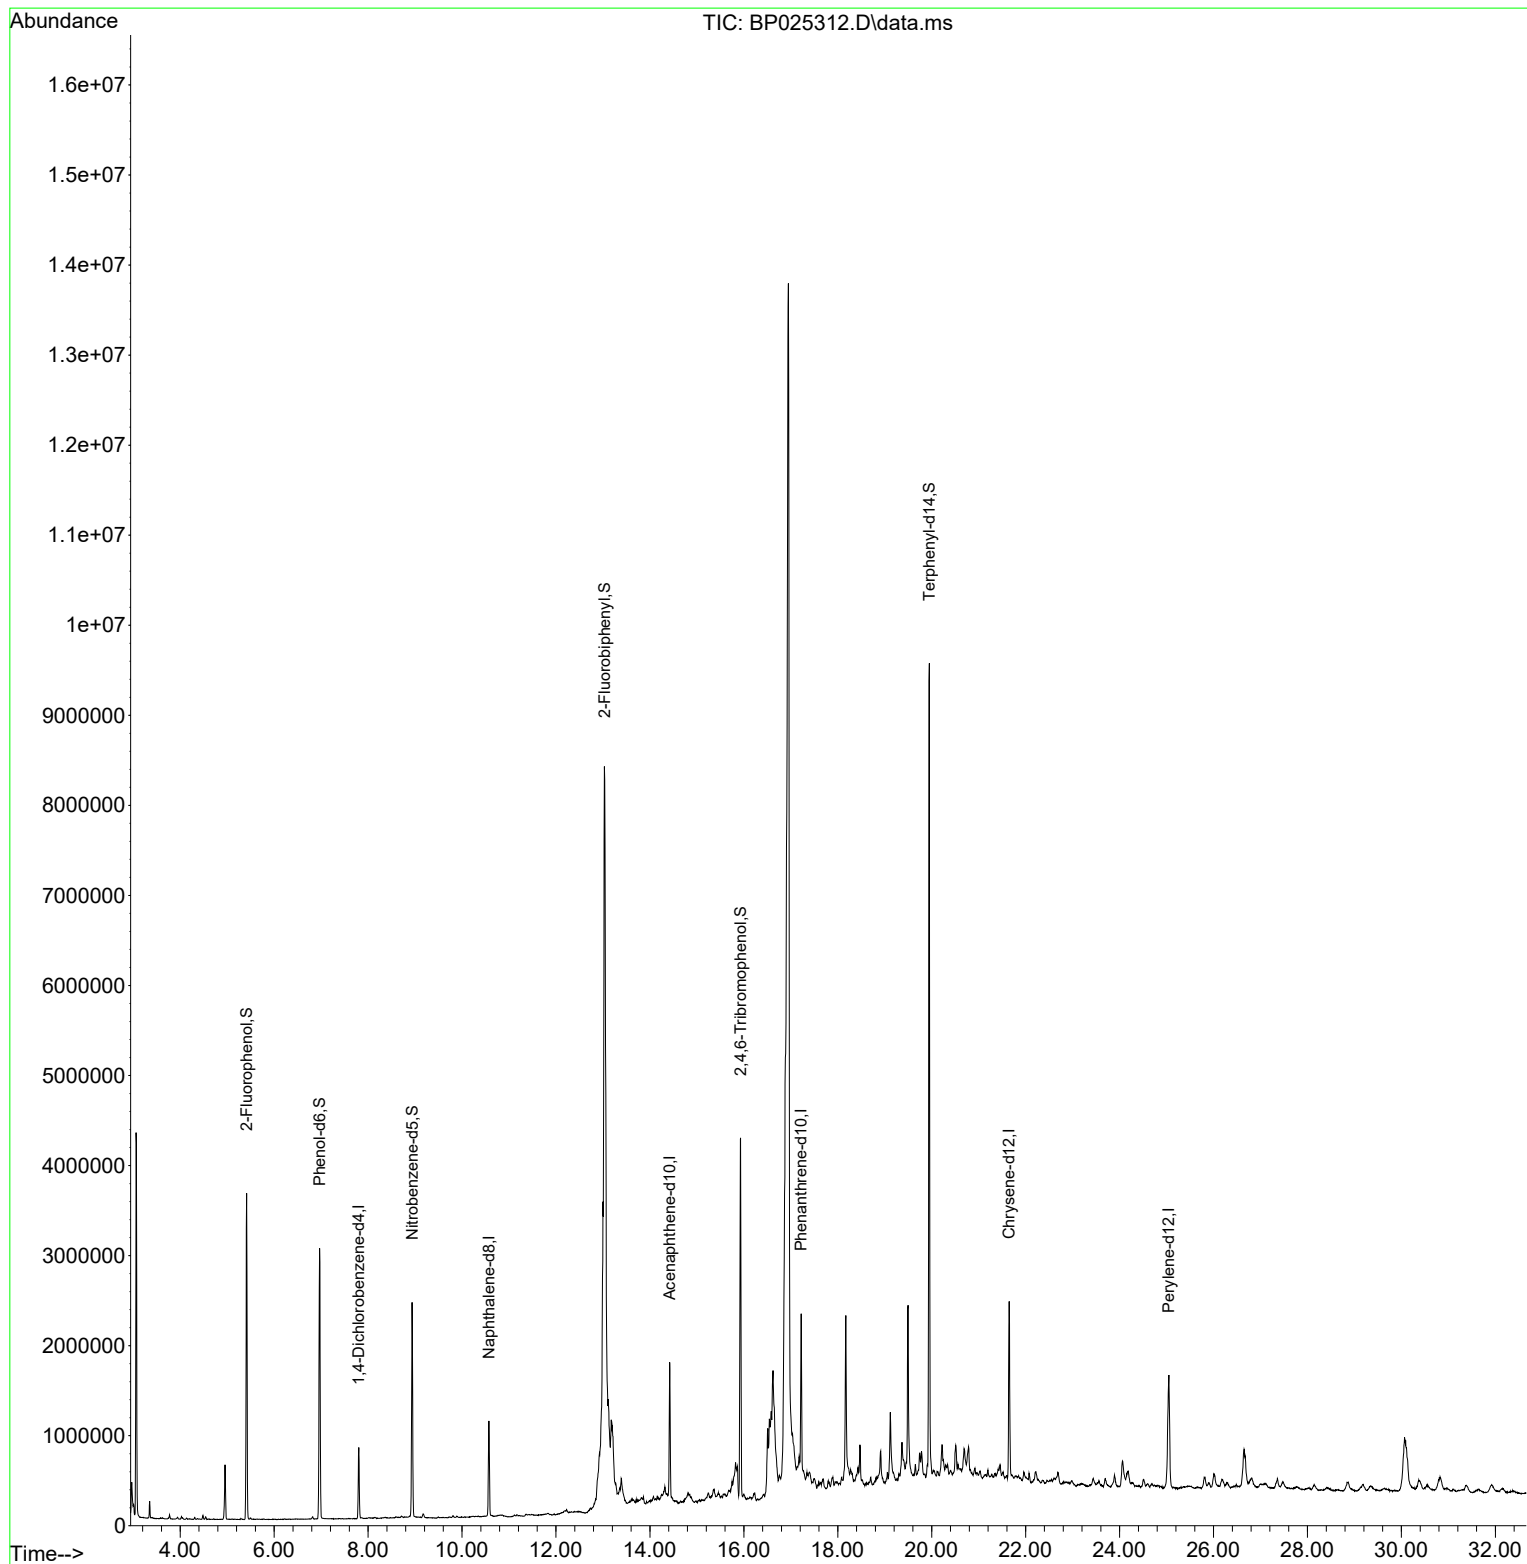




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.802 min Scan# 81
Delta R.T. -0.000 min
Lab File: BP025312.D
Acq: 07 Aug 2025 13:47




Instrument :
BNA_P
ClientSampleId :
TP-2


Tgt Ion:152 Resp: 212342
Ion Ratio Lower Upper
152 100
150 157.3 125.1 187.7
115 61.4 48.4 72.6

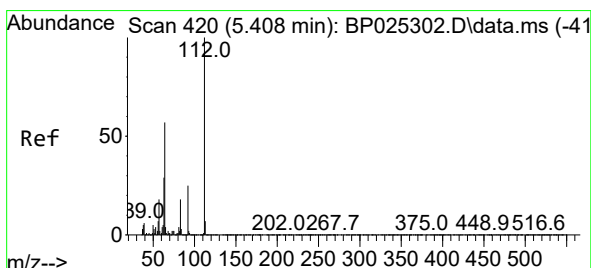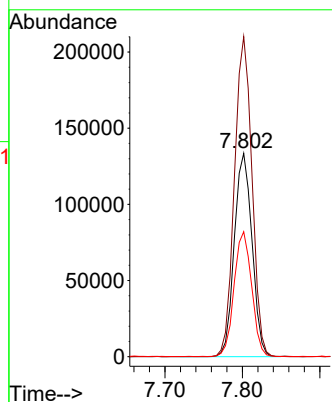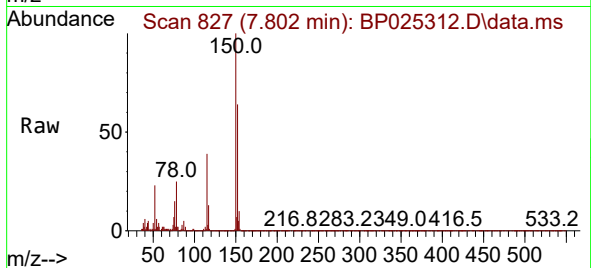

#5
2-Fluorophenol
Concen: 115.355 ng
RT: 5.414 min Scan# 421
Delta R.T. 0.006 min
Lab File: BP025312.D
Acq: 07 Aug 2025 13:47

Tgt Ion:112 Resp: 1522961
Ion Ratio Lower Upper
112 100
64 55.8 45.3 67.9
63 29.3 23.0 34.6


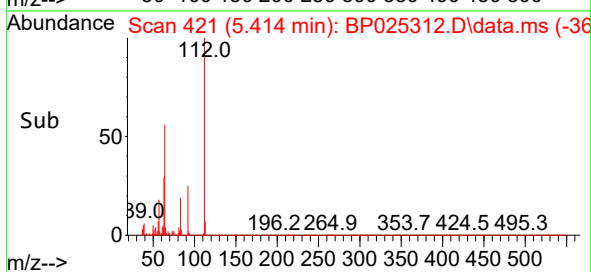
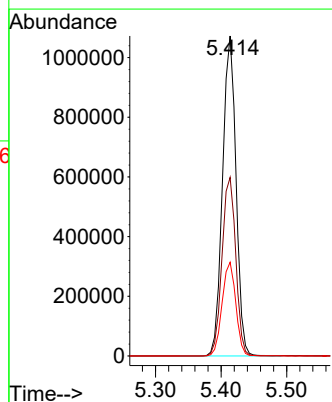





#7
Phenol-d6
Concen: 104.258 ng
RT: 6.966 min Scan# 685
Delta R.T. 0.000 min
Lab File: BP025312.D
Acq: 07 Aug 2025 13:47




Instrument :
BNA_P
ClientSampleId :
TP-2


Tgt Ion: 99 Resp: 1811520
Ion Ratio Lower Upper
99 100
42 18.7 15.0 22.6
71 32.6 25.5 38.3

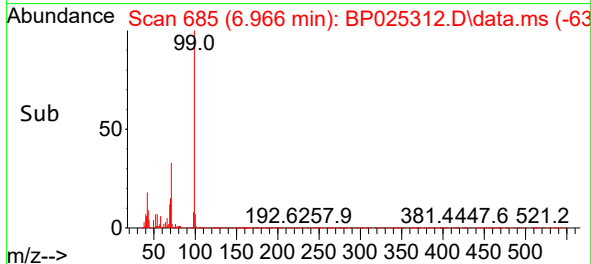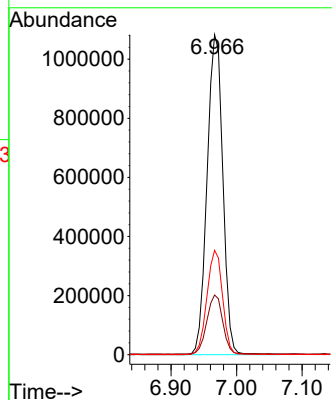

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.572 min Scan# 1298
Delta R.T. 0.000 min
Lab File: BP025312.D
Acq: 07 Aug 2025 13:47

Tgt Ion: 136 Resp: 839386
Ion Ratio Lower Upper
136 100
137 10.8 8.9 13.3
54 8.3 7.0 10.6
68 6.3 5.0 7.6


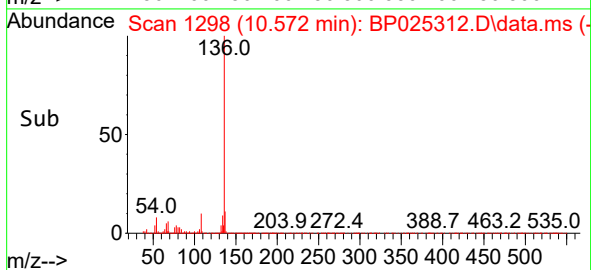
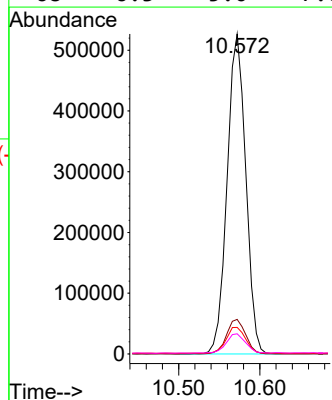
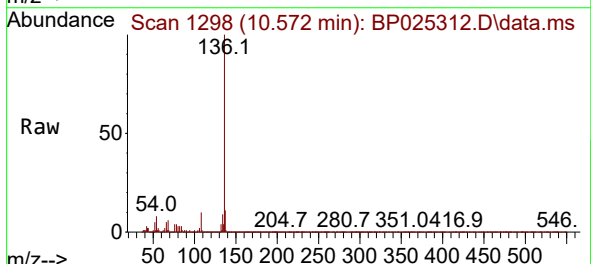




#23
Nitrobenzene-d5
Concen: 83.917 ng
RT: 8.937 min Scan# 1021
Delta R.T. -0.006 min
Lab File: BP025312.D
Acq: 07 Aug 2025 13:47




Instrument :
BNA_P
ClientSampleId :
TP-2


Tgt Ion: 82 Resp: 1271427
Ion Ratio Lower Upper
82 100
128 45.4 35.4 53.2
54 52.6 42.9 64.3

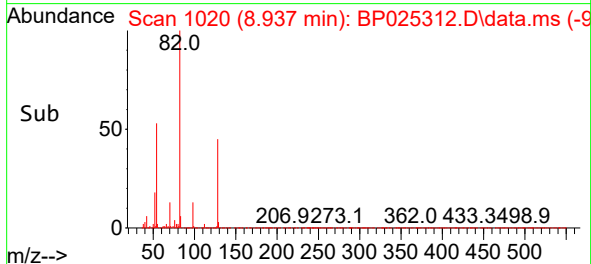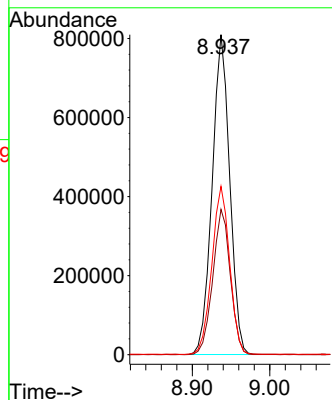

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.419 min Scan# 1952
Delta R.T. -0.000 min
Lab File: BP025312.D
Acq: 07 Aug 2025 13:47

Tgt Ion: 164 Resp: 512353
Ion Ratio Lower Upper
164 100
162 98.2 80.6 120.8
160 43.8 35.9 53.9

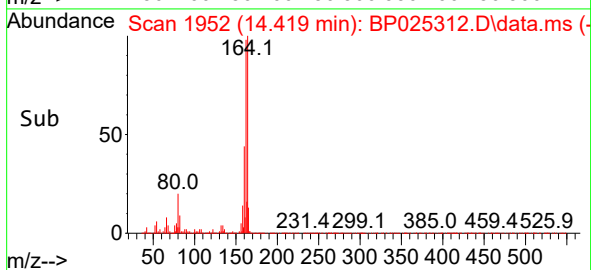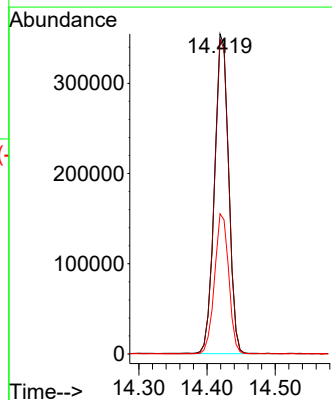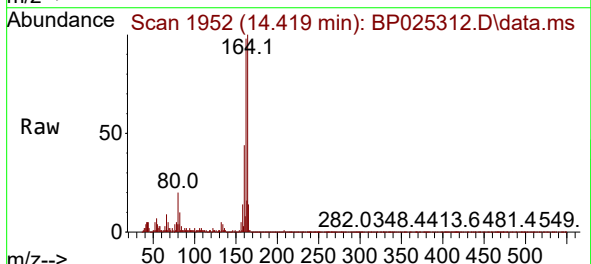

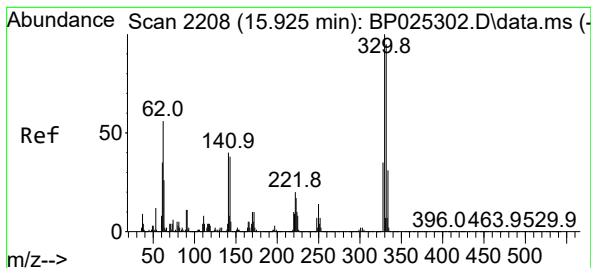

#42

2,4,6-Tribromophenol

Concen: 150.952 ng

RT: 15.931 min Scan# 2209

Delta R.T. 0.006 min

Lab File: BP025312.D

Acq: 07 Aug 2025 13:47

Instrument :

BNA_P

ClientSampleId :

TP-2





Tgt Ion:330 Resp: 771562

Ion Ratio Lower Upper

330 100

332 96.8 77.4 116.0

141 39.0 31.7 47.5

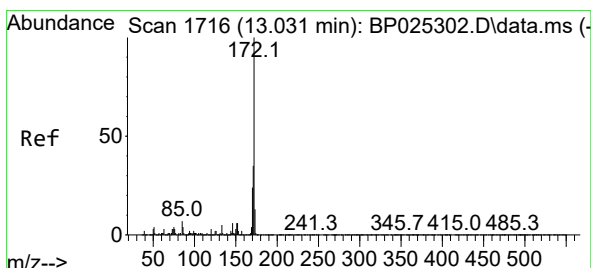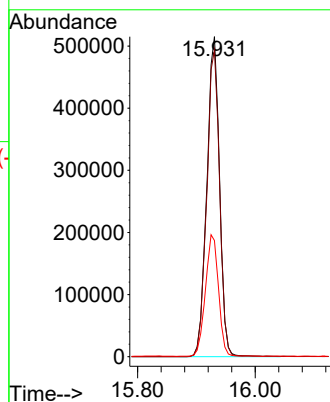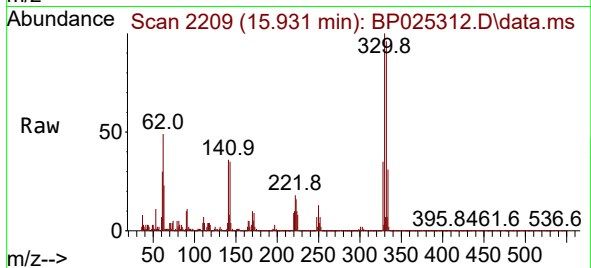

#45

2-Fluorobiphenyl

Concen: 68.879 ng

RT: 13.037 min Scan# 1717

Delta R.T. 0.006 min

Lab File: BP025312.D

Acq: 07 Aug 2025 13:47




Tgt Ion:172 Resp: 2555047


Ion Ratio Lower Upper

172 100

171 36.9 27.9 41.9

170 23.6 18.9 28.3


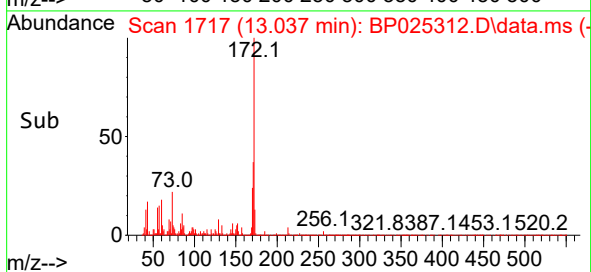
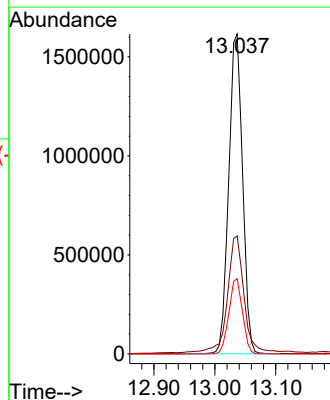





#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.219 min Scan# 2428
Delta R.T. -0.006 min
Lab File: BP025312.D
Acq: 07 Aug 2025 13:47




Instrument :
BNA_P
ClientSampleId :
TP-2


Tgt Ion:188 Resp: 988138
Ion Ratio Lower Upper
188 100
94 10.1 8.0 12.0
80 11.2 8.5 12.7

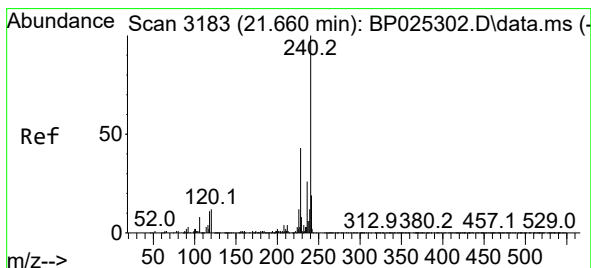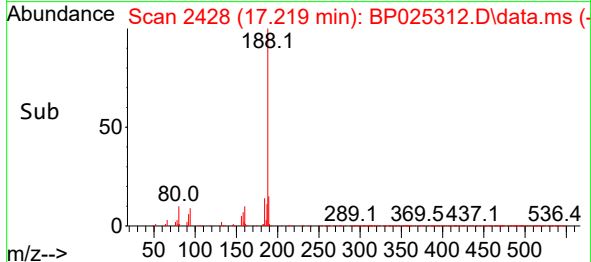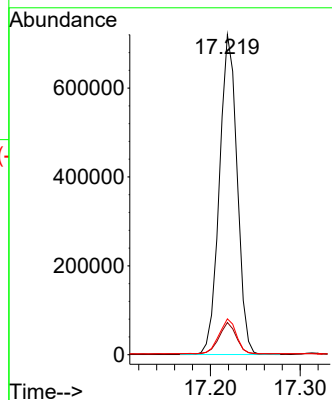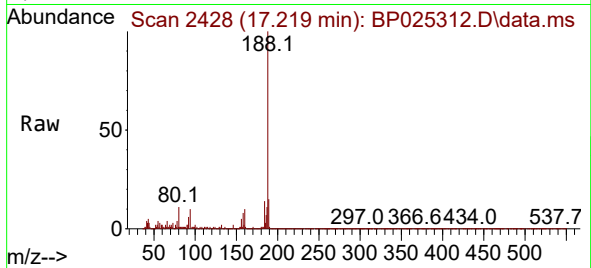

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.648 min Scan# 3181
Delta R.T. -0.012 min
Lab File: BP025312.D
Acq: 07 Aug 2025 13:47

Tgt Ion:240 Resp: 1150288
Ion Ratio Lower Upper
240 100
120 11.6 9.6 14.4
236 25.7 20.4 30.6


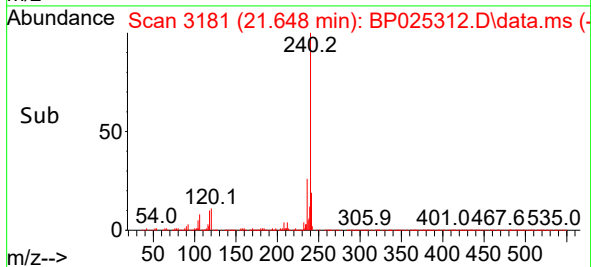
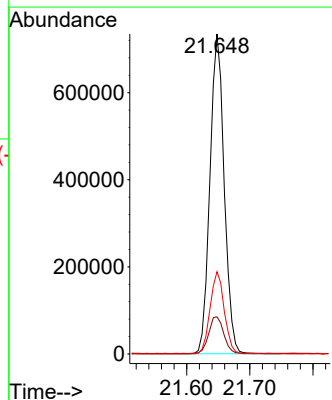
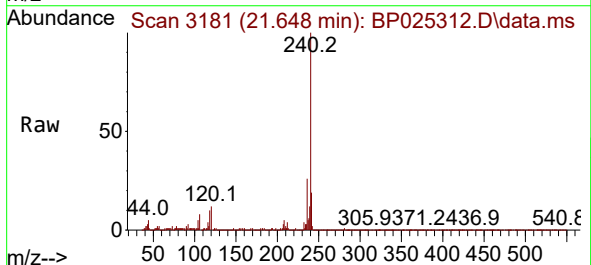




#79
 Terphenyl-d14
 Concen: 75.013 ng
 RT: 19.948 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: BP025312.D
 Acq: 07 Aug 2025 13:47

Instrument :
 BNA_P
 ClientSampleId :
 TP-2

Tgt Ion:244 Resp: 4568357
 Ion Ratio Lower Upper
 244 100
 212 7.4 5.9 8.9
 122 10.7 9.5 14.3

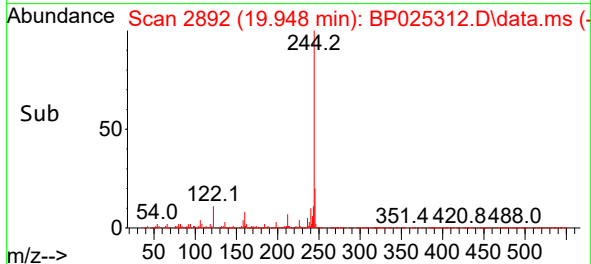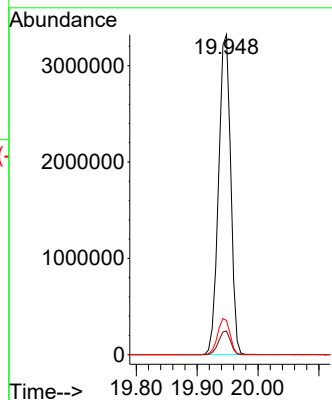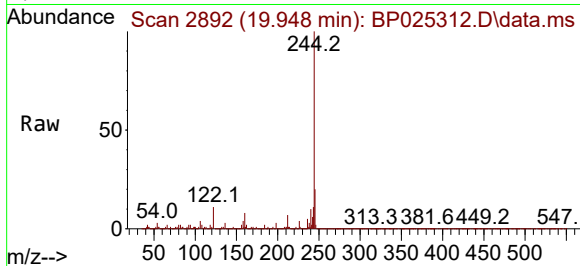

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 25.048 min Scan# 3759
 Delta R.T. 0.012 min
 Lab File: BP025312.D
 Acq: 07 Aug 2025 13:47

Tgt Ion:264 Resp: 1281191
 Ion Ratio Lower Upper
 264 100
 260 23.2 19.2 28.8
 265 21.1 17.1 25.7

