
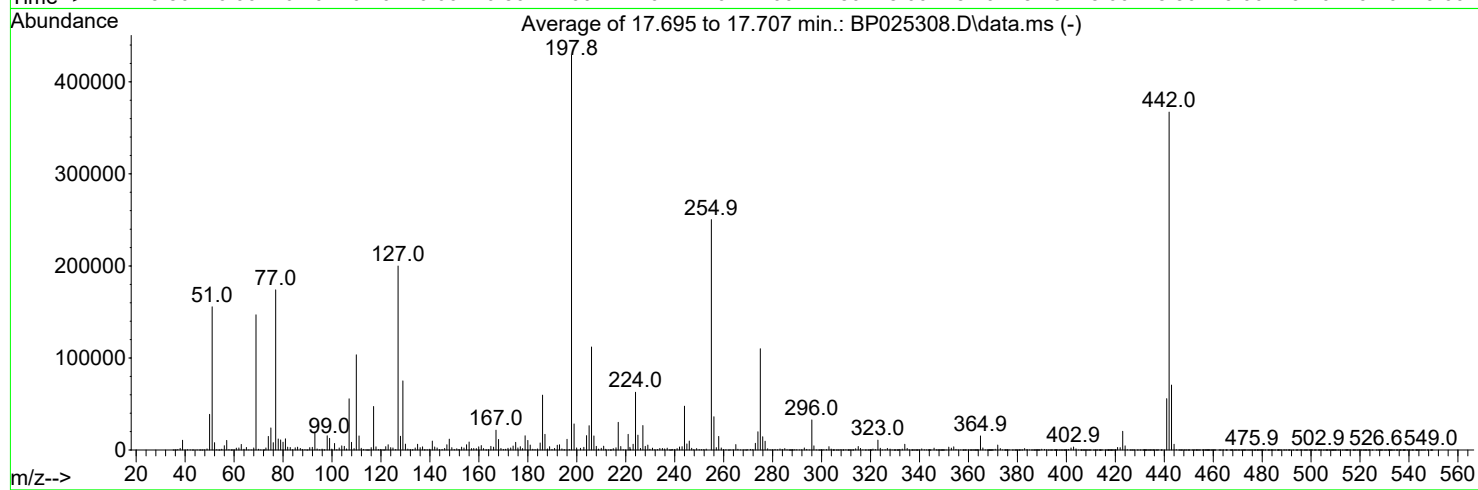


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080725\
Data File : BP025308.D
Acq On : 07 Aug 2025 11:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 06 06:41:44 2025

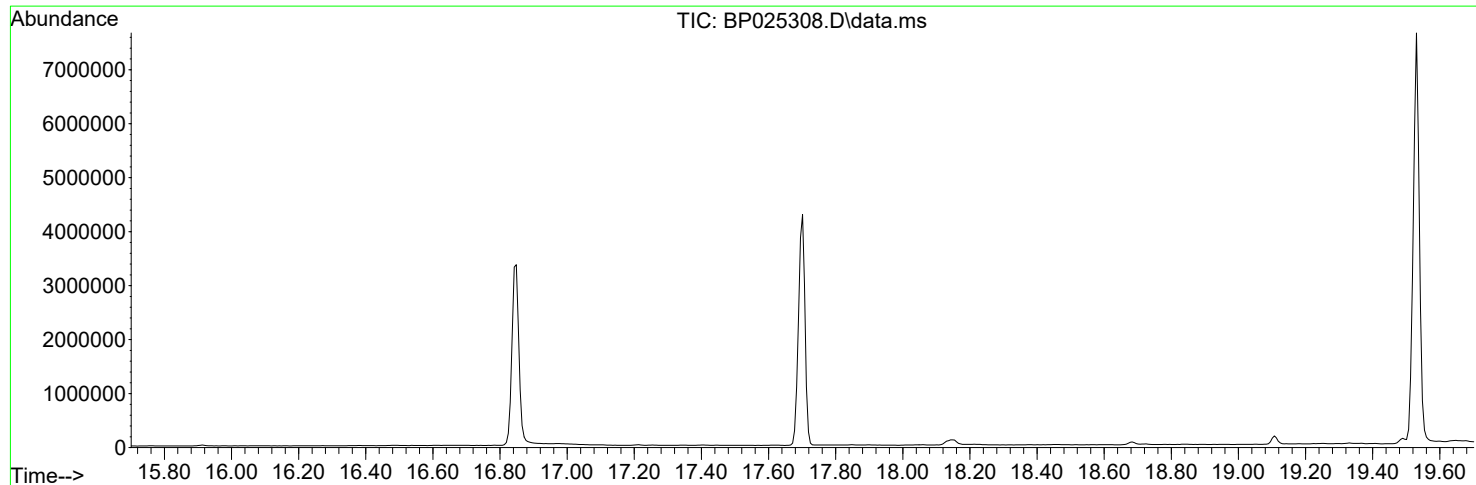

AutoFind: Scans 2509, 2510, 2511; Background Corrected with Scan 2500

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.6	2339	PASS
69	69	100	100	100.0	146849	PASS
70	69	0.00	2	0.6	824	PASS
197	198	0.00	2	0.2	658	PASS
198	198	100	100	100.0	429004	PASS
199	198	5	9	6.6	28302	PASS
365	198	1	100	3.6	15355	PASS
441	443	0.01	150	79.1	55884	PASS
442	442	100	100	100.0	367275	PASS
443	442	15	24	19.2	70680	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/7/2025	BNA_P	<u>BP025308.D</u>
Compound Name	Response	Retention Time
DDT	1578321	20.83
DDD	15364	20.43
DDE	492	19.848
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15856	1594177	0.99

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080725\
Data File : BP025308.D
Acq On : 07 Aug 2025 11:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 07 12:25:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 06:41:44 2025
Response via : Initial Calibration

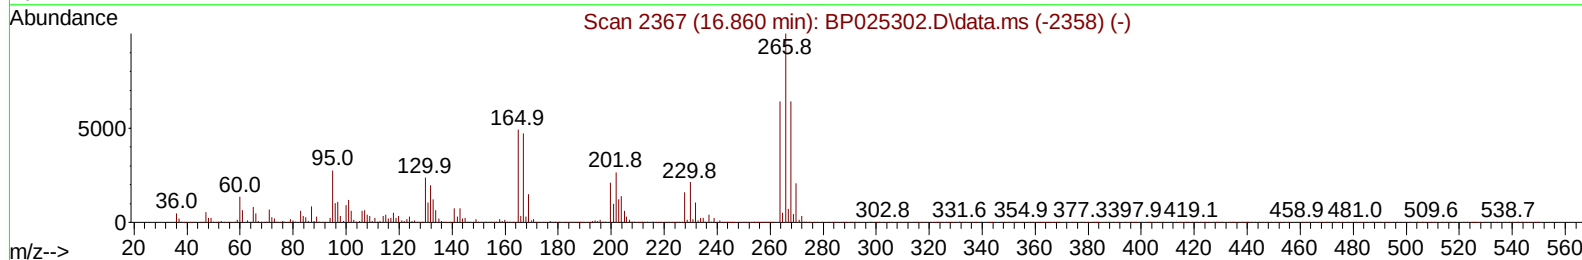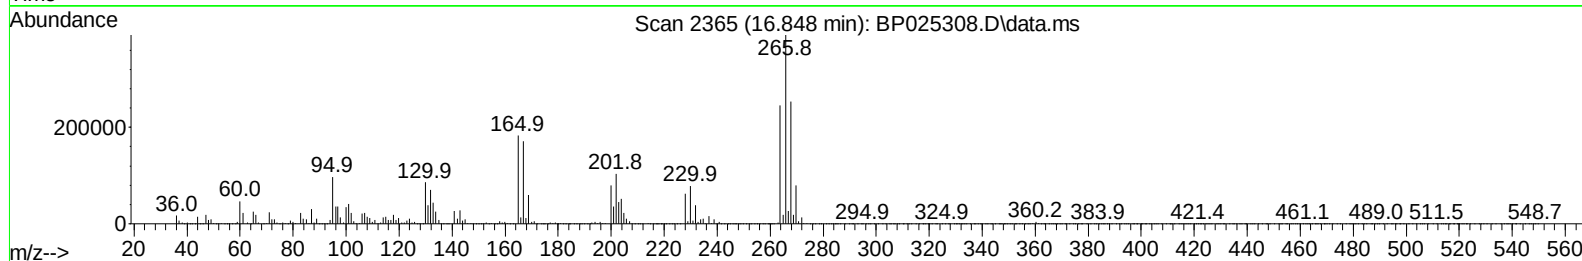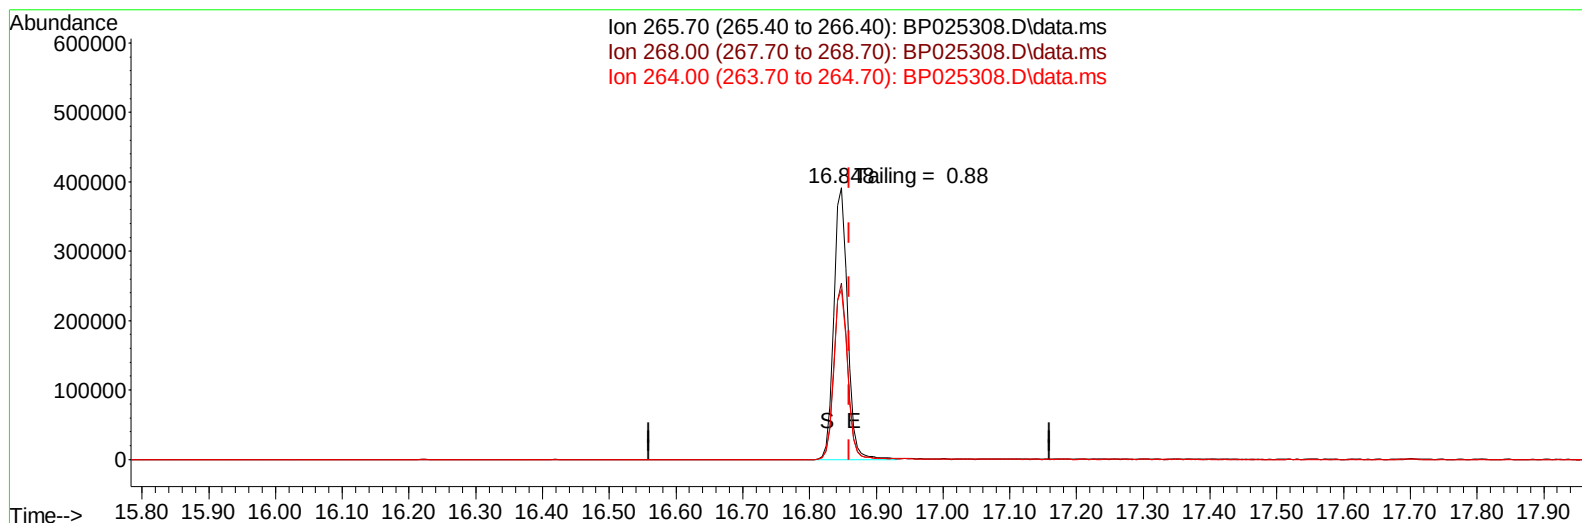

TIC: BP025308.D\data.ms

(70) Pentachlorophenol (C)

16.848min (-0.012) 12862.36 ng




response 556675

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	64.89
264.00	63.90	62.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080725\
Data File : BP025308.D
Acq On : 07 Aug 2025 11:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 07 12:25:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 06:41:44 2025
Response via : Initial Calibration

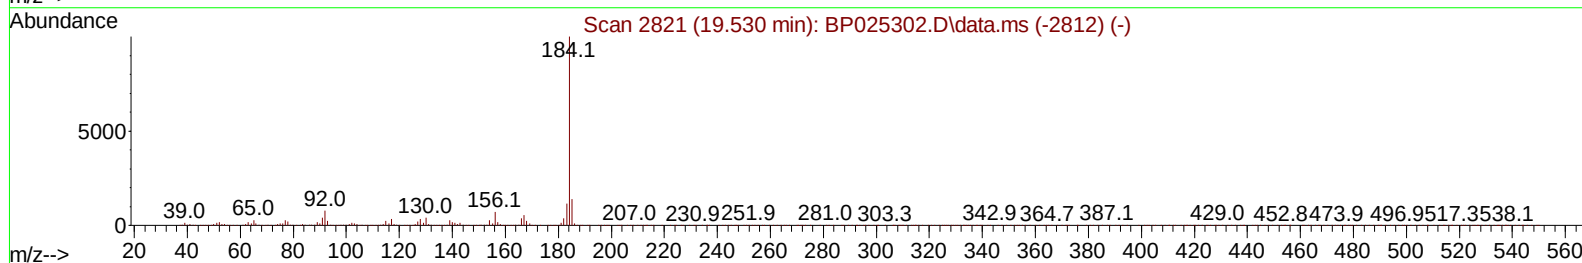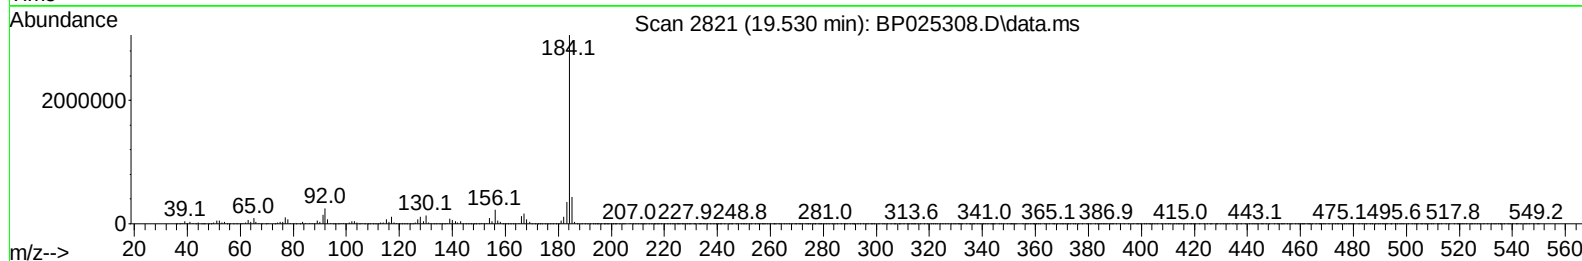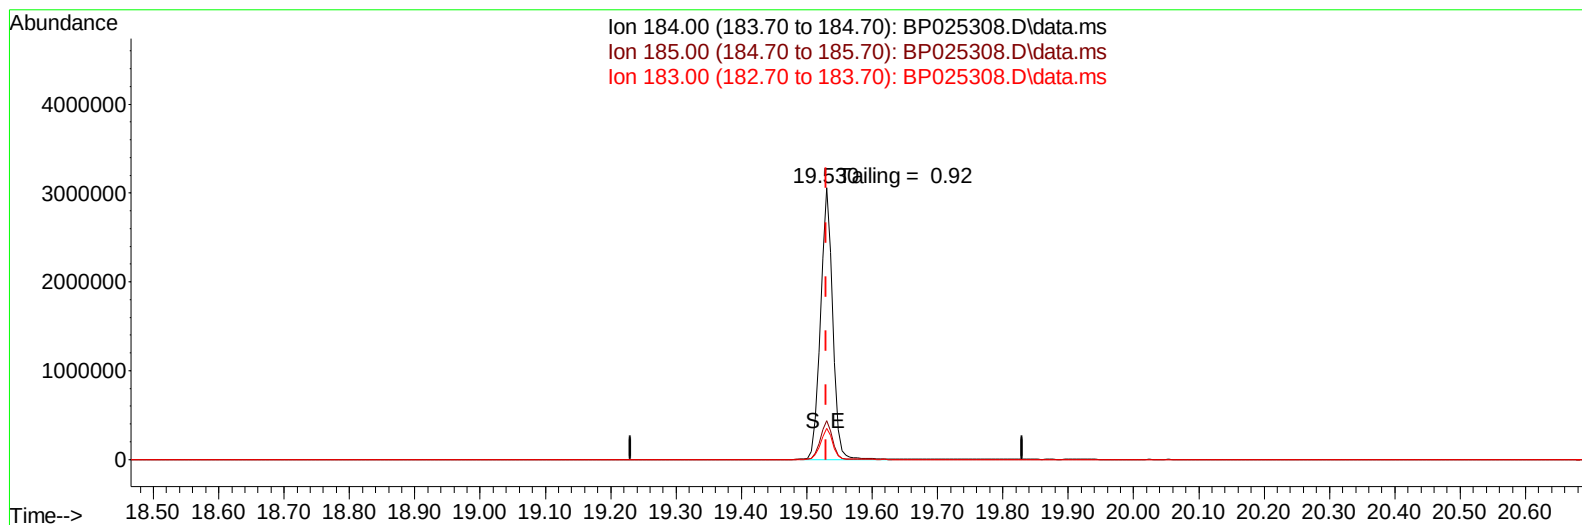

TIC: BP025308.D\data.ms

(77) Benzidine

19.530min (+ 0.000) 8796.27 ng

response 3944680

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.29
183.00	11.50	11.56
0.00	0.00	0.00