




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080824\
Data File : BP021475.D
Acq On : 09 Aug 2024 18:04
Operator : RC/JU
Sample : P3171-05MEDL 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCVW9MEDL

Manual IntegrationsAPPROVED

Quant Time: Aug 09 22:45:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 08 18:23:21 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/10/2024
Supervised By :mohammad ahmed 08/12/2024

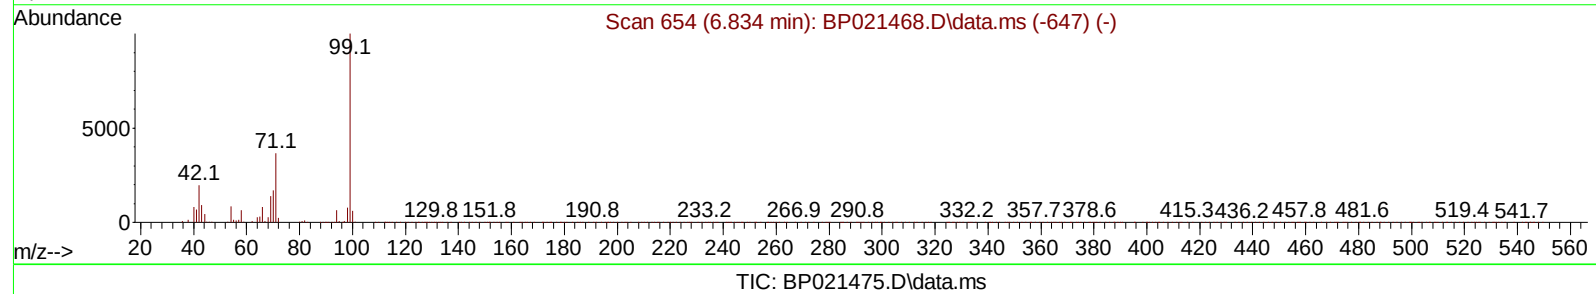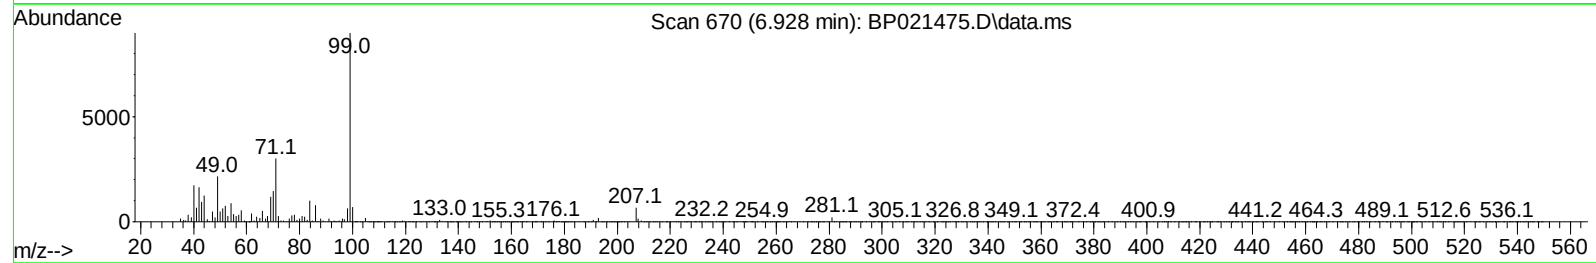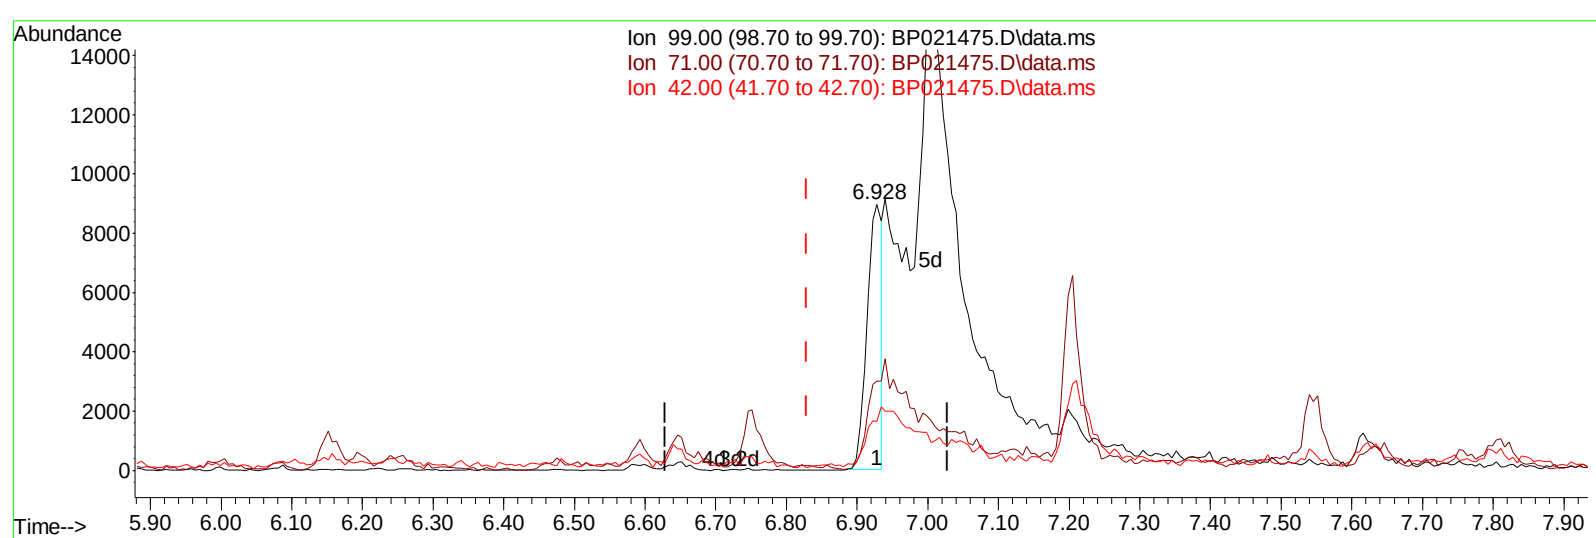

(7) Phenol-d5 (S)

6.928min (+ 0.100) 1.07 ng/u1

response 13028

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	35.60	33.46
42.00	19.30	18.47
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080824\
Data File : BP021475.D
Acq On : 09 Aug 2024 18:04
Operator : RC/JU
Sample : P3171-05MEDL 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCVW9MEDL

Manual IntegrationsAPPROVED

Quant Time: Aug 09 22:45:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 08 18:23:21 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/10/2024
Supervised By :mohammad ahmed 08/12/2024

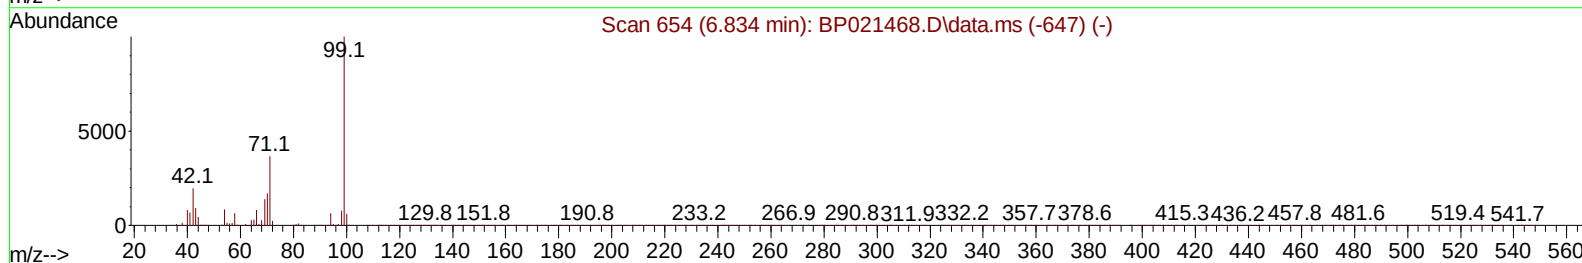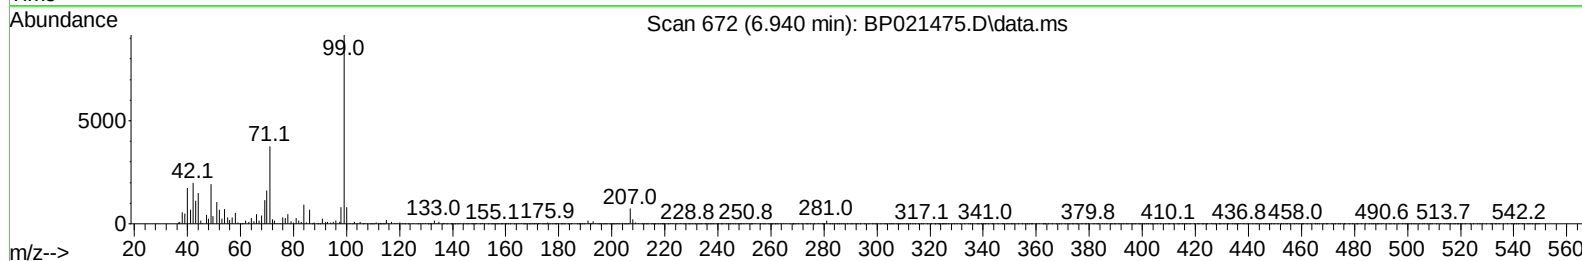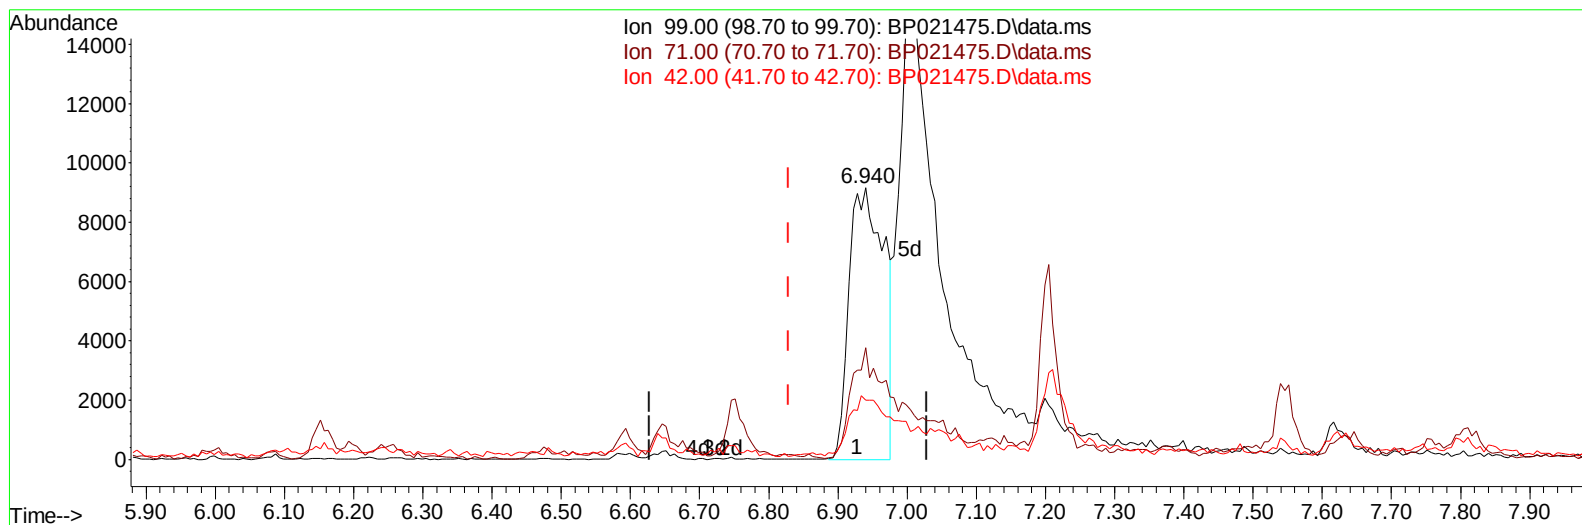

TIC: BP021475.D\data.ms

(7) Phenol-d5 (S)

6.940min (+ 0.112) 2.64 ng/ul m

response 32138

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	35.60	41.15
42.00	19.30	21.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080824\
 Data File : BP021475.D
 Acq On : 09 Aug 2024 18:04
 Operator : RC/JU
 Sample : P3171-05MEDL 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :

BNA_P




ClientSampleId :

DCVW9MEDL

Manual IntegrationsAPPROVED

Quant Time: Aug 09 22:45:37 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 08 18:23:21 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/10/2024
 Supervised By :mohammad ahmed 08/12/2024

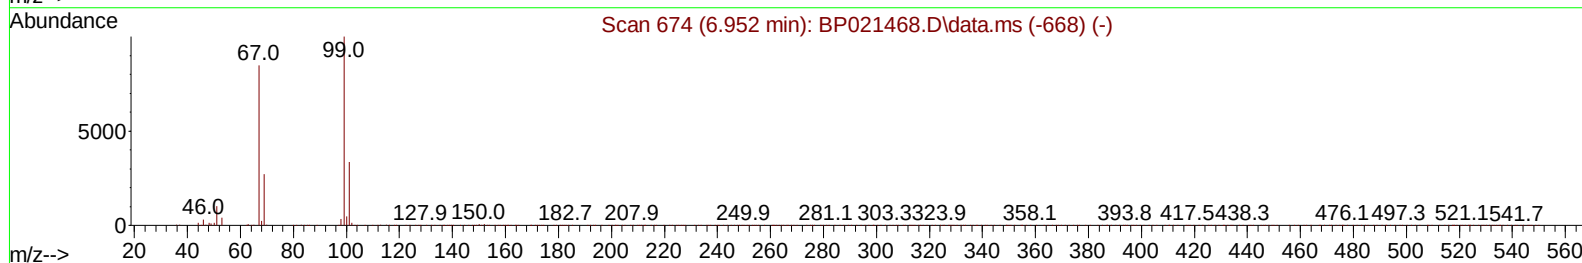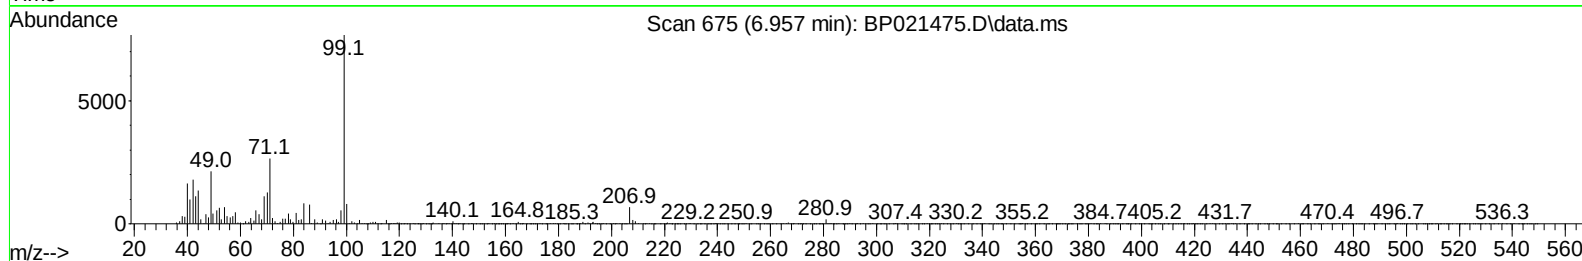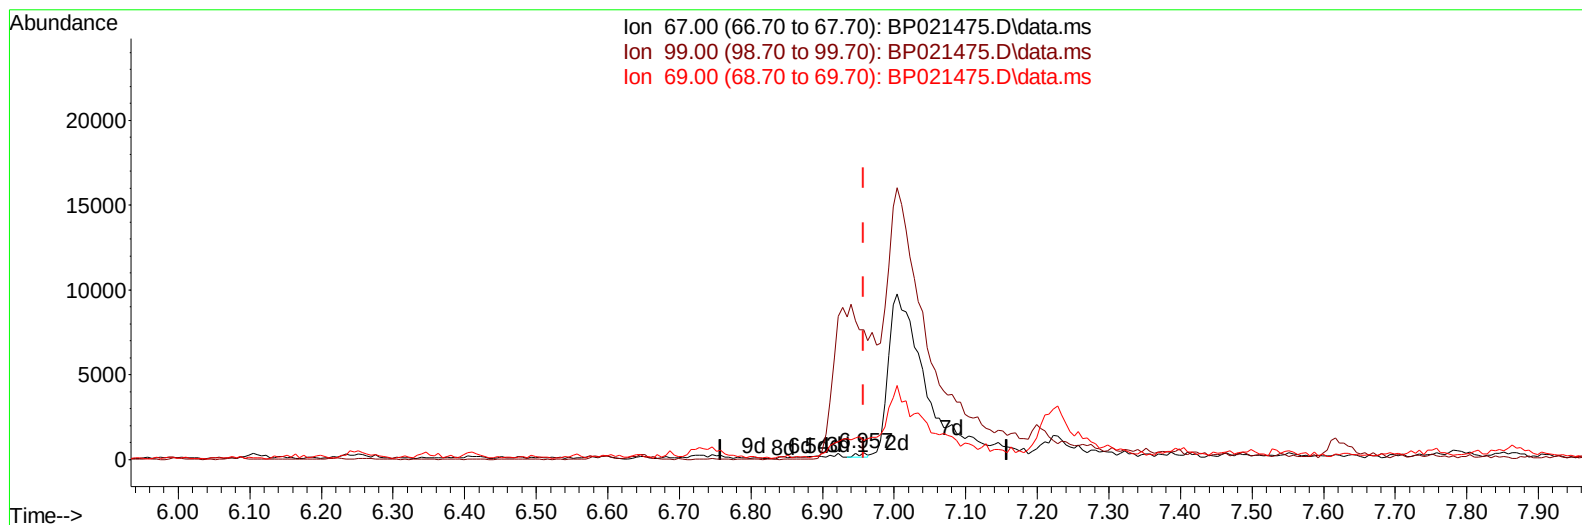

TIC: BP021475.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)

6.957min (-0.000) 0.03 ng/u1

response 234

Ion	Exp%	Act%
67.00	100.00	100.00
99.00	122.50	1955.61#
69.00	30.60	286.48#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080824\
Data File : BP021475.D
Acq On : 09 Aug 2024 18:04
Operator : RC/JU
Sample : P3171-05MEDL 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :

BNA_P




ClientSampleId :

DCVW9MEDL

Manual IntegrationsAPPROVED

Quant Time: Aug 09 22:45:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 08 18:23:21 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/10/2024
Supervised By :mohammad ahmed 08/12/2024

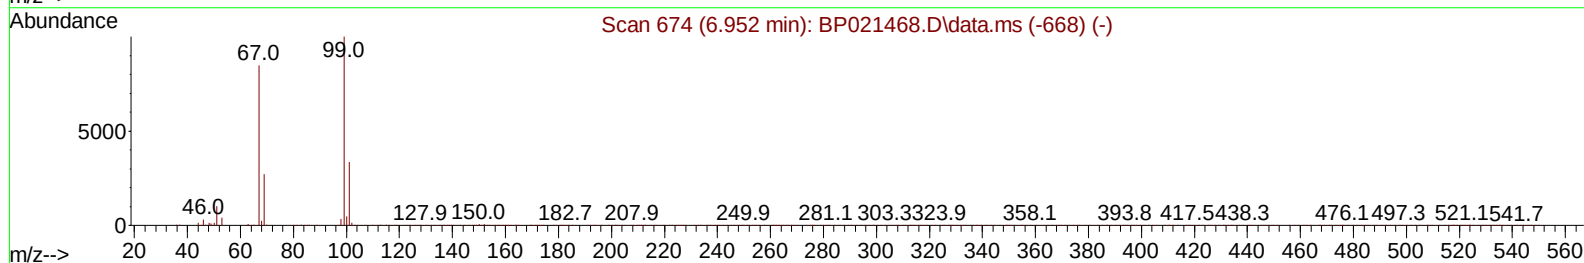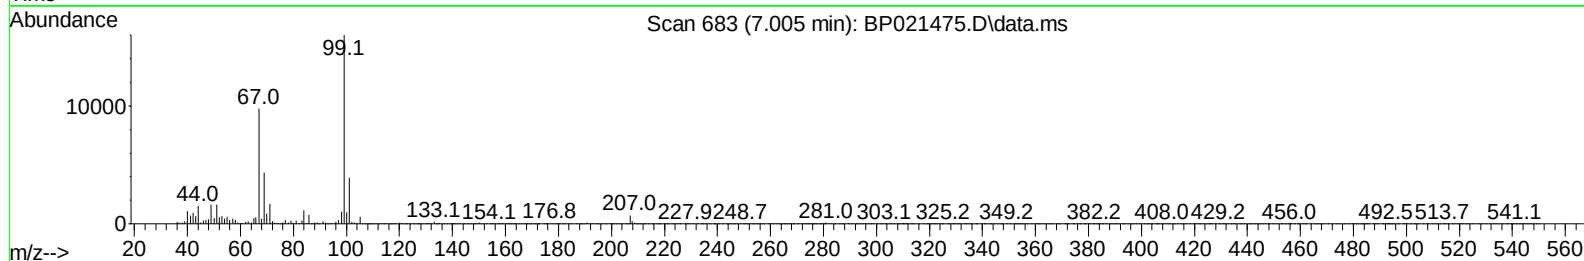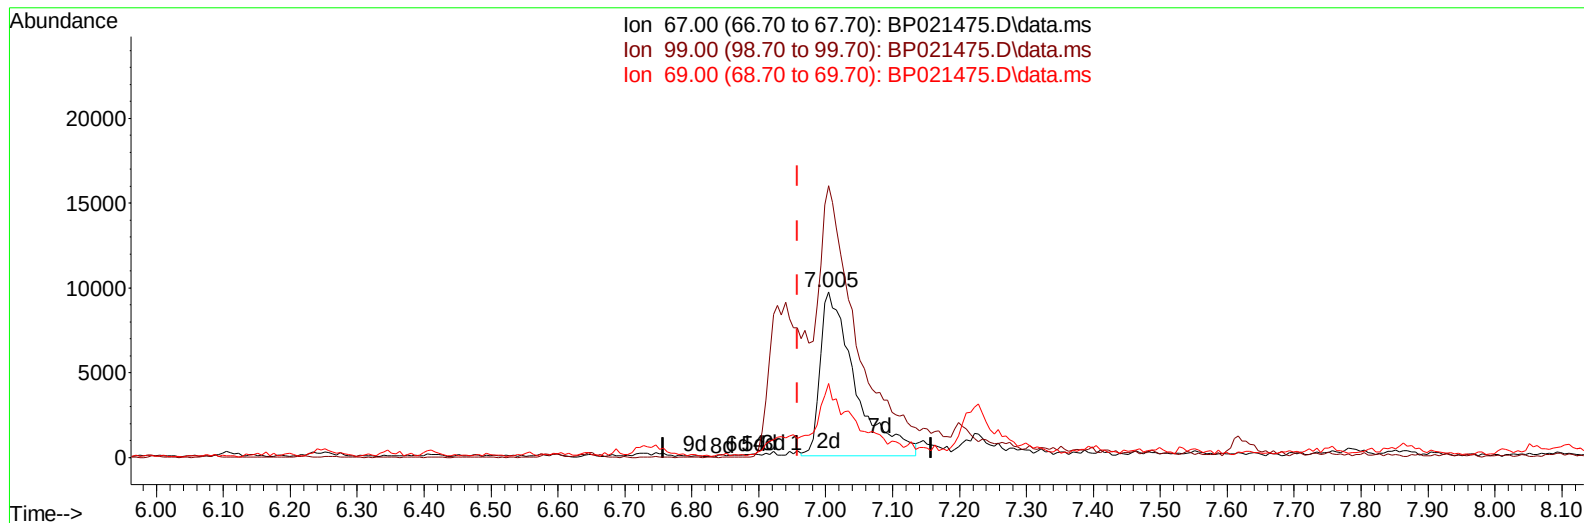

TIC: BP021475.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)

7.005min (+ 0.047) 4.79 ng/ul m

response 35285

Ion	Exp%	Act%
67.00	100.00	100.00
99.00	122.50	164.26#
69.00	30.60	44.81#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080824\
Data File : BP021475.D
Acq On : 09 Aug 2024 18:04
Operator : RC/JU
Sample : P3171-05MEDL 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :

BNA_P




ClientSampleId :

DCVW9MEDL

Manual IntegrationsAPPROVED

Quant Time: Aug 09 22:45:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 08 18:23:21 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/10/2024
Supervised By :mohammad ahmed 08/12/2024

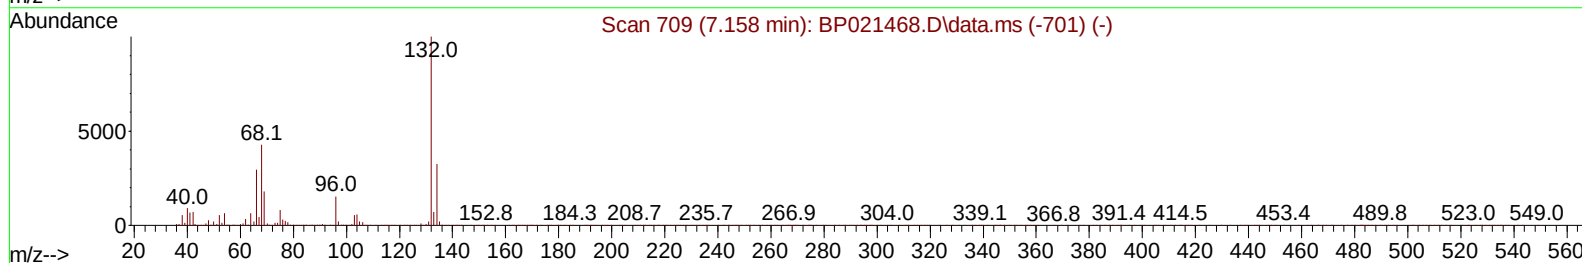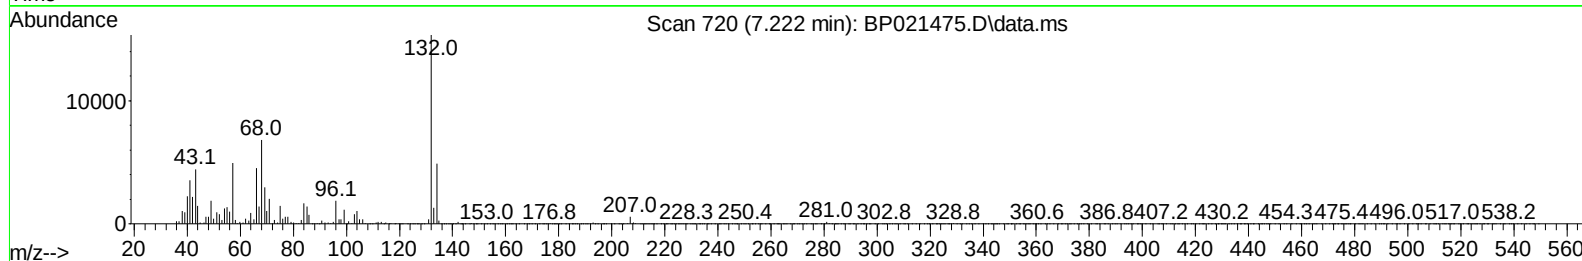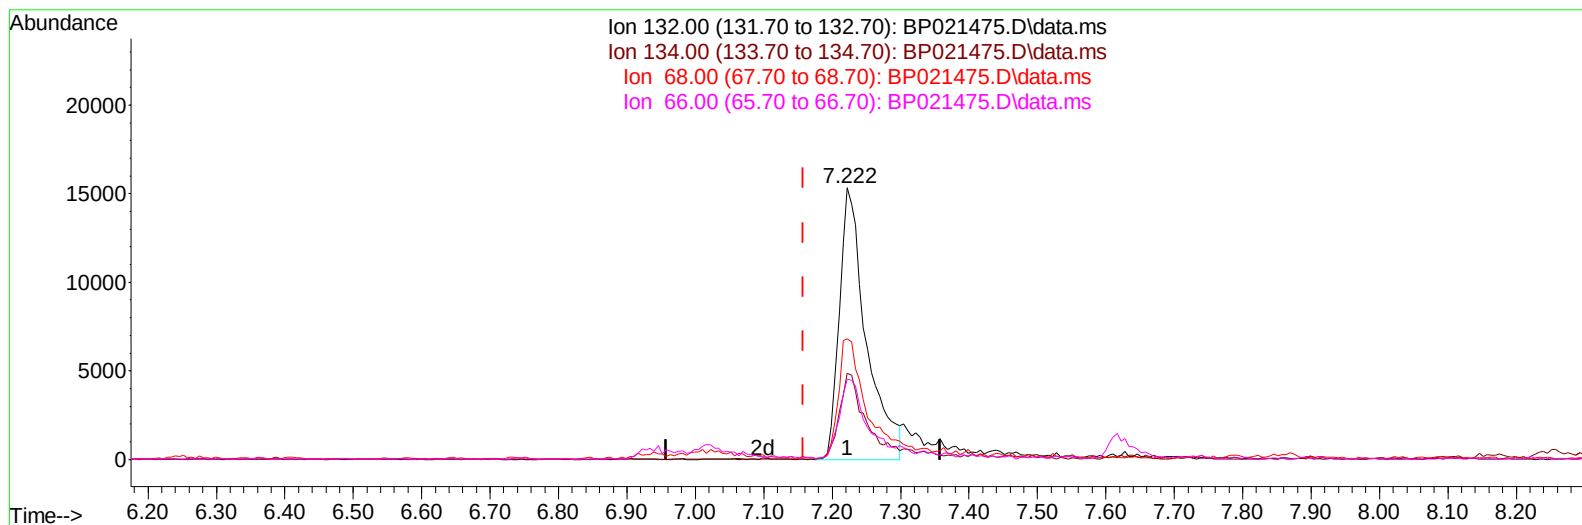

TIC: BP021475.D\data.ms

(11) 2-Chlorophenol-d4 (S)

7.222min (+ 0.065) 4.16 ng/uI

response 41659

Ion	Exp%	Act%
132.00	100.00	100.00
134.00	32.30	31.82
68.00	39.60	44.54
66.00	27.60	29.53




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080824\
Data File : BP021475.D
Acq On : 09 Aug 2024 18:04
Operator : RC/JU
Sample : P3171-05MEDL 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCVW9MEDL

Manual IntegrationsAPPROVED

Quant Time: Aug 09 22:45:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 08 18:23:21 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/10/2024
Supervised By :mohammad ahmed 08/12/2024

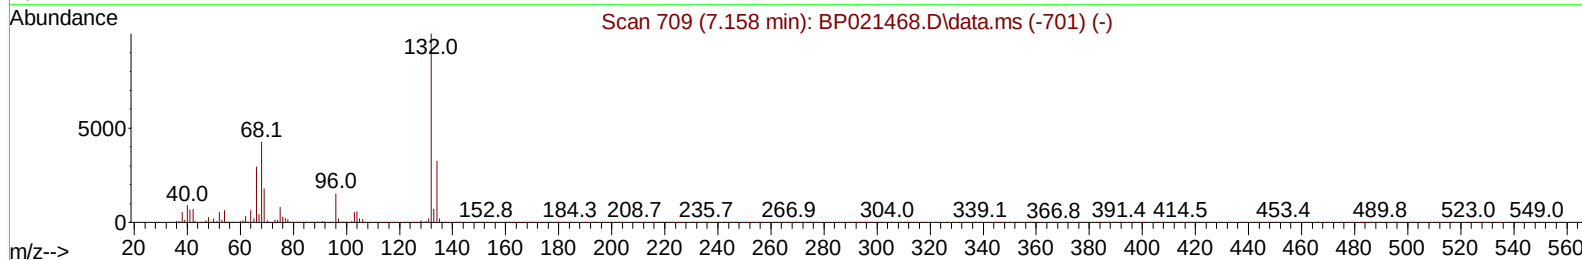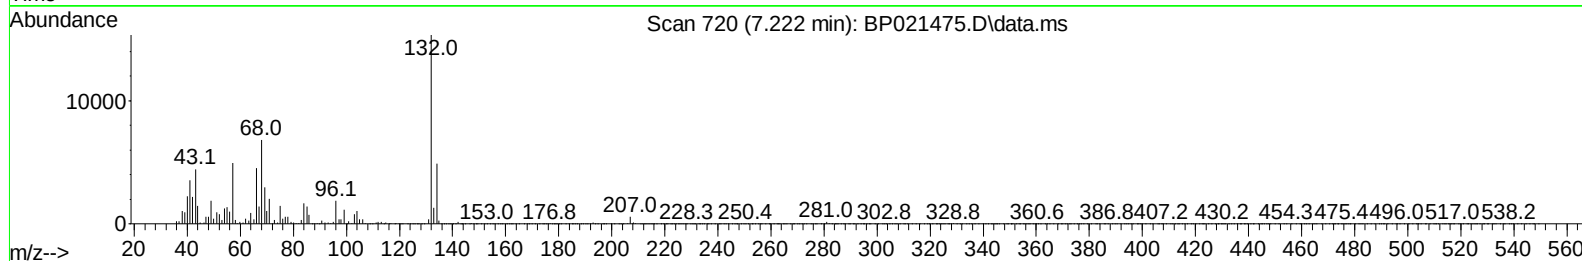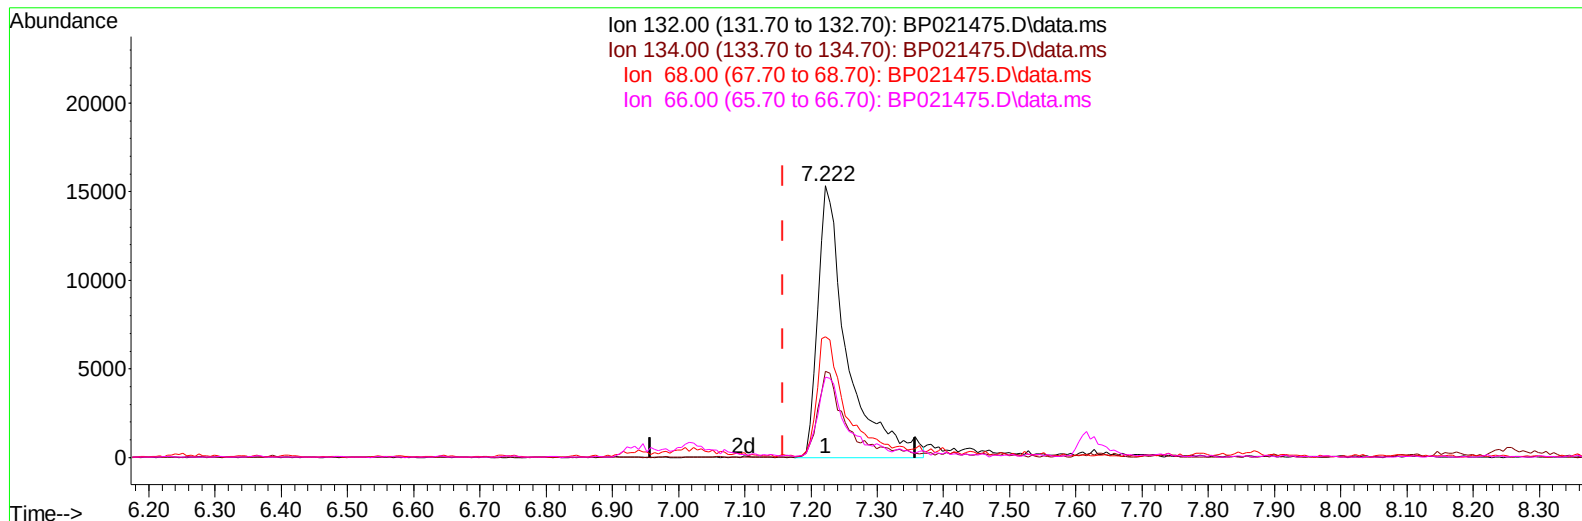

TIC: BP021475.D\data.ms

(11) 2-Chlorophenol-d4 (S)

7.222min (+ 0.065) 4.64 ng/ul m

response 46496

Ion	Exp%	Act%
132.00	100.00	100.00
134.00	32.30	31.82
68.00	39.60	44.54
66.00	27.60	29.53

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080824\
Data File : BP021475.D
Acq On : 09 Aug 2024 18:04
Operator : RC/JU
Sample : P3171-05MEDL 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :

BNA_P




ClientSampleId :

DCVW9MEDL

Manual IntegrationsAPPROVED

Quant Time: Aug 09 22:45:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 08 18:23:21 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/10/2024
Supervised By :mohammad ahmed 08/12/2024

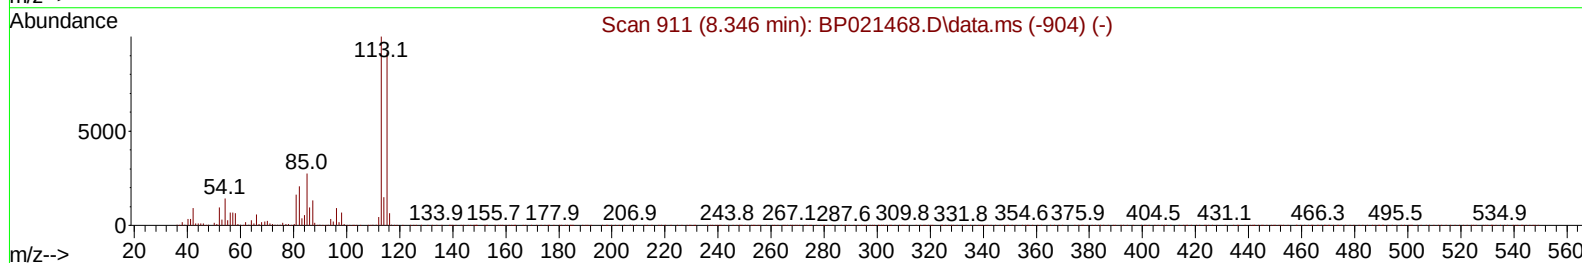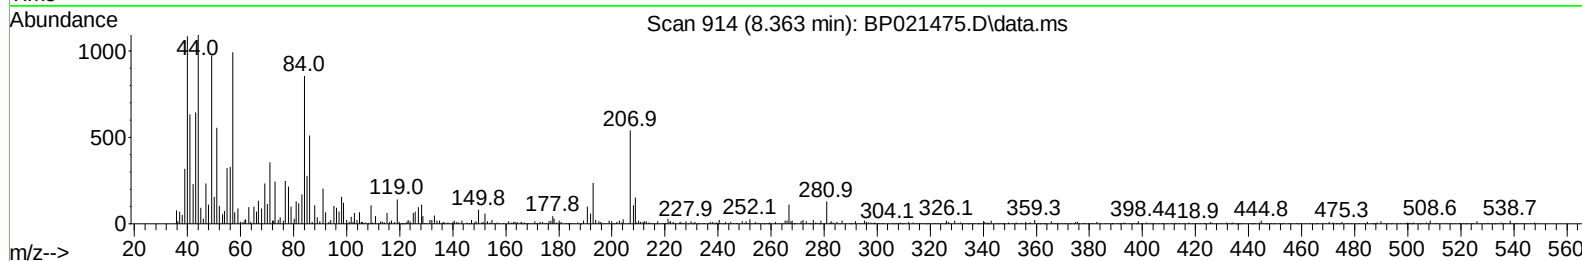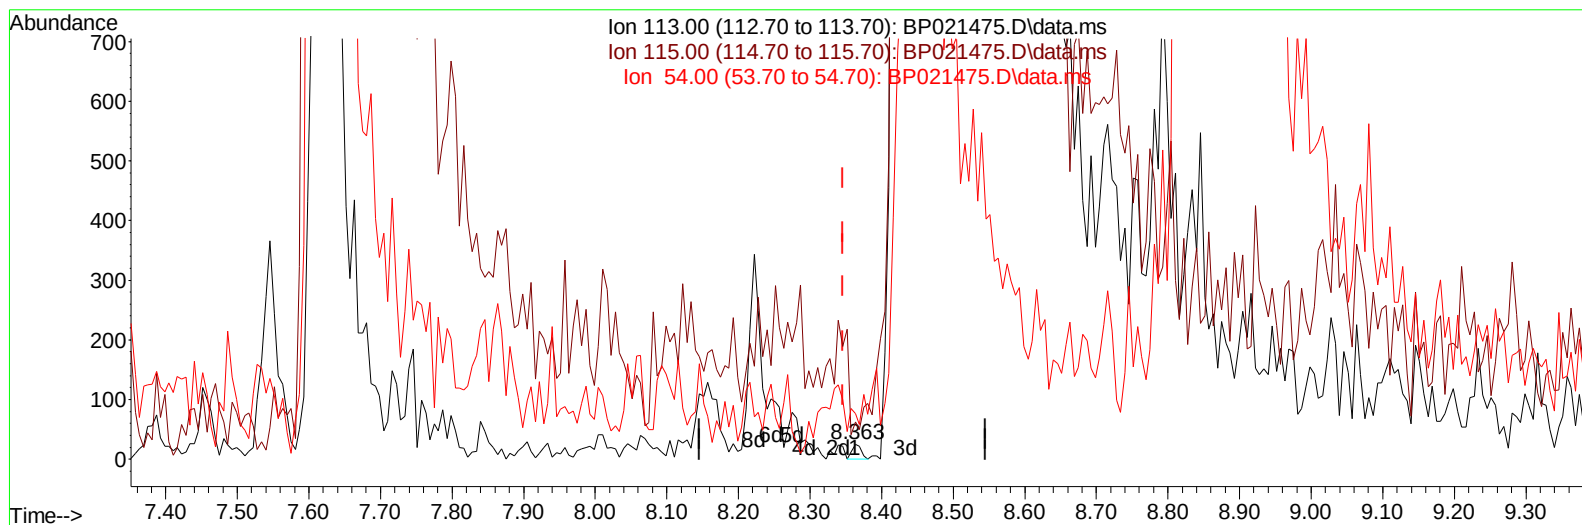

TIC: BP021475.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.363min (+ 0.018) 0.00 ng/u1

response 23

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	93.20	248.00#
54.00	13.70	304.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080824\
Data File : BP021475.D
Acq On : 09 Aug 2024 18:04
Operator : RC/JU
Sample : P3171-05MEDL 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCVW9MEDL

Manual IntegrationsAPPROVED

Quant Time: Aug 09 22:45:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 08 18:23:21 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/10/2024
Supervised By :mohammad ahmed 08/12/2024

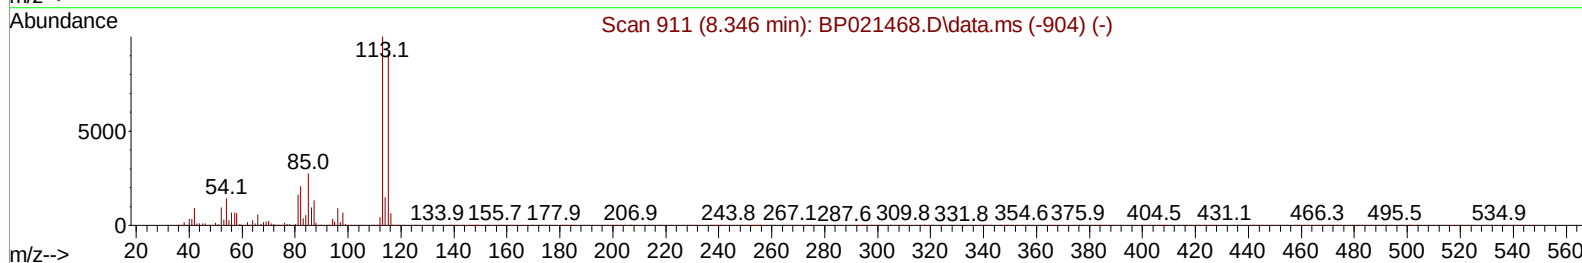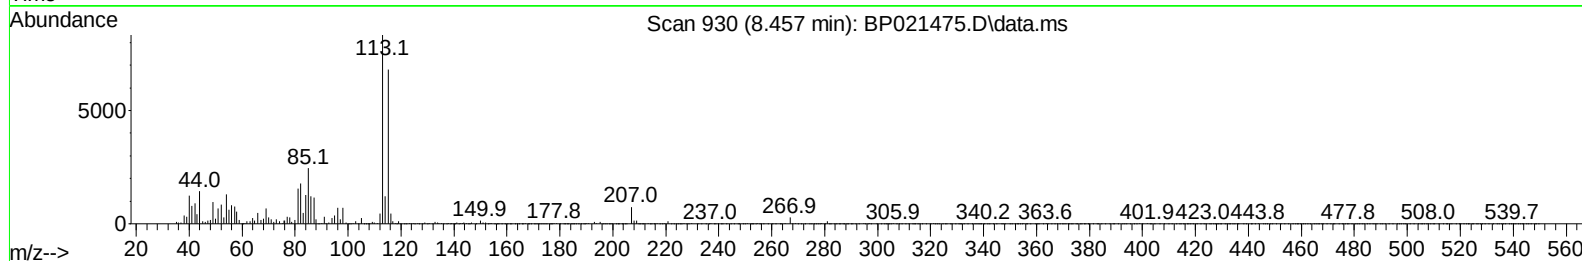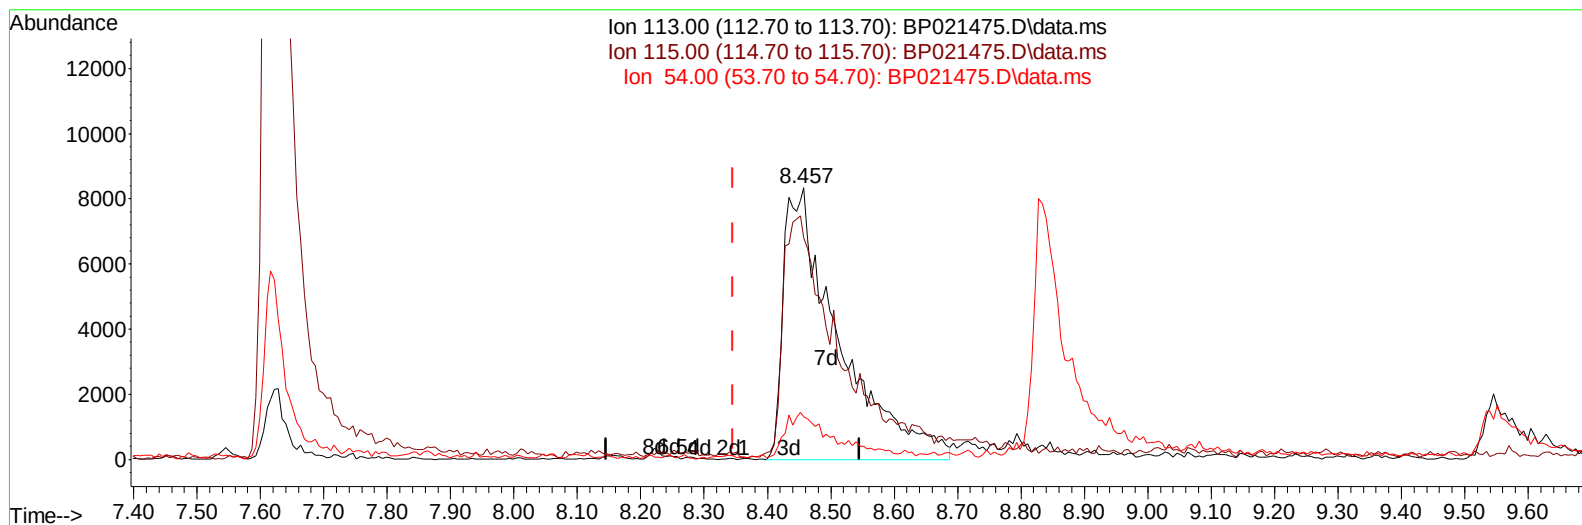

TIC: BP021475.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.457min (+ 0.112) 4.98 ng/u1 m

response 50281

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	93.20	81.69
54.00	13.70	15.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080824\
 Data File : BP021475.D
 Acq On : 09 Aug 2024 18:04
 Operator : RC/JU
 Sample : P3171-05MEDL 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :

BNA_P




ClientSampleId :

DCVW9MEDL

Manual IntegrationsAPPROVED

Quant Time: Aug 09 23:02:54 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 08 18:23:21 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/10/2024
 Supervised By :mohammad ahmed 08/12/2024

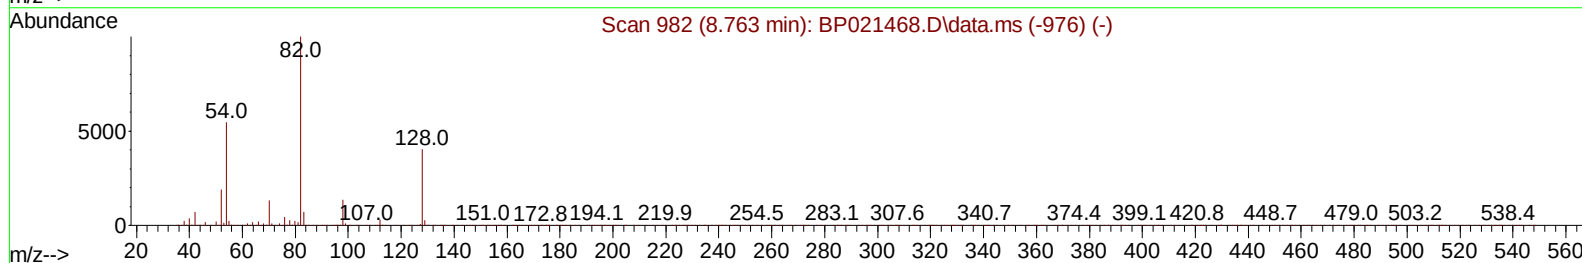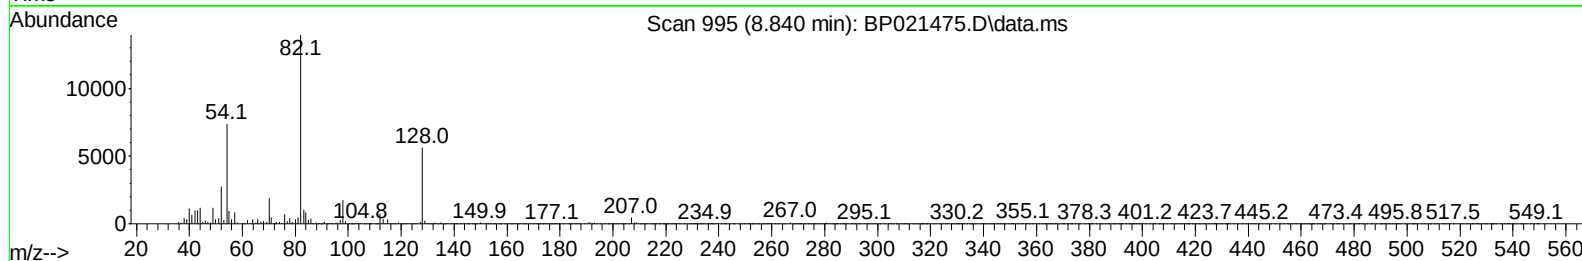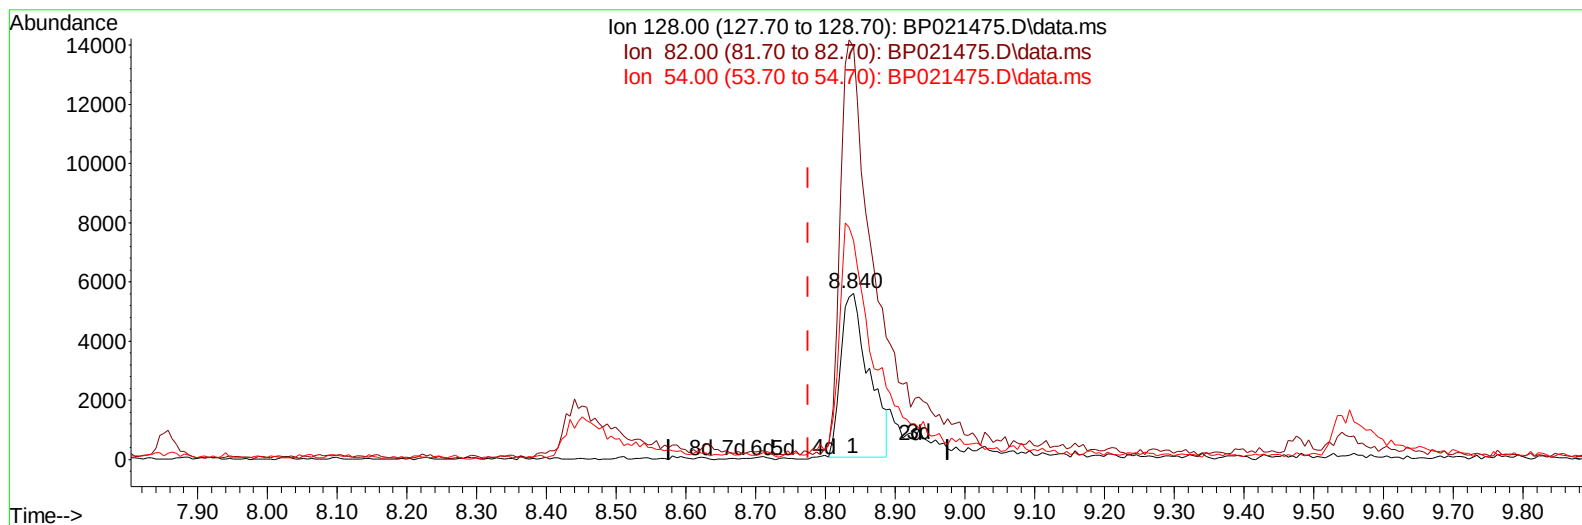

TIC: BP021475.D\data.ms

(21) Nitrobenzene-d5 (S)

8.840min (+ 0.065) 3.50 ng/u1

response 15563

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	236.60	248.34
54.00	125.70	131.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080824\
Data File : BP021475.D
Acq On : 09 Aug 2024 18:04
Operator : RC/JU
Sample : P3171-05MEDL 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :

BNA_P




ClientSampleId :

DCVW9MEDL

Manual IntegrationsAPPROVED

Quant Time: Aug 09 23:02:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 08 18:23:21 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/10/2024
Supervised By :mohammad ahmed 08/12/2024

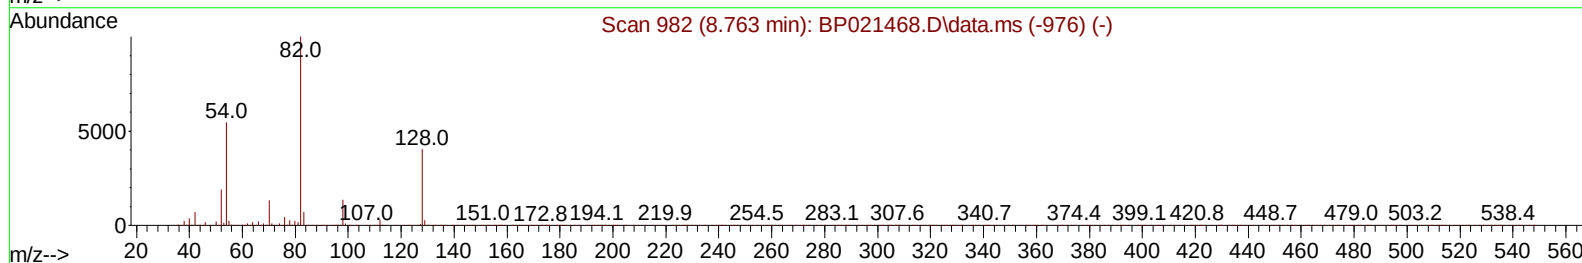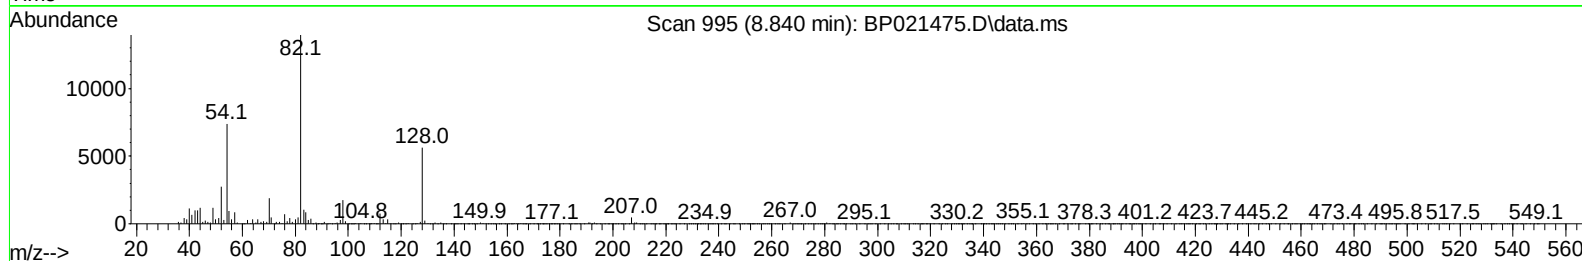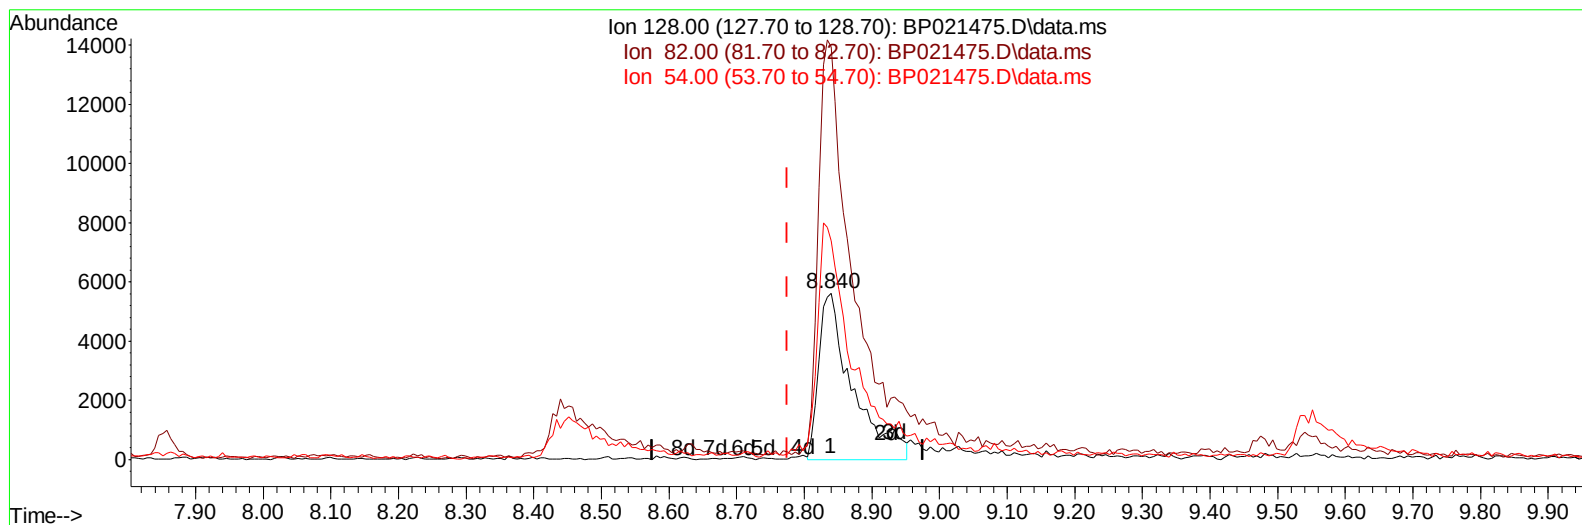

TIC: BP021475.D\data.ms

(21) Nitrobenzene-d5 (S)

8.840min (+ 0.065) 4.38 ng/ul m

response 19514

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	236.60	248.34
54.00	125.70	131.59
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080824\
Data File : BP021475.D
Acq On : 09 Aug 2024 18:04
Operator : RC/JU
Sample : P3171-05MEDL 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCVW9MEDL

Manual IntegrationsAPPROVED

Quant Time: Aug 09 23:02:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 08 18:23:21 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/10/2024
Supervised By :mohammad ahmed 08/12/2024

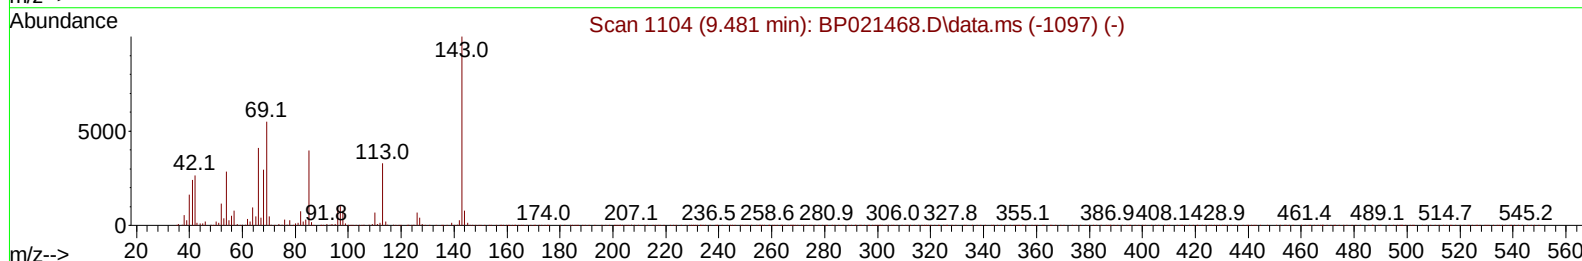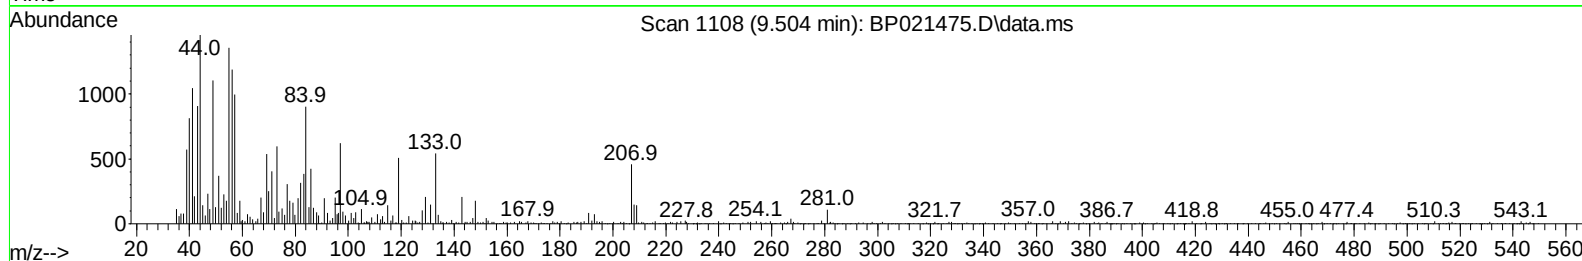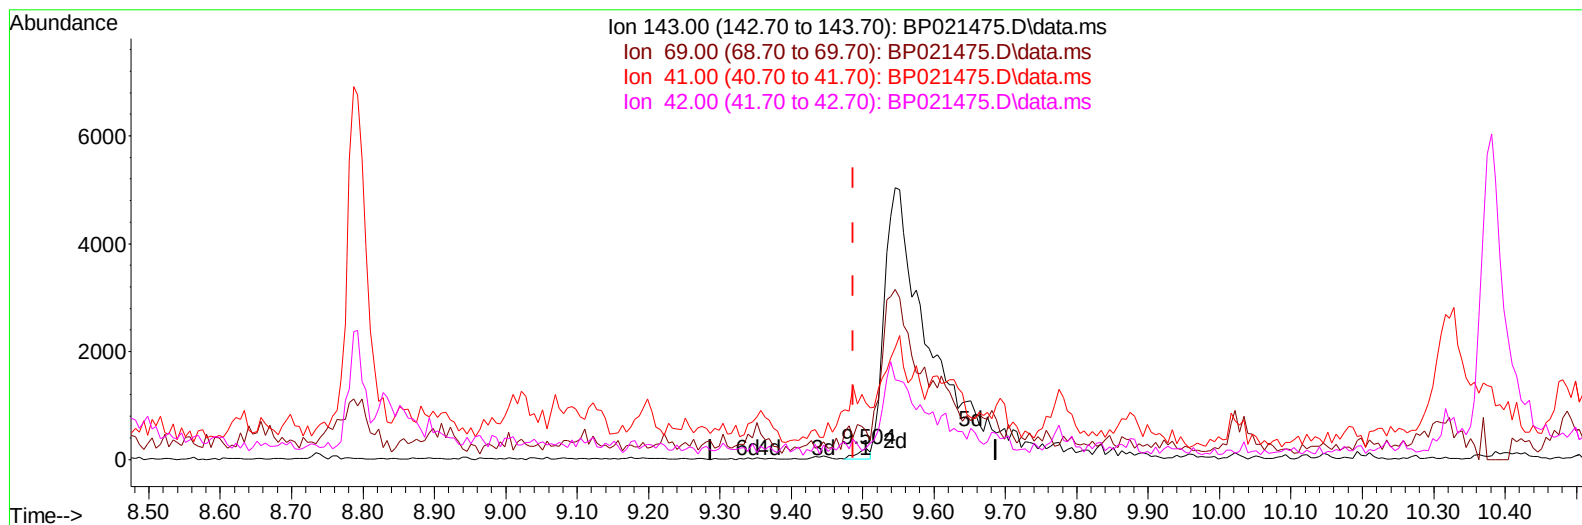

TIC: BP021475.D\data.ms

(24) 2-Nitrophenol-d4 (S)

9.504min (+ 0.018) 0.05 ng/u1

response 259

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	50.20	262.44#
41.00	22.70	510.24#
42.00	22.10	102.44#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080824\
Data File : BP021475.D
Acq On : 09 Aug 2024 18:04
Operator : RC/JU
Sample : P3171-05MEDL 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCVW9MEDL

Manual IntegrationsAPPROVED

Quant Time: Aug 09 23:02:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 08 18:23:21 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/10/2024
Supervised By :mohammad ahmed 08/12/2024

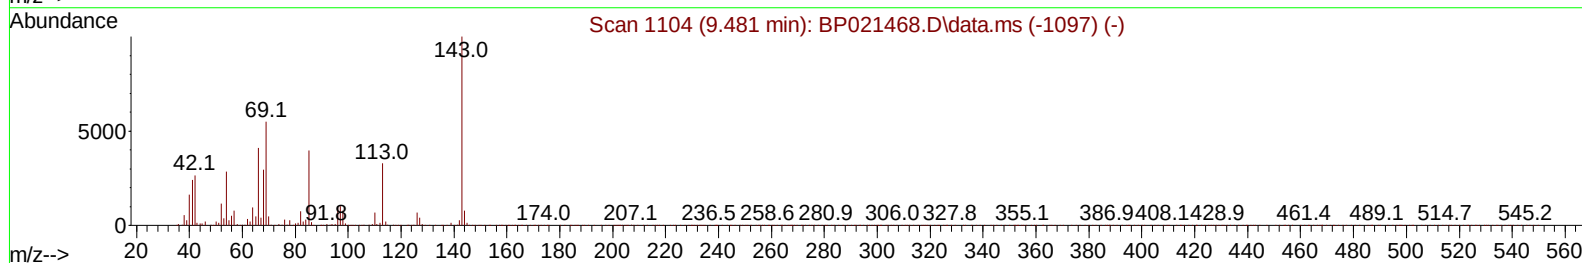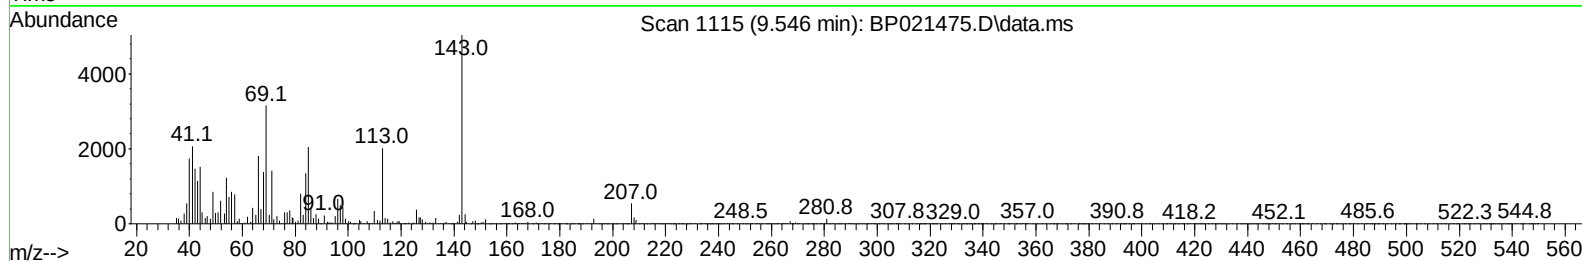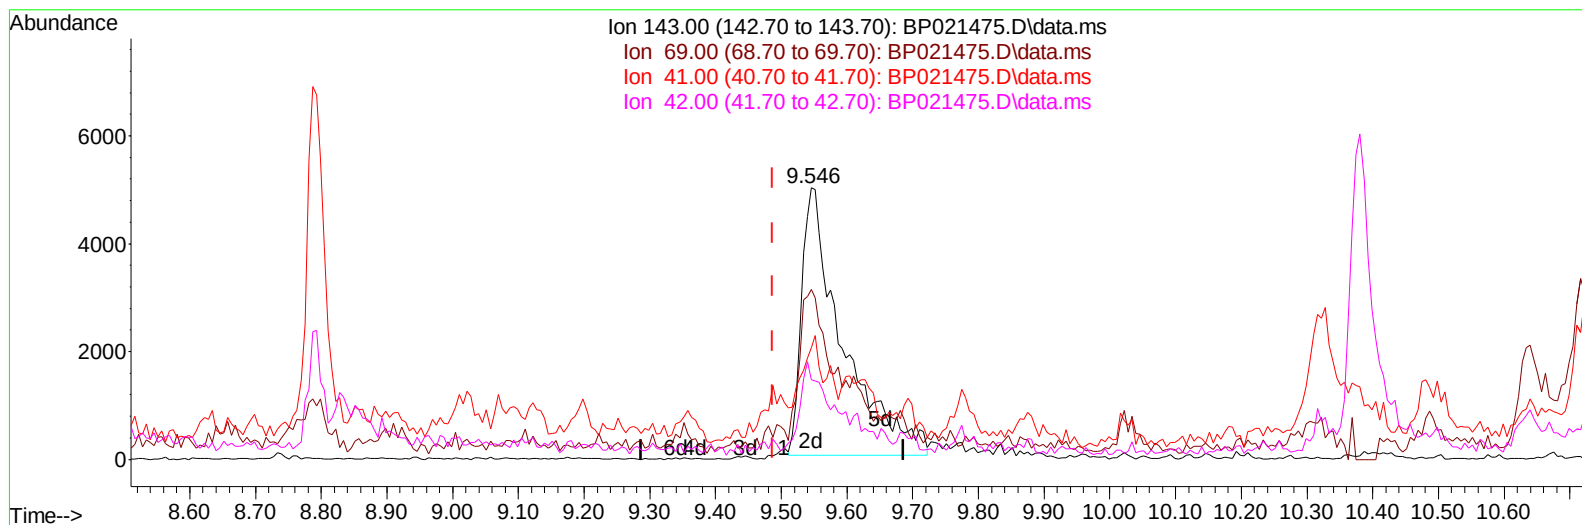

TIC: BP021475.D\data.ms

(24) 2-Nitrophenol-d4 (S)

9.546min (+ 0.059) 4.24 ng/ul m

response 21607

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	50.20	62.58#
41.00	22.70	41.11#
42.00	22.10	29.31#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080824\
 Data File : BP021475.D
 Acq On : 09 Aug 2024 18:04
 Operator : RC/JU
 Sample : P3171-05MEDL 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCVW9MEDL

Manual IntegrationsAPPROVED

Quant Time: Aug 09 23:02:54 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 08 18:23:21 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/10/2024
 Supervised By :mohammad ahmed 08/12/2024

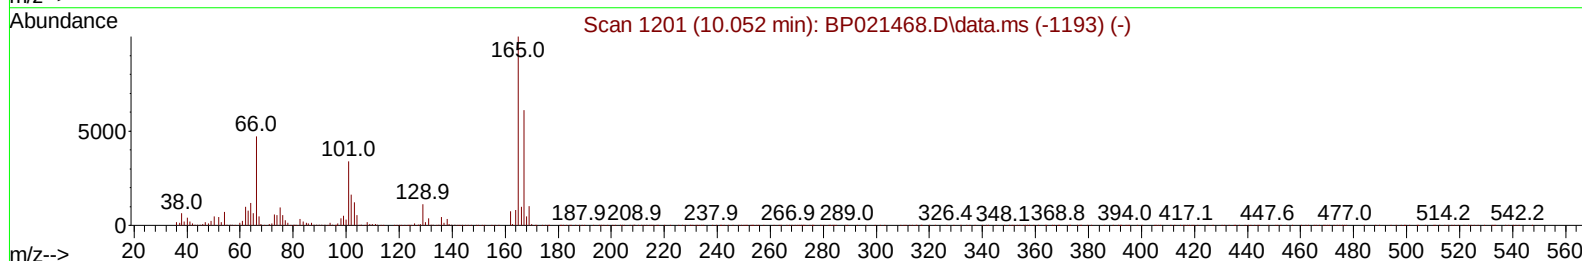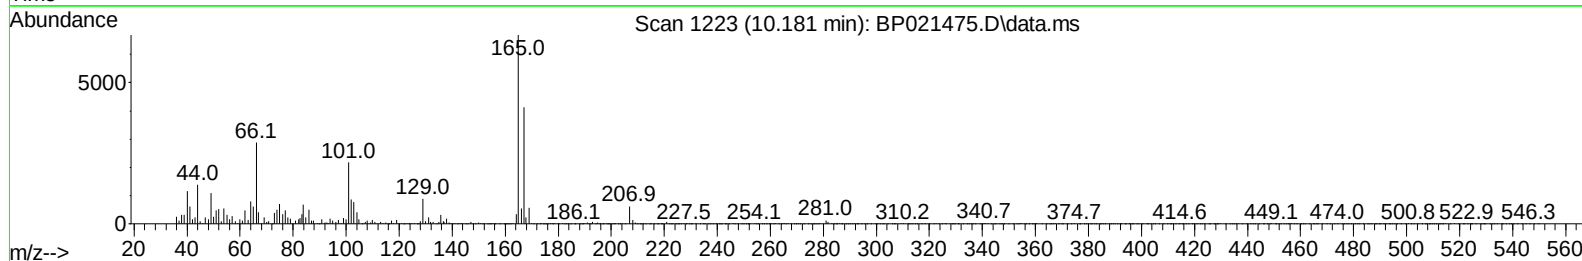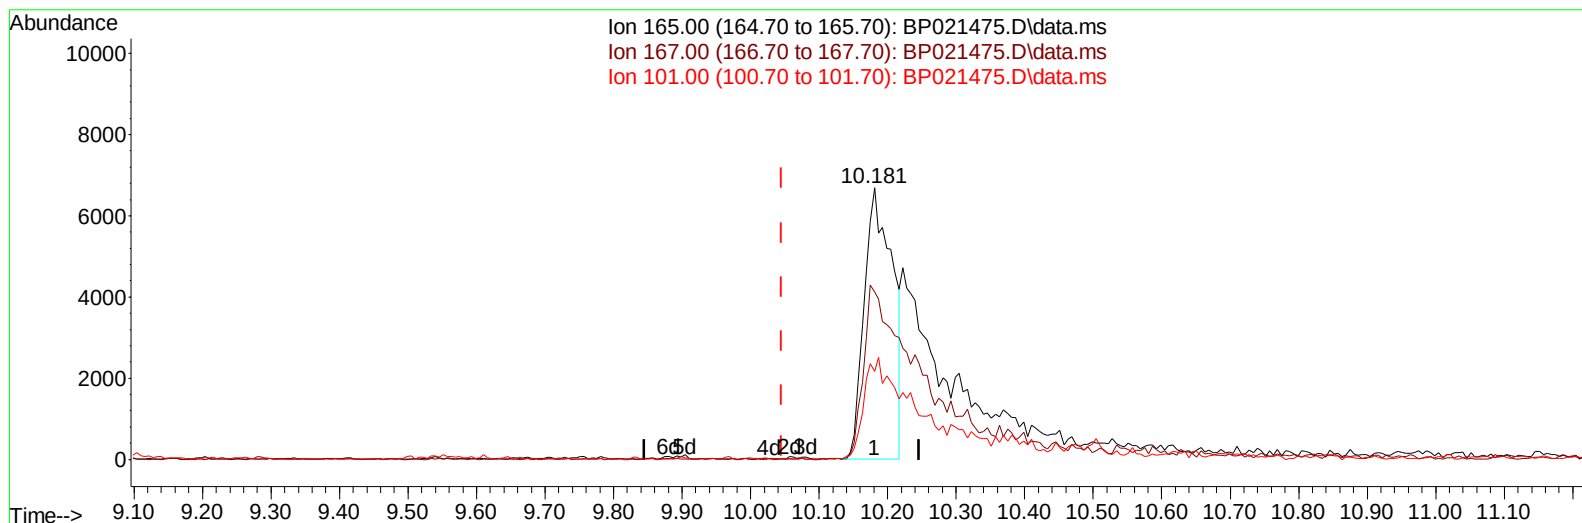

TIC: BP021475.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.181min (+ 0.135) 2.05 ng/ul

response 18912

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	62.80	61.72
101.00	35.50	32.47
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080824\
 Data File : BP021475.D
 Acq On : 09 Aug 2024 18:04
 Operator : RC/JU
 Sample : P3171-05MEDL 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCVW9MEDL

Manual IntegrationsAPPROVED

Quant Time: Aug 09 23:02:54 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 08 18:23:21 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/10/2024
 Supervised By :mohammad ahmed 08/12/2024

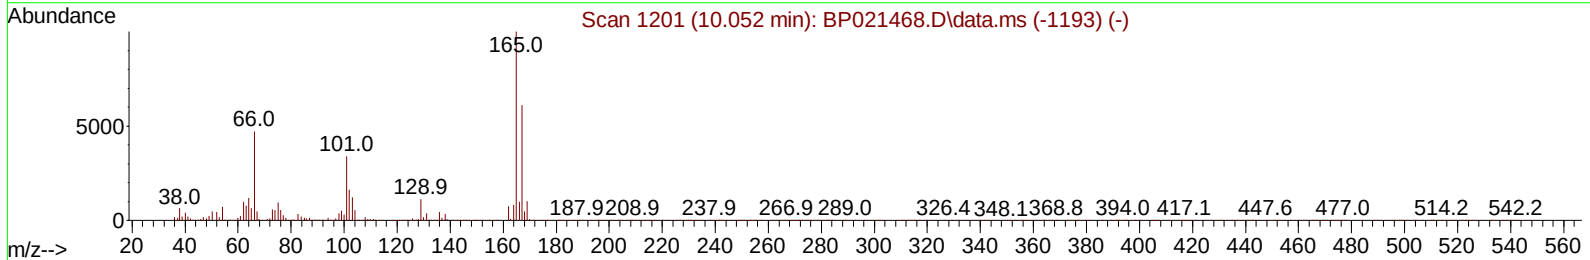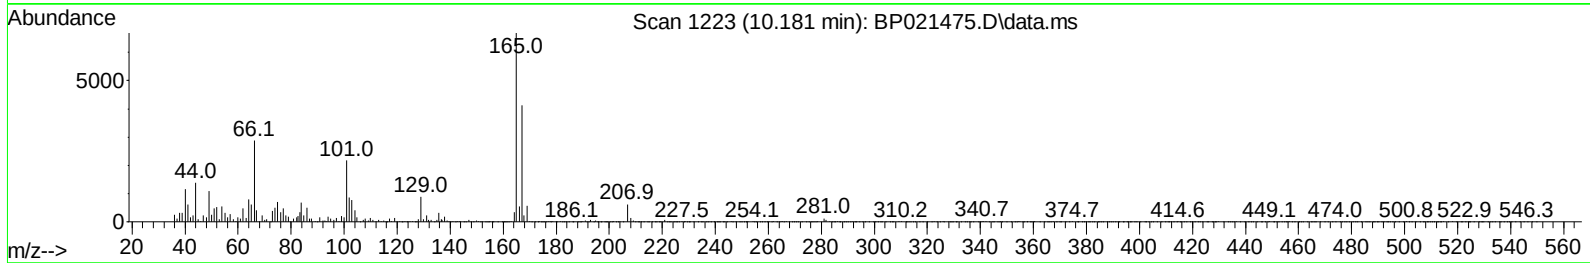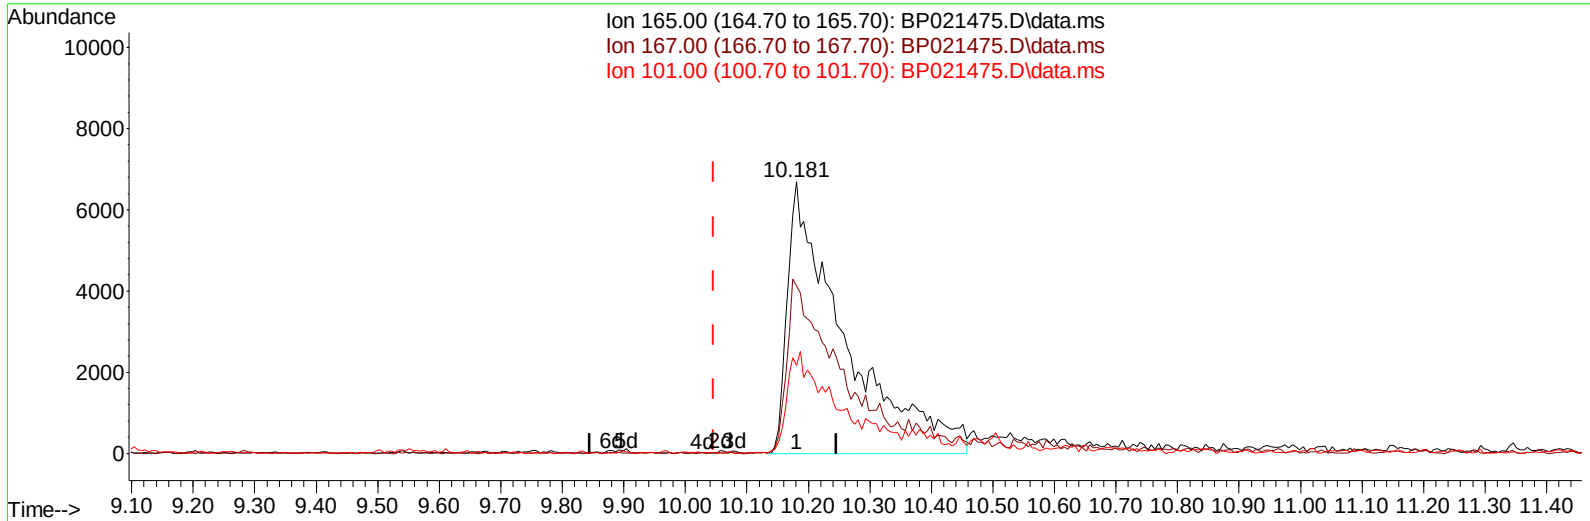

TIC: BP021475.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.181min (+ 0.135) 4.66 ng/ul m

response 42909

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	62.80	61.72
101.00	35.50	32.47
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080824\
Data File : BP021475.D
Acq On : 09 Aug 2024 18:04
Operator : RC/JU
Sample : P3171-05MEDL 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCVW9MEDL

Manual IntegrationsAPPROVED

Quant Time: Aug 09 23:02:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 08 18:23:21 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/10/2024
Supervised By :mohammad ahmed 08/12/2024

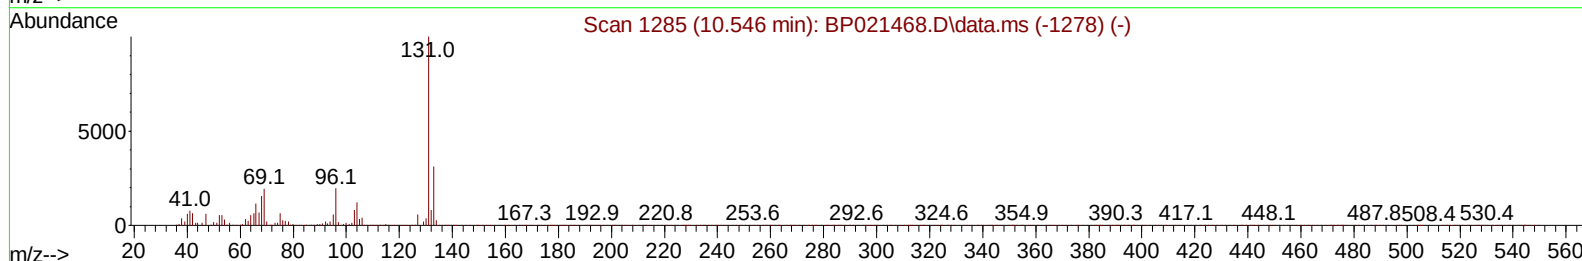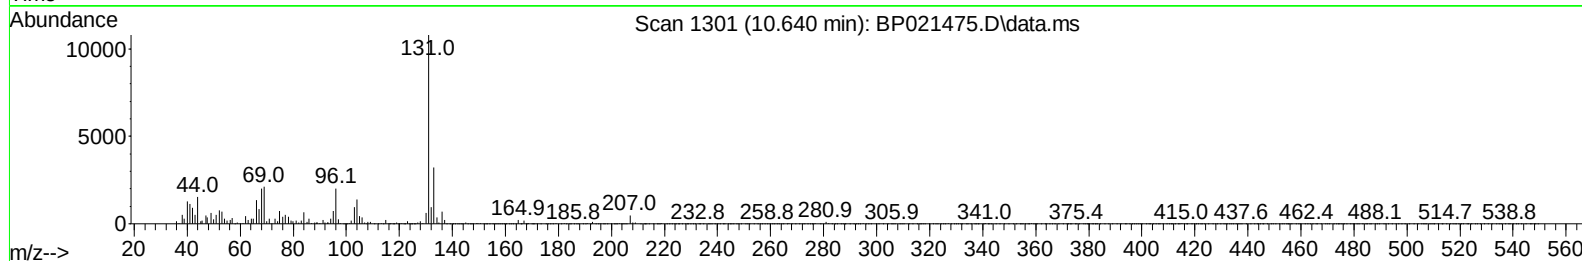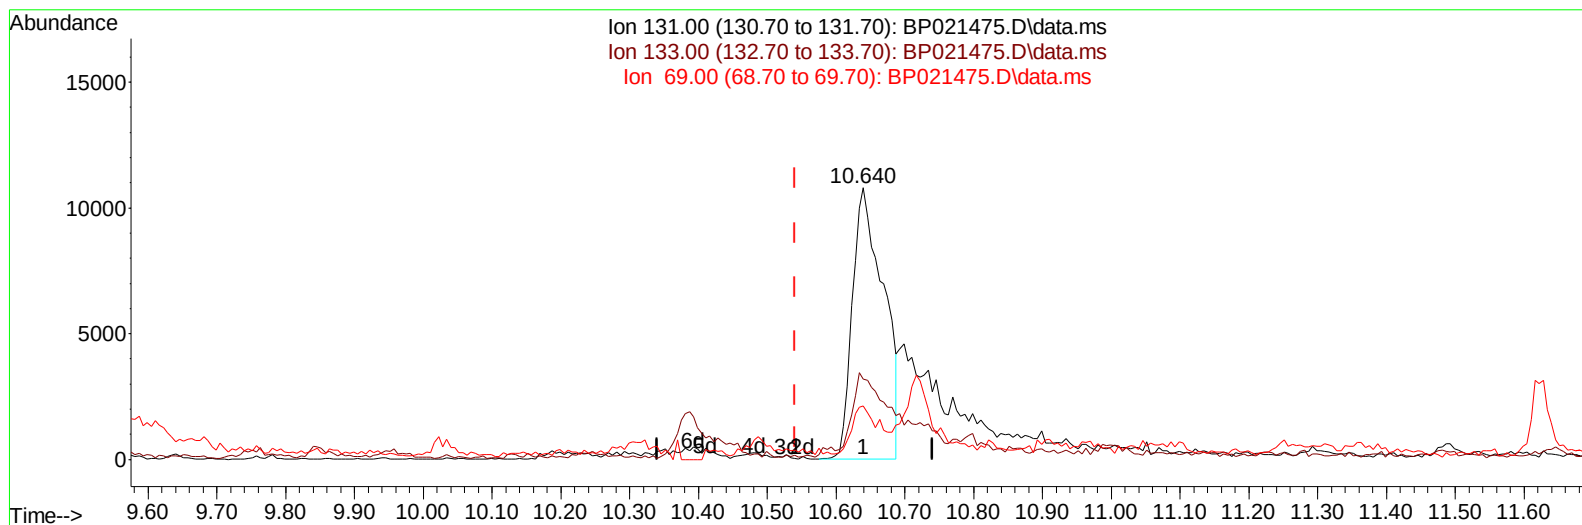

TIC: BP021475.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.640min (+ 0.100) 2.77 ng/u1

response 33749

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.50	29.68
69.00	17.40	19.66
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080824\
 Data File : BP021475.D
 Acq On : 09 Aug 2024 18:04
 Operator : RC/JU
 Sample : P3171-05MEDL 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCVW9MEDL

Manual IntegrationsAPPROVED

Quant Time: Aug 09 23:02:54 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 08 18:23:21 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/10/2024
 Supervised By :mohammad ahmed 08/12/2024

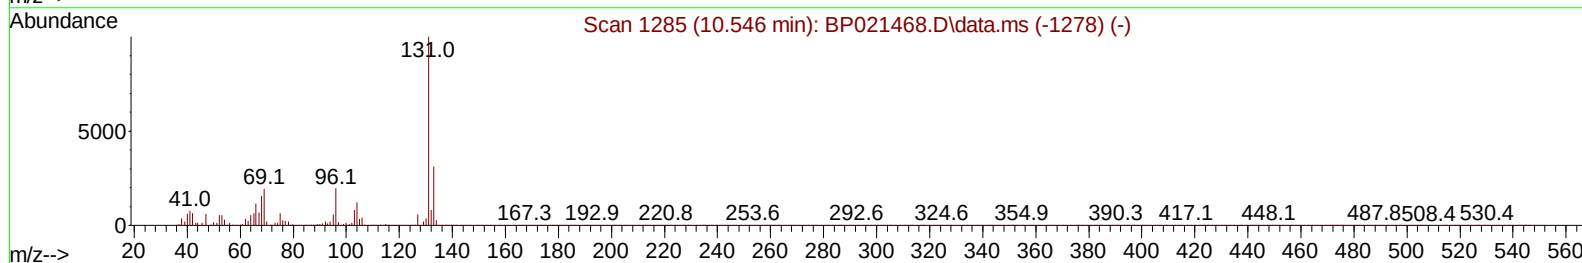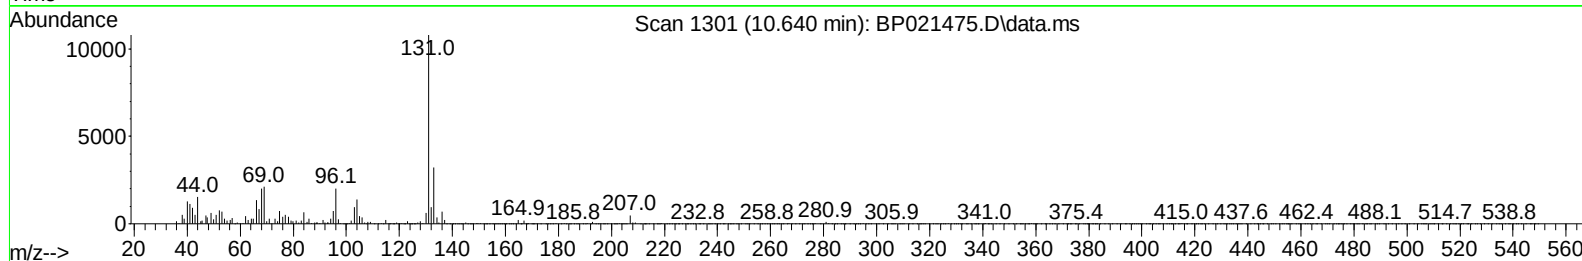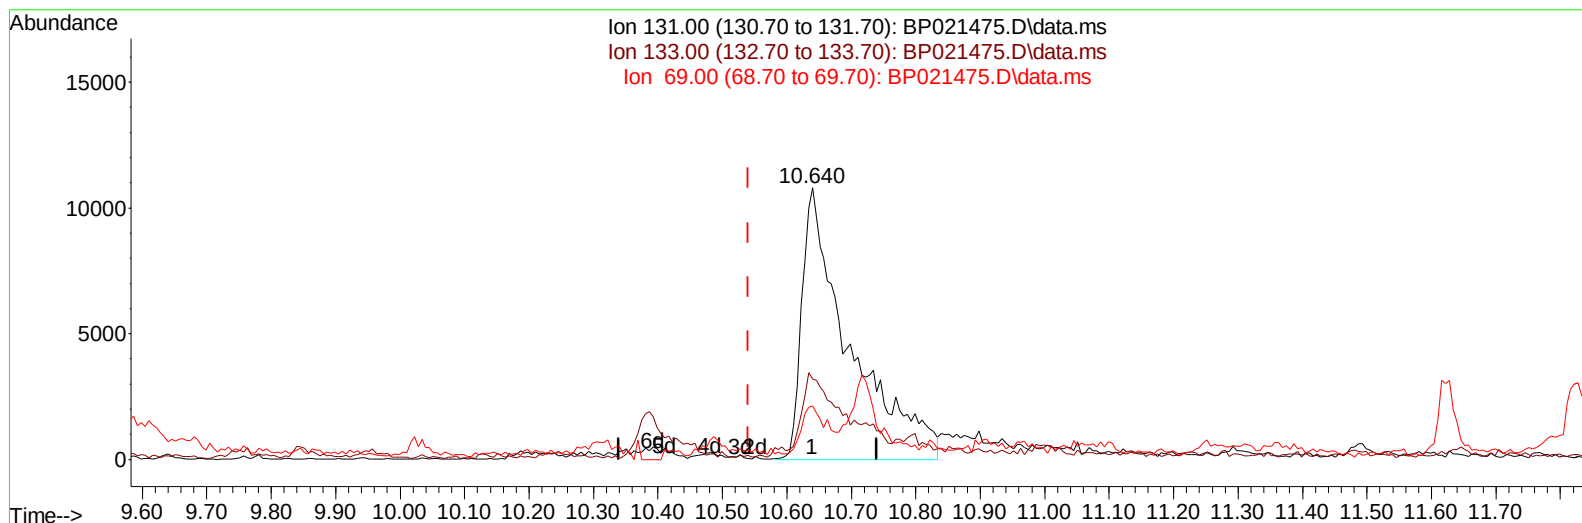

TIC: BP021475.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.640min (+ 0.100) 4.54 ng/ul m

response 55355

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.50	29.68
69.00	17.40	19.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080824\
 Data File : BP021475.D
 Acq On : 09 Aug 2024 18:04
 Operator : RC/JU
 Sample : P3171-05MEDL 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :

BNA_P




ClientSampleId :

DCVW9MEDL

Manual IntegrationsAPPROVED

Quant Time: Aug 09 23:05:24 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 08 18:23:21 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/10/2024
 Supervised By :mohammad ahmed 08/12/2024

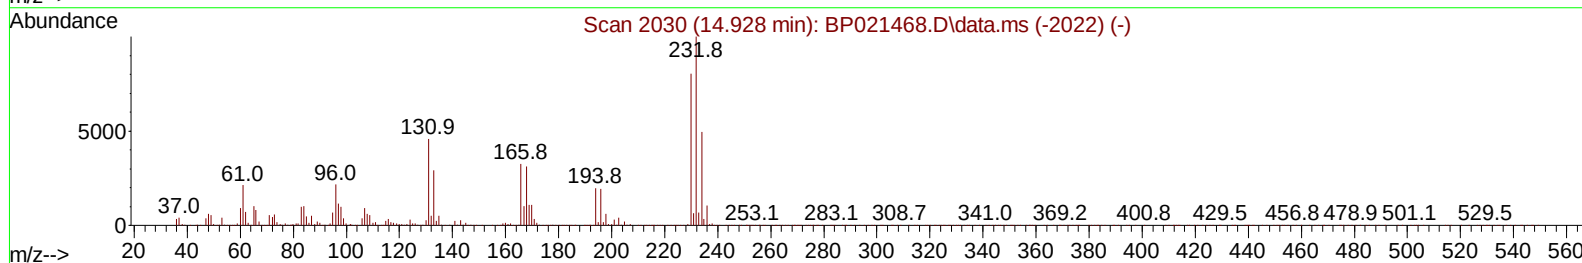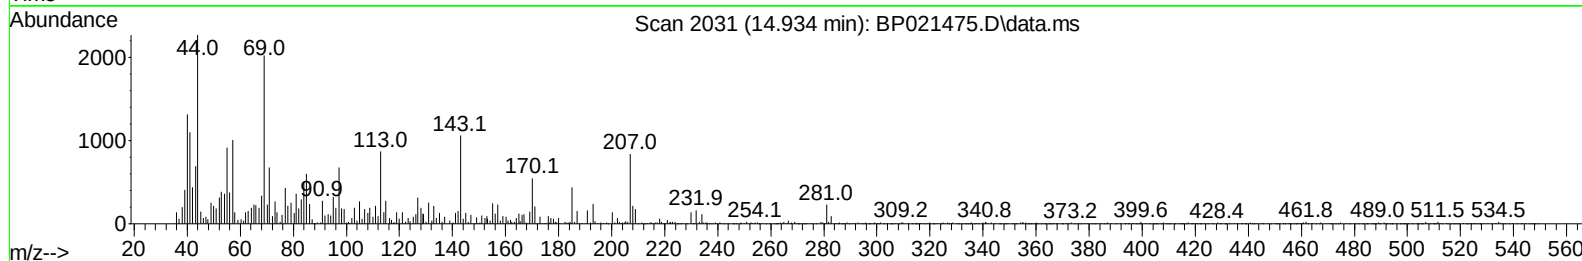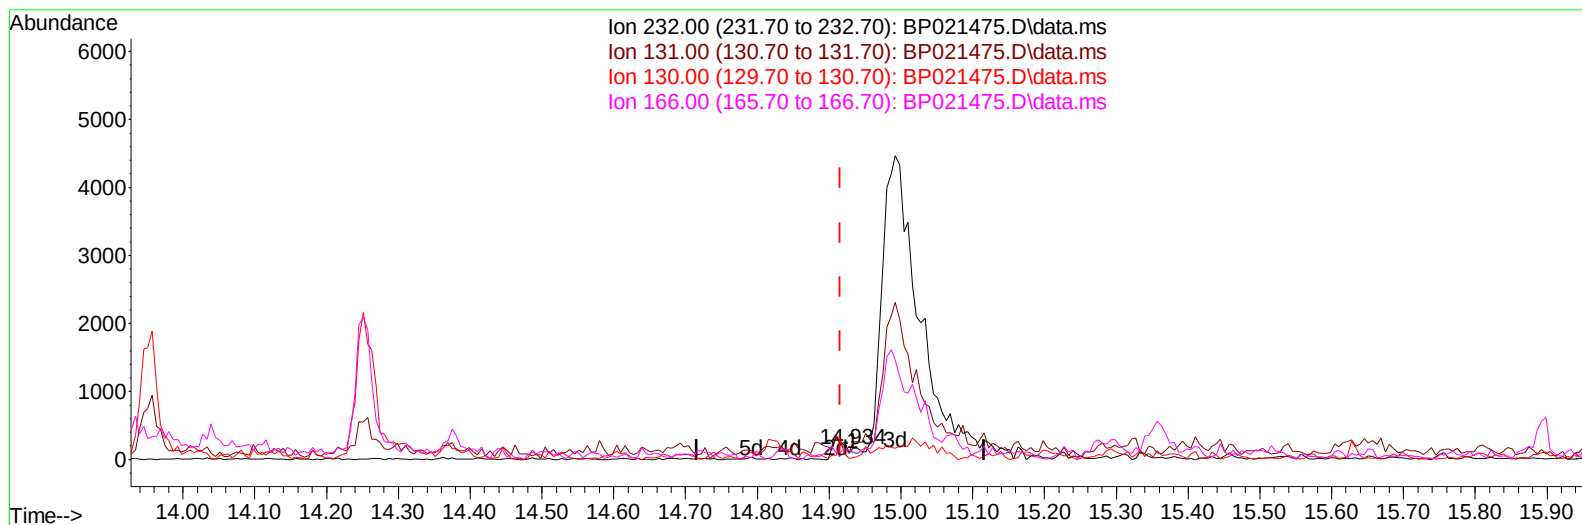

TIC: BP021475.D\data.ms

(58) 2,3,4,6-Tetrachlorophenol

14.934min (+ 0.018) 0.01 ng/uI

response 55

Ion	Exp%	Act%
232.00	100.00	100.00
131.00	43.00	156.71#
130.00	2.50	14.02#
166.00	30.50	65.24#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080824\
 Data File : BP021475.D
 Acq On : 09 Aug 2024 18:04
 Operator : RC/JU
 Sample : P3171-05MEDL 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :

BNA_P




ClientSampleId :

DCVW9MEDL

Manual IntegrationsAPPROVED

Quant Time: Aug 09 23:05:24 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 08 18:23:21 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/10/2024
 Supervised By :mohammad ahmed 08/12/2024

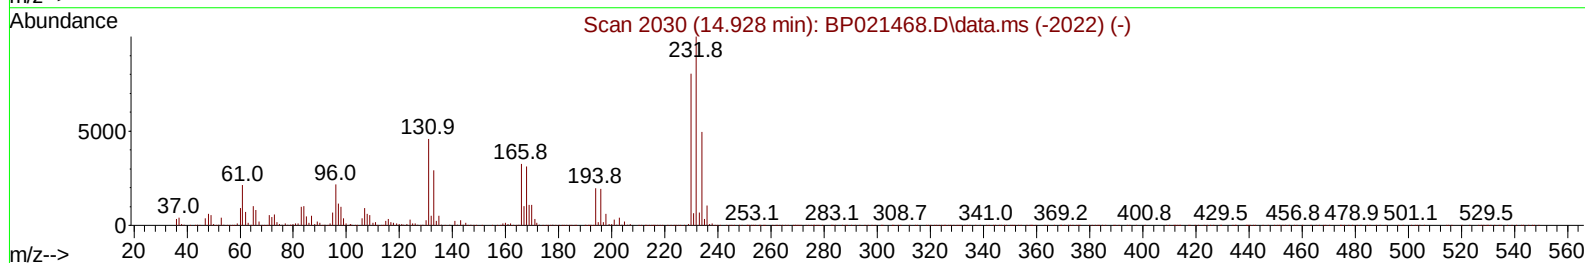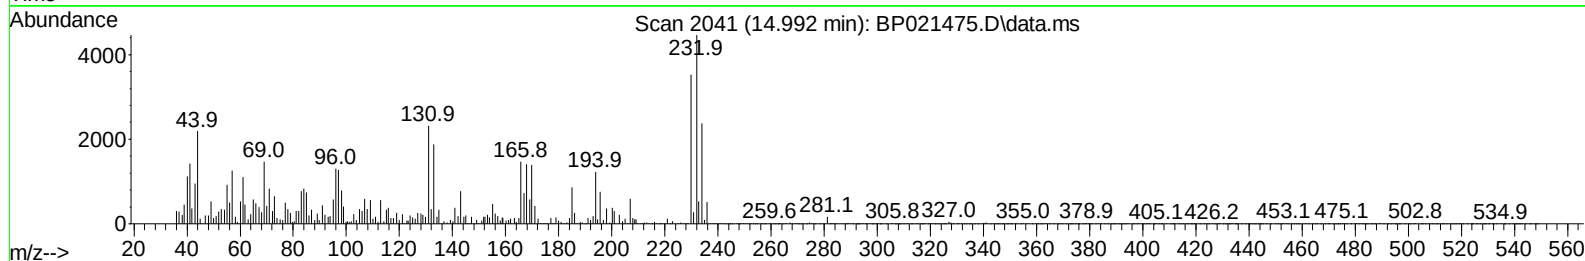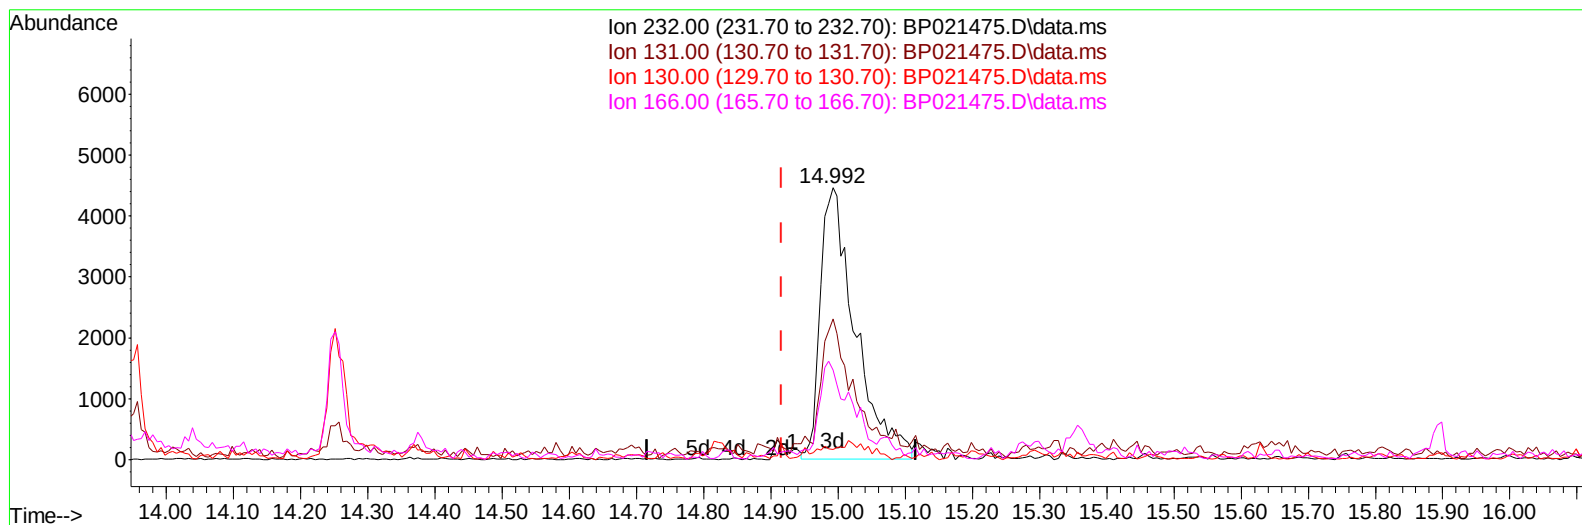

TIC: BP021475.D\data.ms

(58) 2,3,4,6-Tetrachlorophenol

14.992min (+ 0.076) 2.13 ng/ul m

response 16082

Ion	Exp%	Act%
232.00	100.00	100.00
131.00	43.00	51.87#
130.00	2.50	3.72#
166.00	30.50	32.83




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080824\
Data File : BP021475.D
Acq On : 09 Aug 2024 18:04
Operator : RC/JU
Sample : P3171-05MEDL 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCVW9MEDL

Manual IntegrationsAPPROVED

Quant Time: Aug 09 23:06:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 08 18:23:21 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/10/2024
Supervised By :mohammad ahmed 08/12/2024

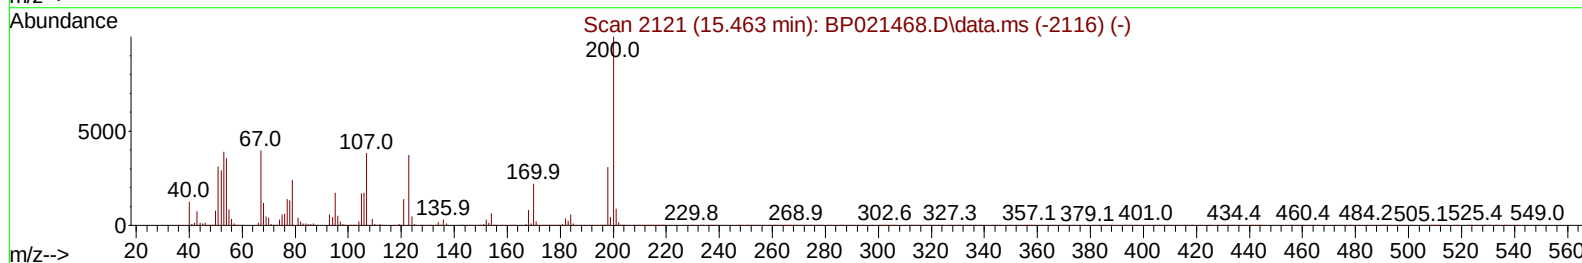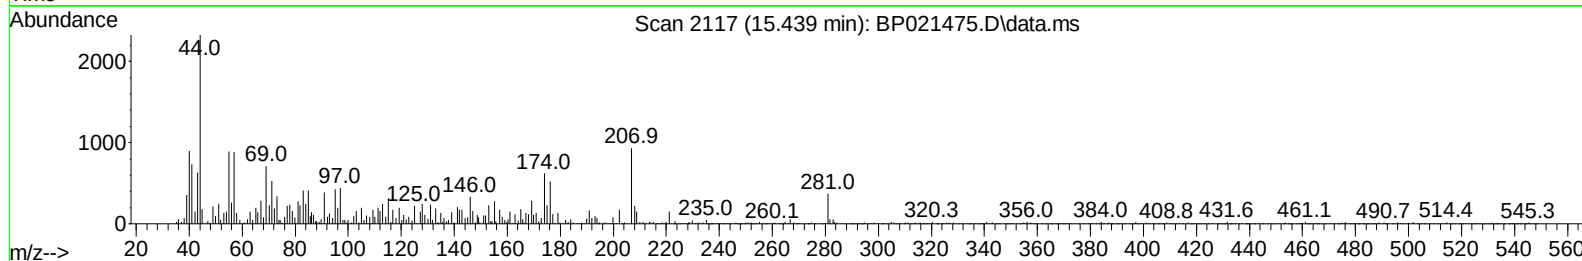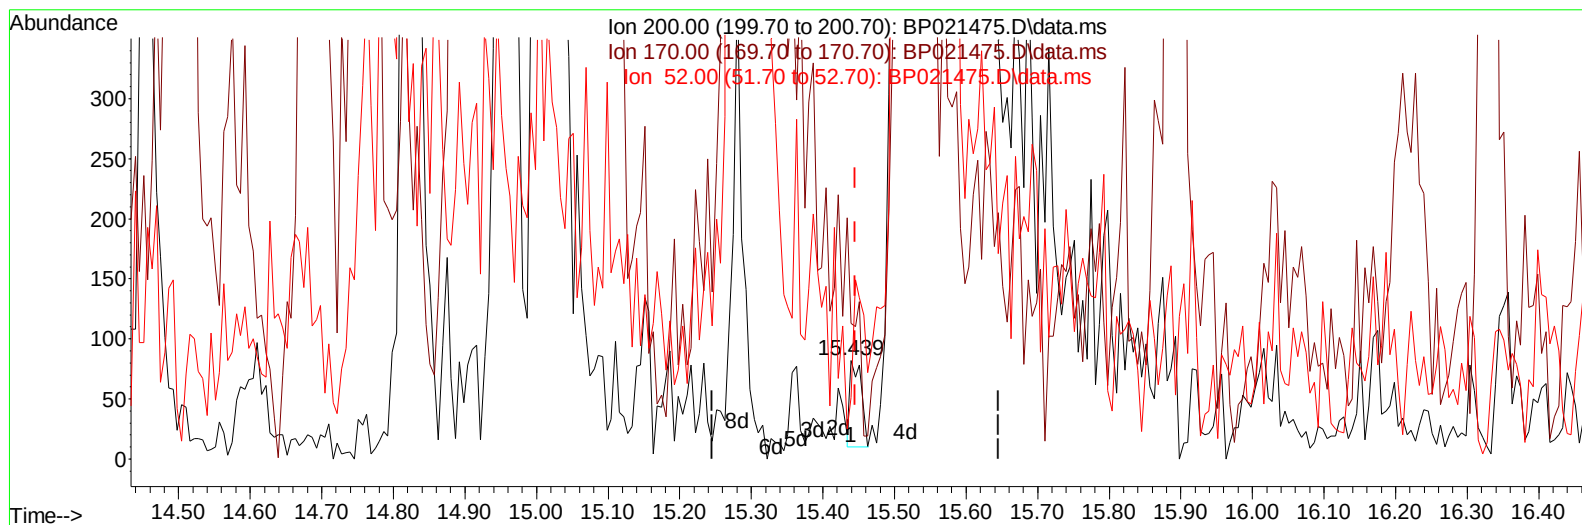

TIC: BP021475.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.439min (-0.006) 0.02 ng/ul

response 80

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	21.00	137.80#
52.00	38.50	62.20#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080824\
Data File : BP021475.D
Acq On : 09 Aug 2024 18:04
Operator : RC/JU
Sample : P3171-05MEDL 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCVW9MEDL

Manual IntegrationsAPPROVED

Quant Time: Aug 09 23:06:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 08 18:23:21 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/10/2024
Supervised By :mohammad ahmed 08/12/2024

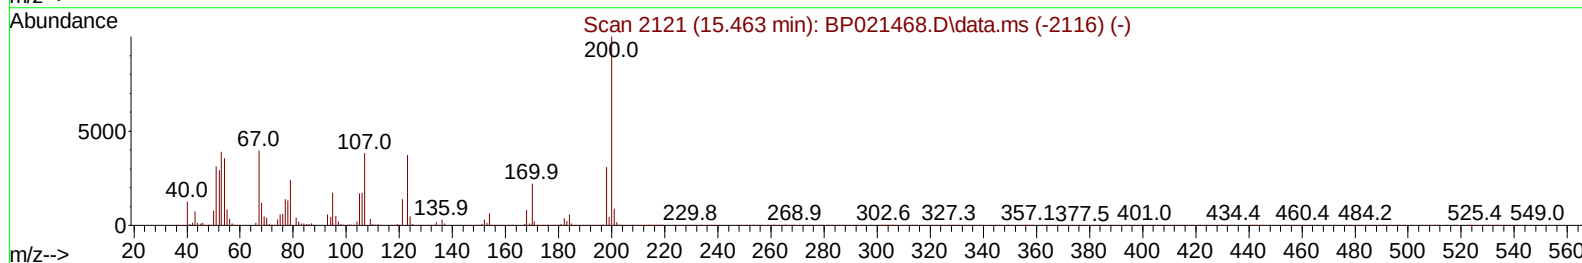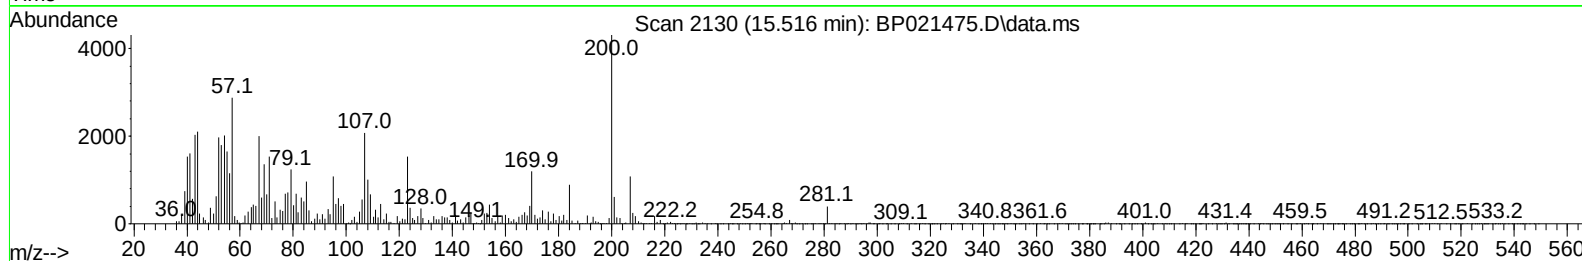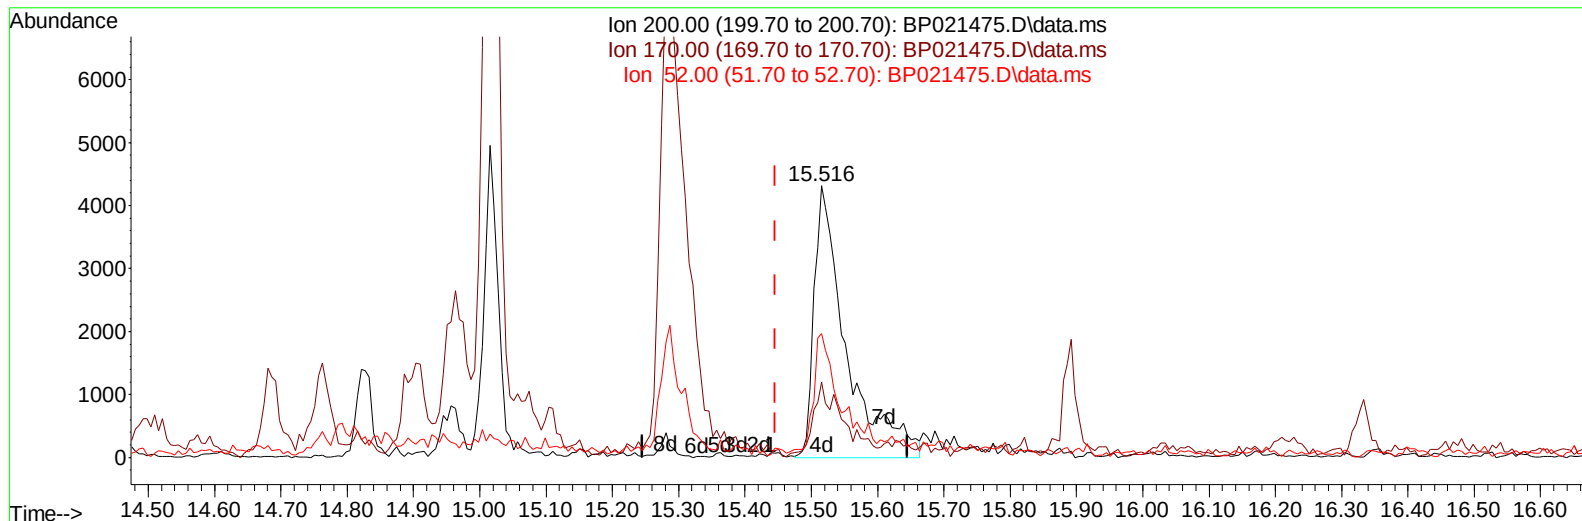

TIC: BP021475.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.516min (+ 0.070) 2.75 ng/ul m

response 14503

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	21.00	27.74#
52.00	38.50	45.64
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080824\
 Data File : BP021475.D
 Acq On : 09 Aug 2024 18:04
 Operator : RC/JU
 Sample : P3171-05MEDL 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCVW9MEDL

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/10/2024
 Supervised By :mohammad ahmed 08/12/2024

Quant Time: Aug 09 23:07:10 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 08 18:23:21 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.616	152	149176	20.000	ng/ul	0.02
20) Naphthalene-d8	10.381	136	572955	20.000	ng/ul	0.01
38) Acenaphthene-d10	14.251	164	405919	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.069	188	870728	20.000	ng/ul	0.00
79) Chrysene-d12	21.527	240	912850	20.000	ng/ul	0.02
88) Perylene-d12	24.786	264	1060504	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.158	96	3607	1.100	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	6.940	99	32138m	2.643	ng/ul	0.11
9) Bis-(2-Chloroethyl)eth...	7.005	67	35285m	4.787	ng/ul	0.05
11) 2-Chlorophenol-d4	7.222	132	46496m	4.640	ng/ul	0.06
15) 4-Methylphenol-d8	8.457	113	50281m	4.978	ng/ul	0.11
21) Nitrobenzene-d5	8.840	128	19514m	4.385	ng/ul	0.06
24) 2-Nitrophenol-d4	9.546	143	21607m	4.242	ng/ul	0.06
28) 2,4-Dichlorophenol-d3	10.181	165	42909m	4.659	ng/ul	0.14
31) 4-Chloroaniline-d4	10.640	131	55355m	4.537	ng/ul	0.10
46) Dimethylphthalate-d6	13.681	166	205158	6.953	ng/ul	0.02
49) Acenaphthylene-d8	13.951	160	205586	6.205	ng/ul	0.02
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
60) Fluorene-d10	15.286	176	164187	6.782	ng/ul	0.02
65) 4,6-Dinitro-2-methylph...	15.516	200	14503m	2.753	ng/ul	0.07
73) Anthracene-d10	17.180	188	293932	7.600	ng/ul	0.00
81) Pyrene-d10	19.569	212	442261	7.836	ng/ul	0.01
92) Benzo(a)pyrene-d12	24.568	264	559263	10.693	ng/ul	0.00
Target Compounds						
58) 2,3,4,6-Tetrachlorophenol	14.992	232	16082m	2.131	ng/ul	Qvalue
71) Pentachlorophenol	16.739	266	219059	34.467	ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080824\
Data File : BP021475.D
Acq On : 09 Aug 2024 18:04
Operator : RC/JU
Sample : P3171-05MEDL 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCVW9MEDL

Manual IntegrationsAPPROVED

Quant Time: Aug 09 23:07:10 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 08 18:23:21 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/10/2024
Supervised By :mohammad ahmed 08/12/2024

