

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080824\
 Data File : BP021453.D
 Acq On : 08 Aug 2024 17:48
 Operator : RC/JU
 Sample : PB162536BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK536

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021453.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.152	24	28	34	rBV	40625	53996	1.34%	0.131%
2	3.358	61	63	69	rBV7	3056	4274	0.11%	0.010%
3	3.575	98	100	124	rBV	346354	701080	17.42%	1.707%
4	3.858	146	148	154	rVB2	9608	12540	0.31%	0.031%
5	6.752	636	640	644	rBV7	1734	4227	0.11%	0.010%
6	6.846	649	656	671	rBV	300539	899685	22.35%	2.190%
7	6.963	671	676	697	rVB	416228	788580	19.59%	1.920%
8	7.169	704	711	729	rBV	504935	965384	23.98%	2.350%
9	7.610	779	786	812	rVB	565291	1029442	25.57%	2.506%
10	8.357	906	913	950	rBV	386679	1228663	30.52%	2.991%
11	8.775	977	984	1006	rBV	401963	956847	23.77%	2.329%
12	9.493	1099	1106	1135	rBV	323226	823462	20.46%	2.005%
13	10.075	1198	1205	1242	rBV	270961	1158216	28.77%	2.819%
14	10.381	1249	1257	1277	rVB	510997	1198033	29.76%	2.916%
15	10.563	1281	1288	1314	rBV	291574	957471	23.79%	2.331%
16	12.045	1531	1540	1546	rBV3	6447	16415	0.41%	0.040%
17	13.663	1808	1815	1834	rBV	840583	1997667	49.63%	4.863%
18	13.786	1834	1836	1841	rVB	7584	10263	0.25%	0.025%
19	13.939	1855	1862	1877	rBV	1429950	2198043	54.61%	5.351%
20	14.251	1909	1915	1932	rBV	1311054	2037929	50.63%	4.961%
21	14.639	1975	1981	1989	rBV	154361	424545	10.55%	1.033%
22	14.763	2000	2002	2009	rVB6	19534	35044	0.87%	0.085%
23	14.892	2020	2024	2032	rVB6	10803	23549	0.59%	0.057%
24	15.275	2082	2089	2107	rBV	1491278	2918243	72.50%	7.104%
25	15.469	2116	2122	2152	rBV	274463	883668	21.95%	2.151%
26	16.080	2222	2226	2229	rBV6	5626	9506	0.24%	0.023%
27	16.863	2354	2359	2360	rBV5	3649	5959	0.15%	0.015%
28	17.075	2388	2395	2406	rBV	1602503	2527160	62.78%	6.152%
29	17.180	2406	2413	2437	rVV	1571061	3166689	78.67%	7.709%
30	18.010	2550	2554	2561	rBV2	68377	127993	3.18%	0.312%
31	19.104	2736	2740	2749	rBV5	28896	61958	1.54%	0.151%
32	19.198	2753	2756	2759	rBV	20499	26016	0.65%	0.063%
33	19.339	2776	2780	2786	rBV7	23708	57693	1.43%	0.140%
34	19.563	2811	2818	2832	rBV	2256326	3912471	97.20%	9.524%
35	21.515	3144	3150	3163	rBV2	1264932	2803094	69.64%	6.824%
36	24.562	3659	3668	3687	rBV2	1437772	4025189	100.00%	9.799%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080824\
Data File : BP021453.D
Acq On : 08 Aug 2024 17:48
Operator : RC/JU
Sample : PB162536BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK536

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Title : SVOA CALIBRATION

37	24.798	3698	3708	3727	rVB	943326	3027974	75.23%	7.371%
----	--------	------	------	------	-----	--------	---------	--------	--------




Sum of corrected areas: 41078968

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080824\
Data File : BP021453.D
Acq On : 08 Aug 2024 17:48
Operator : RC/JU
Sample : PB162536BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK536

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

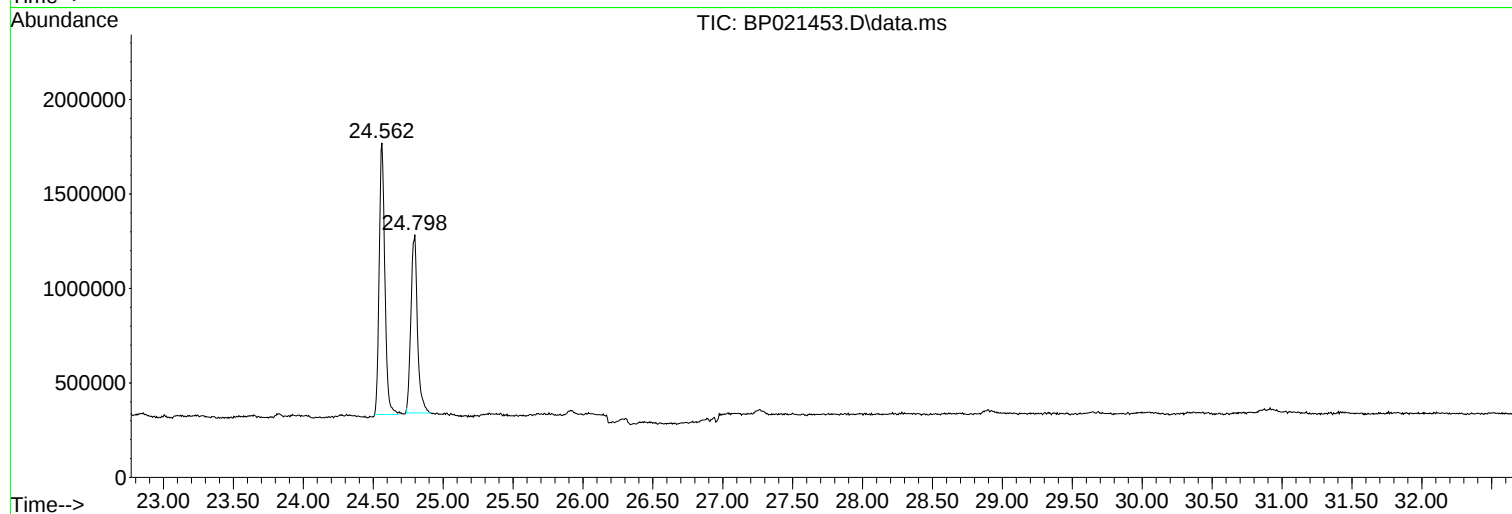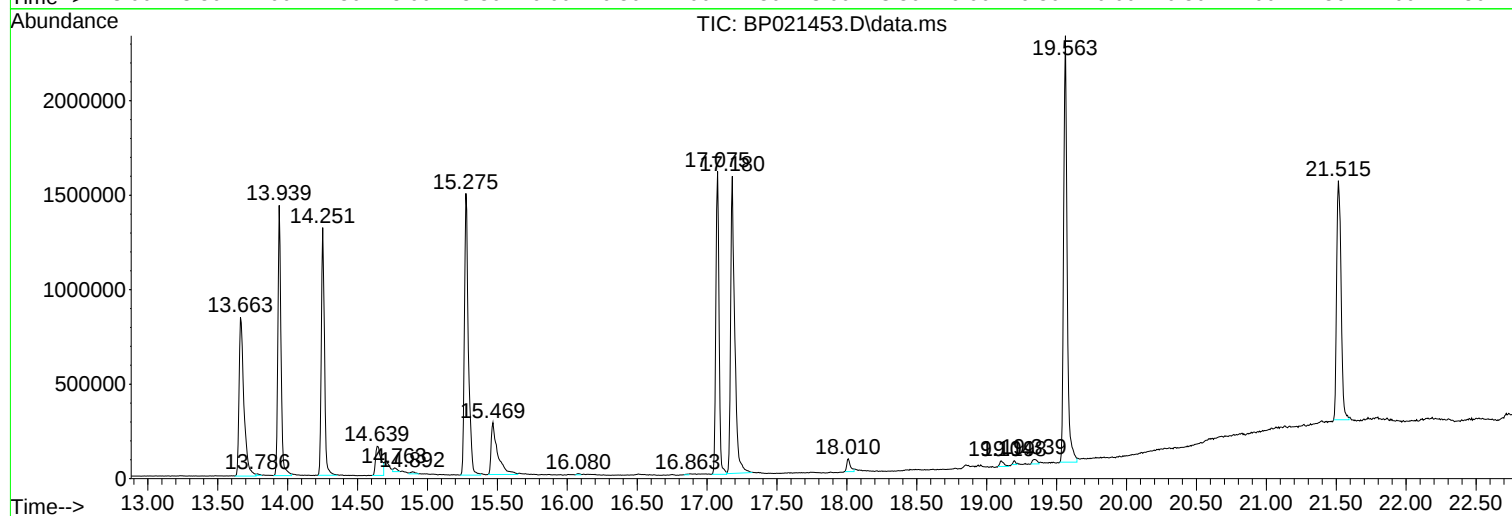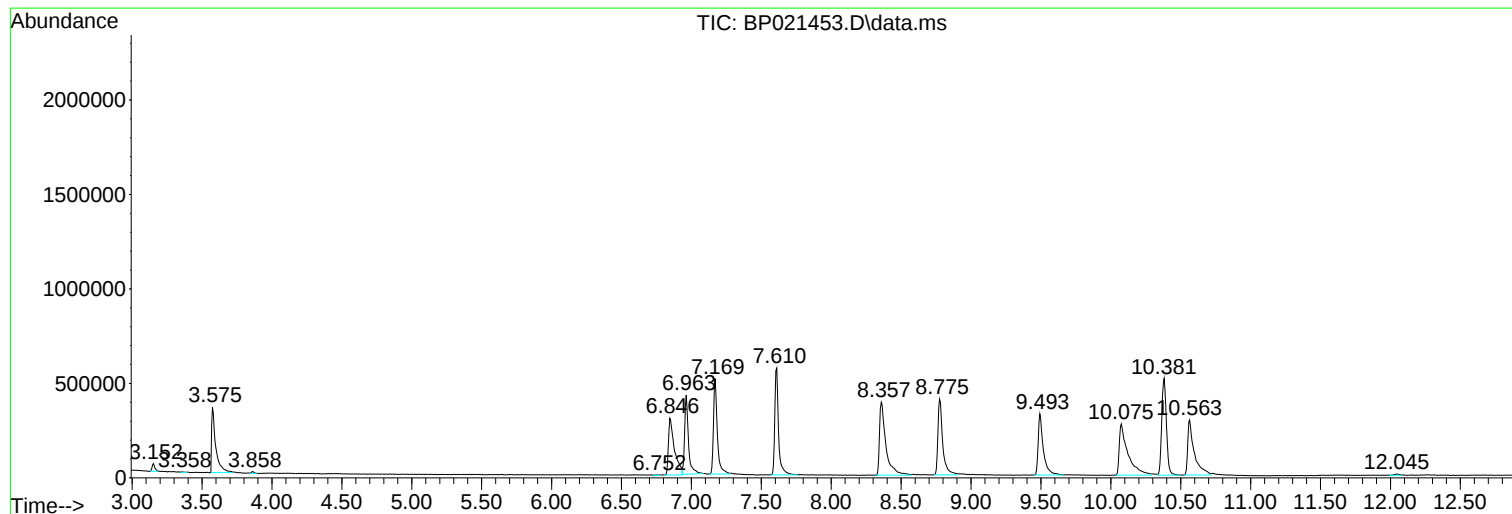

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080824\
Data File : BP021453.D
Acq On : 08 Aug 2024 17:48
Operator : RC/JU
Sample : PB162536BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK536

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080824\
Data File : BP021453.D
Acq On : 08 Aug 2024 17:48
Operator : RC/JU
Sample : PB162536BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK536

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------