
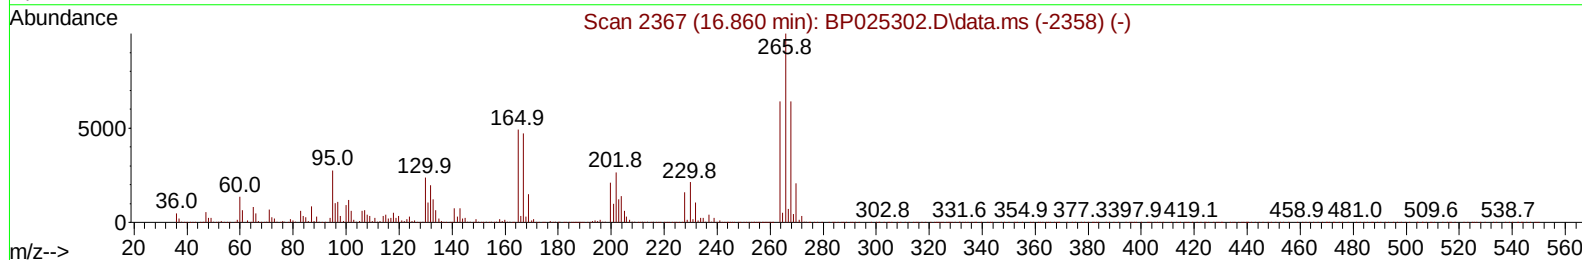
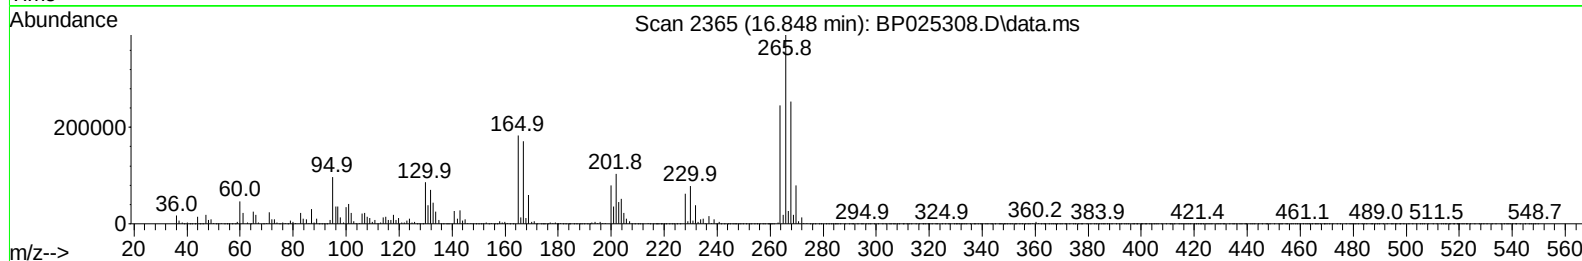


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080725\
Data File : BP025308.D
Acq On : 07 Aug 2025 11:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 07 12:25:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 06:41:44 2025
Response via : Initial Calibration

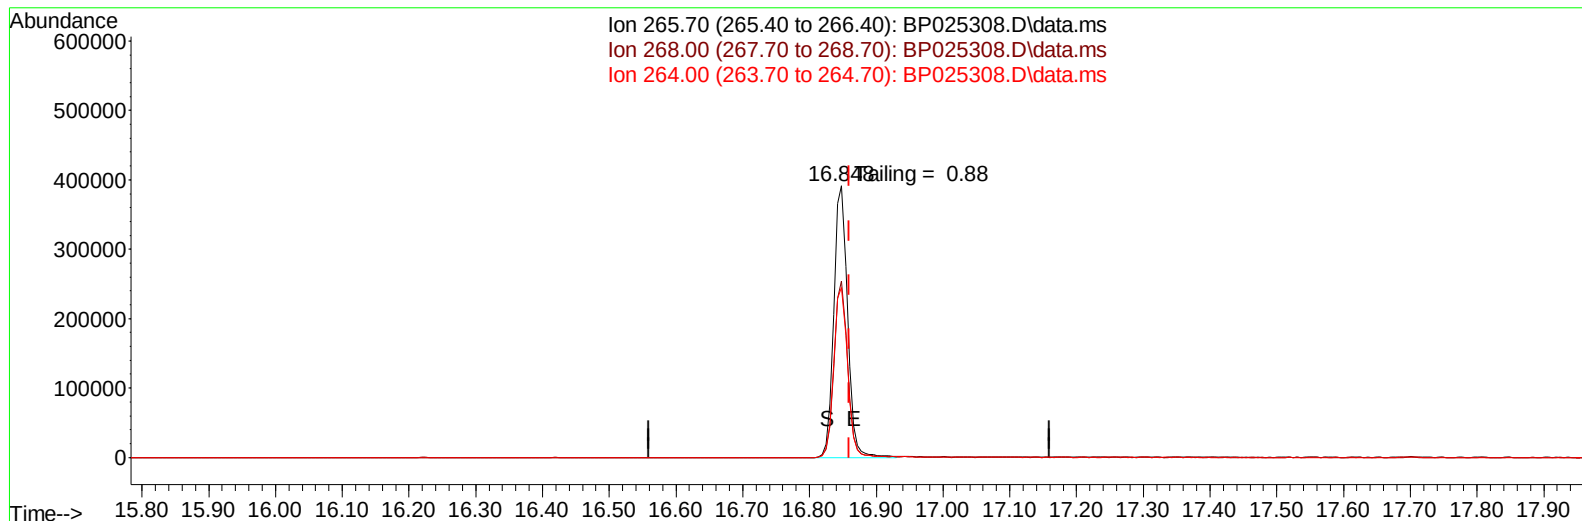

TIC: BP025308.D\data.ms

(70) Pentachlorophenol (C)




16.848min (-0.012) 12862.36 ng

response 556675

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	64.89
264.00	63.90	62.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080725\
Data File : BP025308.D
Acq On : 07 Aug 2025 11:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 07 12:25:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 06:41:44 2025
Response via : Initial Calibration

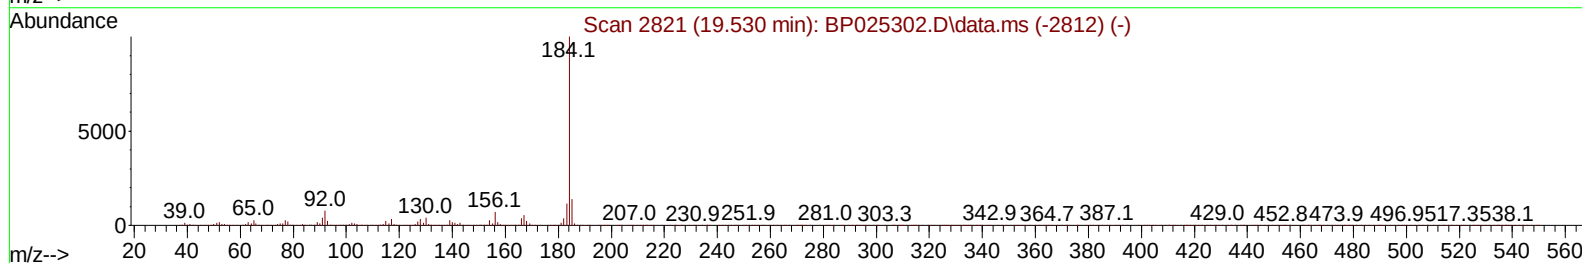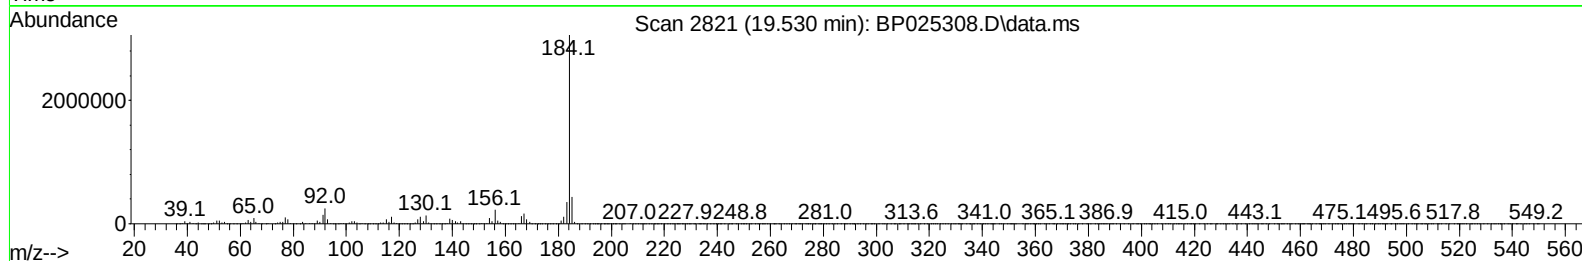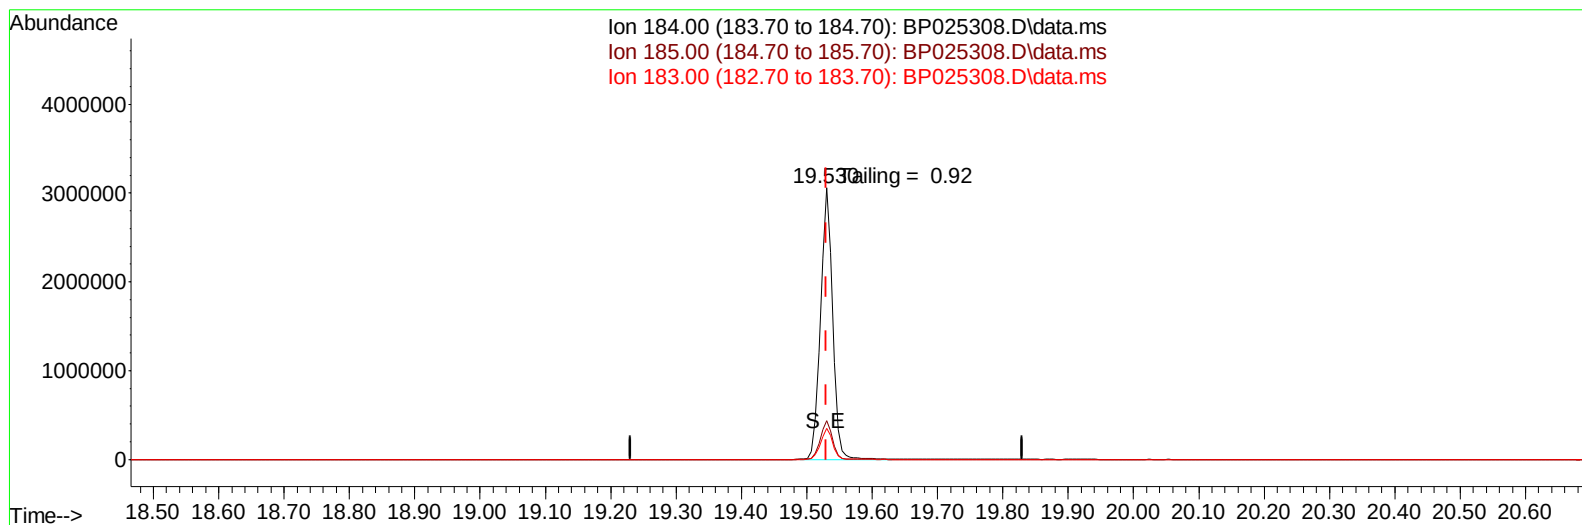

TIC: BP025308.D\data.ms

(77) Benzidine**19.530min (+ 0.000) 8796.27 ng****response 3944680**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.29
183.00	11.50	11.56
0.00	0.00	0.00