

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080921\
 Data File : BP006606.D
 Acq On : 09 Aug 2021 10:17
 Operator : CG/JU
 Sample : PB138195BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK195

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Title : SVOA CALIBRATION

Signal : TIC: BP006606.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.681	97	101	122	rVB	711602	1180013	28.78%	2.302%
2	6.934	648	654	662	rVB	947492	1483145	36.17%	2.893%
3	7.099	676	682	693	rVB	748484	1186708	28.94%	2.315%
4	7.287	708	714	721	rVB	1003665	1550629	37.82%	3.024%
5	7.752	787	793	802	rVB	866065	1337686	32.63%	2.609%
6	8.463	908	914	924	rBV	1176339	1839066	44.86%	3.587%
7	8.910	983	990	1000	rVB	927388	1511525	36.87%	2.948%
8	9.622	1104	1111	1127	rBV	739333	1259388	30.72%	2.456%
9	10.157	1195	1202	1223	rBV	1058294	1825067	44.51%	3.560%
10	10.534	1258	1266	1274	rBV	1235975	2029241	49.49%	3.958%
11	10.681	1283	1291	1309	rBV	1103646	1898824	46.31%	3.703%
12	11.340	1400	1403	1406	rBV5	4315	5571	0.14%	0.011%
13	12.122	1531	1536	1545	rVB2	20022	36320	0.89%	0.071%
14	12.334	1569	1572	1576	rBV6	4309	6995	0.17%	0.014%
15	13.110	1700	1704	1708	rBV7	3198	5977	0.15%	0.012%
16	13.351	1740	1745	1749	rVB7	5424	7675	0.19%	0.015%
17	13.798	1812	1821	1829	rBV	1791418	2502921	61.05%	4.882%
18	13.887	1833	1836	1843	rVV9	5193	13118	0.32%	0.026%
19	14.075	1858	1868	1876	rBV	2049657	3083194	75.20%	6.013%
20	14.381	1913	1920	1928	rBV	1749603	2484341	60.59%	4.845%
21	14.434	1928	1929	1935	rVB6	4402	5538	0.14%	0.011%
22	14.598	1948	1957	1974	rBV	679190	1263108	30.81%	2.464%
23	15.375	2082	2089	2103	rBV	2469452	3580228	87.32%	6.983%
24	15.504	2105	2111	2120	rBV	685978	901812	22.00%	1.759%
25	15.616	2125	2130	2139	rVB2	32533	54084	1.32%	0.105%
26	15.939	2182	2185	2190	rBV7	3722	6644	0.16%	0.013%
27	16.169	2217	2224	2227	rVB9	6627	10620	0.26%	0.021%
28	16.810	2327	2333	2339	rVB9	6443	12040	0.29%	0.023%
29	16.916	2345	2351	2358	rBV5	10571	21674	0.53%	0.042%
30	17.134	2382	2388	2396	rBV	1855462	2684339	65.47%	5.236%
31	17.234	2398	2405	2419	rVV	2758903	3819166	93.15%	7.449%
32	17.328	2419	2421	2425	rVB5	3822	4481	0.11%	0.009%
33	17.392	2430	2432	2439	rVV8	6397	10889	0.27%	0.021%
34	17.516	2450	2453	2457	rBV4	4125	5105	0.12%	0.010%
35	17.810	2498	2503	2506	rBV6	3469	6362	0.16%	0.012%
36	18.039	2537	2542	2547	rBV8	12321	25190	0.61%	0.049%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080921\
Data File : BP006606.D
Acq On : 09 Aug 2021 10:17
Operator : CG/JU
Sample : PB138195BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK195

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Title : SVOA CALIBRATION

37	19.051	2711	2714	2718	rBV2	17623	23746	0.58%	0.046%
38	19.122	2722	2726	2730	rBV2	34183	47784	1.17%	0.093%
39	19.369	2765	2768	2771	rBV2	12743	16695	0.41%	0.033%
40	19.480	2781	2787	2796	rBV	2988680	4099927	100.00%	7.997%
41	21.233	3080	3085	3092	rBV	2162060	2735408	66.72%	5.335%
42	23.416	3449	3456	3462	rBV2	2105052	3978350	97.03%	7.759%
43	23.563	3475	3481	3493	rVB2	1386718	2710643	66.11%	5.287%




Sum of corrected areas: 51271237

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080921\
Data File : BP006606.D
Acq On : 09 Aug 2021 10:17
Operator : CG/JU
Sample : PB138195BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK195

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

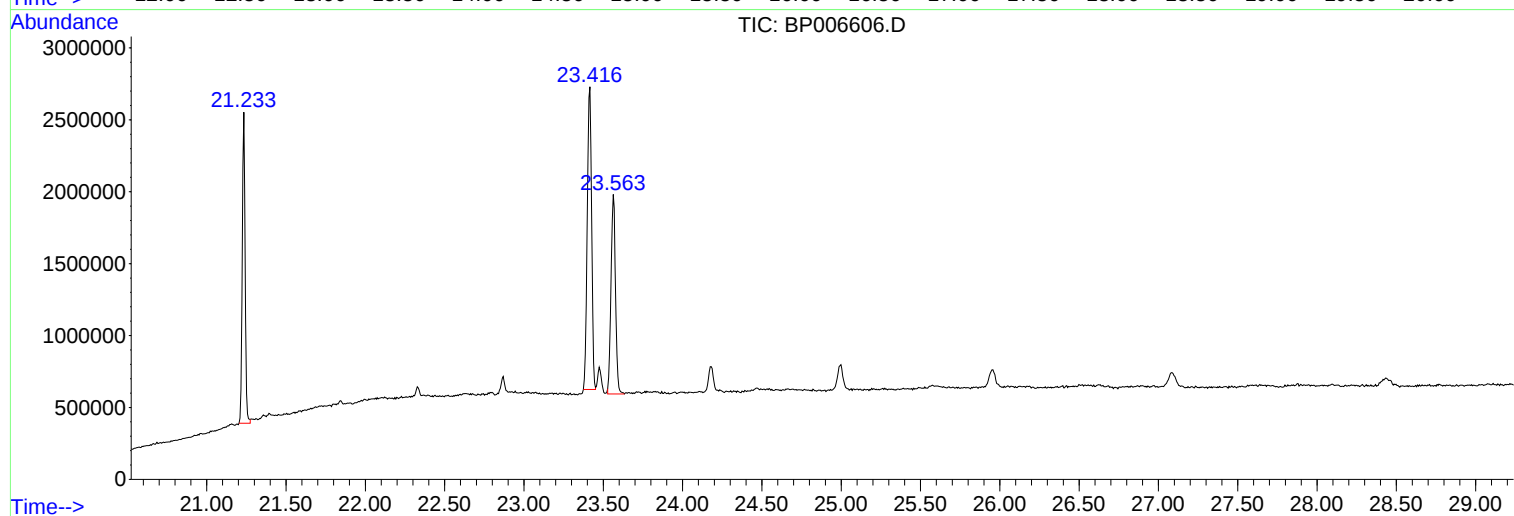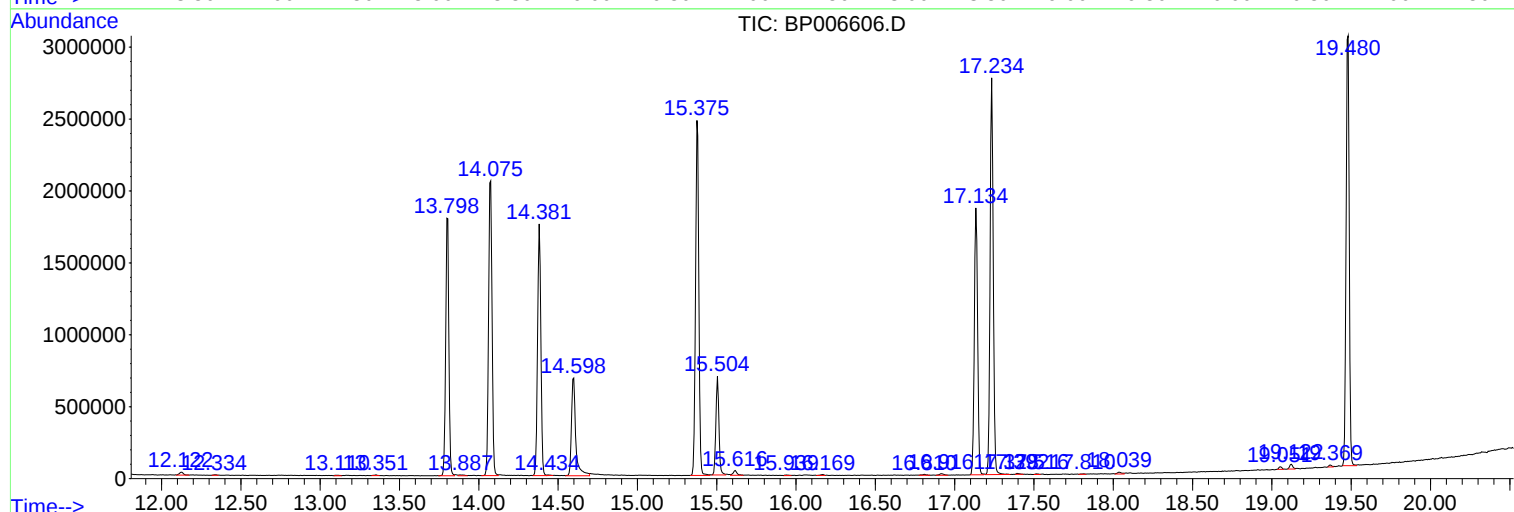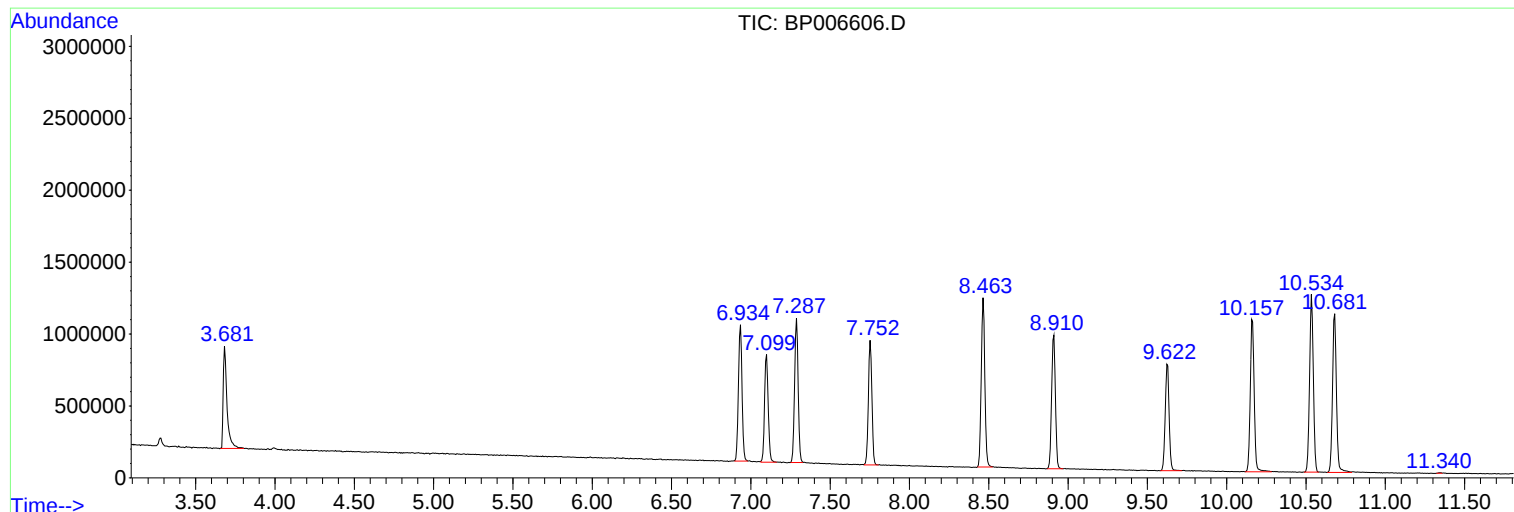

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080921\
Data File : BP006606.D
Acq On : 09 Aug 2021 10:17
Operator : CG/JU
Sample : PB138195BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK195

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080921\
Data File : BP006606.D
Acq On : 09 Aug 2021 10:17
Operator : CG/JU
Sample : PB138195BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK195

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------