

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
 Data File : BP011371.D
 Acq On : 10 Aug 2022 15:46
 Operator : CG/JU
 Sample : N4128-10
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Aug 11 00:01:26 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 08 18:47:19 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.581	152	76787	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.375	136	327615	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.257	164	183104	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.028	188	372770	20.000	ng/u1	-0.01
79) Chrysene-d12	21.163	240	367187	20.000	ng/u1	0.00
88) Perylene-d12	23.469	264	386260	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.087	96	12779	5.102	ng/uL	0.00
4) Pyridine-d5	3.505	84	50468	7.988	ng/u1	0.00
7) Phenol-d5	6.769	99	45594	6.709	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.934	67	129124	26.799	ng/u1	0.00
11) 2-Chlorophenol-d4	7.116	132	123319	23.129	ng/u1	0.00
15) 4-Methylphenol-d8	8.305	113	77407	14.507	ng/u1	-0.01
21) Nitrobenzene-d5	8.746	128	69755	31.285	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.469	143	65519	32.096	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.005	165	107705	26.126	ng/u1	0.00
31) 4-Chloroaniline-d4	10.528	131	136610	18.955	ng/u1	0.00
46) Dimethylphthalate-d6	13.681	166	412815	32.493	ng/u1	0.00
49) Acenaphthylene-d8	13.946	160	477125	31.198	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.504	143	7027	3.028	ng/u1	0.01
60) Fluorene-d10	15.263	176	347042	31.941	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.393	200	50201	28.993	ng/u1	0.00
73) Anthracene-d10	17.128	188	601526	35.901	ng/u1	-0.01
81) Pyrene-d10	19.392	212	706684	34.933	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.322	264	705706	36.228	ng/u1	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.086	149	15967	1.201	ng/u1	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011371.D
Acq On : 10 Aug 2022 15:46
Operator : CG/JU
Sample : N4128-10
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :


Quant Time: Aug 11 00:01:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 08 18:47:19 2022
Response via : Initial Calibration

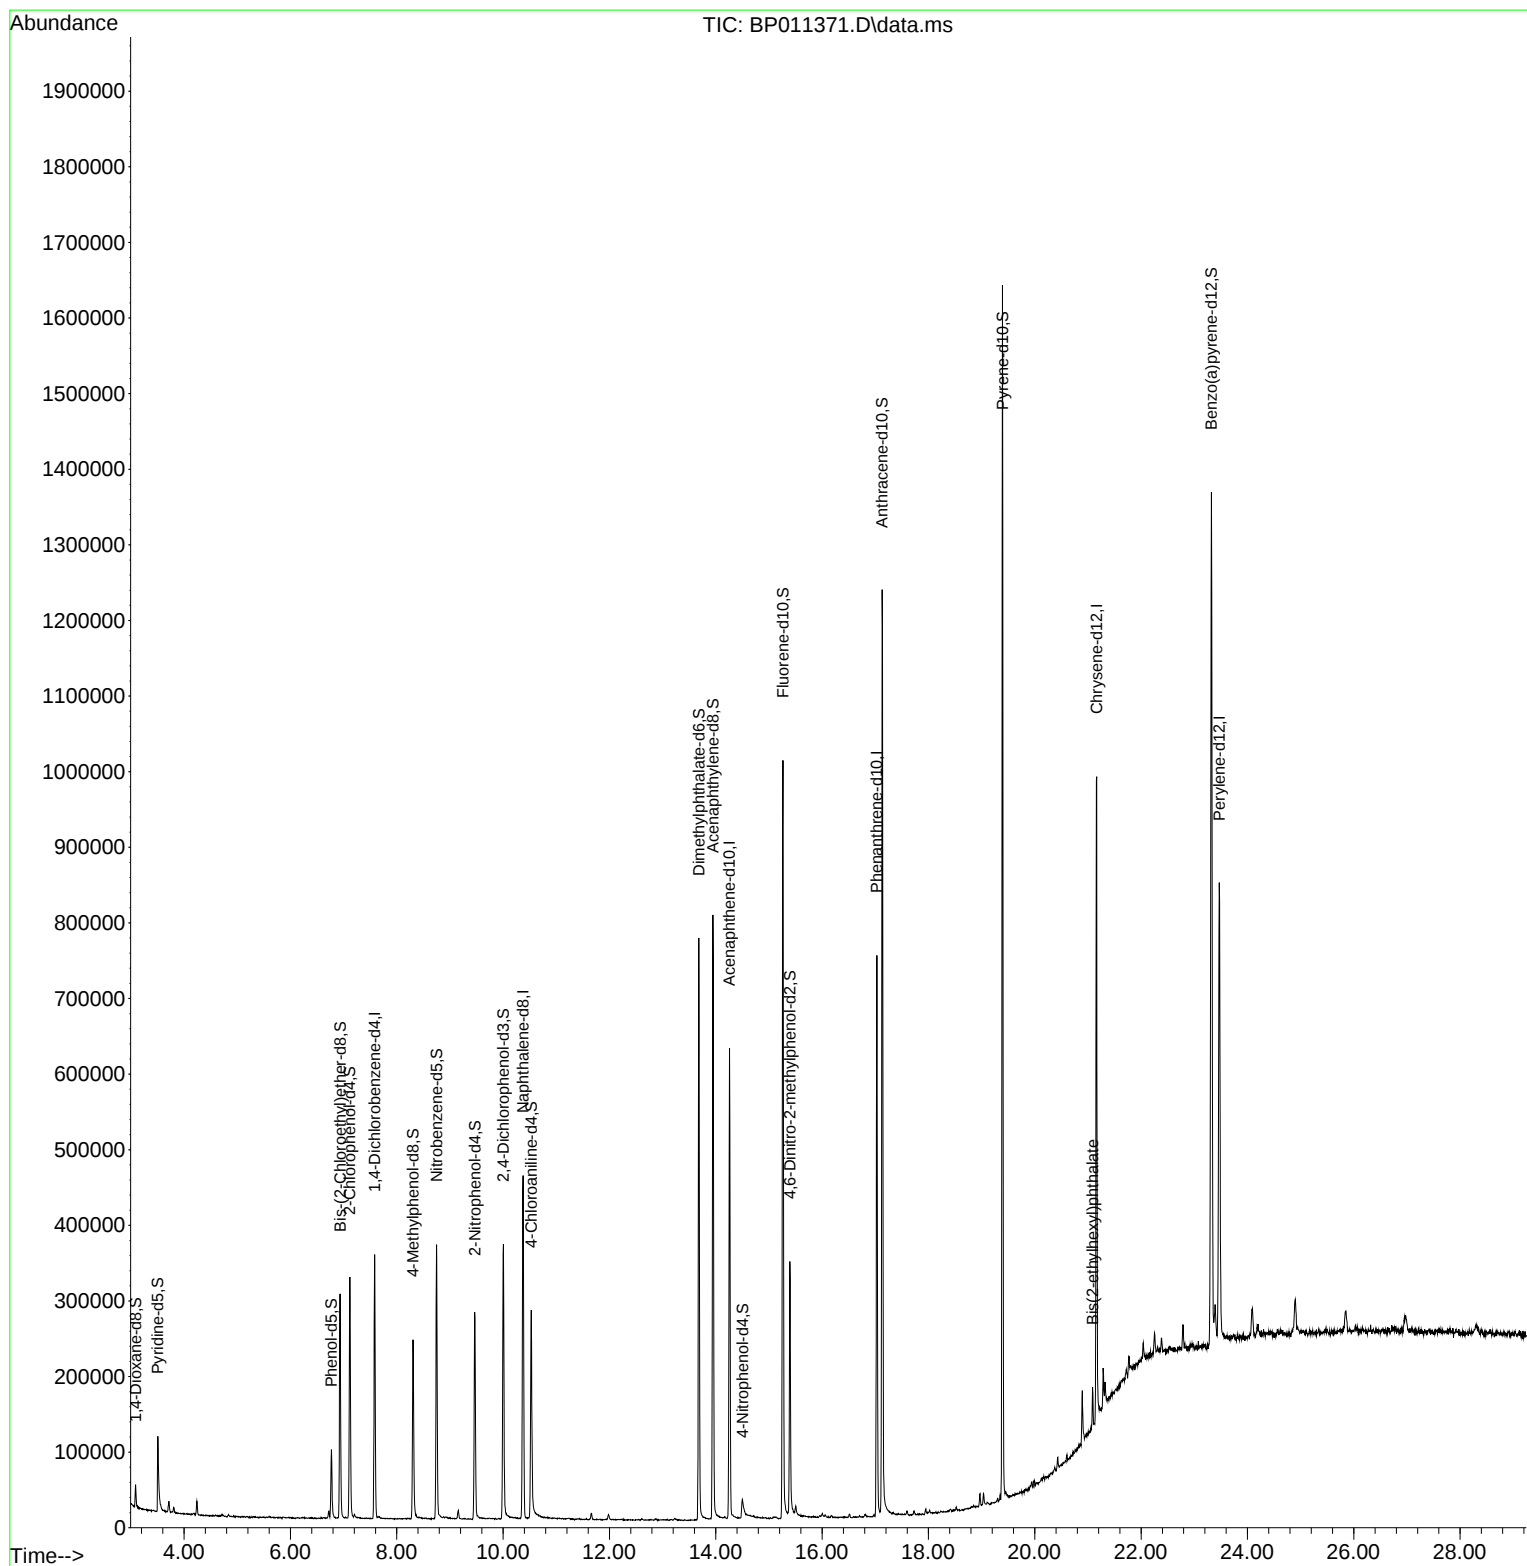

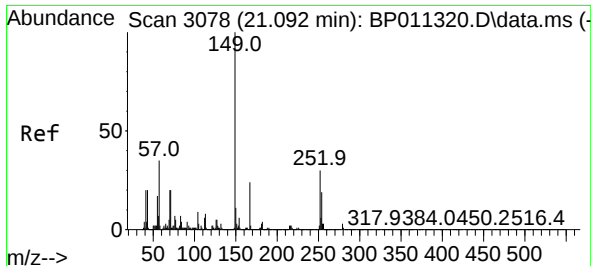

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.201 ng/ul
 RT: 21.086 min Scan# 3077
 Delta R.T. -0.006 min
 Lab File: BP011371.D
 Acq: 10 Aug 2022 15:46

Instrument :
 BNA_P
 ClientSampleId :

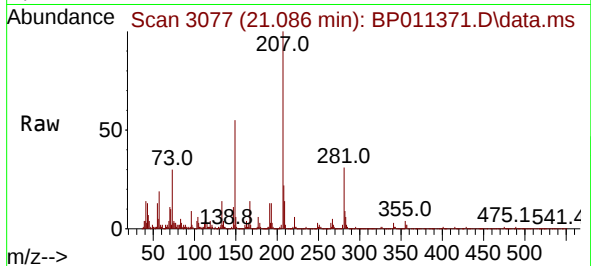

Tgt Ion:	149	Resp:	15967
Ion Ratio	Lower	Upper	
149	100		
167	25.5	20.4	30.6
279	3.8	2.9	4.3

