




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011324.D
Acq On : 09 Aug 2022 12:01
Operator : CG/JU
Sample : N3900-17
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CB8

Manual IntegrationsAPPROVED

Quant Time: Aug 09 23:09:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 08 18:47:19 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/10/2022
Supervised By :Sohil Jodhani 08/10/2022

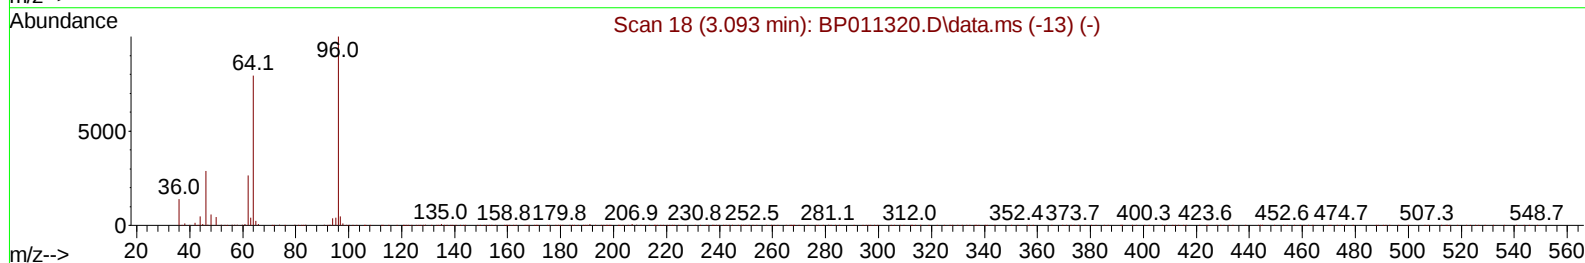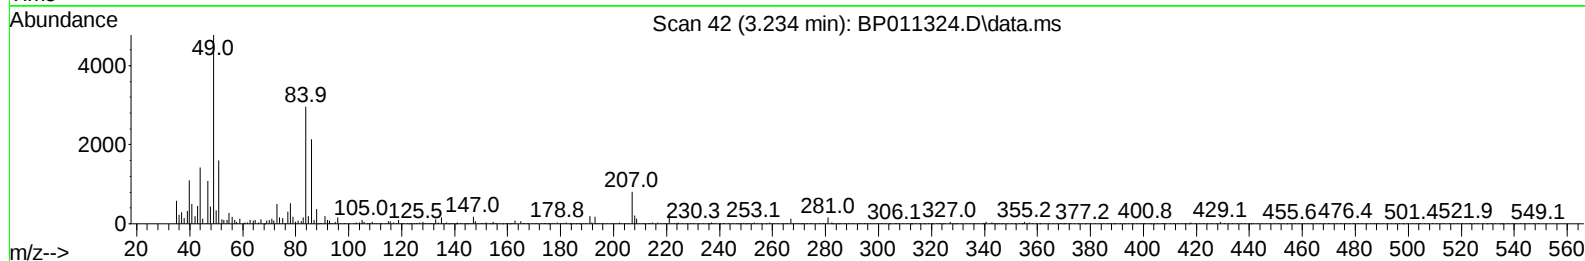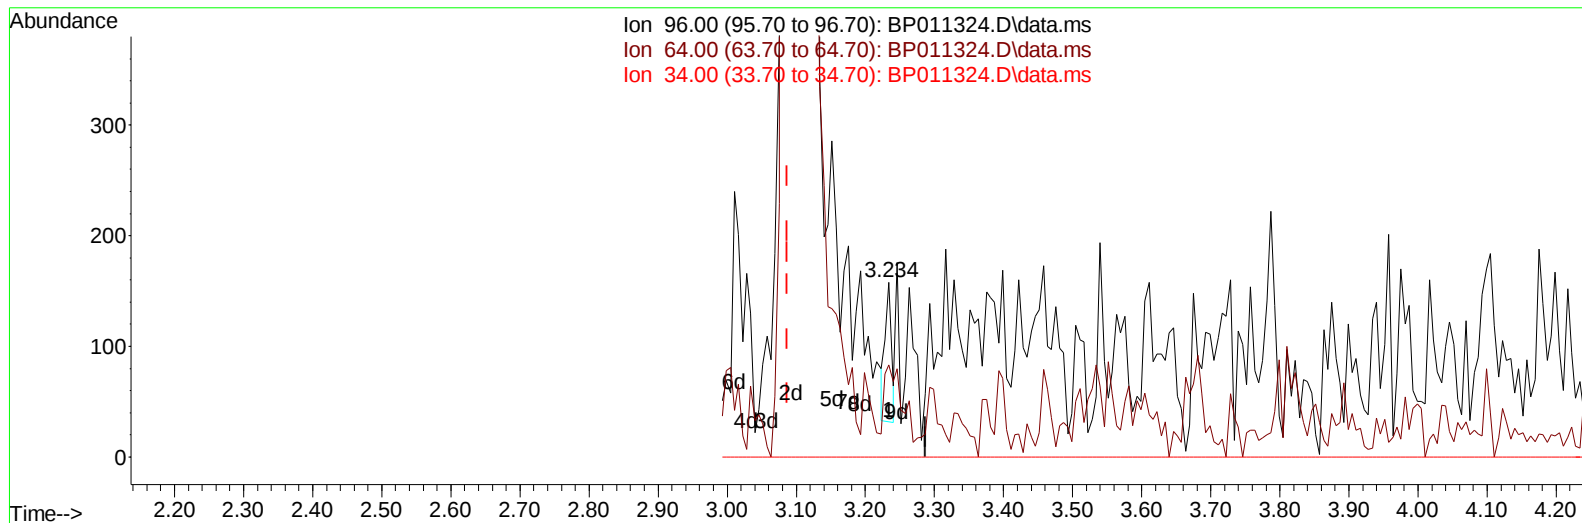

TIC: BP011324.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.234min (+ 0.147) 0.02 ng/uL

response 82

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	61.00	52.53
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
 Data File : BP011324.D
 Acq On : 09 Aug 2022 12:01
 Operator : CG/JU
 Sample : N3900-17
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0CB8

Manual IntegrationsAPPROVED

Quant Time: Aug 09 23:09:48 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 08 18:47:19 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/10/2022
 Supervised By :Sohil Jodhani 08/10/2022

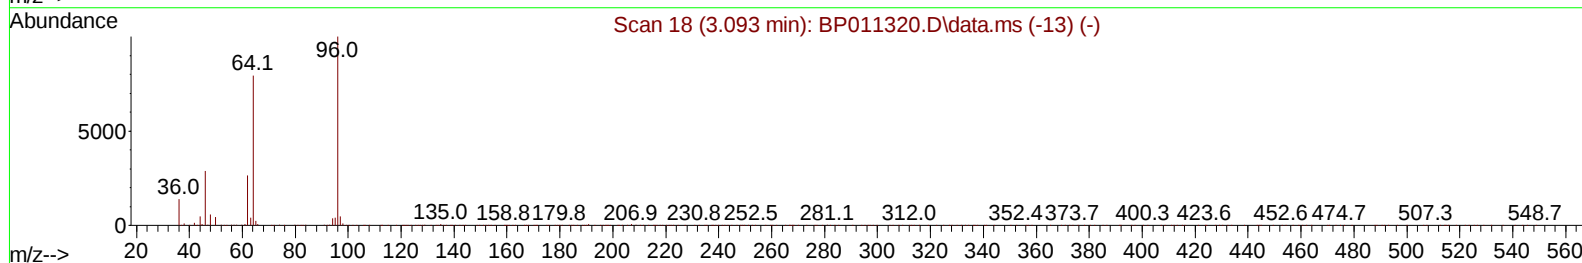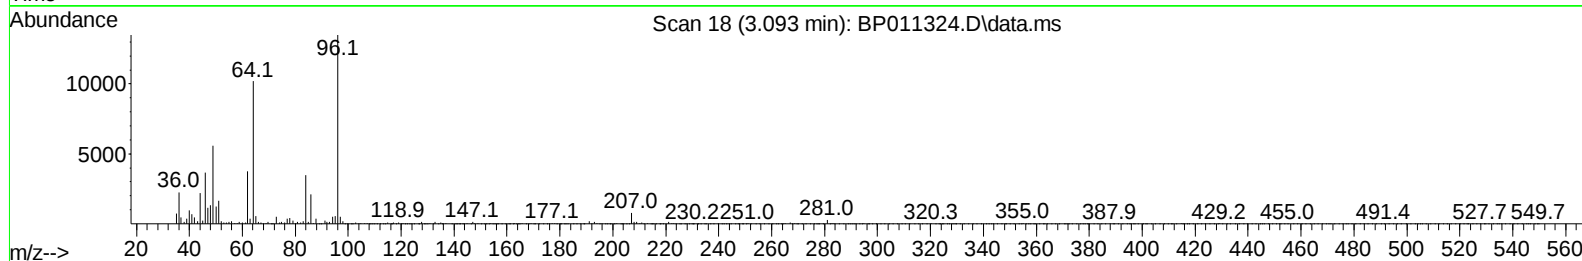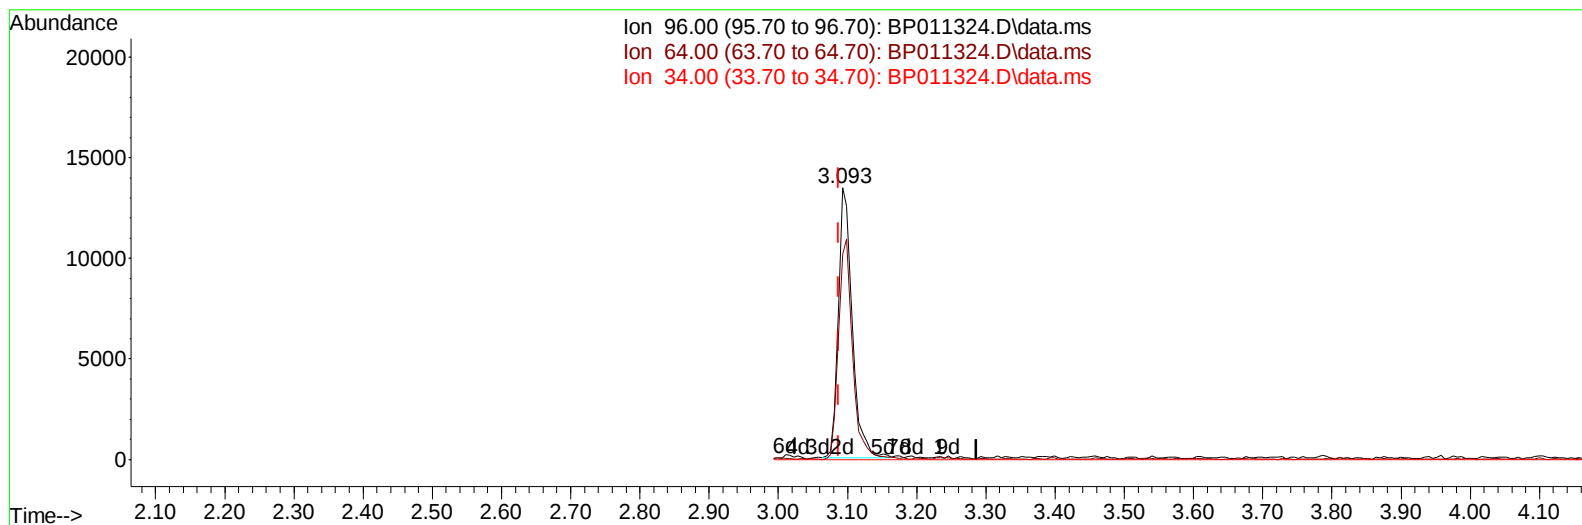

TIC: BP011324.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.093min (+ 0.006) 4.61 ng/uL m

response 18888

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	61.00	75.49#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011324.D
Acq On : 09 Aug 2022 12:01
Operator : CG/JU
Sample : N3900-17
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CB8

Manual IntegrationsAPPROVED

Quant Time: Aug 09 23:09:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 08 18:47:19 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/10/2022
Supervised By :Sohil Jodhani 08/10/2022

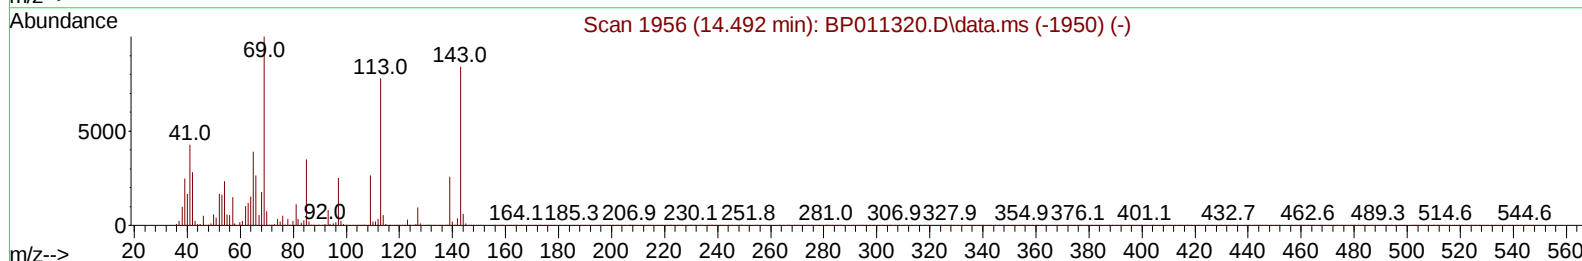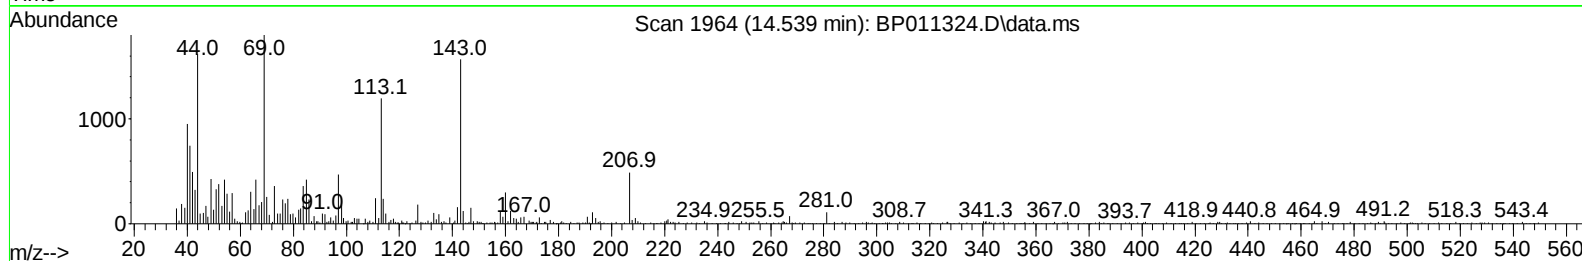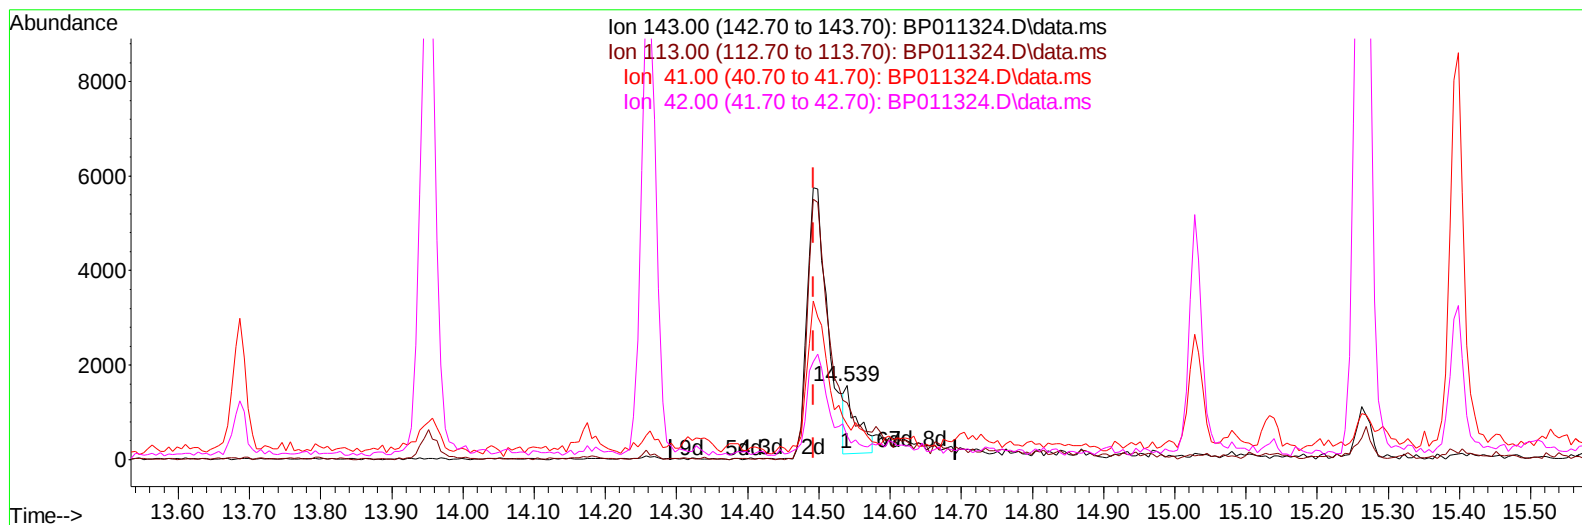

TIC: BP011324.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.539min (+ 0.047) 0.46 ng/u1

response 1749

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	75.70	76.36
41.00	54.40	47.41
42.00	35.50	31.76




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011324.D
Acq On : 09 Aug 2022 12:01
Operator : CG/JU
Sample : N3900-17
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CB8

Manual IntegrationsAPPROVED

Quant Time: Aug 09 23:09:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 08 18:47:19 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/10/2022
Supervised By :Sohil Jodhani 08/10/2022

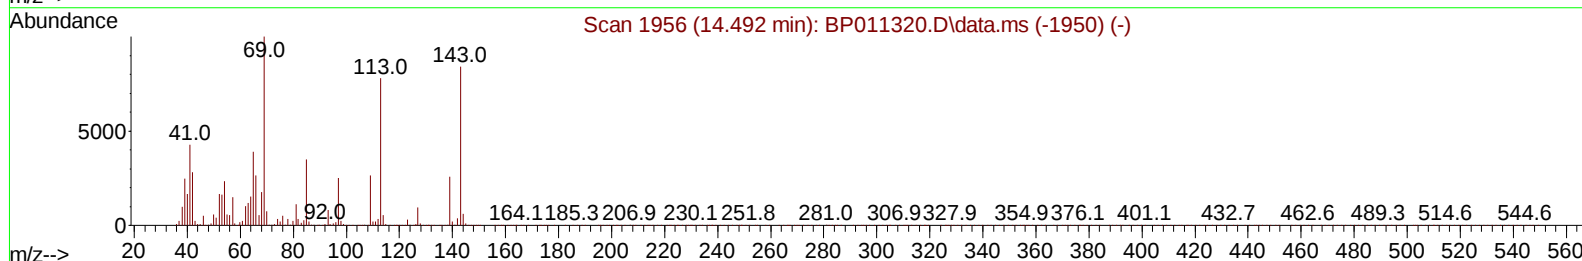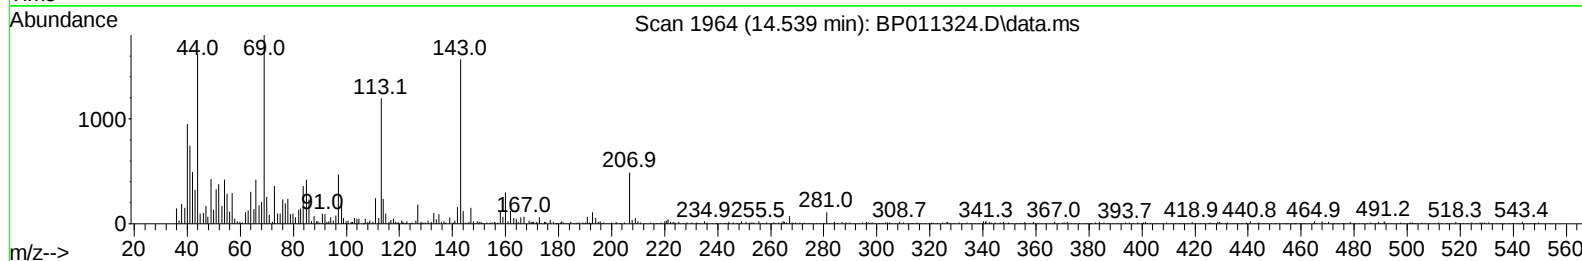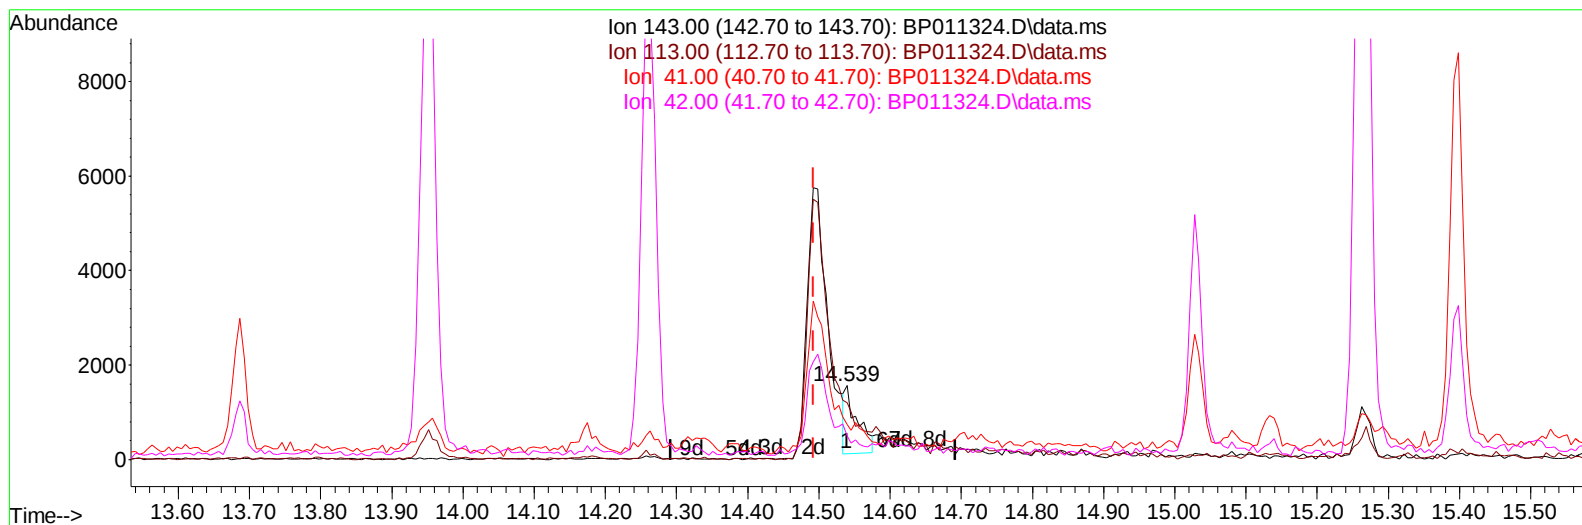

TIC: BP011324.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.539min (+ 0.047) 0.46 ng/u1

response 1749

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	75.70	76.36
41.00	54.40	47.41
42.00	35.50	31.76




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011324.D
Acq On : 09 Aug 2022 12:01
Operator : CG/JU
Sample : N3900-17
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CB8

Manual IntegrationsAPPROVED

Quant Time: Aug 09 23:09:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 08 18:47:19 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/10/2022
Supervised By :Sohil Jodhani 08/10/2022

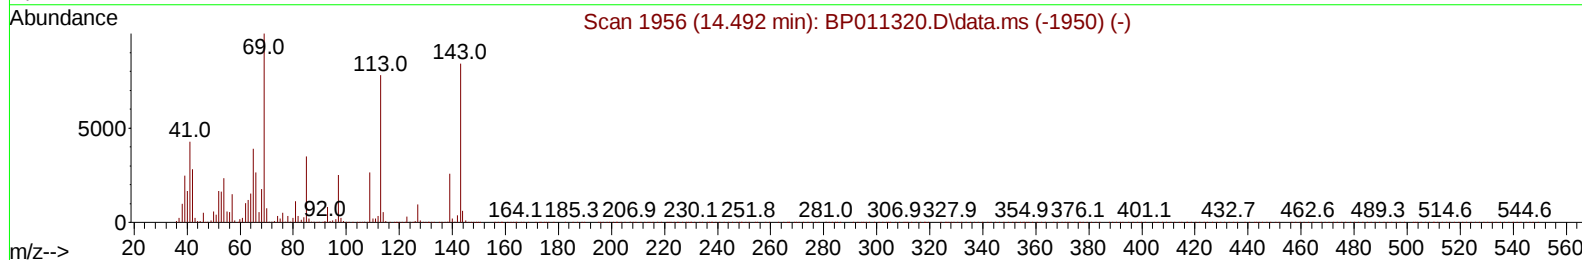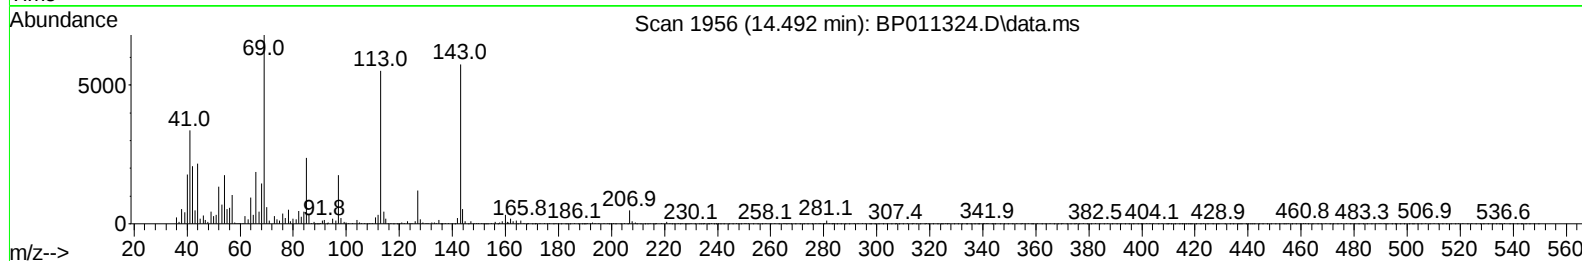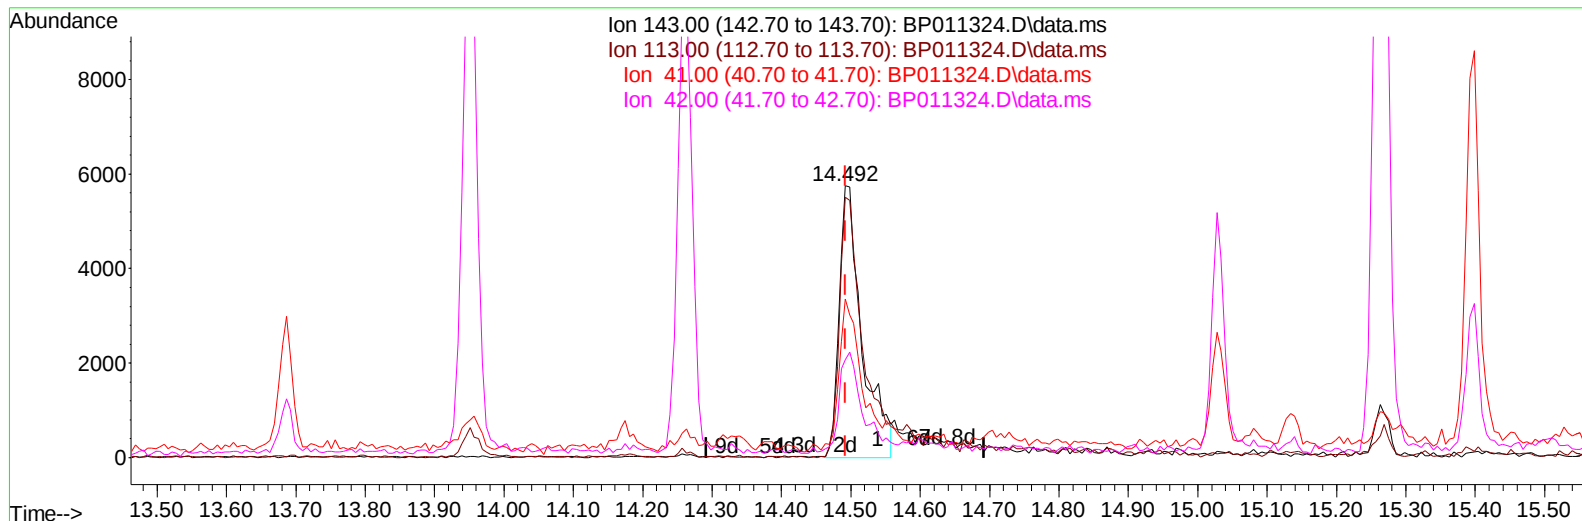

TIC: BP011324.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.492min (-0.000) 3.43 ng/u1 m

response 13169

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	75.70	95.86#
41.00	54.40	58.45
42.00	35.50	36.07

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
 Data File : BP011324.D
 Acq On : 09 Aug 2022 12:01
 Operator : CG/JU
 Sample : N3900-17
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0CB8

Manual IntegrationsAPPROVED

Quant Time: Aug 09 23:09:48 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 08 18:47:19 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/10/2022
 Supervised By :Sohil Jodhani 08/10/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.593	152	125516	20.000	ng/ul	0.00
20) Naphthalene-d8	10.381	136	528898	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.263	164	303274	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.033	188	606383	20.000	ng/ul	0.00
79) Chrysene-d12	21.163	240	573446	20.000	ng/ul	0.00
88) Perylene-d12	23.474	264	583707	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.093	96	18888m	4.613	ng/uL	0.00
4) Pyridine-d5	3.516	84	38456	3.723	ng/ul	0.02
7) Phenol-d5	6.775	99	67593	6.085	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.940	67	246051	31.241	ng/ul	0.00
11) 2-Chlorophenol-d4	7.122	132	210766	24.183	ng/ul	0.00
15) 4-Methylphenol-d8	8.310	113	132377	15.178	ng/ul	0.00
21) Nitrobenzene-d5	8.757	128	129025	35.845	ng/ul	0.00
24) 2-Nitrophenol-d4	9.475	143	117012	35.506	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.004	165	202935	30.493	ng/ul	0.00
31) 4-Chloroaniline-d4	10.534	131	234570	20.161	ng/ul	0.00
46) Dimethylphthalate-d6	13.687	166	805088	38.260	ng/ul	0.00
49) Acenaphthylene-d8	13.951	160	906616	35.792	ng/ul	0.00
54) 4-Nitrophenol-d4	14.492	143	13169m	3.426	ng/ul	0.00
60) Fluorene-d10	15.263	176	677360	37.640	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.398	200	90754	32.221	ng/ul	0.00
73) Anthracene-d10	17.133	188	1121137	41.134	ng/ul	0.00
81) Pyrene-d10	19.398	212	1323265	41.884	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.321	264	1232913	41.883	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011324.D
Acq On : 09 Aug 2022 12:01
Operator : CG/JU
Sample : N3900-17
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CB8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/10/2022
Supervised By :Sohil Jodhani 08/10/2022

Quant Time: Aug 09 23:09:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 08 18:47:19 2022
Response via : Initial Calibration

