




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011343.D
Acq On : 09 Aug 2022 23:04
Operator : CG/JU
Sample : N3956-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXF01

Manual IntegrationsAPPROVED

Quant Time: Aug 10 00:37:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 08 18:47:19 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/11/2022
Supervised By :Sohil Jodhani 08/12/2022

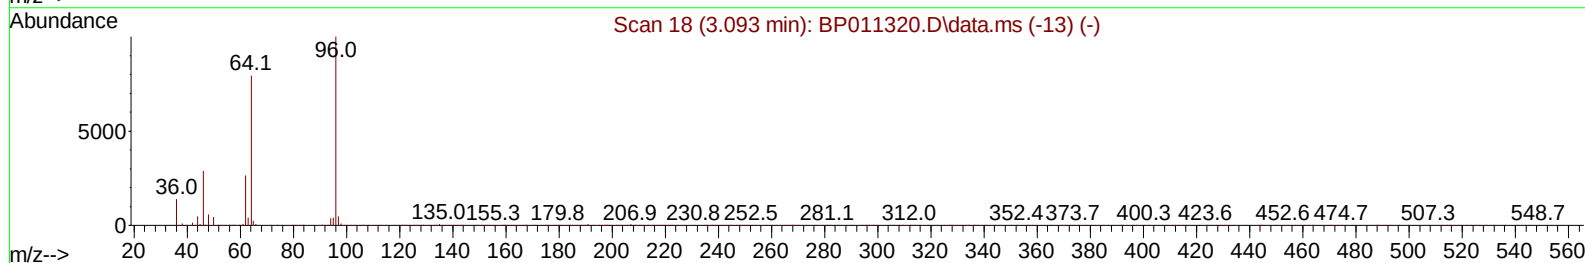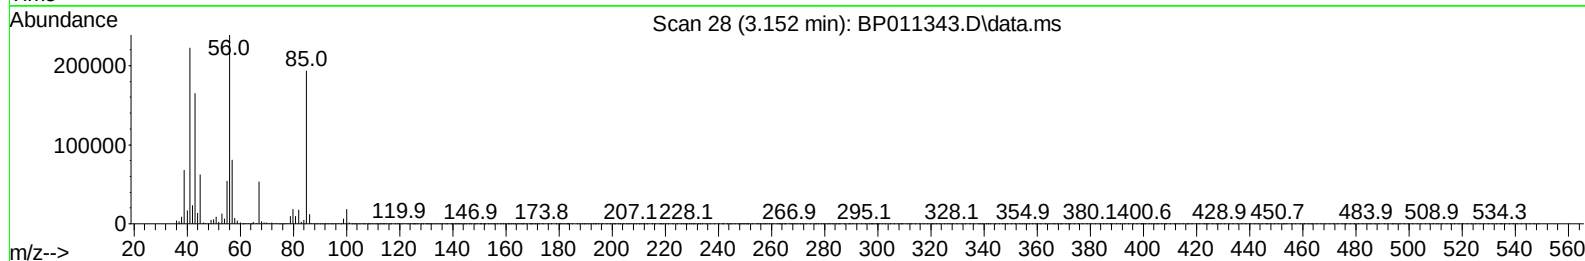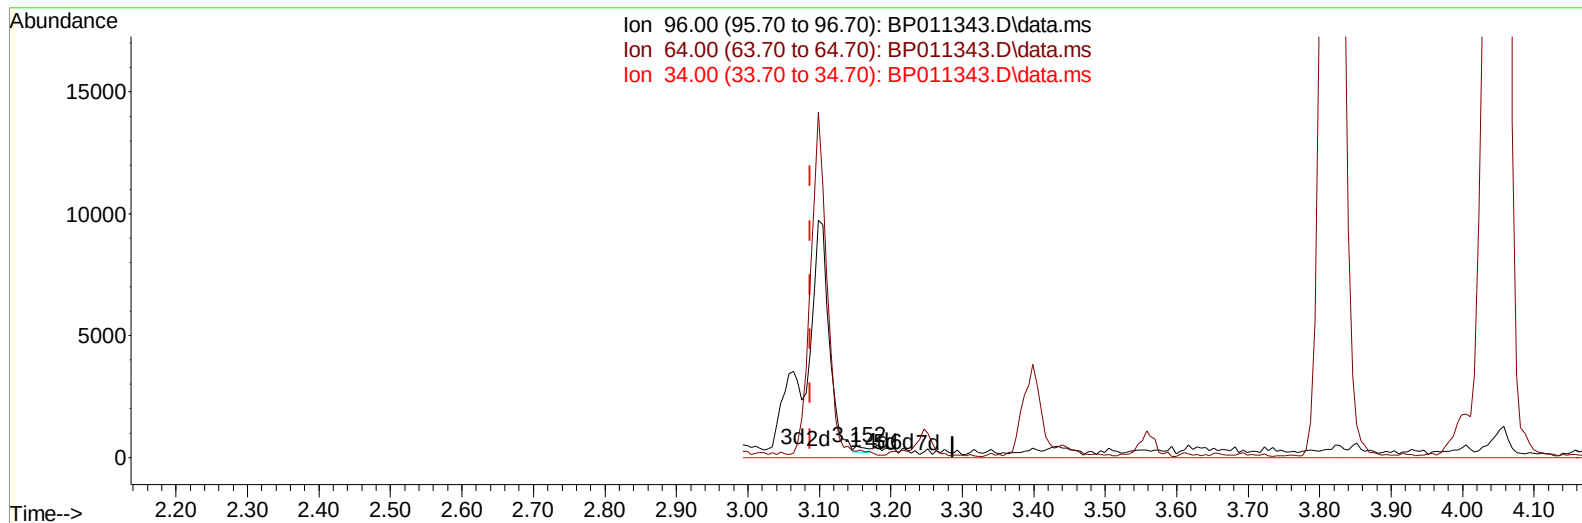

TIC: BP011343.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.152min (+ 0.065) 0.06 ng/uL

response	251	
Ion	Exp%	Act%
96.00	100.00	100.00
64.00	61.00	56.00
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
 Data File : BP011343.D
 Acq On : 09 Aug 2022 23:04
 Operator : CG/JU
 Sample : N3956-02
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXF01

Manual IntegrationsAPPROVED

Quant Time: Aug 10 00:37:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 08 18:47:19 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/11/2022
 Supervised By :Sohil Jodhani 08/12/2022

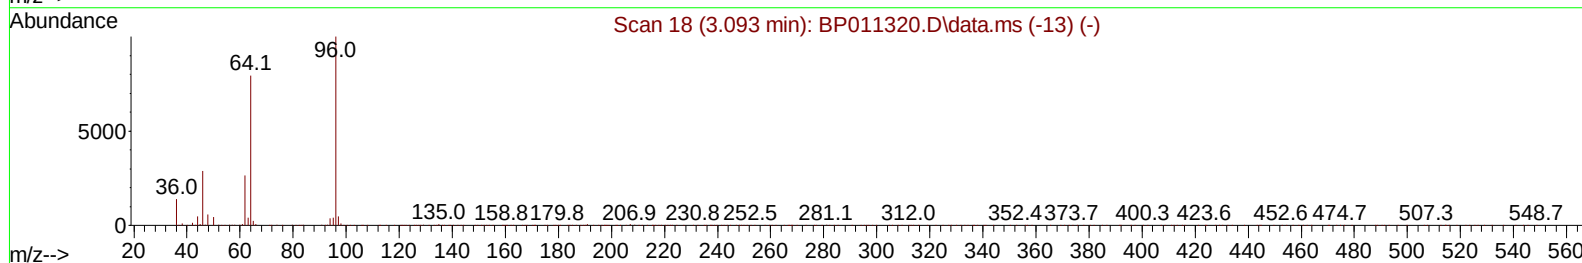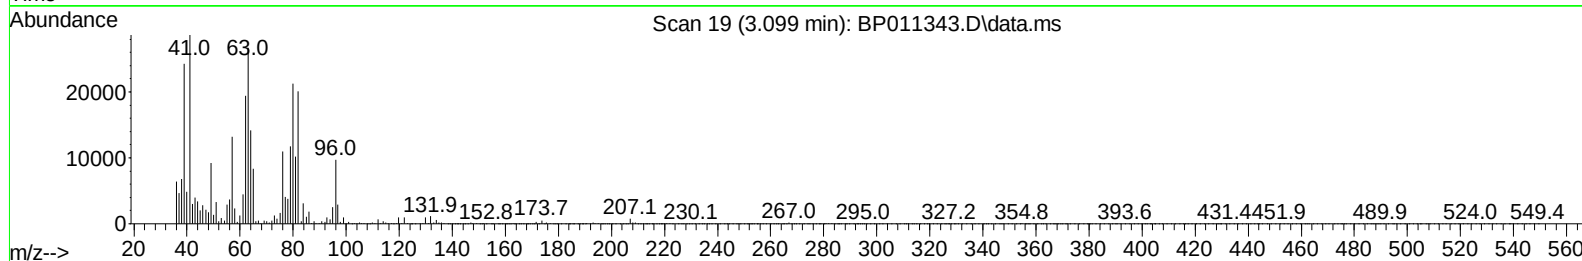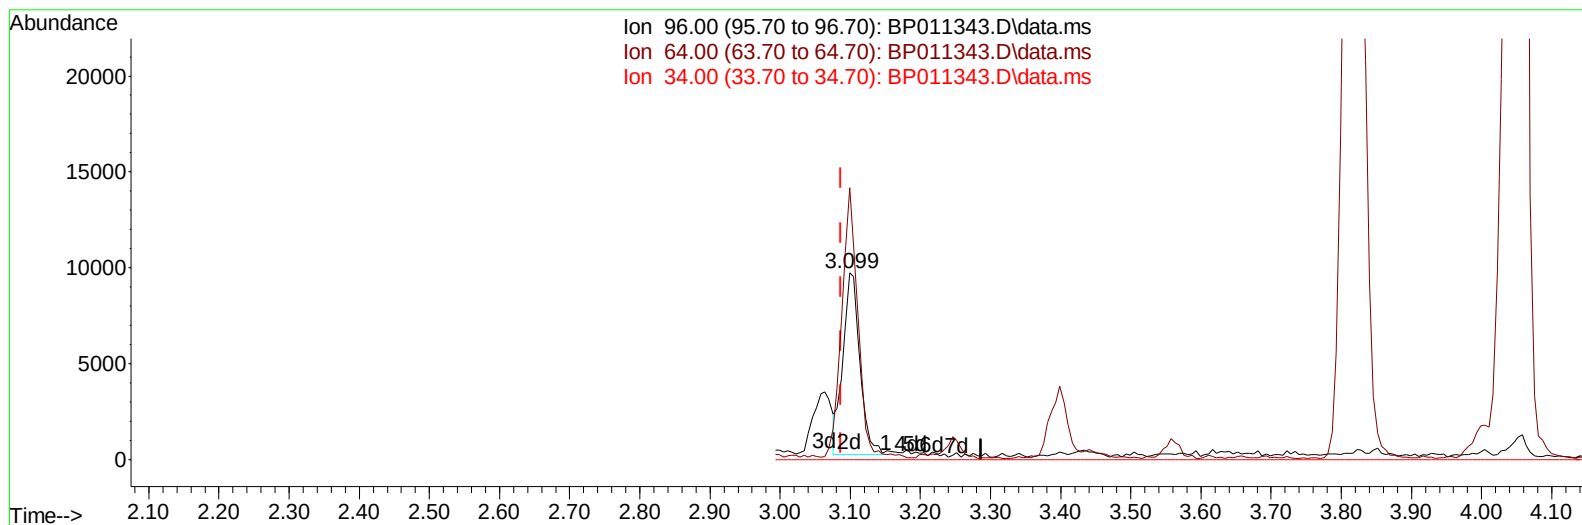

TIC: BP011343.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.099min (+ 0.012) 4.01 ng/uL m

response 15892

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	61.00	145.69#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011343.D
Acq On : 09 Aug 2022 23:04
Operator : CG/JU
Sample : N3956-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXF01

Manual IntegrationsAPPROVED

Quant Time: Aug 10 00:37:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 08 18:47:19 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/11/2022
Supervised By :Sohil Jodhani 08/12/2022

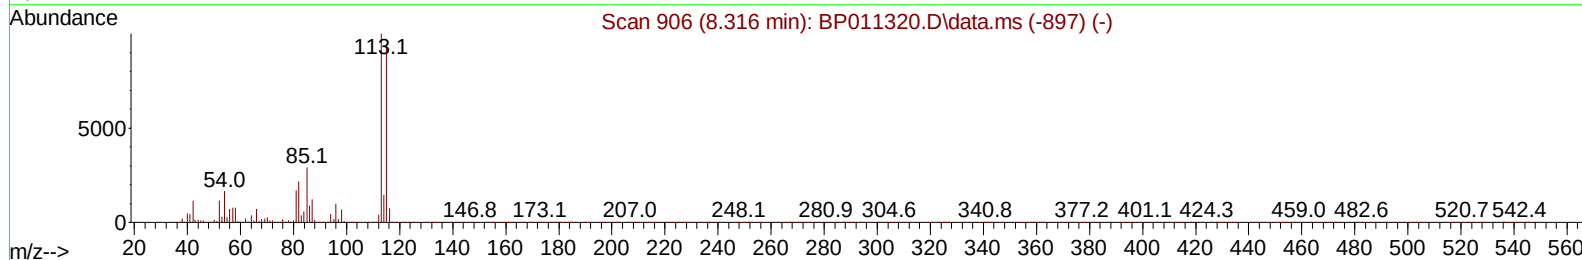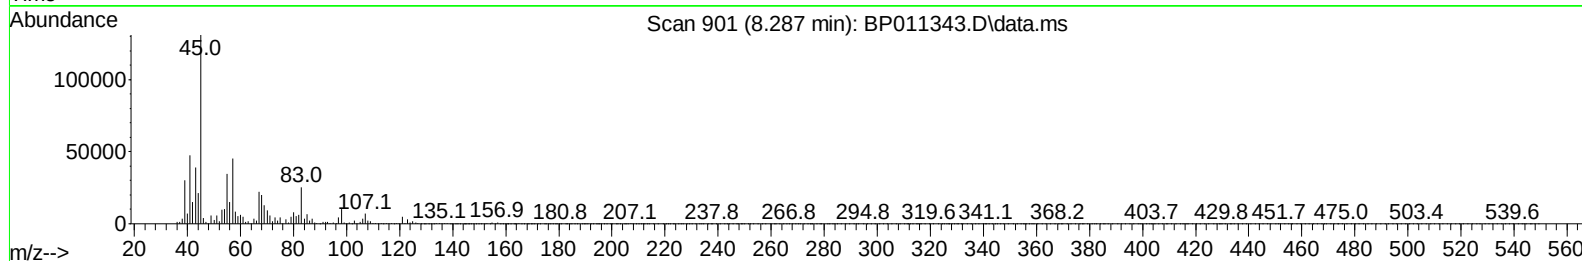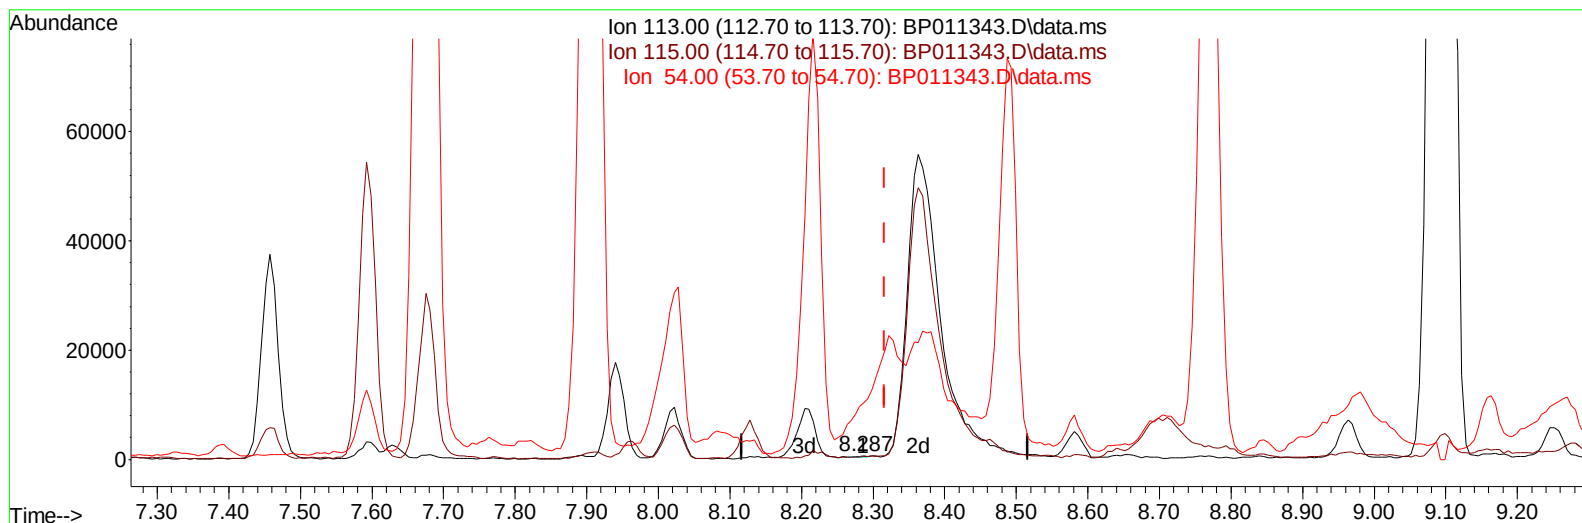

TIC: BP011343.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.287min (-0.029) 0.03 ng/u1

response 244

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	92.60	75.80
54.00	17.50	1575.19#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011343.D
Acq On : 09 Aug 2022 23:04
Operator : CG/JU
Sample : N3956-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXF01

Manual IntegrationsAPPROVED

Quant Time: Aug 10 00:37:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 08 18:47:19 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/11/2022
Supervised By :Sohil Jodhani 08/12/2022

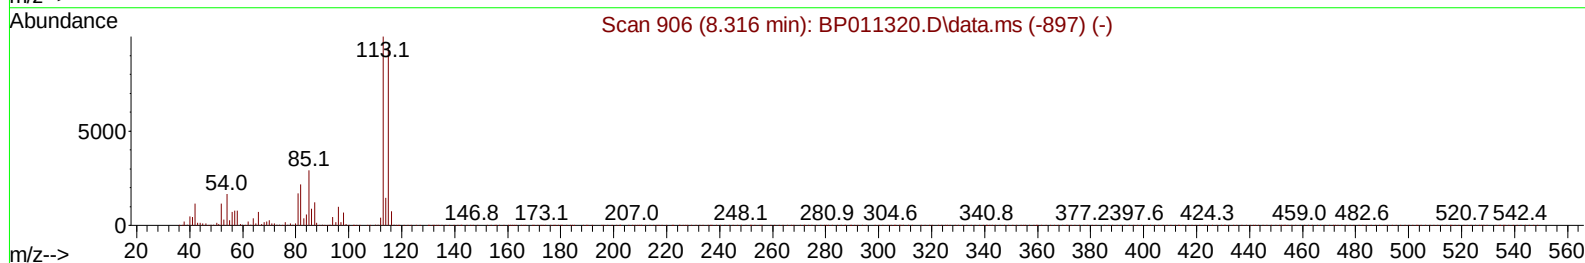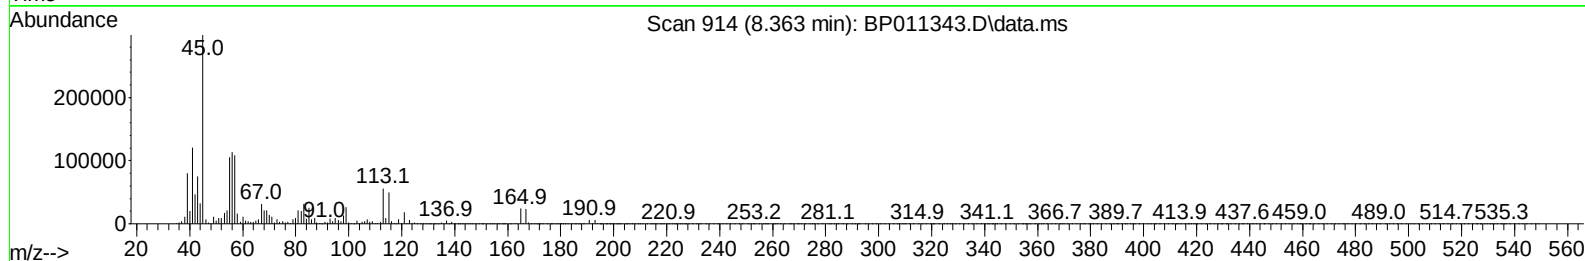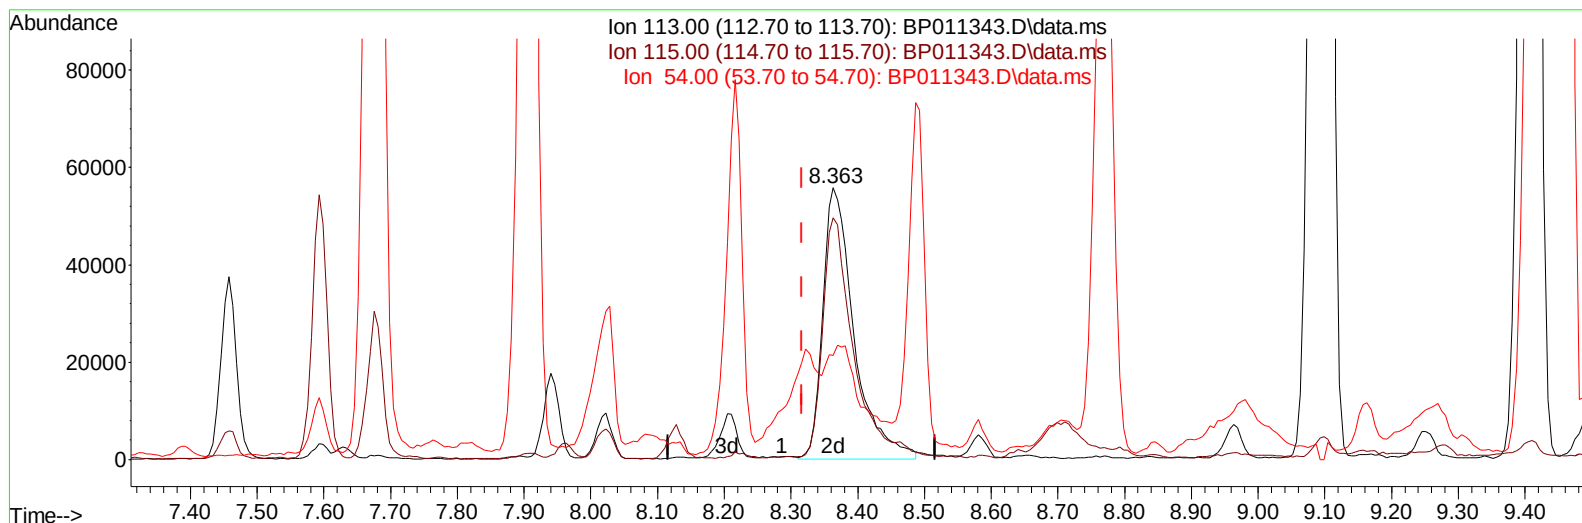

TIC: BP011343.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.363min (+ 0.047) 21.47 ng/ul m

response 181034

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	92.60	89.02
54.00	17.50	38.37#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011343.D
Acq On : 09 Aug 2022 23:04
Operator : CG/JU
Sample : N3956-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXF01

Manual IntegrationsAPPROVED

Quant Time: Aug 10 00:37:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 08 18:47:19 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/11/2022
Supervised By :Sohil Jodhani 08/12/2022

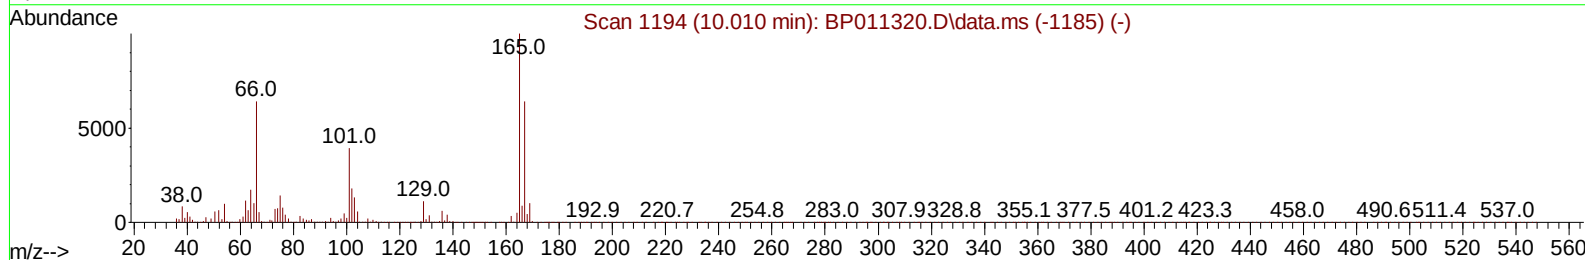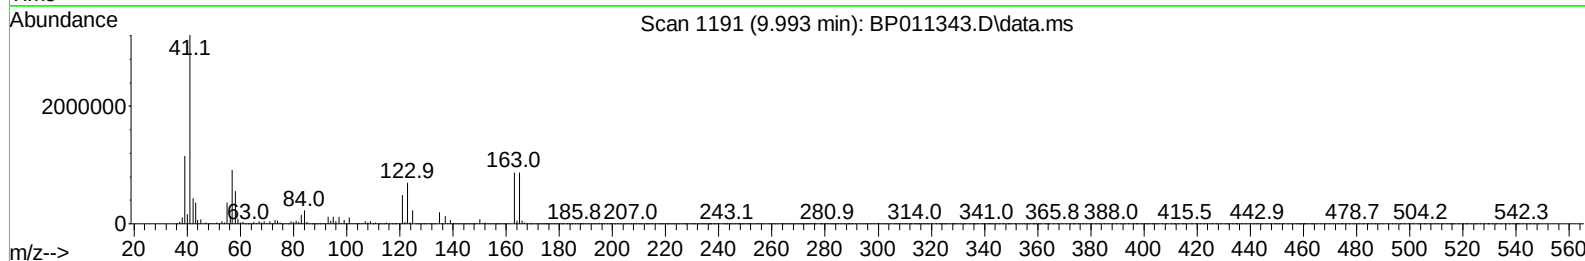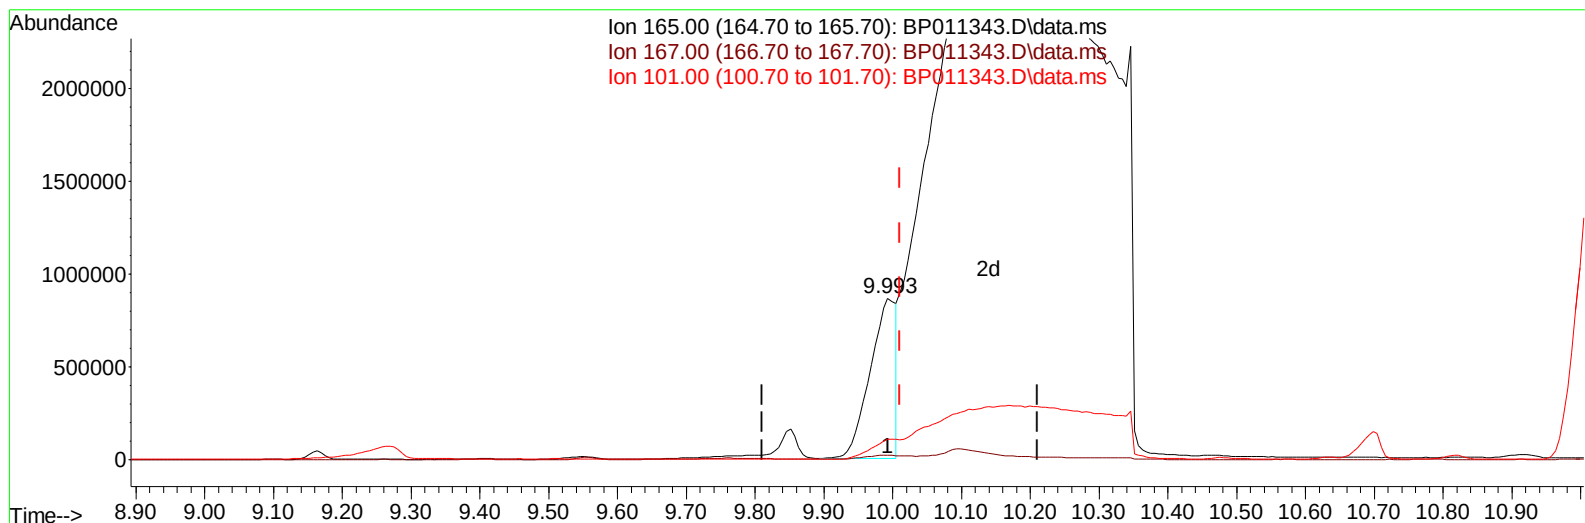

TIC: BP011343.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

9.993min (-0.018) 282.02 ng/uI

response 2260563

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	62.30	2.50#
101.00	39.10	12.63#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011343.D
Acq On : 09 Aug 2022 23:04
Operator : CG/JU
Sample : N3956-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXF01

Manual IntegrationsAPPROVED

Quant Time: Aug 10 00:37:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 08 18:47:19 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/11/2022
Supervised By :Sohil Jodhani 08/12/2022

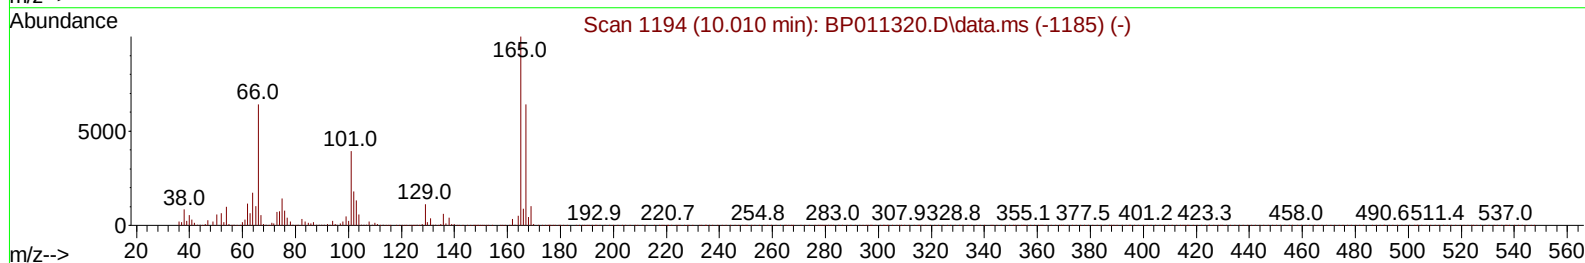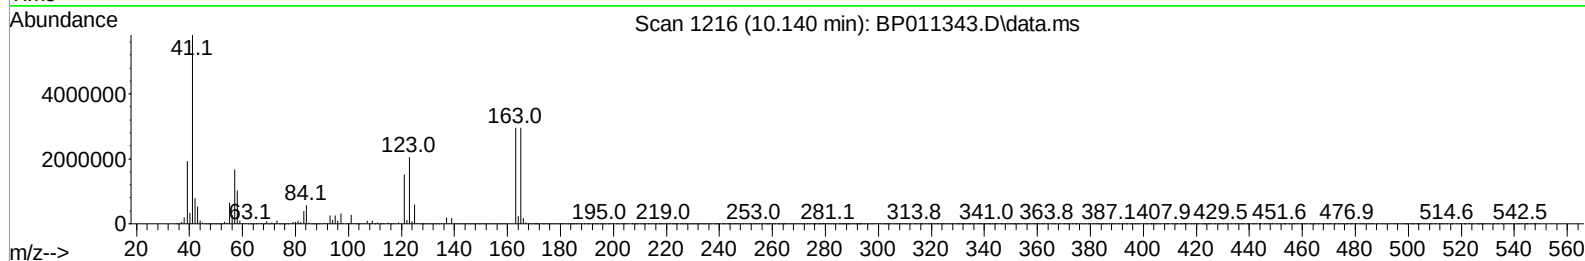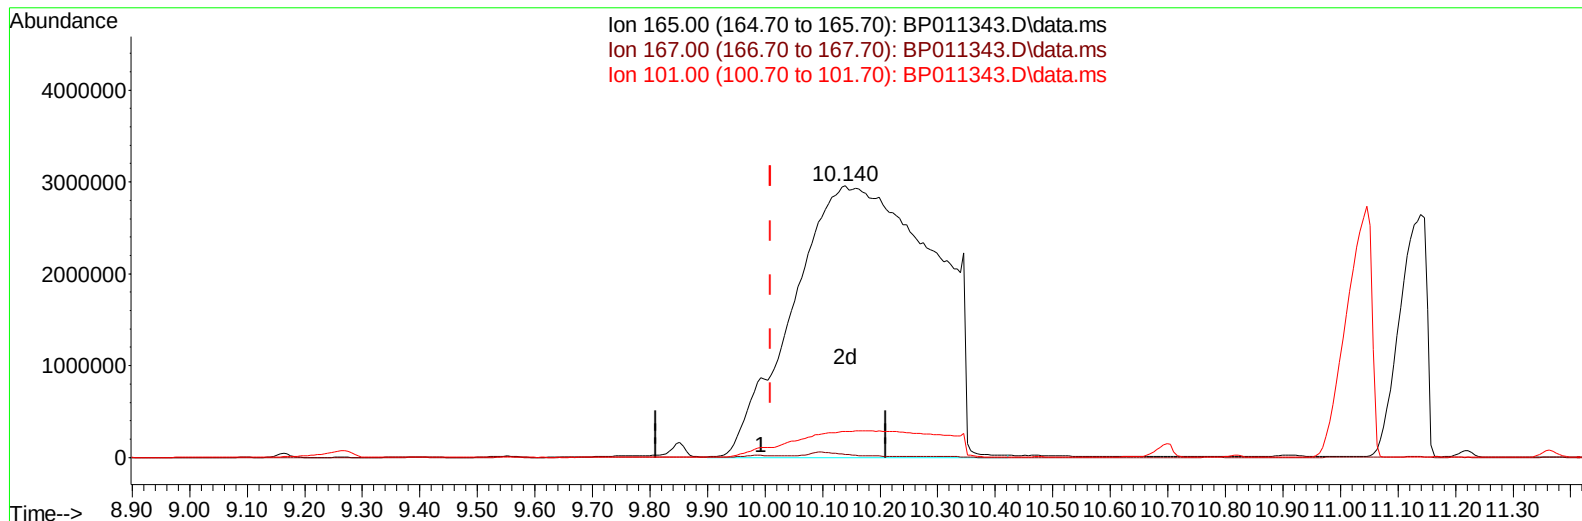

TIC: BP011343.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.140min (+ 0.129) 6296.12 ng/ul m

response 50467669

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	62.30	1.08#
101.00	39.10	9.67#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011343.D
Acq On : 09 Aug 2022 23:04
Operator : CG/JU
Sample : N3956-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXF01

Manual IntegrationsAPPROVED

Quant Time: Aug 10 00:37:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 08 18:47:19 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/11/2022
Supervised By :Sohil Jodhani 08/12/2022

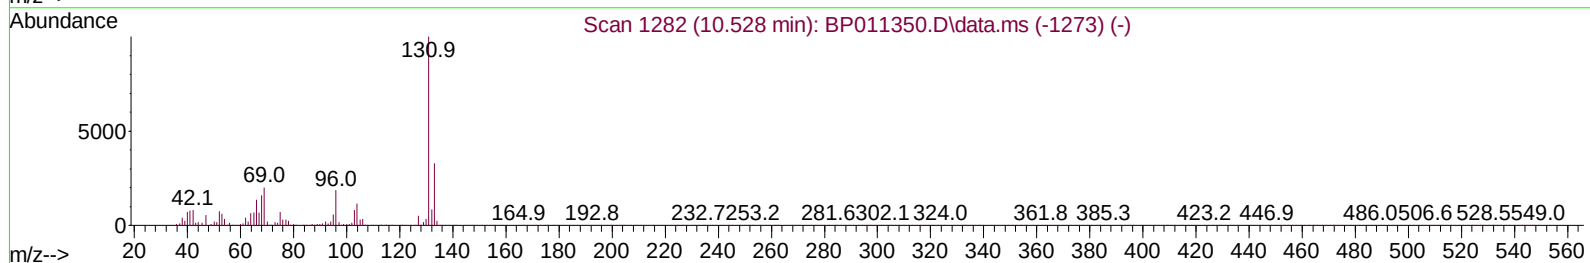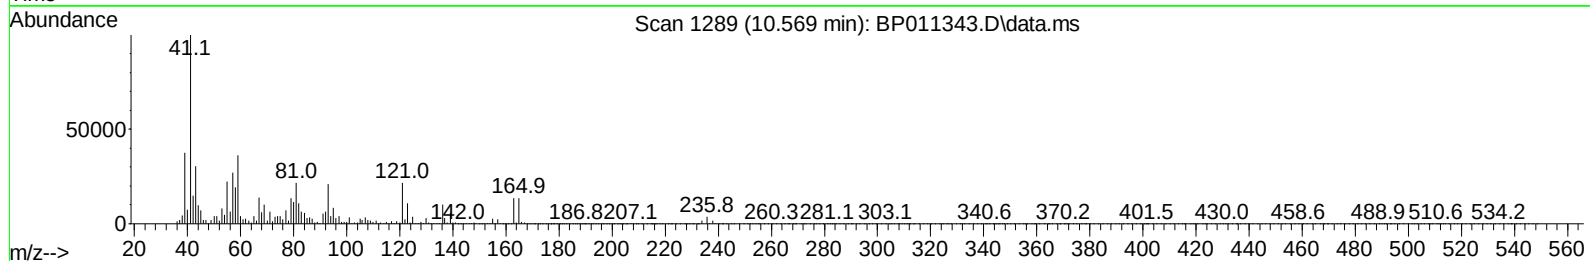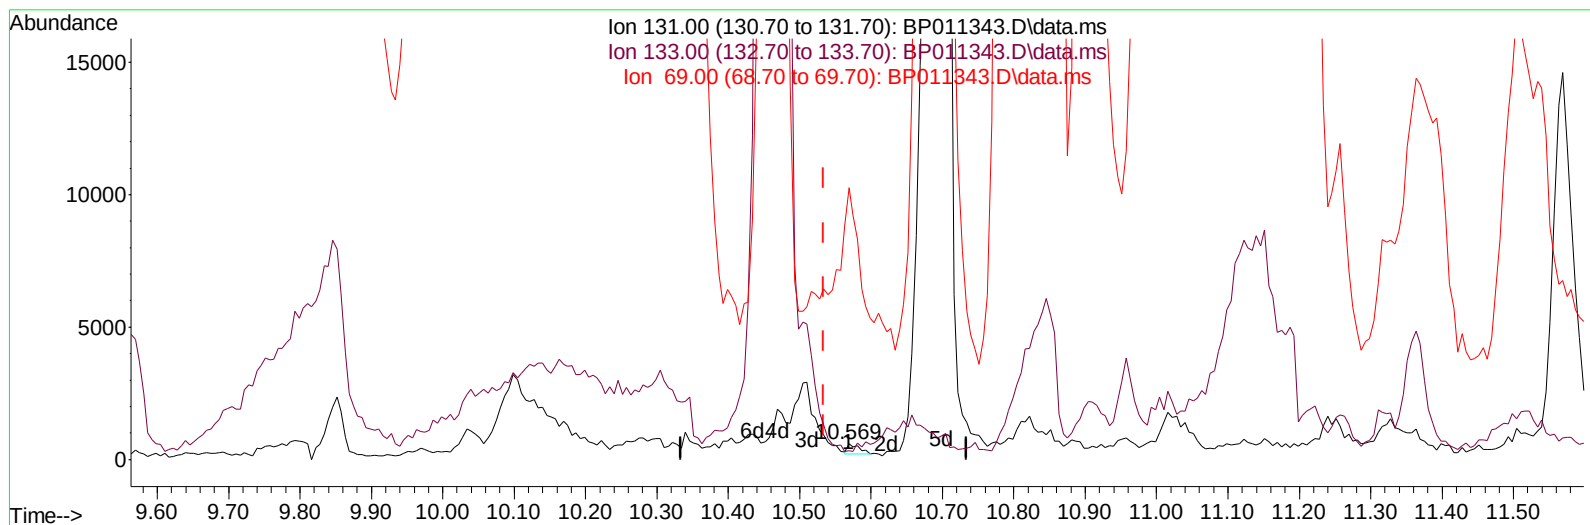

TIC: BP011343.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.569min (+ 0.035) 0.03 ng/u1

response 449

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	31.00	55.88#
69.00	19.00	1747.19#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011343.D
Acq On : 09 Aug 2022 23:04
Operator : CG/JU
Sample : N3956-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXF01

Manual IntegrationsAPPROVED

Quant Time: Aug 10 00:37:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 08 18:47:19 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/11/2022
Supervised By :Sohil Jodhani 08/12/2022

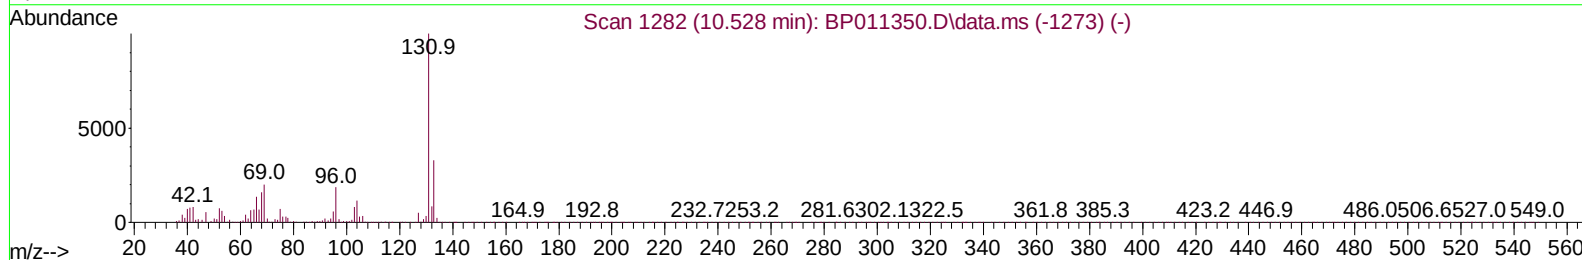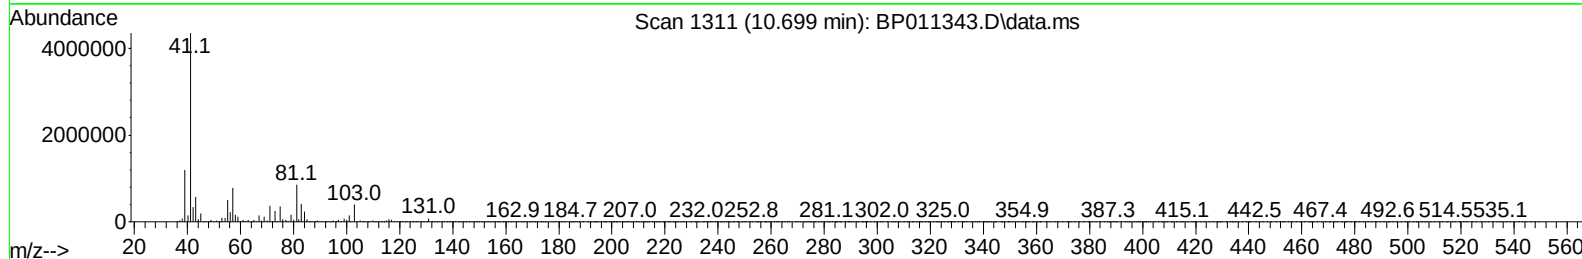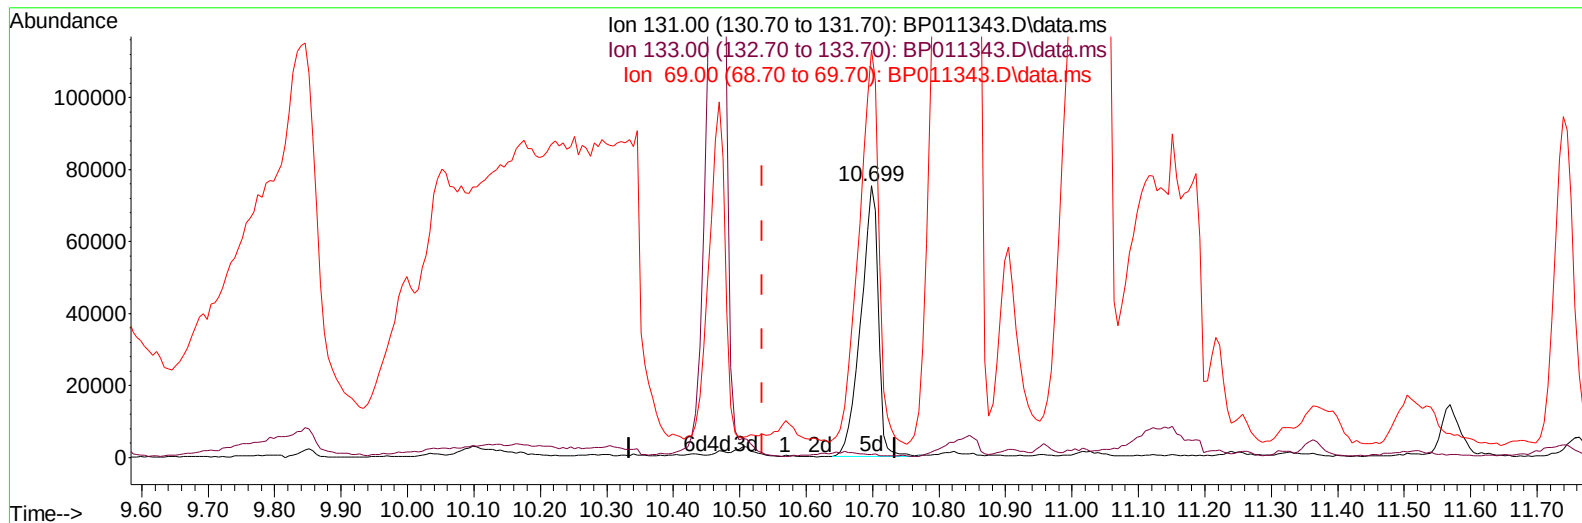

TIC: BP011343.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.699min (+ 0.165) 9.73 ng/ul m

response 136322

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	31.00	1.16#
69.00	19.00	150.07#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
 Data File : BP011343.D
 Acq On : 09 Aug 2022 23:04
 Operator : CG/JU
 Sample : N3956-02
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXF01

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/11/2022
 Supervised By :Sohil Jodhani 08/12/2022

Quant Time: Aug 10 00:37:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 08 18:47:19 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.593	152	121367	20.000	ng/ul	0.00
20) Naphthalene-d8	10.428	136	637014	20.000	ng/ul	0.05
38) Acenaphthene-d10	14.298	164	306305	20.000	ng/ul	0.04
64) Phenanthrene-d10	17.057	188	672885	20.000	ng/ul	0.02
79) Chrysene-d12	21.169	240	523696	20.000	ng/ul	0.00
88) Perylene-d12	23.474	264	427223	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.099	96	15892m	4.014	ng/uL	0.01
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	6.834	99	229090	21.329	ng/ul	0.06
9) Bis-(2-Chloroethyl)eth...	6.946	67	261700	34.363	ng/ul	0.00
11) 2-Chlorophenol-d4	7.140	132	237038	28.127	ng/ul	0.02
15) 4-Methylphenol-d8	8.363	113	181034m	21.466	ng/ul	0.05
21) Nitrobenzene-d5	8.769	128	161630	37.282	ng/ul	0.01
24) 2-Nitrophenol-d4	9.516	143	163706	41.244	ng/ul	0.04
28) 2,4-Dichlorophenol-d3	10.140	165	50467669m	6296.117	ng/ul	0.13
31) 4-Chloroaniline-d4	10.699	131	136322m	9.728	ng/ul	0.16
46) Dimethylphthalate-d6	13.757	166	977641	46.000	ng/ul	0.07
49) Acenaphthylene-d8	13.998	160	1042251	40.739	ng/ul	0.04
54) 4-Nitrophenol-d4	14.545	143	19600	5.049	ng/ul	0.05
60) Fluorene-d10	15.281	176	705074	38.793	ng/ul	0.01
65) 4,6-Dinitro-2-methylph...	15.410	200	116887	37.398	ng/ul	0.01
73) Anthracene-d10	17.157	188	1088288	35.983	ng/ul	0.02
81) Pyrene-d10	19.398	212	1100372	38.138	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.321	264	830235	38.535	ng/ul	0.00
Target Compounds						
12) 2-Chlorophenol	7.175	128	33272	3.789	ng/ul#	Qvalue 85

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011343.D
Acq On : 09 Aug 2022 23:04
Operator : CG/JU
Sample : N3956-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EXF01

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/11/2022
Supervised By :Sohil Jodhani 08/12/2022

Quant Time: Aug 10 00:37:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 08 18:47:19 2022
Response via : Initial Calibration

