




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
 Data File : BP011357.D
 Acq On : 10 Aug 2022 07:43
 Operator : CG/JU
 Sample : N4069-11
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJL5

Manual IntegrationsAPPROVED

Quant Time: Aug 10 08:31:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 08 18:47:19 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/10/2022
 Supervised By :Sohil Jodhani 08/10/2022

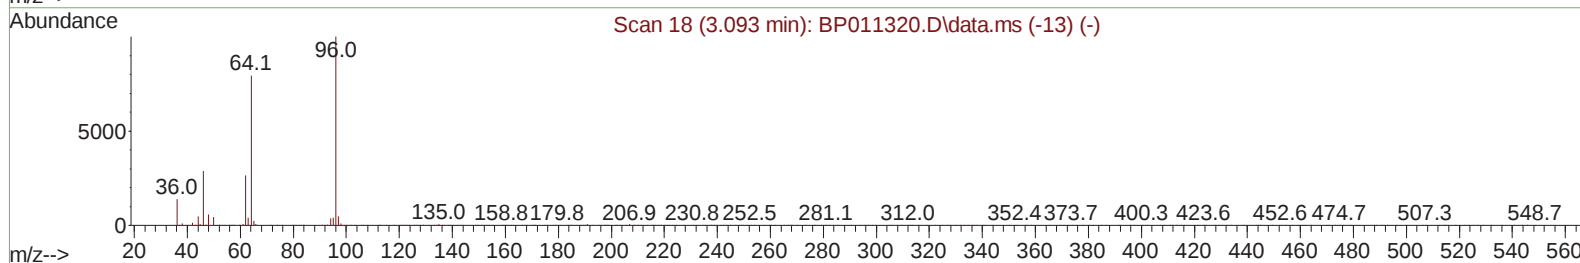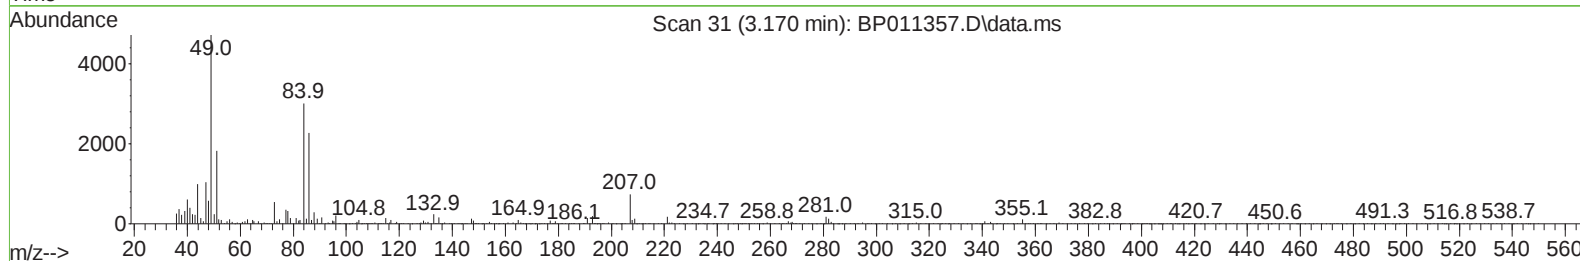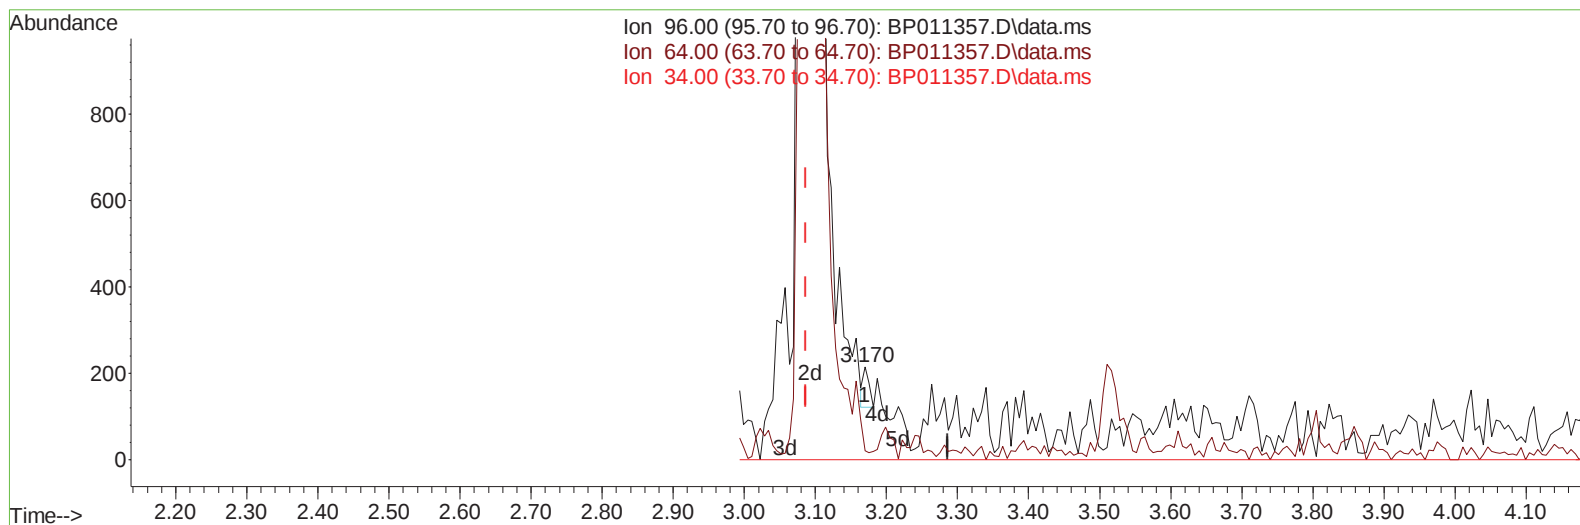

TIC: BP011357.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.170min (+ 0.083) 0.02 ng/uL

response 53

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	61.00	57.48
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011357.D
Acq On : 10 Aug 2022 07:43
Operator : CG/JU
Sample : N4069-11
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJL5

Manual IntegrationsAPPROVED

Quant Time: Aug 10 08:31:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 08 18:47:19 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/10/2022
Supervised By :Sohil Jodhani 08/10/2022

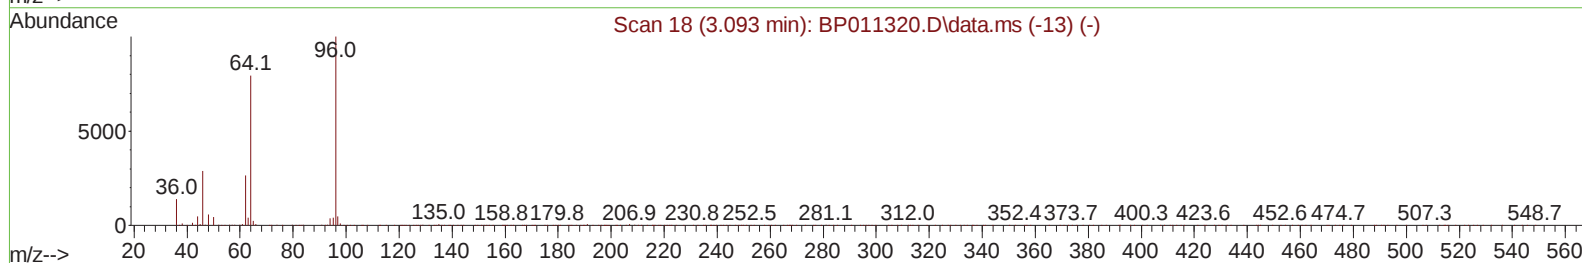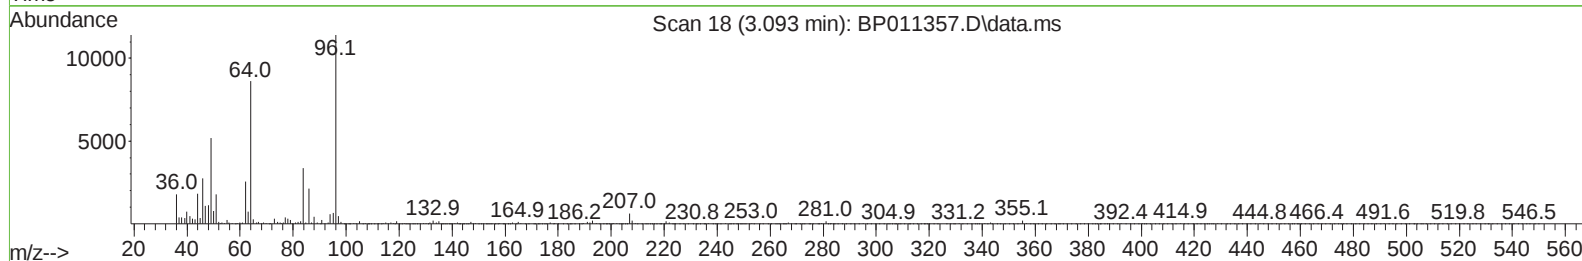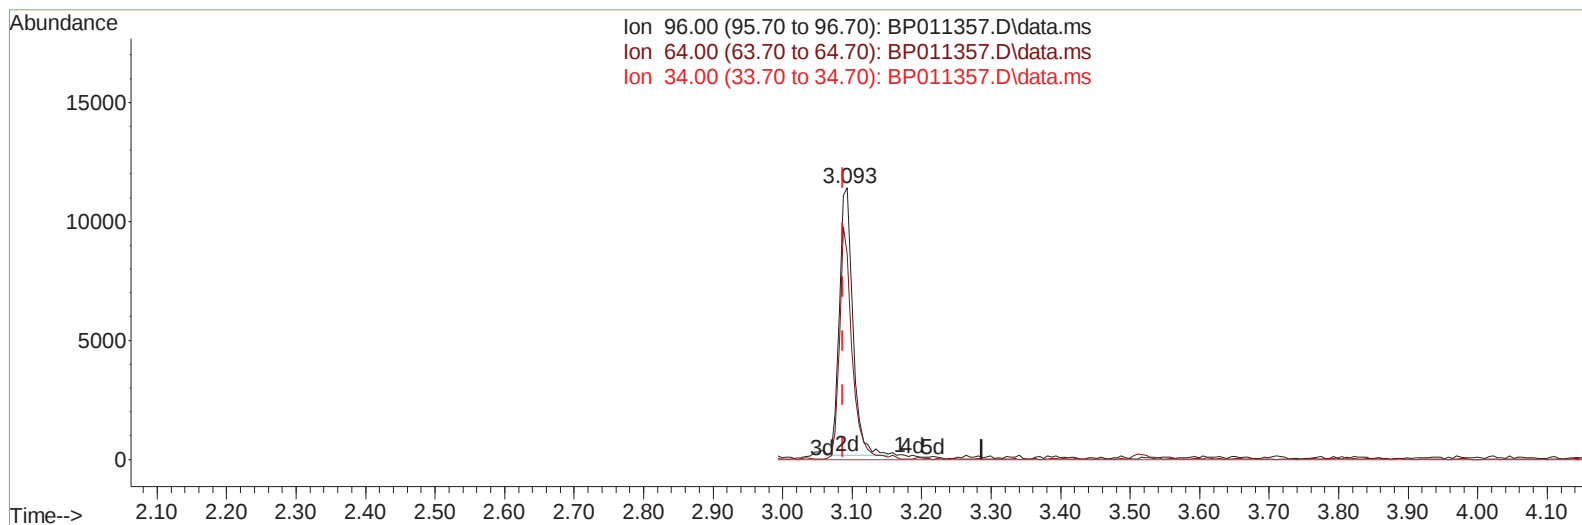

TIC: BP011357.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.093min (+ 0.006) 4.45 ng/uL m

response 15189

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	61.00	75.59#
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
 Data File : BP011357.D
 Acq On : 10 Aug 2022 07:43
 Operator : CG/JU
 Sample : N4069-11
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJL5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/10/2022
 Supervised By :Sohil Jodhani 08/10/2022

Quant Time: Aug 10 08:31:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 08 18:47:19 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.587	152	104732	20.000	ng/ul	0.00
20) Naphthalene-d8	10.375	136	442897	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.257	164	251867	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.028	188	507881	20.000	ng/ul	-0.01
79) Chrysene-d12	21.157	240	477611	20.000	ng/ul	-0.01
88) Perylene-d12	23.463	264	475109	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.093	96	15189m	4.446	ng/uL	0.00
4) Pyridine-d5	3.511	84	63289	7.344	ng/ul	0.01
7) Phenol-d5	6.769	99	61593	6.645	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.934	67	172321	26.221	ng/ul	0.00
11) 2-Chlorophenol-d4	7.116	132	163807	22.525	ng/ul	0.00
15) 4-Methylphenol-d8	8.305	113	106808	14.677	ng/ul	-0.01
21) Nitrobenzene-d5	8.752	128	94845	31.466	ng/ul	0.00
24) 2-Nitrophenol-d4	9.463	143	92990	33.696	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.004	165	150572	27.018	ng/ul	0.00
31) 4-Chloroaniline-d4	10.528	131	150504	15.447	ng/ul	0.00
46) Dimethylphthalate-d6	13.681	166	582650	33.340	ng/ul	0.00
49) Acenaphthylene-d8	13.945	160	645375	30.679	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.492	143	13034	4.083	ng/ul	0.00
60) Fluorene-d10	15.263	176	480130	32.126	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.392	200	73037	30.960	ng/ul	0.00
73) Anthracene-d10	17.128	188	831340	36.417	ng/ul	-0.01
81) Pyrene-d10	19.392	212	953879	36.251	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.321	264	888189	37.070	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011357.D
Acq On : 10 Aug 2022 07:43
Operator : CG/JU
Sample : N4069-11
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJL5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/10/2022
Supervised By :Sohil Jodhani 08/10/2022

Quant Time: Aug 10 08:31:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 08 18:47:19 2022
Response via : Initial Calibration

