

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
 Data File : BP011343.D
 Acq On : 09 Aug 2022 23:04
 Operator : CG/JU
 Sample : N3956-02
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EXF01

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 08/11/2022
 Supervised By :Sohil Jodhani 08/12/2022

Quant Time: Aug 10 00:37:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 08 18:47:19 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.593	152	121367	20.000	ng/u1	0.00
20) Naphthalene-d8	10.428	136	637014	20.000	ng/u1	0.05
38) Acenaphthene-d10	14.298	164	306305	20.000	ng/u1	0.04
64) Phenanthrene-d10	17.057	188	672885	20.000	ng/u1	0.02
79) Chrysene-d12	21.169	240	523696	20.000	ng/u1	0.00
88) Perylene-d12	23.474	264	427223	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.099	96	15892m	4.014	ng/uL	0.01
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	6.834	99	229090	21.329	ng/u1	0.06
9) Bis-(2-Chloroethyl)eth...	6.946	67	261700	34.363	ng/u1	0.00
11) 2-Chlorophenol-d4	7.140	132	237038	28.127	ng/u1	0.02
15) 4-Methylphenol-d8	8.363	113	181034m	21.466	ng/u1	0.05
21) Nitrobenzene-d5	8.769	128	161630	37.282	ng/u1	0.01
24) 2-Nitrophenol-d4	9.516	143	163706	41.244	ng/u1	0.04
28) 2,4-Dichlorophenol-d3	10.140	165	50467669m	6296.117	ng/u1	0.13
31) 4-Chloroaniline-d4	10.699	131	136322m	9.728	ng/u1	0.16
46) Dimethylphthalate-d6	13.757	166	977641	46.000	ng/u1	0.07
49) Acenaphthylene-d8	13.998	160	1042251	40.739	ng/u1	0.04
54) 4-Nitrophenol-d4	14.545	143	19600	5.049	ng/u1	0.05
60) Fluorene-d10	15.281	176	705074	38.793	ng/u1	0.01
65) 4,6-Dinitro-2-methylph...	15.410	200	116887	37.398	ng/u1	0.01
73) Anthracene-d10	17.157	188	1088288	35.983	ng/u1	0.02
81) Pyrene-d10	19.398	212	1100372	38.138	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.321	264	830235	38.535	ng/u1	0.00
Target Compounds						
12) 2-Chlorophenol	7.175	128	33272	3.789	ng/u1#	Qvalue 85

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011343.D
Acq On : 09 Aug 2022 23:04
Operator : CG/JU
Sample : N3956-02
Misc :
ALS Vial : 24 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
EXF01

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 08/11/2022
Supervised By :Sohil Jodhani 08/12/2022

Quant Time: Aug 10 00:37:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Aug 08 18:47:19 2022
Response via : Initial Calibration

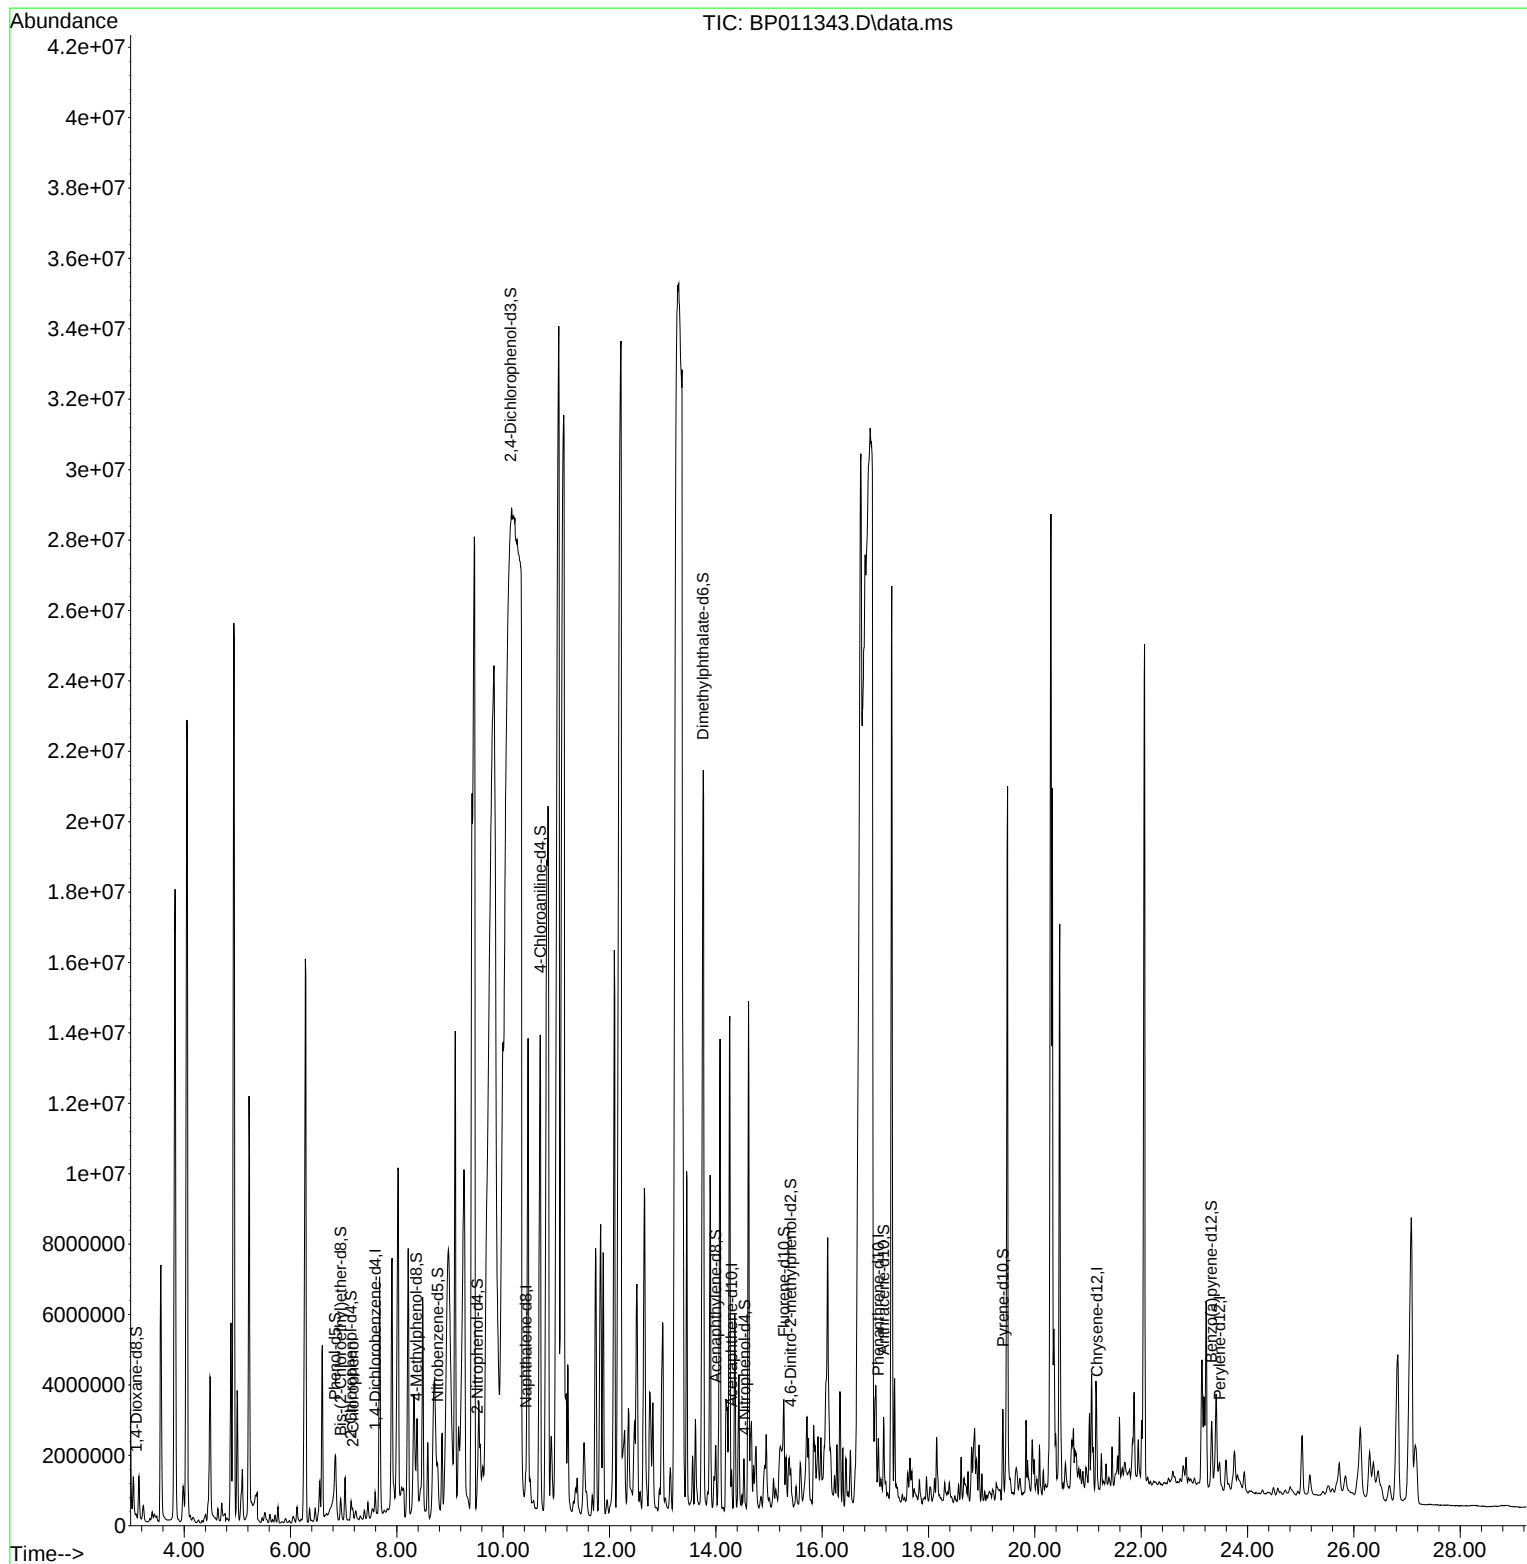

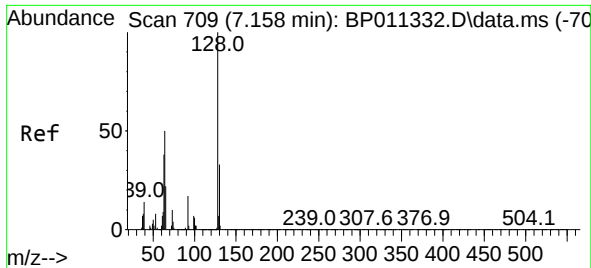

#12
2-Chlorophenol
Concen: 3.789 ng/ul
RT: 7.175 min Scan# 712
Delta R.T. 0.018 min
Lab File: BP011343.D
Acq: 09 Aug 2022 23:04

Instrument :
BNA_P
ClientSampleId :
EXF01

Tgt Ion:128 Resp: 33272
Ion Ratio Lower Upper
128 100
64 70.7 43.8 65.6
130 30.8 25.4 38.2

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 08/11/2022
Supervised By :Sohil Jodhani 08/12/2022

