

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
 Data File : BP011321.D
 Acq On : 09 Aug 2022 10:16
 Operator : CG/JU
 Sample : PB146785BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK785

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011321.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.093	14	18	28	rVB	54958	76410	2.56%	0.212%
2	3.505	85	88	107	rBV	594255	948777	31.76%	2.633%
3	3.811	136	140	149	rVB	15258	25067	0.84%	0.070%
4	6.775	636	644	658	rBV	690679	1105277	37.00%	3.067%
5	6.940	665	672	682	rVB	563662	863015	28.89%	2.395%
6	7.122	696	703	717	rBV	724580	1121580	37.54%	3.112%
7	7.587	775	782	796	rVB	639426	1021024	34.18%	2.833%
8	8.310	896	905	925	rBV	797380	1283918	42.98%	3.563%
9	8.752	973	980	992	rBV	636461	1008941	33.77%	2.800%
10	9.469	1095	1102	1111	rBV	455476	741515	24.82%	2.058%
11	9.869	1166	1170	1175	rVB8	1925	3491	0.12%	0.010%
12	10.004	1187	1193	1211	rBV	703899	1174906	39.33%	3.260%
13	10.381	1249	1257	1265	rBV	856012	1394229	46.67%	3.869%
14	10.534	1275	1283	1300	rBV	666619	1200797	40.19%	3.332%
15	11.987	1524	1530	1537	rBV2	9771	20905	0.70%	0.058%
16	12.210	1562	1568	1571	rBV7	1808	3342	0.11%	0.009%
17	12.975	1691	1698	1700	rBV8	2559	4702	0.16%	0.013%
18	13.234	1738	1742	1746	rBV7	3369	5540	0.19%	0.015%
19	13.687	1812	1819	1832	rBV	1294844	1767160	59.15%	4.904%
20	13.951	1856	1864	1876	rBV	1395121	1988138	66.55%	5.517%
21	14.263	1910	1917	1925	rBV	1201787	1673601	56.02%	4.644%
22	14.486	1949	1955	1974	rBV	349589	712974	23.87%	1.978%
23	15.263	2080	2087	2103	rBV	1712754	2464404	82.49%	6.839%
24	15.398	2104	2110	2122	rVV	486514	691673	23.15%	1.919%
25	15.510	2125	2129	2139	rVB3	19144	33337	1.12%	0.093%
26	15.957	2200	2205	2209	rBV7	2972	6280	0.21%	0.017%
27	16.057	2217	2222	2226	rVB8	4810	7145	0.24%	0.020%
28	16.169	2237	2241	2244	rBV6	2703	4230	0.14%	0.012%
29	16.710	2329	2333	2338	rBV8	3743	5208	0.17%	0.014%
30	16.822	2347	2352	2359	rVB7	4302	8794	0.29%	0.024%
31	17.033	2381	2388	2399	rBV	1373271	1931756	64.66%	5.361%
32	17.133	2399	2405	2435	rVB	1932128	2703904	90.51%	7.503%
33	18.416	2619	2623	2626	rBV6	4866	6998	0.23%	0.019%
34	18.516	2638	2640	2644	rBV5	3110	3466	0.12%	0.010%
35	18.969	2713	2717	2723	rBV4	22791	35731	1.20%	0.099%
36	19.039	2725	2729	2734	rVV2	20383	30541	1.02%	0.085%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011321.D
Acq On : 09 Aug 2022 10:16
Operator : CG/JU
Sample : PB146785BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK785

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Title : SVOA CALIBRATION

37	19.392	2784	2789	2799	rBV	2271890	2987494	100.00%	8.290%
38	21.163	3085	3090	3098	rBV	1595048	2022167	67.69%	5.611%
39	21.286	3108	3111	3117	rBV	85223	138415	4.63%	0.384%
40	23.321	3451	3457	3466	rBV2	1480021	2803343	93.84%	7.779%
41	23.474	3476	3483	3497	rVB2	1032758	2006293	67.16%	5.567%




Sum of corrected areas: 36036488

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011321.D
Acq On : 09 Aug 2022 10:16
Operator : CG/JU
Sample : PB146785BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK785

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

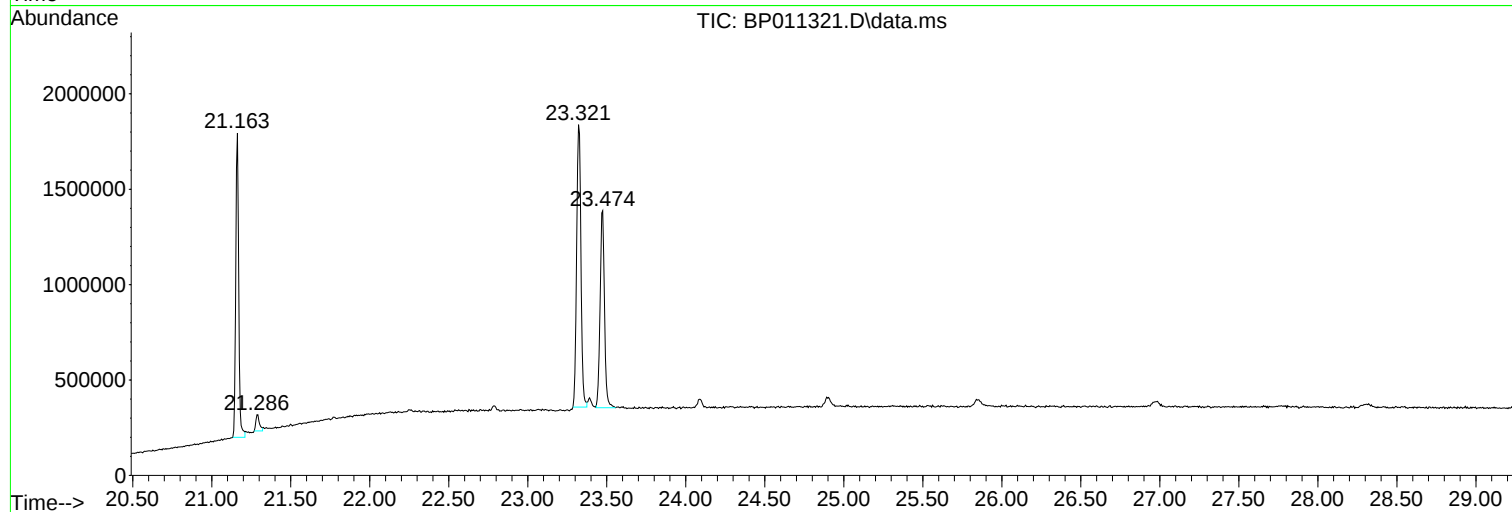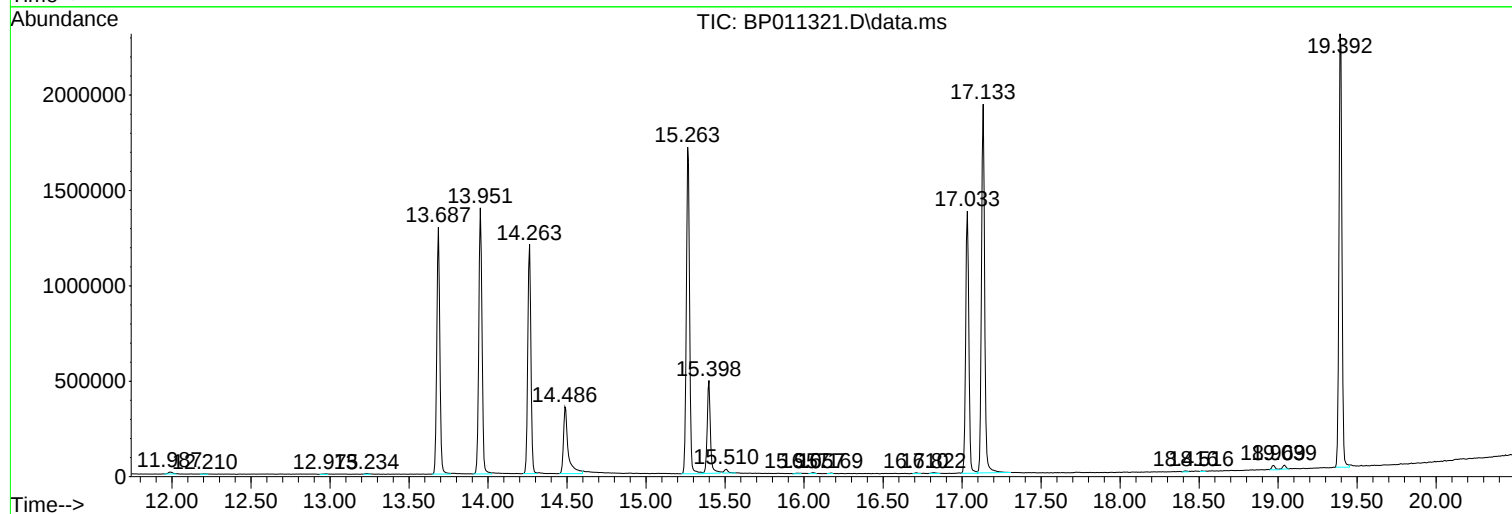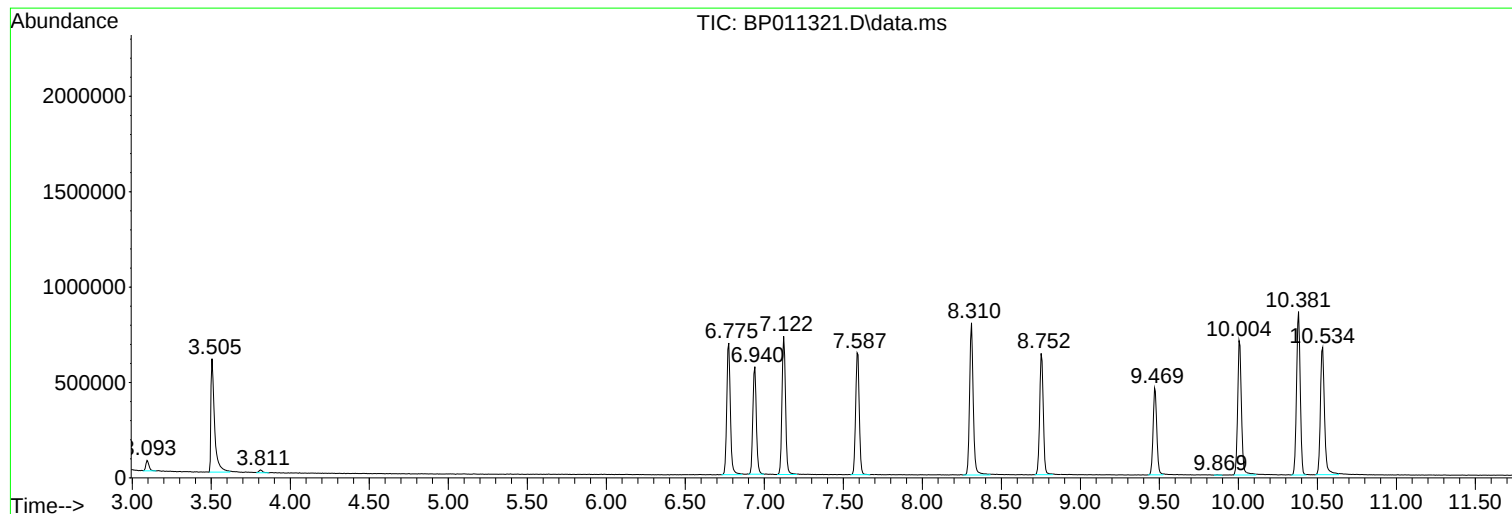

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011321.D
Acq On : 09 Aug 2022 10:16
Operator : CG/JU
Sample : PB146785BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK785

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011321.D
Acq On : 09 Aug 2022 10:16
Operator : CG/JU
Sample : PB146785BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK785

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc