

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
 Data File : BP011323.D
 Acq On : 09 Aug 2022 11:26
 Operator : CG/JU
 Sample : N3900-11
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0C88

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011323.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.093	14	18	25	rVB	42481	55057	1.46%	0.149%
2	3.517	88	90	103	rVV	82386	145448	3.85%	0.393%
3	3.717	120	124	130	rVB3	21376	39154	1.04%	0.106%
4	3.811	136	140	145	rVV2	13382	19611	0.52%	0.053%
5	3.887	149	153	161	rVB3	9087	14890	0.39%	0.040%
6	4.111	185	191	197	rVB3	7813	18229	0.48%	0.049%
7	4.264	212	217	219	rBV4	9107	14570	0.39%	0.039%
8	4.299	219	223	227	rVB	26910	39432	1.04%	0.106%
9	4.558	257	267	270	rBV3	18254	34290	0.91%	0.093%
10	4.593	270	273	277	rVB5	14832	19946	0.53%	0.054%
11	4.799	304	308	314	rVB3	8219	12333	0.33%	0.033%
12	4.875	315	321	327	rVB6	15786	33081	0.88%	0.089%
13	5.028	342	347	350	rBV7	6855	12429	0.33%	0.034%
14	5.111	358	361	367	rVB8	7259	11078	0.29%	0.030%
15	5.393	406	409	415	rVB8	6886	11447	0.30%	0.031%
16	5.475	415	423	429	rBV10	6841	17891	0.47%	0.048%
17	5.534	429	433	440	rBV6	9340	15169	0.40%	0.041%
18	5.687	452	459	465	rVB8	6927	15914	0.42%	0.043%
19	5.893	489	494	501	rVB8	9081	17934	0.47%	0.048%
20	6.081	519	526	538	rVB	21890	45608	1.21%	0.123%
21	6.510	594	599	603	rVB8	5924	10356	0.27%	0.028%
22	6.569	603	609	615	rBV3	8308	14636	0.39%	0.040%
23	6.775	638	644	657	rVV	112042	185764	4.91%	0.502%
24	6.940	665	672	684	rBV	539531	875173	23.16%	2.363%
25	7.122	697	703	711	rBV	490331	744651	19.70%	2.011%
26	7.187	711	714	723	rVB7	10641	22022	0.58%	0.059%
27	7.487	762	765	772	rVB2	12549	19232	0.51%	0.052%
28	7.587	775	782	791	rBV	626111	986046	26.09%	2.662%
29	7.699	798	801	809	rVB8	6323	12512	0.33%	0.034%
30	7.893	829	834	840	rVB	19485	30817	0.82%	0.083%
31	8.081	861	866	872	rBV4	9065	14243	0.38%	0.038%
32	8.310	893	905	915	rVV	332334	545074	14.42%	1.472%
33	8.693	963	970	974	rBV2	24796	40813	1.08%	0.110%
34	8.757	974	981	992	rVB2	750252	1381278	36.55%	3.729%
35	8.934	1007	1011	1021	rVB9	11311	25111	0.66%	0.068%
36	9.034	1021	1028	1032	rBV2	14182	22798	0.60%	0.062%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
 Data File : BP011323.D
 Acq On : 09 Aug 2022 11:26
 Operator : CG/JU
 Sample : N3900-11
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0C88

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

37	9.163	1040	1050	1054	rBV4	12405	25369	0.67%	0.068%
38	9.387	1083	1088	1094	rVB	17029	26995	0.71%	0.073%
39	9.475	1094	1103	1112	rBV	409780	676128	17.89%	1.826%
40	9.575	1115	1120	1125	rVV2	33124	54100	1.43%	0.146%
41	9.634	1125	1130	1132	rVV2	17753	32239	0.85%	0.087%
42	9.663	1132	1135	1141	rVB	18761	29885	0.79%	0.081%
43	9.775	1147	1154	1164	rBV3	68124	132262	3.50%	0.357%
44	9.951	1180	1184	1187	rVB3	8680	12141	0.32%	0.033%
45	10.004	1187	1193	1203	rBV	611773	1010859	26.75%	2.729%
46	10.228	1226	1231	1236	rBV2	9765	19060	0.50%	0.051%
47	10.381	1241	1257	1263	rBV	848604	1475167	39.03%	3.983%
48	10.434	1263	1266	1271	rVB2	32808	48410	1.28%	0.131%
49	10.493	1271	1276	1278	rBV	61167	92082	2.44%	0.249%
50	10.528	1278	1282	1291	rVB	462386	797228	21.09%	2.153%
51	10.640	1298	1301	1306	rVB6	7593	10635	0.28%	0.029%
52	10.846	1329	1336	1340	rBV6	5902	10892	0.29%	0.029%
53	10.957	1351	1355	1361	rBV5	5739	9721	0.26%	0.026%
54	11.040	1366	1369	1374	rVB	7057	10146	0.27%	0.027%
55	11.298	1405	1413	1420	rBV3	14234	25446	0.67%	0.069%
56	11.410	1423	1432	1438	rBV6	7503	19324	0.51%	0.052%
57	11.487	1438	1445	1451	rBV8	9926	18643	0.49%	0.050%
58	11.663	1471	1475	1482	rVB2	7771	14232	0.38%	0.038%
59	11.957	1519	1525	1527	rBV3	11508	21805	0.58%	0.059%
60	11.981	1527	1529	1534	rVV	13690	20456	0.54%	0.055%
61	12.275	1570	1579	1580	rBV7	5067	10756	0.28%	0.029%
62	12.598	1626	1634	1638	rBV8	6088	12402	0.33%	0.033%
63	12.669	1641	1646	1649	rVV7	6025	9885	0.26%	0.027%
64	12.981	1693	1699	1705	rVB8	6362	14081	0.37%	0.038%
65	13.134	1721	1725	1731	rBV8	12469	22920	0.61%	0.062%
66	13.240	1736	1743	1747	rVV8	9901	19085	0.50%	0.052%
67	13.316	1751	1756	1763	rVB10	6675	12660	0.33%	0.034%
68	13.434	1771	1776	1782	rVB	16006	23965	0.63%	0.065%
69	13.504	1782	1788	1795	rBV	45937	68213	1.80%	0.184%
70	13.687	1807	1819	1828	rBV	1434891	1931865	51.11%	5.216%
71	13.769	1830	1833	1838	rVV6	8861	16257	0.43%	0.044%
72	13.951	1857	1864	1877	rBV	1432870	2062839	54.58%	5.570%
73	14.045	1877	1880	1884	rVV5	7082	12522	0.33%	0.034%
74	14.087	1884	1887	1893	rVB2	13186	20680	0.55%	0.056%
75	14.263	1910	1917	1922	rBV	1177172	1691288	44.75%	4.567%
76	14.304	1922	1924	1935	rVB2	38795	63011	1.67%	0.170%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
 Data File : BP011323.D
 Acq On : 09 Aug 2022 11:26
 Operator : CG/JU
 Sample : N3900-11
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0C88

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

77	14.492	1951	1956	1969	rBV2	39157	94853	2.51%	0.256%
78	14.598	1970	1974	1979	rVV5	11758	23375	0.62%	0.063%
79	14.904	2020	2026	2035	rBV6	13822	25373	0.67%	0.069%
80	15.104	2054	2060	2067	rVB6	8032	17918	0.47%	0.048%
81	15.263	2078	2087	2100	rBV	1903000	2702564	71.50%	7.297%
82	15.398	2103	2110	2121	rVV	575428	817103	21.62%	2.206%
83	15.504	2125	2128	2139	rVB	20028	37416	0.99%	0.101%
84	15.675	2155	2157	2167	rVB	5093	13950	0.37%	0.038%
85	15.792	2172	2177	2181	rVB7	6874	11773	0.31%	0.032%
86	16.816	2347	2351	2358	rBV8	5406	11576	0.31%	0.031%
87	17.033	2381	2388	2397	rVV	1421879	1936015	51.22%	5.227%
88	17.133	2398	2405	2425	rVB2	2338297	3309403	87.56%	8.935%
89	17.945	2540	2543	2548	rBV7	10321	15257	0.40%	0.041%
90	18.369	2612	2615	2618	rBV5	8824	10567	0.28%	0.029%
91	18.969	2713	2717	2723	rBV	32056	49270	1.30%	0.133%
92	19.039	2724	2729	2737	rVB	34506	56156	1.49%	0.152%
93	19.186	2750	2754	2763	rBV3	33709	89958	2.38%	0.243%
94	19.251	2763	2765	2769	rVB5	10013	11999	0.32%	0.032%
95	19.392	2784	2789	2798	rVV	2927099	3779569	100.00%	10.205%
96	19.533	2810	2813	2817	rBV3	18274	19014	0.50%	0.051%
97	21.157	3085	3089	3097	rBV	1532021	2029228	53.69%	5.479%
98	21.286	3108	3111	3115	rBV	104242	133993	3.55%	0.362%
99	23.321	3450	3457	3465	rBV2	1965911	3667652	97.04%	9.903%
100	23.468	3476	3482	3499	rVB2	1050747	2063036	54.58%	5.570%




Sum of corrected areas: 37036709

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011323.D
Acq On : 09 Aug 2022 11:26
Operator : CG/JU
Sample : N3900-11
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0C88

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

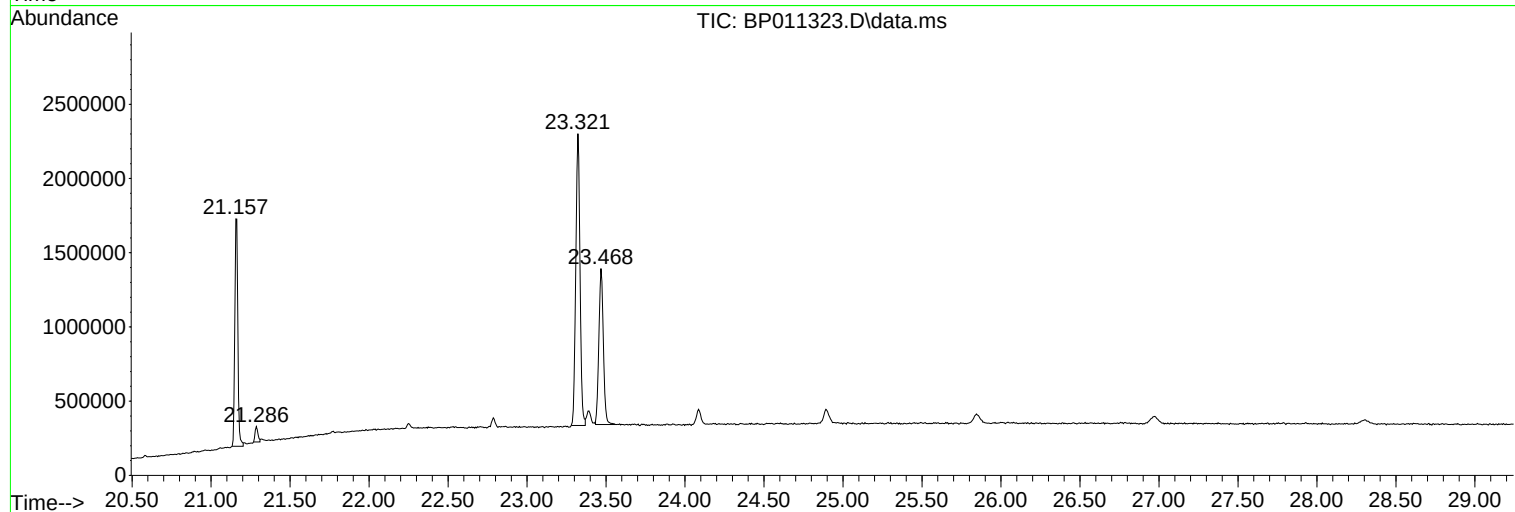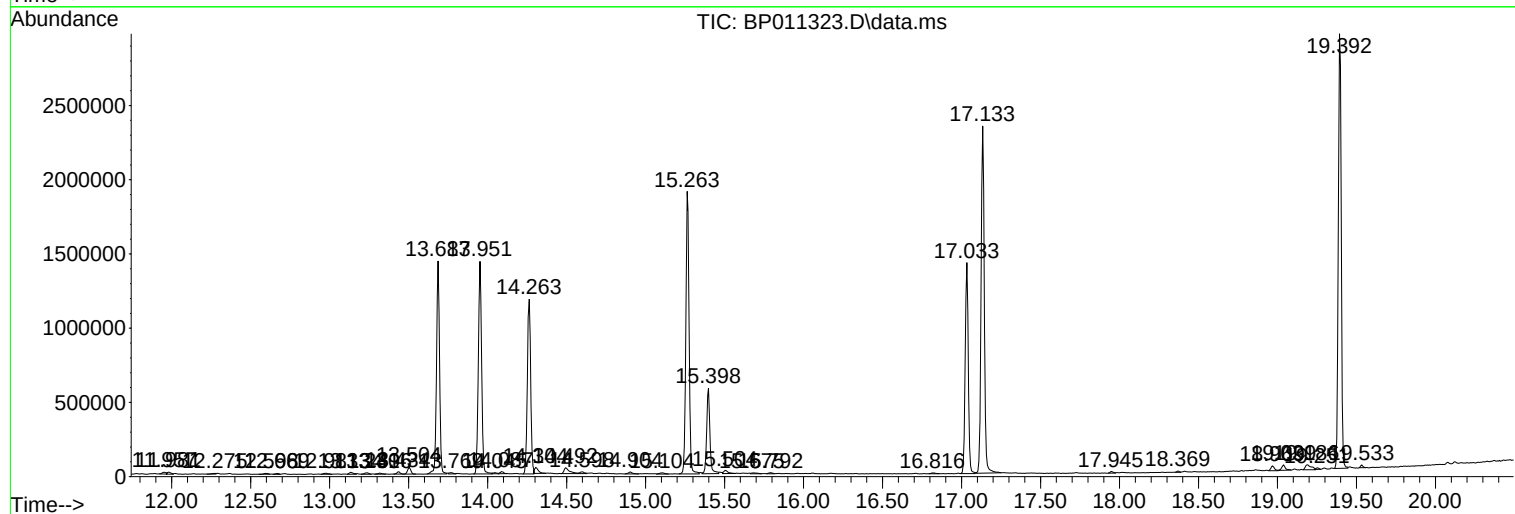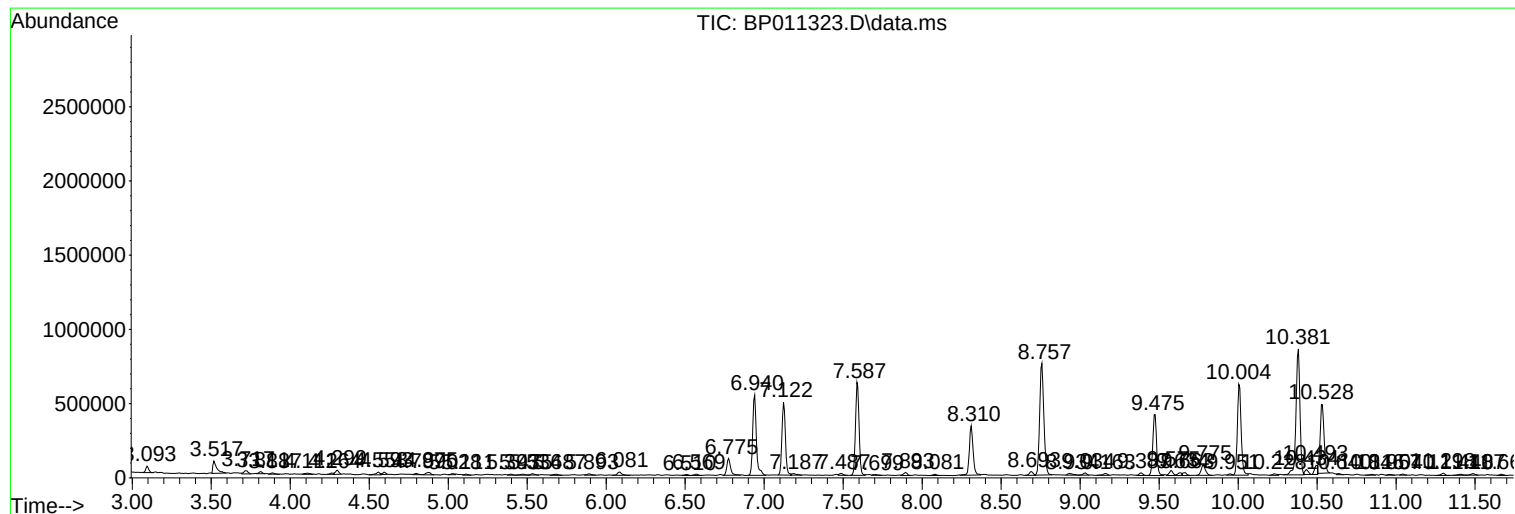

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011323.D
Acq On : 09 Aug 2022 11:26
Operator : CG/JU
Sample : N3900-11
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0C88

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011323.D
Acq On : 09 Aug 2022 11:26
Operator : CG/JU
Sample : N3900-11
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0C88

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc