

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
 Data File : BP011328.D
 Acq On : 09 Aug 2022 14:20
 Operator : CG/JU
 Sample : N4026-21
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJJ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011328.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.093	15	18	26	rVB	28574	42512	1.64%	0.159%
2	3.517	88	90	107	rBV	83083	148797	5.72%	0.558%
3	3.717	120	124	130	rVB2	16277	25923	1.00%	0.097%
4	3.811	136	140	145	rVB	15929	24116	0.93%	0.090%
5	4.187	199	204	206	rBV5	3182	4851	0.19%	0.018%
6	4.246	210	214	219	rVB	19721	27457	1.06%	0.103%
7	4.328	223	228	234	rVB2	25212	37903	1.46%	0.142%
8	4.840	311	315	321	rVB8	4088	6993	0.27%	0.026%
9	6.728	631	636	639	rBV	10568	16215	0.62%	0.061%
10	6.775	639	644	658	rVB	84915	142984	5.50%	0.536%
11	6.940	665	672	684	rBV	430603	671273	25.82%	2.517%
12	7.122	694	703	715	rBV	366165	582994	22.42%	2.186%
13	7.210	715	718	722	rVB6	4648	7704	0.30%	0.029%
14	7.587	775	782	791	rBV	517864	829159	31.89%	3.109%
15	8.310	898	905	920	rBV	258172	420495	16.17%	1.577%
16	8.752	973	980	997	rBV	502179	844668	32.49%	3.167%
17	8.893	997	1004	1006	rBV6	4494	8301	0.32%	0.031%
18	9.163	1045	1050	1057	rVB2	15752	26255	1.01%	0.098%
19	9.475	1095	1103	1115	rBV	327336	545003	20.96%	2.044%
20	10.010	1186	1194	1204	rBV	445356	755779	29.07%	2.834%
21	10.381	1249	1257	1266	rBV	694456	1138667	43.80%	4.270%
22	10.534	1274	1283	1299	rBV	409561	737276	28.36%	2.765%
23	11.663	1470	1475	1483	rBV	9658	16041	0.62%	0.060%
24	11.987	1525	1530	1539	rBV3	9318	18649	0.72%	0.070%
25	12.881	1676	1682	1685	rBV8	2845	4716	0.18%	0.018%
26	13.163	1727	1730	1737	rVB7	4158	5706	0.22%	0.021%
27	13.240	1737	1743	1745	rBV7	3736	5531	0.21%	0.021%
28	13.687	1812	1819	1833	rBV	1076676	1491106	57.35%	5.591%
29	13.951	1857	1864	1878	rBV	1136576	1653573	63.60%	6.201%
30	14.263	1910	1917	1926	rBV	967136	1388310	53.40%	5.206%
31	14.498	1952	1957	1971	rBV4	17357	56732	2.18%	0.213%
32	14.998	2036	2042	2044	rVB6	1533	2709	0.10%	0.010%
33	15.087	2052	2057	2061	rVB	10598	15614	0.60%	0.059%
34	15.122	2061	2063	2070	rVB8	2113	3085	0.12%	0.012%
35	15.269	2081	2088	2103	rBV	1429905	2080271	80.02%	7.801%
36	15.398	2104	2110	2122	rVV	341968	483881	18.61%	1.814%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
 Data File : BP011328.D
 Acq On : 09 Aug 2022 14:20
 Operator : CG/JU
 Sample : N4026-21
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJJ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

37	15.510	2125	2129	2136	rVB	15513	25056	0.96%	0.094%
38	15.963	2200	2206	2209	rBV7	1791	4167	0.16%	0.016%
39	15.998	2209	2212	2219	rVV8	3924	8818	0.34%	0.033%
40	16.051	2219	2221	2229	rVB6	4183	7757	0.30%	0.029%
41	16.169	2237	2241	2242	rBV4	3818	3178	0.12%	0.012%
42	16.522	2295	2301	2305	rBV5	6467	9870	0.38%	0.037%
43	16.710	2330	2333	2339	rVB8	2927	3933	0.15%	0.015%
44	16.816	2347	2351	2359	rVB6	3481	7414	0.29%	0.028%
45	16.981	2375	2379	2382	rBV6	3747	5668	0.22%	0.021%
46	17.033	2382	2388	2399	rBV	1121032	1582863	60.88%	5.935%
47	17.133	2399	2405	2421	rVV2	1598760	2323664	89.38%	8.713%
48	17.598	2481	2484	2491	rBV6	5486	8258	0.32%	0.031%
49	17.733	2504	2507	2514	rVB8	4805	8007	0.31%	0.030%
50	17.963	2542	2546	2547	rBV4	2051	2683	0.10%	0.010%
51	18.022	2553	2556	2561	rBV4	4502	5613	0.22%	0.021%
52	18.416	2620	2623	2631	rBV9	3014	5560	0.21%	0.021%
53	18.528	2640	2642	2645	rVB4	4049	3800	0.15%	0.014%
54	18.975	2714	2718	2722	rBV	18428	24389	0.94%	0.091%
55	19.039	2726	2729	2735	rVB2	17820	25364	0.98%	0.095%
56	19.398	2784	2790	2799	rBV	2055246	2599818	100.00%	9.749%
57	21.163	3085	3090	3098	rBV	1287512	1658335	63.79%	6.218%
58	21.292	3109	3112	3115	rBV	87472	103246	3.97%	0.387%
59	23.327	3452	3458	3465	rBV2	1273842	2401083	92.36%	9.004%
60	23.480	3477	3484	3491	rBV2	805278	1568035	60.31%	5.880%




Sum of corrected areas: 26667828

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011328.D
Acq On : 09 Aug 2022 14:20
Operator : CG/JU
Sample : N4026-21
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJJ6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

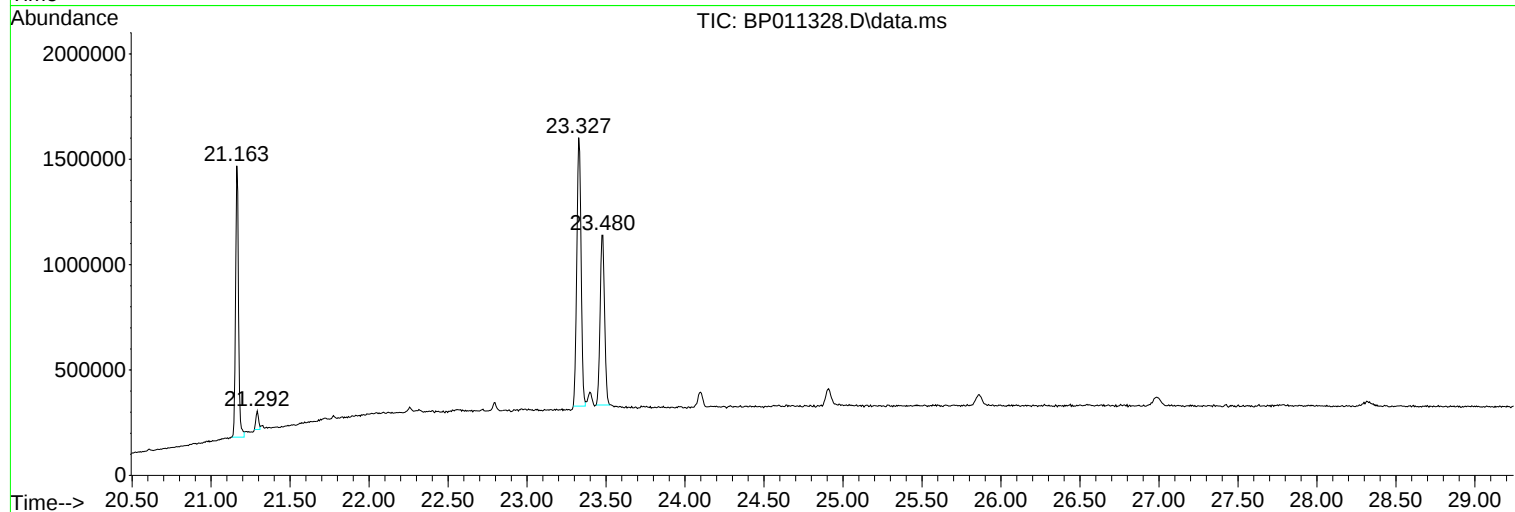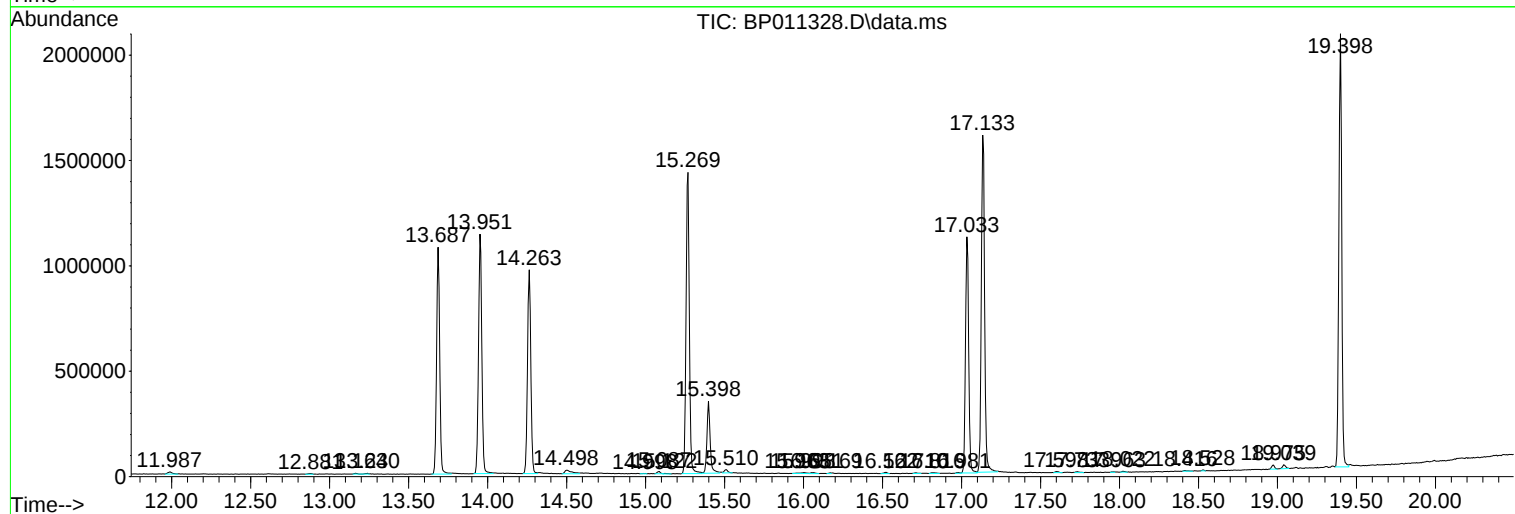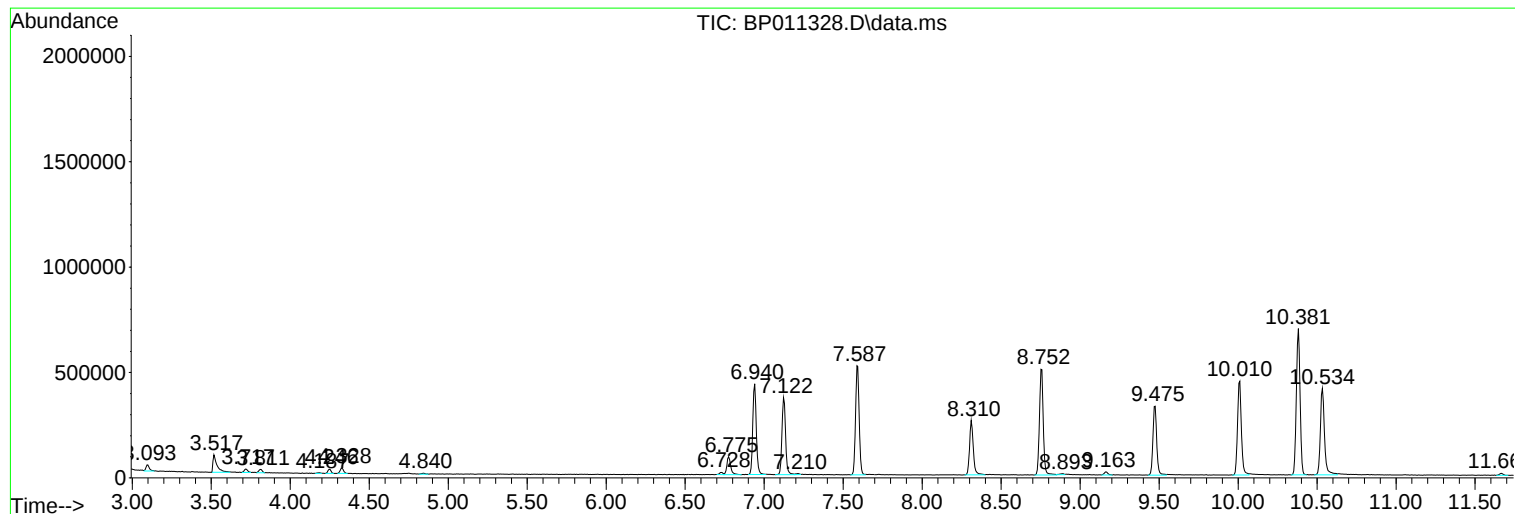

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011328.D
Acq On : 09 Aug 2022 14:20
Operator : CG/JU
Sample : N4026-21
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJJ6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011328.D
Acq On : 09 Aug 2022 14:20
Operator : CG/JU
Sample : N4026-21
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJJ6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc