

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
 Data File : BP011333.D
 Acq On : 09 Aug 2022 17:14
 Operator : CG/JU
 Sample : PB146591BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK591

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011333.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.093	14	18	25	rVB	42949	63168	2.53%	0.219%
2	3.511	85	89	109	rBV	285343	468216	18.72%	1.623%
3	3.816	136	141	150	rVB2	15731	27108	1.08%	0.094%
4	6.775	637	644	663	rBV	558522	901457	36.05%	3.125%
5	6.940	665	672	686	rVB	445630	696811	27.86%	2.415%
6	7.122	695	703	716	rBV	602761	912835	36.50%	3.164%
7	7.587	775	782	794	rBV	511714	790207	31.60%	2.739%
8	8.310	898	905	920	rBV	656309	1057045	42.27%	3.664%
9	8.752	973	980	990	rBV	526167	854769	34.18%	2.963%
10	9.469	1094	1102	1115	rBV	391245	649614	25.98%	2.252%
11	10.004	1183	1193	1205	rBV	575634	984364	39.36%	3.412%
12	10.381	1247	1257	1270	rBV	668603	1087670	43.49%	3.770%
13	10.534	1275	1283	1299	rBV	343972	640408	25.61%	2.220%
14	10.640	1299	1301	1307	rVB7	3087	4468	0.18%	0.015%
15	11.993	1523	1531	1540	rBV3	9453	20137	0.81%	0.070%
16	12.204	1564	1567	1570	rBV5	1836	2801	0.11%	0.010%
17	13.222	1736	1740	1746	rBV8	2995	5274	0.21%	0.018%
18	13.687	1812	1819	1832	rBV	1101728	1508258	60.31%	5.228%
19	13.951	1857	1864	1877	rBV	1172488	1660983	66.42%	5.758%
20	14.263	1910	1917	1926	rBV	913363	1310286	52.39%	4.542%
21	14.328	1926	1928	1934	rVB7	4253	6222	0.25%	0.022%
22	14.487	1949	1955	1978	rBV	334684	673775	26.94%	2.336%
23	15.263	2079	2087	2103	rBV	1417261	2074213	82.94%	7.190%
24	15.398	2104	2110	2121	rVV	435151	613075	24.51%	2.125%
25	15.504	2124	2128	2137	rVB3	16863	30231	1.21%	0.105%
26	16.057	2219	2222	2227	rVB6	4338	6045	0.24%	0.021%
27	16.375	2274	2276	2281	rVB6	1923	2650	0.11%	0.009%
28	16.516	2295	2300	2303	rBV7	1585	2591	0.10%	0.009%
29	16.692	2326	2330	2331	rBV4	2155	2554	0.10%	0.009%
30	16.710	2331	2333	2339	rVB7	3130	4196	0.17%	0.015%
31	16.822	2345	2352	2357	rBV6	3882	6823	0.27%	0.024%
32	16.980	2376	2379	2381	rBV4	2515	2569	0.10%	0.009%
33	17.033	2381	2388	2398	rVV	1053311	1484319	59.35%	5.145%
34	17.133	2398	2405	2421	rVV	1615809	2272112	90.85%	7.876%
35	17.728	2501	2506	2512	rVB9	4381	6749	0.27%	0.023%
36	18.510	2637	2639	2641	rBV3	2573	3236	0.13%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011333.D
Acq On : 09 Aug 2022 17:14
Operator : CG/JU
Sample : PB146591BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK591

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Title : SVOA CALIBRATION

37	18.969	2713	2717	2723	rBV3	19876	26515	1.06%	0.092%
38	19.039	2725	2729	2733	rVV	18269	24382	0.97%	0.085%
39	19.392	2783	2789	2799	rBV	1889386	2500890	100.00%	8.669%
40	21.163	3085	3090	3100	rBV	1178084	1512008	60.46%	5.241%
41	21.286	3108	3111	3116	rBV	77757	112503	4.50%	0.390%
42	23.321	3450	3457	3466	rBV2	1231508	2339825	93.56%	8.111%
43	23.468	3476	3482	3494	rVB2	782762	1494330	59.75%	5.180%




Sum of corrected areas: 28847692

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011333.D
Acq On : 09 Aug 2022 17:14
Operator : CG/JU
Sample : PB146591BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK591

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

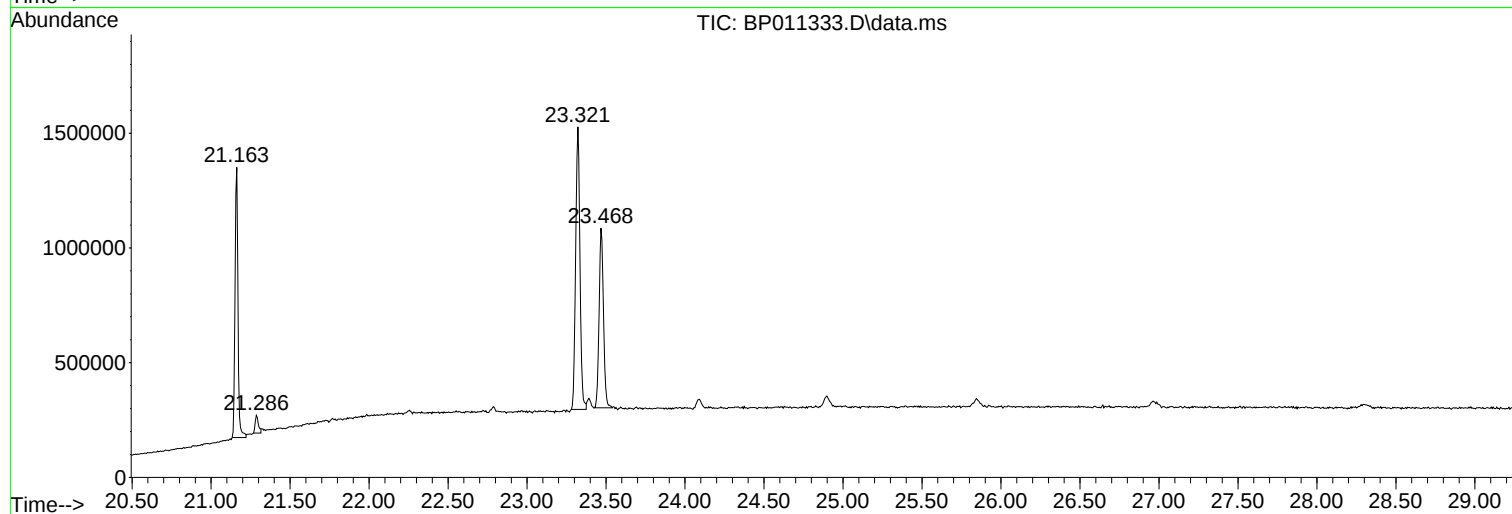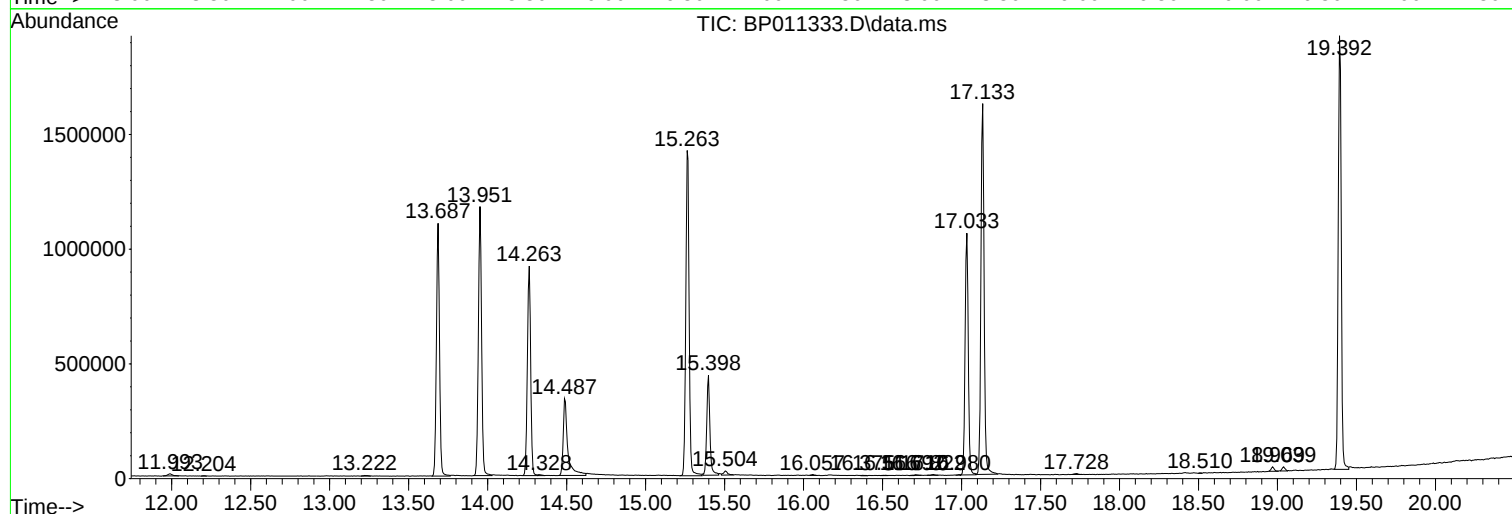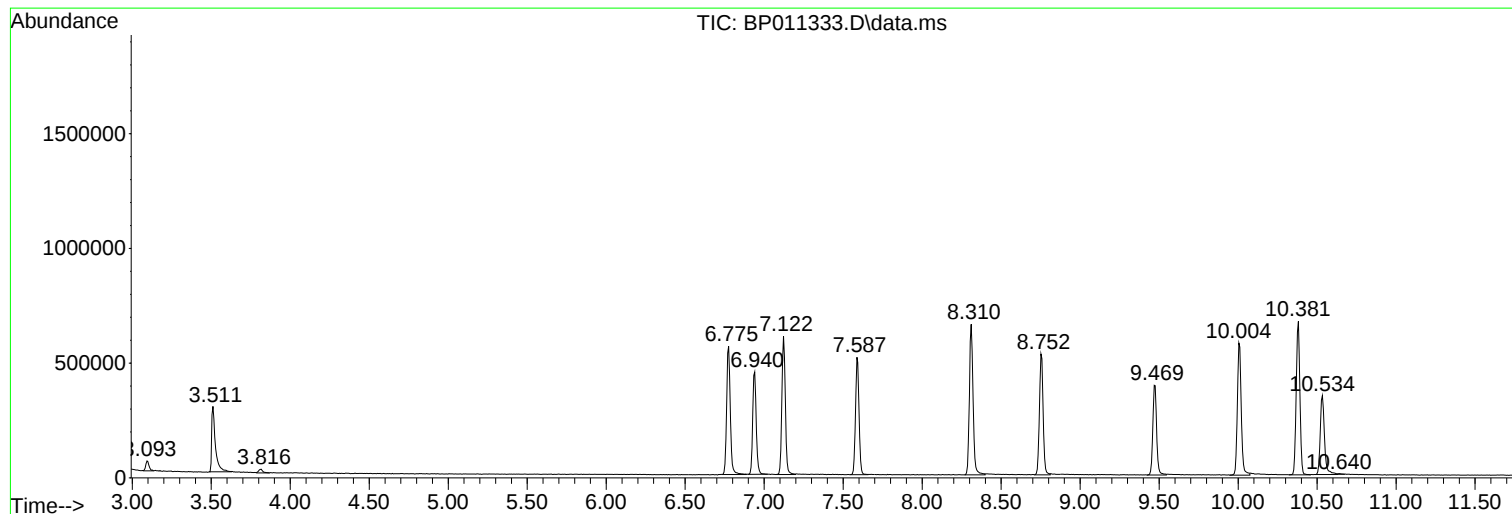

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011333.D
Acq On : 09 Aug 2022 17:14
Operator : CG/JU
Sample : PB146591BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK591

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011333.D
Acq On : 09 Aug 2022 17:14
Operator : CG/JU
Sample : PB146591BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK591

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc