

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
 Data File : BP011334.D
 Acq On : 09 Aug 2022 17:49
 Operator : CG/JU
 Sample : PB146820BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK820

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011334.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.093	14	18	28	rVB	42699	62492	1.93%	0.182%
2	3.505	84	88	115	rBV	521580	850279	26.23%	2.473%
3	3.811	136	140	145	rVB	9351	13532	0.42%	0.039%
4	4.446	244	248	250	rBV4	2536	3791	0.12%	0.011%
5	6.775	636	644	655	rBV	634574	987852	30.47%	2.873%
6	6.940	666	672	682	rVB	483143	741695	22.88%	2.157%
7	7.122	697	703	716	rBV	635927	971249	29.96%	2.825%
8	7.587	775	782	797	rBV	487321	767709	23.68%	2.233%
9	8.310	898	905	918	rBV	761788	1215092	37.48%	3.534%
10	8.752	973	980	995	rBV	591539	978274	30.17%	2.845%
11	9.469	1094	1102	1118	rBV	461970	766535	23.64%	2.230%
12	10.004	1186	1193	1208	rBV	678942	1155457	35.64%	3.361%
13	10.381	1248	1257	1267	rBV	645412	1053658	32.50%	3.065%
14	10.534	1274	1283	1302	rBV	699658	1248863	38.52%	3.632%
15	11.993	1519	1531	1539	rBV3	11145	24446	0.75%	0.071%
16	13.228	1736	1741	1745	rBV7	2810	5099	0.16%	0.015%
17	13.687	1812	1819	1832	rBV	1422794	1919172	59.20%	5.582%
18	13.951	1855	1864	1876	rBV	1468441	2084131	64.28%	6.062%
19	14.263	1907	1917	1924	rBV	882534	1280196	39.49%	3.724%
20	14.487	1949	1955	1976	rBV	505839	909520	28.05%	2.645%
21	15.263	2081	2087	2103	rBV	1733743	2553887	78.77%	7.428%
22	15.398	2103	2110	2124	rVV	608812	834773	25.75%	2.428%
23	15.504	2124	2128	2134	rVB2	20203	33015	1.02%	0.096%
24	15.969	2201	2207	2211	rVB8	2368	4030	0.12%	0.012%
25	16.057	2217	2222	2226	rBV6	6276	10130	0.31%	0.029%
26	16.175	2237	2242	2249	rBV10	2905	7124	0.22%	0.021%
27	16.816	2345	2351	2356	rBV9	3868	7962	0.25%	0.023%
28	17.034	2381	2388	2398	rVV	1043897	1444607	44.56%	4.202%
29	17.134	2398	2405	2425	rVV	2124091	2858184	88.16%	8.313%
30	18.404	2618	2621	2623	rBV4	3556	4363	0.13%	0.013%
31	18.969	2713	2717	2724	rBV3	23700	32819	1.01%	0.095%
32	19.039	2724	2729	2735	rBV	23528	37354	1.15%	0.109%
33	19.392	2783	2789	2802	rBV	2440379	3242075	100.00%	9.430%
34	21.163	3085	3090	3100	rBV	1135407	1490476	45.97%	4.335%
35	21.286	3108	3111	3115	rBV	74501	93765	2.89%	0.273%
36	23.321	3450	3457	3464	rBV2	1703749	3177118	98.00%	9.241%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011334.D
Acq On : 09 Aug 2022 17:49
Operator : CG/JU
Sample : PB146820BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK820

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Title : SVOA CALIBRATION

37	23.474	3476	3483	3497	rVB2	770995	1510140	46.58%	4.392%
----	--------	------	------	------	------	--------	---------	--------	--------




Sum of corrected areas: 34380864

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011334.D
Acq On : 09 Aug 2022 17:49
Operator : CG/JU
Sample : PB146820BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK820

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

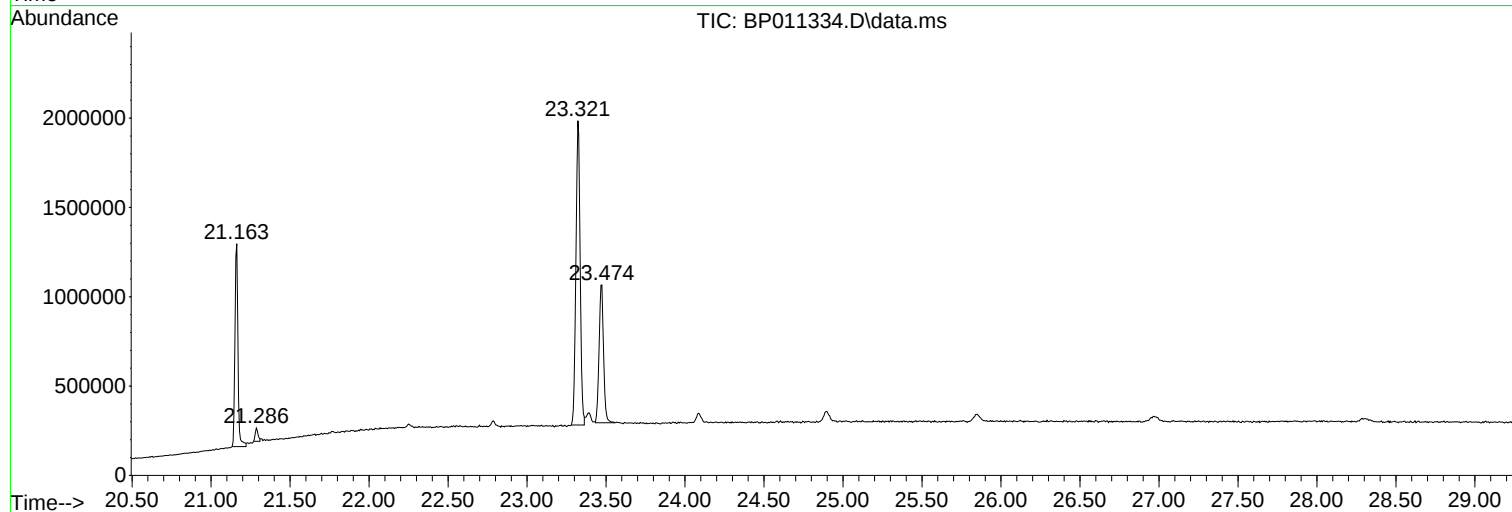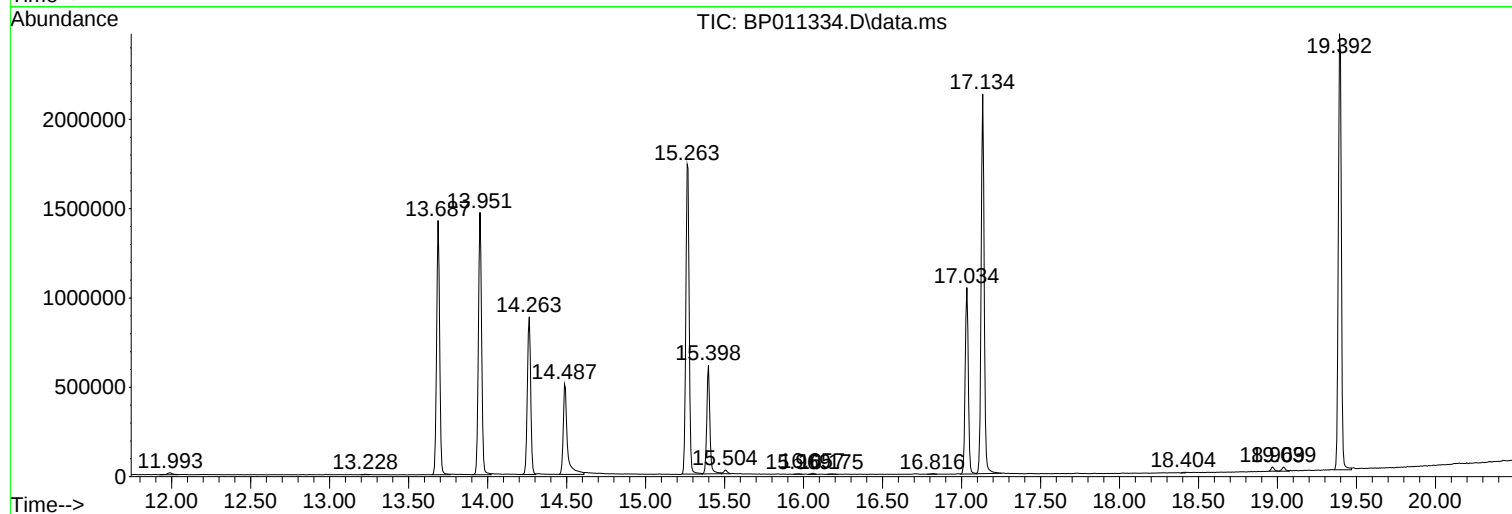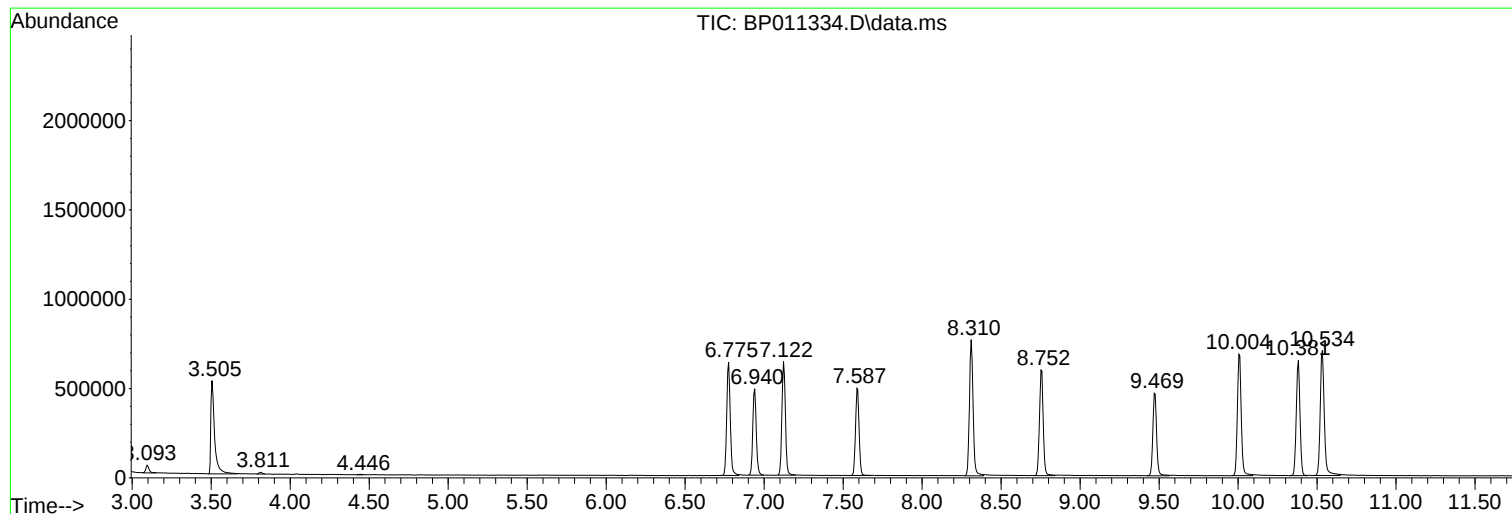

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011334.D
Acq On : 09 Aug 2022 17:49
Operator : CG/JU
Sample : PB146820BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK820

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011334.D
Acq On : 09 Aug 2022 17:49
Operator : CG/JU
Sample : PB146820BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK820

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc