

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
 Data File : BP011338.D
 Acq On : 09 Aug 2022 20:09
 Operator : CG/JU
 Sample : N3900-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0C80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011338.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.093	14	18	31	rVB	39023	62624	1.73%	0.177%
2	3.364	60	64	68	rVB2	7708	11981	0.33%	0.034%
3	3.511	86	89	104	rBV	163571	272987	7.56%	0.770%
4	3.723	120	125	132	rVB	20120	31286	0.87%	0.088%
5	3.811	136	140	144	rVB	12384	15337	0.42%	0.043%
6	4.111	188	191	197	rVB7	4163	6394	0.18%	0.018%
7	4.428	242	245	251	rVB5	4047	5899	0.16%	0.017%
8	4.599	270	274	278	rBV7	2923	4953	0.14%	0.014%
9	4.722	289	295	299	rVV7	4046	7992	0.22%	0.023%
10	4.775	300	304	311	rVV8	4933	10603	0.29%	0.030%
11	4.828	311	313	321	rVB9	2656	4404	0.12%	0.012%
12	5.058	348	352	358	rVB5	5058	8102	0.22%	0.023%
13	5.605	442	445	450	rVB7	2678	4417	0.12%	0.012%
14	5.693	450	460	464	rBV9	4424	10899	0.30%	0.031%
15	5.852	481	487	491	rBV2	9234	14893	0.41%	0.042%
16	5.893	491	494	500	rVB8	4314	6643	0.18%	0.019%
17	6.081	520	526	531	rBV	8658	14586	0.40%	0.041%
18	6.422	581	584	588	rVB6	2477	4187	0.12%	0.012%
19	6.775	638	644	652	rBV	139632	230241	6.38%	0.649%
20	6.864	655	659	663	rVB2	12795	18801	0.52%	0.053%
21	6.940	665	672	684	rBV	580699	938863	26.00%	2.648%
22	7.122	696	703	712	rBV	590232	898309	24.88%	2.533%
23	7.187	712	714	718	rVB4	4029	4058	0.11%	0.011%
24	7.264	724	727	732	rVB8	2724	4111	0.11%	0.012%
25	7.452	754	759	761	rBV4	3921	5290	0.15%	0.015%
26	7.487	761	765	770	rVB	10889	17020	0.47%	0.048%
27	7.587	770	782	791	rBV	563152	883366	24.47%	2.491%
28	7.699	797	801	804	rVB5	4379	5915	0.16%	0.017%
29	7.893	829	834	840	rVB2	11409	18140	0.50%	0.051%
30	7.958	840	845	850	rBV7	4654	7887	0.22%	0.022%
31	8.081	860	866	871	rVB9	5406	8928	0.25%	0.025%
32	8.311	897	905	915	rBV	415774	668872	18.53%	1.886%
33	8.687	965	969	973	rVB7	3910	5995	0.17%	0.017%
34	8.752	973	980	991	rBV	728826	1161138	32.16%	3.275%
35	8.858	997	998	1004	rVB5	3740	5341	0.15%	0.015%
36	8.928	1004	1010	1020	rVB5	5335	16051	0.44%	0.045%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
 Data File : BP011338.D
 Acq On : 09 Aug 2022 20:09
 Operator : CG/JU
 Sample : N3900-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0C80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

37	9.028	1020	1027	1031	rVB7	4406	8504	0.24%	0.024%
38	9.163	1046	1050	1054	rVB7	3183	4228	0.12%	0.012%
39	9.210	1054	1058	1061	rVB4	2942	4140	0.11%	0.012%
40	9.399	1082	1090	1095	rVV7	10242	24896	0.69%	0.070%

41	9.469	1095	1102	1117	rVV	526172	848443	23.50%	2.393%
42	9.575	1117	1120	1125	rVB6	4136	7156	0.20%	0.020%
43	9.781	1148	1155	1161	rVB2	21923	38924	1.08%	0.110%
44	10.005	1186	1193	1201	rBV	739718	1180479	32.70%	3.329%
45	10.381	1247	1257	1263	rBV	735220	1214661	33.64%	3.425%

46	10.528	1274	1282	1297	rBV	635225	1188538	32.92%	3.352%
47	10.746	1317	1319	1324	rVB6	3403	5103	0.14%	0.014%
48	11.204	1389	1397	1398	rBV7	3620	7069	0.20%	0.020%
49	11.640	1462	1471	1480	rBV4	12412	30427	0.84%	0.086%
50	11.728	1480	1486	1487	rBV6	2857	4785	0.13%	0.013%

51	11.840	1502	1505	1511	rVB5	4387	7817	0.22%	0.022%
52	11.952	1518	1524	1526	rBV3	11322	18713	0.52%	0.053%
53	11.981	1526	1529	1538	rVB2	16155	27155	0.75%	0.077%
54	12.104	1544	1550	1556	rVB	8795	13203	0.37%	0.037%
55	12.187	1559	1564	1569	rVV7	4232	8464	0.23%	0.024%

56	12.251	1573	1575	1583	rVB9	2730	5692	0.16%	0.016%
57	12.416	1602	1603	1610	rVB6	2804	3893	0.11%	0.011%
58	12.863	1675	1679	1684	rVB8	2892	4586	0.13%	0.013%
59	12.969	1695	1697	1706	rVB9	3502	5556	0.15%	0.016%
60	13.093	1714	1718	1721	rBV6	3215	4508	0.12%	0.013%

61	13.163	1726	1730	1735	rBV4	9432	12966	0.36%	0.037%
62	13.222	1735	1740	1744	rBV5	4993	10690	0.30%	0.030%
63	13.269	1744	1748	1755	rVB3	25086	38934	1.08%	0.110%
64	13.687	1811	1819	1833	rBV	1491753	1996184	55.29%	5.629%
65	13.951	1856	1864	1881	rBV	1608238	2265182	62.74%	6.388%

66	14.263	1908	1917	1925	rBV	1001709	1471114	40.75%	4.149%
67	14.322	1925	1927	1936	rVB9	8029	12942	0.36%	0.036%
68	14.493	1950	1956	1972	rBV2	52233	131719	3.65%	0.371%
69	14.928	2026	2030	2033	rVV6	2924	4847	0.13%	0.014%
70	14.975	2035	2038	2044	rVB8	2851	4397	0.12%	0.012%

71	15.075	2050	2055	2058	rBV7	2994	5186	0.14%	0.015%
72	15.104	2058	2060	2068	rVB8	2815	4755	0.13%	0.013%
73	15.263	2080	2087	2094	rBV	1979014	2763328	76.54%	7.793%
74	15.398	2104	2110	2122	rBV	633529	879719	24.37%	2.481%
75	15.504	2124	2128	2137	rVB2	21153	38545	1.07%	0.109%

76	15.810	2174	2180	2187	rBV2	4252	12929	0.36%	0.036%
----	--------	------	------	------	------	------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
 Data File : BP011338.D
 Acq On : 09 Aug 2022 20:09
 Operator : CG/JU
 Sample : N3900-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0C80

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

77	15.963	2201	2206	2212	rBV10	2838	6453	0.18%	0.018%
78	16.051	2214	2221	2232	rVB10	6128	17856	0.49%	0.050%
79	16.181	2236	2243	2247	rBV10	3393	7972	0.22%	0.022%
80	16.245	2249	2254	2257	rBV7	3371	4795	0.13%	0.014%
81	16.404	2274	2281	2284	rBV9	2053	4038	0.11%	0.011%
82	16.604	2311	2315	2319	rVB7	3306	4700	0.13%	0.013%
83	16.704	2330	2332	2338	rVB6	4258	4623	0.13%	0.013%
84	16.810	2345	2350	2356	rBV8	7882	12805	0.35%	0.036%
85	16.975	2375	2378	2381	rBV4	3709	5153	0.14%	0.015%
86	17.034	2381	2388	2398	rBV	1208675	1683040	46.62%	4.746%
87	17.134	2398	2405	2423	rVV	2176154	3173276	87.89%	8.949%
88	17.722	2500	2505	2509	rBV7	4717	9046	0.25%	0.026%
89	17.951	2538	2544	2548	rBV9	8047	13434	0.37%	0.038%
90	18.016	2553	2555	2559	rVV3	2732	3945	0.11%	0.011%
91	18.239	2590	2593	2597	rBV6	3279	5446	0.15%	0.015%
92	18.410	2618	2622	2629	rBV10	5385	12801	0.35%	0.036%
93	18.469	2629	2632	2636	rVV6	2706	4784	0.13%	0.013%
94	18.969	2713	2717	2724	rBV2	26878	38854	1.08%	0.110%
95	19.033	2724	2728	2734	rBV	24421	37365	1.03%	0.105%
96	19.392	2783	2789	2803	rBV	2782967	3610507	100.00%	10.182%
97	21.157	3085	3089	3102	rBV	1333847	1766595	48.93%	4.982%
98	21.286	3108	3111	3115	rBV	73743	96617	2.68%	0.272%
99	23.321	3450	3457	3465	rBV2	1821297	3428319	94.95%	9.668%
100	23.469	3476	3482	3494	rVB2	919139	1790325	49.59%	5.049%




Sum of corrected areas: 35459639

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011338.D
Acq On : 09 Aug 2022 20:09
Operator : CG/JU
Sample : N3900-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0C80

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

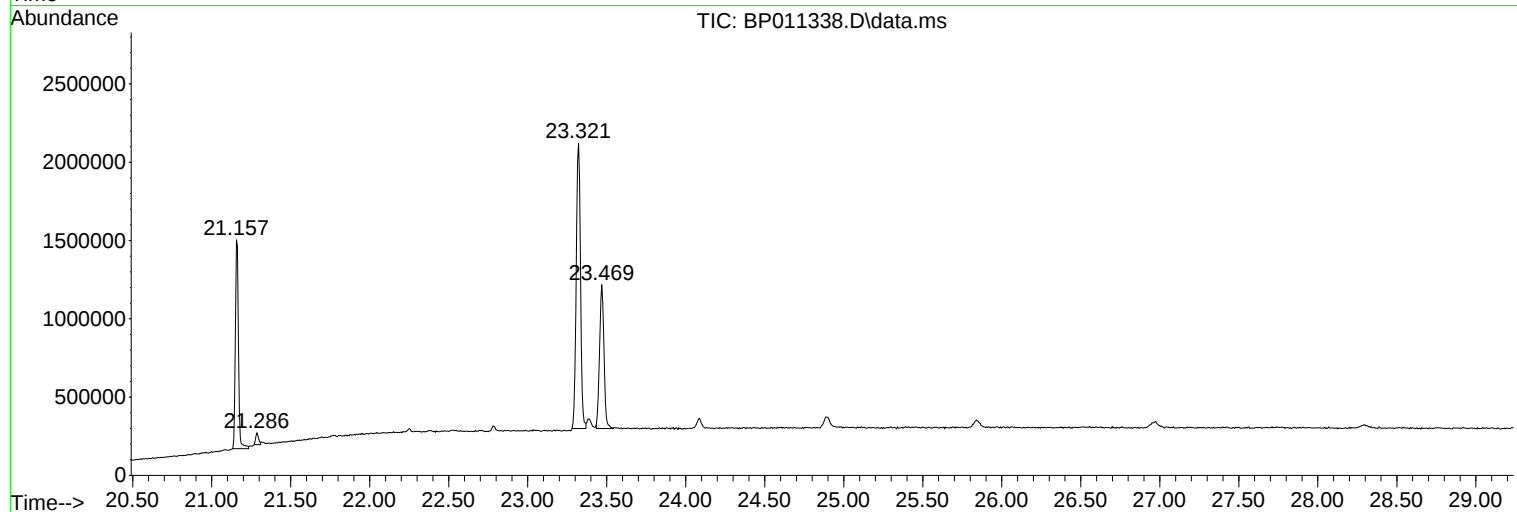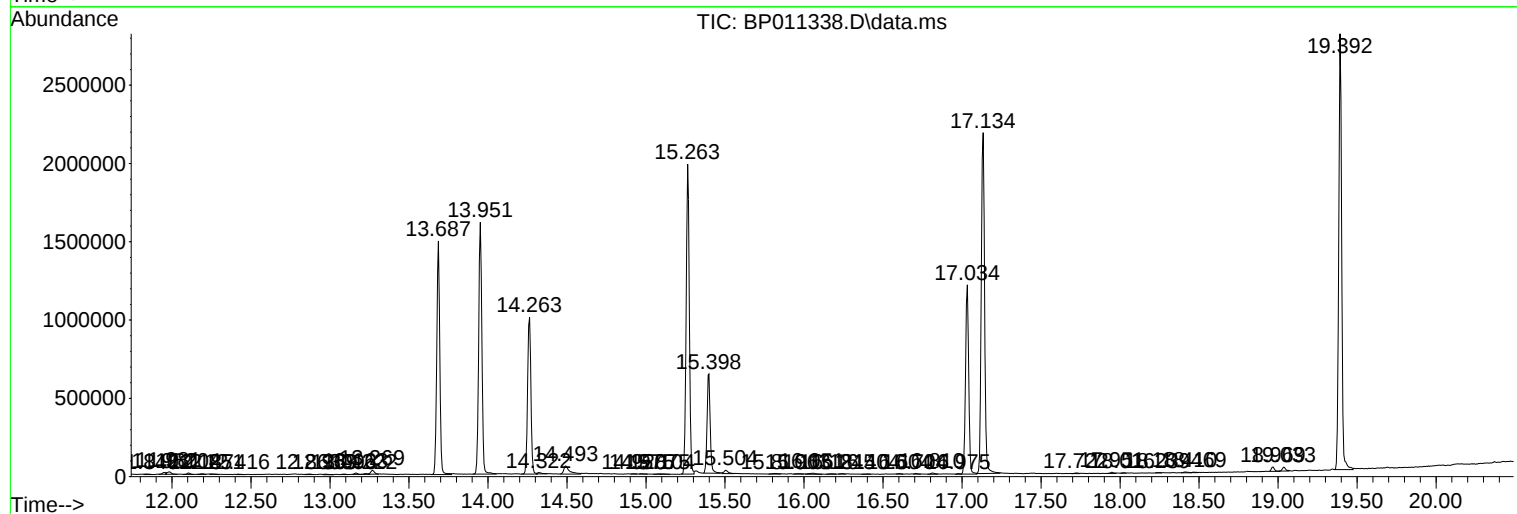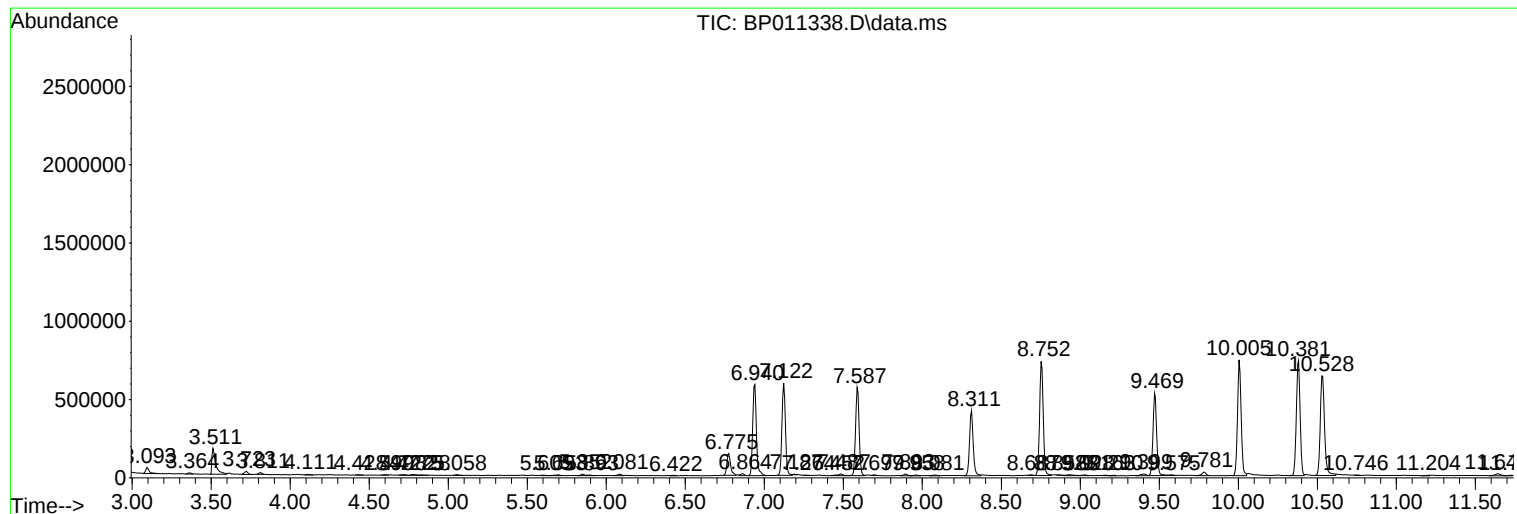

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011338.D
Acq On : 09 Aug 2022 20:09
Operator : CG/JU
Sample : N3900-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0C80

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011338.D
Acq On : 09 Aug 2022 20:09
Operator : CG/JU
Sample : N3900-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0C80

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc