

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
 Data File : BP011339.D
 Acq On : 09 Aug 2022 20:44
 Operator : CG/JU
 Sample : N3900-05
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0C96

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011339.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.099	15	19	26	rVB	39876	60430	1.69%	0.168%
2	3.517	87	90	105	rBV	118464	195482	5.47%	0.544%
3	3.723	120	125	131	rVB	20796	34296	0.96%	0.095%
4	3.811	137	140	145	rVB	11122	15080	0.42%	0.042%
5	4.723	292	295	300	rBV4	3367	4842	0.14%	0.013%
6	6.775	638	644	656	rVB	153141	248899	6.96%	0.693%
7	6.940	665	672	684	rBV	586415	917662	25.66%	2.554%
8	7.034	684	688	695	rVB4	3318	6096	0.17%	0.017%
9	7.122	697	703	714	rBV	599783	927152	25.93%	2.580%
10	7.211	716	718	721	rVB3	4270	4586	0.13%	0.013%
11	7.587	775	782	792	rBV	593273	932450	26.08%	2.595%
12	7.664	792	795	801	rVB5	4994	8790	0.25%	0.024%
13	8.311	896	905	920	rBV	433668	708558	19.82%	1.972%
14	8.752	972	980	993	rBV	742651	1171762	32.77%	3.261%
15	9.163	1043	1050	1053	rBV	6066	9102	0.25%	0.025%
16	9.469	1095	1102	1120	rBV	555652	883117	24.70%	2.457%
17	10.005	1186	1193	1212	rBV	753989	1237472	34.61%	3.444%
18	10.381	1249	1257	1269	rBV	781511	1304844	36.49%	3.631%
19	10.528	1275	1282	1297	rBV	595561	1071081	29.95%	2.981%
20	10.822	1329	1332	1337	rBV6	2416	3993	0.11%	0.011%
21	11.622	1463	1468	1472	rBV5	8663	15040	0.42%	0.042%
22	11.663	1472	1475	1478	rVB4	3674	4812	0.13%	0.013%
23	11.722	1481	1485	1488	rBV6	2713	4792	0.13%	0.013%
24	11.987	1521	1530	1536	rBV2	13676	27096	0.76%	0.075%
25	13.087	1712	1717	1723	rVB3	8338	12579	0.35%	0.035%
26	13.163	1725	1730	1736	rVV5	5175	10846	0.30%	0.030%
27	13.234	1737	1742	1750	rVB8	4273	7851	0.22%	0.022%
28	13.687	1812	1819	1830	rBV	1466443	2014794	56.35%	5.607%
29	13.775	1830	1834	1837	rVB5	4594	7601	0.21%	0.021%
30	13.951	1857	1864	1883	rBV	1577227	2276037	63.65%	6.334%
31	14.175	1899	1902	1906	rVB4	4245	5233	0.15%	0.015%
32	14.257	1909	1916	1926	rBV	1104125	1619359	45.29%	4.506%
33	14.493	1948	1956	1973	rBV2	60110	144060	4.03%	0.401%
34	15.028	2043	2047	2052	rVB2	6339	9278	0.26%	0.026%
35	15.134	2062	2065	2069	rVB6	3018	4516	0.13%	0.013%
36	15.263	2080	2087	2103	rBV	1963943	2775773	77.63%	7.724%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
 Data File : BP011339.D
 Acq On : 09 Aug 2022 20:44
 Operator : CG/JU
 Sample : N3900-05
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0C96

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

37	15.393	2103	2109	2123	rVV	646727	894481	25.02%	2.489%
38	15.504	2124	2128	2133	rVB3	18381	28929	0.81%	0.081%
39	16.057	2218	2222	2227	rVB7	5997	7562	0.21%	0.021%
40	16.645	2318	2322	2326	rVB7	4340	6290	0.18%	0.018%
41	16.710	2330	2333	2337	rVB6	3276	4415	0.12%	0.012%
42	16.810	2346	2350	2355	rBV6	7186	11223	0.31%	0.031%
43	16.975	2374	2378	2381	rBV6	3211	5394	0.15%	0.015%
44	17.034	2381	2388	2398	rVV	1281518	1846096	51.63%	5.137%
45	17.134	2398	2405	2420	rVV	2232681	3180279	88.94%	8.850%
46	17.434	2450	2456	2457	rBV6	3017	5024	0.14%	0.014%
47	17.551	2473	2476	2480	rVB6	4574	4384	0.12%	0.012%
48	17.728	2501	2506	2510	rBV8	5016	8929	0.25%	0.025%
49	17.945	2539	2543	2547	rBV3	22034	29913	0.84%	0.083%
50	18.016	2553	2555	2558	rVB	4399	4634	0.13%	0.013%
51	18.234	2589	2592	2595	rBV5	4065	5286	0.15%	0.015%
52	18.410	2620	2622	2624	rBV3	3618	3734	0.10%	0.010%
53	18.963	2713	2716	2722	rVB2	26032	34365	0.96%	0.096%
54	19.034	2724	2728	2733	rBV	26581	36535	1.02%	0.102%
55	19.392	2783	2789	2797	rBV	2783199	3575655	100.00%	9.950%
56	20.892	3041	3044	3051	rBV	62822	94071	2.63%	0.262%
57	21.157	3084	3089	3100	rBV	1563538	1967728	55.03%	5.476%
58	21.286	3108	3111	3115	rBV	74226	93201	2.61%	0.259%
59	23.316	3450	3456	3464	rBV2	1873606	3451010	96.51%	9.603%
60	23.463	3475	3481	3493	rVB2	949957	1951280	54.57%	5.430%




Sum of corrected areas: 35935779

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011339.D
Acq On : 09 Aug 2022 20:44
Operator : CG/JU
Sample : N3900-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0C96

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

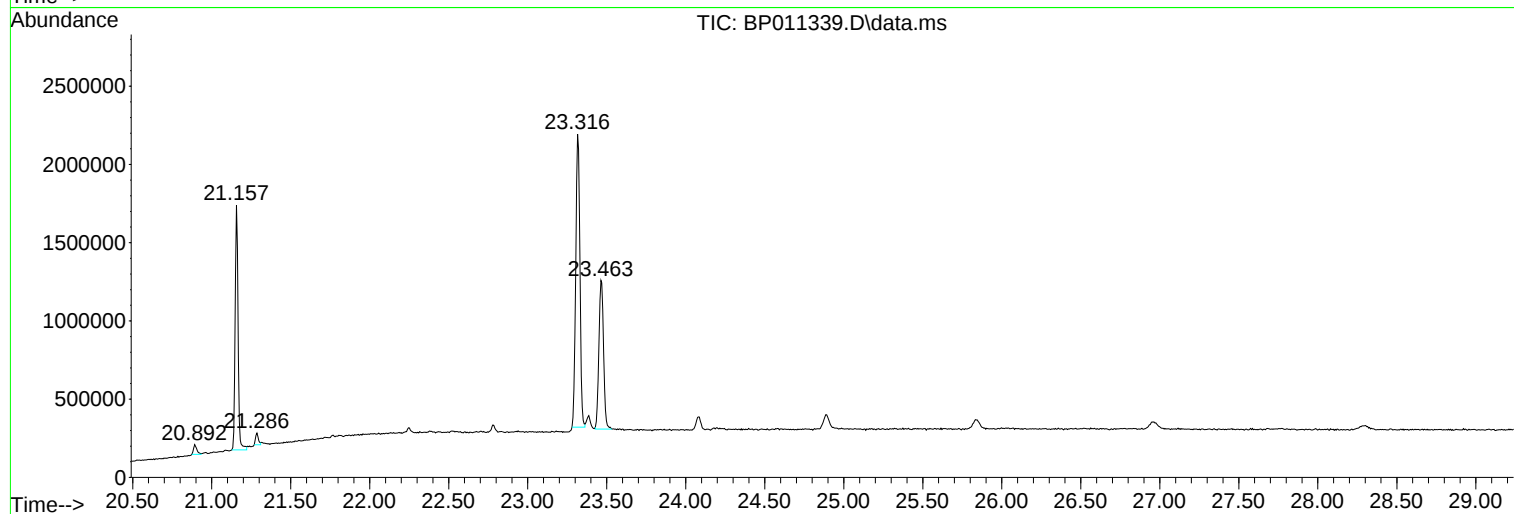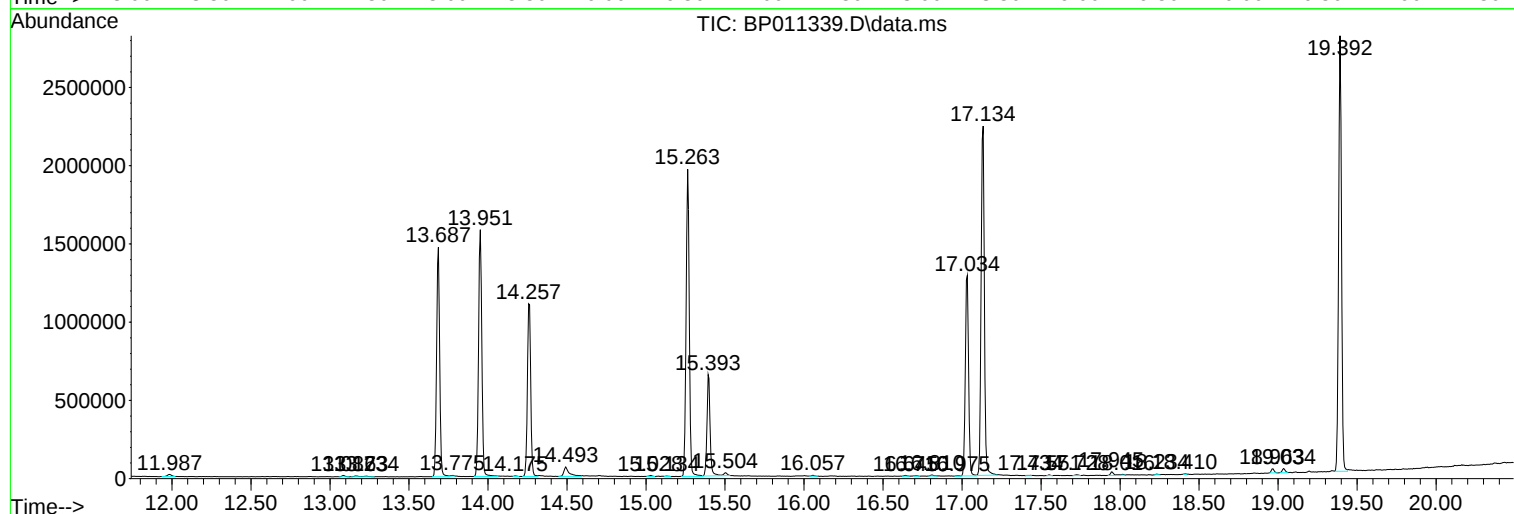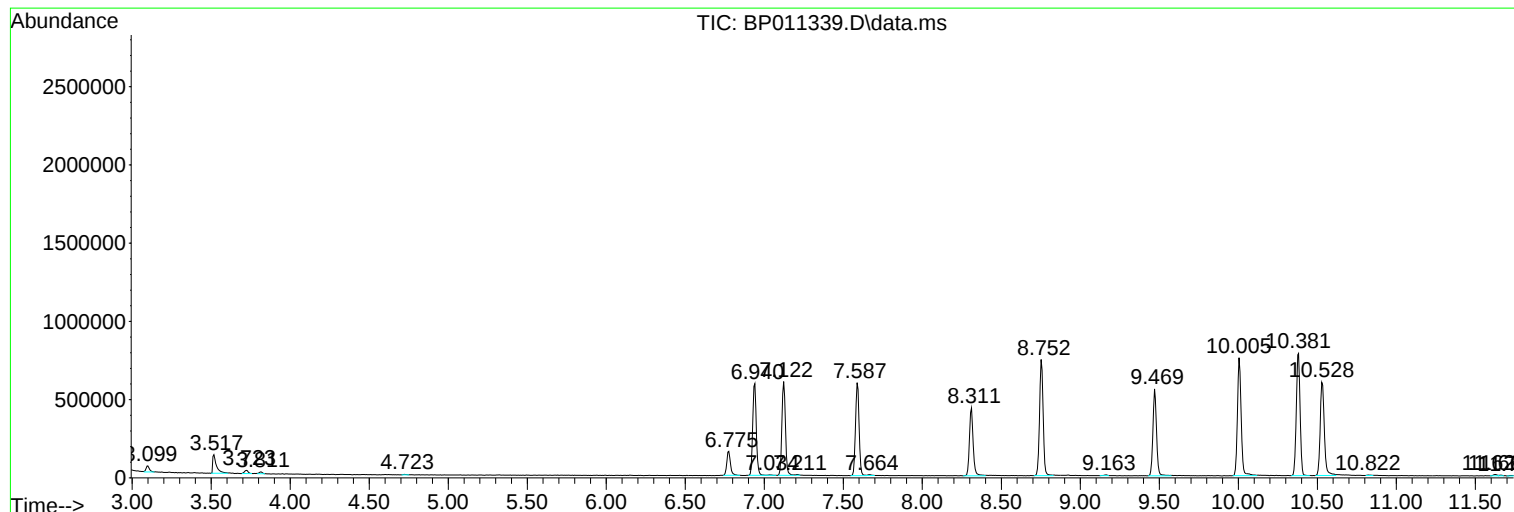

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011339.D
Acq On : 09 Aug 2022 20:44
Operator : CG/JU
Sample : N3900-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0C96

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011339.D
Acq On : 09 Aug 2022 20:44
Operator : CG/JU
Sample : N3900-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0C96

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc