

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
 Data File : BP011340.D
 Acq On : 09 Aug 2022 21:19
 Operator : CG/JU
 Sample : N3900-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0C84

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011340.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.093	15	18	27	rVB	32977	47540	1.33%	0.138%
2	3.511	86	89	110	rBV	130962	235748	6.61%	0.684%
3	3.722	119	125	131	rVB	18013	28437	0.80%	0.082%
4	3.811	137	140	145	rVB	10599	14422	0.40%	0.042%
5	6.775	637	644	655	rBV	123918	207060	5.81%	0.600%
6	6.940	665	672	682	rBV	505307	810884	22.75%	2.351%
7	7.034	684	688	693	rVB2	4779	8049	0.23%	0.023%
8	7.122	696	703	713	rBV	527725	806466	22.62%	2.338%
9	7.587	775	782	791	rBV	594226	907042	25.44%	2.630%
10	7.669	791	796	803	rVB4	6457	11582	0.32%	0.034%
11	8.310	896	905	919	rBV	374085	611326	17.15%	1.772%
12	8.752	972	980	994	rBV	658819	1046066	29.34%	3.033%
13	9.163	1041	1050	1057	rBV4	5372	11182	0.31%	0.032%
14	9.469	1095	1102	1112	rBV	473072	758700	21.28%	2.200%
15	10.004	1184	1193	1208	rBV	655757	1083662	30.40%	3.142%
16	10.381	1248	1257	1264	rBV	757717	1265907	35.51%	3.670%
17	10.528	1274	1282	1304	rBV	571007	1040003	29.17%	3.015%
18	11.810	1493	1500	1508	rVB3	11688	22727	0.64%	0.066%
19	11.987	1525	1530	1539	rVB2	12070	21363	0.60%	0.062%
20	13.087	1713	1717	1724	rVB3	7923	11382	0.32%	0.033%
21	13.228	1735	1741	1745	rBV8	3028	4840	0.14%	0.014%
22	13.598	1800	1804	1807	rBV5	2820	3637	0.10%	0.011%
23	13.687	1812	1819	1833	rBV	1404388	1951685	54.75%	5.659%
24	13.793	1836	1837	1843	rVB6	3047	3881	0.11%	0.011%
25	13.951	1856	1864	1879	rBV	1454739	2077085	58.26%	6.022%
26	14.175	1899	1902	1906	rVB5	5100	6026	0.17%	0.017%
27	14.257	1909	1916	1925	rBV	1044934	1546434	43.38%	4.484%
28	14.492	1950	1956	1967	rBV2	47817	113558	3.19%	0.329%
29	14.704	1988	1992	2002	rVB2	7271	15637	0.44%	0.045%
30	15.028	2043	2047	2051	rBV	18753	25392	0.71%	0.074%
31	15.263	2079	2087	2103	rBV	1916743	2704004	75.85%	7.840%
32	15.392	2103	2109	2123	rVV	638267	887851	24.91%	2.574%
33	15.504	2123	2128	2137	rVB2	21000	35796	1.00%	0.104%
34	16.057	2217	2222	2228	rVB9	6193	9623	0.27%	0.028%
35	16.169	2238	2241	2244	rBV5	3075	4400	0.12%	0.013%
36	16.704	2329	2332	2337	rVB7	3670	4538	0.13%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
 Data File : BP011340.D
 Acq On : 09 Aug 2022 21:19
 Operator : CG/JU
 Sample : N3900-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0C84

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

37	16.810	2346	2350	2357	rBV6	5235	9126	0.26%	0.026%
38	17.034	2381	2388	2398	rBV	1208647	1747531	49.02%	5.067%
39	17.134	2398	2405	2426	rVB	2219769	3219585	90.31%	9.335%
40	17.598	2480	2484	2489	rVB7	4564	7471	0.21%	0.022%
41	17.728	2501	2506	2512	rVB8	5769	9267	0.26%	0.027%
42	17.951	2540	2544	2550	rBV2	26903	36469	1.02%	0.106%
43	18.016	2553	2555	2559	rVB2	4393	5223	0.15%	0.015%
44	18.404	2619	2621	2626	rBV6	3640	5816	0.16%	0.017%
45	18.963	2712	2716	2721	rBV5	25818	37839	1.06%	0.110%
46	19.033	2724	2728	2734	rVV	25440	38099	1.07%	0.110%
47	19.198	2754	2756	2758	rBV2	5842	4663	0.13%	0.014%
48	19.392	2783	2789	2798	rBV	2789303	3564911	100.00%	10.336%
49	19.722	2841	2845	2850	rVB6	32692	40482	1.14%	0.117%
50	20.892	3040	3044	3052	rBV3	87148	163857	4.60%	0.475%
51	21.157	3084	3089	3099	rBV	1471737	1831205	51.37%	5.309%
52	21.286	3107	3111	3115	rBV	82650	117560	3.30%	0.341%
53	23.316	3449	3456	3464	rBV2	1833890	3502537	98.25%	10.155%
54	23.463	3475	3481	3493	rVB2	927910	1805447	50.64%	5.235%




Sum of corrected areas: 34491023

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011340.D
Acq On : 09 Aug 2022 21:19
Operator : CG/JU
Sample : N3900-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0C84

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

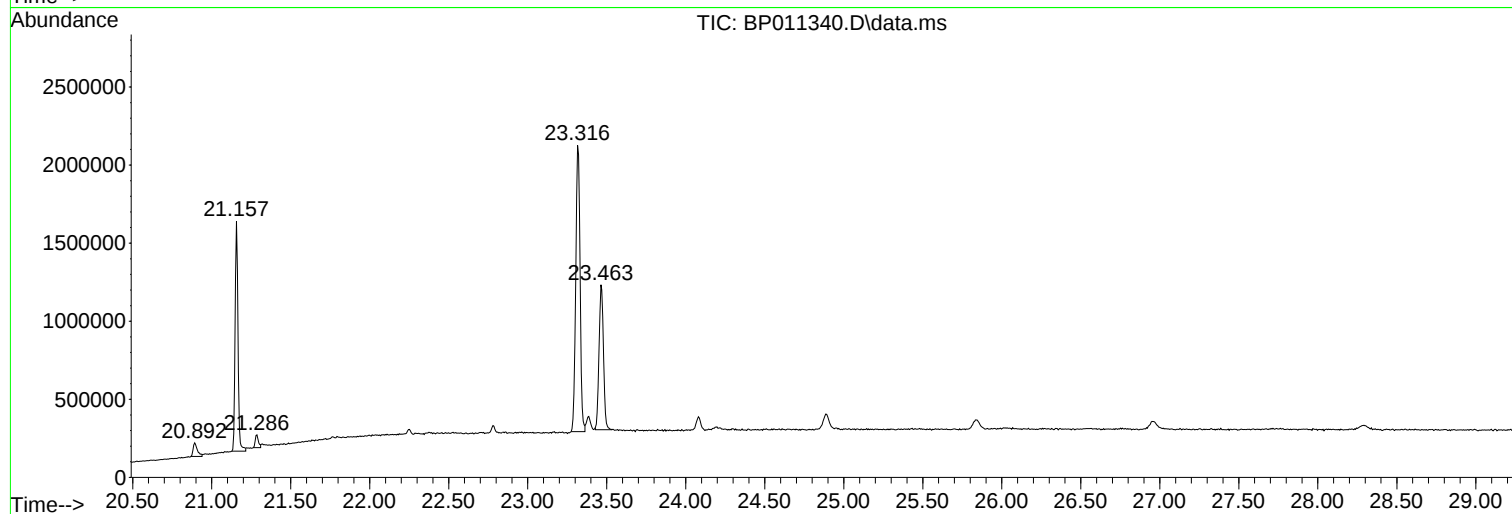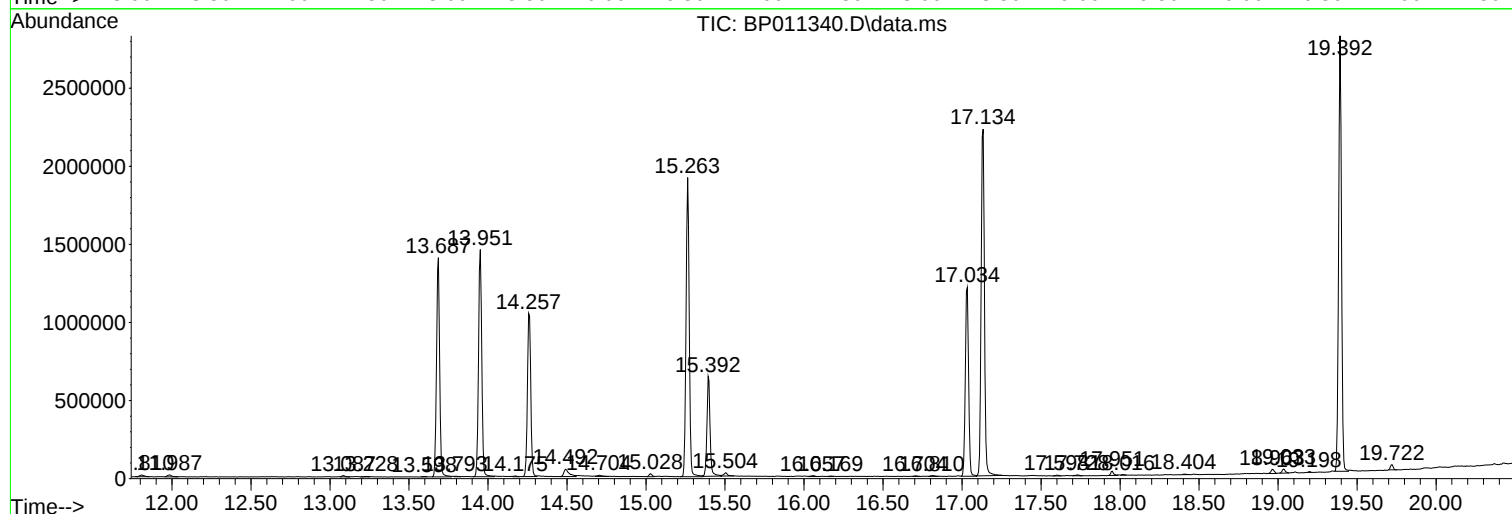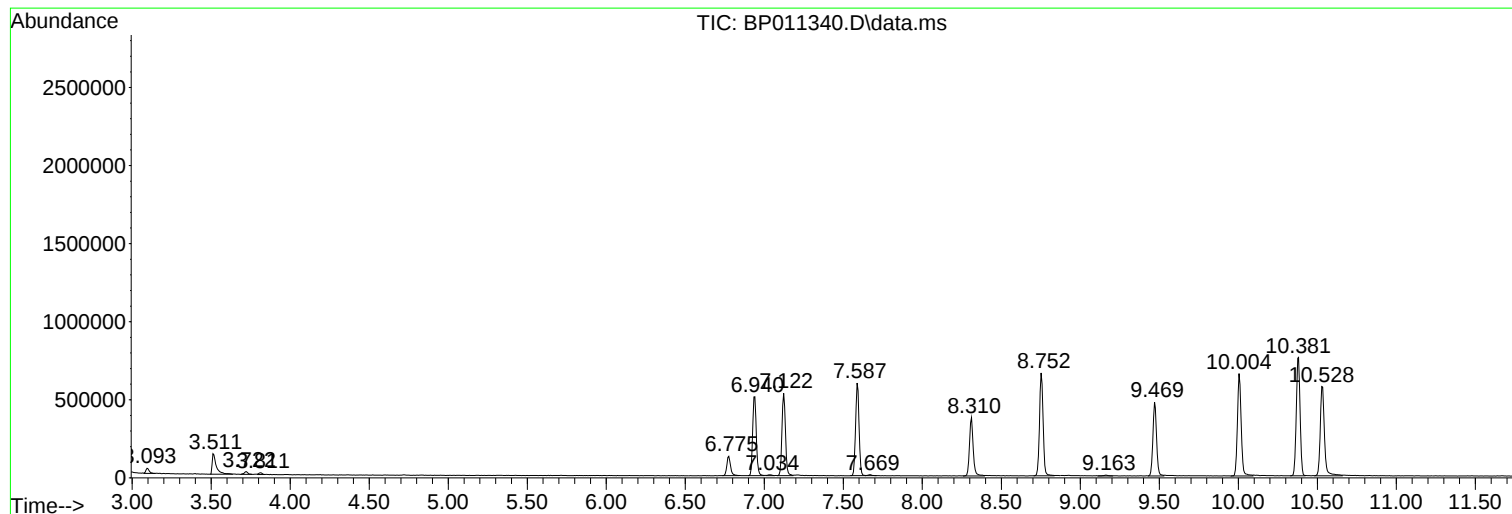

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011340.D
Acq On : 09 Aug 2022 21:19
Operator : CG/JU
Sample : N3900-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0C84

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011340.D
Acq On : 09 Aug 2022 21:19
Operator : CG/JU
Sample : N3900-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0C84

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc