

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
 Data File : BP011341.D
 Acq On : 09 Aug 2022 21:54
 Operator : CG/JU
 Sample : N3900-02
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0C86

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011341.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.093	15	18	26	rVB	34051	49539	1.32%	0.139%
2	3.511	87	89	111	rVB	150496	255900	6.81%	0.716%
3	3.722	120	125	131	rVB	17657	29064	0.77%	0.081%
4	3.811	136	140	145	rVB	12748	16942	0.45%	0.047%
5	4.722	292	295	299	rVB5	2841	3758	0.10%	0.011%
6	6.775	638	644	654	rBV	134880	218118	5.81%	0.611%
7	6.934	665	671	685	rVB	559667	881486	23.46%	2.468%
8	7.122	696	703	715	rBV	575231	872740	23.23%	2.443%
9	7.210	716	718	723	rVB5	3729	5168	0.14%	0.014%
10	7.587	775	782	791	rBV	584039	890476	23.70%	2.493%
11	7.675	791	797	804	rVB8	4907	10597	0.28%	0.030%
12	8.310	898	905	917	rBV	403784	646654	17.21%	1.810%
13	8.752	973	980	991	rBV	710385	1129141	30.05%	3.161%
14	9.163	1046	1050	1054	rVB3	5806	8592	0.23%	0.024%
15	9.469	1095	1102	1118	rBV	526175	843885	22.46%	2.363%
16	10.004	1185	1193	1206	rBV	730296	1178117	31.36%	3.298%
17	10.381	1249	1257	1266	rBV	736896	1234786	32.87%	3.457%
18	10.528	1274	1282	1297	rBV	642764	1128084	30.03%	3.158%
19	11.663	1471	1475	1481	rVB6	2674	4871	0.13%	0.014%
20	11.981	1520	1529	1537	rBV3	12709	26699	0.71%	0.075%
21	13.087	1713	1717	1721	rBV4	6661	9983	0.27%	0.028%
22	13.228	1734	1741	1744	rBV5	3926	5499	0.15%	0.015%
23	13.687	1811	1819	1828	rBV	1520086	2056110	54.73%	5.756%
24	13.951	1855	1864	1883	rBV	1584440	2264781	60.28%	6.340%
25	14.175	1897	1902	1905	rVB6	3171	3892	0.10%	0.011%
26	14.263	1908	1917	1925	rBV	1032563	1517159	40.38%	4.247%
27	14.322	1925	1927	1931	rVB5	3500	4406	0.12%	0.012%
28	14.492	1951	1956	1967	rBV2	48565	119332	3.18%	0.334%
29	14.710	1989	1993	1997	rVB7	3610	6771	0.18%	0.019%
30	15.028	2044	2047	2052	rVB	9696	13367	0.36%	0.037%
31	15.075	2052	2055	2059	rBV6	2920	4186	0.11%	0.012%
32	15.263	2080	2087	2104	rBV	2070240	2904829	77.32%	8.132%
33	15.392	2104	2109	2121	rVV	649870	921370	24.52%	2.579%
34	15.504	2123	2128	2133	rVB2	21199	32625	0.87%	0.091%
35	15.834	2181	2184	2188	rBV5	2719	4101	0.11%	0.011%
36	15.957	2200	2205	2211	rBV9	2984	6993	0.19%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
 Data File : BP011341.D
 Acq On : 09 Aug 2022 21:54
 Operator : CG/JU
 Sample : N3900-02
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0C86

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

37	16.057	2217	2222	2228	rVB7	5873	10275	0.27%	0.029%
38	16.169	2238	2241	2247	rVB8	2898	5055	0.13%	0.014%
39	16.710	2327	2333	2335	rBV6	4509	7175	0.19%	0.020%
40	16.810	2345	2350	2355	rBV6	4711	8073	0.21%	0.023%
41	16.969	2374	2377	2381	rBV6	4075	6168	0.16%	0.017%
42	17.033	2381	2388	2397	rBV	1186780	1696492	45.16%	4.749%
43	17.133	2398	2405	2422	rVV	2366037	3385852	90.12%	9.479%
44	17.598	2481	2484	2488	rVB6	2940	4347	0.12%	0.012%
45	17.728	2502	2506	2510	rVB7	4062	6231	0.17%	0.017%
46	17.945	2539	2543	2548	rBV5	15566	23604	0.63%	0.066%
47	18.298	2599	2603	2606	rBV6	3804	7115	0.19%	0.020%
48	18.410	2619	2622	2626	rBV5	5336	6744	0.18%	0.019%
49	18.963	2712	2716	2721	rBV3	29537	44584	1.19%	0.125%
50	19.033	2724	2728	2733	rVV	29222	38473	1.02%	0.108%
51	19.110	2738	2741	2743	rVV4	5990	7146	0.19%	0.020%
52	19.392	2783	2789	2798	rBV	2906547	3757022	100.00%	10.518%
53	19.716	2842	2844	2850	rVB5	13975	16842	0.45%	0.047%
54	20.892	3041	3044	3051	rBV5	42150	66384	1.77%	0.186%
55	21.157	3084	3089	3098	rBV	1414810	1760689	46.86%	4.929%
56	21.280	3108	3110	3119	rVB	63156	84786	2.26%	0.237%
57	23.315	3449	3456	3464	rBV2	1963064	3703360	98.57%	10.368%
58	23.463	3475	3481	3492	rVB2	910436	1762974	46.92%	4.936%




Sum of corrected areas: 35719412

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011341.D
Acq On : 09 Aug 2022 21:54
Operator : CG/JU
Sample : N3900-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0C86

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

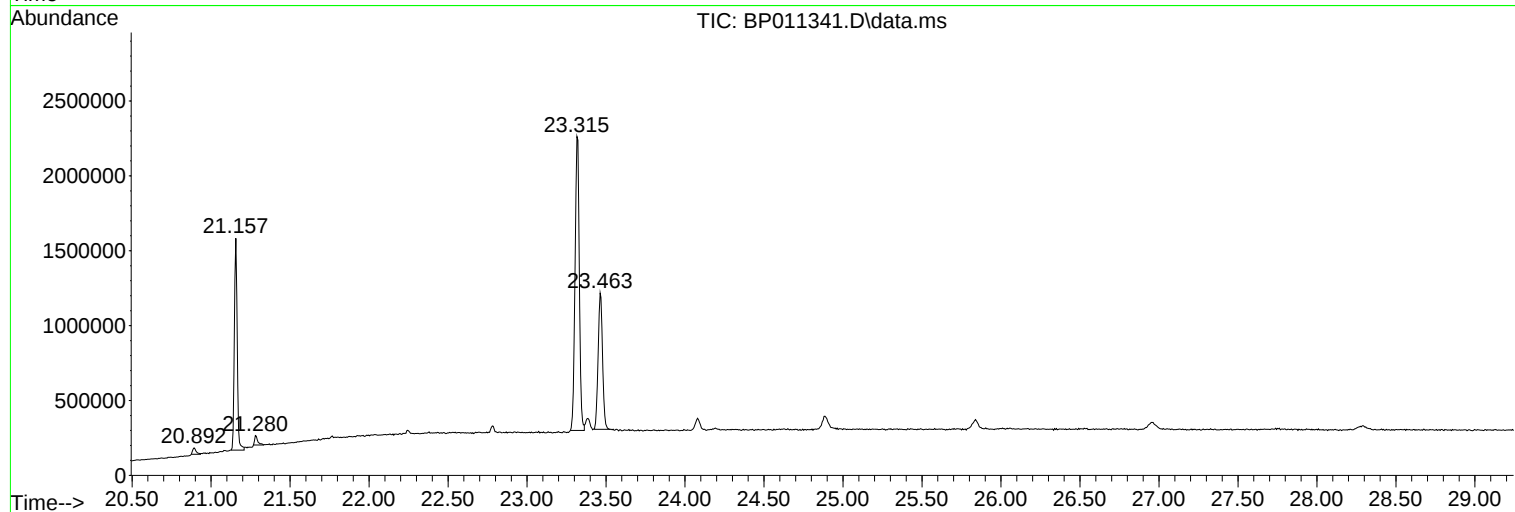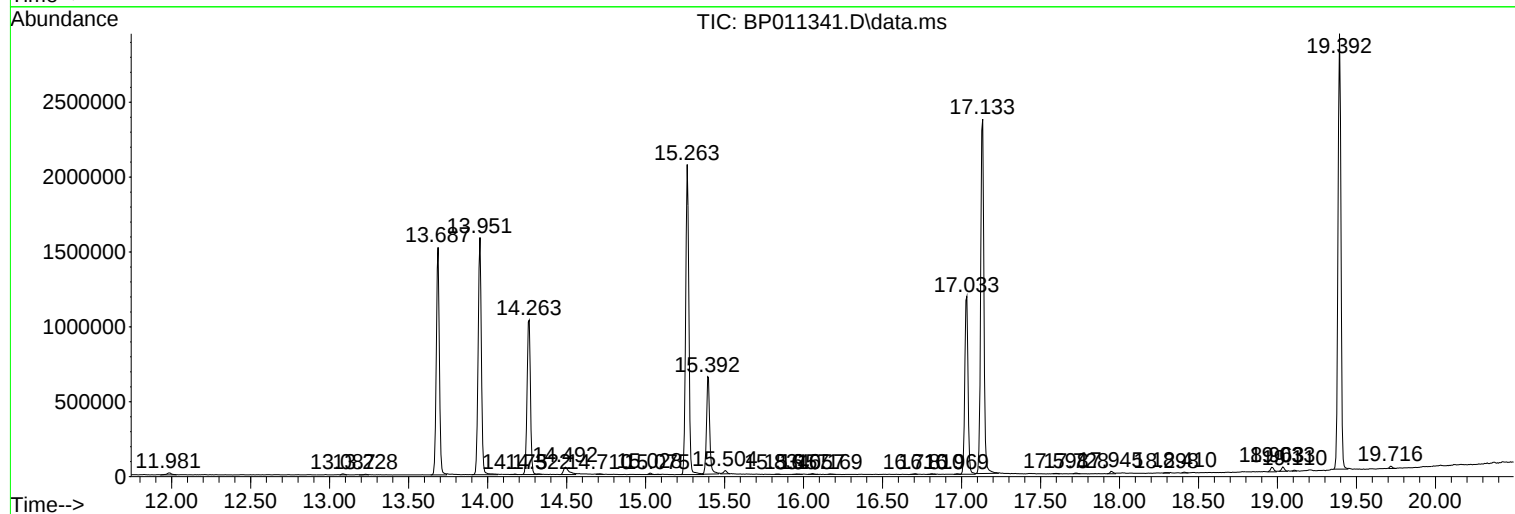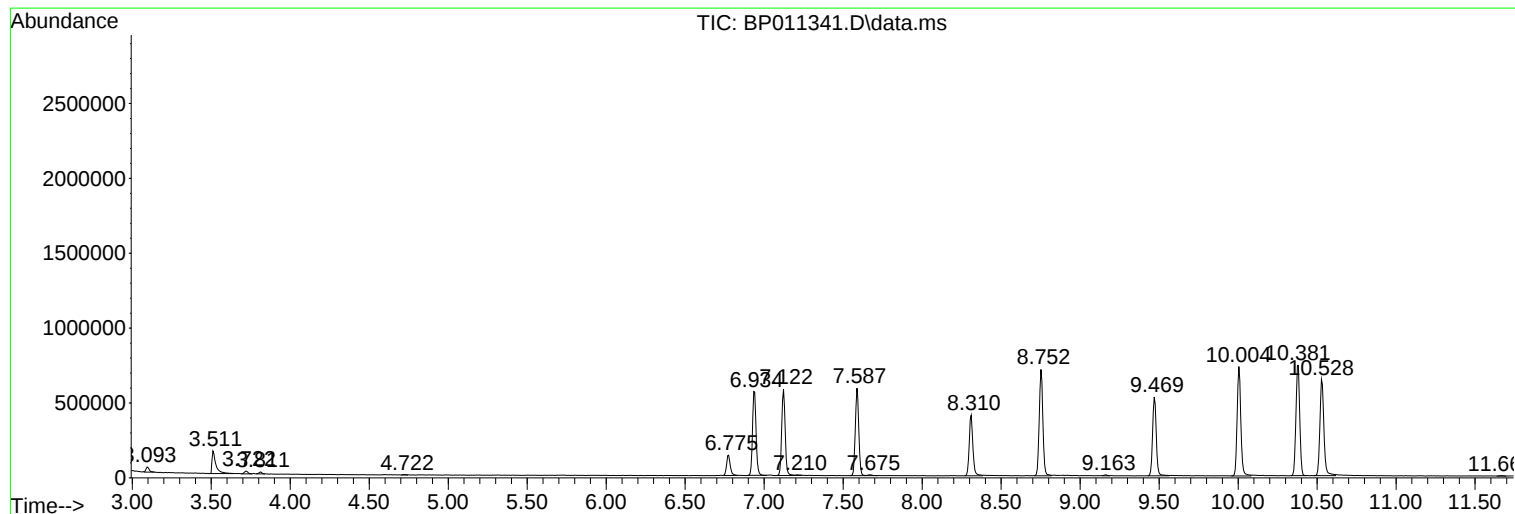

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011341.D
Acq On : 09 Aug 2022 21:54
Operator : CG/JU
Sample : N3900-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0C86

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011341.D
Acq On : 09 Aug 2022 21:54
Operator : CG/JU
Sample : N3900-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0C86

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc