

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
 Data File : BP011345.D
 Acq On : 10 Aug 2022 00:13
 Operator : CG/JU
 Sample : N3900-14
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0CA2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011345.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.093	15	18	29	rVB	36767	57412	1.49%	0.152%
2	3.517	87	90	102	rBV	102988	178720	4.65%	0.474%
3	3.723	119	125	129	rVB	17781	29925	0.78%	0.079%
4	3.811	136	140	146	rVB	15634	22442	0.58%	0.060%
5	4.181	201	203	208	rVB6	3127	4275	0.11%	0.011%
6	6.775	638	644	655	rBV	126523	204334	5.32%	0.542%
7	6.934	665	671	683	rBV	532534	837544	21.80%	2.223%
8	7.028	683	687	694	rVV	6948	11972	0.31%	0.032%
9	7.122	696	703	714	rVV	534387	819125	21.32%	2.174%
10	7.199	714	716	723	rVB8	4994	8940	0.23%	0.024%
11	7.587	775	782	790	rBV	666451	1013586	26.38%	2.691%
12	7.664	790	795	799	rVB4	7472	10535	0.27%	0.028%
13	8.311	899	905	920	rBV	376652	610324	15.89%	1.620%
14	8.752	973	980	992	rBV	693321	1105104	28.76%	2.934%
15	9.158	1046	1049	1053	rVB3	5892	8700	0.23%	0.023%
16	9.469	1095	1102	1115	rBV	523062	846738	22.04%	2.248%
17	10.005	1186	1193	1209	rBV	654942	1118471	29.11%	2.969%
18	10.375	1248	1256	1264	rBV	848992	1410096	36.70%	3.743%
19	10.534	1275	1283	1302	rBV	400566	768438	20.00%	2.040%
20	11.210	1393	1398	1401	rBV7	3386	6603	0.17%	0.018%
21	11.981	1522	1529	1539	rVB	14204	25223	0.66%	0.067%
22	12.875	1675	1681	1683	rBV6	3347	4229	0.11%	0.011%
23	13.081	1712	1716	1725	rVB2	10677	15900	0.41%	0.042%
24	13.169	1725	1731	1734	rBV6	4703	9624	0.25%	0.026%
25	13.687	1811	1819	1829	rBV	1540590	2092367	54.46%	5.554%
26	13.951	1855	1864	1878	rBV	1542752	2268776	59.05%	6.022%
27	14.169	1898	1901	1906	rVB6	5864	8365	0.22%	0.022%
28	14.257	1909	1916	1925	rBV	1147580	1696004	44.14%	4.502%
29	14.328	1925	1928	1936	rVB10	7941	14839	0.39%	0.039%
30	14.498	1952	1957	1976	rBV3	50636	150014	3.90%	0.398%
31	14.704	1989	1992	2000	rVB10	7802	13042	0.34%	0.035%
32	15.028	2043	2047	2052	rBV2	6669	9969	0.26%	0.026%
33	15.075	2052	2055	2058	rBV3	3880	5530	0.14%	0.015%
34	15.263	2080	2087	2096	rBV	2048384	2852321	74.24%	7.572%
35	15.393	2103	2109	2123	rBV	732499	1005842	26.18%	2.670%
36	15.504	2124	2128	2134	rVB2	21492	31615	0.82%	0.084%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
 Data File : BP011345.D
 Acq On : 10 Aug 2022 00:13
 Operator : CG/JU
 Sample : N3900-14
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0CA2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

37	15.840	2181	2185	2190	rVB7	3357	4858	0.13%	0.013%
38	15.957	2201	2205	2208	rBV4	3524	5483	0.14%	0.015%
39	15.998	2211	2212	2215	rVV2	4240	4249	0.11%	0.011%
40	16.057	2218	2222	2226	rVB7	7142	9657	0.25%	0.026%
41	16.810	2346	2350	2354	rBV6	7524	12898	0.34%	0.034%
42	16.969	2373	2377	2381	rBV7	6229	9474	0.25%	0.025%
43	17.028	2381	2387	2398	rBV	1336555	1933229	50.32%	5.132%
44	17.134	2398	2405	2419	rVV	2315133	3340790	86.96%	8.868%
45	17.345	2437	2441	2447	rVB4	5391	9434	0.25%	0.025%
46	17.563	2474	2478	2480	rBV5	5774	9284	0.24%	0.025%
47	17.728	2502	2506	2513	rVB9	11851	16876	0.44%	0.045%
48	17.945	2538	2543	2548	rBV	115325	156571	4.08%	0.416%
49	18.016	2552	2555	2560	rVB	18458	26467	0.69%	0.070%
50	18.969	2713	2717	2721	rVB3	29422	38954	1.01%	0.103%
51	19.033	2725	2728	2732	rBV	28762	36393	0.95%	0.097%
52	19.192	2752	2755	2760	rBV3	36657	43331	1.13%	0.115%
53	19.392	2783	2789	2796	rBV	3016260	3841957	100.00%	10.199%
54	20.886	3039	3043	3061	rVB2	415763	949974	24.73%	2.522%
55	21.157	3084	3089	3101	rBV	1612934	2196222	57.16%	5.830%
56	21.286	3108	3111	3115	rBV	101798	128297	3.34%	0.341%
57	23.316	3449	3456	3464	rBV2	1941721	3635608	94.63%	9.651%
58	23.463	3475	3481	3493	rVB2	1027033	1984814	51.66%	5.269%




Sum of corrected areas: 37671764

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011345.D
Acq On : 10 Aug 2022 00:13
Operator : CG/JU
Sample : N3900-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CA2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

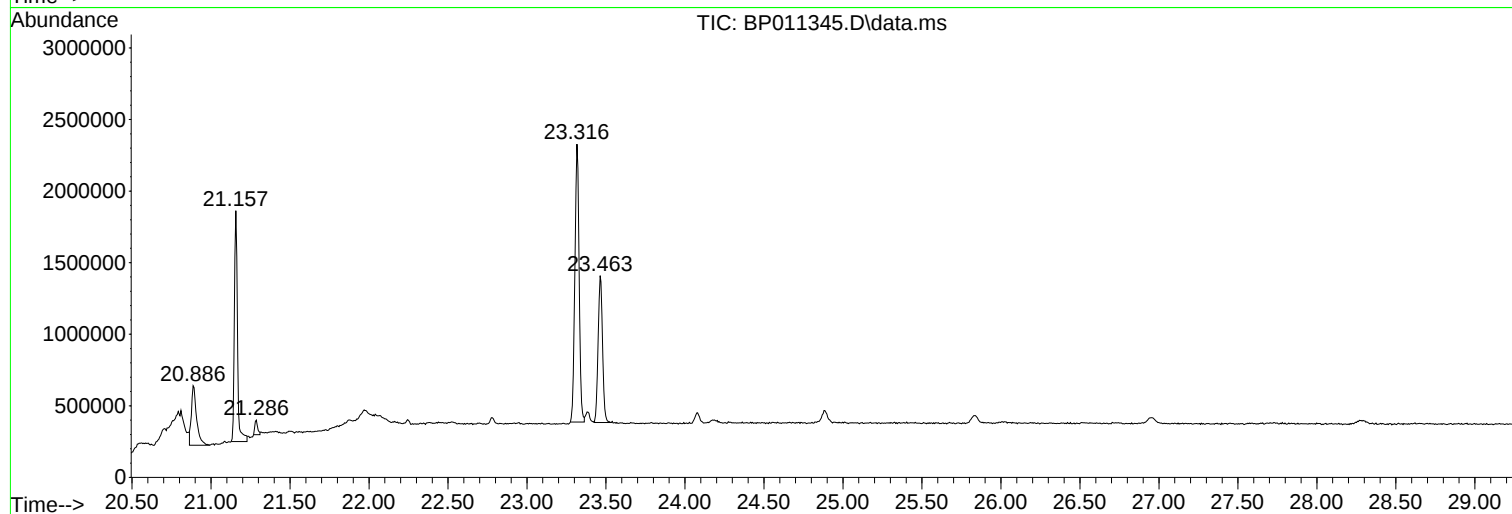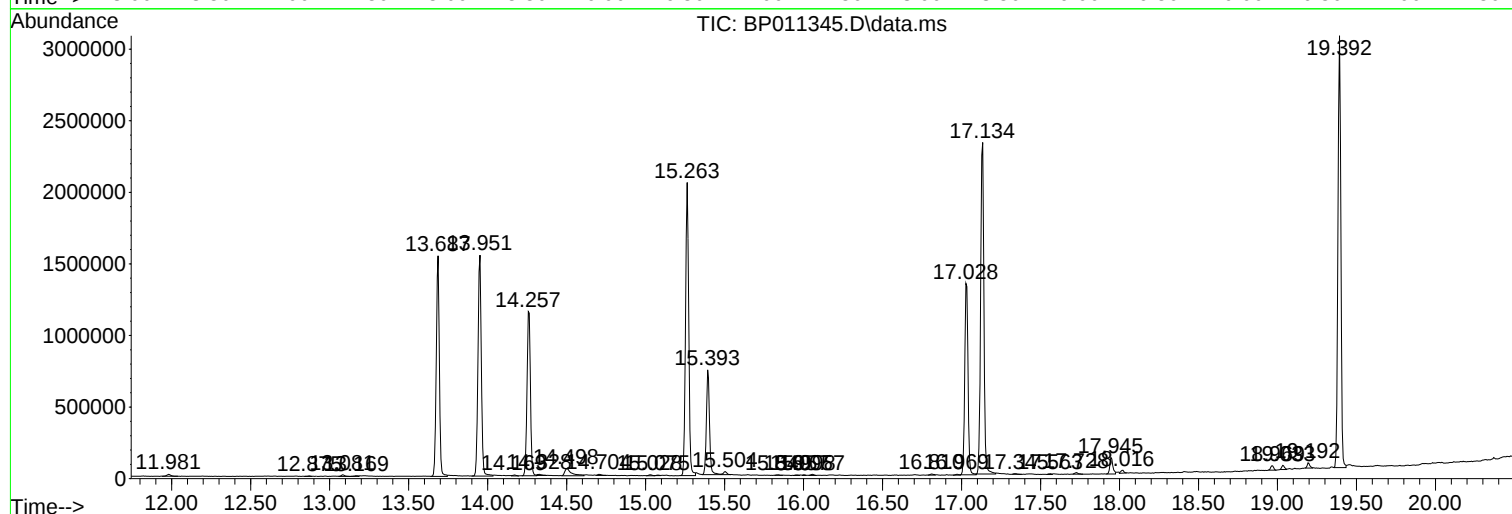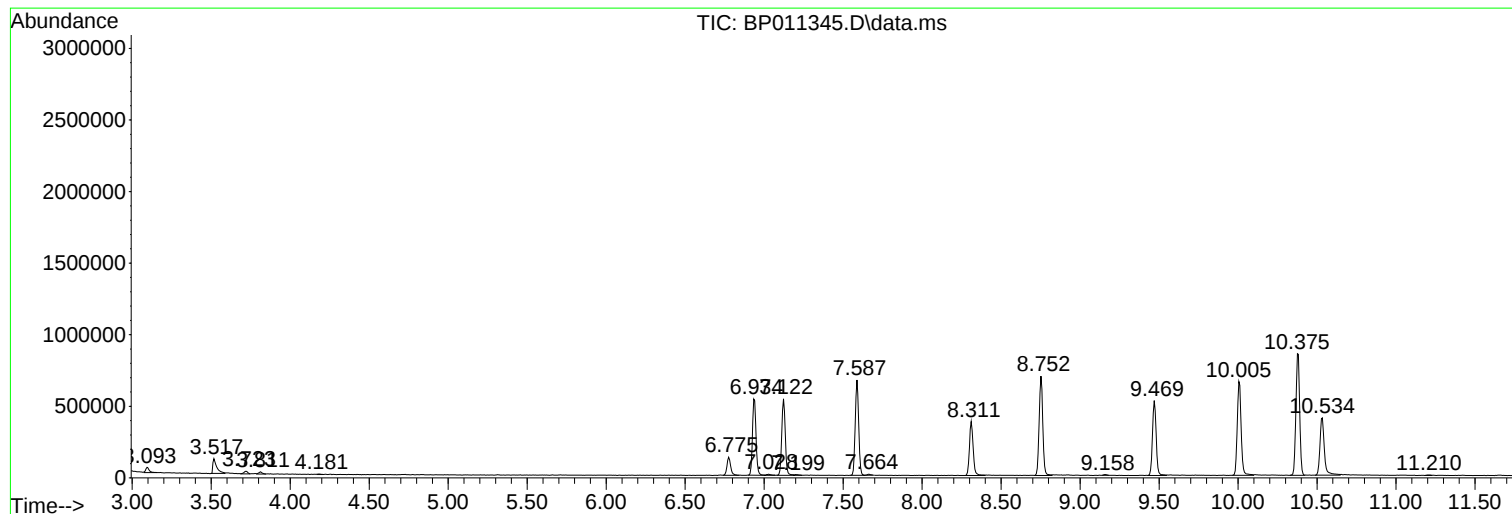

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011345.D
Acq On : 10 Aug 2022 00:13
Operator : CG/JU
Sample : N3900-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CA2










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.886	8.65 ng/ul	949974	Chrysene-d12	21.157

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Docosene			308	C22H44	001599-67-3	87
2	Octacosyl acetate			452	C30H60O2	018206-97-8	83
3	Trichloroacetic acid, pentadecyl...			372	C17H31Cl3O2	074339-53-0	70
4	1,2-Tetradecanediol			230	C14H30O2	021129-09-9	64
5	1-Hexacosene			364	C26H52	018835-33-1	64

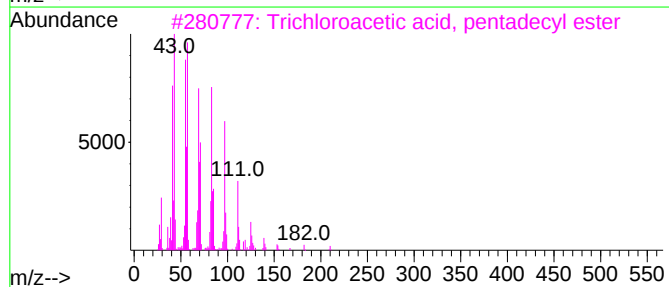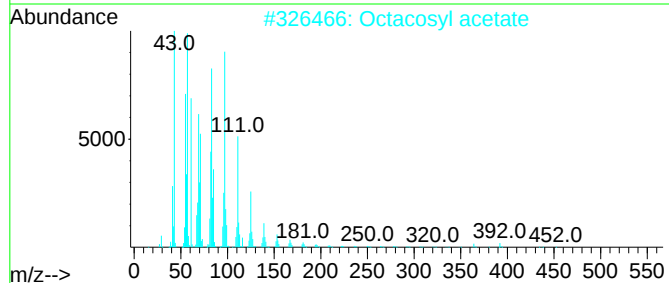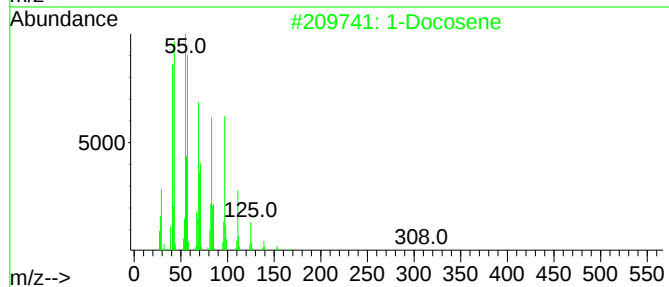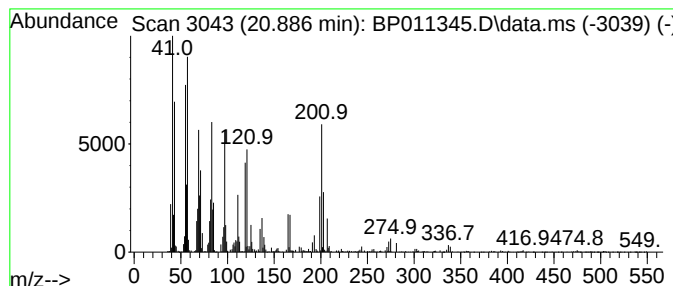

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011345.D
Acq On : 10 Aug 2022 00:13
Operator : CG/JU
Sample : N3900-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CA2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	20.886	8.7	ng/u1	949974	5	21.157	2196220	20.0