

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
 Data File : BP011356.D
 Acq On : 10 Aug 2022 07:08
 Operator : CG/JU
 Sample : N4069-03
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJK1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011356.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.087	14	17	26	rVB	41203	52710	1.55%	0.160%
2	3.517	88	90	102	rBV	44396	75805	2.22%	0.230%
3	3.717	118	124	130	rVB	17763	28382	0.83%	0.086%
4	3.805	135	139	143	rVB3	10391	15309	0.45%	0.047%
5	4.240	209	213	220	rVB	24766	36399	1.07%	0.111%
6	4.711	289	293	303	rBV4	3199	7223	0.21%	0.022%
7	4.834	311	314	320	rVB6	4545	7436	0.22%	0.023%
8	5.993	509	511	516	rVB6	3152	4668	0.14%	0.014%
9	6.722	630	635	638	rBV	13127	19050	0.56%	0.058%
10	6.769	638	643	656	rVB	162390	262286	7.70%	0.797%
11	6.934	665	671	681	rBV	497099	758572	22.27%	2.306%
12	7.028	683	687	695	rVV	3149	6327	0.19%	0.019%
13	7.116	695	702	713	rVV	539979	839590	24.64%	2.552%
14	7.205	715	717	725	rVB6	5775	8716	0.26%	0.026%
15	7.587	773	782	790	rBV	499566	785469	23.05%	2.388%
16	7.664	791	795	800	rVB3	6542	10043	0.29%	0.031%
17	8.305	898	904	915	rBV	422532	690699	20.27%	2.100%
18	8.752	972	980	988	rBV	621441	991651	29.11%	3.015%
19	8.881	997	1002	1008	rBV2	12197	17796	0.52%	0.054%
20	9.158	1041	1049	1056	rVB	19052	29594	0.87%	0.090%
21	9.469	1093	1102	1119	rBV	489255	811540	23.82%	2.467%
22	10.005	1185	1193	1209	rBV	664296	1129418	33.15%	3.434%
23	10.375	1249	1256	1262	rBV	673551	1091124	32.03%	3.317%
24	10.440	1262	1267	1275	rVV3	19219	47866	1.40%	0.146%
25	10.528	1275	1282	1296	rVB	324031	577882	16.96%	1.757%
26	11.040	1366	1369	1375	rBV8	1778	3672	0.11%	0.011%
27	11.204	1391	1397	1398	rBV5	4800	6922	0.20%	0.021%
28	11.657	1466	1474	1481	rBV2	12412	19611	0.58%	0.060%
29	11.810	1496	1500	1506	rVB9	2177	3943	0.12%	0.012%
30	11.981	1524	1529	1536	rVB4	12349	20737	0.61%	0.063%
31	12.204	1565	1567	1575	rVB9	1904	3940	0.12%	0.012%
32	12.404	1596	1601	1603	rBV6	2136	3435	0.10%	0.010%
33	12.599	1631	1634	1639	rBV6	3294	4536	0.13%	0.014%
34	12.863	1675	1679	1684	rBV7	4232	6911	0.20%	0.021%
35	13.081	1713	1716	1722	rVB8	2966	3641	0.11%	0.011%
36	13.163	1725	1730	1735	rBV5	5748	10550	0.31%	0.032%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
 Data File : BP011356.D
 Acq On : 10 Aug 2022 07:08
 Operator : CG/JU
 Sample : N4069-03
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJK1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

37	13.222	1735	1740	1745	rVB7	3425	6061	0.18%	0.018%
38	13.681	1811	1818	1825	rBV	1369212	1922058	56.42%	5.843%
39	13.951	1856	1864	1876	rBV	1360429	2046561	60.07%	6.222%
40	14.169	1898	1901	1909	rVB9	3806	5795	0.17%	0.018%
41	14.257	1909	1916	1930	rBV	928648	1345078	39.48%	4.089%
42	14.493	1948	1956	1970	rBV	64667	169332	4.97%	0.515%
43	14.704	1989	1992	1997	rVB7	4246	5288	0.16%	0.016%
44	14.863	2014	2019	2024	rBV9	1697	3573	0.10%	0.011%
45	15.075	2051	2055	2059	rBV	14835	19770	0.58%	0.060%
46	15.263	2080	2087	2102	rBV	1810242	2582695	75.81%	7.852%
47	15.393	2103	2109	2123	rVV	667999	893075	26.21%	2.715%
48	15.504	2124	2128	2134	rVB3	19646	34596	1.02%	0.105%
49	15.998	2209	2212	2216	rBV6	3017	4764	0.14%	0.014%
50	16.057	2219	2222	2230	rVB8	9356	15461	0.45%	0.047%
51	16.181	2238	2243	2244	rBV4	3065	4802	0.14%	0.015%
52	16.516	2295	2300	2305	rBV3	7899	12487	0.37%	0.038%
53	16.704	2328	2332	2337	rBV8	5716	8435	0.25%	0.026%
54	16.810	2346	2350	2354	rBV7	6104	10956	0.32%	0.033%
55	16.969	2374	2377	2381	rBV6	3223	4046	0.12%	0.012%
56	17.028	2381	2387	2398	rBV	1122805	1537898	45.14%	4.675%
57	17.128	2398	2404	2422	rVV2	2114021	2997741	87.99%	9.114%
58	17.339	2437	2440	2444	rVB4	6108	7092	0.21%	0.022%
59	17.592	2479	2483	2488	rVB2	8650	12880	0.38%	0.039%
60	17.728	2503	2506	2511	rVB5	8749	10575	0.31%	0.032%
61	17.945	2539	2543	2549	rBV6	18030	26362	0.77%	0.080%
62	18.016	2550	2555	2562	rVV	478663	570495	16.74%	1.734%
63	18.522	2638	2641	2650	rVB7	6610	10334	0.30%	0.031%
64	18.963	2712	2716	2720	rBV2	28919	38182	1.12%	0.116%
65	19.033	2724	2728	2732	rVB	25325	33401	0.98%	0.102%
66	19.339	2778	2780	2783	rBV4	8446	9192	0.27%	0.028%
67	19.392	2783	2789	2798	rBV	2685651	3406991	100.00%	10.358%
68	20.886	3040	3043	3051	rBV3	92461	145483	4.27%	0.442%
69	21.157	3084	3089	3103	rBV	1236230	1652055	48.49%	5.023%
70	21.286	3108	3111	3114	rBV2	63071	77393	2.27%	0.235%
71	23.322	3450	3457	3465	rBV2	1772927	3269220	95.96%	9.939%
72	23.469	3476	3482	3495	rVB2	833545	1599487	46.95%	4.863%




Sum of corrected areas: 32893067

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011356.D
Acq On : 10 Aug 2022 07:08
Operator : CG/JU
Sample : N4069-03
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJK1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

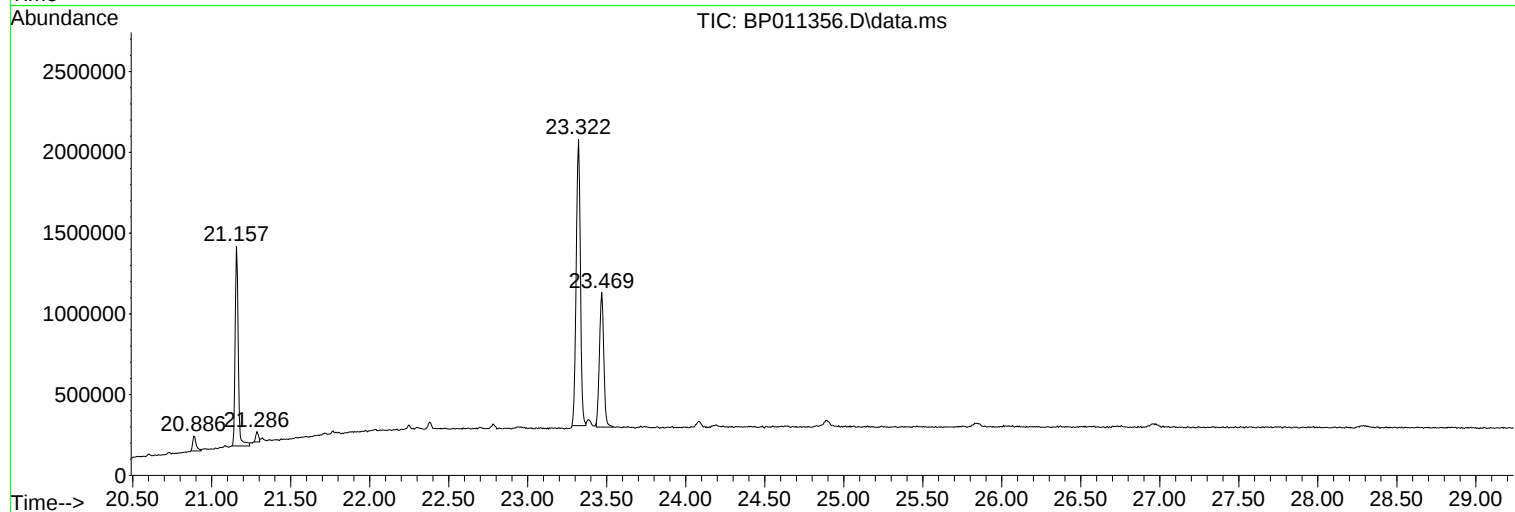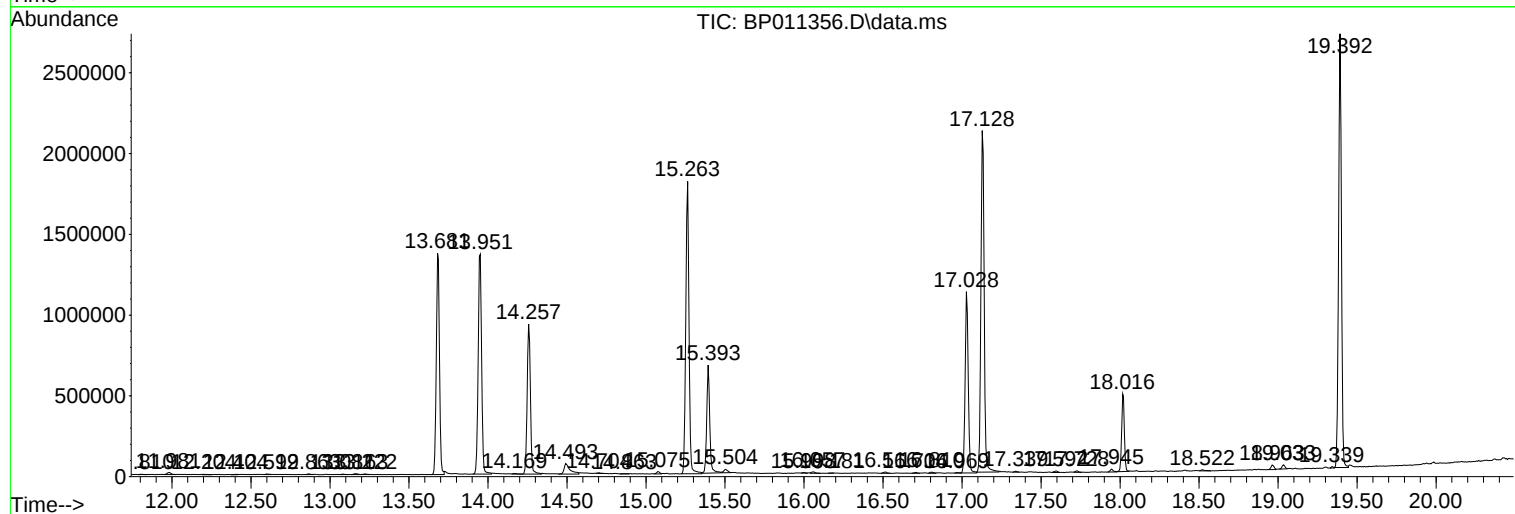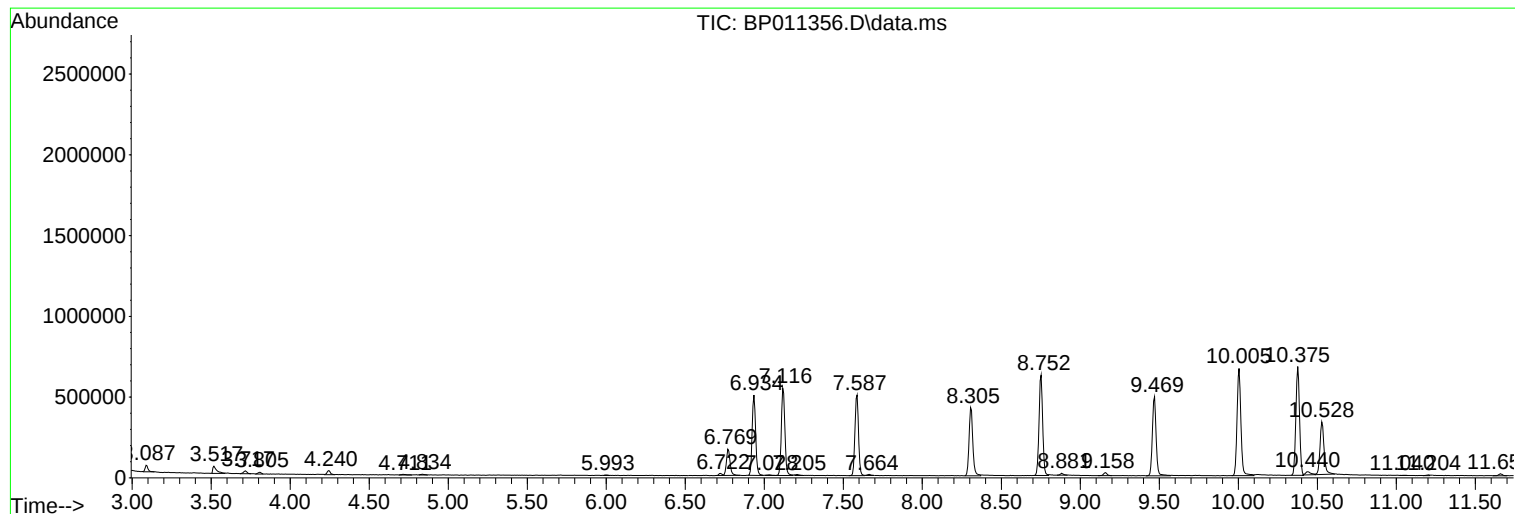

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011356.D
Acq On : 10 Aug 2022 07:08
Operator : CG/JU
Sample : N4069-03
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJK1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Dibutyl phthalate Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
18.016	7.42 ng/ul	570495	Phenanthrene-d10	17.028

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Dibutyl phthalate	278	C16H22O4	000084-74-2	97
2			1,2-Benzenedicarboxylic acid, bu...	334	C20H30O4	000085-69-8	90
3			1,2-Benzenedicarboxylic acid, bu...	278	C16H22O4	017851-53-5	90
4			Di-sec-butyl phthalate	278	C16H22O4	1000373-65-4	86
5			Dibutyl phthalate	278	C16H22O4	000084-74-2	83

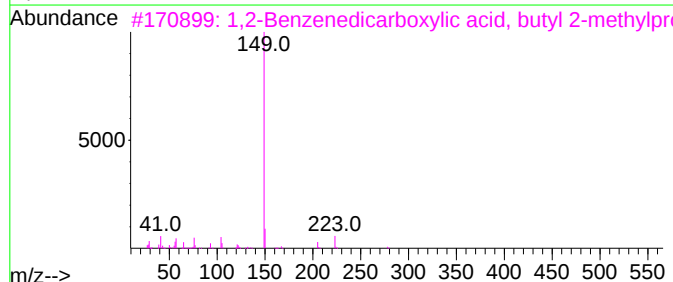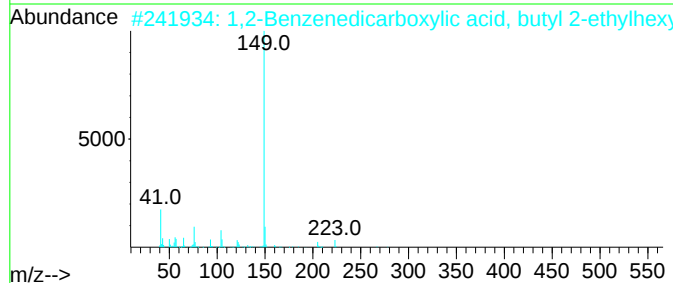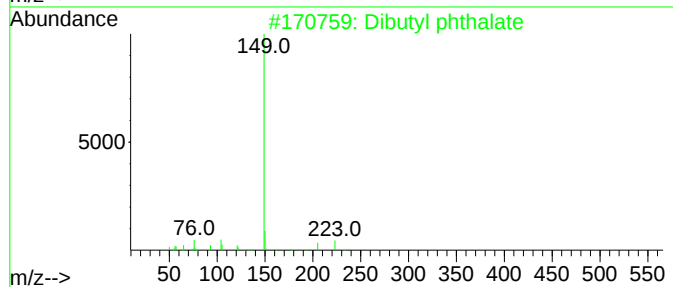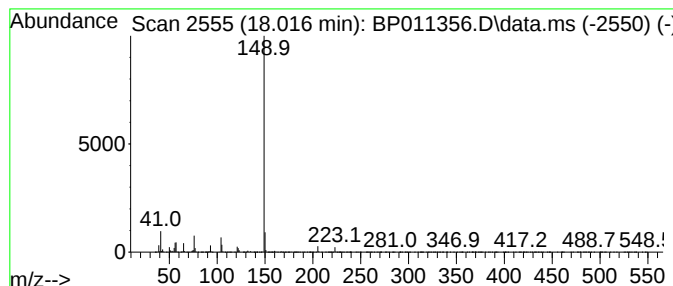

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011356.D
Acq On : 10 Aug 2022 07:08
Operator : CG/JU
Sample : N4069-03
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJK1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Dibutyl phthalate	18.016	7.4	ng/ul	570495	4	17.028	1537900	20.0