

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
 Data File : BP011358.D
 Acq On : 10 Aug 2022 08:17
 Operator : CG/JU
 Sample : N4069-07
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJL3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011358.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.052	5	11	26	rVB	598865	995425	33.19%	3.280%
2	3.505	85	88	102	rBV	145996	245785	8.20%	0.810%
3	3.711	118	123	130	rVB3	18119	32131	1.07%	0.106%
4	3.805	136	139	143	rVB	10823	13773	0.46%	0.045%
5	4.240	209	213	220	rVB	23548	33926	1.13%	0.112%
6	4.716	291	294	301	rVB5	2776	4886	0.16%	0.016%
7	4.834	307	314	317	rBV7	4342	6588	0.22%	0.022%
8	6.722	630	635	638	rBV2	17823	27296	0.91%	0.090%
9	6.769	638	643	654	rVB	134770	217828	7.26%	0.718%
10	6.934	664	671	682	rVB	440090	675464	22.52%	2.226%
11	7.116	693	702	711	rBV	484082	741853	24.74%	2.444%
12	7.199	714	716	725	rVB9	5017	10019	0.33%	0.033%
13	7.581	774	781	789	rBV	484295	778793	25.97%	2.566%
14	7.663	789	795	801	rVB3	8107	14627	0.49%	0.048%
15	7.781	813	815	821	rVB7	1857	3057	0.10%	0.010%
16	8.304	898	904	916	rBV	368085	598971	19.97%	1.974%
17	8.746	972	979	989	rBV	542178	881929	29.41%	2.906%
18	8.875	998	1001	1006	rBV7	3002	4980	0.17%	0.016%
19	9.157	1042	1049	1054	rVB	34774	54536	1.82%	0.180%
20	9.463	1093	1101	1115	rBV	426941	711896	23.74%	2.346%
21	10.004	1185	1193	1206	rBV	577081	1008933	33.64%	3.324%
22	10.198	1222	1226	1228	rVB5	2560	3141	0.10%	0.010%
23	10.375	1245	1256	1265	rBV	653395	1086637	36.24%	3.581%
24	10.528	1275	1282	1298	rBV	190934	394903	13.17%	1.301%
25	11.046	1366	1370	1378	rVB9	3359	6529	0.22%	0.022%
26	11.163	1385	1390	1394	rBV7	4008	5793	0.19%	0.019%
27	11.657	1467	1474	1481	rBV2	16452	25256	0.84%	0.083%
28	11.981	1520	1529	1537	rBV2	11013	22064	0.74%	0.073%
29	12.063	1537	1543	1548	rBV8	3530	6785	0.23%	0.022%
30	12.610	1630	1636	1638	rBV7	2644	4476	0.15%	0.015%
31	12.863	1675	1679	1685	rBV9	2572	3776	0.13%	0.012%
32	13.157	1724	1729	1736	rBV6	5086	10616	0.35%	0.035%
33	13.222	1736	1740	1744	rBV6	2475	3916	0.13%	0.013%
34	13.681	1810	1818	1831	rBV	1230358	1679358	56.00%	5.534%
35	13.792	1831	1837	1843	rVB9	5728	15530	0.52%	0.051%
36	13.945	1857	1863	1879	rBV	1221107	1803518	60.14%	5.943%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
 Data File : BP011358.D
 Acq On : 10 Aug 2022 08:17
 Operator : CG/JU
 Sample : N4069-07
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBJL3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

37	14.051	1879	1881	1890	rVB10	3720	9722	0.32%	0.032%
38	14.169	1898	1901	1905	rVB6	3018	4099	0.14%	0.014%
39	14.257	1909	1916	1924	rBV	936578	1327231	44.26%	4.373%
40	14.492	1949	1956	1971	rBV	45190	123341	4.11%	0.406%
41	14.645	1979	1982	1987	rVB6	4449	5988	0.20%	0.020%
42	14.804	2006	2009	2014	rVB7	3764	5260	0.18%	0.017%
43	15.075	2051	2055	2061	rBV	10451	15041	0.50%	0.050%
44	15.263	2080	2087	2102	rBV	1554197	2265461	75.54%	7.465%
45	15.392	2103	2109	2123	rVV	615460	815796	27.20%	2.688%
46	15.504	2124	2128	2134	rVB2	16033	26334	0.88%	0.087%
47	15.839	2178	2185	2186	rBV6	2392	3660	0.12%	0.012%
48	16.051	2217	2221	2225	rBV7	4335	6412	0.21%	0.021%
49	16.163	2238	2240	2248	rVB9	4037	6751	0.23%	0.022%
50	16.328	2264	2268	2269	rBV4	2454	3456	0.12%	0.011%
51	16.445	2285	2288	2290	rBV4	2303	3211	0.11%	0.011%
52	16.510	2293	2299	2305	rVV4	6147	12950	0.43%	0.043%
53	16.622	2313	2318	2321	rBV7	5563	8425	0.28%	0.028%
54	16.704	2329	2332	2339	rVB9	3971	7446	0.25%	0.025%
55	16.810	2345	2350	2354	rBV7	4404	8280	0.28%	0.027%
56	17.028	2381	2387	2398	rBV	1116817	1545320	51.53%	5.092%
57	17.128	2398	2404	2421	rVV	1879549	2695121	89.87%	8.881%
58	17.339	2437	2440	2447	rVB2	6711	9159	0.31%	0.030%
59	17.592	2480	2483	2490	rVB2	7754	11972	0.40%	0.039%
60	17.945	2539	2543	2547	rBV4	11207	14633	0.49%	0.048%
61	18.016	2551	2555	2560	rVB	11966	16452	0.55%	0.054%
62	18.410	2619	2622	2626	rVB5	5253	6830	0.23%	0.023%
63	18.963	2712	2716	2721	rBV3	24550	32651	1.09%	0.108%
64	19.033	2724	2728	2733	rVV2	25171	33493	1.12%	0.110%
65	19.392	2783	2789	2796	rBV	2396492	2998834	100.00%	9.881%
66	20.886	3041	3043	3049	rVB2	39483	50048	1.67%	0.165%
67	21.157	3084	3089	3099	rBV	1321974	1622895	54.12%	5.348%
68	21.286	3108	3111	3115	rBV3	57553	71939	2.40%	0.237%
69	23.321	3450	3457	3464	rBV2	1564351	2844299	94.85%	9.372%
70	23.468	3476	3482	3495	rVB2	850034	1600997	53.39%	5.275%




Sum of corrected areas: 30348501

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011358.D
Acq On : 10 Aug 2022 08:17
Operator : CG/JU
Sample : N4069-07
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJL3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

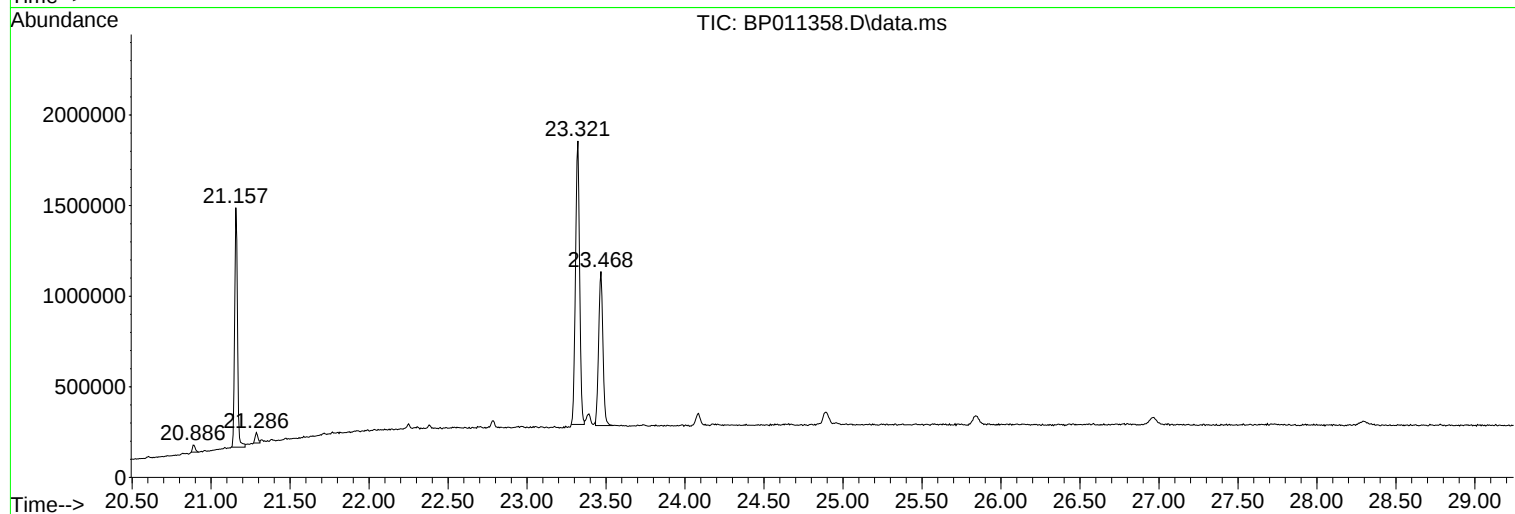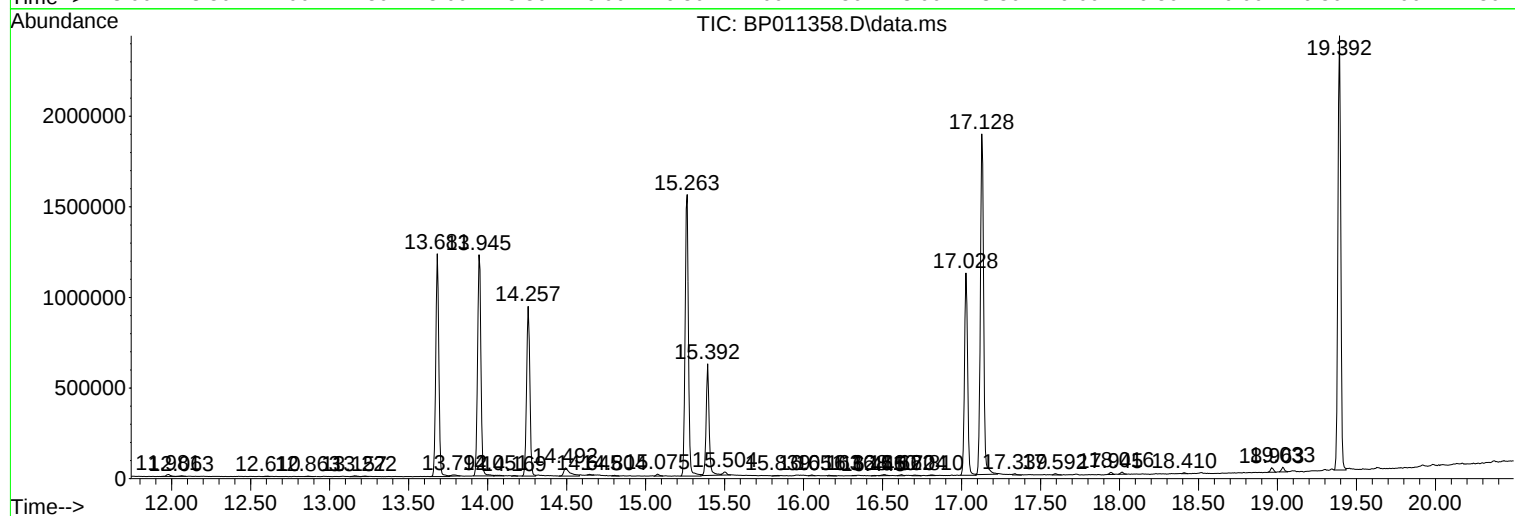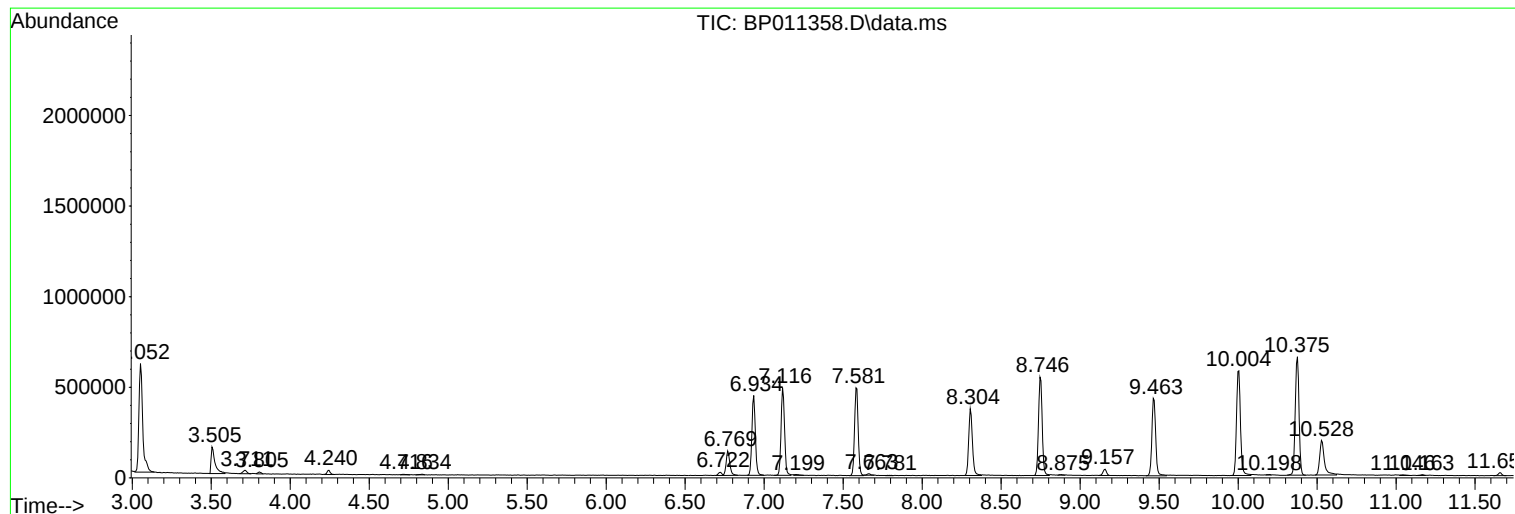

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011358.D
Acq On : 10 Aug 2022 08:17
Operator : CG/JU
Sample : N4069-07
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJL3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080922\
Data File : BP011358.D
Acq On : 10 Aug 2022 08:17
Operator : CG/JU
Sample : N4069-07
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBJL3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc