

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP081120\
 Data File : BP002944.D
 Acq On : 11 Aug 2020 18:27
 Operator : CG/JU
 Sample : L3624-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SS-TP-1

Quant Time: Aug 13 06:51:24 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP073020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 11 17:14:14 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	507411	20.00	ng	0.00
21) Naphthalene-d8	10.48	136	1964339	20.00	ng	0.00
39) Acenaphthene-d10	14.34	164	1088794	20.00	ng	0.00
64) Phenanthrene-d10	17.09	188	2118052	20.00	ng	0.00
76) Chrysene-d12	21.18	240	1597847	20.00	ng	0.00
86) Perylene-d12	23.43	264	1512437	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.31	112	2876838	86.77	ng	0.00
7) Phenol-d6	6.88	99	2982027	64.79	ng	0.00
23) Nitrobenzene-d5	8.85	82	2182184	60.17	ng	0.00
42) 2,4,6-Tribromophenol	15.83	330	1257922	92.96	ng	0.00
45) 2-Fluorobiphenyl	12.96	172	5676964	71.24	ng	0.00
79) Terphenyl-d14	19.66	244	6165251	77.24	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP081120\
Data File : BP002944.D
Acq On : 11 Aug 2020 18:27
Operator : CG/JU
Sample : L3624-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SS-TP-1

Quant Time: Aug 13 06:51:24 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP073020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 11 17:14:14 2020
Response via : Initial Calibration

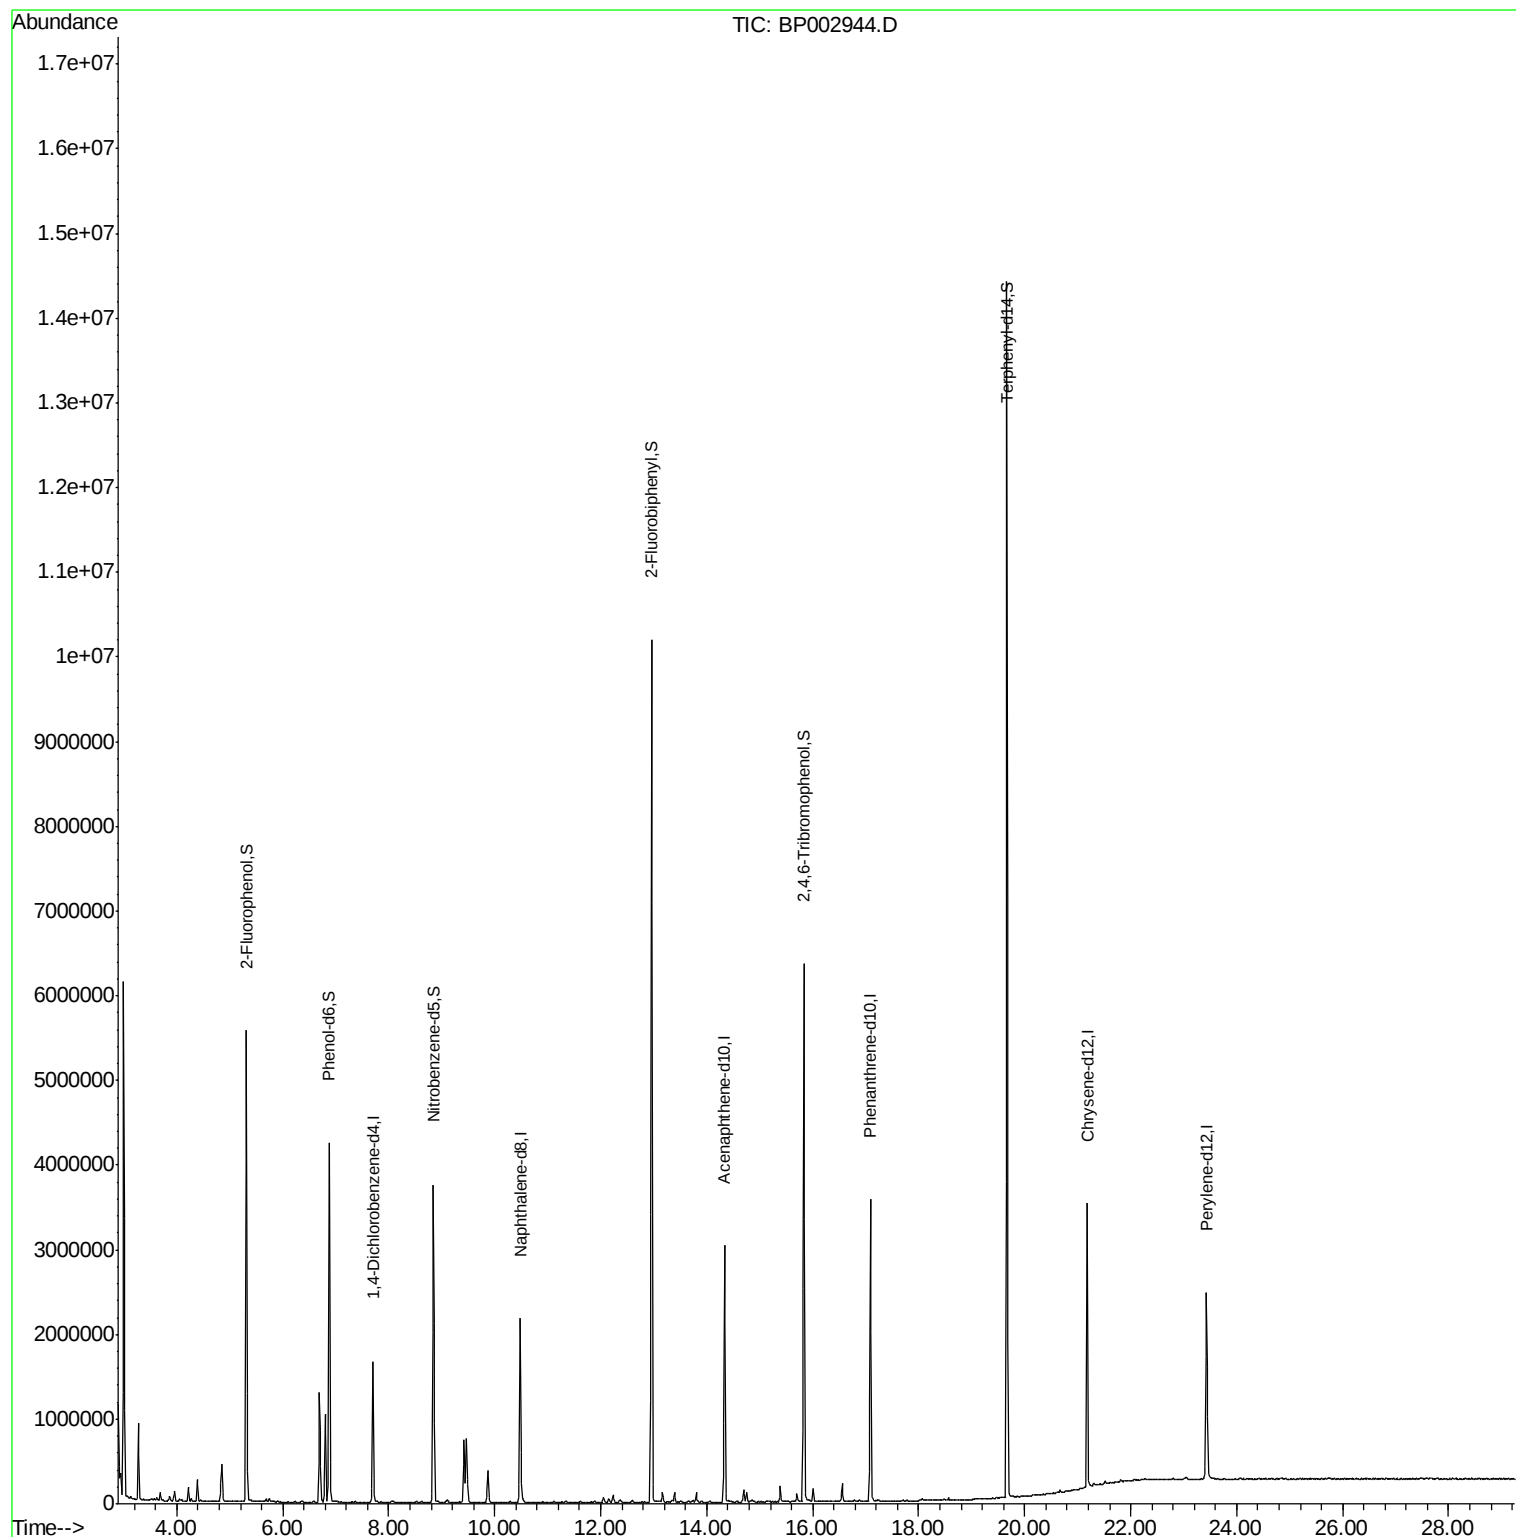




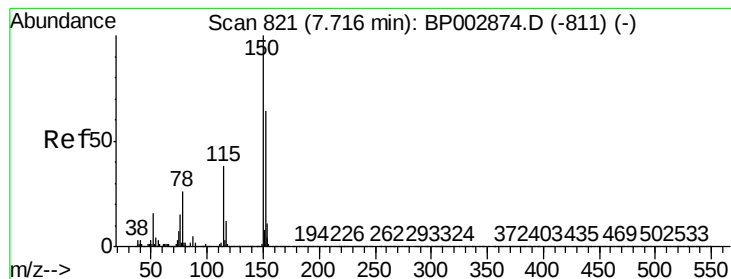


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.70 min Scan# 819
Delta R.T. -0.00 min
Lab File: BP002944.D
Acq: 11 Aug 2020 18:27

Instrument :
BNA_P
ClientSampleId :
SS-TP-1




Tot Ion:152 Resp: 507411
Ion Ratio Lower Upper
152 100
150 153.0 124.2 186.4
115 53.1 42.1 63.1

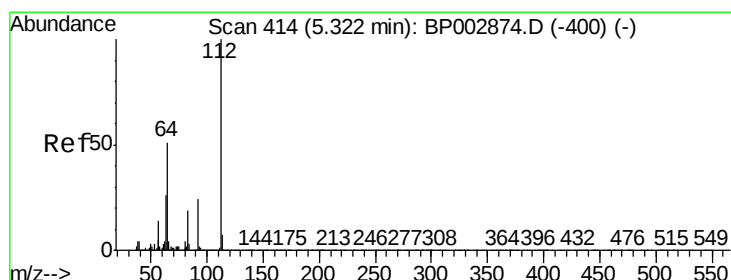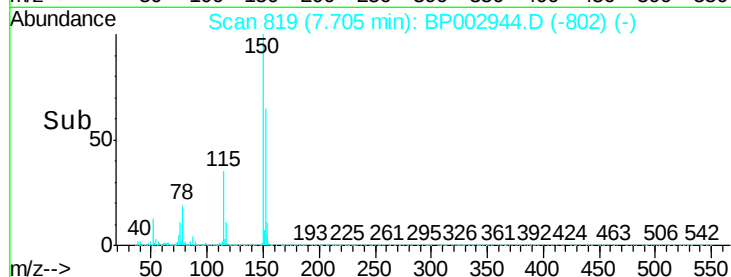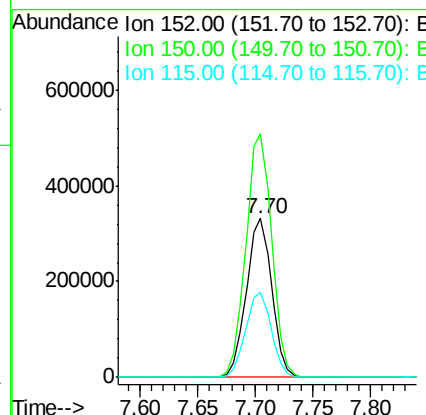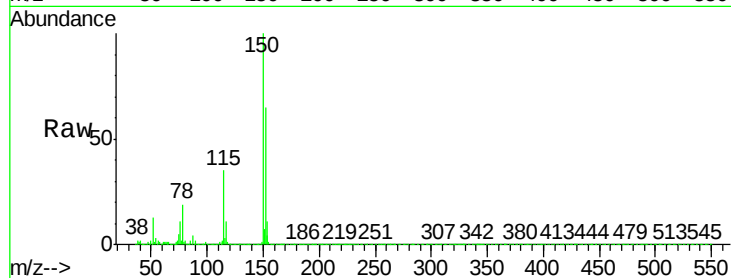

#5

2-Fluorophenol
Concen: 86.774 ng
RT: 5.31 min Scan# 412
Delta R.T. 0.01 min
Lab File: BP002944.D
Acq: 11 Aug 2020 18:27

Tgt Ion:112 Resp: 2876838
Ion Ratio Lower Upper
112 100
64 41.5 33.8 50.8
63 20.7 17.2 25.8

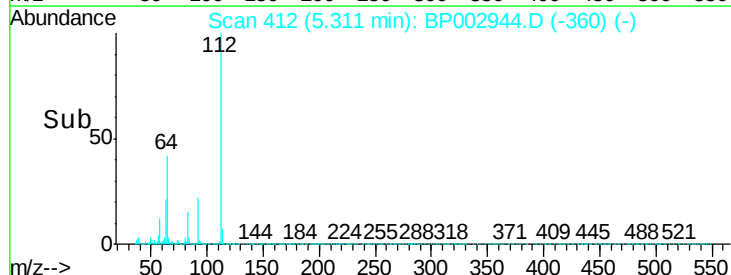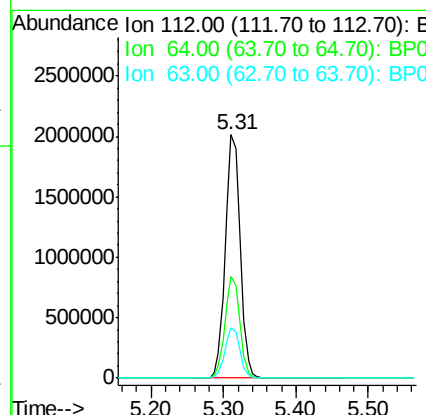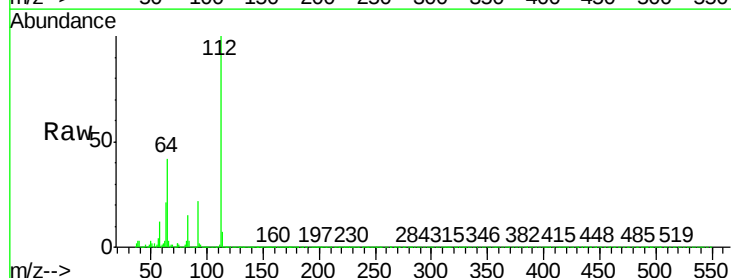



#7

Phenol-d6

Concen: 64.786 ng

RT: 6.88 min Scan# 679

Delta R.T. -0.00 min

Lab File: BP002944.D

Acq: 11 Aug 2020 18:27

Instrument :


BNA_P

ClientSampleId :

SS-TP-1

Tot Ion: 99 Resp: 2982027

Ion	Ratio	Lower	Upper
99	100		
42	9.9	8.1	12.1
71	25.8	21.0	31.4



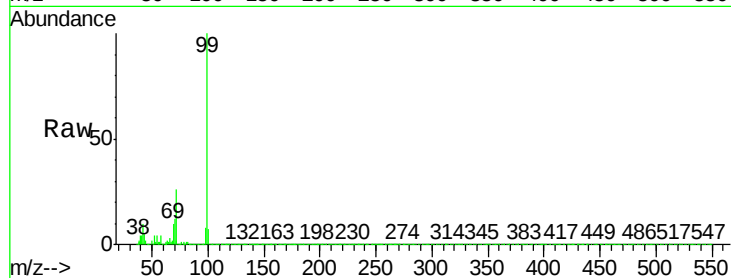


Abundance

Ion 99.00 (98.70 to 99.70): BP0

Ion 42.00 (41.70 to 42.70): BP0

Ion 71.00 (70.70 to 71.70): BP0

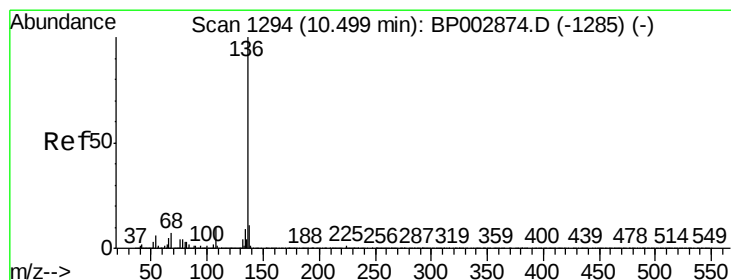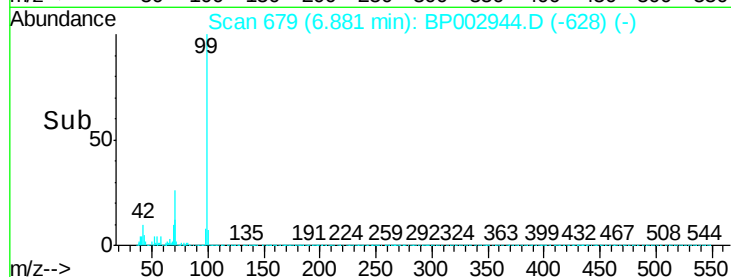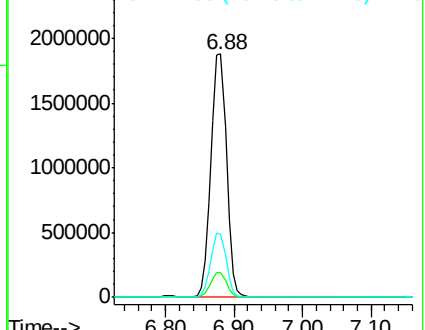

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.48 min Scan# 1291


Delta R.T. -0.00 min

Lab File: BP002944.D

Acq: 11 Aug 2020 18:27

Tgt Ion: 136 Resp: 1964339

Ion	Ratio	Lower	Upper
136	100		
137	11.0	9.0	13.4
54	5.1	3.9	5.9
68	4.8	3.8	5.8

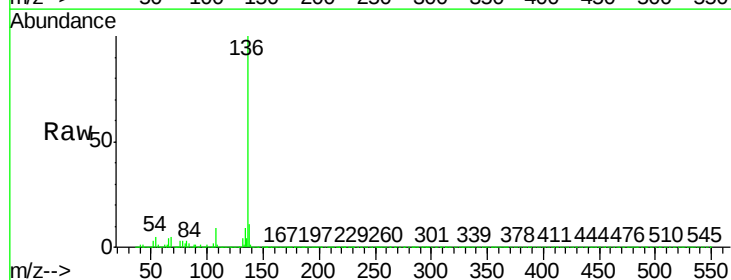



Abundance


Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BP0

Ion 68.00 (67.70 to 68.70): BP0



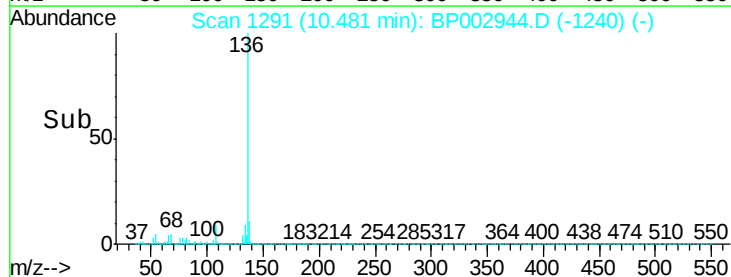
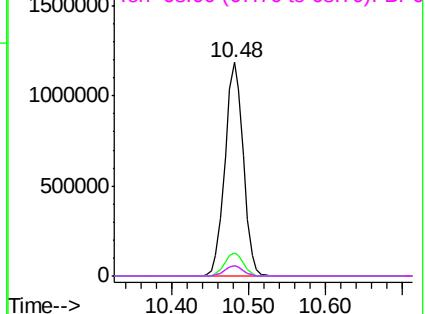


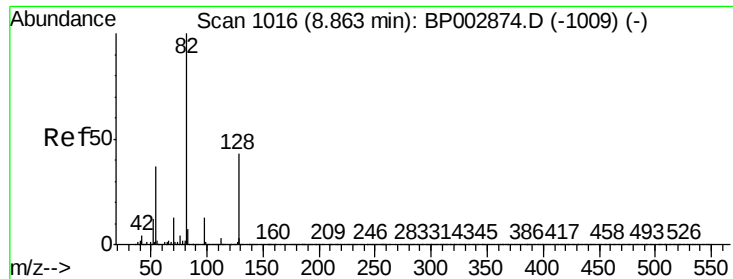

#23
Nitrobenzene-d5
Concen: 60.169 ng
RT: 8.85 min Scan# 1013
Delta R.T. -0.00 min
Lab File: BP002944.D
Acq: 11 Aug 2020 18:27




Instrument :
BNA_P
ClientSampleId :
SS-TP-1


Tot Ion: 82 Resp: 2182184
Ion Ratio Lower Upper
82 100
128 55.8 44.6 66.8
54 36.5 29.2 43.8

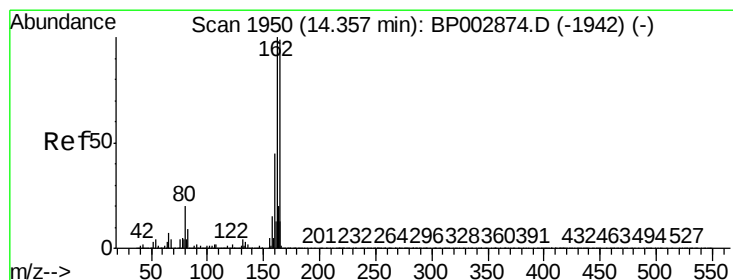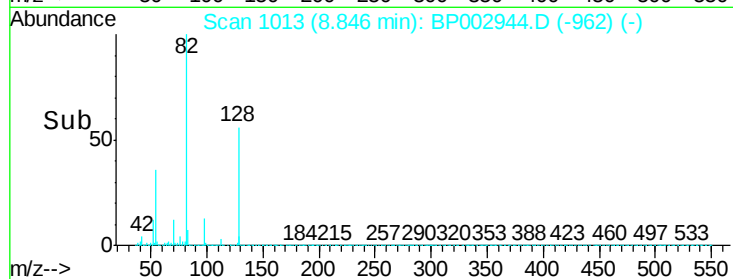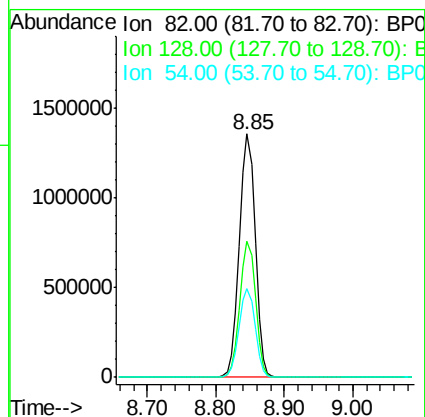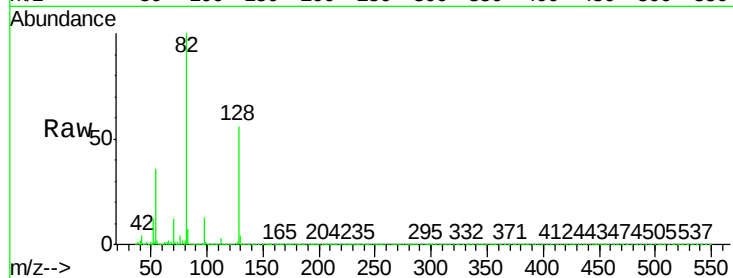

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.34 min Scan# 1947
Delta R.T. -0.00 min
Lab File: BP002944.D
Acq: 11 Aug 2020 18:27

Tgt Ion:164 Resp: 1088794
Ion Ratio Lower Upper
164 100
162 102.0 81.0 121.4
160 45.5 36.2 54.4


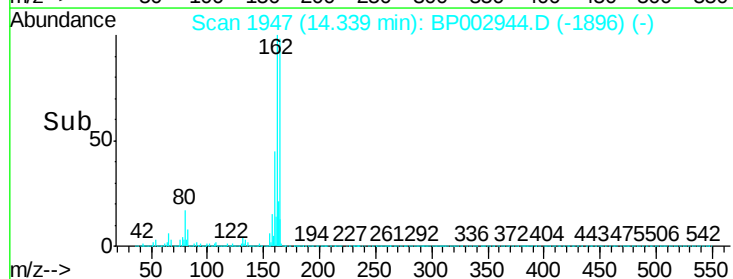
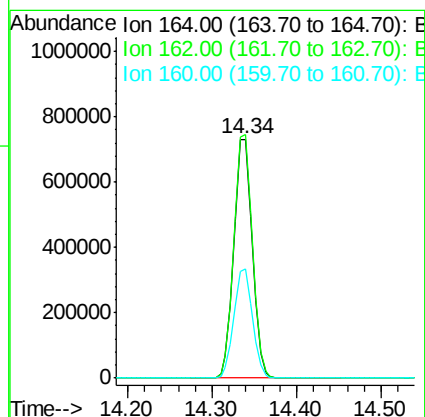
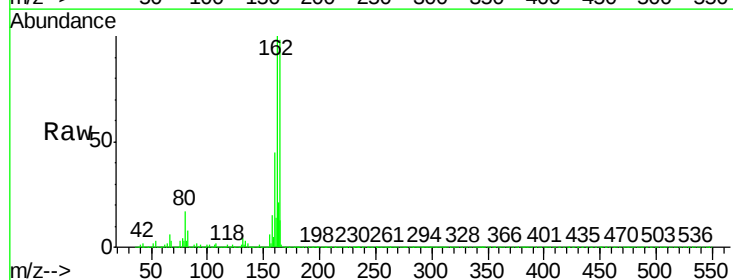


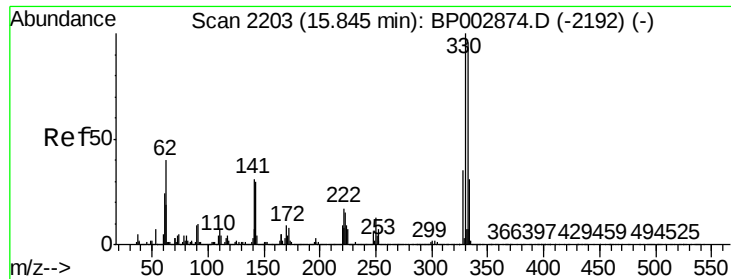

#42
 2,4,6-Tribromophenol
 Concen: 92.956 ng
 RT: 15.83 min Scan# 2200
 Delta R.T. -0.01 min
 Lab File: BP002944.D
 Acq: 11 Aug 2020 18:27




Instrument :
 BNA_P
 ClientSampleID :
 SS-TP-1


Tot Ion:330 Resp: 1257922
 Ion Ratio Lower Upper
 330 100
 332 96.4 77.0 115.4
 141 35.1 28.6 43.0

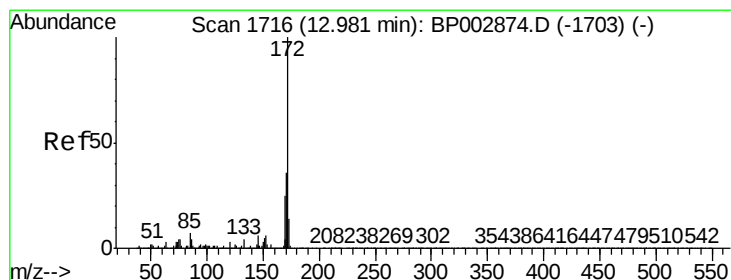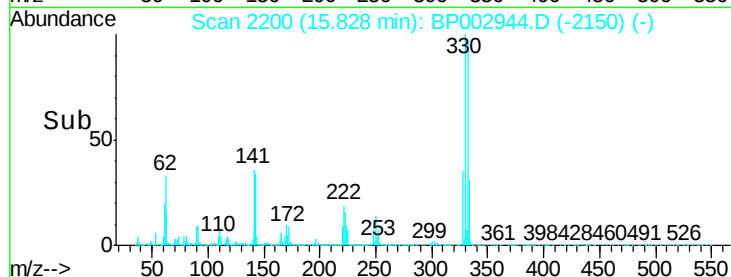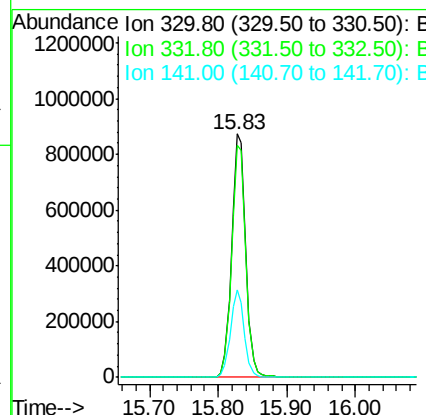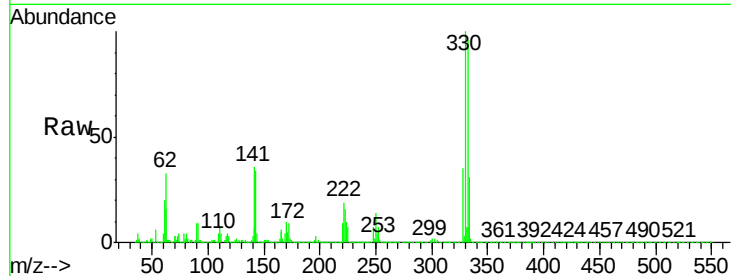

#45
 2-Fluorobiphenyl
 Concen: 71.239 ng
 RT: 12.96 min Scan# 1713
 Delta R.T. -0.00 min
 Lab File: BP002944.D
 Acq: 11 Aug 2020 18:27

Tgt Ion:172 Resp: 5676964
 Ion Ratio Lower Upper
 172 100
 171 36.0 29.6 44.4
 170 24.1 19.6 29.4

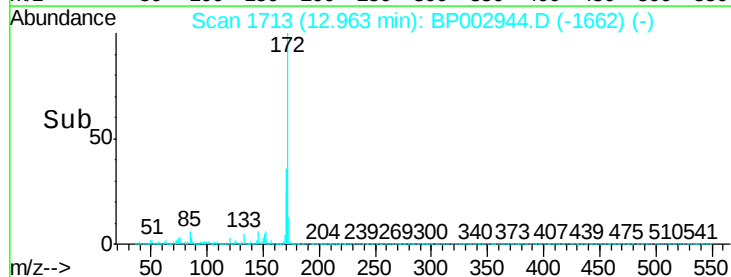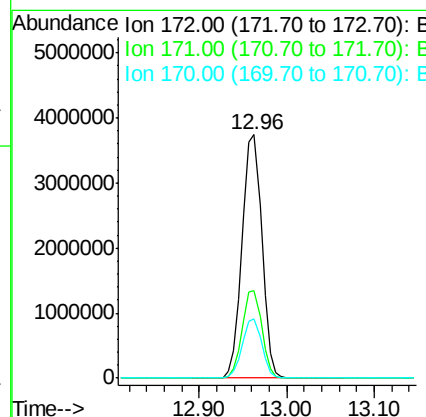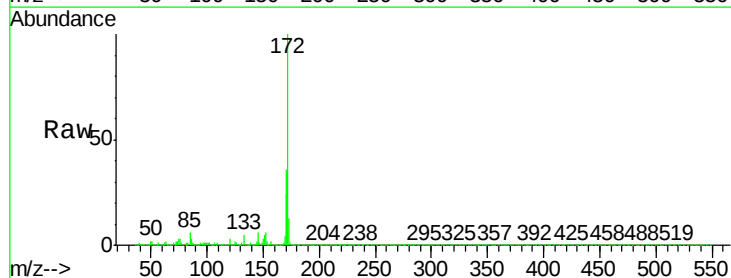

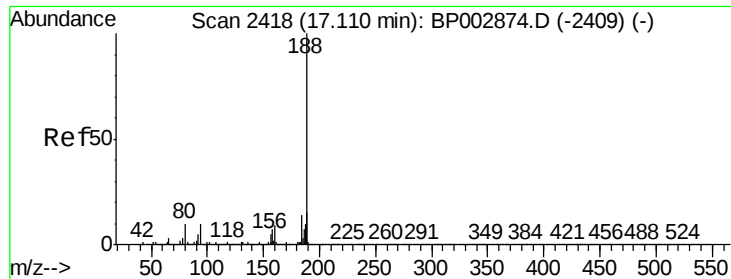

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.09 min Scan# 2414

Delta R.T. -0.01 min

Lab File: BP002944.D

Acq: 11 Aug 2020 18:27

Instrument :

BNA_P

ClientSampleId :

SS-TP-1


Tot Ion:188 Resp: 2118052

Ion Ratio Lower Upper

188 100

94 9.3 7.0 10.6




80 9.4 7.0 10.6

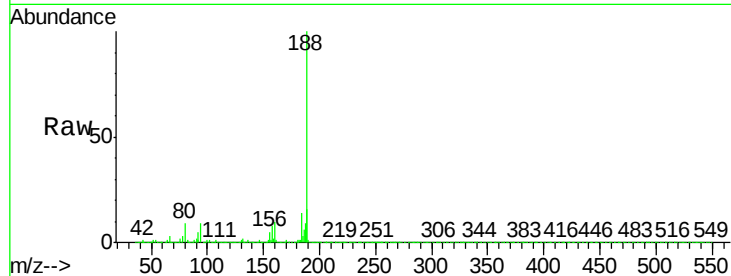

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BP0

Ion 80.00 (79.70 to 80.70): BP0

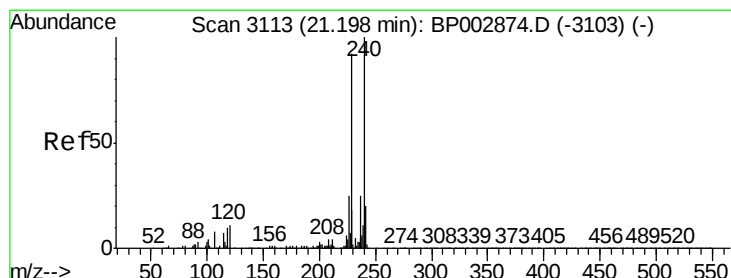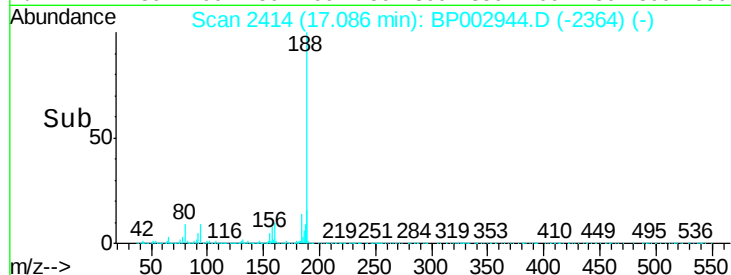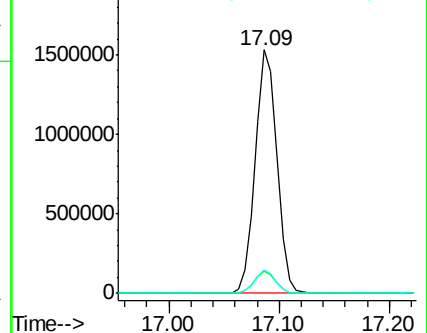

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.18 min Scan# 3110

Delta R.T. -0.00 min

Lab File: BP002944.D

Acq: 11 Aug 2020 18:27


Tgt Ion:240 Resp: 1597847

Ion Ratio Lower Upper

240 100

120 11.2 10.6 16.0



236 25.9 20.7 31.1

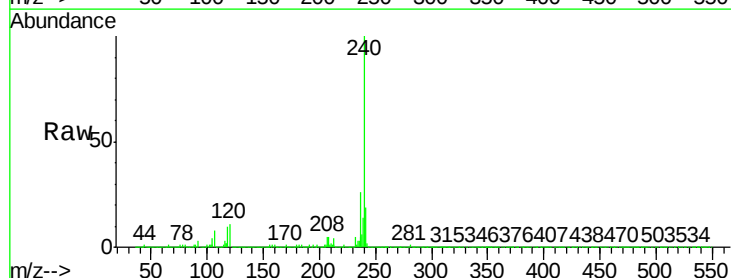


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

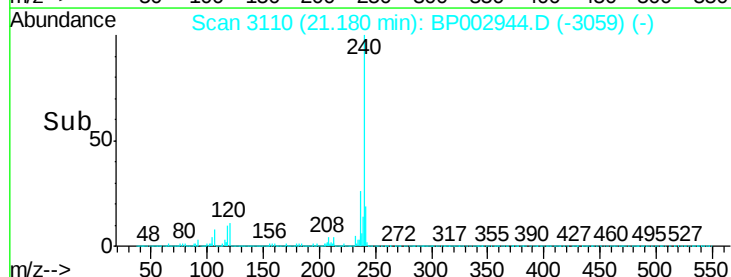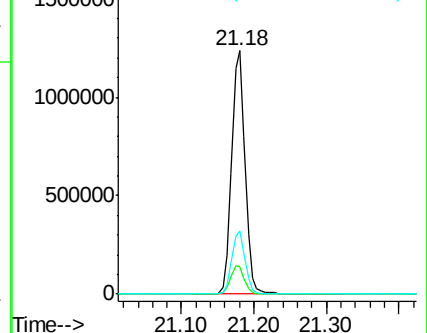

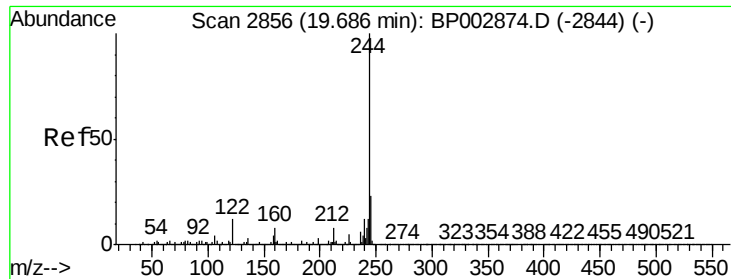

#79

Terphenyl-d14

Concen: 77.245 ng

RT: 19.66 min Scan# 2852

Delta R.T. -0.01 min

Lab File: BP002944.D

Acq: 11 Aug 2020 18:27

Instrument :

BNA_P

ClientSampleId :

SS-TP-1


Tot Ion:244 Resp: 6165251

Ion Ratio Lower Upper

244 100

212 7.7 6.3 9.5




122 13.3 9.9 14.9

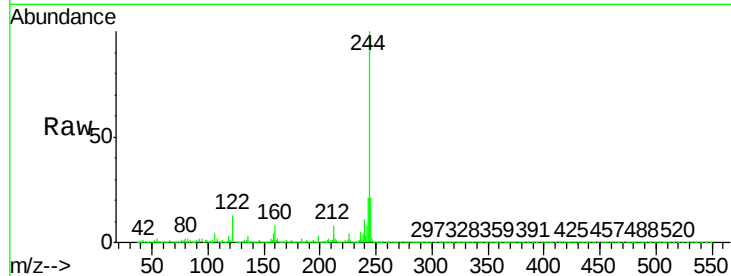

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

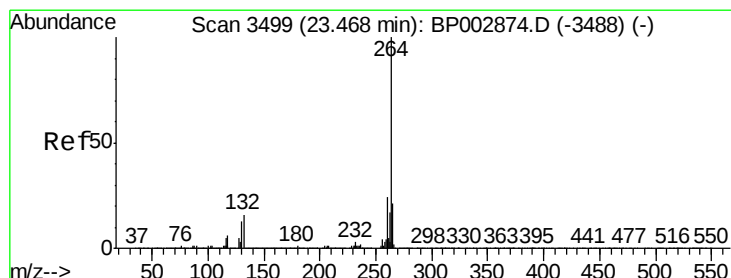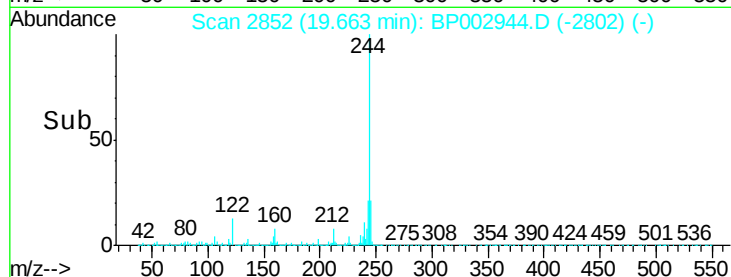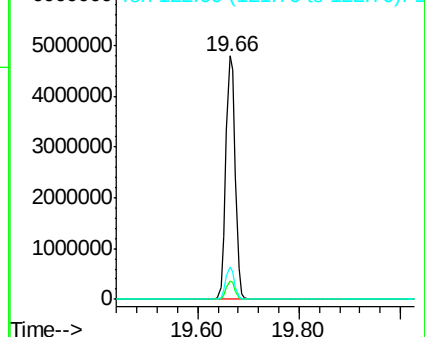

#86

Perylene-d12

Concen: 20.000 ng

RT: 23.43 min Scan# 3493

Delta R.T. -0.00 min

Lab File: BP002944.D

Acq: 11 Aug 2020 18:27


Tgt Ion:264 Resp: 1512437

Ion Ratio Lower Upper

264 100

260 23.7 18.7 28.1

265 21.9 17.6 26.4

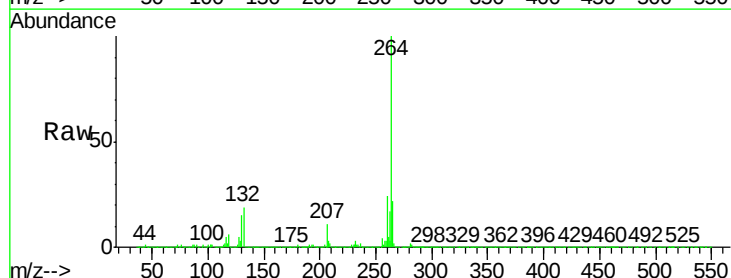

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

