




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011397.D
Acq On : 11 Aug 2022 21:23
Operator : CG/JU
Sample : PB146869BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK869

Manual IntegrationsAPPROVED

Quant Time: Aug 11 23:06:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 23:05:53 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/12/2022
Supervised By :Sohil Jodhani 08/13/2022

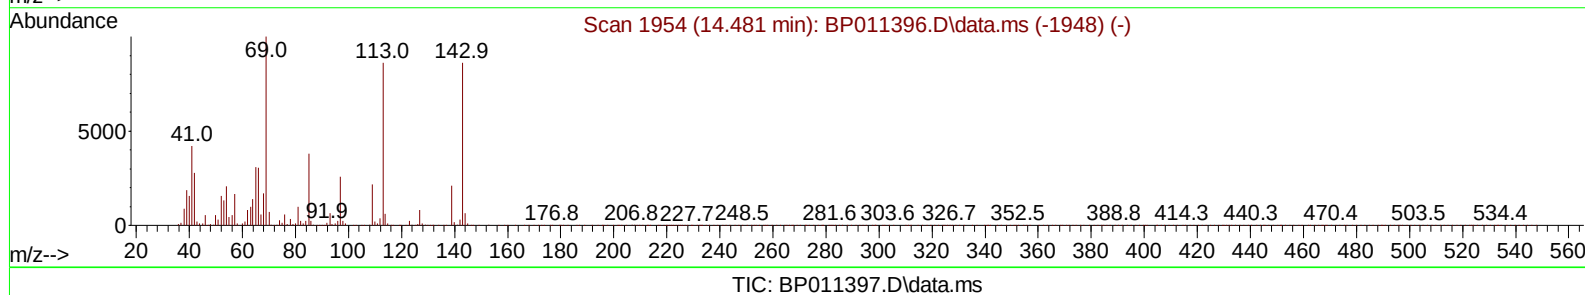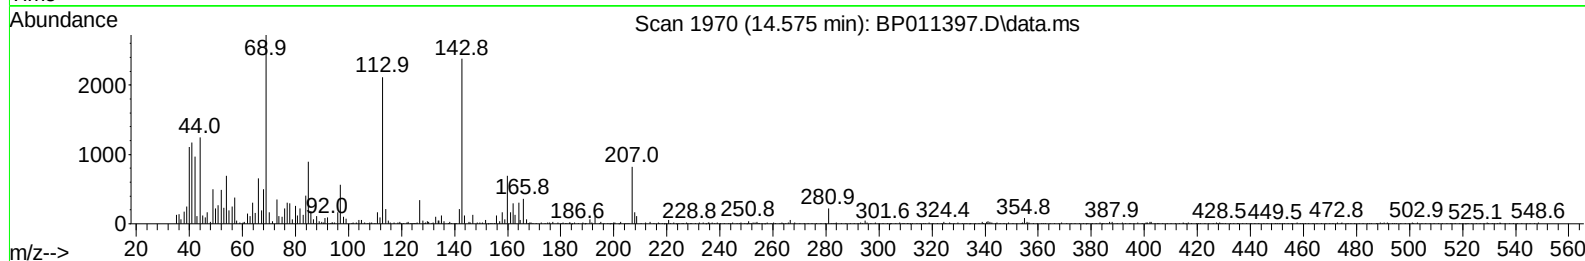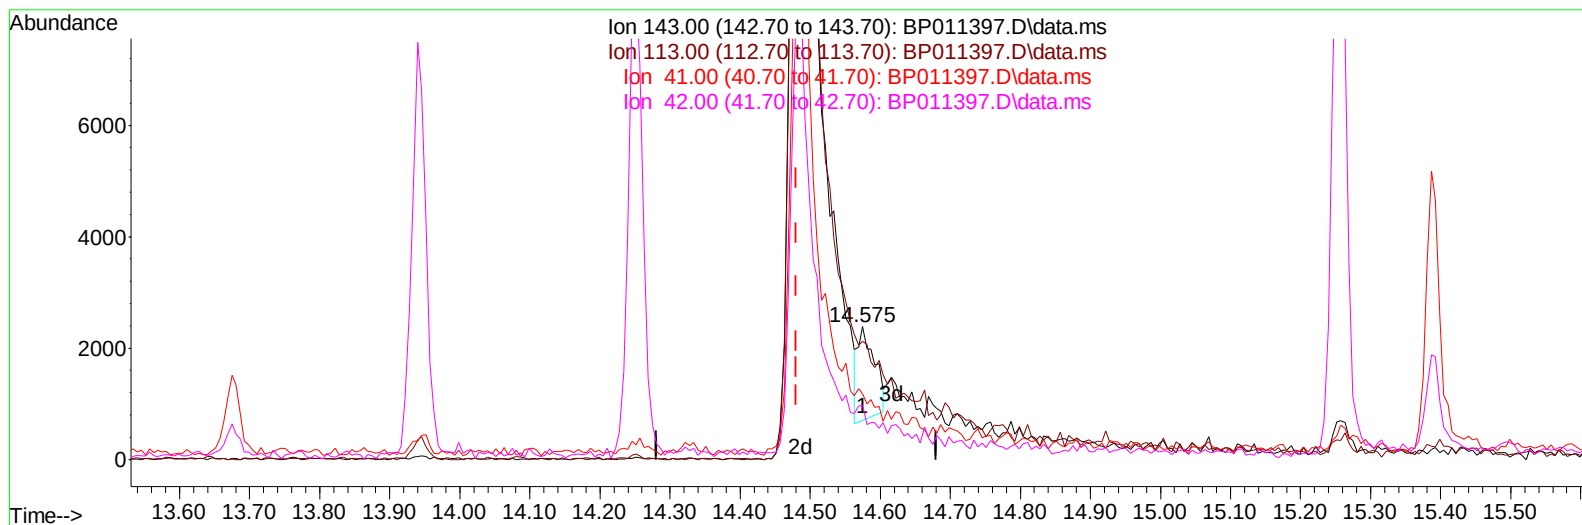

(54) 4-Nitrophenol-d4 (S)

14.575min (+ 0.094) 0.79 ng/ul

response 2753

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	75.70	88.80
41.00	54.40	49.33
42.00	35.50	40.60




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011397.D
Acq On : 11 Aug 2022 21:23
Operator : CG/JU
Sample : PB146869BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK869

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/12/2022
Supervised By :Sohil Jodhani 08/13/2022

Quant Time: Aug 11 23:06:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 23:05:53 2022
Response via : Initial Calibration

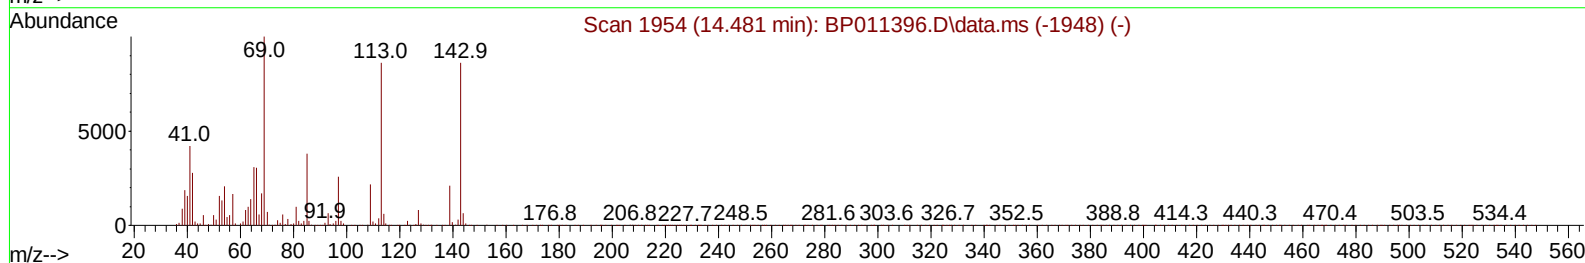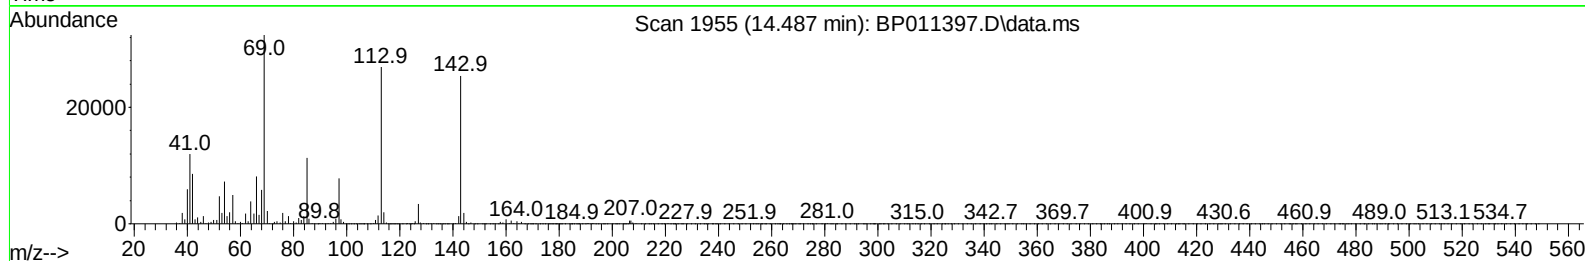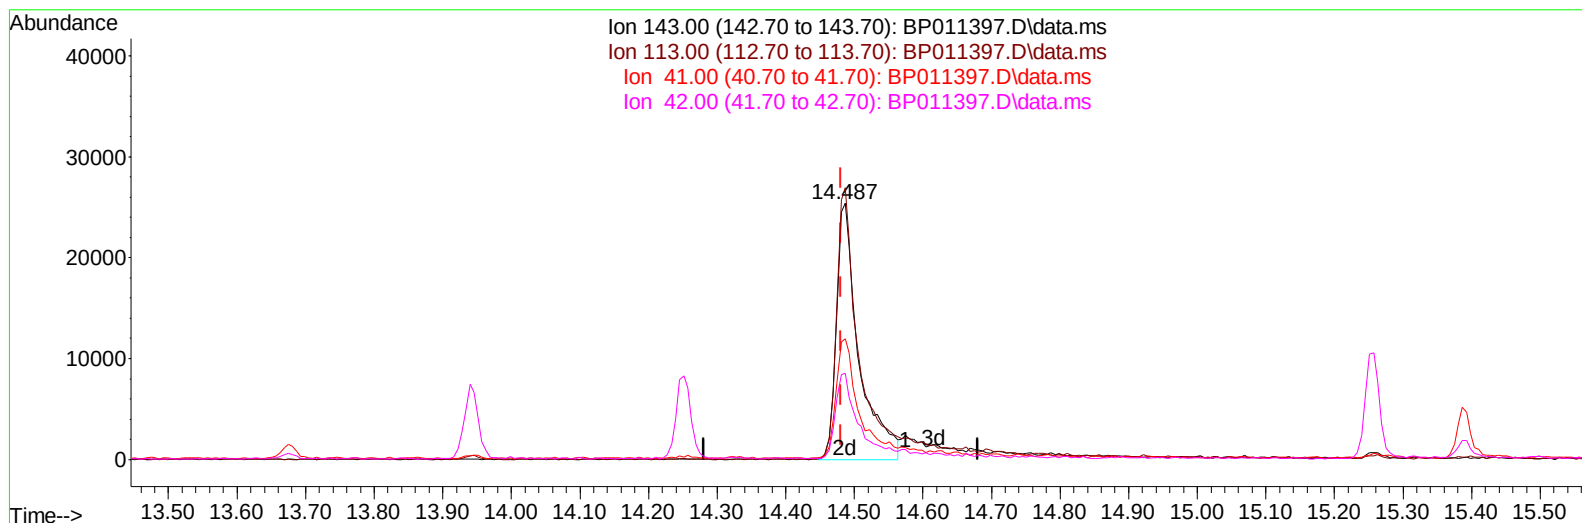

TIC: BP011397.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.487min (+ 0.006) 16.61 ng/ul m

response 57730

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	75.70	105.92#
41.00	54.40	47.04
42.00	35.50	33.60

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011397.D
 Acq On : 11 Aug 2022 21:23
 Operator : CG/JU
 Sample : PB146869BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK869

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/12/2022
 Supervised By :Sohil Jodhani 08/13/2022

Quant Time: Aug 11 23:06:42 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 11 23:05:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.575	152	114610	20.000	ng/ul	0.00
20) Naphthalene-d8	10.369	136	474118	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.251	164	274200	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.022	188	587872	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.151	240	610146	20.000	ng/ul	# 0.00
88) Perylene-d12	23.457	264	661222	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.081	96	17073	4.567	ng/uL	0.00
4) Pyridine-d5	3.493	84	204890	21.726	ng/ul	0.00
7) Phenol-d5	6.764	99	222696	21.956	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.928	67	153709	21.373	ng/ul	0.00
11) 2-Chlorophenol-d4	7.111	132	193751	24.346	ng/ul	0.00
15) 4-Methylphenol-d8	8.299	113	173678	21.808	ng/ul	0.00
21) Nitrobenzene-d5	8.746	128	85989	26.649	ng/ul	0.00
24) 2-Nitrophenol-d4	9.463	143	85954	29.095	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.993	165	143424	24.041	ng/ul	0.00
31) 4-Chloroaniline-d4	10.522	131	216294	20.738	ng/ul	0.00
46) Dimethylphthalate-d6	13.675	166	514814	27.059	ng/ul	0.00
49) Acenaphthylene-d8	13.940	160	578354	25.254	ng/ul	0.00
54) 4-Nitrophenol-d4	14.487	143	57730m	16.613	ng/ul	0.00
60) Fluorene-d10	15.257	176	420573	25.849	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.392	200	61370	22.475	ng/ul	0.00
73) Anthracene-d10	17.122	188	698583	26.438	ng/ul	0.00
81) Pyrene-d10	19.386	212	820936	24.422	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.310	264	846373	25.382	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011397.D
Acq On : 11 Aug 2022 21:23
Operator : CG/JU
Sample : PB146869BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK869

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/12/2022
Supervised By :Sohil Jodhani 08/13/2022

Quant Time: Aug 11 23:06:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 23:05:53 2022
Response via : Initial Calibration

