




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011399.D
Acq On : 11 Aug 2022 22:32
Operator : CG/JU
Sample : N4128-20
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGC08

Manual IntegrationsAPPROVED

Quant Time: Aug 11 23:28:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 23:05:53 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/12/2022
Supervised By :Sohil Jodhani 08/13/2022

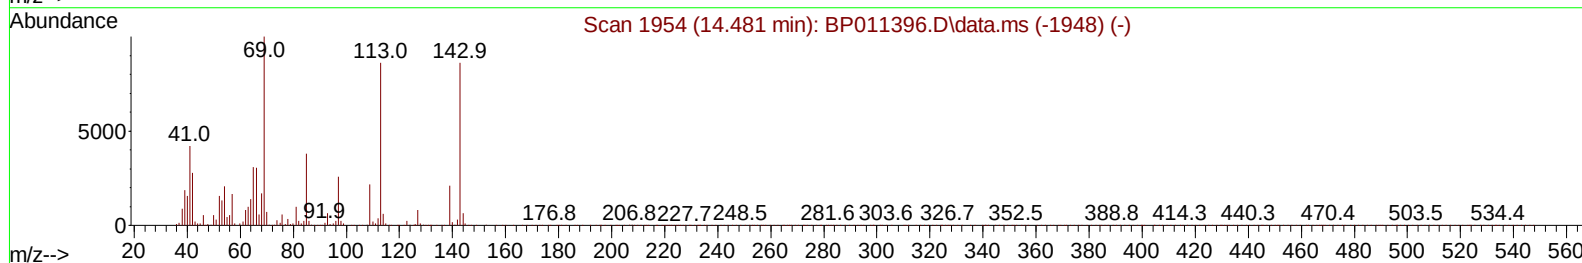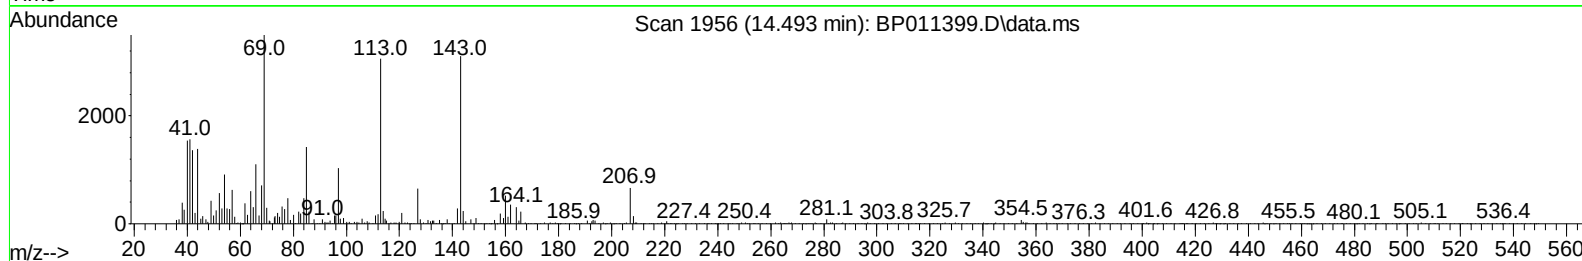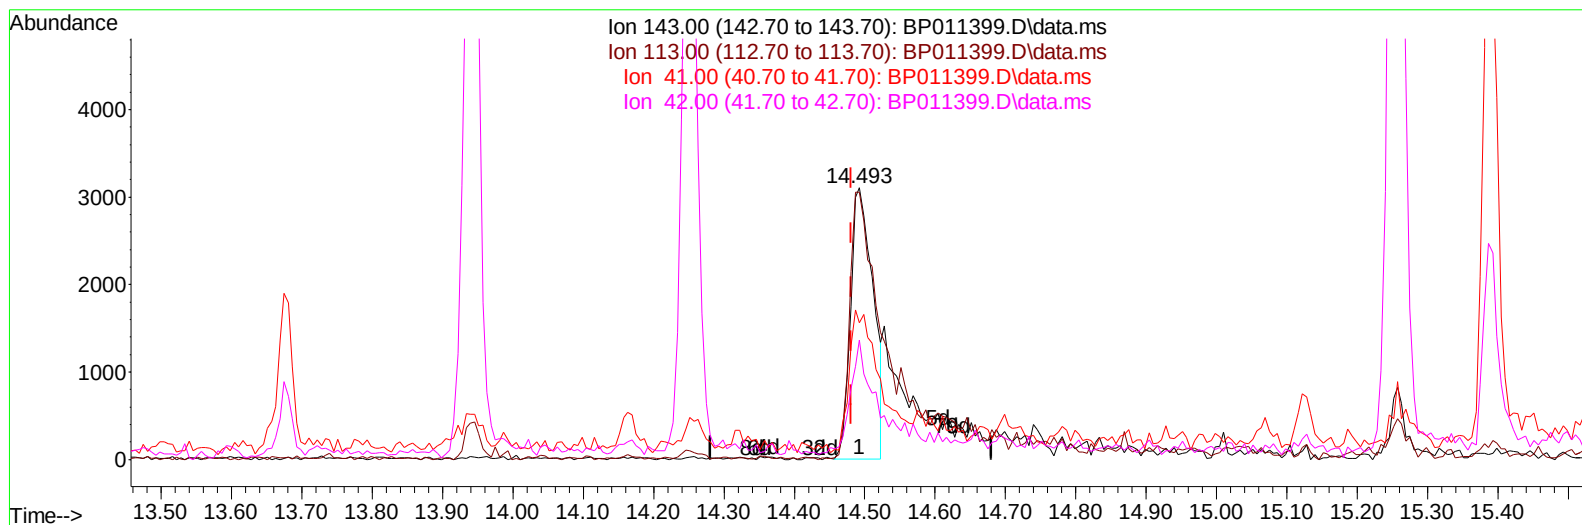

TIC: BP011399.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.493min (+ 0.012) 2.27 ng/ul

response 6830

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	75.70	98.52#
41.00	54.40	50.27
42.00	35.50	43.93#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011399.D
Acq On : 11 Aug 2022 22:32
Operator : CG/JU
Sample : N4128-20
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGC08

Manual IntegrationsAPPROVED

Quant Time: Aug 11 23:28:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 23:05:53 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/12/2022
Supervised By :Sohil Jodhani 08/13/2022

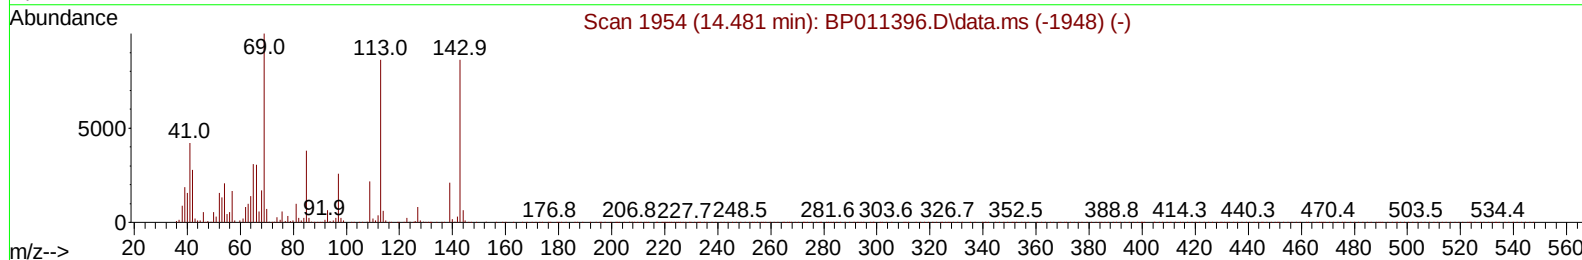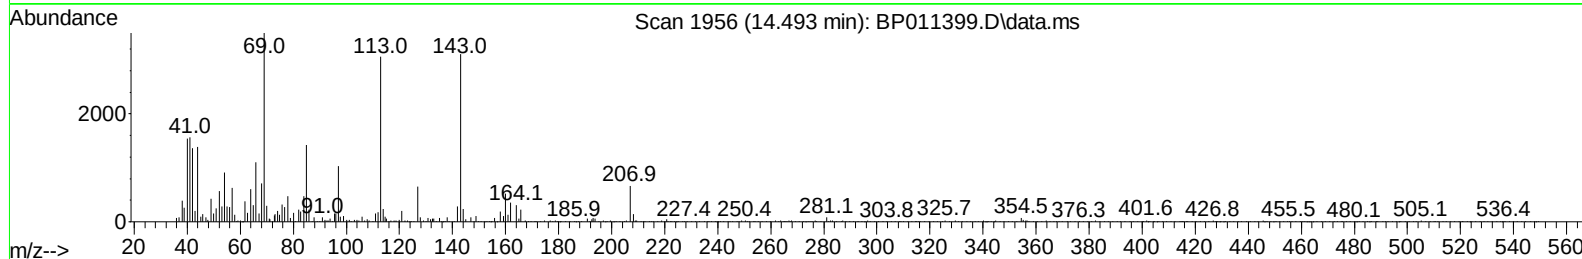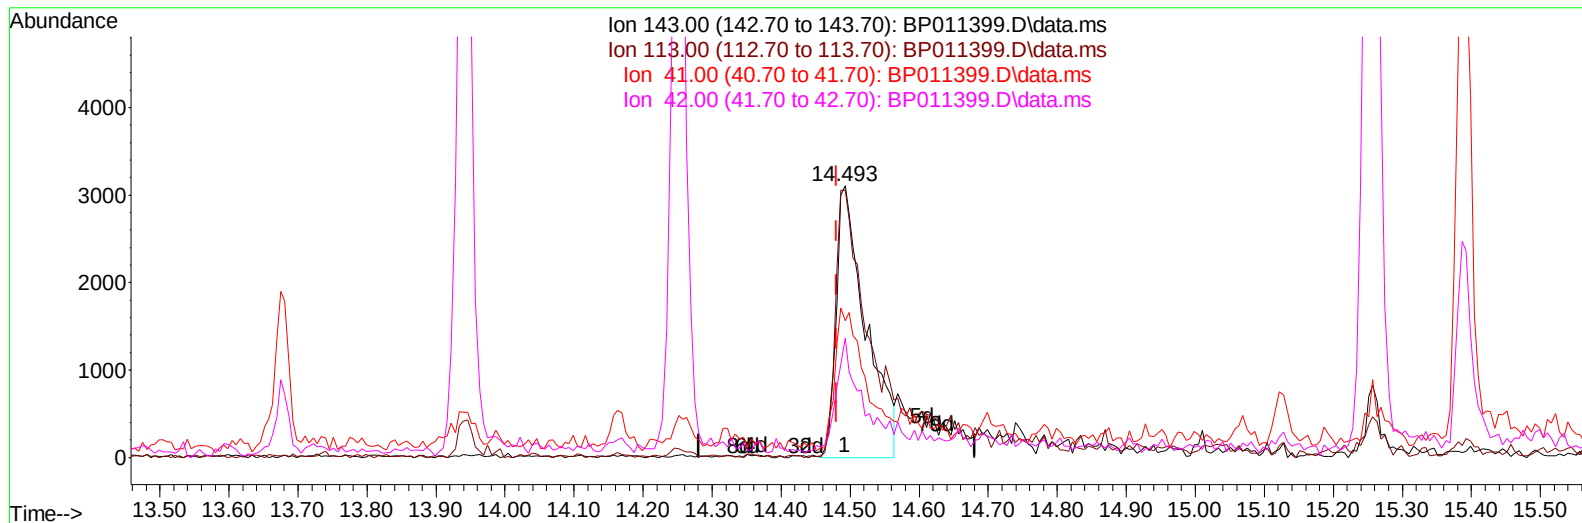

TIC: BP011399.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.493min (+ 0.012) 3.07 ng/ul m

response 9213

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	75.70	98.52#
41.00	54.40	50.27
42.00	35.50	43.93#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011399.D
 Acq On : 11 Aug 2022 22:32
 Operator : CG/JU
 Sample : N4128-20
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGC08

Manual IntegrationsAPPROVED

Quant Time: Aug 11 23:28:07 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 11 23:05:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/12/2022
 Supervised By :Sohil Jodhani 08/13/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.575	152	96946	20.000	ng/ul	0.00
20) Naphthalene-d8	10.369	136	397343	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.251	164	236919	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.022	188	513526	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.157	240	544743	20.000	ng/ul	# 0.00
88) Perylene-d12	23.463	264	602509	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.081	96	11731	3.710	ng/uL	0.00
4) Pyridine-d5	3.499	84	45537	5.708	ng/ul	0.01
7) Phenol-d5	6.764	99	46005	5.362	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.928	67	158084	25.987	ng/ul	0.00
11) 2-Chlorophenol-d4	7.111	132	150457	22.351	ng/ul	0.00
15) 4-Methylphenol-d8	8.299	113	87543	12.995	ng/ul	0.00
21) Nitrobenzene-d5	8.740	128	93612	34.617	ng/ul	0.00
24) 2-Nitrophenol-d4	9.463	143	89850	36.291	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.999	165	138104	27.622	ng/ul	0.00
31) 4-Chloroaniline-d4	10.522	131	187753	21.479	ng/ul	0.00
46) Dimethylphthalate-d6	13.675	166	580005	35.283	ng/ul	0.00
49) Acenaphthylene-d8	13.946	160	658486	33.277	ng/ul	0.00
54) 4-Nitrophenol-d4	14.493	143	9213m	3.068	ng/ul	0.01
60) Fluorene-d10	15.257	176	482192	34.299	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.393	200	79955	33.520	ng/ul	0.00
73) Anthracene-d10	17.128	188	916829	39.721	ng/ul	0.00
81) Pyrene-d10	19.386	212	1101677	36.708	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.316	264	1200209	39.500	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011399.D
Acq On : 11 Aug 2022 22:32
Operator : CG/JU
Sample : N4128-20
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGC08

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/12/2022
Supervised By :Sohil Jodhani 08/13/2022

Quant Time: Aug 11 23:28:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 23:05:53 2022
Response via : Initial Calibration

