




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011403.D
 Acq On : 12 Aug 2022 00:50
 Operator : CG/JU
 Sample : N4128-06
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBX2

Manual IntegrationsAPPROVED

Quant Time: Aug 12 01:43:32 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 11 23:05:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/12/2022
 Supervised By :Sohil Jodhani 08/13/2022

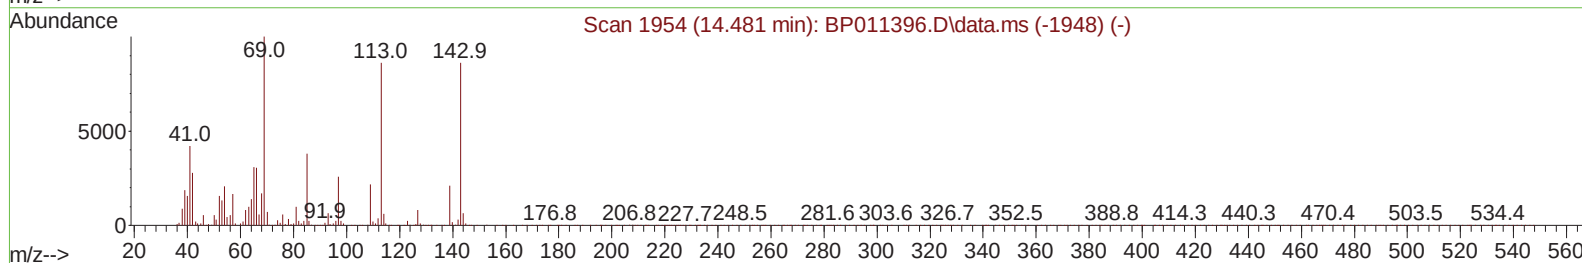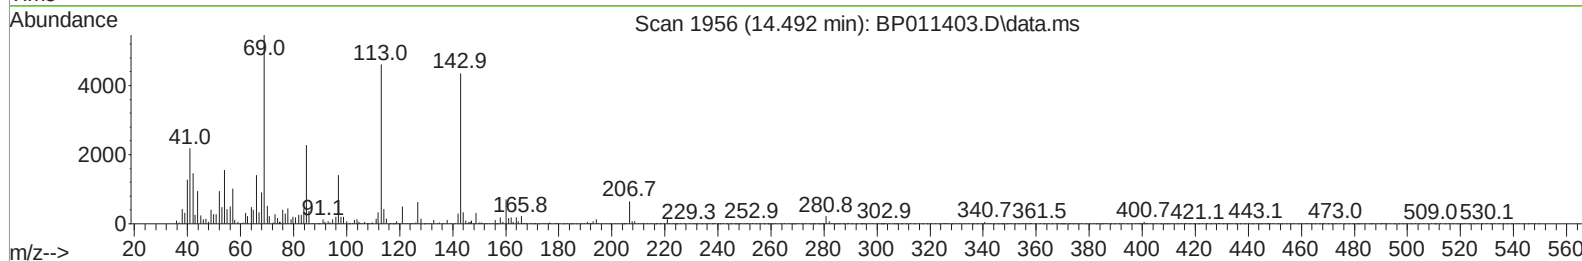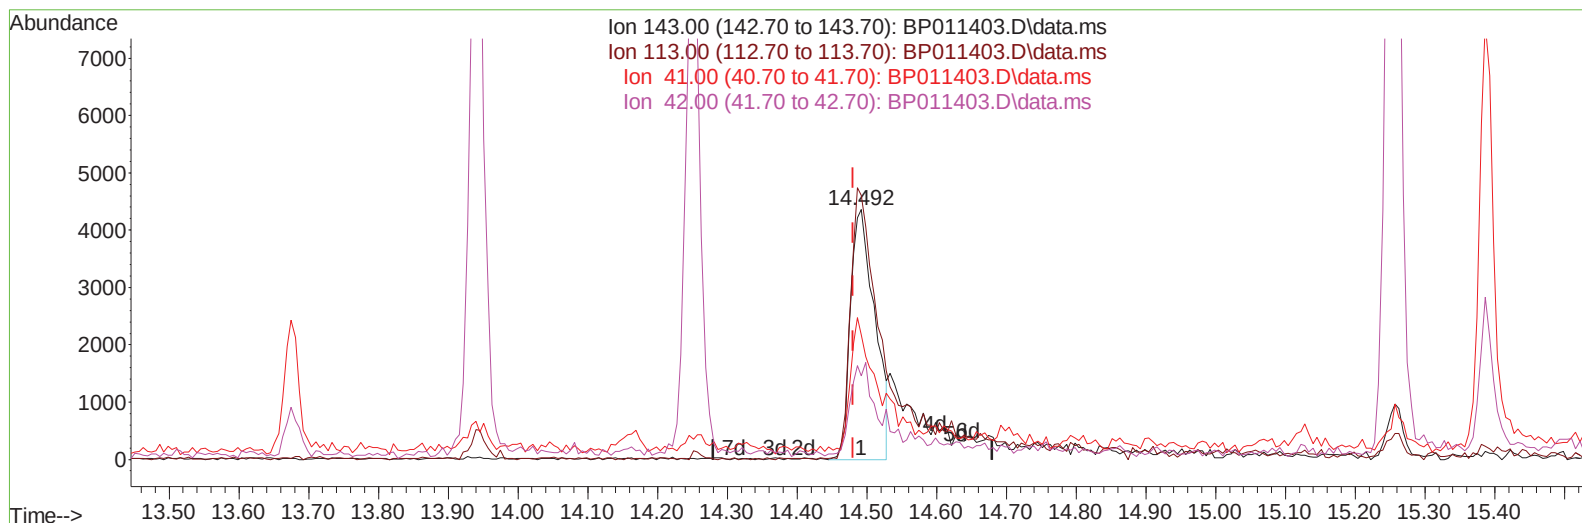

TIC: BP011403.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.492min (+ 0.012) 3.05 ng/ul

response 10551

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	75.70	105.69#
41.00	54.40	49.92
42.00	35.50	33.56




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011403.D
Acq On : 12 Aug 2022 00:50
Operator : CG/JU
Sample : N4128-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBX2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/12/2022
Supervised By :Sohil Jodhani 08/13/2022

Quant Time: Aug 12 01:43:32 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 23:05:53 2022
Response via : Initial Calibration

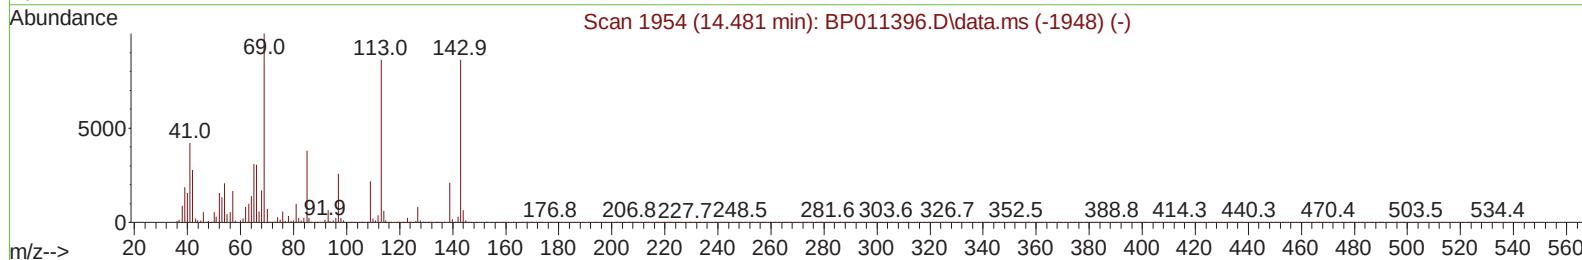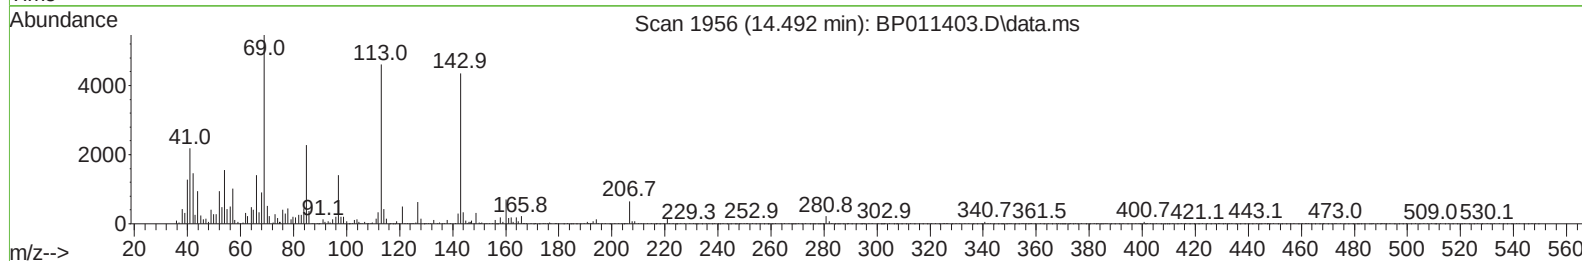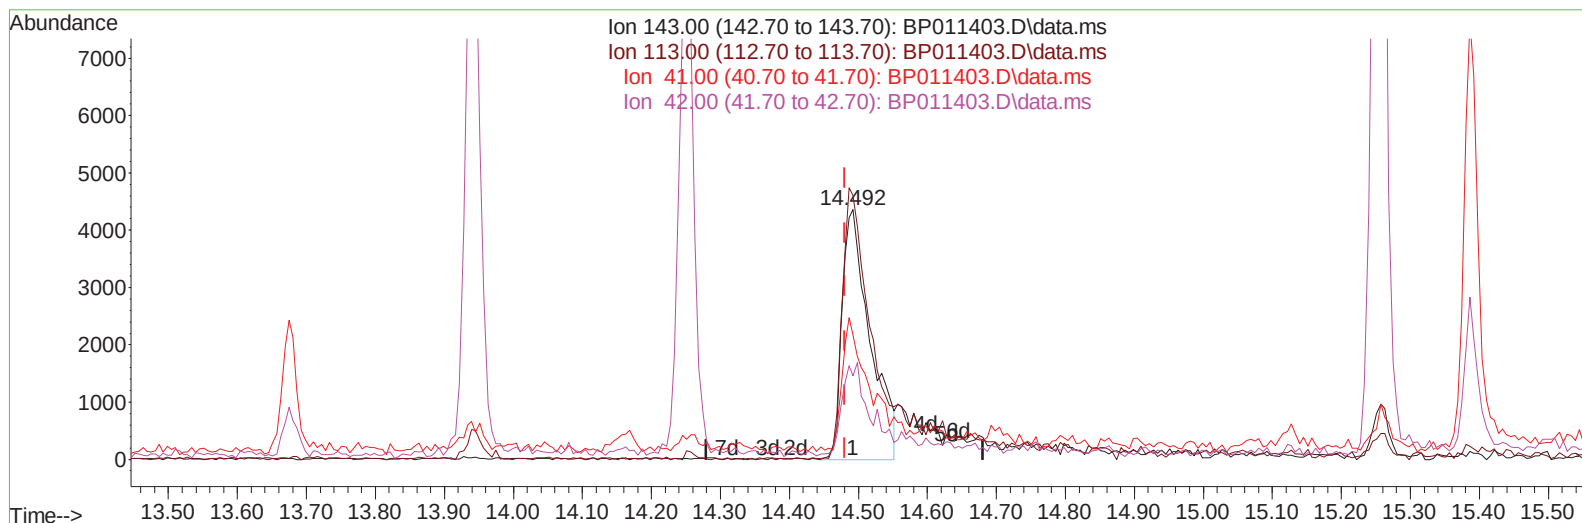

TIC: BP011403.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.492min (+ 0.012) 3.54 ng/ul m

response 12228

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	75.70	105.69#
41.00	54.40	49.92
42.00	35.50	33.56

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011403.D
 Acq On : 12 Aug 2022 00:50
 Operator : CG/JU
 Sample : N4128-06
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBX2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/12/2022
 Supervised By :Sohil Jodhani 08/13/2022

Quant Time: Aug 12 01:43:32 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 11 23:05:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.575	152	110576	20.000	ng/ul	0.00
20) Naphthalene-d8	10.369	136	458673	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.251	164	272593	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.022	188	581343	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.157	240	634785	20.000	ng/ul	# 0.00
88) Perylene-d12	23.462	264	717330	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.081	96	15140	4.197	ng/uL	0.00
4) Pyridine-d5	3.499	84	35070	3.854	ng/ul	0.01
7) Phenol-d5	6.763	99	68615	7.012	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.922	67	208349	30.028	ng/ul	0.00
11) 2-Chlorophenol-d4	7.110	132	202243	26.340	ng/ul	0.00
15) 4-Methylphenol-d8	8.299	113	127790	16.632	ng/ul	0.00
21) Nitrobenzene-d5	8.740	128	120895	38.728	ng/ul	0.00
24) 2-Nitrophenol-d4	9.457	143	117939	41.267	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.993	165	190334	32.978	ng/ul	0.00
31) 4-Chloroaniline-d4	10.522	131	241322	23.916	ng/ul	0.00
46) Dimethylphthalate-d6	13.675	166	737652	39.001	ng/ul	0.00
49) Acenaphthylene-d8	13.939	160	849821	37.326	ng/ul	0.00
54) 4-Nitrophenol-d4	14.492	143	12228m	3.540	ng/ul	0.01
60) Fluorene-d10	15.257	176	604570	37.377	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.386	200	90030	33.341	ng/ul	0.00
73) Anthracene-d10	17.122	188	1014252	38.815	ng/ul	0.00
81) Pyrene-d10	19.386	212	1244849	35.595	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.315	264	1402546	38.771	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011403.D
Acq On : 12 Aug 2022 00:50
Operator : CG/JU
Sample : N4128-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBX2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/12/2022
Supervised By :Sohil Jodhani 08/13/2022

Quant Time: Aug 12 01:43:32 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 23:05:53 2022
Response via : Initial Calibration

