

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011424.D
 Acq On : 12 Aug 2022 14:39
 Operator : CG/JU
 Sample : N4129-15
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBW7

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/12/2022
 Supervised By :Sohil Jodhani 08/13/2022

Quant Time: Aug 12 15:08:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 11 23:05:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.575	152	89682	20.000	ng/ul	0.00
20) Naphthalene-d8	10.363	136	382095	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.251	164	218501	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.022	188	456197	20.000	ng/ul	0.00
79) Chrysene-d12	21.157	240	445767	20.000	ng/ul	0.00
88) Perylene-d12	23.463	264	472591	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.081	96	10784m	3.686	ng/uL	0.00
4) Pyridine-d5	3.499	84	48486	6.570	ng/ul	0.01
7) Phenol-d5	6.758	99	41189	5.190	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.922	67	150940	26.822	ng/ul	0.00
11) 2-Chlorophenol-d4	7.105	132	134339	21.573	ng/ul	0.00
15) 4-Methylphenol-d8	8.293	113	78682	12.626	ng/ul	-0.01
21) Nitrobenzene-d5	8.740	128	83971	32.291	ng/ul	0.00
24) 2-Nitrophenol-d4	9.458	143	78312	32.893	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.993	165	125457	26.093	ng/ul	0.00
31) 4-Chloroaniline-d4	10.516	131	170148	20.242	ng/ul	0.00
46) Dimethylphthalate-d6	13.675	166	517830	34.156	ng/ul	0.00
49) Acenaphthylene-d8	13.940	160	575127	31.514	ng/ul	0.00
54) 4-Nitrophenol-d4	14.493	143	7330m	2.647	ng/ul	0.01
60) Fluorene-d10	15.257	176	421038	32.474	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.387	200	64286	30.338	ng/ul	0.00
73) Anthracene-d10	17.122	188	749966	36.575	ng/ul	0.00
81) Pyrene-d10	19.386	212	872229	35.516	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.316	264	850365	35.680	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011424.D
Acq On : 12 Aug 2022 14:39
Operator : CG/JU
Sample : N4129-15
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBW7

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 08/12/2022
Supervised By :Sohil Jodhani 08/13/2022

Quant Time: Aug 12 15:08:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 23:05:53 2022
Response via : Initial Calibration

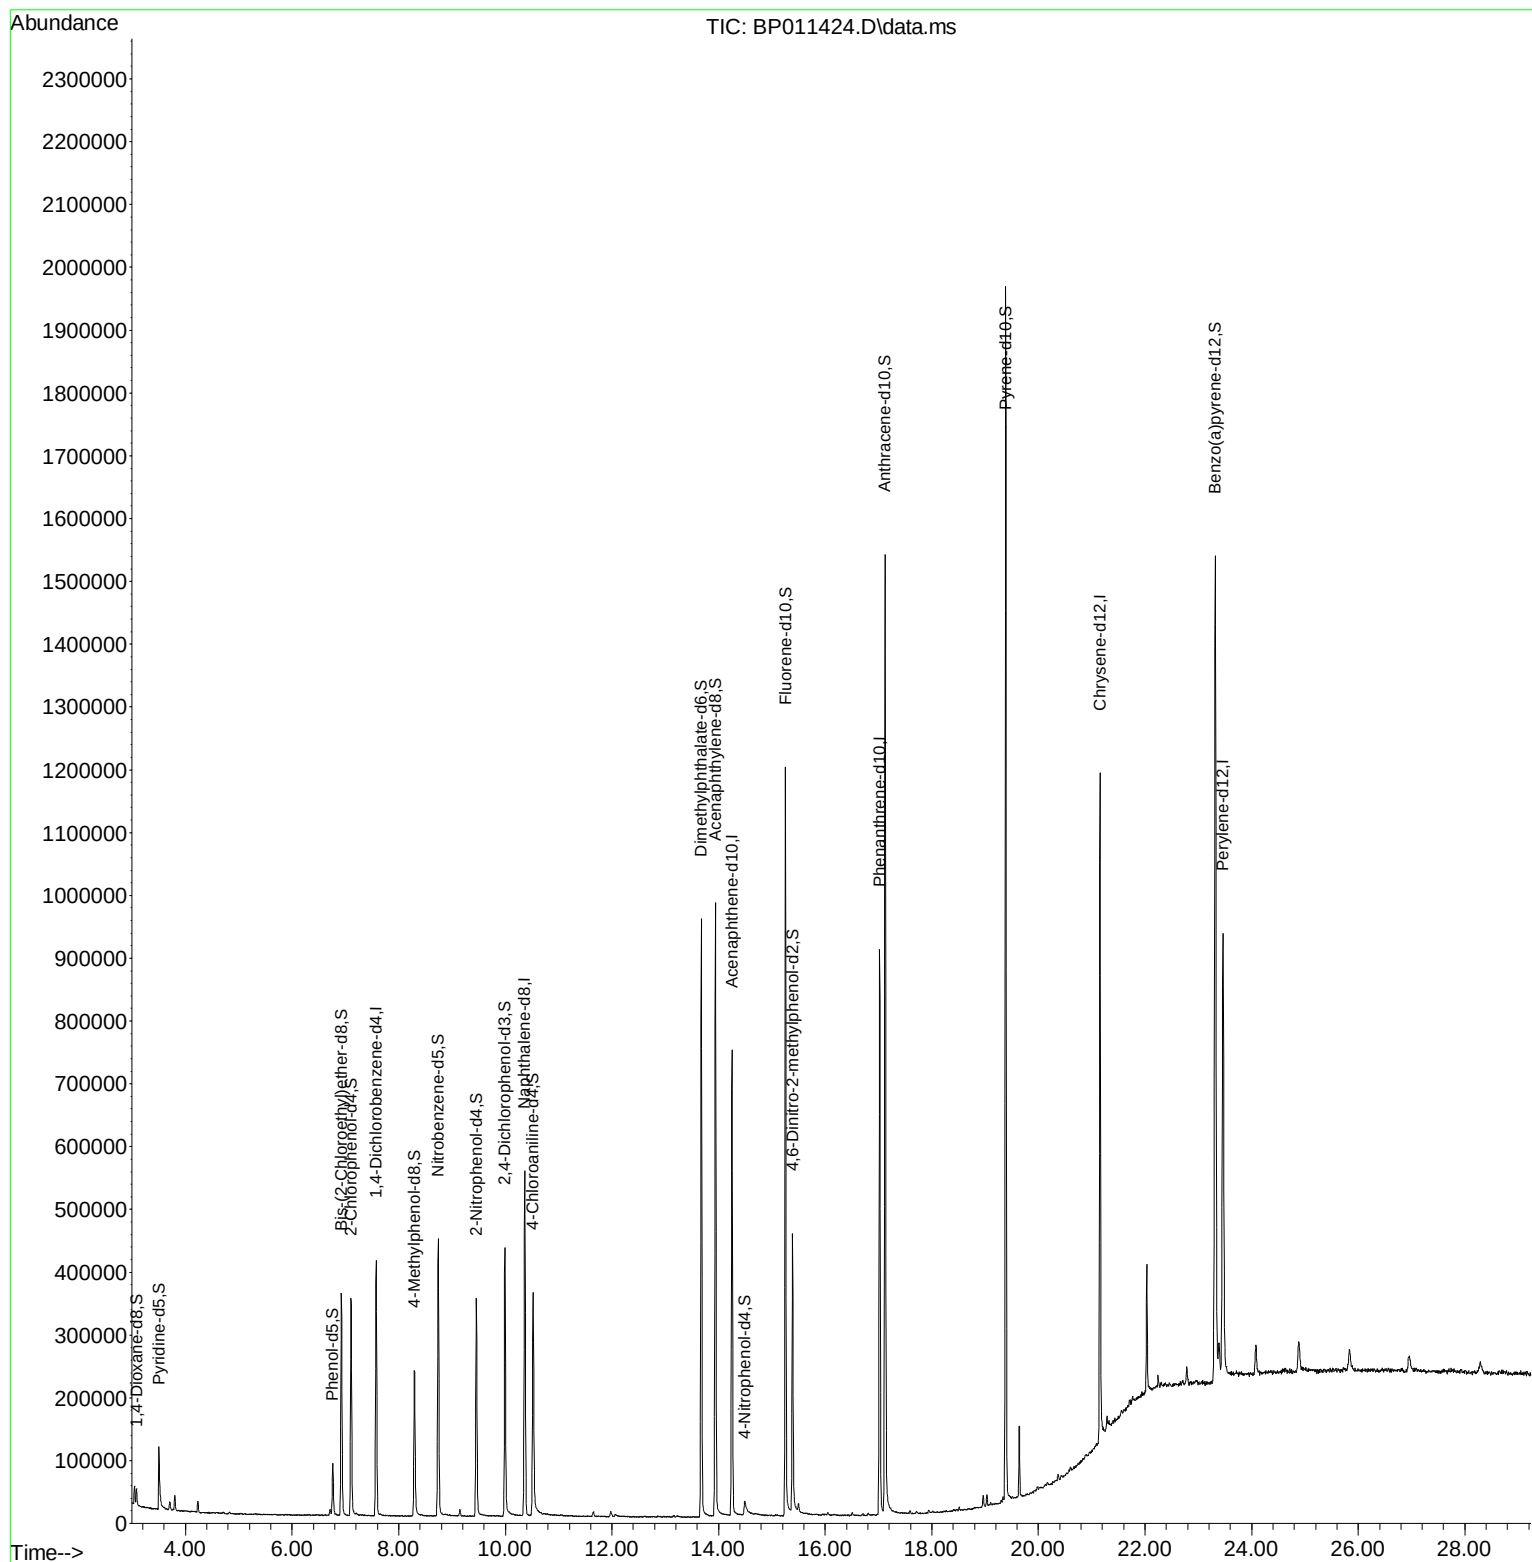




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011424.D
 Acq On : 12 Aug 2022 14:39
 Operator : CG/JU
 Sample : N4129-15
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBW7

Manual IntegrationsAPPROVED

Quant Time: Aug 12 15:08:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 11 23:05:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/12/2022
 Supervised By :Sohil Jodhani 08/13/2022

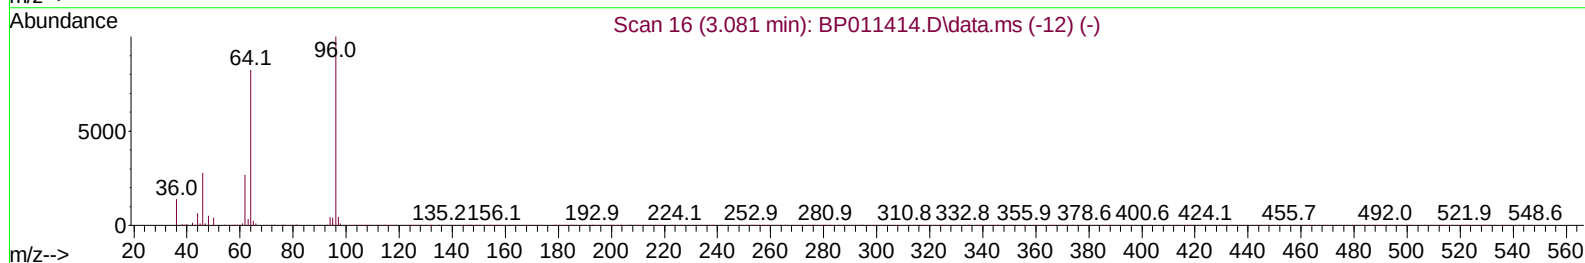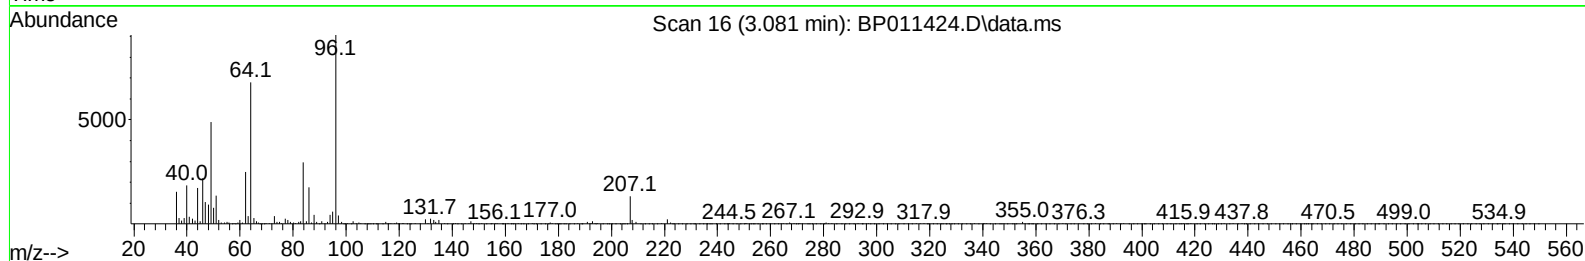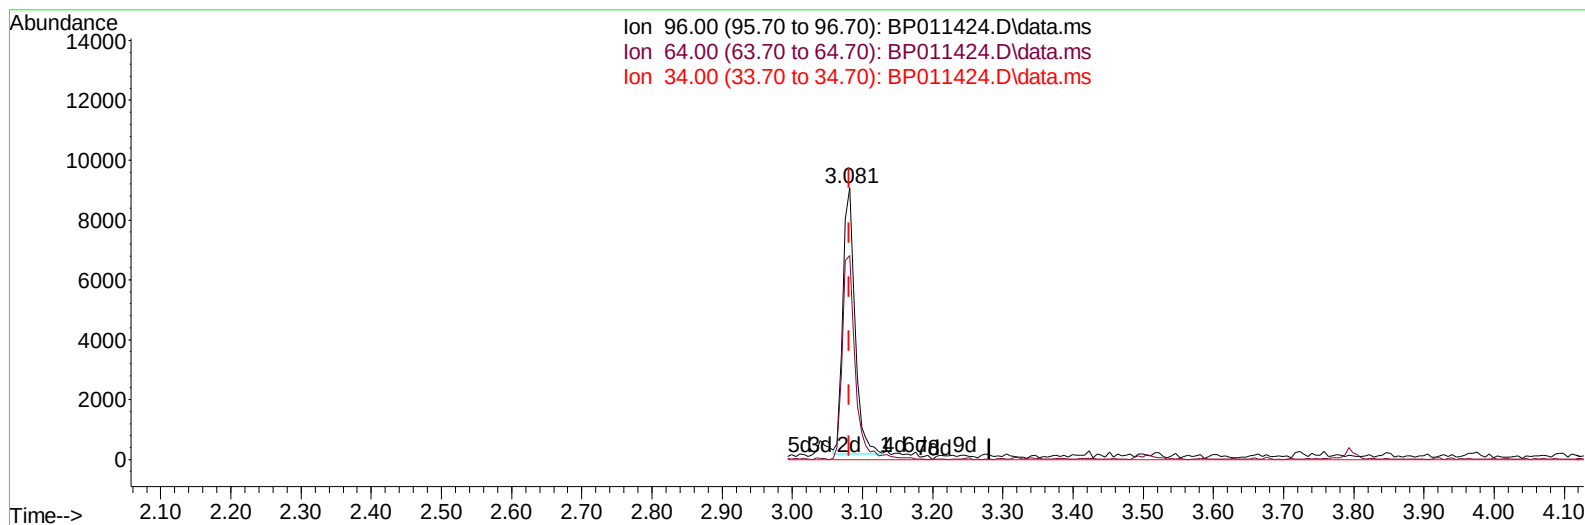

TIC: BP011424.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.081min (+ 0.000) 3.69 ng/uL m

response 10784

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	61.00	75.04#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011424.D
Acq On : 12 Aug 2022 14:39
Operator : CG/JU
Sample : N4129-15
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBW7

Manual IntegrationsAPPROVED

Quant Time: Aug 12 15:08:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 23:05:53 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/12/2022
Supervised By :Sohil Jodhani 08/13/2022

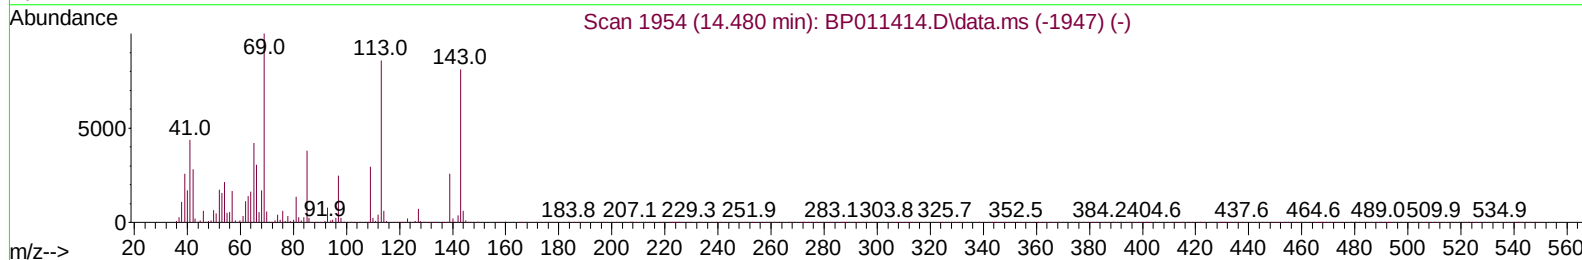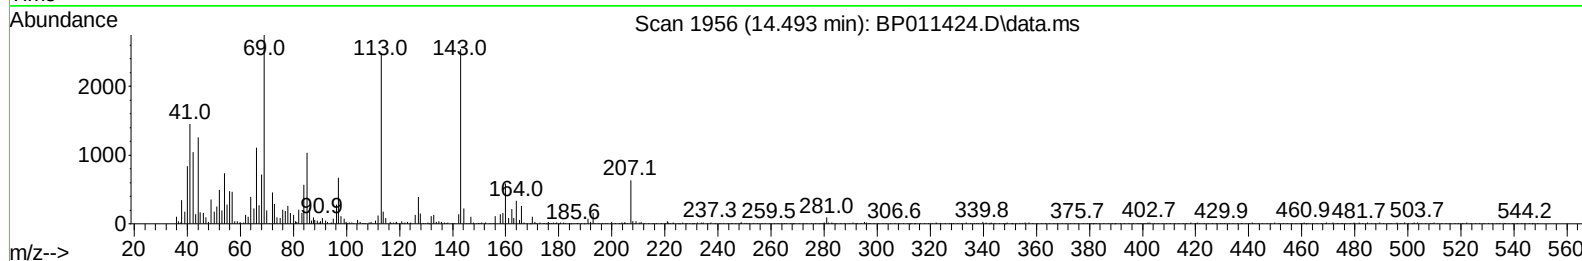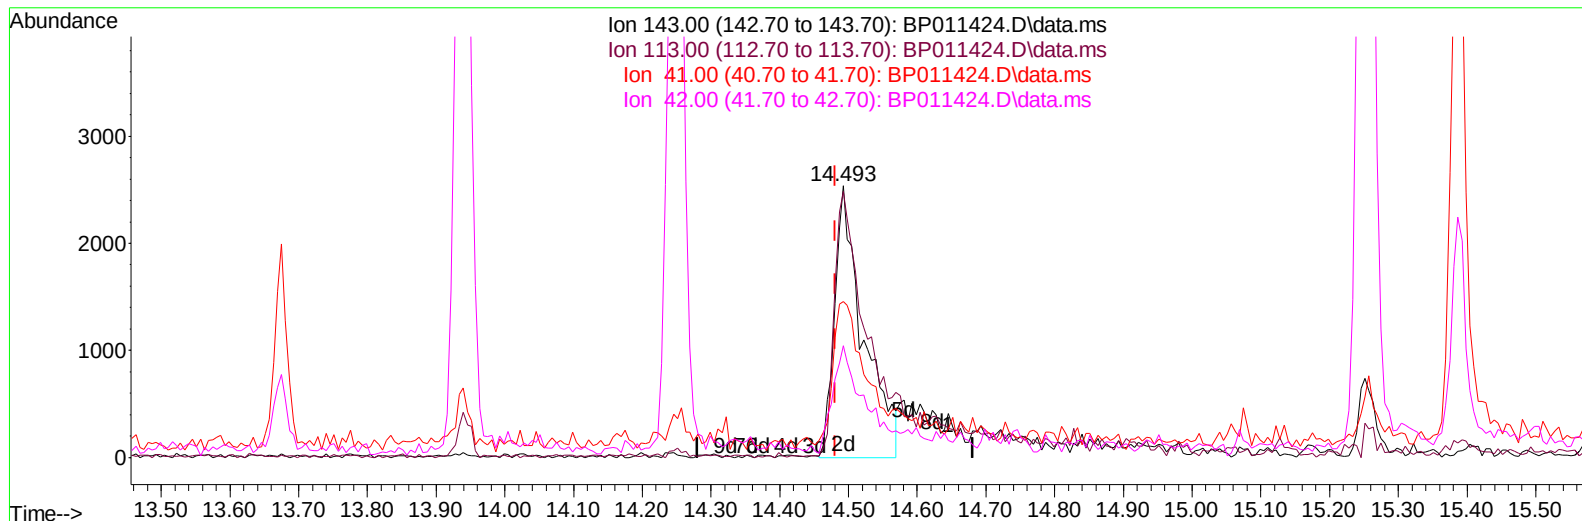

TIC: BP011424.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.493min (+ 0.012) 2.65 ng/ul m

response 7330

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	75.70	97.91#
41.00	54.40	57.37
42.00	35.50	41.05




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011424.D
 Acq On : 12 Aug 2022 14:39
 Operator : CG/JU
 Sample : N4129-15
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBW7

Manual IntegrationsAPPROVED

Quant Time: Aug 14 05:24:30 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 11 23:05:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/12/2022
 Supervised By :Sohil Jodhani 08/13/2022

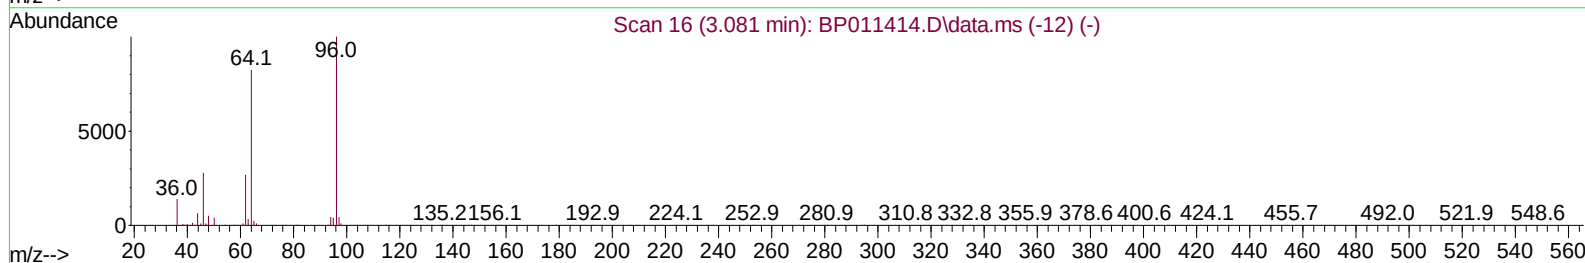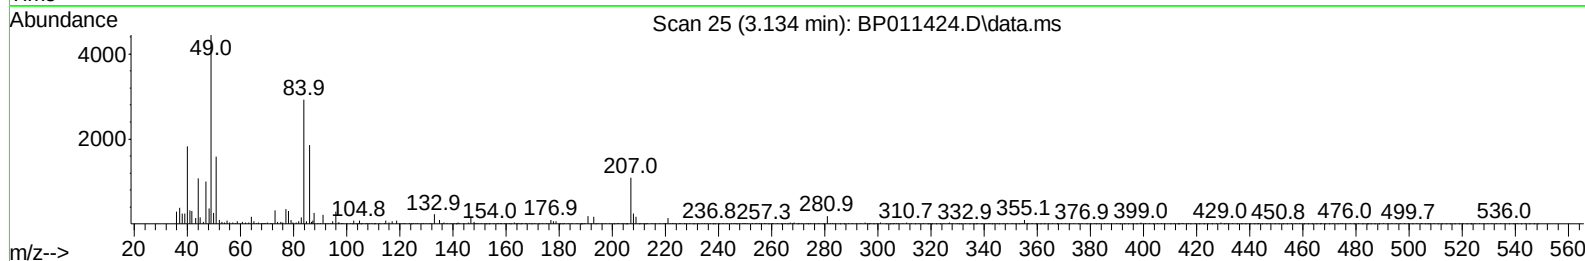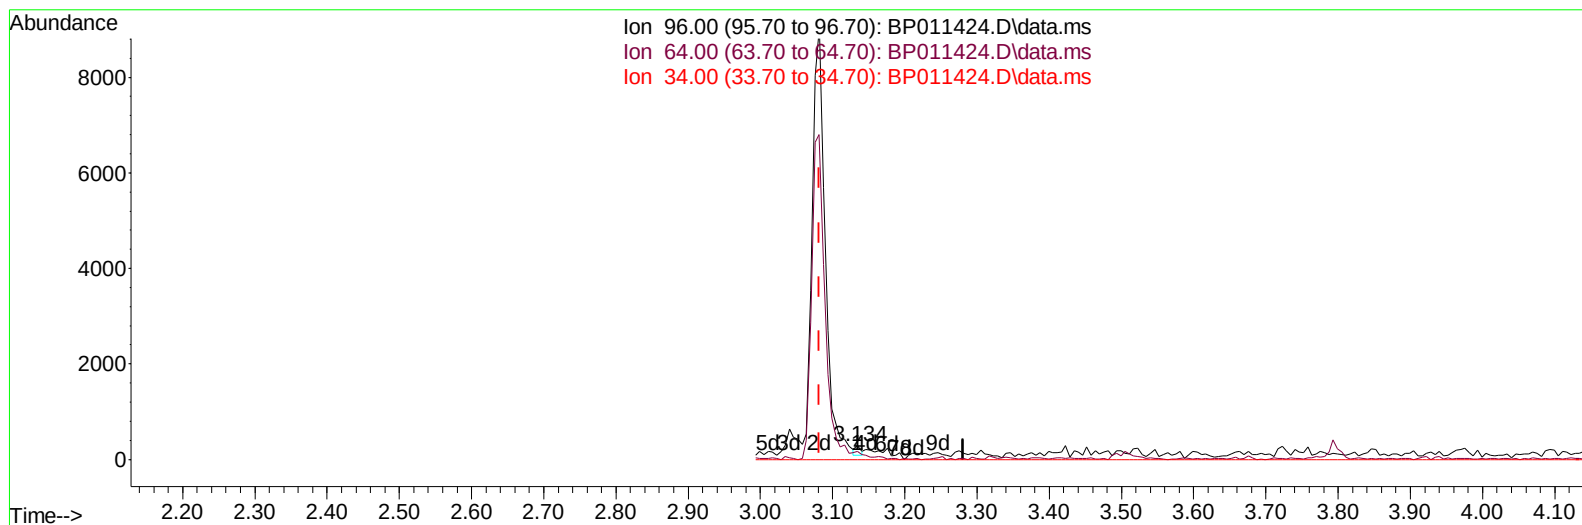

TIC: BP011424.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.134min (+ 0.053) 0.03 ng/uL

response	101	
Ion	Exp%	Act%
96.00	100.00	100.00
64.00	61.00	55.93
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011424.D
 Acq On : 12 Aug 2022 14:39
 Operator : CG/JU
 Sample : N4129-15
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBW7

Manual IntegrationsAPPROVED

Quant Time: Aug 14 05:24:30 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 11 23:05:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 08/12/2022
 Supervised By :Sohil Jodhani 08/13/2022

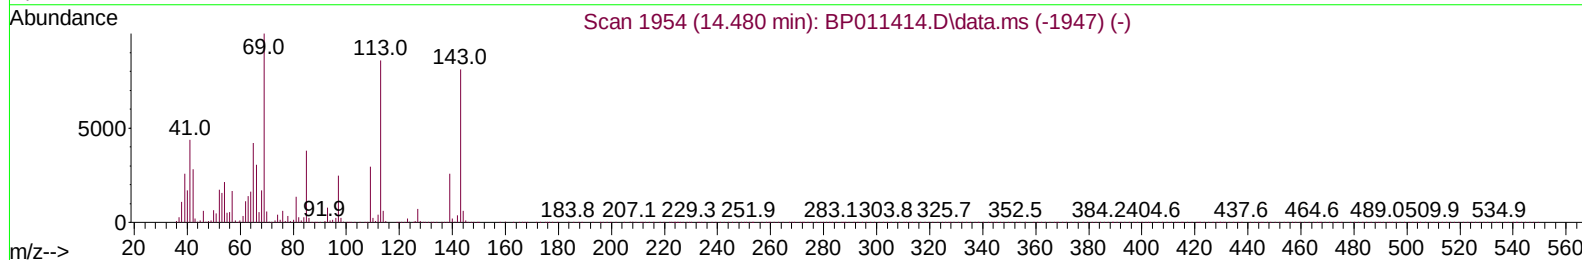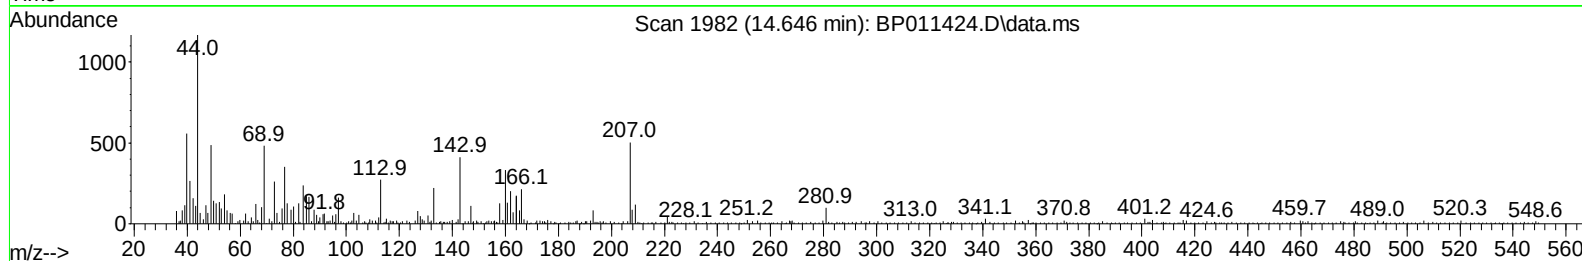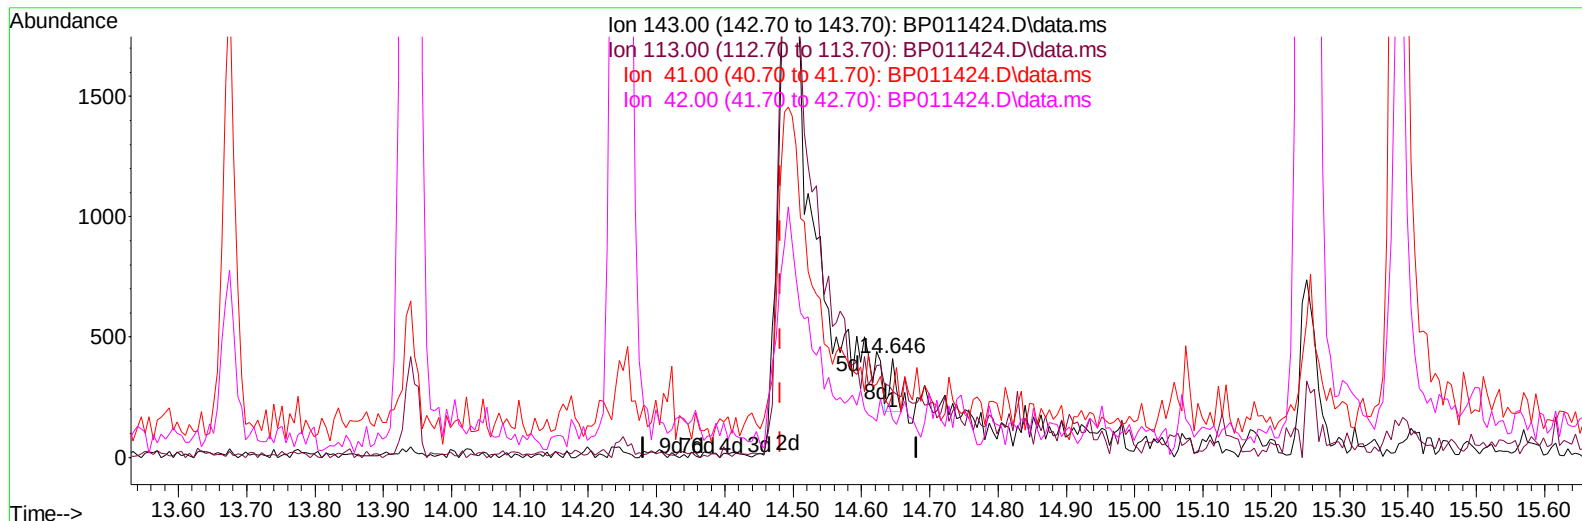

TIC: BP011424.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.646min (+ 0.165) 0.05 ng/ul

response 134

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	75.70	66.50
41.00	54.40	64.32
42.00	35.50	38.59