




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011425.D
 Acq On : 12 Aug 2022 15:14
 Operator : CG/JU
 Sample : PB146917BS
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLCS917

Manual IntegrationsAPPROVED

Quant Time: Aug 12 17:40:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 11 23:05:53 2022
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/13/2022
 Supervised By :Sohil Jodhani 08/13/2022

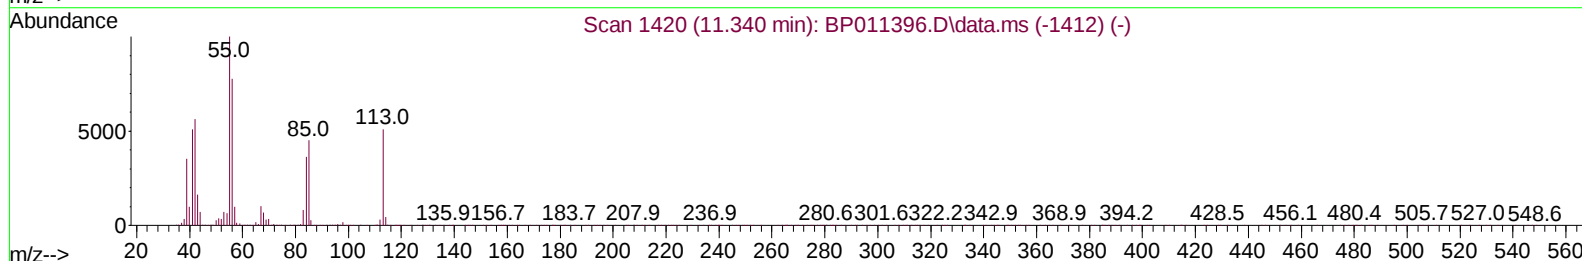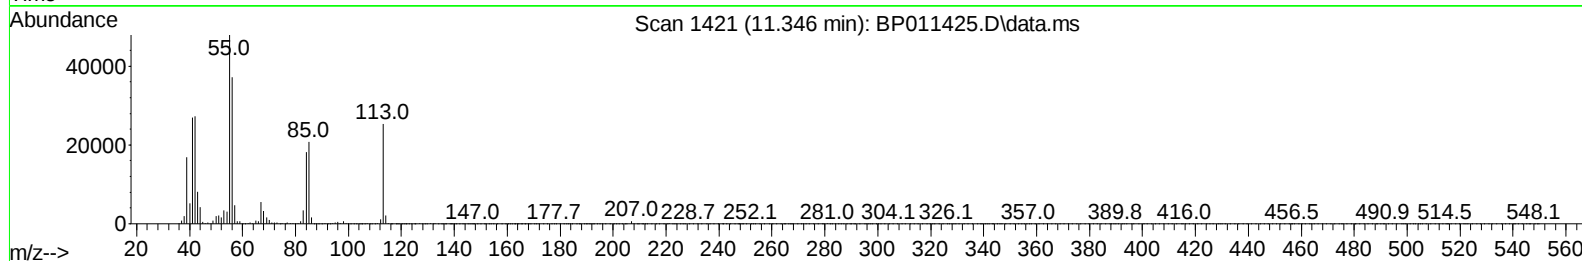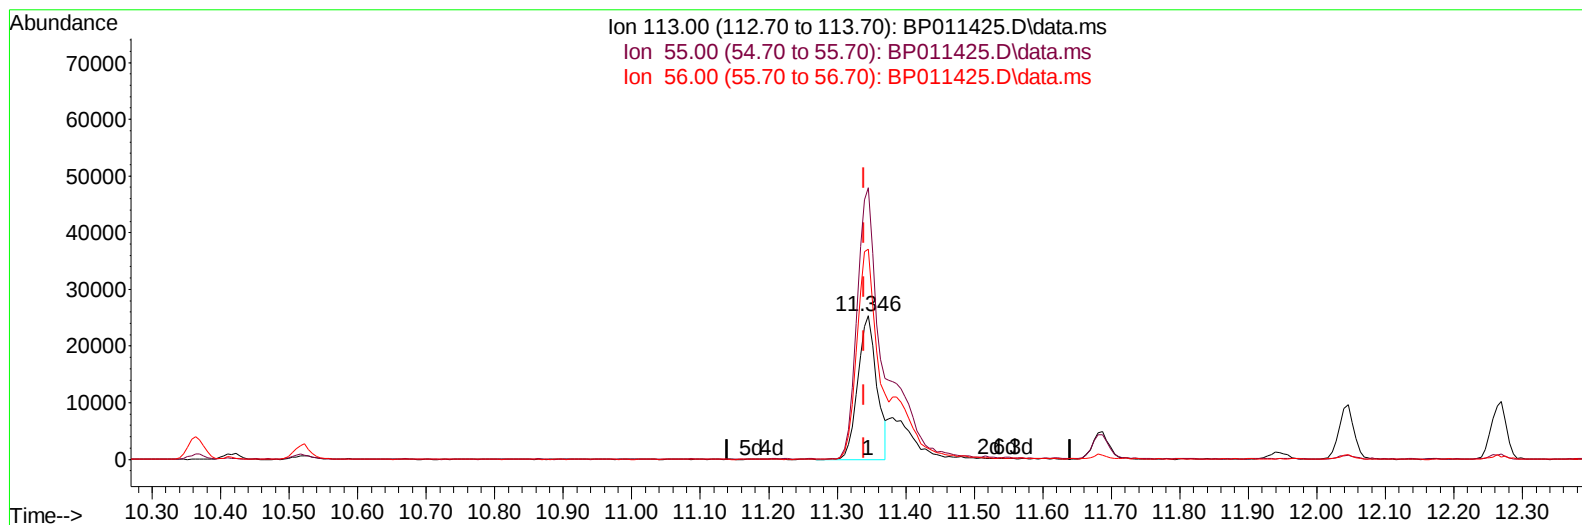

TIC: BP011425.D\data.ms

(34) Caprolactam

11.346min (+ 0.006) 25.56 ng/ul

response 48364

Ion	Exp%	Act%
113.00	100.00	100.00
55.00	205.30	188.75
56.00	158.80	146.41
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011425.D
 Acq On : 12 Aug 2022 15:14
 Operator : CG/JU
 Sample : PB146917BS
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLCS917

Manual IntegrationsAPPROVED

Quant Time: Aug 12 17:40:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 11 23:05:53 2022
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/13/2022
 Supervised By :Sohil Jodhani 08/13/2022

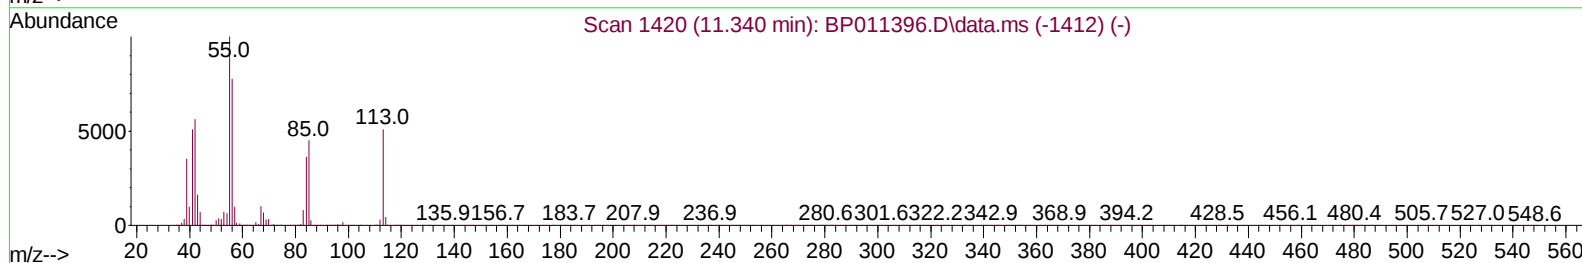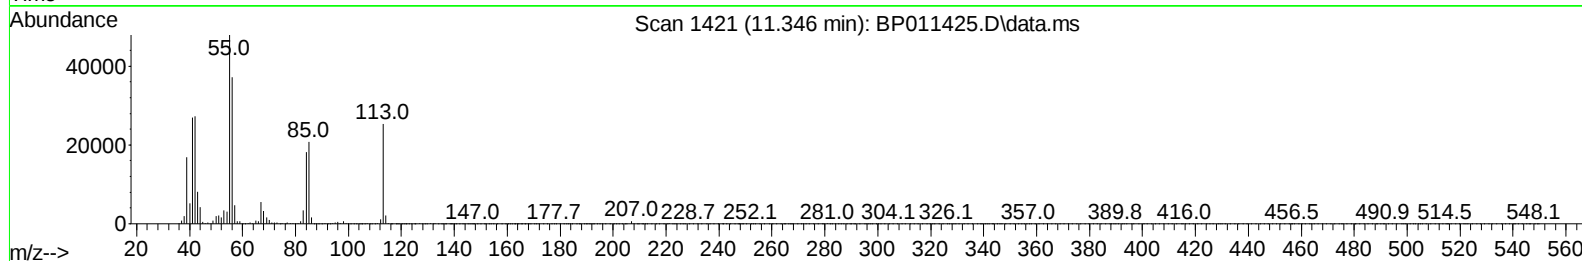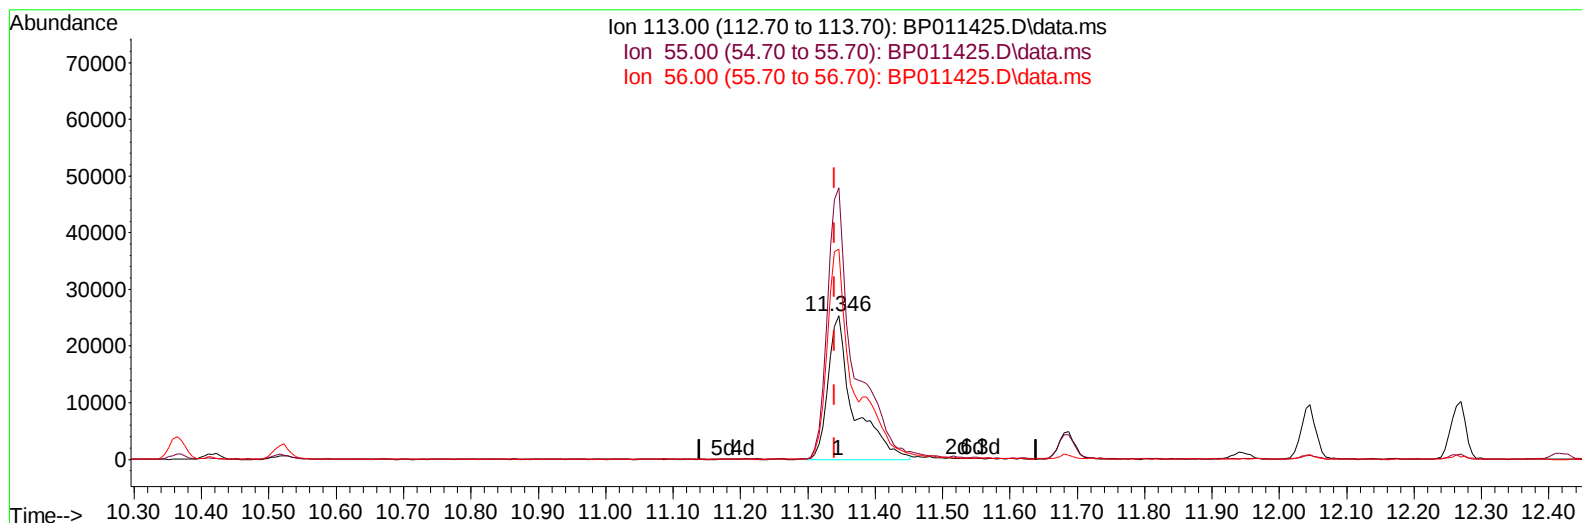

TIC: BP011425.D\data.ms

(34) Caprolactam

11.346min (+ 0.006) 35.46 ng/ul m

response 67088

Ion	Exp%	Act%
113.00	100.00	100.00
55.00	205.30	188.75
56.00	158.80	146.41
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011425.D
 Acq On : 12 Aug 2022 15:14
 Operator : CG/JU
 Sample : PB146917BS
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLCS917

Manual IntegrationsAPPROVED

Quant Time: Aug 12 17:40:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 11 23:05:53 2022
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/13/2022
 Supervised By :Sohil Jodhani 08/13/2022

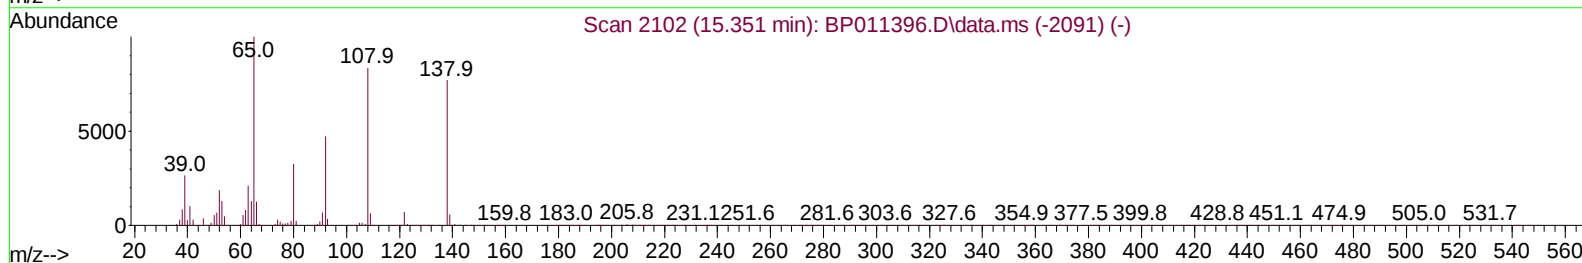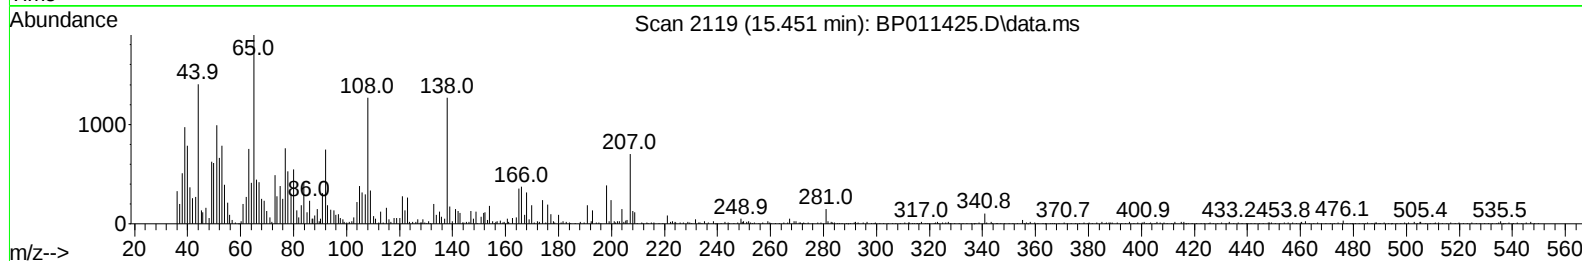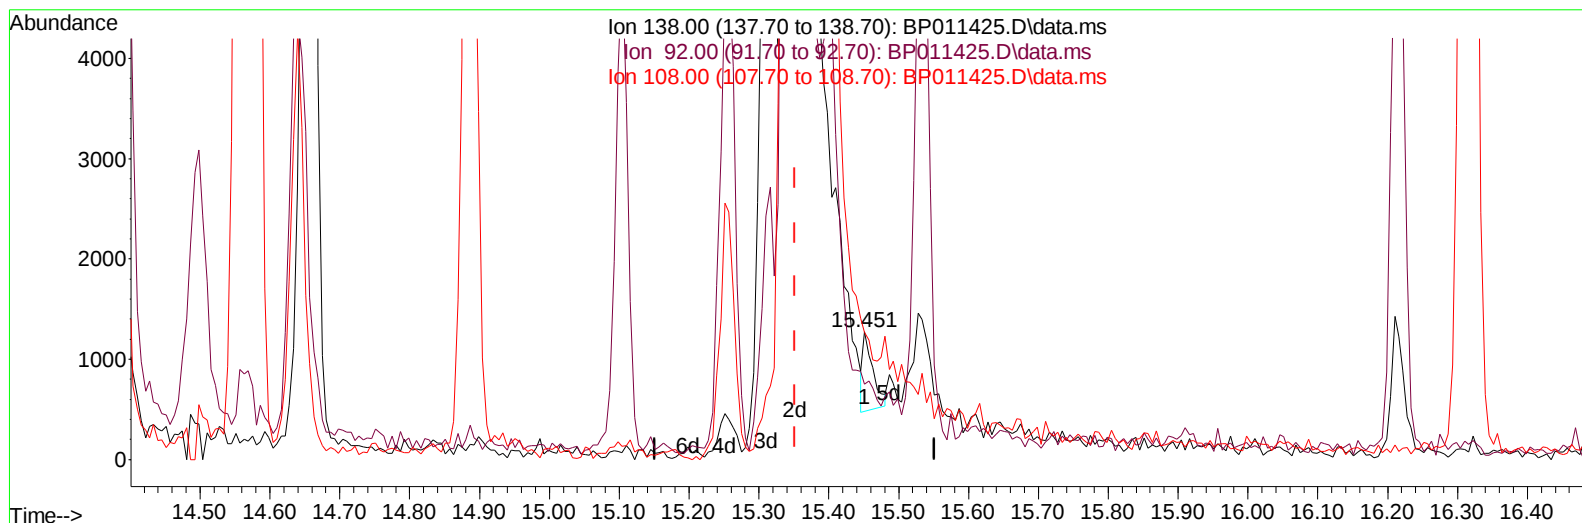

TIC: BP011425.D\data.ms

(63) 4-Nitroaniline

15.451min (+ 0.100) 0.25 ng/ul

response 785

Ion	Exp%	Act%
138.00	100.00	100.00
92.00	69.90	59.01
108.00	83.90	99.69
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011425.D
 Acq On : 12 Aug 2022 15:14
 Operator : CG/JU
 Sample : PB146917BS
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLCS917

Manual IntegrationsAPPROVED

Quant Time: Aug 12 17:40:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 11 23:05:53 2022
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/13/2022
 Supervised By :Sohil Jodhani 08/13/2022

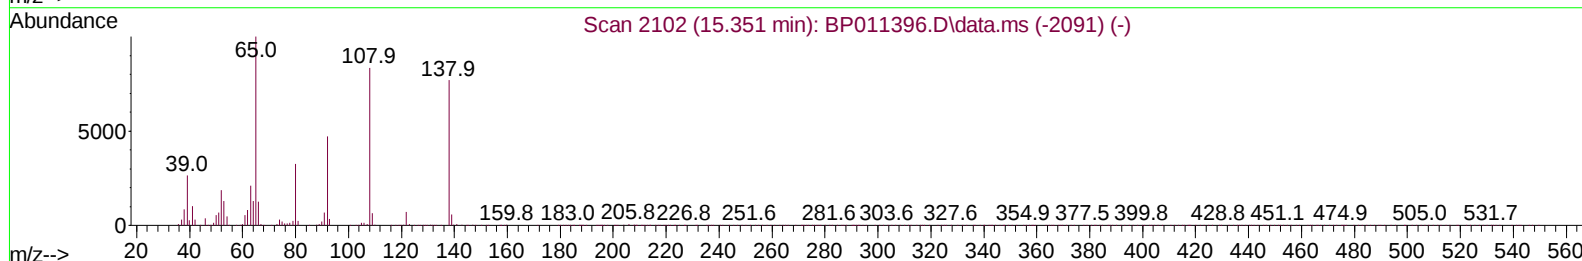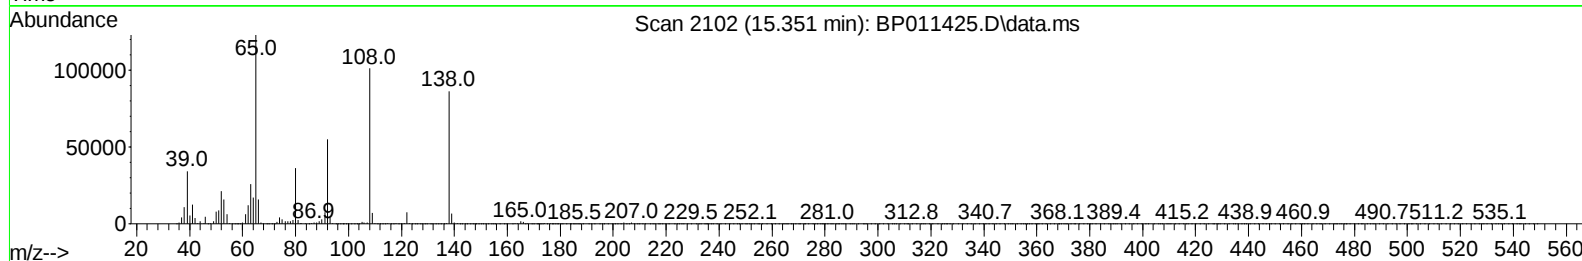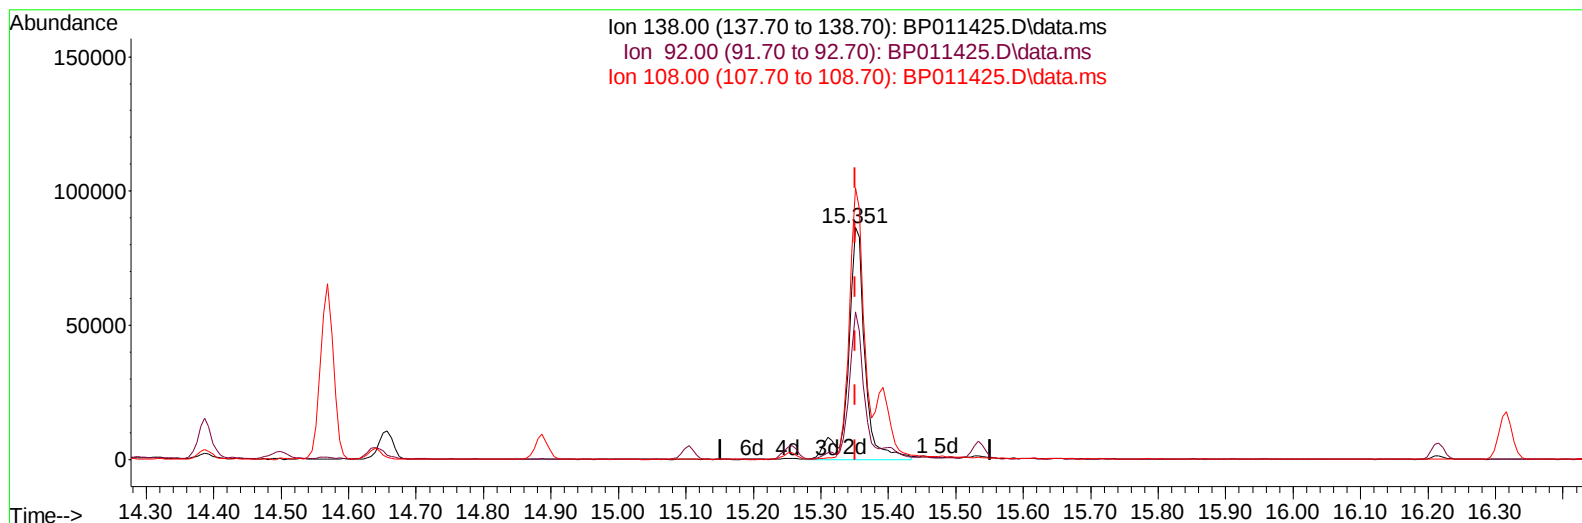

TIC: BP011425.D\data.ms

(63) 4-Nitroaniline

15.351min (+ 0.000) 47.49 ng/ul m

response 147936

Ion	Exp%	Act%
138.00	100.00	100.00
92.00	69.90	63.77
108.00	83.90	117.14#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011425.D
 Acq On : 12 Aug 2022 15:14
 Operator : CG/JU
 Sample : PB146917BS
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLCS917

Manual IntegrationsAPPROVED

Quant Time: Aug 12 17:40:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 11 23:05:53 2022
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/13/2022
 Supervised By :Sohil Jodhani 08/13/2022

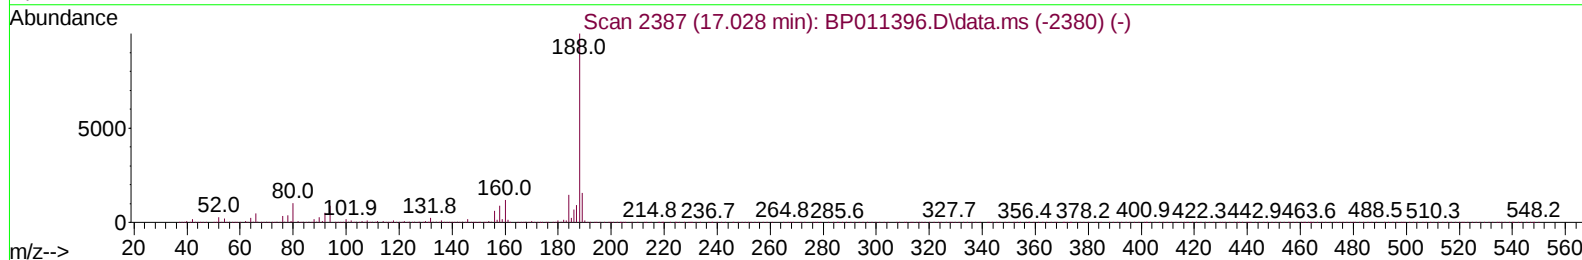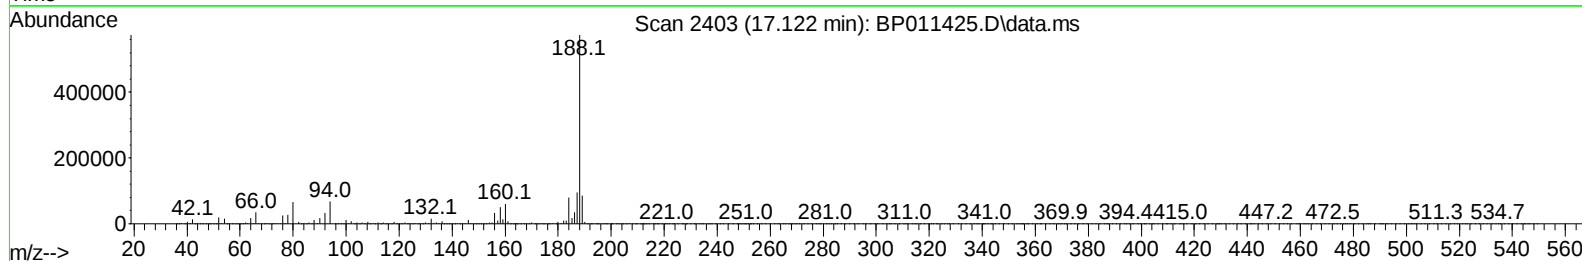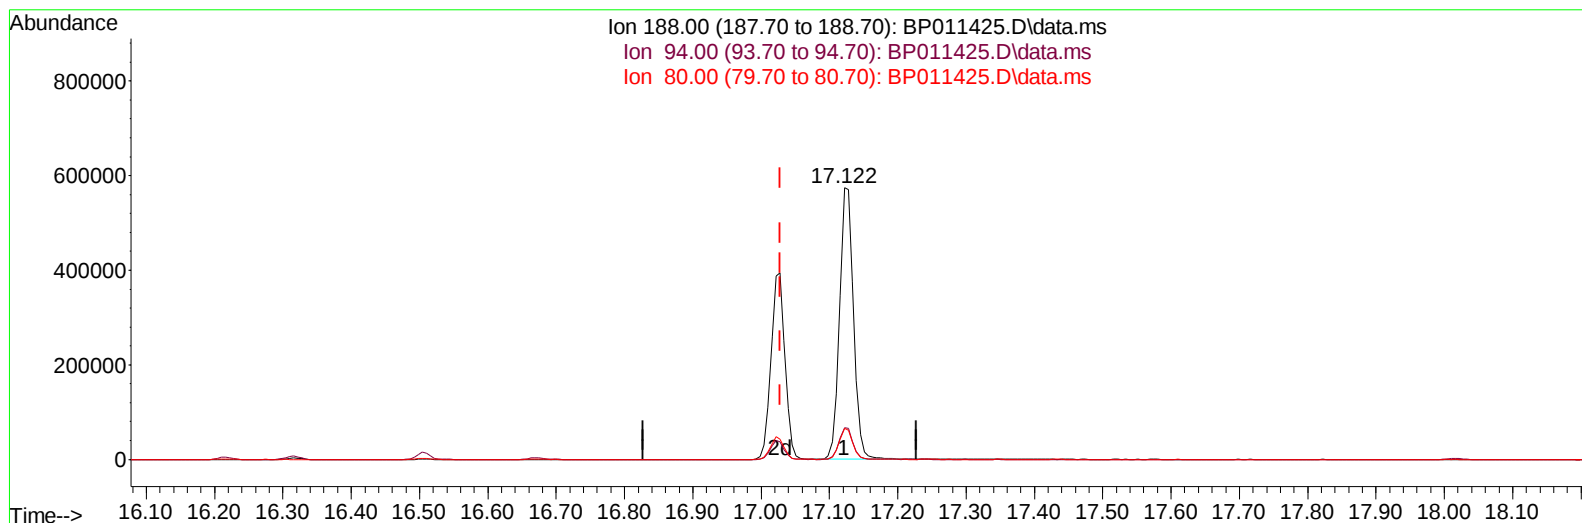

TIC: BP011425.D\data.ms

(64) Phenanthrene-d10 (I)

17.122min (+ 0.094) 20.00 ng/u1

response 813252

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.10	11.77
80.00	13.70	11.39
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011425.D
 Acq On : 12 Aug 2022 15:14
 Operator : CG/JU
 Sample : PB146917BS
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLCS917

Manual IntegrationsAPPROVED

Quant Time: Aug 12 17:40:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 11 23:05:53 2022
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/13/2022
 Supervised By :Sohil Jodhani 08/13/2022

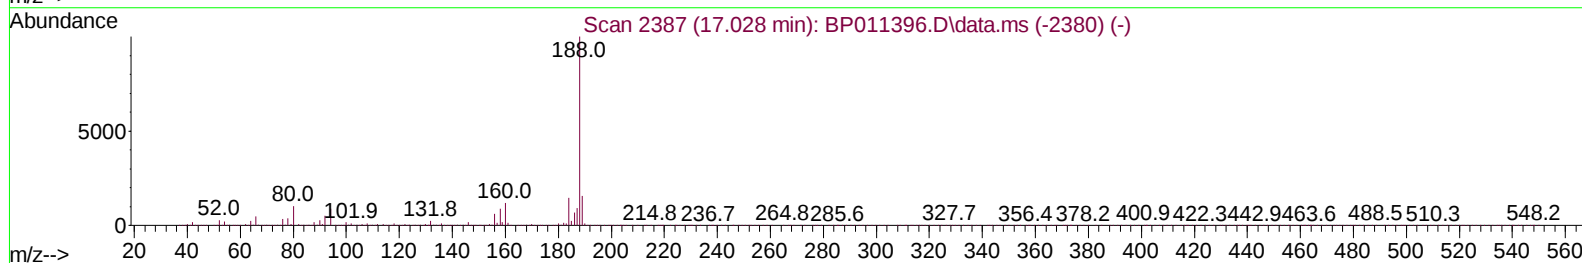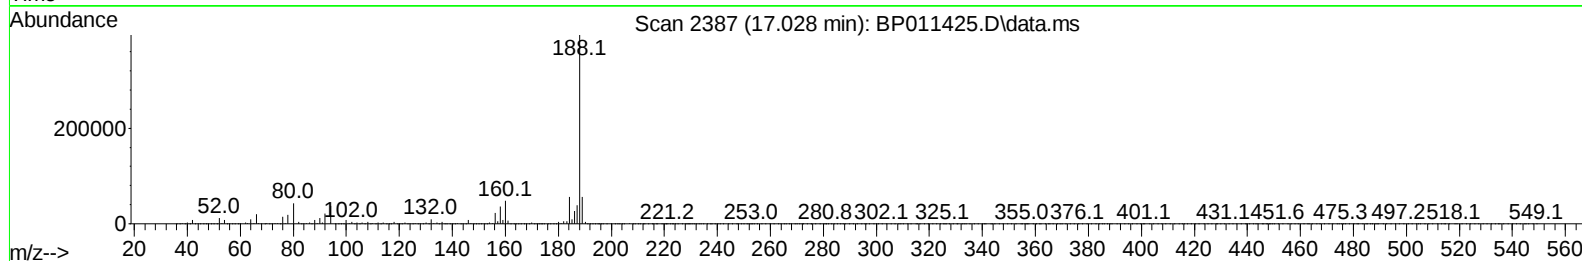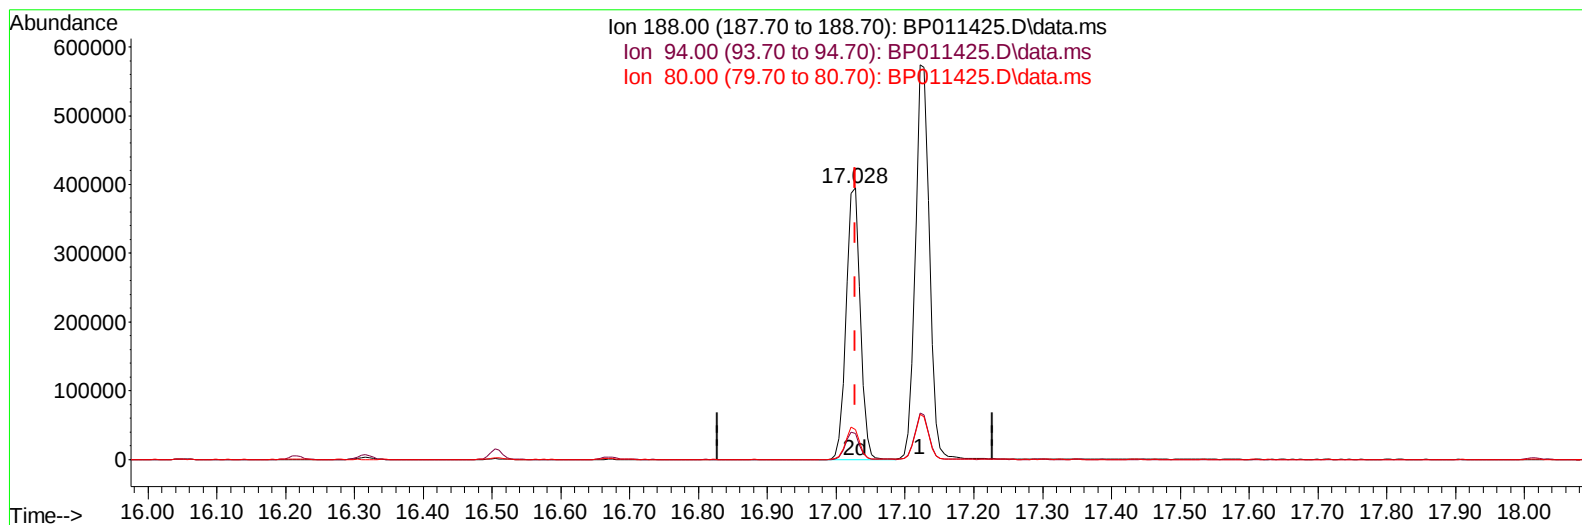

TIC: BP011425.D\data.ms

(64) Phenanthrene-d10 (I)

17.028min (+ 0.000) 20.00 ng/ul m

response 562912

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.10	9.46#
80.00	13.70	10.99
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011425.D
 Acq On : 12 Aug 2022 15:14
 Operator : CG/JU
 Sample : PB146917BS
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLCS917

Manual IntegrationsAPPROVED

Quant Time: Aug 12 17:40:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 11 23:05:53 2022
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/13/2022
 Supervised By :Sohil Jodhani 08/13/2022

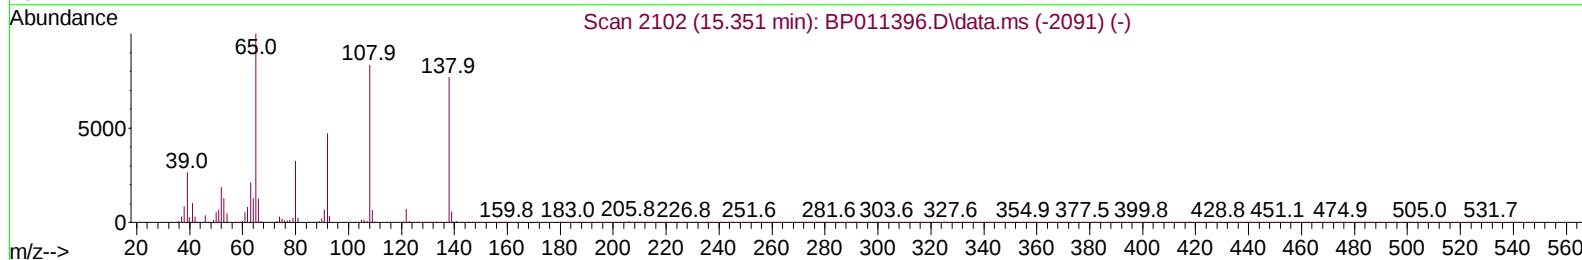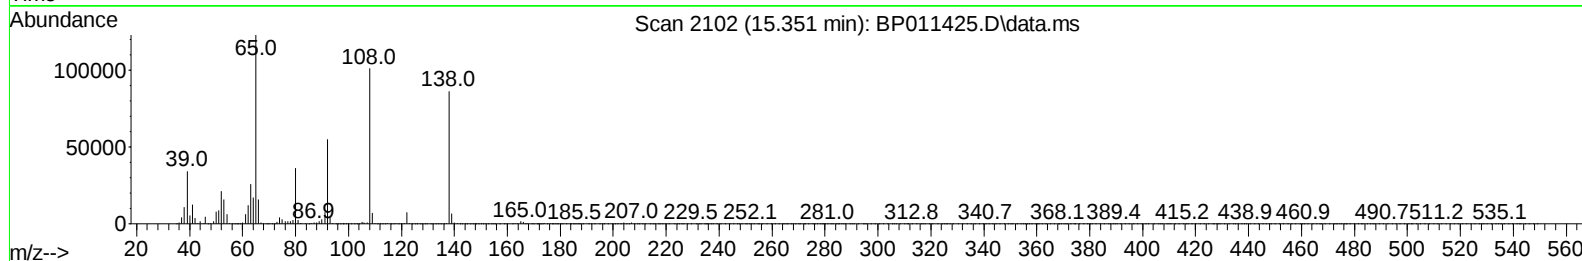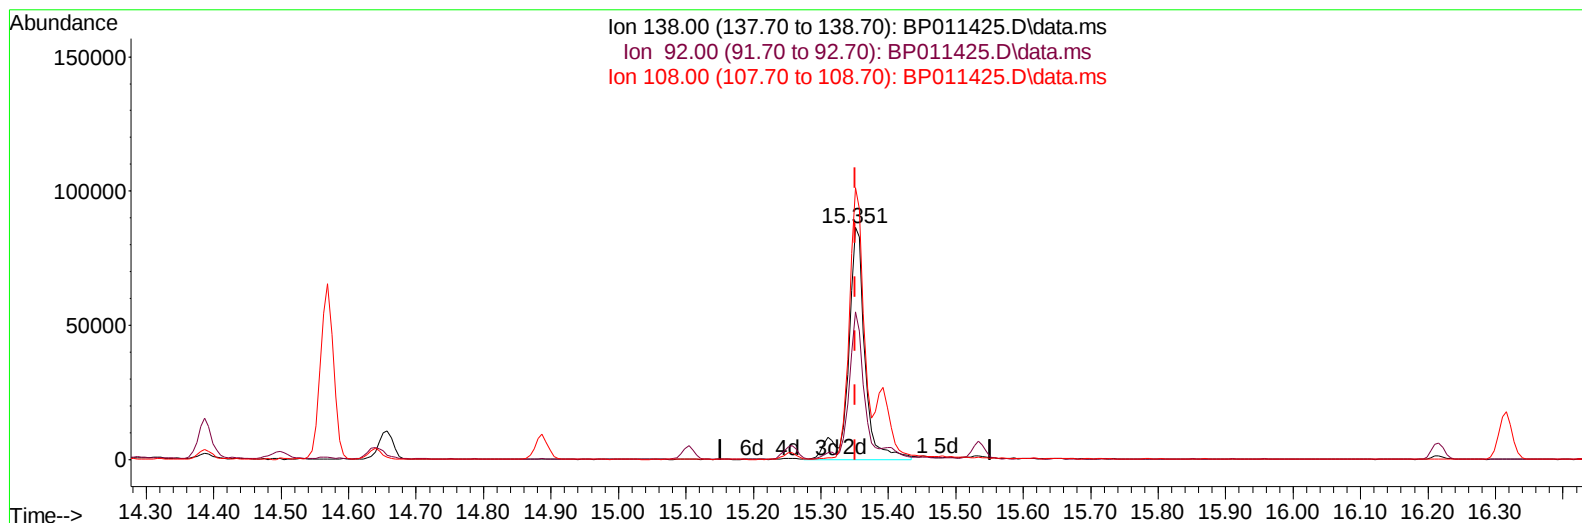

TIC: BP011425.D\data.ms

(63) 4-Nitroaniline

15.351min (+ 0.000) 47.49 ng/ul m

response 147936

Ion	Exp%	Act%
138.00	100.00	100.00
92.00	69.90	63.77
108.00	83.90	117.14#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011425.D
Acq On : 12 Aug 2022 15:14
Operator : CG/JU
Sample : PB146917BS
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLCS917

Manual IntegrationsAPPROVED

Quant Time: Aug 12 17:40:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 23:05:53 2022
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/13/2022
Supervised By :Sohil Jodhani 08/13/2022

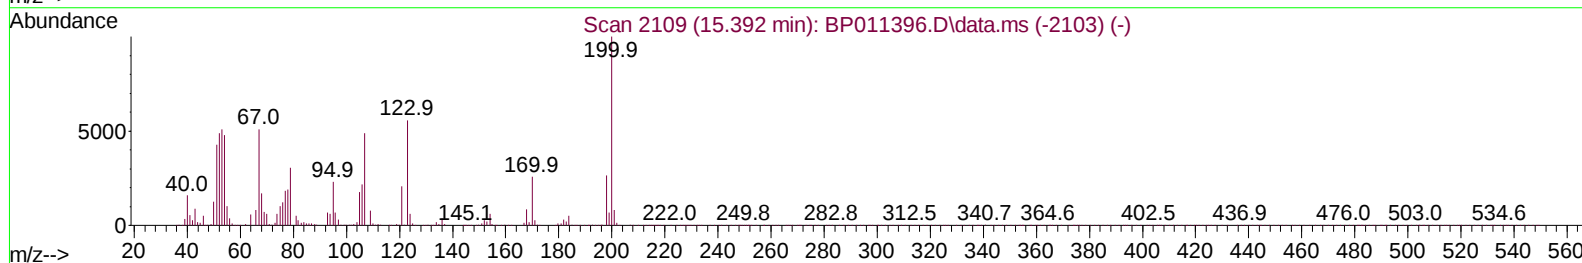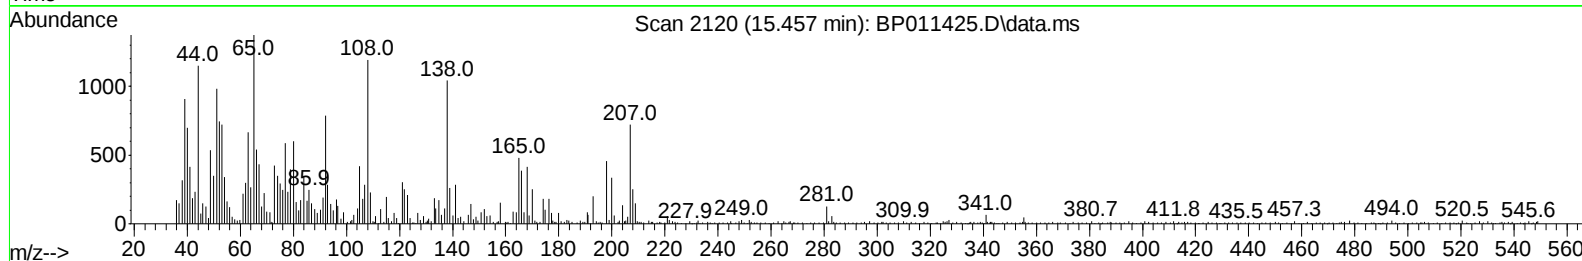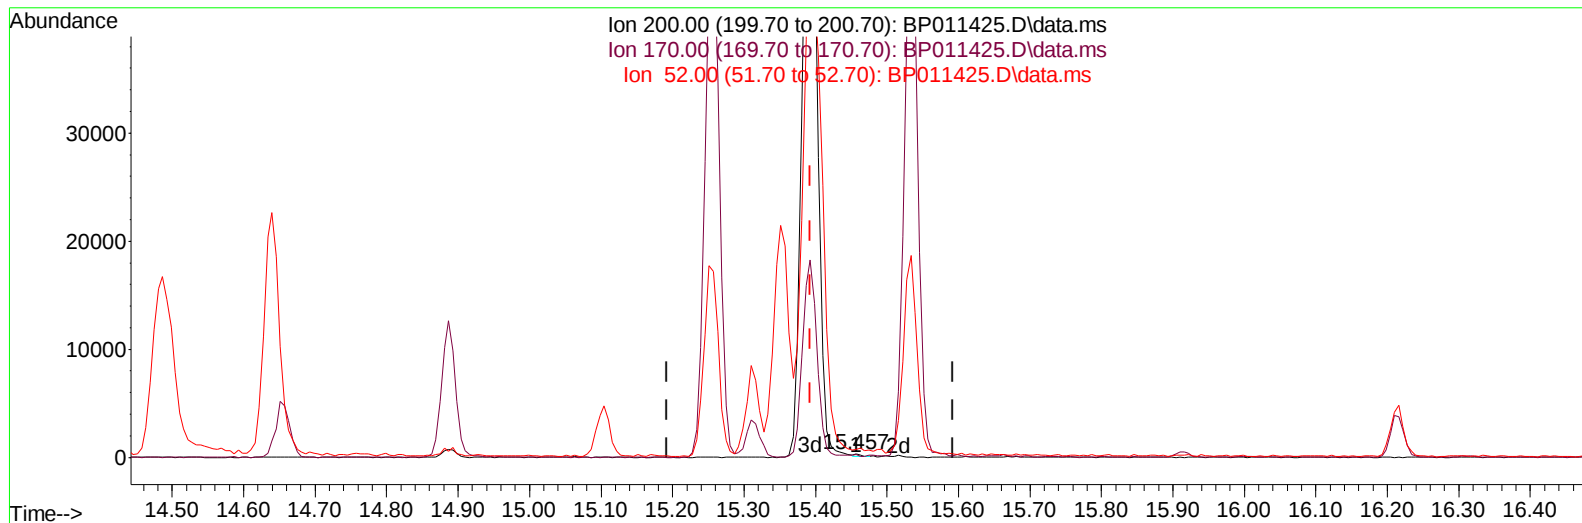

TIC: BP011425.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.457min (+ 0.065) 0.06 ng/u1

response 144

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	21.40	75.15#
52.00	71.00	222.75#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011425.D
Acq On : 12 Aug 2022 15:14
Operator : CG/JU
Sample : PB146917BS
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLCS917

Manual IntegrationsAPPROVED

Quant Time: Aug 12 17:40:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 23:05:53 2022
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/13/2022
Supervised By :Sohil Jodhani 08/13/2022

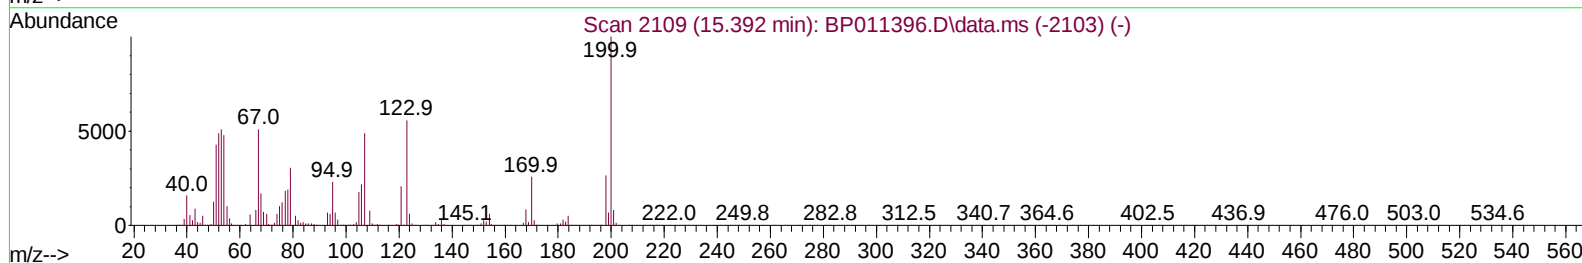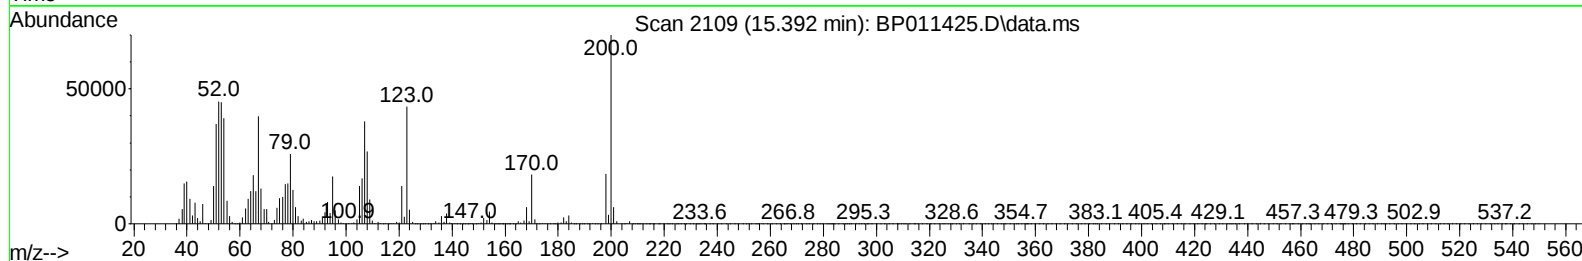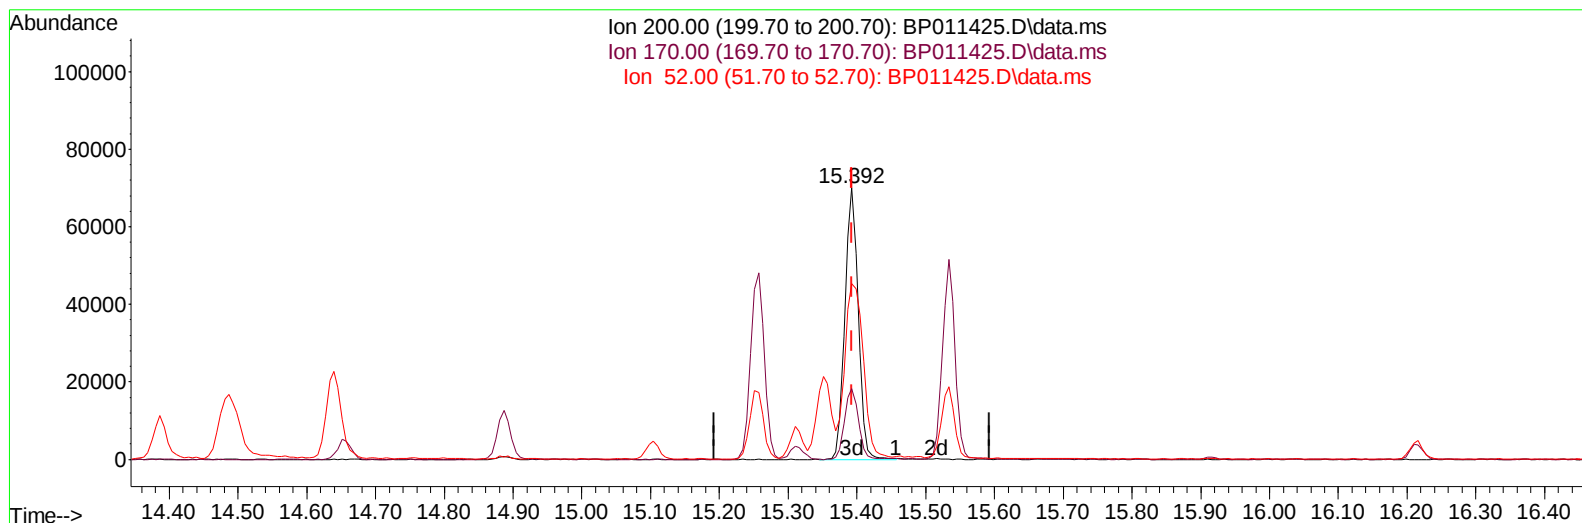

TIC: BP011425.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.392min (+ 0.000) 36.15 ng/ul m

response 94513

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	21.40	26.07#
52.00	71.00	64.79
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011425.D
Acq On : 12 Aug 2022 15:14
Operator : CG/JU
Sample : PB146917BS
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLCS917

Manual IntegrationsAPPROVED

Quant Time: Aug 12 17:40:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 23:05:53 2022
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/13/2022
Supervised By :Sohil Jodhani 08/13/2022

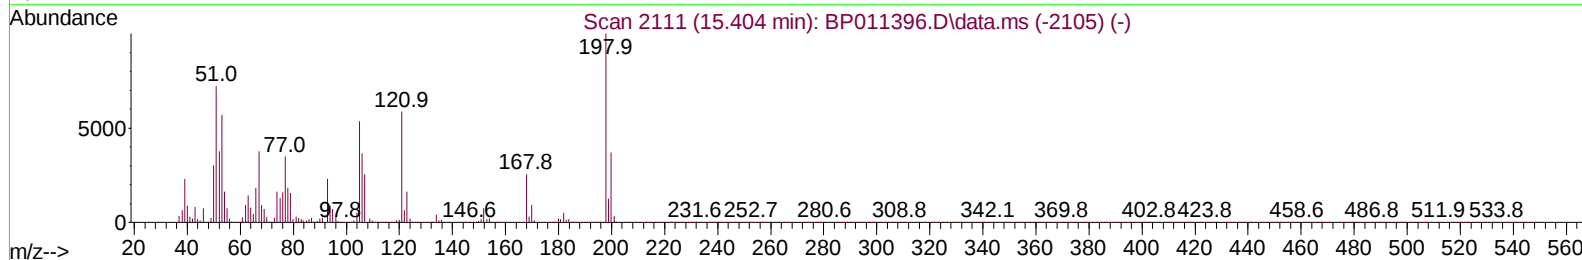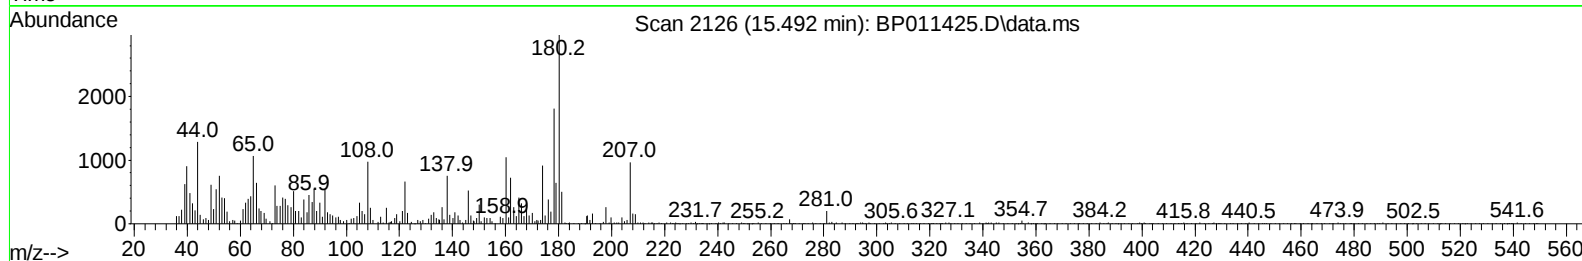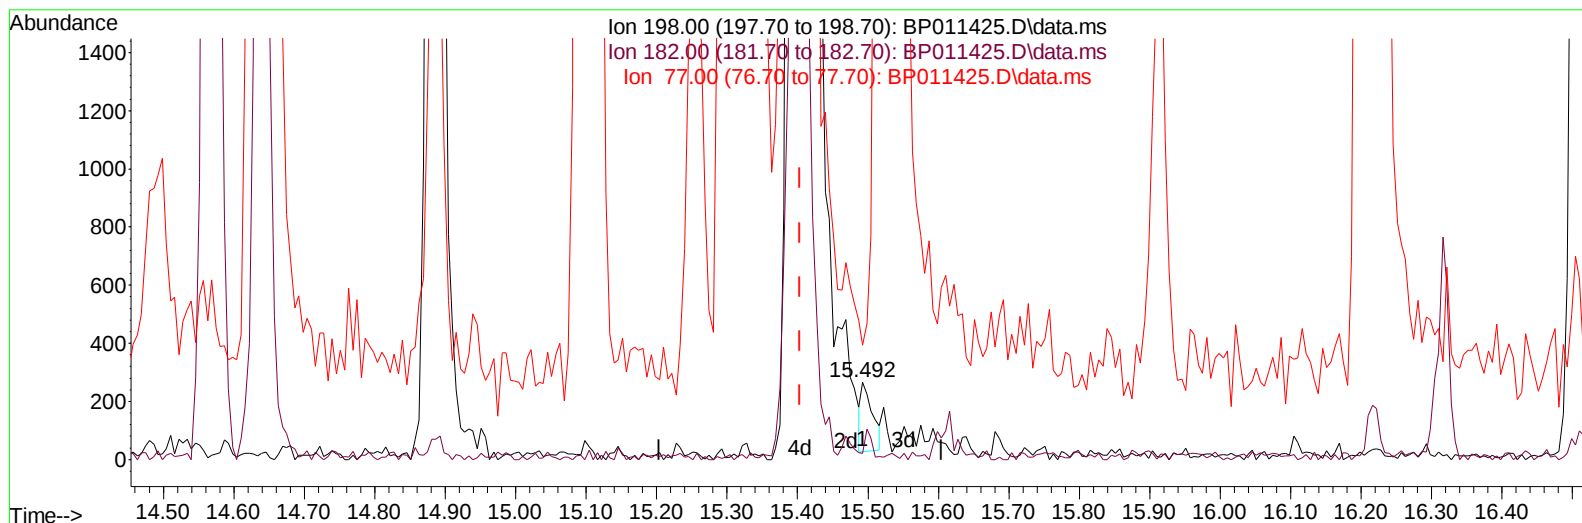

TIC: BP011425.D\data.ms

(66) 4,6-Dinitro-2-methylphenol

15.492min (+ 0.088) 0.10 ng/u1

response 268

Ion	Exp%	Act%
198.00	100.00	100.00
182.00	9.20	7.89
77.00	35.70	148.12#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011425.D
 Acq On : 12 Aug 2022 15:14
 Operator : CG/JU
 Sample : PB146917BS
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLCS917

Manual IntegrationsAPPROVED

Quant Time: Aug 12 17:40:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 11 23:05:53 2022
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/13/2022
 Supervised By :Sohil Jodhani 08/13/2022

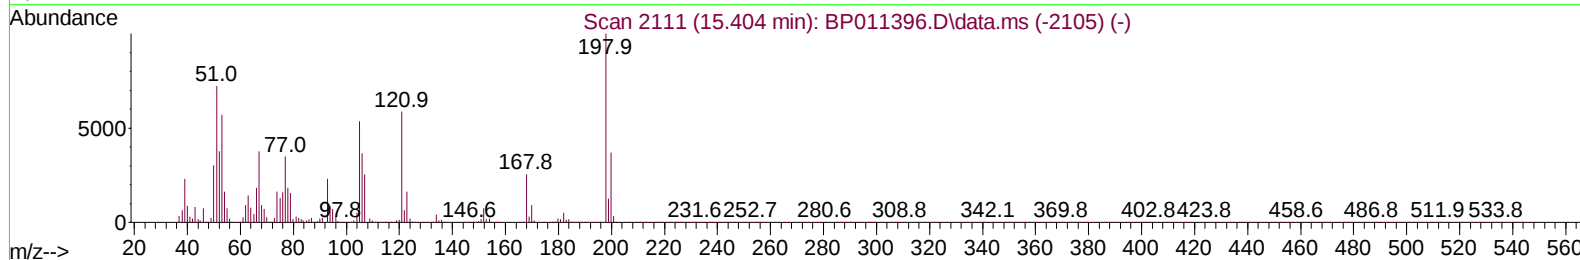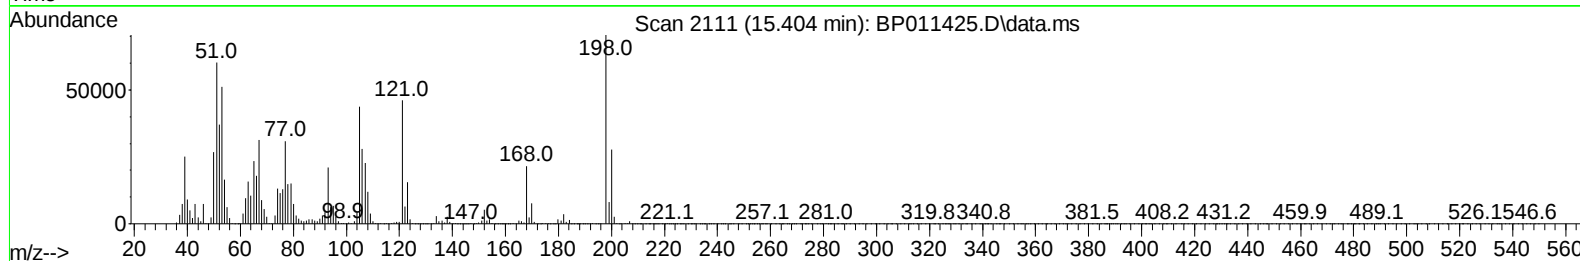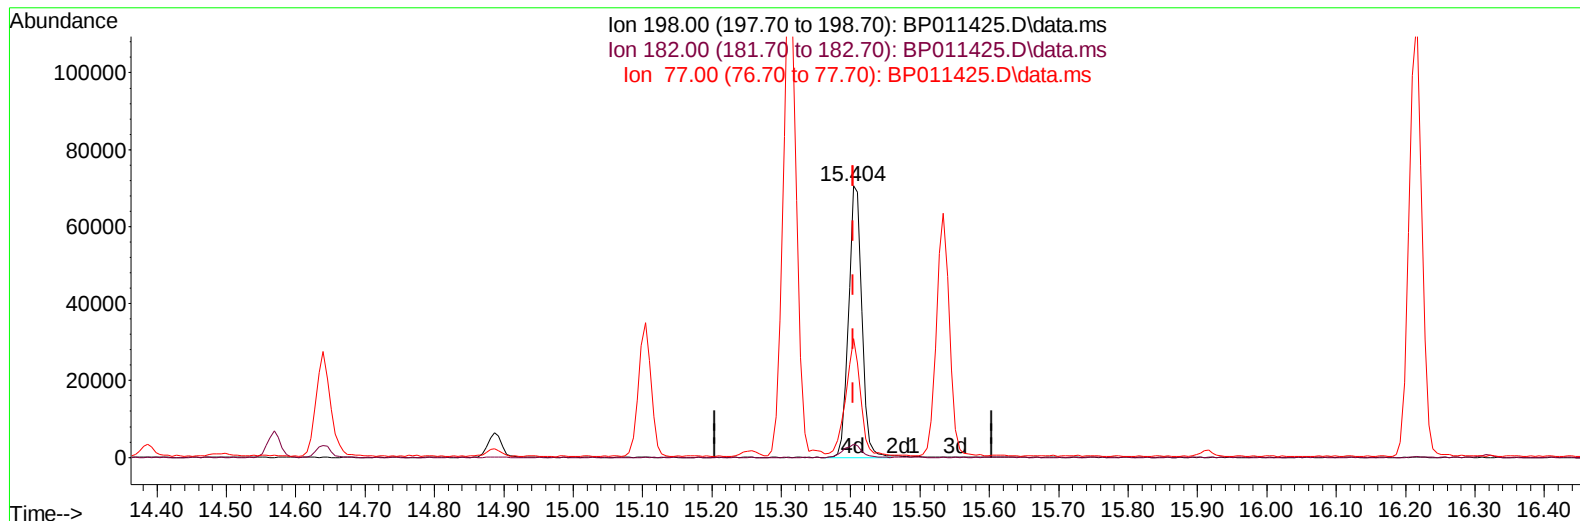

TIC: BP011425.D\data.ms

(66) 4,6-Dinitro-2-methylphenol

15.404min (+ 0.000) 35.12 ng/ul m

response 94543

Ion	Exp%	Act%
198.00	100.00	100.00
182.00	9.20	4.96#
77.00	35.70	43.86#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011425.D
 Acq On : 12 Aug 2022 15:14
 Operator : CG/JU
 Sample : PB146917BS
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLCS917

Manual IntegrationsAPPROVED

Quant Time: Aug 12 17:40:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 11 23:05:53 2022
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/13/2022
 Supervised By :Sohil Jodhani 08/13/2022

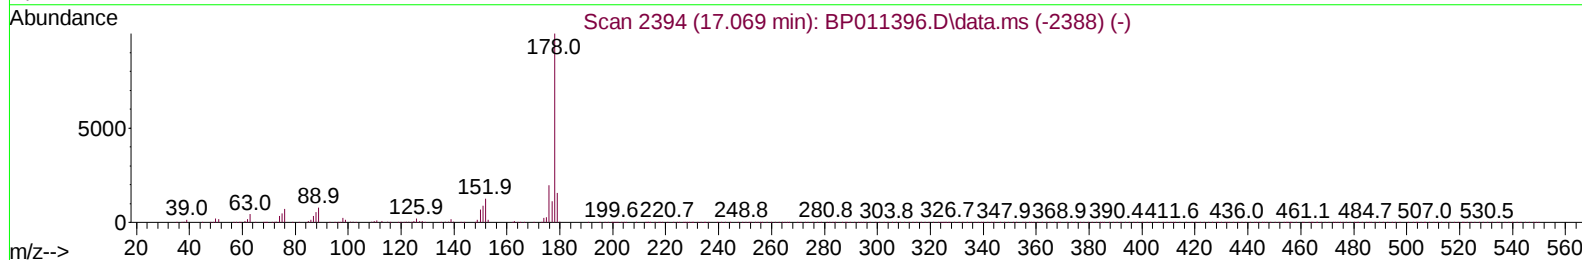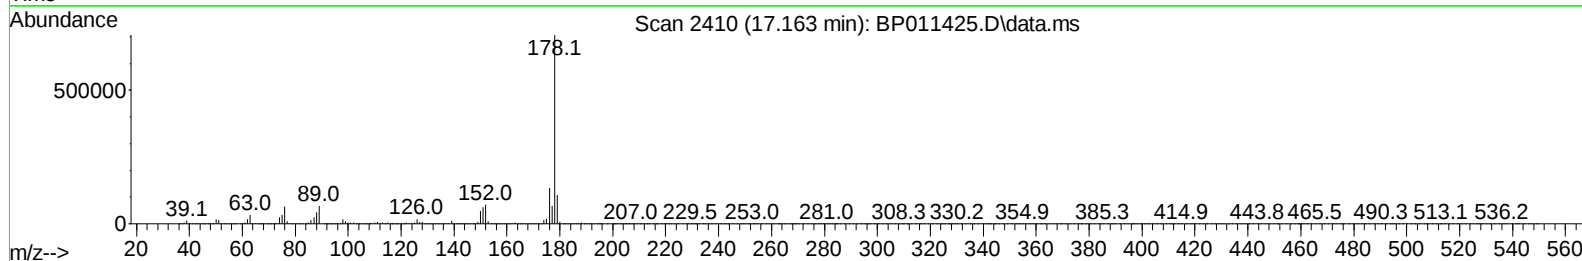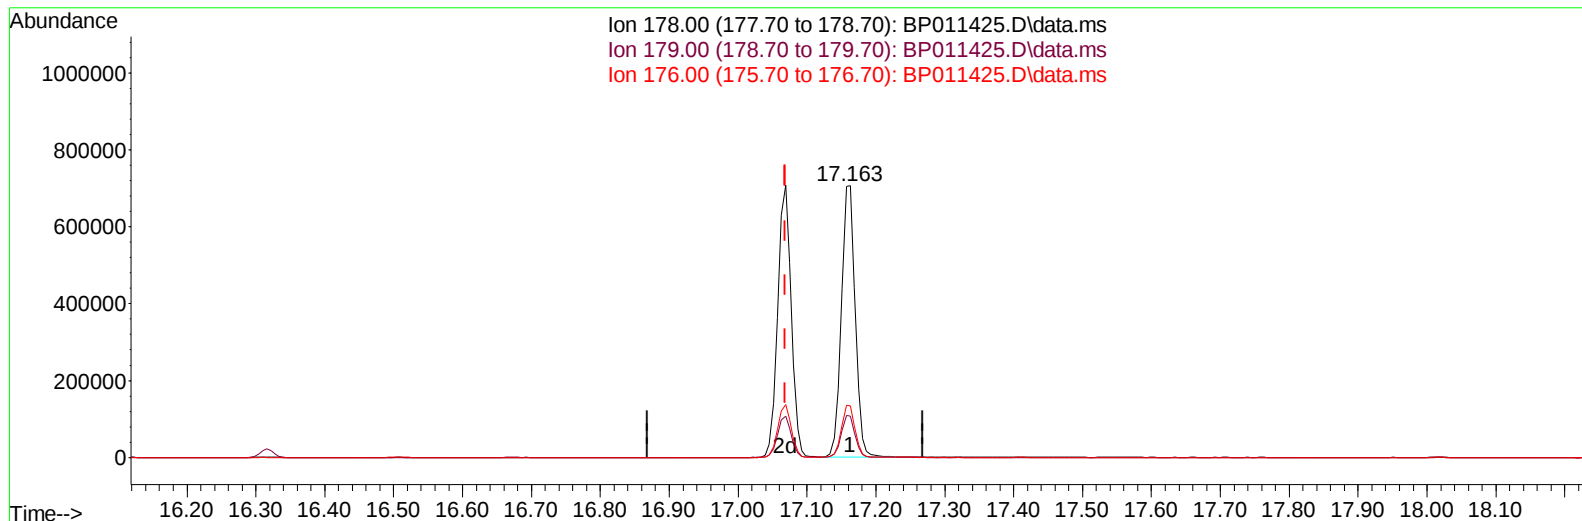

TIC: BP011425.D\data.ms

(72) Phenanthrene

17.163min (+ 0.094) 31.09 ng/u1

response 981443

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	15.10	15.14
176.00	19.30	18.89
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011425.D
Acq On : 12 Aug 2022 15:14
Operator : CG/JU
Sample : PB146917BS
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLCS917

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/13/2022
Supervised By :Sohil Jodhani 08/13/2022

Quant Time: Aug 12 17:40:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 23:05:53 2022
Response via : Initial Calibration

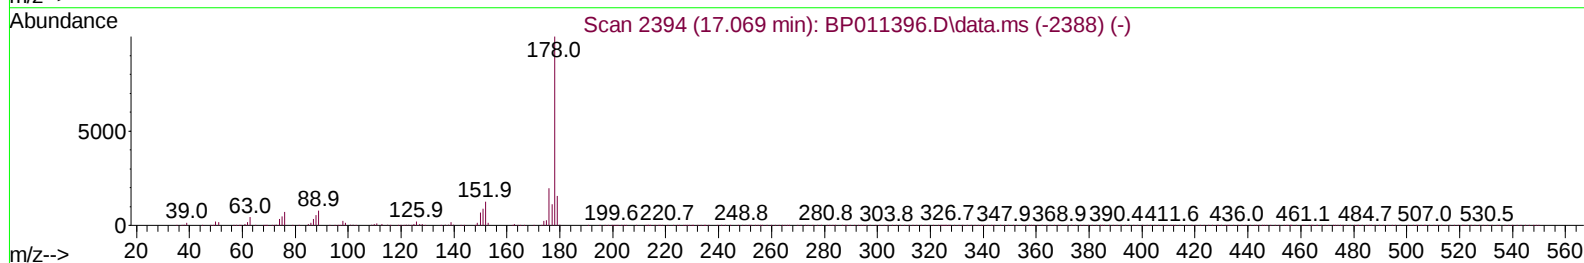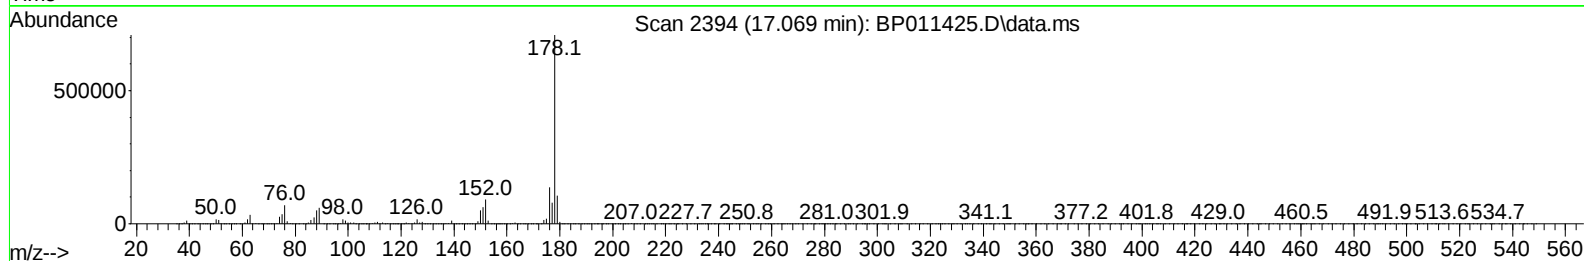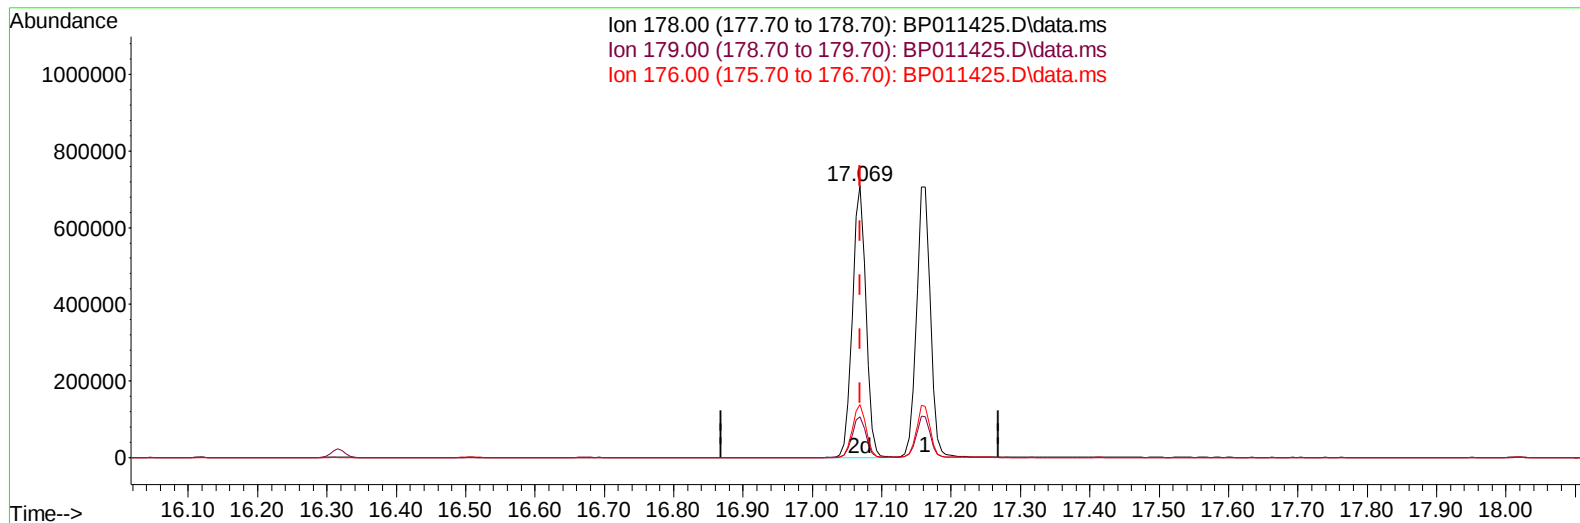

TIC: BP011425.D\data.ms

(72) Phenanthrene

17.069min (+ 0.000) 30.57 ng/ul m

response 964861

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	15.10	15.08
176.00	19.30	19.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011425.D
 Acq On : 12 Aug 2022 15:14
 Operator : CG/JU
 Sample : PB146917BS
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLCS917

Manual IntegrationsAPPROVED

Quant Time: Aug 12 17:40:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 11 23:05:53 2022
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/13/2022
 Supervised By :Sohil Jodhani 08/13/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.575	152	97125	20.000	ng/ul	0.00
20) Naphthalene-d8	10.363	136	429926	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.251	164	264823	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.028	188	562912m	20.000	ng/ul	0.00
79) Chrysene-d12	21.157	240	557370	20.000	ng/ul	0.00
88) Perylene-d12	23.468	264	555265	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.081	96	17372	5.483	ng/uL	0.00
4) Pyridine-d5	3.487	84	214755	26.872	ng/ul	0.00
7) Phenol-d5	6.758	99	264559	30.779	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.922	67	175489	28.795	ng/ul	0.00
11) 2-Chlorophenol-d4	7.110	132	214613	31.822	ng/ul	0.00
15) 4-Methylphenol-d8	8.299	113	213375	31.616	ng/ul	0.00
21) Nitrobenzene-d5	8.740	128	102286	34.958	ng/ul	0.00
24) 2-Nitrophenol-d4	9.457	143	105514	39.388	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.993	165	190712	35.253	ng/ul	0.00
31) 4-Chloroaniline-d4	10.516	131	273679	28.937	ng/ul	0.00
46) Dimethylphthalate-d6	13.675	166	630367	34.306	ng/ul	0.00
49) Acenaphthylene-d8	13.940	160	742735	33.580	ng/ul	0.00
54) 4-Nitrophenol-d4	14.481	143	116688	34.769	ng/ul	0.00
60) Fluorene-d10	15.257	176	520053	33.095	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.392	200	94513m	36.147	ng/ul	0.00
73) Anthracene-d10	17.122	188	813107	32.136	ng/ul	0.00
81) Pyrene-d10	19.386	212	942906	30.706	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.316	264	924775	33.025	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.111	88	36960	10.983	ng/ul#	81
5) Pyridine	3.505	79	218774	26.281	ng/ul#	81
6) Benzaldehyde	6.728	77	159860	42.676	ng/ul	98
8) Phenol	6.787	94	268658	28.876	ng/ul#	88
10) Bis(2-Chloroethyl)ether	7.016	93	213592	28.506	ng/ul	97
12) 2-Chlorophenol	7.140	128	220091	31.319	ng/ul	98
13) 2-Methylphenol	8.028	108	199155	29.722	ng/ul	97
14) 2,2'-oxybis(1-Chloropr...	8.116	45	323530	28.788	ng/ul	96
16) Acetophenone	8.405	105	349132	31.974	ng/ul	95
17) N-Nitroso-di-n-propyla...	8.399	70	184342	34.270	ng/ul	96
18) 4-Methylphenol	8.363	108	216533	30.149	ng/ul	97
19) Hexachloroethane	8.640	117	100522	33.877	ng/ul	100
22) Nitrobenzene	8.781	77	273693	33.414	ng/ul	98
23) Isophorone	9.310	82	503365	33.502	ng/ul	98
25) 2-Nitrophenol	9.487	139	115561	37.015	ng/ul#	80
26) 2,4-Dimethylphenol	9.557	107	259729	32.925	ng/ul	92
27) Bis(2-Chloroethoxy)met...	9.799	93	292228	30.435	ng/ul	98
29) 2,4-Dichlorophenol	10.022	162	188912	33.393	ng/ul	98
30) Naphthalene	10.416	128	706774	30.216	ng/ul	100
32) 4-Chloroaniline	10.540	127	254115	26.805	ng/ul	99
33) Hexachlorobutadiene	10.699	225	120594	34.747	ng/ul	98
34) Caprolactam	11.346	113	67088m	35.462	ng/ul	
35) 4-Chloro-3-methylphenol	11.687	107	242880	36.515	ng/ul	97

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011425.D
 Acq On : 12 Aug 2022 15:14
 Operator : CG/JU
 Sample : PB146917BS
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLCS917

Manual IntegrationsAPPROVED

Quant Time: Aug 12 17:40:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 11 23:05:53 2022
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/13/2022
 Supervised By :Sohil Jodhani 08/13/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
36) 2-Methylnaphthalene	12.046	142	467412	32.238	ng/ul	100
37) 1-Methylnaphthalene	12.263	142	472420	32.123	ng/ul	100
39) 1,2,4,5-Tetrachloroben...	12.416	216	209853	30.100	ng/ul	98
40) Hexachlorocyclopentadiene	12.387	237	113989	30.511	ng/ul	99
41) 2,4,6-Trichlorophenol	12.669	196	141576	33.562	ng/ul	98
42) 2,4,5-Trichlorophenol	12.740	196	149278	33.156	ng/ul	99
43) 1,1'-Biphenyl	13.075	154	605233	29.104	ng/ul	98
44) 2-Chloronaphthalene	13.116	162	462019	29.612	ng/ul	95
45) 2-Nitroaniline	13.340	65	174138	43.944	ng/ul	97
47) Dimethylphthalate	13.722	163	623671	33.511	ng/ul	100
48) 2,6-Dinitrotoluene	13.845	165	120225	41.315	ng/ul	98
50) Acenaphthylene	13.969	152	797564	31.281	ng/ul	100
51) 3-Nitroaniline	14.175	138	132145	41.282	ng/ul	100
52) Acenaphthene	14.316	153	525940	30.929	ng/ul	98
53) 2,4-Dinitrophenol	14.387	184	57826	33.493	ng/ul#	81
55) 4-Nitrophenol	14.498	109	129771	41.682	ng/ul#	71
56) Dibenzofuran	14.657	168	718747	31.178	ng/ul	91
57) 2,4-Dinitrotoluene	14.640	165	182189	40.847	ng/ul	91
58) 2,3,4,6-Tetrachlorophenol	14.887	232	128064	36.564	ng/ul#	95
59) Diethylphthalate	15.104	149	715459	37.109	ng/ul	97
61) Fluorene	15.310	166	605473	32.340	ng/ul	98
62) 4-Chlorophenyl-phenyle...	15.316	204	269591	32.942	ng/ul	91
63) 4-Nitroaniline	15.351	138	147936m	47.494	ng/ul	
66) 4,6-Dinitro-2-methylph...	15.404	198	94543m	35.116	ng/ul	
67) N-Nitrosodiphenylamine	15.534	169	519695	31.330	ng/ul	100
68) 4-Bromophenyl-phenylether	16.216	248	158973	31.914	ng/ul	91
69) Hexachlorobenzene	16.316	284	185865	31.938	ng/ul	94
70) Atrazine	16.510	200	156541	28.313	ng/ul	97
71) Pentachlorophenol	16.675	266	111778	33.086	ng/ul	98
72) Phenanthrene	17.069	178	964861m	30.568	ng/ul	
74) Anthracene	17.163	178	979115	31.159	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.034	216	209673	25.946	ng/uL	99
76) Pentachlorobenzene	14.569	250	208402	29.612	ng/uL	99
77) Carbazole	17.445	167	911631	31.047	ng/ul	98
78) Di-n-butylphthalate	18.016	149	1261124	39.278	ng/ul	99
80) Fluoranthene	19.063	202	1138175	30.452	ng/ul	94
82) Pyrene	19.416	202	1172868	29.730	ng/ul	94
83) Butylbenzylphthalate	20.316	149	580738	46.194	ng/ul	96
84) 3,3'-Dichlorobenzidine	21.086	252	361371	35.625	ng/ul	99
85) Benzo(a)anthracene	21.145	228	1117927	31.263	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.086	149	872760	43.245	ng/ul	98
87) Chrysene	21.198	228	1105241	31.223	ng/ul	99
89) Di-n-octyl phthalate	21.986	149	1469964	38.155	ng/ul	100
90) Benzo(b)fluoranthene	22.768	252	1131597	30.964	ng/ul	98
91) Benzo(k)fluoranthene	22.816	252	1114609	31.172	ng/ul	97
93) Benzo(a)pyrene	23.368	252	1122528	31.847	ng/ul#	96
94) Indeno(1,2,3-cd)pyrene	25.851	276	1242155	31.878	ng/ul	94
95) Dibenzo(a,h)anthracene	25.868	278	1061207	32.022	ng/ul#	94
96) Benzo(g,h,i)perylene	26.580	276	1048988	31.903	ng/ul	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :

BNA_P

ClientSampleId :

SLCS917

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/13/2022
Supervised By :Sohil Jodhani 08/13/2022

