




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011437.D
Acq On : 12 Aug 2022 22:42
Operator : CG/JU
Sample : N4166-01
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBZ1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/13/2022
Supervised By :Sohil Jodhani 08/13/2022

Quant Time: Aug 12 23:48:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 23:05:53 2022
Response via : Initial Calibration

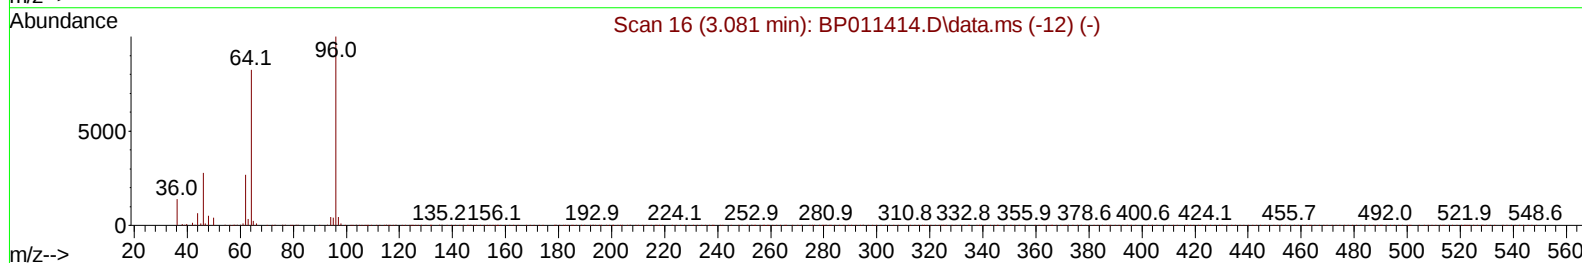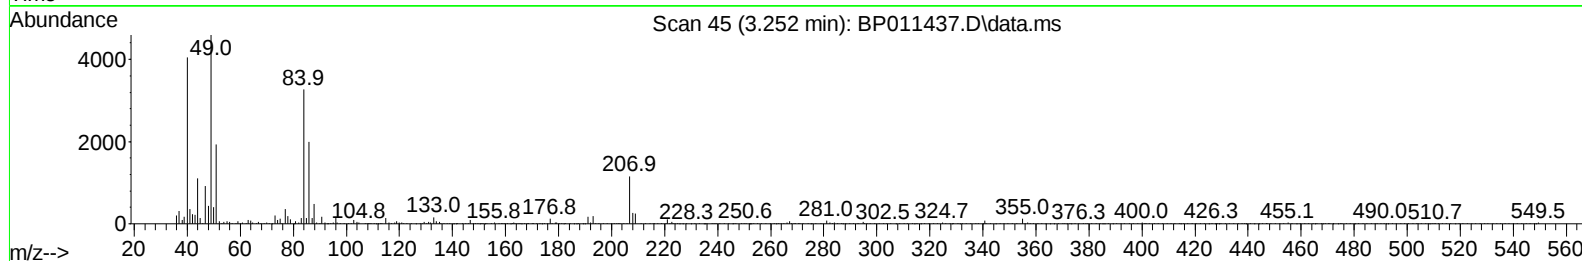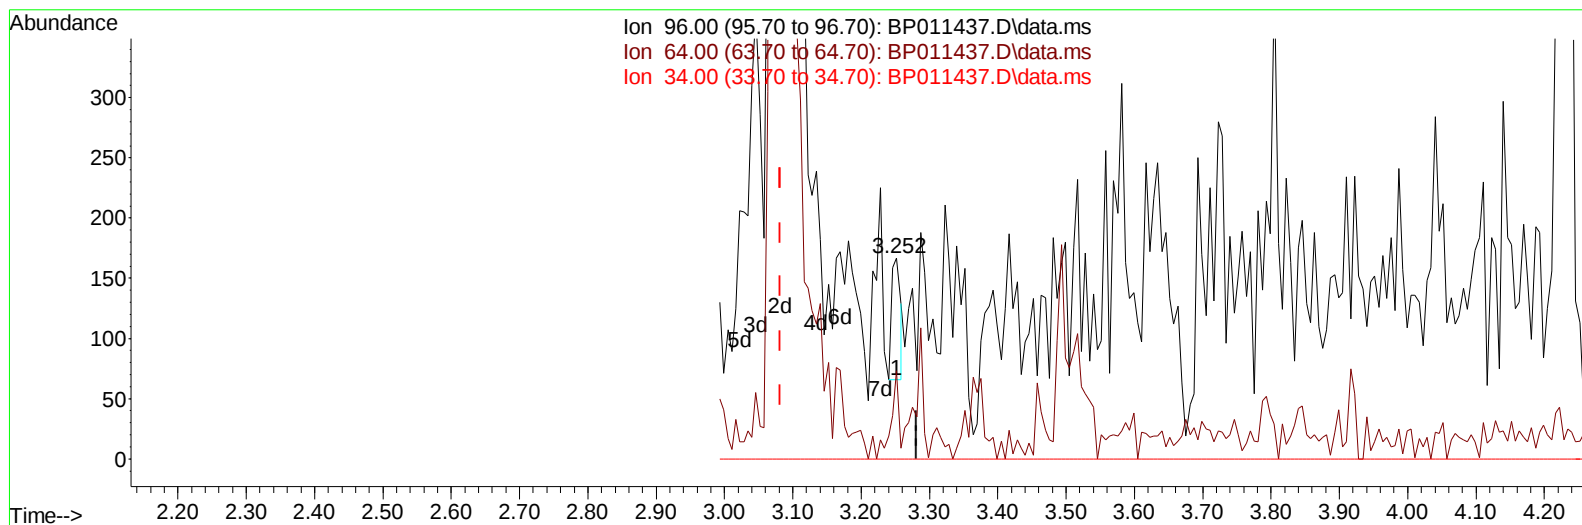

TIC: BP011437.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.252min (+ 0.171) 0.03 ng/uL

response	91
Ion	Exp% Act%
96.00	100.00 100.00
64.00	61.00 58.08
34.00	0.00 0.00
0.00	0.00 0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011437.D
Acq On : 12 Aug 2022 22:42
Operator : CG/JU
Sample : N4166-01
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBZ1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/13/2022
Supervised By :Sohil Jodhani 08/13/2022

Quant Time: Aug 12 23:48:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 23:05:53 2022
Response via : Initial Calibration

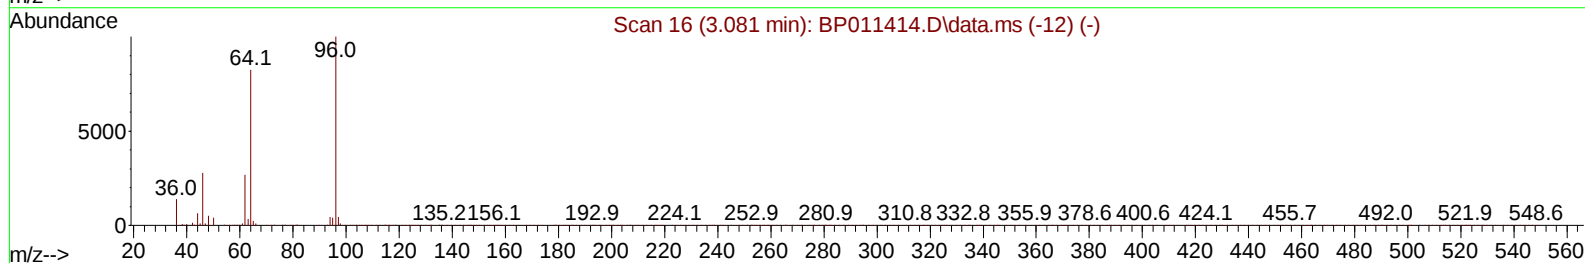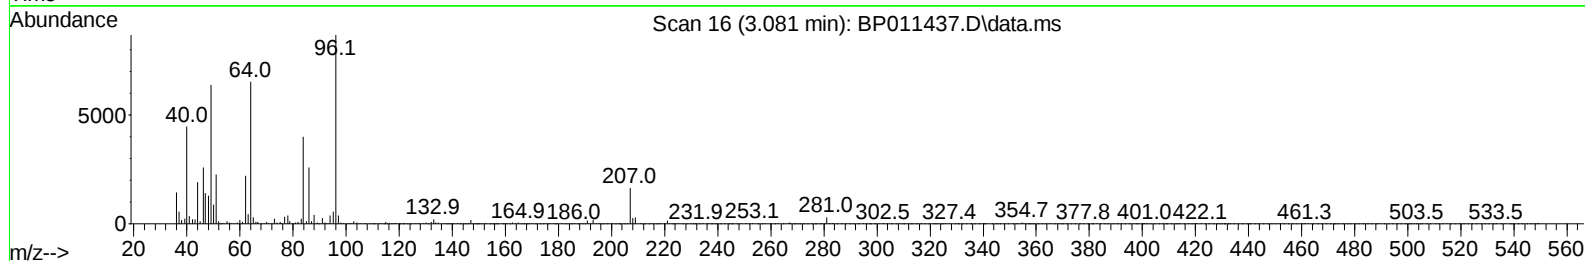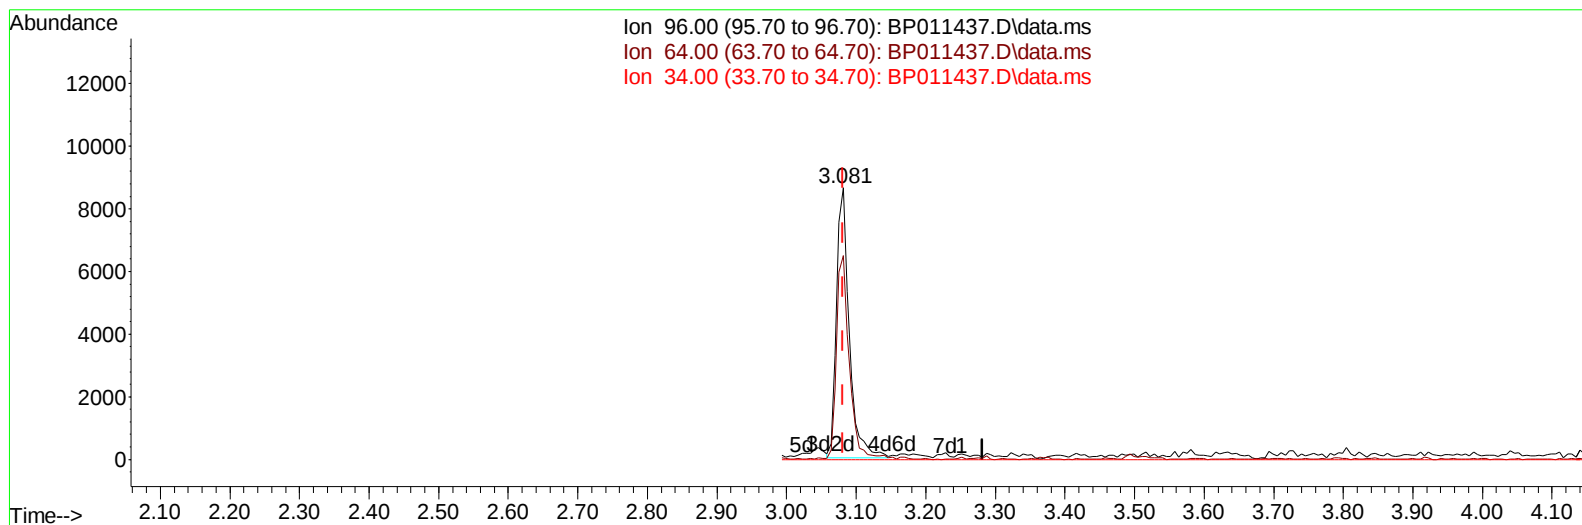

TIC: BP011437.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.081min (+ 0.000) 3.80 ng/uL m

response 10915

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	61.00	75.13#
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011437.D
 Acq On : 12 Aug 2022 22:42
 Operator : CG/JU
 Sample : N4166-01
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBZ1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/13/2022
 Supervised By :Sohil Jodhani 08/13/2022

Quant Time: Aug 12 23:48:59 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 11 23:05:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.569	152	88110	20.000	ng/ul	0.00
20) Naphthalene-d8	10.363	136	387632	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.245	164	227416	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.022	188	471091	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.151	240	474788	20.000	ng/ul	0.00
88) Perylene-d12	23.457	264	515094	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.081	96	10915m	3.798	ng/uL	0.00
4) Pyridine-d5	3.493	84	57678	7.956	ng/ul	0.00
7) Phenol-d5	6.758	99	32845	4.212	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.922	67	136109	24.618	ng/ul	0.00
11) 2-Chlorophenol-d4	7.105	132	113125	18.490	ng/ul	0.00
15) 4-Methylphenol-d8	8.293	113	66511	10.863	ng/ul	-0.01
21) Nitrobenzene-d5	8.734	128	76518	29.005	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.457	143	66889	27.694	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.987	165	105925	21.716	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.516	131	171407	20.101	ng/ul	0.00
46) Dimethylphthalate-d6	13.669	166	472115	29.920	ng/ul	-0.01
49) Acenaphthylene-d8	13.940	160	503911	26.530	ng/ul	0.00
54) 4-Nitrophenol-d4	14.492	143	5394	1.872	ng/ul	0.01
60) Fluorene-d10	15.251	176	394943	29.267	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.387	200	51708	23.631	ng/ul	0.00
73) Anthracene-d10	17.122	188	700261	33.071	ng/ul	0.00
81) Pyrene-d10	19.380	212	812459	31.060	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.310	264	830793	31.982	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011437.D
Acq On : 12 Aug 2022 22:42
Operator : CG/JU
Sample : N4166-01
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBZ1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/13/2022
Supervised By :Sohil Jodhani 08/13/2022

Quant Time: Aug 12 23:48:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 23:05:53 2022
Response via : Initial Calibration

