




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011438.D
Acq On : 12 Aug 2022 23:16
Operator : CG/JU
Sample : N4166-02
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBZ2

Manual IntegrationsAPPROVED

Quant Time: Aug 12 23:49:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 23:05:53 2022
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/13/2022
Supervised By :Sohil Jodhani 08/13/2022

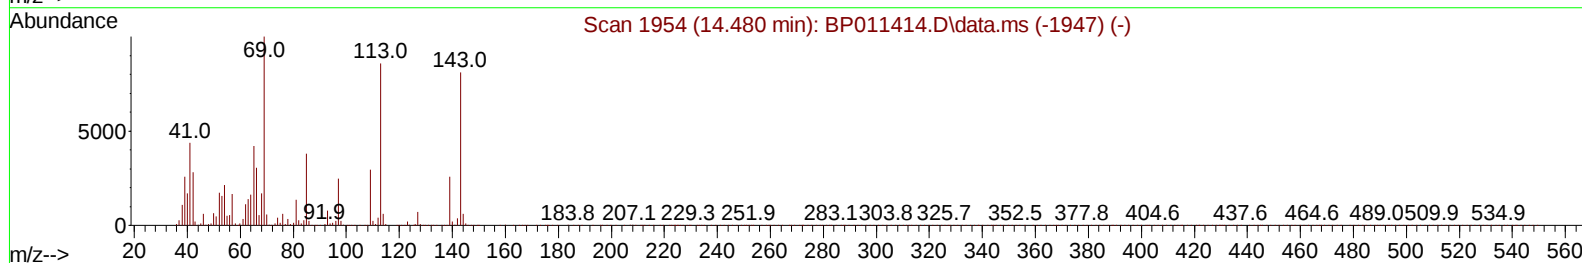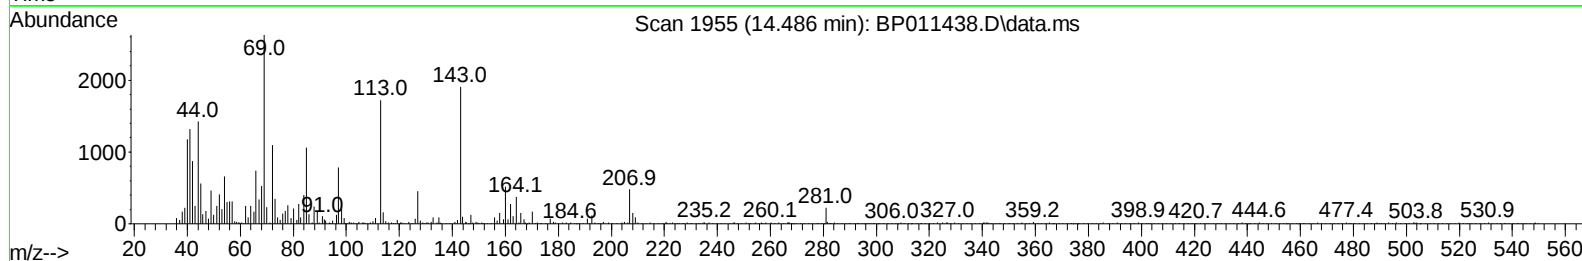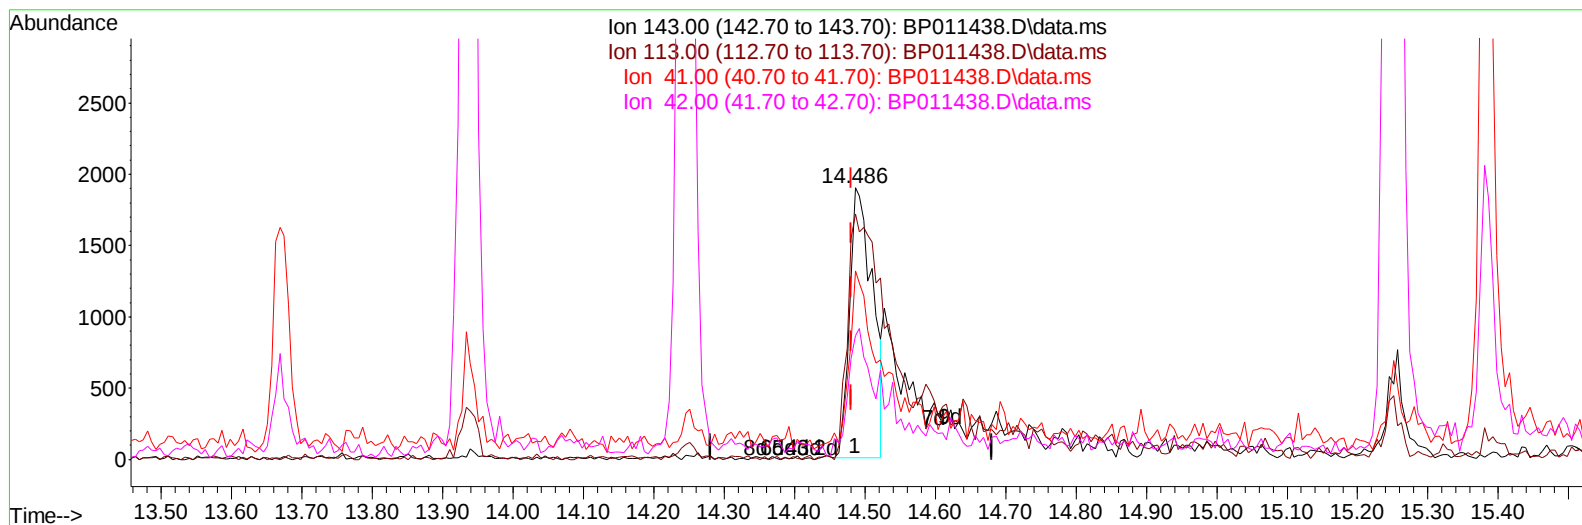

TIC: BP011438.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.486min (+ 0.006) 1.57 ng/u1

response 4228

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	75.70	90.39
41.00	54.40	69.43#
42.00	35.50	45.69#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011438.D
 Acq On : 12 Aug 2022 23:16
 Operator : CG/JU
 Sample : N4166-02
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBZ2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/13/2022
 Supervised By :Sohil Jodhani 08/13/2022

Quant Time: Aug 12 23:49:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 11 23:05:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.575	152	81235	20.000	ng/ul	0.00
20) Naphthalene-d8	10.363	136	354772	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.245	164	213033	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.022	188	441811	20.000	ng/ul	0.00
79) Chrysene-d12	21.151	240	433312	20.000	ng/ul	0.00
88) Perylene-d12	23.456	264	449672	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.081	96	10867	4.101	ng/uL	0.00
4) Pyridine-d5	3.493	84	55648	8.325	ng/ul	0.00
7) Phenol-d5	6.757	99	34390	4.784	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.922	67	135863	26.653	ng/ul	0.00
11) 2-Chlorophenol-d4	7.104	132	114460	20.292	ng/ul	0.00
15) 4-Methylphenol-d8	8.293	113	68445	12.125	ng/ul	-0.01
21) Nitrobenzene-d5	8.740	128	76851	31.829	ng/ul	0.00
24) 2-Nitrophenol-d4	9.457	143	71122	32.174	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.987	165	109292	24.482	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.516	131	179800	23.038	ng/ul	0.00
46) Dimethylphthalate-d6	13.675	166	494937	33.484	ng/ul	0.00
49) Acenaphthylene-d8	13.939	160	526151	29.571	ng/ul	0.00
54) 4-Nitrophenol-d4	14.486	143	6010m	2.226	ng/ul	0.00
60) Fluorene-d10	15.251	176	404704	32.015	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.386	200	54356	26.487	ng/ul	0.00
73) Anthracene-d10	17.122	188	718952	36.204	ng/ul	0.00
81) Pyrene-d10	19.380	212	804608	33.704	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.309	264	797820	35.182	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011438.D
Acq On : 12 Aug 2022 23:16
Operator : CG/JU
Sample : N4166-02
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBZ2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/13/2022
Supervised By :Sohil Jodhani 08/13/2022

Quant Time: Aug 12 23:49:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 23:05:53 2022
Response via : Initial Calibration

