




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011439.D
 Acq On : 12 Aug 2022 23:51
 Operator : CG/JU
 Sample : N4166-03
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBZ6

Manual IntegrationsAPPROVED

Quant Time: Aug 13 00:15:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 11 23:05:53 2022
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/13/2022
 Supervised By :Sohil Jodhani 08/13/2022

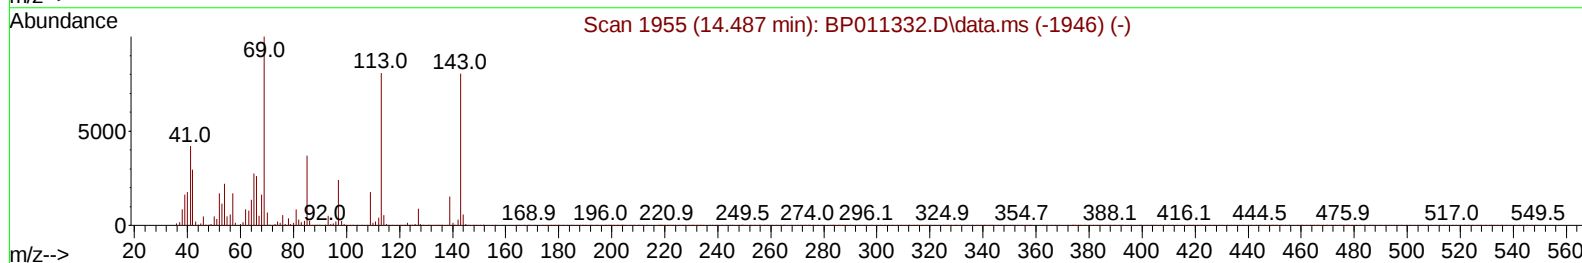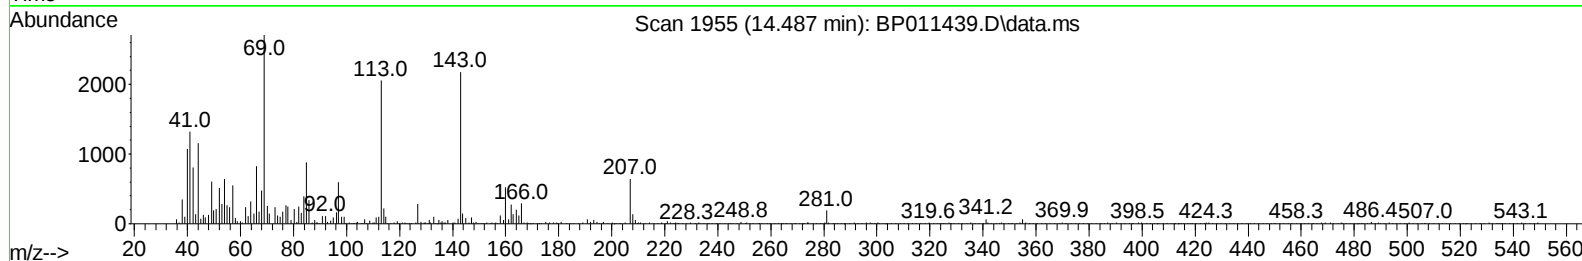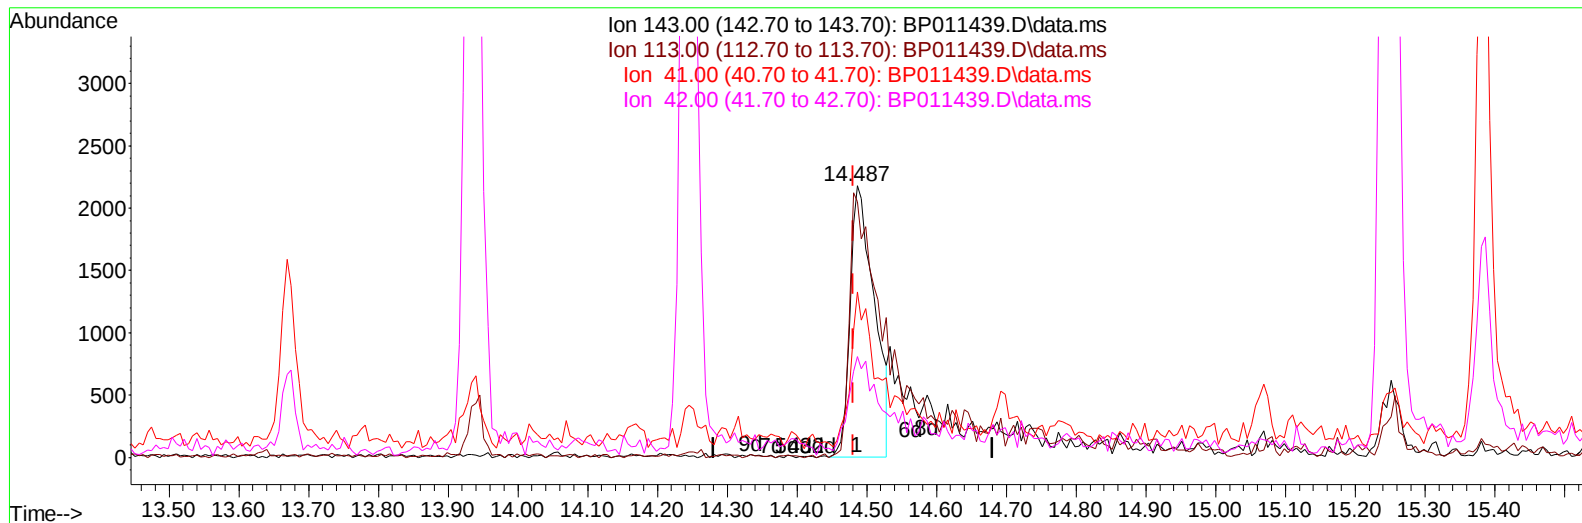

TIC: BP011439.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.487min (+ 0.006) 1.93 ng/u1

response 5210

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	75.70	94.26#
41.00	54.40	60.88
42.00	35.50	37.14




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011439.D
Acq On : 12 Aug 2022 23:51
Operator : CG/JU
Sample : N4166-03
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBZ6

Manual IntegrationsAPPROVED

Quant Time: Aug 13 00:15:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 23:05:53 2022
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/13/2022
Supervised By :Sohil Jodhani 08/13/2022

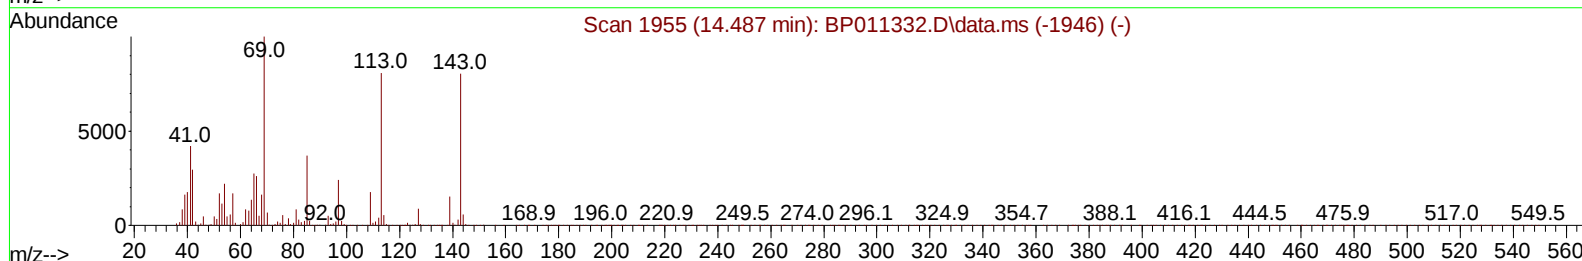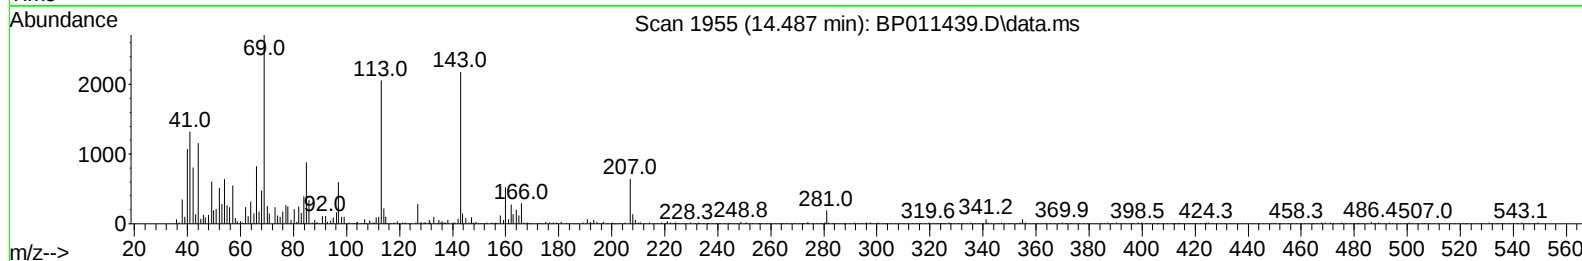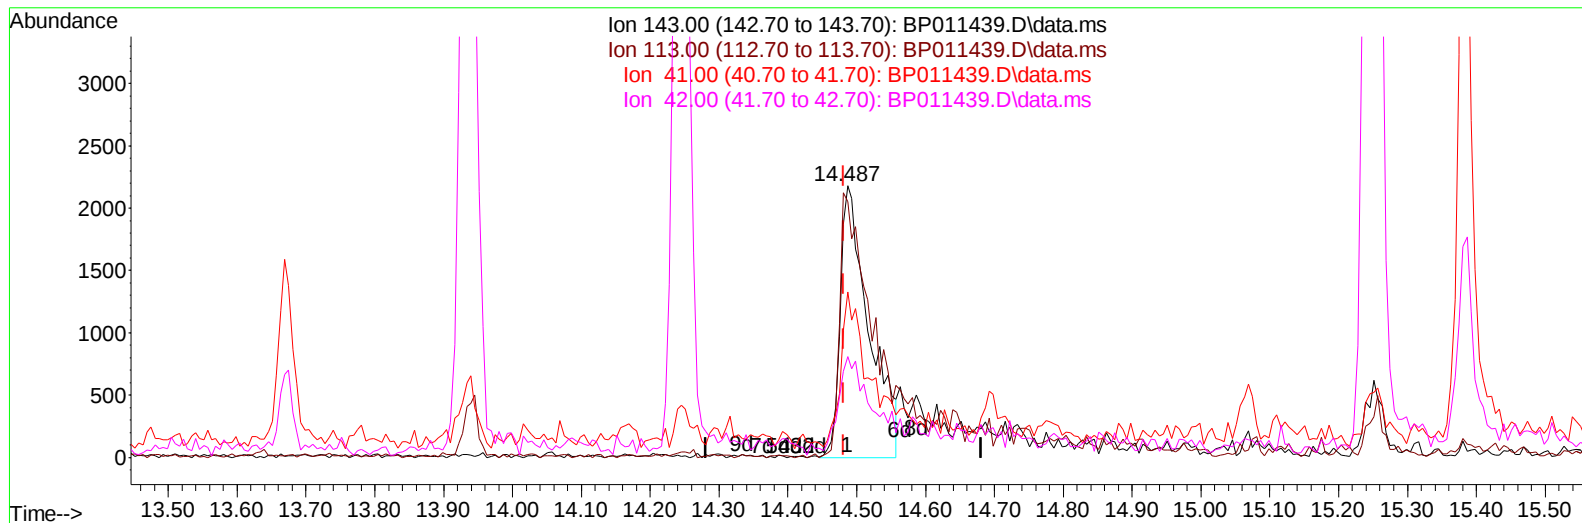

TIC: BP011439.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.487min (+ 0.006) 2.34 ng/ul m

response 6316

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	75.70	94.26#
41.00	54.40	60.88
42.00	35.50	37.14

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011439.D
 Acq On : 12 Aug 2022 23:51
 Operator : CG/JU
 Sample : N4166-03
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBZ6

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/13/2022
 Supervised By :Sohil Jodhani 08/13/2022

Quant Time: Aug 13 00:15:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 11 23:05:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.569	152	85076	20.000	ng/ul	0.00
20) Naphthalene-d8	10.363	136	368094	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.245	164	212756	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.022	188	442284	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.151	240	433864	20.000	ng/ul	0.00
88) Perylene-d12	23.457	264	461026	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.081	96	10987	3.959	ng/uL	0.00
4) Pyridine-d5	3.493	84	51415	7.345	ng/ul	0.00
7) Phenol-d5	6.758	99	34196	4.542	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.922	67	137563	25.768	ng/ul	0.00
11) 2-Chlorophenol-d4	7.105	132	116472	19.716	ng/ul	0.00
15) 4-Methylphenol-d8	8.293	113	70615	11.945	ng/ul	-0.01
21) Nitrobenzene-d5	8.734	128	76273	30.447	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.451	143	70448	30.715	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	9.987	165	111845	24.147	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.516	131	157463	19.446	ng/ul	0.00
46) Dimethylphthalate-d6	13.669	166	493969	33.462	ng/ul	-0.01
49) Acenaphthylene-d8	13.934	160	516495	29.066	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.487	143	6316m	2.343	ng/ul	0.00
60) Fluorene-d10	15.251	176	397443	31.482	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.386	200	53539	26.061	ng/ul	0.00
73) Anthracene-d10	17.122	188	682894	34.351	ng/ul	0.00
81) Pyrene-d10	19.386	212	791459	33.111	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.310	264	787800	33.884	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011439.D
Acq On : 12 Aug 2022 23:51
Operator : CG/JU
Sample : N4166-03
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBZ6

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/13/2022
Supervised By :Sohil Jodhani 08/13/2022

Quant Time: Aug 13 00:15:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 23:05:53 2022
Response via : Initial Calibration

