




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011440.D
Acq On : 13 Aug 2022 00:25
Operator : CG/JU
Sample : N4166-04
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBZ7

Manual IntegrationsAPPROVED

Quant Time: Aug 13 00:53:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 23:05:53 2022
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/13/2022
Supervised By :Sohil Jodhani 08/13/2022

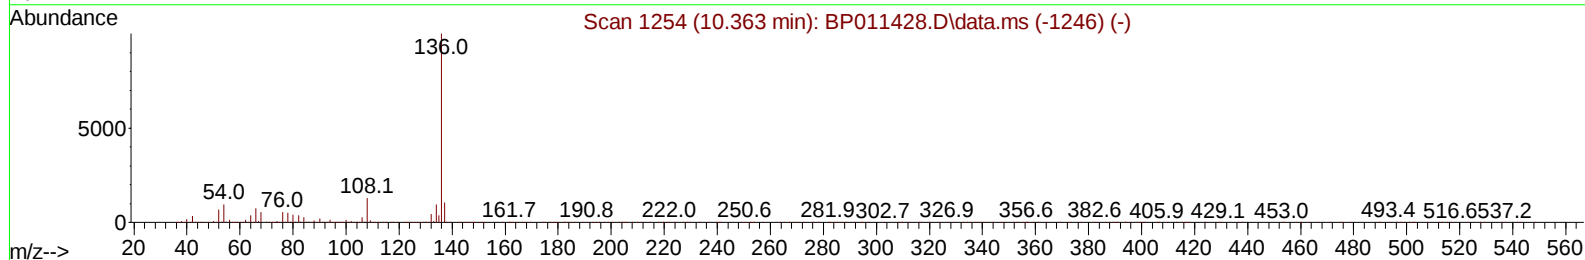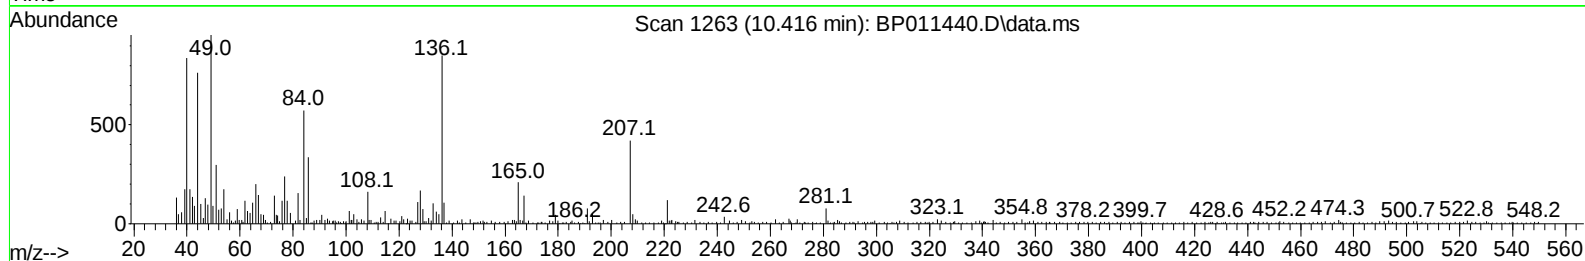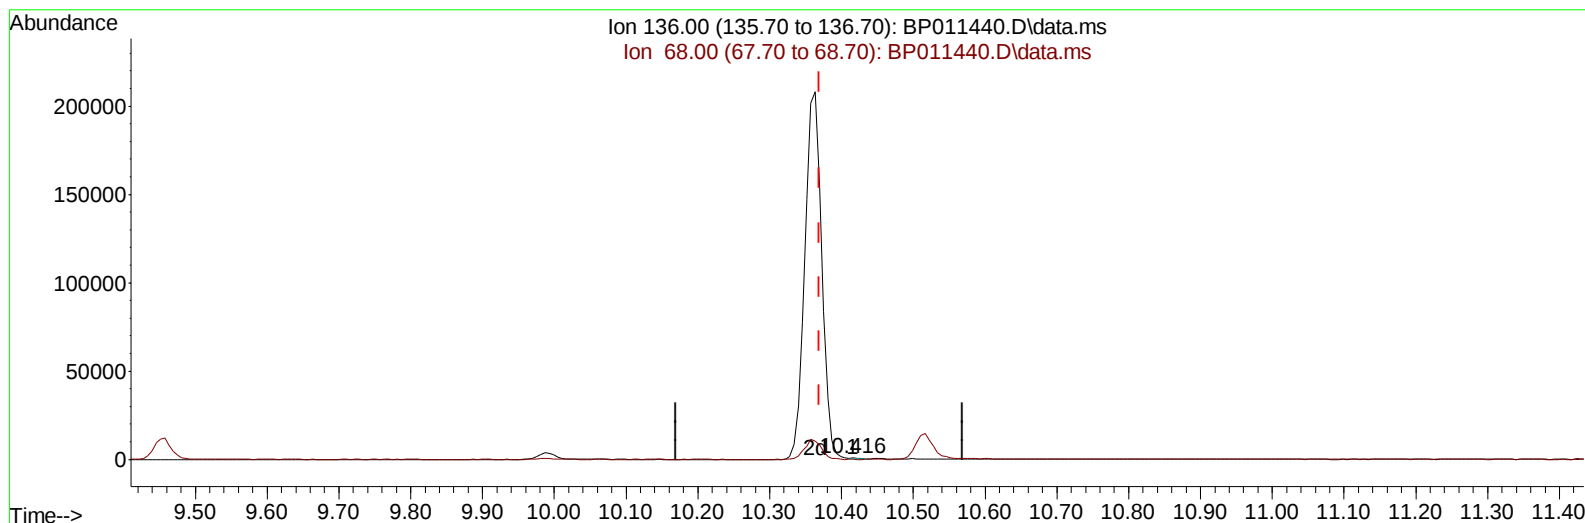

TIC: BP011440.D\data.ms

(20) Naphthalene-d8 (I)

10.416min (+ 0.047) 20.00 ng/u1

response 585

Ion	Exp%	Act%
136.00	100.00	100.00
68.00	6.70	5.88
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011440.D
 Acq On : 13 Aug 2022 00:25
 Operator : CG/JU
 Sample : N4166-04
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBZ7

Manual IntegrationsAPPROVED

Quant Time: Aug 13 00:53:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 11 23:05:53 2022
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/13/2022
 Supervised By :Sohil Jodhani 08/13/2022

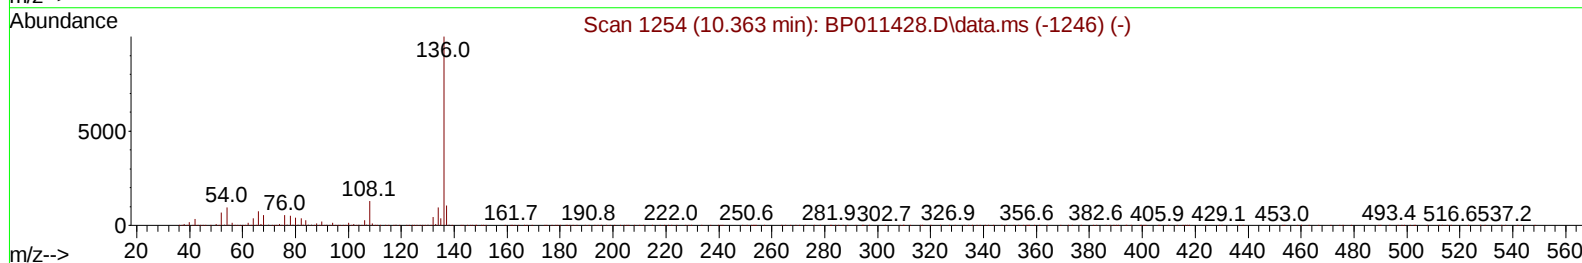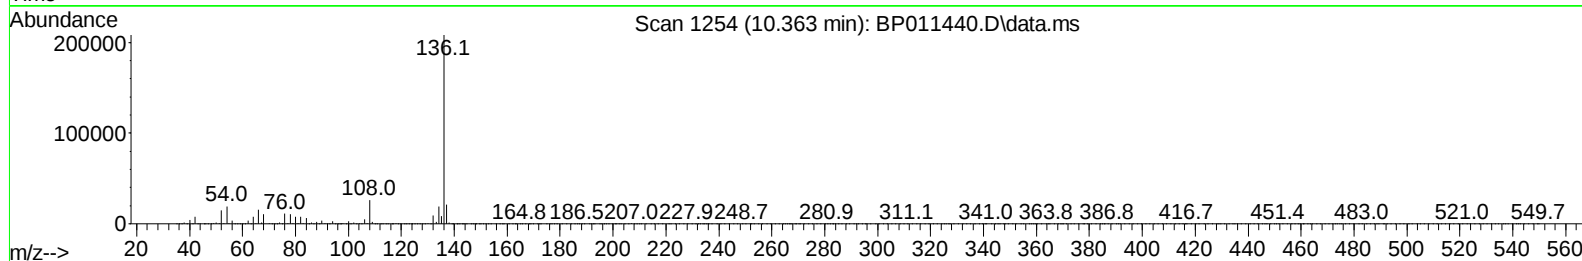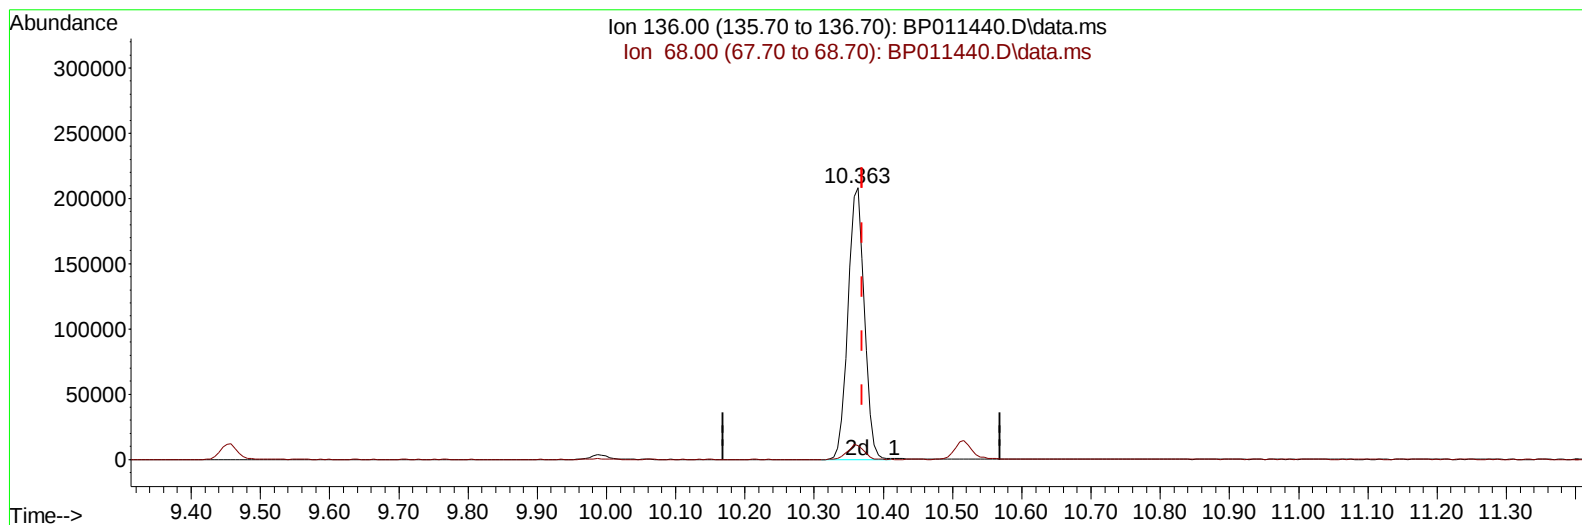

TIC: BP011440.D\data.ms

(20) Naphthalene-d8 (I)

10.363min (-0.006) 20.00 ng/ul m

response 340536

Ion	Exp%	Act%
136.00	100.00	100.00
68.00	6.70	5.01#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011440.D
 Acq On : 13 Aug 2022 00:25
 Operator : CG/JU
 Sample : N4166-04
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBZ7

Manual IntegrationsAPPROVED

Quant Time: Aug 13 00:53:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 11 23:05:53 2022
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/13/2022
 Supervised By :Sohil Jodhani 08/13/2022

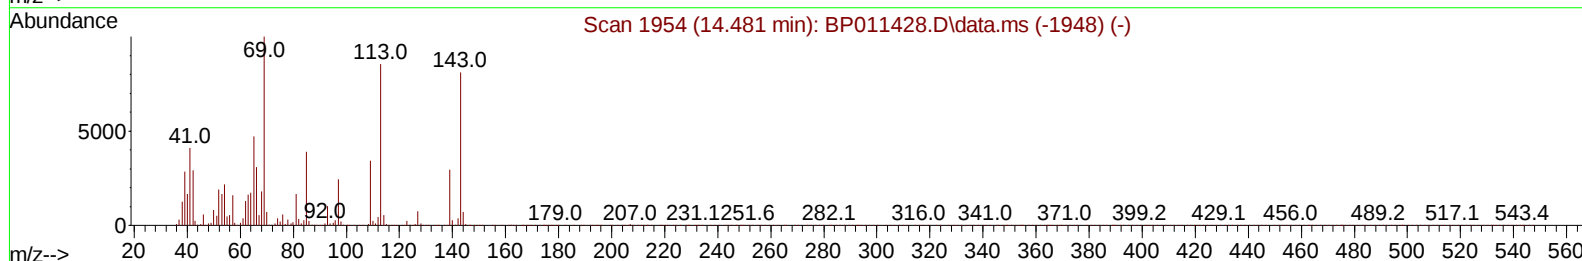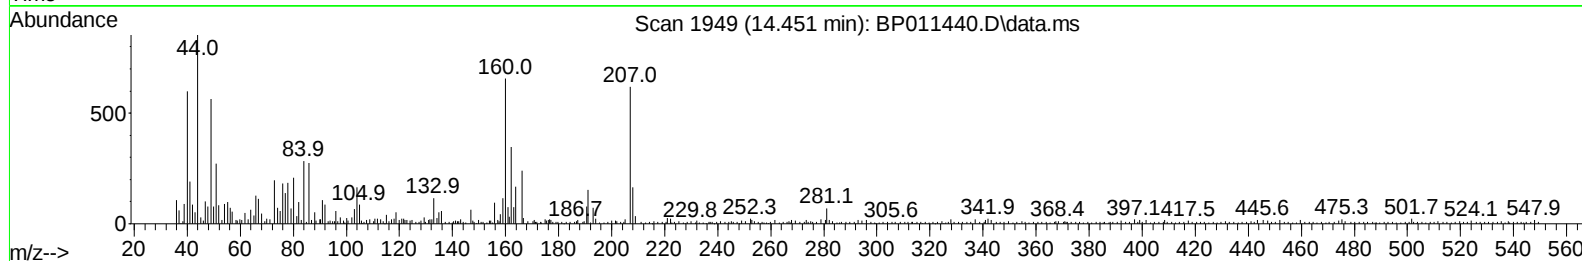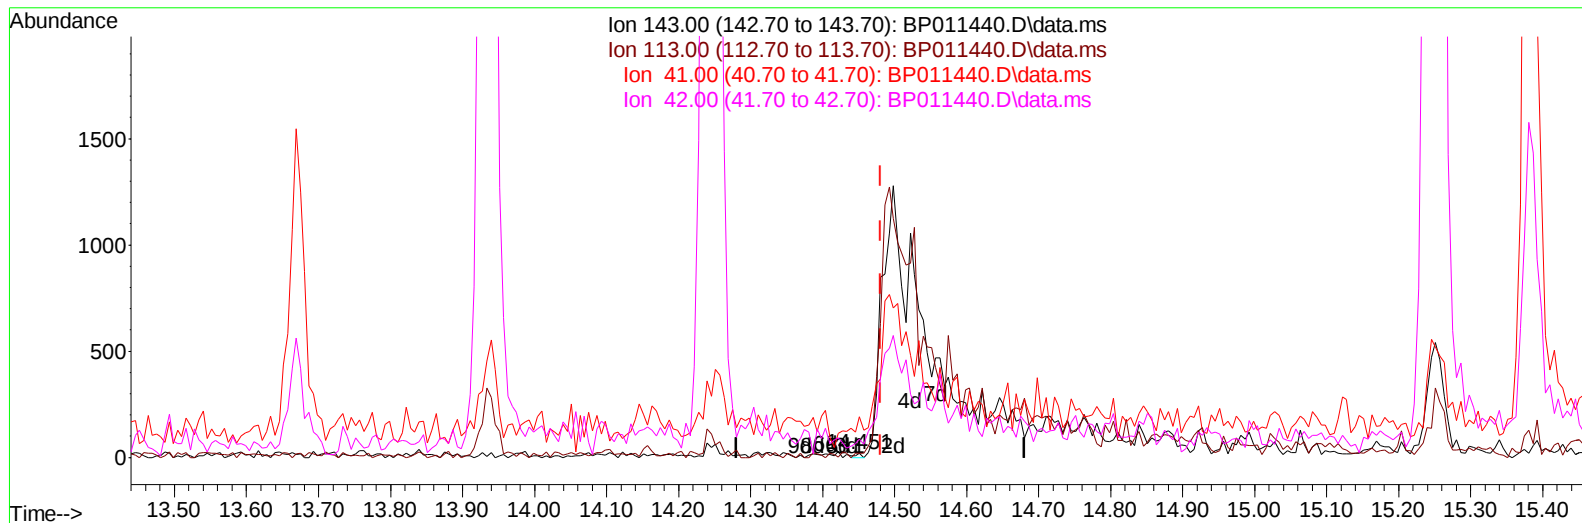

TIC: BP011440.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.451min (-0.029) 0.00 ng/u1

response 10

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	75.70	105.26#
41.00	54.40	1000.00#
42.00	35.50	452.63#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011440.D
Acq On : 13 Aug 2022 00:25
Operator : CG/JU
Sample : N4166-04
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBZ7

Manual IntegrationsAPPROVED

Quant Time: Aug 13 00:53:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 23:05:53 2022
Response via : Initial Calibration

Reviewed By :Yogesh Patel 08/13/2022
Supervised By :Sohil Jodhani 08/13/2022

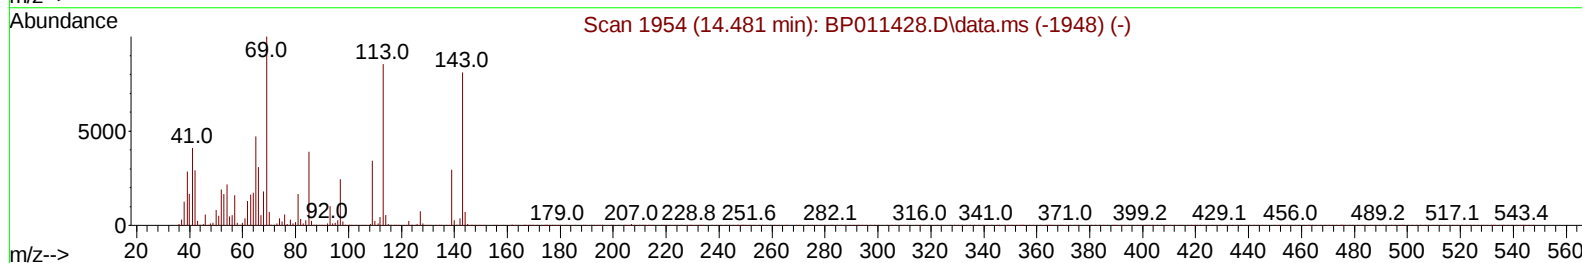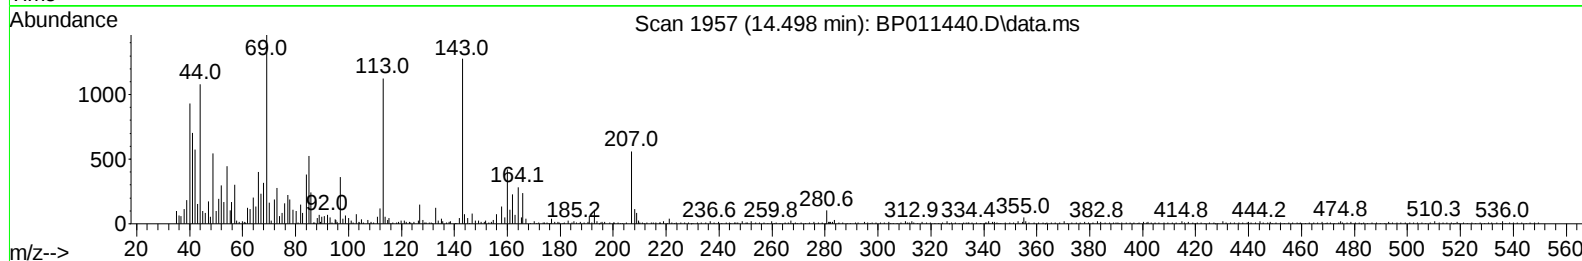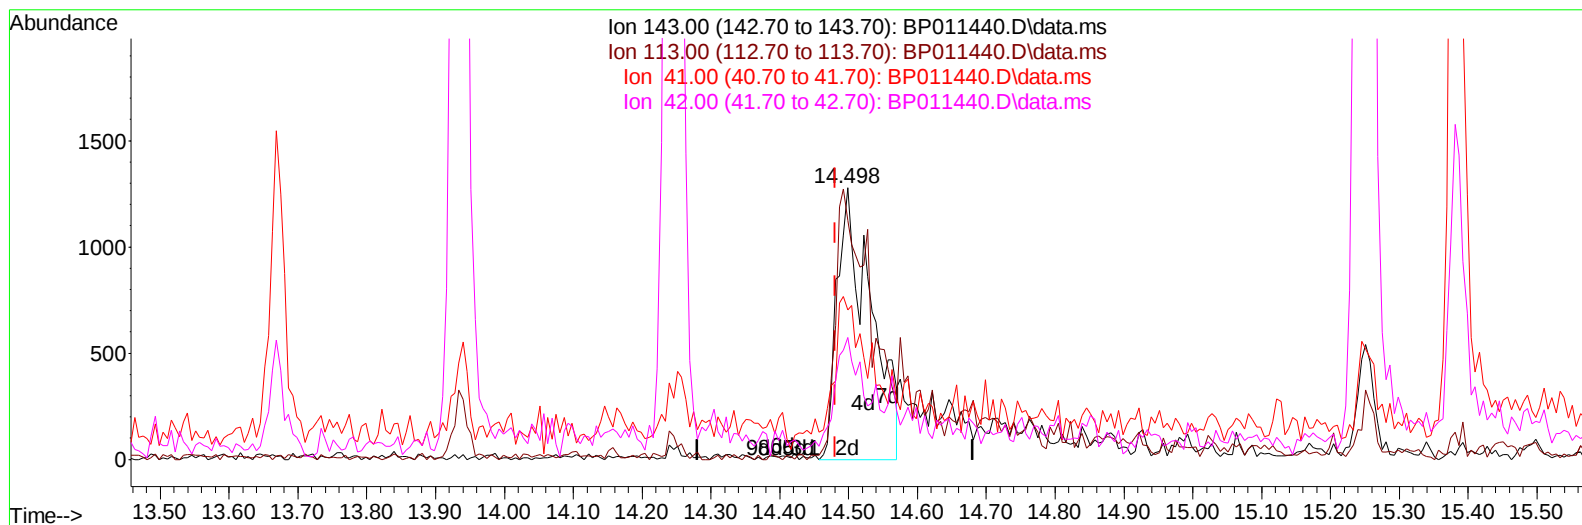

TIC: BP011440.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.498min (+ 0.018) 1.74 ng/ul m

response 4340

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	75.70	88.03
41.00	54.40	55.16
42.00	35.50	44.84#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011440.D
 Acq On : 13 Aug 2022 00:25
 Operator : CG/JU
 Sample : N4166-04
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBZ7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/13/2022
 Supervised By :Sohil Jodhani 08/13/2022

Quant Time: Aug 13 00:53:27 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Aug 11 23:05:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.569	152	80221	20.000	ng/ul	0.00
20) Naphthalene-d8	10.363	136	340536m	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.246	164	196263	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.022	188	408977	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.151	240	415080	20.000	ng/ul	# 0.00
88) Perylene-d12	23.457	264	448067	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.075	96	10839	4.142	ng/uL	0.00
4) Pyridine-d5	3.493	84	51813	7.849	ng/ul	0.00
7) Phenol-d5	6.758	99	25140	3.541	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.922	67	123519	24.538	ng/ul	0.00
11) 2-Chlorophenol-d4	7.105	132	93824	16.844	ng/ul	0.00
15) 4-Methylphenol-d8	8.293	113	53905	9.670	ng/ul	-0.01
21) Nitrobenzene-d5	8.734	128	66559	28.719	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.458	143	60096	28.322	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.987	165	91354	21.319	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.516	131	151921	20.279	ng/ul	0.00
46) Dimethylphthalate-d6	13.669	166	418183	30.709	ng/ul	-0.01
49) Acenaphthylene-d8	13.934	160	444304	27.104	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.498	143	4340m	1.745	ng/ul	0.02
60) Fluorene-d10	15.251	176	347084	29.803	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.387	200	47149	24.820	ng/ul	0.00
73) Anthracene-d10	17.122	188	614076	33.405	ng/ul	0.00
81) Pyrene-d10	19.381	212	726260	31.758	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.310	264	742343	32.852	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011440.D
Acq On : 13 Aug 2022 00:25
Operator : CG/JU
Sample : N4166-04
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBZ7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 08/13/2022
Supervised By :Sohil Jodhani 08/13/2022

Quant Time: Aug 13 00:53:27 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Aug 11 23:05:53 2022
Response via : Initial Calibration

