

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011394.D
 Acq On : 11 Aug 2022 19:04
 Operator : CG/JU
 Sample : PB146900BS
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLCS900

Quant Time: Aug 11 22:48:07 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 08 18:47:19 2022
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By :Jagrut Upadhyay 08/12/2022
 Supervised By :Sohil Jodhani 08/13/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.581	152	99955	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.369	136	434045	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.257	164	258844	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.028	188	529090	20.000	ng/u1	-0.01
79) Chrysene-d12	21.157	240	509865	20.000	ng/u1	-0.01
88) Perylene-d12	23.469	264	502628	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.081	96	19554	5.997	ng/uL	0.00
4) Pyridine-d5	3.487	84	241760	29.394	ng/u1	-0.01
7) Phenol-d5	6.764	99	291869	32.995	ng/u1	-0.01
9) Bis-(2-Chloroethyl)eth...	6.928	67	191242	30.491	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.111	132	233543	33.649	ng/u1	-0.01
15) 4-Methylphenol-d8	8.305	113	231093	33.272	ng/u1	-0.01
21) Nitrobenzene-d5	8.746	128	113148	38.303	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.463	143	113282	41.886	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	9.999	165	201574	36.907	ng/u1	-0.01
31) 4-Chloroaniline-d4	10.522	131	294371	30.829	ng/u1	-0.01
46) Dimethylphthalate-d6	13.681	166	655430	36.494	ng/u1	0.00
49) Acenaphthylene-d8	13.946	160	769161	35.578	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.487	143	118512	36.128	ng/u1	0.00
60) Fluorene-d10	15.257	176	530813	34.560	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.393	200	98196	39.957	ng/u1	0.00
73) Anthracene-d10	17.128	188	820022	34.482	ng/u1	-0.01
81) Pyrene-d10	19.392	212	927200	33.008	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.322	264	909786	35.892	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.117	88	39503	11.406	ng/uL#	83
5) Pyridine	3.511	79	235348	27.471	ng/u1	90
6) Benzaldehyde	6.734	77	168082	43.601	ng/u1	98
8) Phenol	6.793	94	288193	30.099	ng/u1	92
10) Bis(2-Chloroethyl)ether	7.022	93	228895	29.683	ng/u1	95
12) 2-Chlorophenol	7.146	128	236645	32.721	ng/u1	97
13) 2-Methylphenol	8.034	108	214444	31.098	ng/u1	100
14) 2,2'-oxybis(1-Chloropr...	8.122	45	337773	29.205	ng/u1#	95
16) Acetophenone	8.411	105	364287	32.418	ng/u1	97
17) N-Nitroso-di-n-propyla...	8.405	70	193272	34.913	ng/u1	97
18) 4-Methylphenol	8.369	108	230728	31.216	ng/u1	97
19) Hexachloroethane	8.646	117	103918	34.030	ng/u1	99
22) Nitrobenzene	8.787	77	284788	34.439	ng/u1	98
23) Isophorone	9.316	82	525674	34.655	ng/u1	98
25) 2-Nitrophenol	9.493	139	123746	39.260	ng/u1#	85
26) 2,4-Dimethylphenol	9.563	107	266216	33.427	ng/u1	94
27) Bis(2-Chloroethoxy)met...	9.805	93	308865	31.862	ng/u1	98
29) 2,4-Dichlorophenol	10.028	162	198058	34.677	ng/u1	99
30) Naphthalene	10.422	128	732299	31.010	ng/u1	99
32) 4-Chloroaniline	10.546	127	260941	27.264	ng/u1	99
33) Hexachlorobutadiene	10.705	225	124752	35.604	ng/u1	97
34) Caprolactam	11.346	113	69705m	36.495	ng/u1	
35) 4-Chloro-3-methylphenol	11.687	107	252906	37.661	ng/u1	96
36) 2-Methylnaphthalene	12.046	142	482223	32.944	ng/u1	98

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011394.D
 Acq On : 11 Aug 2022 19:04
 Operator : CG/JU
 Sample : PB146900BS
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLCS900


Quant Time: Aug 11 22:48:07 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Aug 08 18:47:19 2022
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By :Jagrut Upadhyay 08/12/2022
 Supervised By :Sohil Jodhani 08/13/2022


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.269	142	487482	32.832	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.422	216	214169	31.429	ng/ul	97
40) Hexachlorocyclopentadiene	12.393	237	110876	30.364	ng/ul	98
41) 2,4,6-Trichlorophenol	12.675	196	144753	35.108	ng/ul	100
42) 2,4,5-Trichlorophenol	12.746	196	156999	35.677	ng/ul	100
43) 1,1'-Biphenyl	13.081	154	620784	30.542	ng/ul	98
44) 2-Chloronaphthalene	13.116	162	474771	31.132	ng/ul	96
45) 2-Nitroaniline	13.340	65	176008	45.442	ng/ul	98
47) Dimethylphthalate	13.728	163	635031	34.910	ng/ul	99
48) 2,6-Dinitrotoluene	13.851	165	122818	43.181	ng/ul	97
50) Acenaphthylene	13.975	152	798906	32.058	ng/ul	99
51) 3-Nitroaniline	14.181	138	133223	42.580	ng/ul	98
52) Acenaphthene	14.322	153	530712	31.931	ng/ul	98
53) 2,4-Dinitrophenol	14.387	184	62651	37.126	ng/ul#	87
55) 4-Nitrophenol	14.498	109	129755	42.640	ng/ul#	72
56) Dibenzofuran	14.657	168	720981	31.997	ng/ul	90
57) 2,4-Dinitrotoluene	14.640	165	185893	42.640	ng/ul	94
58) 2,3,4,6-Tetrachlorophenol	14.893	232	127051	37.113	ng/ul#	95
59) Diethylphthalate	15.104	149	709086	37.628	ng/ul	97
61) Fluorene	15.316	166	602085	32.902	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.316	204	268794	33.603	ng/ul	89
63) 4-Nitroaniline	15.357	138	148716m	48.847	ng/ul	
66) 4,6-Dinitro-2-methylph...	15.410	198	94285	37.258	ng/ul#	91
67) N-Nitrosodiphenylamine	15.540	169	512723	32.885	ng/ul	99
68) 4-Bromophenyl-phenylether	16.222	248	157283	33.593	ng/ul	93
69) Hexachlorobenzene	16.322	284	182076	33.287	ng/ul	95
70) Atrazine	16.510	200	150805	29.019	ng/ul	96
71) Pentachlorophenol	16.675	266	106795	33.632	ng/ul	98
72) Phenanthrene	17.069	178	948331	31.965	ng/ul	99
74) Anthracene	17.163	178	956568	32.388	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.040	216	212784	28.014	ng/uL	98
76) Pentachlorobenzene	14.575	250	205252	31.028	ng/uL	98
77) Carbazole	17.445	167	896939	32.499	ng/ul	98
78) Di-n-butylphthalate	18.016	149	1221121	40.463	ng/ul	99
80) Fluoranthene	19.063	202	1094784	32.020	ng/ul	94
82) Pyrene	19.422	202	1127726	31.249	ng/ul#	92
83) Butylbenzylphthalate	20.322	149	554665	48.231	ng/ul	98
84) 3,3'-Dichlorobenzidine	21.086	252	347998	37.503	ng/ul	99
85) Benzo(a)anthracene	21.145	228	1061194	32.442	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.086	149	833991	45.174	ng/ul	97
87) Chrysene	21.198	228	1061926	32.795	ng/ul	99
89) Di-n-octyl phthalate	21.986	149	1392021	39.916	ng/ul	100
90) Benzo(b)fluoranthene	22.769	252	1123299	33.956	ng/ul	98
91) Benzo(k)fluoranthene	22.816	252	1014470	31.343	ng/ul	97
93) Benzo(a)pyrene	23.369	252	1068593	33.491	ng/ul	97
94) Indeno(1,2,3-cd)pyrene	25.851	276	1175733	33.333	ng/ul	95
95) Dibenzo(a,h)anthracene	25.868	278	1008501	33.619	ng/ul#	93
96) Benzo(g,h,i)perylene	26.580	276	1003572	33.718	ng/ul	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2
1,4-Dioxane
Concen: 11.406 ng/uL
RT: 3.117 min Scan# 21
Delta R.T. -0.005 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04




Instrument :
BNA_P
ClientSampleId :
SLCS900



Tgt Ion: 88 Resp: 39500
Ion Ratio Lower Upper
88 100
43 37.4 29.6 44.4
58 81.6 49.1 73.7




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 08/12/2022
Supervised By :Sohil Jodhani 08/13/2022



#5
Pyridine
Concen: 27.471 ng/uL
RT: 3.511 min Scan# 89
Delta R.T. -0.006 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04


Tgt Ion: 79 Resp: 235348
Ion Ratio Lower Upper
79 100
52 81.7 57.8 86.6
51 44.1 31.5 47.3

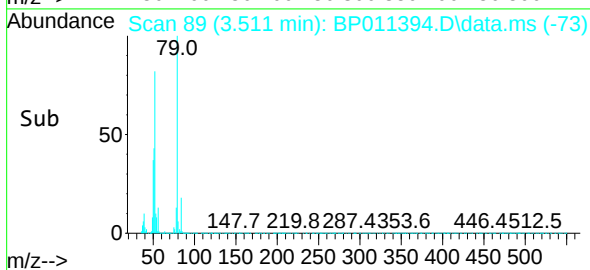



#6
Benzaldehyde
Concen: 43.601 ng/ul
RT: 6.734 min Scan# 61
Delta R.T. -0.012 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04




Instrument :
BNA_P
ClientSampleId :
SLCS900




Tgt Ion: 77 Resp: 168082
Ion Ratio Lower Upper
77 100
105 91.6 72.0 108.0
106 88.3 69.4 104.0

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 08/12/2022
Supervised By :Sohil Jodhani 08/13/2022

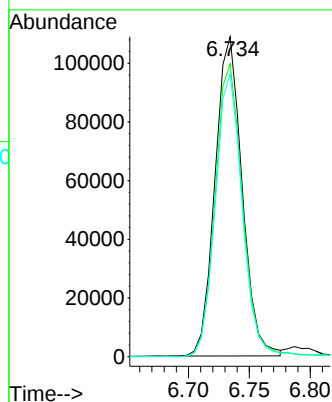


#8
Phenol
Concen: 30.099 ng/ul
RT: 6.793 min Scan# 647
Delta R.T. -0.006 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04




Tgt Ion: 94 Resp: 288193
Ion Ratio Lower Upper
94 100
65 34.2 24.7 37.1
66 46.2 32.6 49.0





#10
Bis(2-Chloroethyl)ether
Concen: 29.683 ng/ul
RT: 7.022 min Scan# 686
Delta R.T. -0.006 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04




Instrument :
BNA_P
Client Sample Id :
SLCS900




Tgt Ion: 93 Resp: 228895
Ion Ratio Lower Upper
93 100
63 82.5 71.0 106.6
95 31.4 26.0 39.0

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 08/12/2022
Supervised By :Sohil Jodhani 08/13/2022




#12
2-Chlorophenol
Concen: 32.721 ng/ul
RT: 7.146 min Scan# 707
Delta R.T. -0.012 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04




Tgt Ion:128 Resp: 236645
Ion Ratio Lower Upper
128 100
64 52.2 43.8 65.6
130 32.7 25.4 38.2

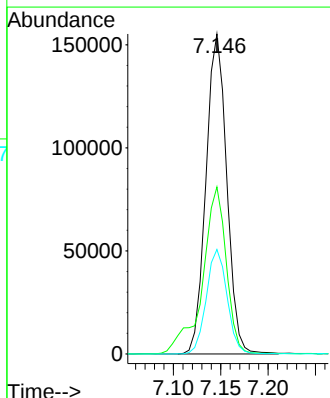



#13
2-Methylphenol
Concen: 31.098 ng/ul
RT: 8.034 min Scan# 81
Delta R.T. -0.012 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04




Instrument :
BNA_P
ClientSampleId :
SLCS900



Tgt Ion:108 Resp: 21444
Ion Ratio Lower Upper
108 100
107 90.1 71.8 107.6




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 08/12/2022
Supervised By :Sohil Jodhani 08/13/2022



#14
2,2'-oxybis(1-Chloropropane)
Concen: 29.205 ng/ul
RT: 8.122 min Scan# 873
Delta R.T. -0.012 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04


Tgt Ion: 45 Resp: 337773
Ion Ratio Lower Upper
45 100
77 14.0 9.9 14.9
79 10.9 7.2 10.8#





#16
Acetophenone
Concen: 32.418 ng/ul
RT: 8.411 min Scan# 911
Delta R.T. -0.012 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04




Instrument :
BNA_P
ClientSampleId :
SLCS900



Tgt Ion: 105 Resp: 36428
Ion Ratio Lower Upper
105 100
77 84.6 65.4 98.0
51 34.6 26.5 39.7




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 08/12/2022
Supervised By :Sohil Jodhani 08/13/2022



#17
N-Nitroso-di-n-propylamine
Concen: 34.913 ng/ul
RT: 8.405 min Scan# 921
Delta R.T. -0.006 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04


Tgt Ion: 70 Resp: 193272
Ion Ratio Lower Upper
70 100
42 67.3 55.5 83.3
101 9.6 7.1 10.7
130 20.2 14.8 22.2





#18
4-Methylphenol
Concen: 31.216 ng/ul
RT: 8.369 min Scan# 915
Delta R.T. -0.006 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04




Instrument :
BNA_P
ClientSampleId :
SLCS900



Tgt Ion:108 Resp: 230728
Ion Ratio Lower Upper
108 100
107 113.6 88.2 132.4




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 08/12/2022
Supervised By :Sohil Jodhani 08/13/2022



#19
Hexachloroethane
Concen: 34.030 ng/ul
RT: 8.646 min Scan# 962
Delta R.T. -0.012 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04


Tgt Ion:117 Resp: 103918
Ion Ratio Lower Upper
117 100
201 77.4 62.2 93.2
199 48.3 39.8 59.6





#22
Nitrobenzene
Concen: 34.439 ng/ul
RT: 8.787 min Scan# 986
Delta R.T. -0.012 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04




Instrument :
BNA_P
ClientSampleId :
SLCS900




Tgt Ion: 77 Resp: 284788
Ion Ratio Lower Upper
77 100
123 40.2 31.4 47.0
65 14.6 10.6 15.8

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 08/12/2022
Supervised By :Sohil Jodhani 08/13/2022




#23
Isophorone
Concen: 34.655 ng/ul
RT: 9.316 min Scan# 1076
Delta R.T. -0.012 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04



Tgt Ion: 82 Resp: 525674
Ion Ratio Lower Upper
82 100
95 8.6 5.8 8.8
138 16.3 12.6 18.8

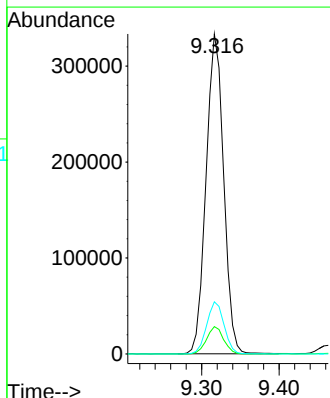







#25
2-Nitrophenol
Concen: 39.260 ng/ul
RT: 9.493 min Scan# 1106
Delta R.T. -0.012 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04

Instrument :
BNA_P
ClientSampleId :
SLCS900

Tgt Ion:139 Resp: 123740
Ion Ratio Lower Upper
139 100
65 66.6 46.7 70.1
109 43.4 24.2 36.2




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 08/12/2022
Supervised By :Sohil Jodhani 08/13/2022



#26
2,4-Dimethylphenol
Concen: 33.427 ng/ul
RT: 9.563 min Scan# 1118
Delta R.T. -0.012 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04

Tgt Ion:107 Resp: 266216
Ion Ratio Lower Upper
107 100
121 47.3 40.3 60.5
122 78.9 67.7 101.5





#27

Bis(2-Chloroethoxy)methane

Concen: 31.862 ng/ul

RT: 9.805 min Scan# 1159

Delta R.T. -0.012 min

Lab File: BP011394.D

Acq: 11 Aug 2022 19:04

Instrument :

BNA_P

ClientSampleId :

SLCS900

Tgt Ion: 93 Resp: 30886

Ion Ratio Lower Upper

93 100

95 32.6 25.2 37.8





123 10.1 8.4 12.6

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 08/12/2022

Supervised By :Sohil Jodhani 08/13/2022



#29

2,4-Dichlorophenol

Concen: 34.677 ng/ul

RT: 10.028 min Scan# 1197

Delta R.T. -0.006 min

Lab File: BP011394.D

Acq: 11 Aug 2022 19:04




Tgt Ion:162 Resp: 198058


Ion Ratio Lower Upper

162 100

164 64.2 52.6 79.0


98 42.7 34.2 51.4

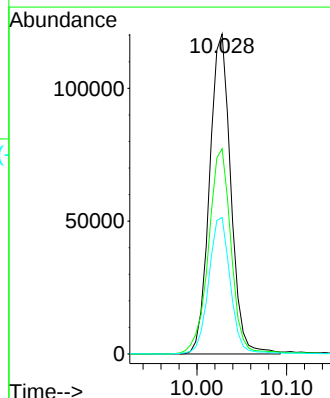



#30
Naphthalene
Concen: 31.010 ng/ul
RT: 10.422 min Scan# 1264
Delta R.T. -0.012 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04




Instrument :
BNA_P
ClientSampleId :
SLCS900




Tgt Ion:128 Resp: 732299
Ion Ratio Lower Upper
128 100
129 10.8 9.0 13.4
127 12.9 10.4 15.6

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 08/12/2022
Supervised By :Sohil Jodhani 08/13/2022




#32
4-Chloroaniline
Concen: 27.264 ng/ul
RT: 10.546 min Scan# 1285
Delta R.T. -0.012 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04




Tgt Ion:127 Resp: 260941
Ion Ratio Lower Upper
127 100
129 33.0 26.6 40.0

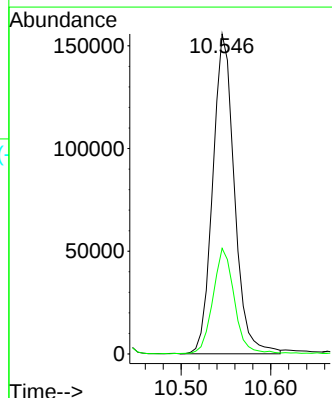



#33
Hexachlorobutadiene
Concen: 35.604 ng/ul
RT: 10.705 min Scan# 1312
Delta R.T. -0.012 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04




Instrument :
BNA_P
ClientSampleId :
SLCS900



Tgt Ion:225 Resp: 124752
Ion Ratio Lower Upper
225 100
223 60.6 51.2 76.8
227 62.6 50.6 75.8




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 08/12/2022
Supervised By :Sohil Jodhani 08/13/2022



#34
Caprolactam
Concen: 36.495 ng/ul m
RT: 11.346 min Scan# 1421
Delta R.T. -0.006 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04


Tgt Ion:113 Resp: 69705
Ion Ratio Lower Upper
113 100
55 186.5 164.2 246.4
56 140.7 127.0 190.6

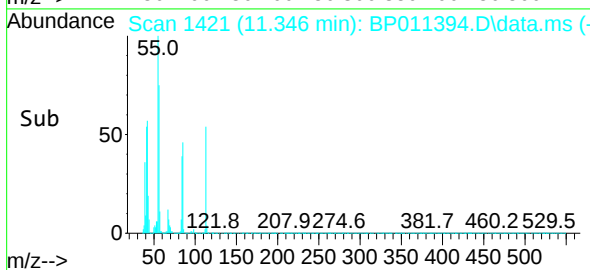



#35
4-Chloro-3-methylphenol
Concen: 37.661 ng/ul
RT: 11.687 min Scan# 14
Delta R.T. -0.012 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04



Instrument :
BNA_P
ClientSampleId :
SLCS900

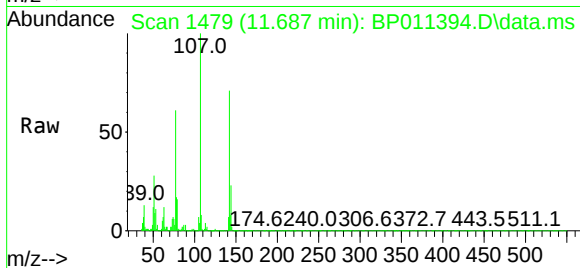


Tgt Ion:107 Resp: 252900
Ion Ratio Lower Upper
107 100
144 22.8 19.0 28.4
142 71.0 59.8 89.8

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 08/12/2022
Supervised By :Sohil Jodhani 08/13/2022

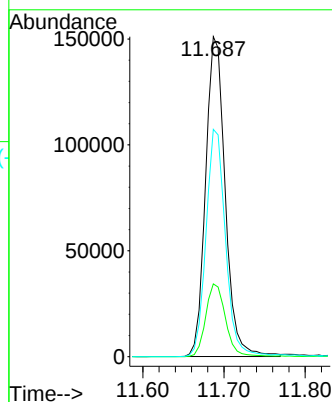


#36
2-Methylnaphthalene
Concen: 32.944 ng/ul
RT: 12.046 min Scan# 1540
Delta R.T. -0.012 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04



Tgt Ion:142 Resp: 482223
Ion Ratio Lower Upper
142 100
141 91.3 71.8 107.8

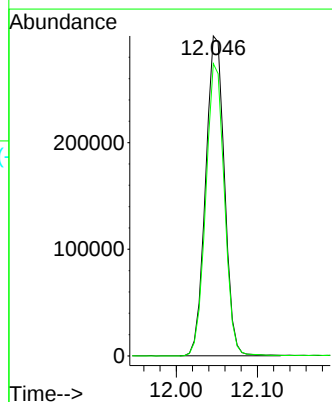







#37
1-Methylnaphthalene
Concen: 32.832 ng/ul
RT: 12.269 min Scan# 1578
Delta R.T. -0.012 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04

Instrument :
BNA_P
ClientSampleId :
SLCS900

Tgt Ion:142 Resp: 48748
Ion Ratio Lower Upper
142 100
141 91.8 74.1 111.1
116 4.9 3.4 5.0




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 08/12/2022
Supervised By :Sohil Jodhani 08/13/2022



#39
1,2,4,5-Tetrachlorobenzene
Concen: 31.429 ng/ul
RT: 12.422 min Scan# 1604
Delta R.T. -0.012 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04


Tgt Ion:216 Resp: 214169
Ion Ratio Lower Upper
216 100
214 78.2 61.1 91.7
179 25.8 18.6 27.8
108 25.7 19.1 28.7

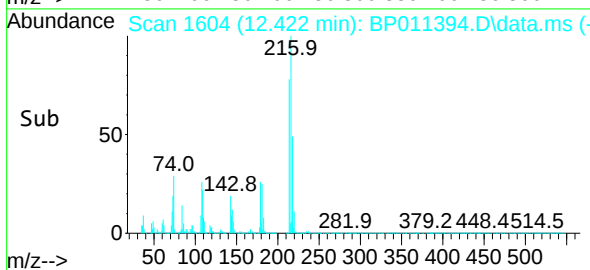



#40
Hexachlorocyclopentadiene
Concen: 30.364 ng/ul
RT: 12.393 min Scan# 110870
Delta R.T. -0.012 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04




Instrument :
BNA_P
ClientSampleId :
SLCS900



Tgt Ion:237 Resp: 110870
Ion Ratio Lower Upper
237 100
235 61.9 50.4 75.6
272 11.1 9.9 14.9




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 08/12/2022
Supervised By :Sohil Jodhani 08/13/2022



#41
2,4,6-Trichlorophenol
Concen: 35.108 ng/ul
RT: 12.675 min Scan# 1647
Delta R.T. -0.012 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04

Tgt Ion:196 Resp: 144753
Ion Ratio Lower Upper
196 100
198 94.9 75.5 113.3
200 30.5 24.4 36.6

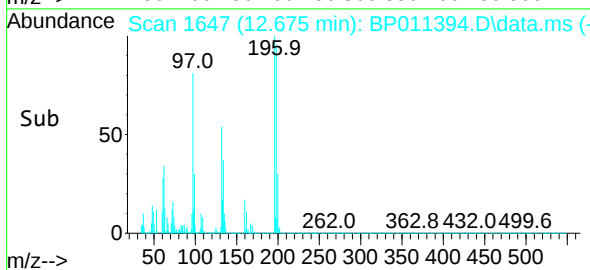



#42

2,4,5-Trichlorophenol

Concen: 35.677 ng/ul

RT: 12.746 min Scan# 1659

Delta R.T. -0.012 min

Lab File: BP011394.D

Acq: 11 Aug 2022 19:04

Instrument :

BNA_P

ClientSampleId :

SLCS900

Tgt Ion:196 Resp: 156999

Ion Ratio Lower Upper

196 100

198 96.0 76.8 115.2





200 30.4 25.0 37.6

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 08/12/2022

Supervised By :Sohil Jodhani 08/13/2022

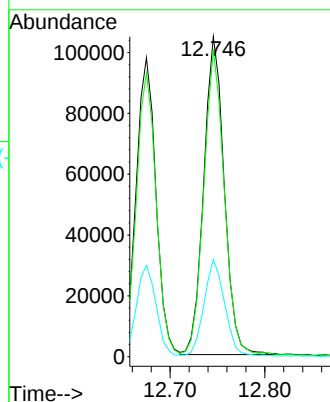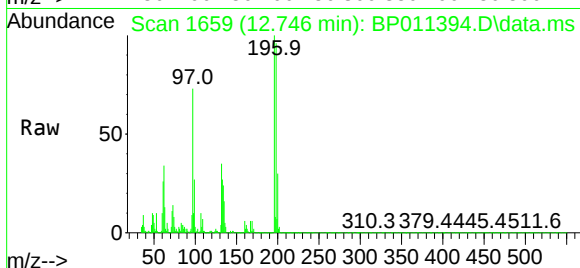

#43

1,1'-Biphenyl

Concen: 30.542 ng/ul

RT: 13.081 min Scan# 1716

Delta R.T. -0.012 min

Lab File: BP011394.D

Acq: 11 Aug 2022 19:04




Tgt Ion:154 Resp: 620784


Ion Ratio Lower Upper

154 100

153 41.2 31.9 47.9


76 13.9 12.2 18.2

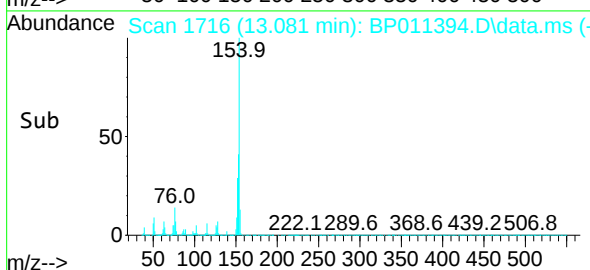



#44
2-Chloronaphthalene
Concen: 31.132 ng/ul
RT: 13.116 min Scan# 1722
Delta R.T. -0.012 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04




Instrument :
BNA_P
ClientSampleId :
SLCS900




Tgt Ion:162 Resp: 47477
Ion Ratio Lower Upper
162 100
164 32.6 25.6 38.4
127 47.1 34.6 51.8

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 08/12/2022
Supervised By :Sohil Jodhani 08/13/2022




#45
2-Nitroaniline
Concen: 45.442 ng/ul
RT: 13.340 min Scan# 1760
Delta R.T. -0.012 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04




Tgt Ion: 65 Resp: 176008
Ion Ratio Lower Upper
65 100
92 63.8 51.4 77.2
138 86.4 67.4 101.0

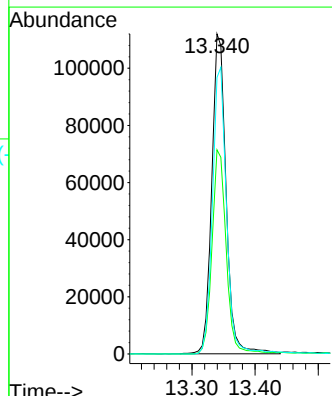



#47
Dimethylphthalate
Concen: 34.910 ng/ul
RT: 13.728 min Scan# 1826
Delta R.T. -0.006 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04




Instrument :
BNA_P
ClientSampleId :
SLCS900




Tgt Ion:163 Resp: 63503
Ion Ratio Lower Upper
163 100
194 3.3 2.9 4.3
164 9.7 8.2 12.4

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 08/12/2022
Supervised By :Sohil Jodhani 08/13/2022




#48
2,6-Dinitrotoluene
Concen: 43.181 ng/ul
RT: 13.851 min Scan# 1847
Delta R.T. -0.006 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04




Tgt Ion:165 Resp: 122818
Ion Ratio Lower Upper
165 100
89 80.5 65.8 98.6
121 27.2 24.2 36.2

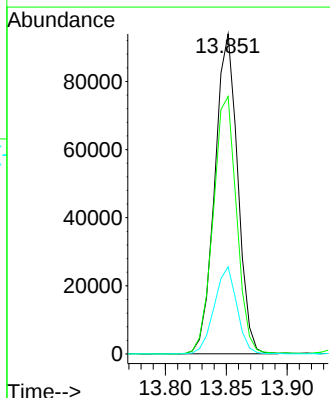



#50
Acenaphthylene
Concen: 32.058 ng/ul
RT: 13.975 min Scan# 1868
Delta R.T. -0.006 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04




Instrument : BNA_P
ClientSampleId : SLCS900



Tgt Ion:152 Resp: 798900
Ion Ratio Lower Upper
152 100
151 20.4 15.8 23.8
153 13.2 10.5 15.7




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 08/12/2022
Supervised By :Sohil Jodhani 08/13/2022

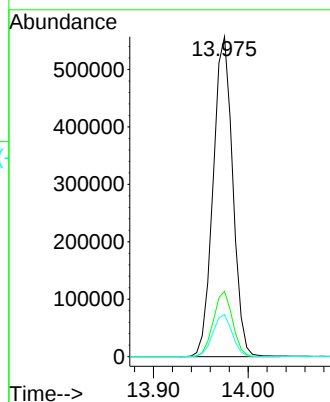

#51
3-Nitroaniline
Concen: 42.580 ng/ul
RT: 14.181 min Scan# 1903
Delta R.T. -0.006 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04


Tgt Ion:138 Resp: 133223
Ion Ratio Lower Upper
138 100
108 12.0 9.9 14.9
92 130.9 106.8 160.2

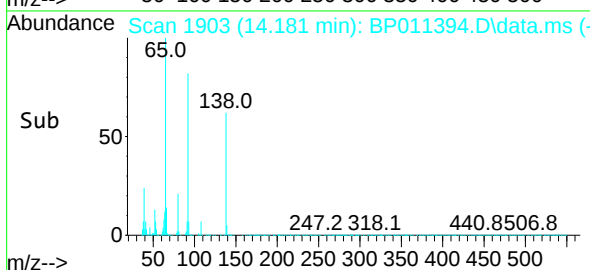



#52
Acenaphthene
Concen: 31.931 ng/ul
RT: 14.322 min Scan# 1927
Delta R.T. -0.006 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04




Instrument :
BNA_P
ClientSampleId :
SLCS900




Tgt Ion:153 Resp: 530712
Ion Ratio Lower Upper
153 100
152 48.3 39.5 59.3
154 87.9 68.6 103.0

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 08/12/2022
Supervised By :Sohil Jodhani 08/13/2022




#53
2,4-Dinitrophenol
Concen: 37.126 ng/ul
RT: 14.387 min Scan# 1938
Delta R.T. -0.012 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04




Tgt Ion:184 Resp: 62651
Ion Ratio Lower Upper
184 100
63 102.1 75.0 112.6
154 81.4 53.1 79.7#

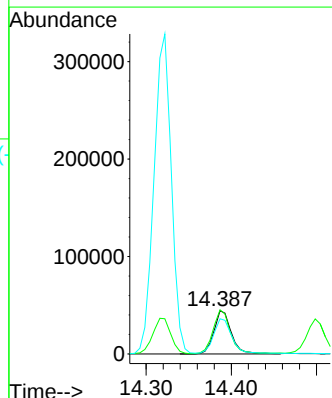



#55
4-Nitrophenol
Concen: 42.640 ng/ul
RT: 14.498 min Scan# 1957
Delta R.T. -0.006 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04




Instrument :
BNA_P
ClientSampleId :
SLCS900



Tgt Ion:109 Resp: 12975
Ion Ratio Lower Upper
109 100
139 94.4 100.6 150.8
65 116.1 122.6 184.0




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 08/12/2022
Supervised By :Sohil Jodhani 08/13/2022



#56
Dibenzofuran
Concen: 31.997 ng/ul
RT: 14.657 min Scan# 1984
Delta R.T. -0.012 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04


Tgt Ion:168 Resp: 720981
Ion Ratio Lower Upper
168 100
139 48.8 34.2 51.2





#57
2,4-Dinitrotoluene
Concen: 42.640 ng/ul
RT: 14.640 min Scan# 1982
Delta R.T. -0.012 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04




Instrument :
BNA_P
ClientSampleId :
SLCS900




Tgt Ion:165 Resp: 18589
Ion Ratio Lower Upper
165 100
63 67.8 50.6 75.8
182 2.8 2.2 3.2

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 08/12/2022
Supervised By :Sohil Jodhani 08/13/2022




#58
2,3,4,6-Tetrachlorophenol
Concen: 37.113 ng/ul
RT: 14.893 min Scan# 2024
Delta R.T. -0.006 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04




Tgt Ion:232 Resp: 127051
Ion Ratio Lower Upper
232 100
131 68.2 50.4 75.6
130 4.0 2.6 3.8#
166 40.8 31.9 47.9

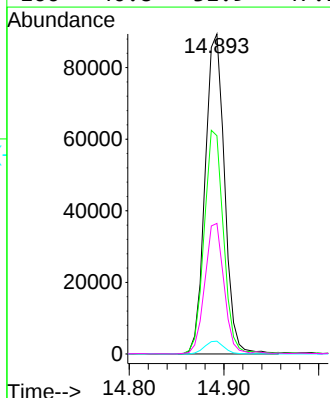



#59
Diethylphthalate
Concen: 37.628 ng/ul
RT: 15.104 min Scan# 2060
Delta R.T. -0.012 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04




Instrument :
BNA_P
ClientSampleId :
SLCS900




Tgt Ion:149 Resp: 709080
Ion Ratio Lower Upper
149 100
177 19.1 16.1 24.1
150 13.0 9.4 14.0

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 08/12/2022
Supervised By :Sohil Jodhani 08/13/2022




#61
Fluorene
Concen: 32.902 ng/ul
RT: 15.316 min Scan# 2096
Delta R.T. -0.006 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04




Tgt Ion:166 Resp: 602085
Ion Ratio Lower Upper
166 100
165 98.6 77.7 116.5
167 13.5 11.0 16.4

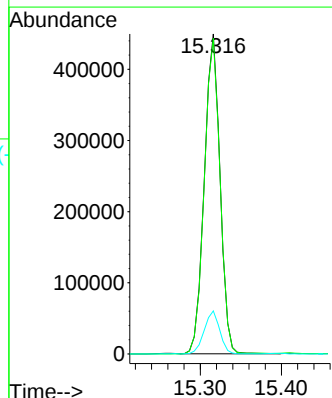



#62
4-Chlorophenyl-phenylether
Concen: 33.603 ng/ul
RT: 15.316 min Scan# 2096
Delta R.T. -0.012 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04




Instrument :
BNA_P
ClientSampleId :
SLCS900




Tgt Ion: 204 Resp: 268794
Ion Ratio Lower Upper
204 100
206 33.1 27.3 40.9
141 84.9 57.7 86.5

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 08/12/2022
Supervised By :Sohil Jodhani 08/13/2022




#63
4-Nitroaniline
Concen: 48.847 ng/ul m
RT: 15.357 min Scan# 2103
Delta R.T. -0.006 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04




Tgt Ion: 138 Resp: 148716
Ion Ratio Lower Upper
138 100
92 57.1 55.9 83.9
108 112.3 67.1 100.7#

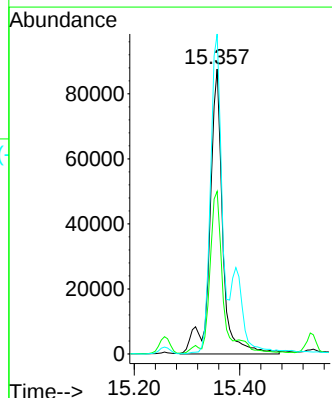



#66
4,6-Dinitro-2-methylphenol
Concen: 37.258 ng/ul
RT: 15.410 min Scan# 2112
Delta R.T. -0.006 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04




Instrument :
BNA_P
ClientSampleId :
SLCS900



Tgt Ion:198 Resp: 94285
Ion Ratio Lower Upper
198 100
182 4.7 7.4 11.0
77 40.5 28.6 42.8




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 08/12/2022
Supervised By :Sohil Jodhani 08/13/2022



#67
N-Nitrosodiphenylamine
Concen: 32.885 ng/ul
RT: 15.540 min Scan# 2134
Delta R.T. -0.006 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04


Tgt Ion:169 Resp: 512723
Ion Ratio Lower Upper
169 100
168 66.5 53.6 80.4
167 37.2 30.0 45.0





#68
4-Bromophenyl-phenylether
Concen: 33.593 ng/ul
RT: 16.222 min Scan# 211
Delta R.T. -0.006 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04




Instrument :
BNA_P
ClientSampleId :
SLCS900

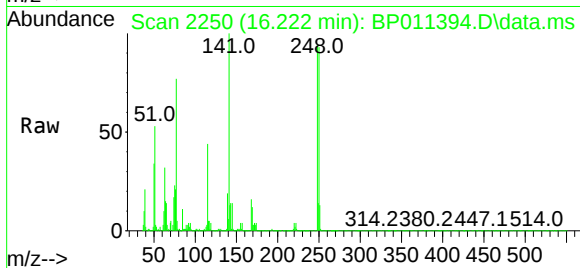

Tgt Ion:248 Resp: 157283
Ion Ratio Lower Upper
248 100
250 98.6 77.3 115.9
141 106.5 76.4 114.6




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 08/12/2022
Supervised By :Sohil Jodhani 08/13/2022

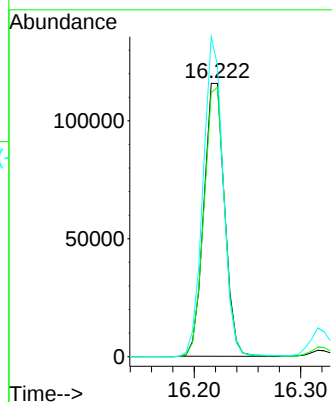

#69
Hexachlorobenzene
Concen: 33.287 ng/ul
RT: 16.322 min Scan# 2267
Delta R.T. -0.006 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04


Tgt Ion:284 Resp: 182076
Ion Ratio Lower Upper
284 100
142 52.8 39.5 59.3
249 34.0 25.1 37.7

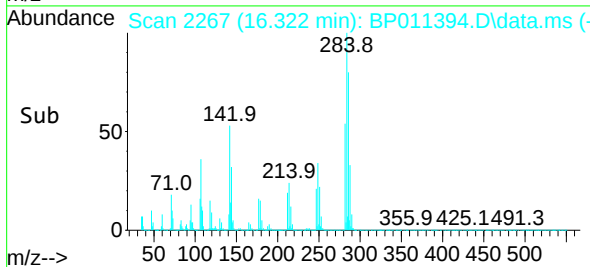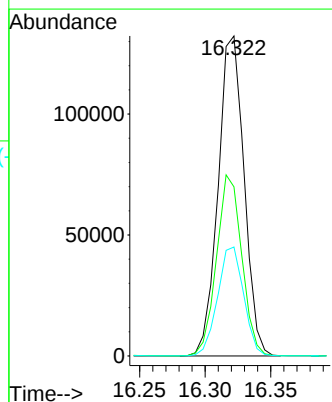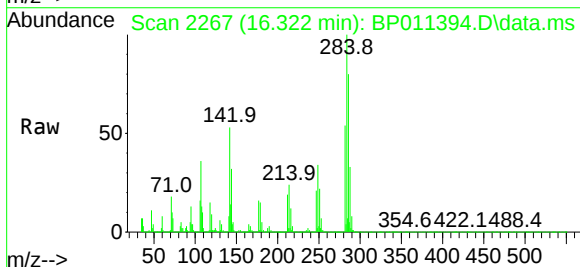



#70
Atrazine
Concen: 29.019 ng/ul
RT: 16.510 min Scan# 2299
Delta R.T. -0.006 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04




Instrument :
BNA_P
ClientSampleId :
SLCS900




Tgt Ion:200 Resp: 150809
Ion Ratio Lower Upper
200 100
173 27.0 22.6 34.0
215 42.5 36.5 54.7

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 08/12/2022
Supervised By :Sohil Jodhani 08/13/2022




#71
Pentachlorophenol
Concen: 33.632 ng/ul
RT: 16.675 min Scan# 2327
Delta R.T. -0.012 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04



Tgt Ion:266 Resp: 106795
Ion Ratio Lower Upper
266 100
264 63.4 52.2 78.2
268 62.0 50.6 75.8

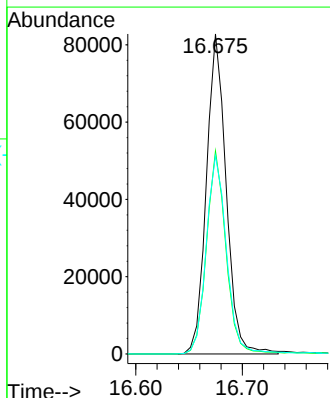







#72
Phenanthrene
Concen: 31.965 ng/uI
RT: 17.069 min Scan# 21
Delta R.T. -0.012 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04

Instrument :
BNA_P
ClientSampleId :
SLCS900

Tgt Ion:178 Resp: 94833
Ion Ratio Lower Upper
178 100
179 15.8 12.1 18.1
176 19.6 15.4 23.2




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 08/12/2022
Supervised By :Sohil Jodhani 08/13/2022



#74
Anthracene
Concen: 32.388 ng/uI
RT: 17.163 min Scan# 2410
Delta R.T. -0.006 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04


Tgt Ion:178 Resp: 956568
Ion Ratio Lower Upper
178 100
179 15.7 12.3 18.5
176 19.1 14.7 22.1





#75
1,2,3,4-Tetrachlorobenzene
Concen: 28.014 ng/uL
RT: 13.040 min Scan# 1709
Delta R.T. -0.012 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04




Instrument :
BNA_P
ClientSampleId :
SLCS900

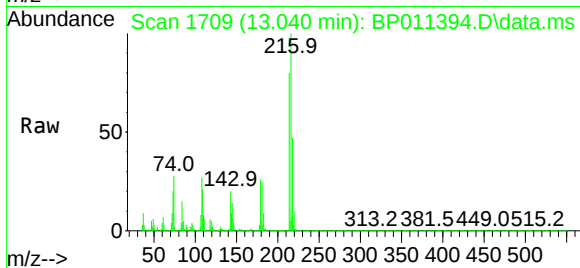


Tgt Ion:216 Resp: 212784
Ion Ratio Lower Upper
216 100
214 79.7 62.0 93.0
218 46.7 38.2 57.4

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 08/12/2022
Supervised By :Sohil Jodhani 08/13/2022




#76
Pentachlorobenzene
Concen: 31.028 ng/uL
RT: 14.575 min Scan# 1970
Delta R.T. -0.006 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04




Tgt Ion:250 Resp: 205252
Ion Ratio Lower Upper
250 100
248 63.3 49.2 73.8
252 65.2 50.8 76.2

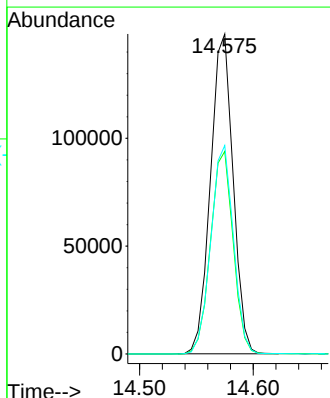



#77
 Carbazole
 Concen: 32.499 ng/ul
 RT: 17.445 min Scan# 2458
 Delta R.T. -0.006 min
 Lab File: BP011394.D
 Acq: 11 Aug 2022 19:04




Instrument :
 BNA_P
 ClientSampleId :
 SLCS900




Tgt Ion:167 Resp: 896939
 Ion Ratio Lower Upper
 167 100
 166 21.7 17.1 25.7
 139 15.9 11.5 17.3

Manual Integrations
 APPROVED



Reviewed By :Jagrut Upadhyay 08/12/2022
 Supervised By :Sohil Jodhani 08/13/2022




#78
 Di-n-butylphthalate
 Concen: 40.463 ng/ul
 RT: 18.016 min Scan# 2555
 Delta R.T. -0.012 min
 Lab File: BP011394.D
 Acq: 11 Aug 2022 19:04




Tgt Ion:149 Resp: 1221121
 Ion Ratio Lower Upper
 149 100
 150 9.0 7.4 11.0
 104 6.7 5.1 7.7

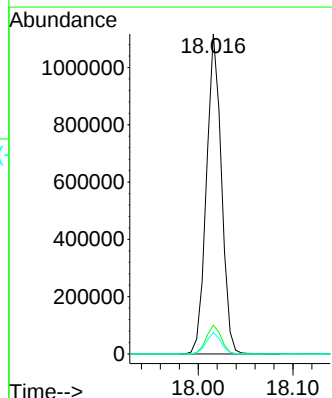



#80
Fluoranthene
Concen: 32.020 ng/u1
RT: 19.063 min Scan# 2733
Delta R.T. -0.006 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04




Instrument :
BNA_P
ClientSampleId :
SLCS900

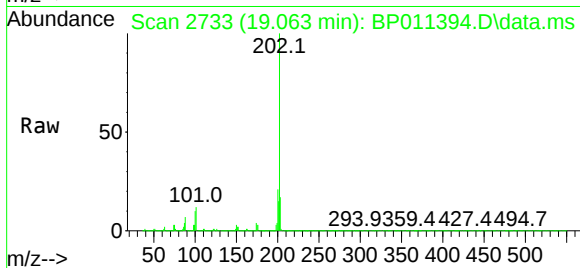


Tgt Ion:202 Resp: 1094784
Ion Ratio Lower Upper
202 100
101 12.2 11.9 17.9
100 9.6 9.3 13.9

Manual Integrations
APPROVED



Reviewed By :Jagrut Upadhyay 08/12/2022
Supervised By :Sohil Jodhani 08/13/2022

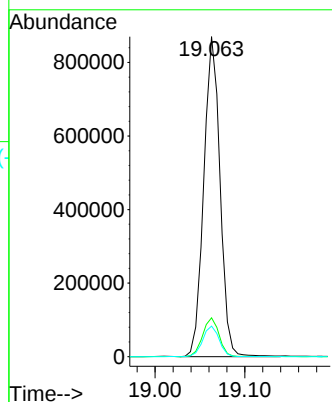


#82
Pyrene
Concen: 31.249 ng/u1
RT: 19.422 min Scan# 2794
Delta R.T. -0.006 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04



Tgt Ion:202 Resp: 1127726
Ion Ratio Lower Upper
202 100
101 13.9 14.3 21.5#
100 11.6 11.8 17.6#

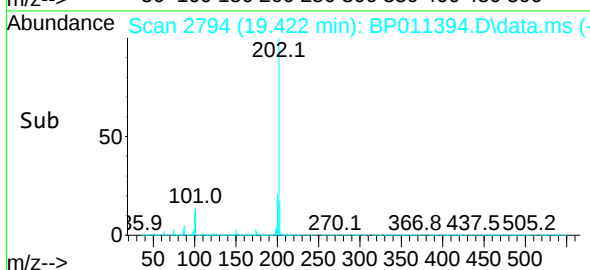



#83

Butylbenzylphthalate

Concen: 48.231 ng/ul

RT: 20.322 min Scan# 2947

Delta R.T. -0.006 min

Lab File: BP011394.D

Acq: 11 Aug 2022 19:04

Instrument :

BNA_P

ClientSampleId :





SLCS900

Tgt Ion:	149	Resp:	55466
Ion Ratio	Lower	Upper	
149	100		
91	78.8	64.2	96.4
206	16.8	14.0	21.0

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 08/12/2022
Supervised By :Sohil Jodhani 08/13/2022

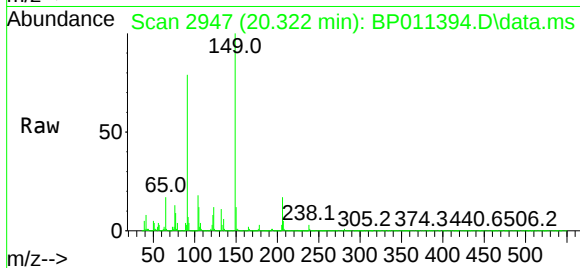

#84

3,3'-Dichlorobenzidine

Concen: 37.503 ng/ul




RT: 21.086 min Scan# 3077


Delta R.T. -0.012 min

Lab File: BP011394.D

Acq: 11 Aug 2022 19:04

Tgt Ion:	252	Resp:	347998
Ion Ratio	Lower	Upper	
252	100		
254	64.5	51.8	77.6
126	15.5	11.4	17.0





#85

Benzo(a)anthracene

Concen: 32.442 ng/ul

RT: 21.145 min Scan# 3087

Delta R.T. -0.006 min

Lab File: BP011394.D

Acq: 11 Aug 2022 19:04

Instrument :

BNA_P

ClientSampleId :

SLCS900

Tgt Ion:228 Resp: 1061194

Ion Ratio Lower Upper

228 100

229 19.9 15.8 23.6





226 27.5 21.8 32.6

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 08/12/2022

Supervised By :Sohil Jodhani 08/13/2022

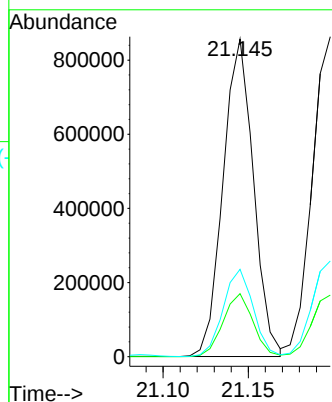

#86

Bis(2-ethylhexyl)phthalate

Concen: 45.174 ng/ul

RT: 21.086 min Scan# 3077

Delta R.T. -0.006 min

Lab File: BP011394.D

Acq: 11 Aug 2022 19:04




Tgt Ion:149 Resp: 833991


Ion Ratio Lower Upper

149 100

167 24.1 20.4 30.6


279 3.2 2.9 4.3

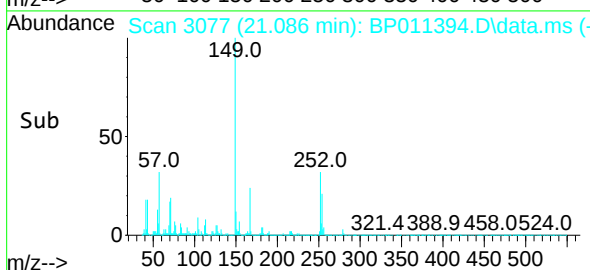



#87
Chrysene
Concen: 32.795 ng/ul
RT: 21.198 min Scan# 3096
Delta R.T. -0.006 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04




Instrument :
BNA_P
ClientSampleId :
SLCS900



Tgt Ion:228 Resp: 1061920
Ion Ratio Lower Upper
228 100
226 29.9 23.8 35.6
229 19.2 15.7 23.5




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 08/12/2022
Supervised By :Sohil Jodhani 08/13/2022



#89
Di-n-octyl phthalate
Concen: 39.916 ng/ul
RT: 21.986 min Scan# 3230
Delta R.T. -0.012 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04


Tgt Ion:149 Resp: 1392021

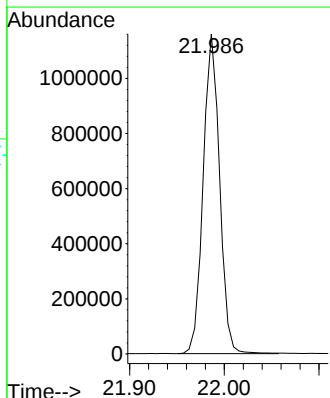



#90
Benzo(b)fluoranthene
Concen: 33.956 ng/ul
RT: 22.769 min Scan# 3363
Delta R.T. -0.006 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04




Instrument :
BNA_P
ClientSampleId :
SLCS900



Tgt Ion:252 Resp: 1123299
Ion Ratio Lower Upper
252 100
253 21.8 17.4 26.0
125 11.7 10.8 16.2




Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 08/12/2022
Supervised By :Sohil Jodhani 08/13/2022



#91
Benzo(k)fluoranthene
Concen: 31.343 ng/ul
RT: 22.816 min Scan# 3371
Delta R.T. -0.006 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04

Tgt Ion:252 Resp: 1014470
Ion Ratio Lower Upper
252 100
253 22.3 17.6 26.4
125 11.5 11.0 16.6





#93

Benzo(a)pyrene

Concen: 33.491 ng/ul

RT: 23.369 min Scan# 3465

Delta R.T. -0.006 min

Lab File: BP011394.D

Acq: 11 Aug 2022 19:04

Instrument :

BNA_P

ClientSampleId :

SLCS900

Tgt Ion:252 Resp: 106859

Ion Ratio Lower Upper

252 100

253 21.5 17.4 26.2





125 12.9 12.5 18.7

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 08/12/2022

Supervised By :Sohil Jodhani 08/13/2022



#94

Indeno(1,2,3-cd)pyrene

Concen: 33.333 ng/ul

RT: 25.851 min Scan# 3887

Delta R.T. -0.006 min

Lab File: BP011394.D

Acq: 11 Aug 2022 19:04




Tgt Ion:276 Resp: 1175733


Ion Ratio Lower Upper

276 100

138 27.2 25.5 38.3


277 25.1 19.8 29.8

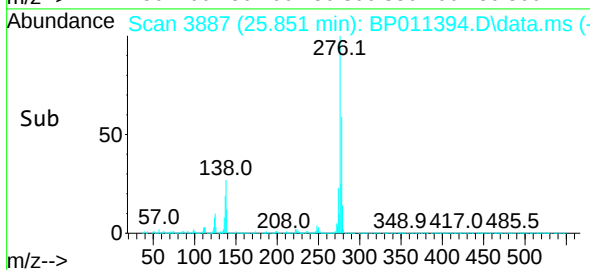



#95
Dibenzo(a,h)anthracene
Concen: 33.619 ng/ul
RT: 25.868 min Scan# 3891
Delta R.T. -0.018 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04




Instrument :
BNA_P
ClientSampleId :
SLCS900



Tgt Ion:278 Resp: 100850
Ion Ratio Lower Upper
278 100
139 17.6 18.5 27.7
279 23.5 19.6 29.4

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 08/12/2022
Supervised By :Sohil Jodhani 08/13/2022



#96
Benzo(g,h,i)perylene
Concen: 33.718 ng/ul
RT: 26.580 min Scan# 4011
Delta R.T. -0.012 min
Lab File: BP011394.D
Acq: 11 Aug 2022 19:04

Tgt Ion:276 Resp: 1003572
Ion Ratio Lower Upper
276 100
138 24.7 22.8 34.2
277 23.9 18.5 27.7

