

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011381.D
 Acq On : 11 Aug 2022 11:35
 Operator : CG/JU
 Sample : PB146902BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK902

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011381.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.081	13	16	22	rVB	38997	45302	2.29%	0.203%
2	3.493	83	86	100	rBV	420193	610684	30.89%	2.733%
3	3.799	135	138	143	rVB	8258	11408	0.58%	0.051%
4	4.228	210	211	214	rBV3	1991	2418	0.12%	0.011%
5	5.404	407	411	412	rBV4	1547	1991	0.10%	0.009%
6	6.763	636	642	654	rBV	444069	703607	35.59%	3.149%
7	6.928	664	670	686	rVB	354940	540024	27.32%	2.417%
8	7.110	693	701	719	rBV	465221	737370	37.30%	3.301%
9	7.581	774	781	792	rBV	346093	537676	27.20%	2.407%
10	8.304	896	904	921	rBV	491172	818377	41.40%	3.663%
11	8.745	972	979	991	rBV	425943	684096	34.61%	3.062%
12	9.463	1093	1101	1111	rBV	341079	543245	27.48%	2.432%
13	9.928	1174	1180	1182	rBV7	1451	2144	0.11%	0.010%
14	9.998	1185	1192	1205	rBV	454952	768745	38.89%	3.441%
15	10.369	1248	1255	1265	rBV	441710	726963	36.77%	3.254%
16	10.522	1274	1281	1310	rBV	413530	780922	39.50%	3.495%
17	11.981	1524	1529	1537	rBV3	6742	12963	0.66%	0.058%
18	13.680	1811	1818	1832	rBV	824339	1147818	58.06%	5.138%
19	13.792	1836	1837	1845	rVB8	2243	2782	0.14%	0.012%
20	13.945	1853	1863	1876	rBV	871537	1266948	64.09%	5.671%
21	14.257	1909	1916	1925	rBV	575200	846142	42.80%	3.787%
22	14.486	1948	1955	1977	rBV	213265	505479	25.57%	2.263%
23	15.257	2079	2086	2099	rBV	1055024	1554480	78.63%	6.958%
24	15.392	2103	2109	2119	rVV	360052	494625	25.02%	2.214%
25	15.498	2124	2127	2136	rVB5	13904	26312	1.33%	0.118%
26	16.051	2218	2221	2225	rVV6	2760	4825	0.24%	0.022%
27	16.169	2238	2241	2243	rVB4	2034	2050	0.10%	0.009%
28	16.522	2296	2301	2304	rVB7	1152	2240	0.11%	0.010%
29	16.816	2348	2351	2356	rVB7	1743	2880	0.15%	0.013%
30	17.027	2380	2387	2398	rBV	731615	1012661	51.23%	4.533%
31	17.127	2398	2404	2425	rVB	1222464	1765440	89.31%	7.902%
32	17.727	2504	2506	2510	rVB5	1785	2415	0.12%	0.011%
33	18.468	2630	2632	2636	rBV4	1927	2015	0.10%	0.009%
34	18.963	2712	2716	2721	rBV2	13699	18302	0.93%	0.082%
35	19.033	2724	2728	2735	rBV3	14057	23698	1.20%	0.106%
36	19.392	2783	2789	2800	rBV	1492661	1976852	100.00%	8.849%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011381.D
Acq On : 11 Aug 2022 11:35
Operator : CG/JU
Sample : PB146902BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK902

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Title : SVOA CALIBRATION

37	21.157	3084	3089	3097	rBV	821959	1090560	55.17%	4.881%
38	23.315	3450	3456	3464	rBV2	1035015	1971161	99.71%	8.823%
39	23.462	3476	3481	3491	rVB2	567670	1093245	55.30%	4.893%




Sum of corrected areas: 22340865

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011381.D
Acq On : 11 Aug 2022 11:35
Operator : CG/JU
Sample : PB146902BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK902

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

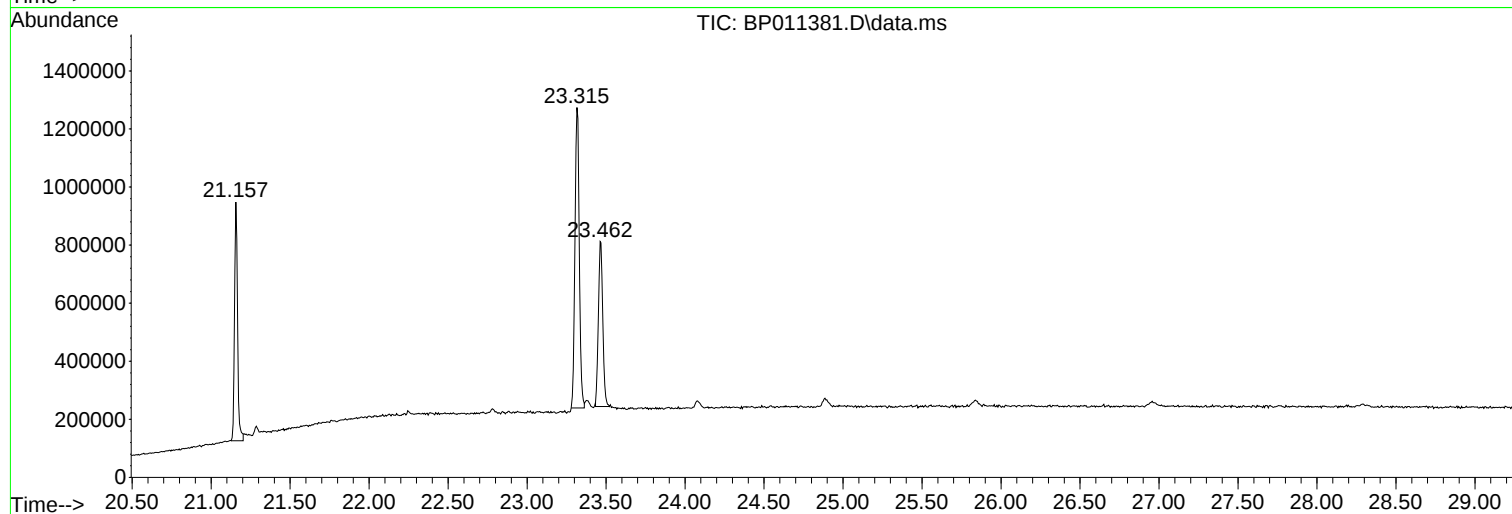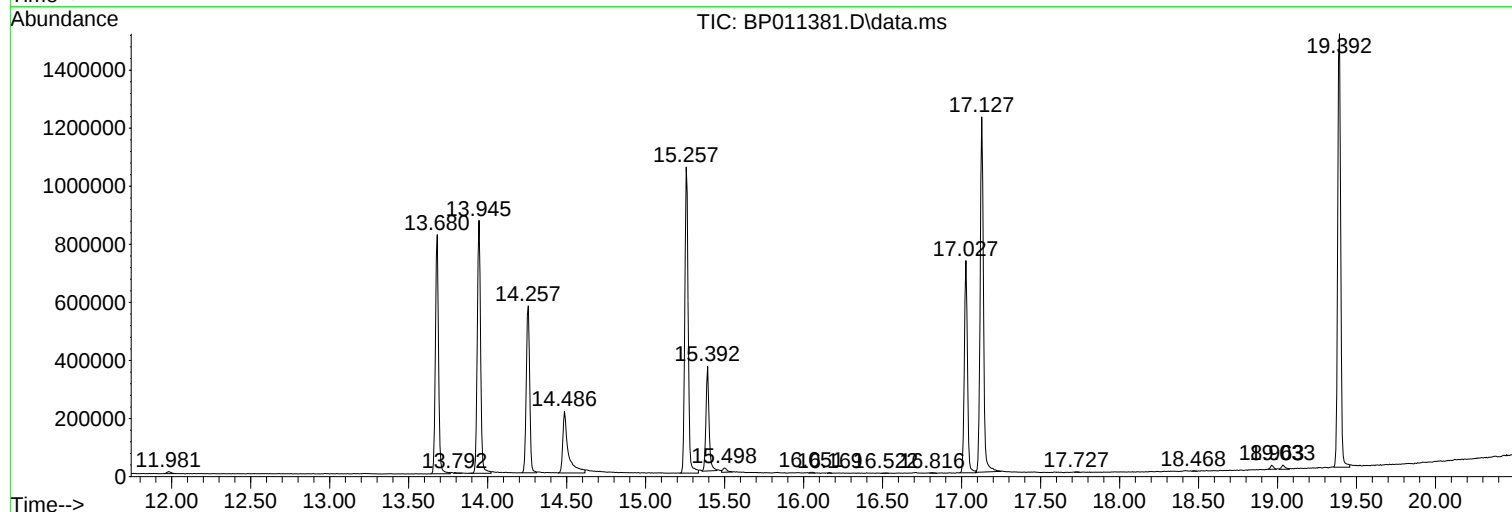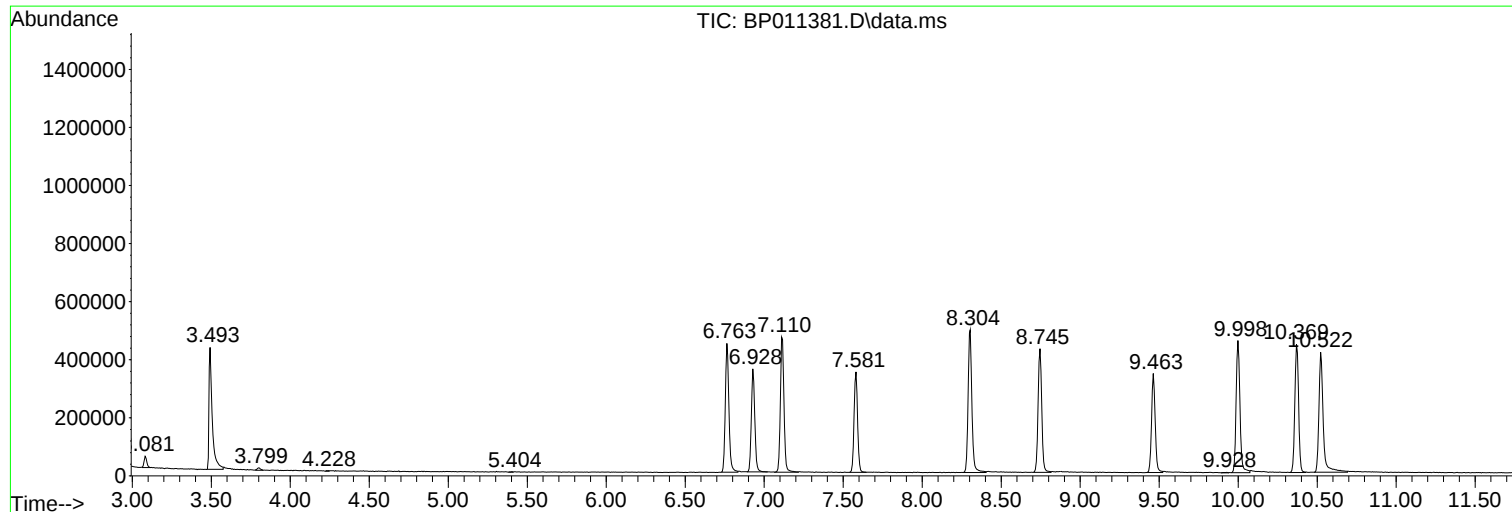

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011381.D
Acq On : 11 Aug 2022 11:35
Operator : CG/JU
Sample : PB146902BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK902

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011381.D
Acq On : 11 Aug 2022 11:35
Operator : CG/JU
Sample : PB146902BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK902

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------