

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011382.D
 Acq On : 11 Aug 2022 12:09
 Operator : CG/JU
 Sample : N4128-07
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBX3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011382.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.081	13	16	22	rVB	28898	34779	1.39%	0.153%
2	3.499	85	87	105	rBV	81581	132414	5.28%	0.583%
3	3.711	117	123	129	rVB	14000	23090	0.92%	0.102%
4	3.799	134	138	142	rBV2	7391	10283	0.41%	0.045%
5	4.234	207	212	220	rVB	18693	28546	1.14%	0.126%
6	4.716	290	294	301	rVB5	3441	5277	0.21%	0.023%
7	4.828	311	313	317	rVB5	4276	4903	0.20%	0.022%
8	6.710	628	633	637	rBV3	9200	15017	0.60%	0.066%
9	6.763	637	642	651	rVB	101837	158795	6.33%	0.699%
10	6.928	664	670	685	rVB	356110	538483	21.47%	2.371%
11	7.110	694	701	713	rBV	360482	575164	22.93%	2.532%
12	7.199	713	716	725	rVB7	4252	8810	0.35%	0.039%
13	7.581	774	781	790	rBV	377253	580365	23.14%	2.555%
14	8.299	895	903	916	rBV	268251	447202	17.83%	1.969%
15	8.746	971	979	988	rBV	432345	693314	27.64%	3.053%
16	8.875	998	1001	1005	rVV6	2100	2559	0.10%	0.011%
17	8.910	1005	1007	1013	rVB7	1893	3002	0.12%	0.013%
18	9.151	1043	1048	1055	rVB2	11871	19382	0.77%	0.085%
19	9.463	1092	1101	1110	rBV	334783	538972	21.49%	2.373%
20	9.998	1185	1192	1208	rBV	426966	714489	28.49%	3.146%
21	10.369	1248	1255	1264	rBV	489660	787442	31.40%	3.467%
22	10.522	1274	1281	1295	rBV	332291	609871	24.32%	2.685%
23	11.210	1392	1398	1399	rBV6	2332	3496	0.14%	0.015%
24	11.651	1470	1473	1478	rVB2	6559	11273	0.45%	0.050%
25	11.975	1523	1528	1535	rBV4	7224	15462	0.62%	0.068%
26	12.975	1694	1698	1703	rBV7	1336	2669	0.11%	0.012%
27	13.681	1811	1818	1832	rBV	903996	1254525	50.02%	5.524%
28	13.945	1856	1863	1884	rBV	936826	1354748	54.02%	5.965%
29	14.257	1909	1916	1925	rBV	647177	948044	37.80%	4.174%
30	14.492	1951	1956	1971	rBV4	25430	80899	3.23%	0.356%
31	15.263	2080	2087	2100	rBV	1124130	1702176	67.87%	7.495%
32	15.392	2103	2109	2124	rVV	423761	625311	24.93%	2.753%
33	15.504	2124	2128	2133	rVB3	13513	22475	0.90%	0.099%
34	16.051	2218	2221	2227	rVB8	4127	5939	0.24%	0.026%
35	16.169	2236	2241	2250	rBV8	1939	5214	0.21%	0.023%
36	16.516	2294	2300	2303	rBV3	5983	8287	0.33%	0.036%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011382.D
 Acq On : 11 Aug 2022 12:09
 Operator : CG/JU
 Sample : N4128-07
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBX3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

37	16.704	2329	2332	2336	rVB5	2721	3482	0.14%	0.015%
38	16.975	2374	2378	2380	rBV4	2291	3556	0.14%	0.016%
39	17.028	2381	2387	2398	rVV	809929	1133250	45.19%	4.990%
40	17.128	2398	2404	2423	rVV2	1442547	2086938	83.21%	9.189%
41	17.592	2479	2483	2488	rBV4	5929	8938	0.36%	0.039%
42	17.727	2502	2506	2508	rBV5	2971	3377	0.13%	0.015%
43	18.022	2552	2556	2561	rBV3	4661	8485	0.34%	0.037%
44	18.522	2639	2641	2644	rVB3	3241	3524	0.14%	0.016%
45	18.969	2713	2717	2722	rVB3	17149	22931	0.91%	0.101%
46	19.039	2725	2729	2734	rVV3	14818	22085	0.88%	0.097%
47	19.298	2771	2773	2776	rVB2	5408	5656	0.23%	0.025%
48	19.392	2783	2789	2799	rBV	1972326	2405233	95.90%	10.590%
49	21.163	3085	3090	3100	rBV	910003	1245331	49.65%	5.483%
50	23.321	3450	3457	3465	rBV2	1337737	2507986	100.00%	11.042%
51	23.468	3476	3482	3494	rVB	656642	1278804	50.99%	5.630%




Sum of corrected areas: 22712253

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011382.D
Acq On : 11 Aug 2022 12:09
Operator : CG/JU
Sample : N4128-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBX3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

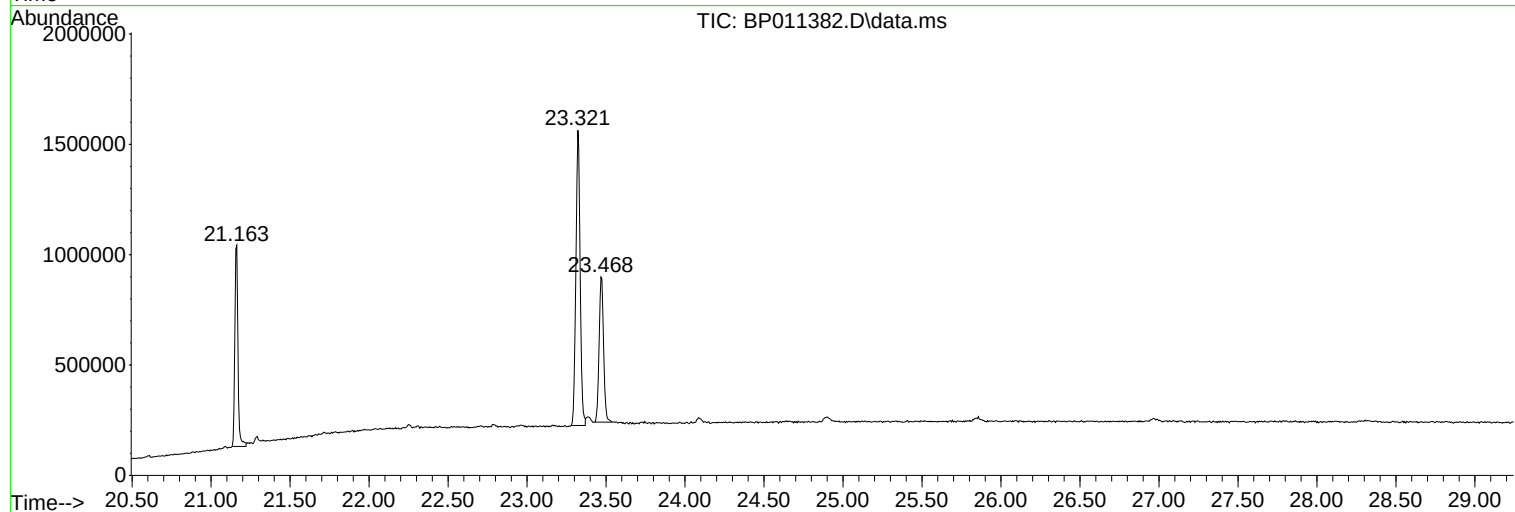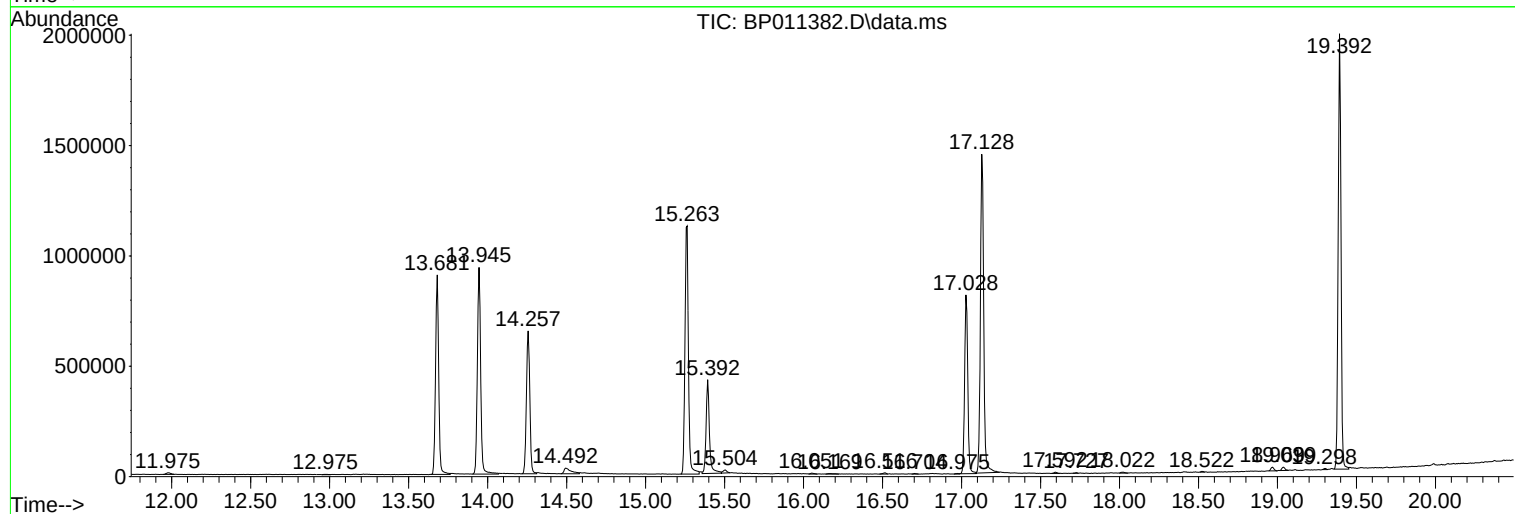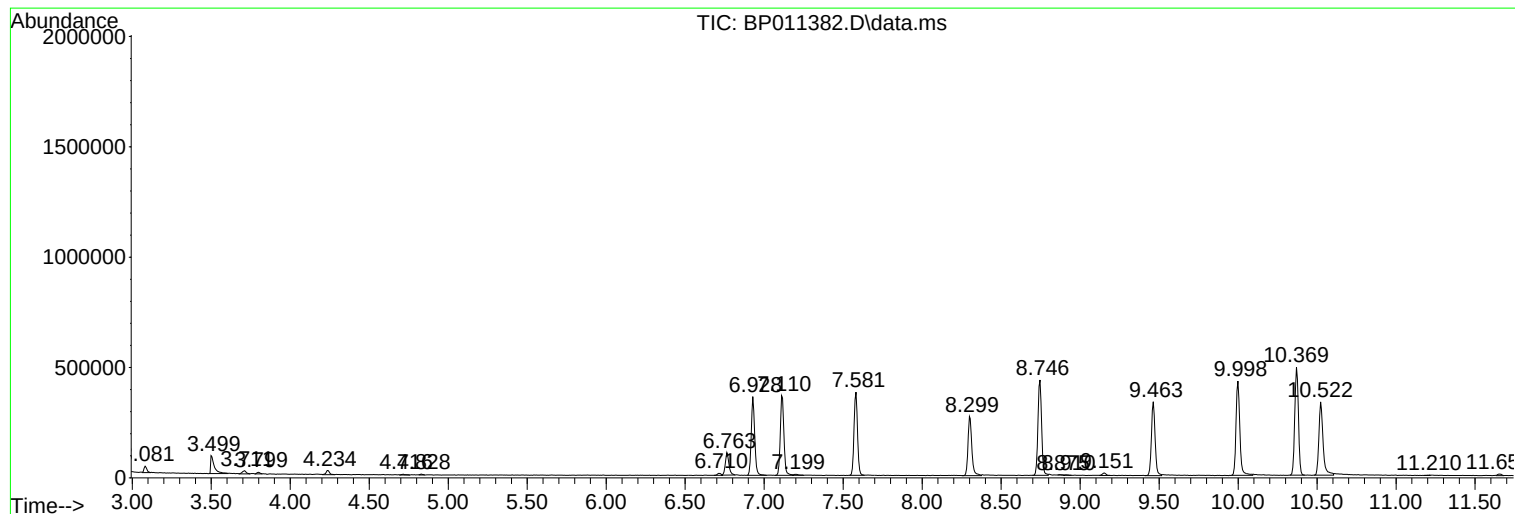

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011382.D
Acq On : 11 Aug 2022 12:09
Operator : CG/JU
Sample : N4128-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBX3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011382.D
Acq On : 11 Aug 2022 12:09
Operator : CG/JU
Sample : N4128-07
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBX3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------