

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011383.D
 Acq On : 11 Aug 2022 12:44
 Operator : CG/JU
 Sample : N4128-04
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGC11

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011383.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.081	13	16	25	rVB	25722	34124	1.38%	0.151%
2	3.499	84	87	100	rBV	110420	171635	6.93%	0.761%
3	3.711	118	123	128	rVB	13909	20835	0.84%	0.092%
4	3.799	135	138	146	rVB2	8250	12994	0.52%	0.058%
5	4.240	208	213	218	rVB	19735	26365	1.07%	0.117%
6	4.716	291	294	298	rVB3	2995	4277	0.17%	0.019%
7	4.828	309	313	317	rVB7	2781	4441	0.18%	0.020%
8	4.887	319	323	329	rVB3	8366	12771	0.52%	0.057%
9	6.452	582	589	592	rBV8	1710	3564	0.14%	0.016%
10	6.716	630	634	637	rBV	9248	12539	0.51%	0.056%
11	6.763	637	642	654	rVB	87225	147185	5.95%	0.653%
12	6.928	664	670	682	rBV	358283	556371	22.47%	2.467%
13	7.116	695	702	713	rBV	353895	569429	23.00%	2.525%
14	7.205	715	717	721	rVB4	3679	3621	0.15%	0.016%
15	7.581	774	781	790	rBV	342126	524715	21.20%	2.326%
16	8.304	896	904	917	rBV	248875	413989	16.72%	1.836%
17	8.746	972	979	991	rBV	450763	721568	29.15%	3.199%
18	8.875	996	1001	1004	rBV6	1775	2885	0.12%	0.013%
19	9.151	1043	1048	1056	rVB2	11107	18546	0.75%	0.082%
20	9.463	1093	1101	1111	rBV	339003	554021	22.38%	2.456%
21	9.998	1184	1192	1208	rBV	430375	738538	29.83%	3.274%
22	10.369	1248	1255	1266	rBV	432815	721391	29.14%	3.198%
23	10.528	1273	1282	1296	rBV	364010	682128	27.55%	3.024%
24	11.210	1396	1398	1406	rVB9	2185	4002	0.16%	0.018%
25	11.657	1468	1474	1479	rVB2	7240	11748	0.47%	0.052%
26	11.981	1522	1529	1535	rBV3	7426	15800	0.64%	0.070%
27	12.863	1674	1679	1684	rVB8	1646	3278	0.13%	0.015%
28	13.228	1733	1741	1746	rBV8	2290	4595	0.19%	0.020%
29	13.681	1811	1818	1832	rBV	944013	1296203	52.36%	5.747%
30	13.945	1856	1863	1879	rBV	961938	1408561	56.90%	6.245%
31	14.175	1898	1902	1906	rVB7	3482	5669	0.23%	0.025%
32	14.257	1909	1916	1925	rBV	607588	869708	35.13%	3.856%
33	14.498	1952	1957	1969	rBV3	20380	64906	2.62%	0.288%
34	15.134	2058	2065	2068	rBV6	4077	6524	0.26%	0.029%
35	15.263	2079	2087	2103	rBV	1186661	1797466	72.61%	7.969%
36	15.392	2103	2109	2119	rVV	419618	584917	23.63%	2.593%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011383.D
 Acq On : 11 Aug 2022 12:44
 Operator : CG/JU
 Sample : N4128-04
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGC11

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

37	15.504	2124	2128	2133	rVB2	13014	21808	0.88%	0.097%
38	15.998	2210	2212	2219	rVV5	5318	8837	0.36%	0.039%
39	16.051	2219	2221	2228	rVB7	4242	7457	0.30%	0.033%
40	16.510	2292	2299	2304	rBV5	5368	8322	0.34%	0.037%
41	16.710	2328	2333	2336	rVB7	2017	3265	0.13%	0.014%
42	16.804	2344	2349	2353	rBV7	4610	7300	0.29%	0.032%
43	16.916	2364	2368	2371	rBV6	2015	3093	0.12%	0.014%
44	16.975	2374	2378	2381	rBV5	2436	3534	0.14%	0.016%
45	17.028	2381	2387	2398	rBV	728769	1033842	41.76%	4.584%
46	17.128	2398	2404	2429	rVB	1454304	2120880	85.67%	9.403%
47	17.551	2474	2476	2480	rVB5	2988	4044	0.16%	0.018%
48	17.598	2480	2484	2487	rBV3	4933	6382	0.26%	0.028%
49	17.727	2502	2506	2510	rVB7	2909	4256	0.17%	0.019%
50	18.022	2552	2556	2558	rVB5	3040	3605	0.15%	0.016%
51	18.422	2619	2624	2628	rBV8	4403	7233	0.29%	0.032%
52	18.969	2712	2717	2722	rBV2	16744	26363	1.06%	0.117%
53	19.039	2725	2729	2735	rVV2	16533	23175	0.94%	0.103%
54	19.392	2783	2789	2804	rBV	1876266	2468214	99.70%	10.943%
55	21.157	3085	3089	3100	rBV	839302	1142652	46.16%	5.066%
56	23.321	3450	3457	3464	rBV2	1338190	2475559	100.00%	10.976%
57	23.474	3476	3483	3493	rVB2	578497	1143430	46.19%	5.070%




Sum of corrected areas: 22554560

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011383.D
Acq On : 11 Aug 2022 12:44
Operator : CG/JU
Sample : N4128-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGC11

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

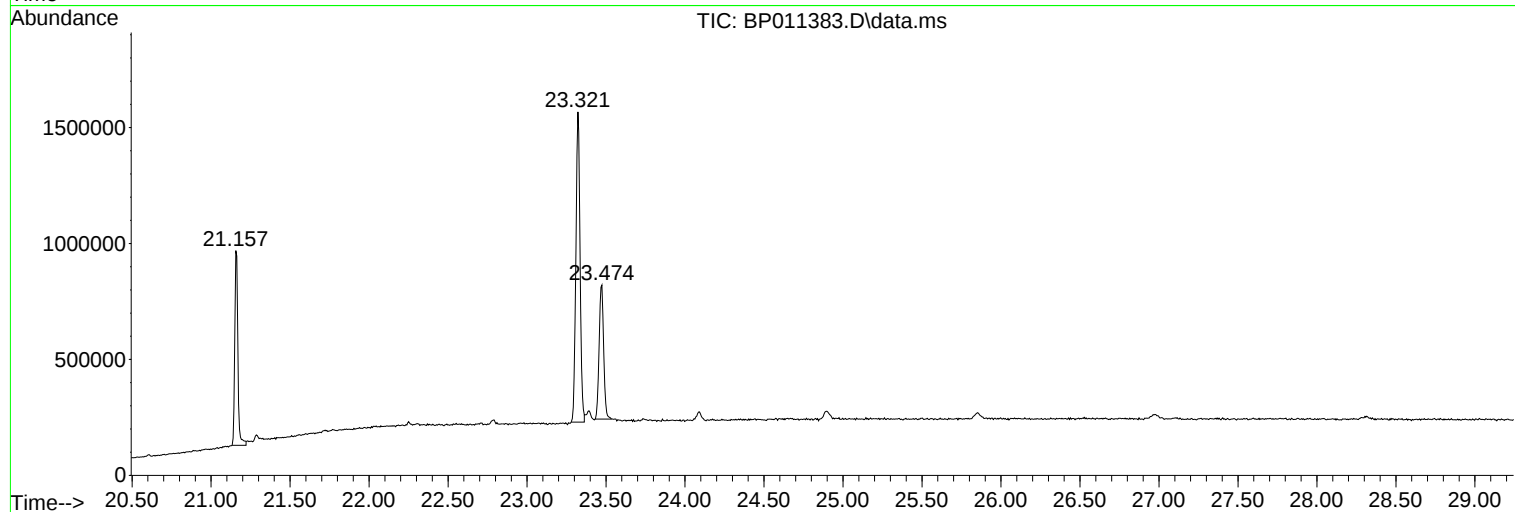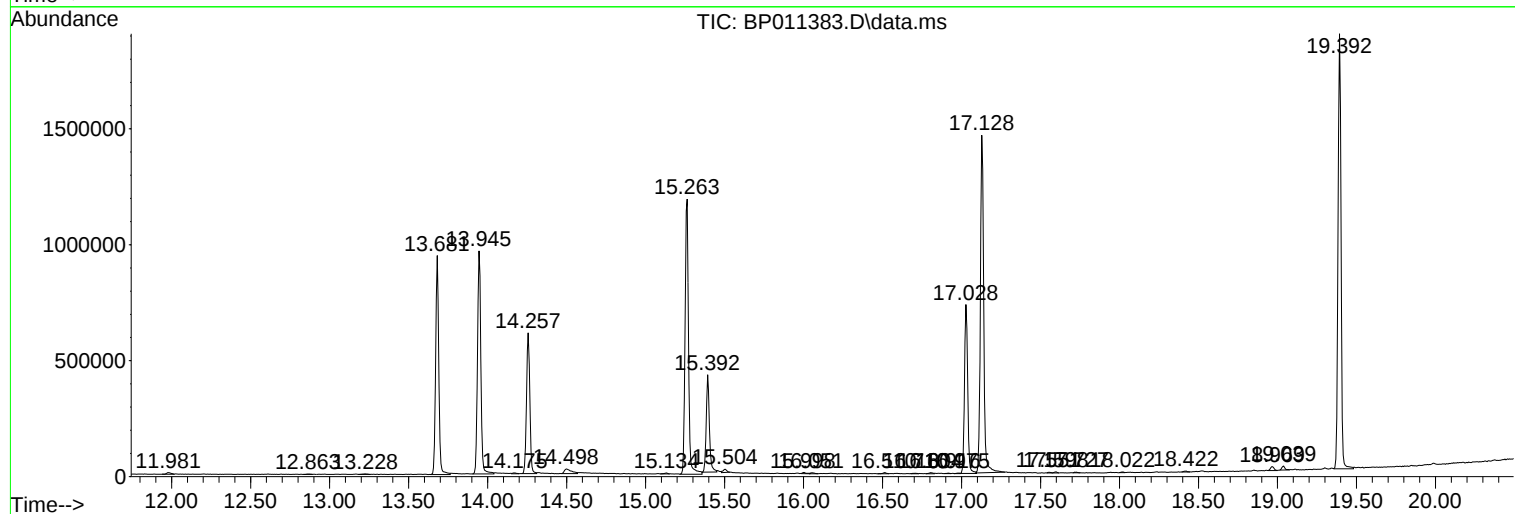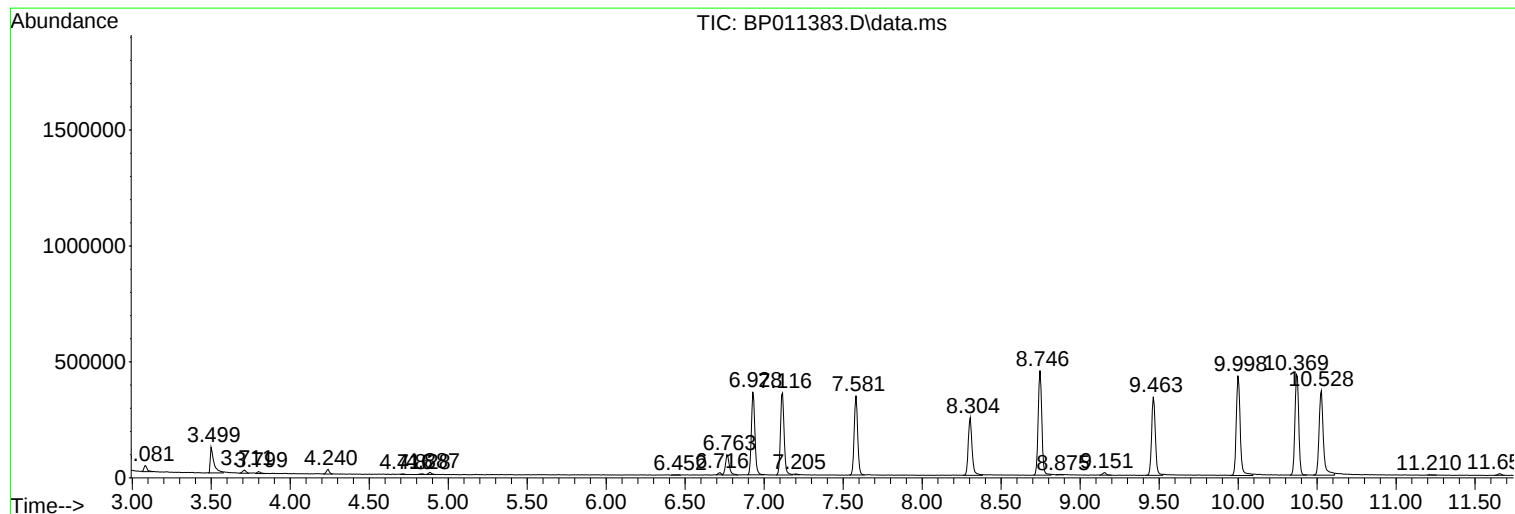

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011383.D
Acq On : 11 Aug 2022 12:44
Operator : CG/JU
Sample : N4128-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGC11

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011383.D
Acq On : 11 Aug 2022 12:44
Operator : CG/JU
Sample : N4128-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGC11

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc