

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011384.D
 Acq On : 11 Aug 2022 13:18
 Operator : CG/JU
 Sample : N4128-11
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBT8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011384.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.046	6	10	14	rBV	103947	129185	5.75%	0.608%
2	3.081	14	16	25	rVB	36804	46668	2.08%	0.220%
3	3.505	85	88	103	rBV	77503	133229	5.93%	0.627%
4	3.711	118	123	129	rBV	14951	21106	0.94%	0.099%
5	3.805	134	139	146	rVB2	9724	16723	0.74%	0.079%
6	4.240	208	213	217	rBV	18065	23036	1.02%	0.108%
7	4.622	276	278	286	rBV8	1671	4089	0.18%	0.019%
8	4.711	292	293	297	rVB4	3677	3386	0.15%	0.016%
9	4.834	309	314	317	rVB7	3299	4993	0.22%	0.024%
10	5.599	441	444	447	rBV5	2345	3034	0.13%	0.014%
11	6.716	629	634	638	rVV2	10058	15501	0.69%	0.073%
12	6.763	638	642	653	rVB	82422	137652	6.12%	0.648%
13	6.928	664	670	682	rBV	337138	514488	22.88%	2.422%
14	7.116	695	702	713	rBV	337739	531920	23.66%	2.504%
15	7.199	713	716	723	rVB5	5135	7246	0.32%	0.034%
16	7.581	774	781	789	rBV	403142	622135	27.67%	2.929%
17	8.304	897	904	918	rBV	226190	385769	17.16%	1.816%
18	8.746	972	979	988	rBV	410002	658274	29.28%	3.099%
19	8.875	999	1001	1005	rVB4	2563	2665	0.12%	0.013%
20	9.157	1042	1049	1057	rVB2	10558	19578	0.87%	0.092%
21	9.463	1093	1101	1117	rBV	305803	497994	22.15%	2.344%
22	9.998	1185	1192	1203	rBV	390889	647814	28.81%	3.049%
23	10.369	1247	1255	1267	rBV	517463	837338	37.24%	3.942%
24	10.522	1272	1281	1293	rBV	314341	573126	25.49%	2.698%
25	11.651	1468	1473	1480	rVB3	6847	13380	0.60%	0.063%
26	11.981	1521	1529	1536	rBV5	7637	14840	0.66%	0.070%
27	12.863	1675	1679	1682	rBV6	1993	2990	0.13%	0.014%
28	12.975	1693	1698	1701	rBV7	1950	2561	0.11%	0.012%
29	13.163	1726	1730	1735	rVB7	2094	3395	0.15%	0.016%
30	13.222	1735	1740	1747	rBV10	2095	4239	0.19%	0.020%
31	13.681	1810	1818	1830	rBV	788221	1076038	47.86%	5.065%
32	13.945	1855	1863	1875	rBV	830516	1187586	52.82%	5.590%
33	14.257	1909	1916	1925	rBV	649657	954097	42.44%	4.491%
34	14.322	1925	1927	1931	rVB4	4601	4818	0.21%	0.023%
35	14.504	1950	1958	1970	rBV3	17890	61398	2.73%	0.289%
36	14.910	2022	2027	2031	rBV8	1544	2440	0.11%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011384.D
 Acq On : 11 Aug 2022 13:18
 Operator : CG/JU
 Sample : N4128-11
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBT8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

37	15.257	2079	2086	2100	rBV	999071	1502522	66.83%	7.073%
38	15.392	2103	2109	2123	rVV	348533	510596	22.71%	2.403%
39	15.498	2124	2127	2135	rVB4	13547	23957	1.07%	0.113%
40	15.710	2158	2163	2165	rBV5	2032	2553	0.11%	0.012%
41	16.057	2217	2222	2229	rVB9	3222	6530	0.29%	0.031%
42	16.163	2237	2240	2245	rVB6	1968	3468	0.15%	0.016%
43	16.516	2295	2300	2303	rBV4	3929	5644	0.25%	0.027%
44	16.704	2330	2332	2335	rVB4	2355	2251	0.10%	0.011%
45	16.804	2346	2349	2355	rVB8	2249	4190	0.19%	0.020%
46	17.028	2381	2387	2398	rBV	802517	1109857	49.37%	5.224%
47	17.128	2398	2404	2421	rVV	1266926	1851128	82.34%	8.714%
48	17.598	2479	2484	2487	rBV4	4634	6719	0.30%	0.032%
49	17.727	2501	2506	2510	rBV7	2725	3820	0.17%	0.018%
50	17.945	2540	2543	2546	rBV5	3159	4466	0.20%	0.021%
51	18.022	2551	2556	2560	rVB2	5103	8709	0.39%	0.041%
52	18.057	2560	2562	2564	rBV3	2113	2839	0.13%	0.013%
53	18.410	2620	2622	2629	rVB8	2800	3436	0.15%	0.016%
54	18.963	2712	2716	2722	rBV3	15772	24073	1.07%	0.113%
55	19.039	2725	2729	2733	rVV3	14431	21008	0.93%	0.099%
56	19.345	2778	2781	2783	rBV4	5834	6913	0.31%	0.033%
57	19.392	2783	2789	2796	rBV	1665206	2121291	94.35%	9.985%
58	21.157	3084	3089	3099	rBV	942601	1277148	56.81%	6.012%
59	23.321	3450	3457	3465	rBV	1176452	2248209	100.00%	10.583%
60	23.468	3476	3482	3496	rVB2	690517	1327948	59.07%	6.251%




Sum of corrected areas: 21244006

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011384.D
Acq On : 11 Aug 2022 13:18
Operator : CG/JU
Sample : N4128-11
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBT8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

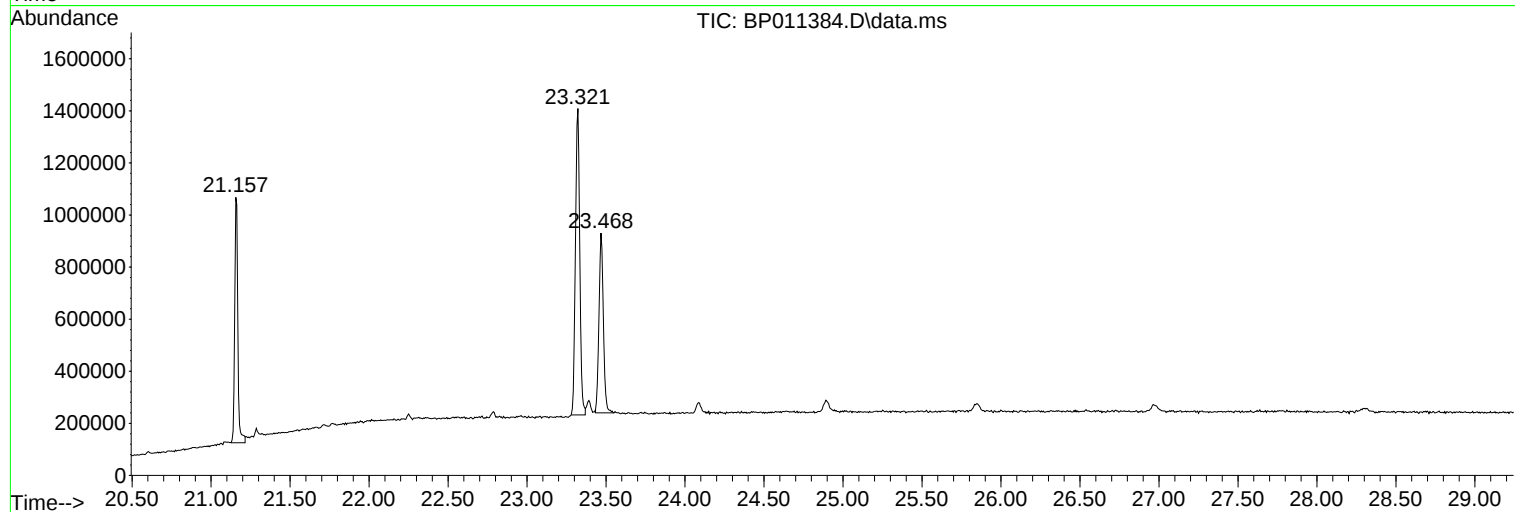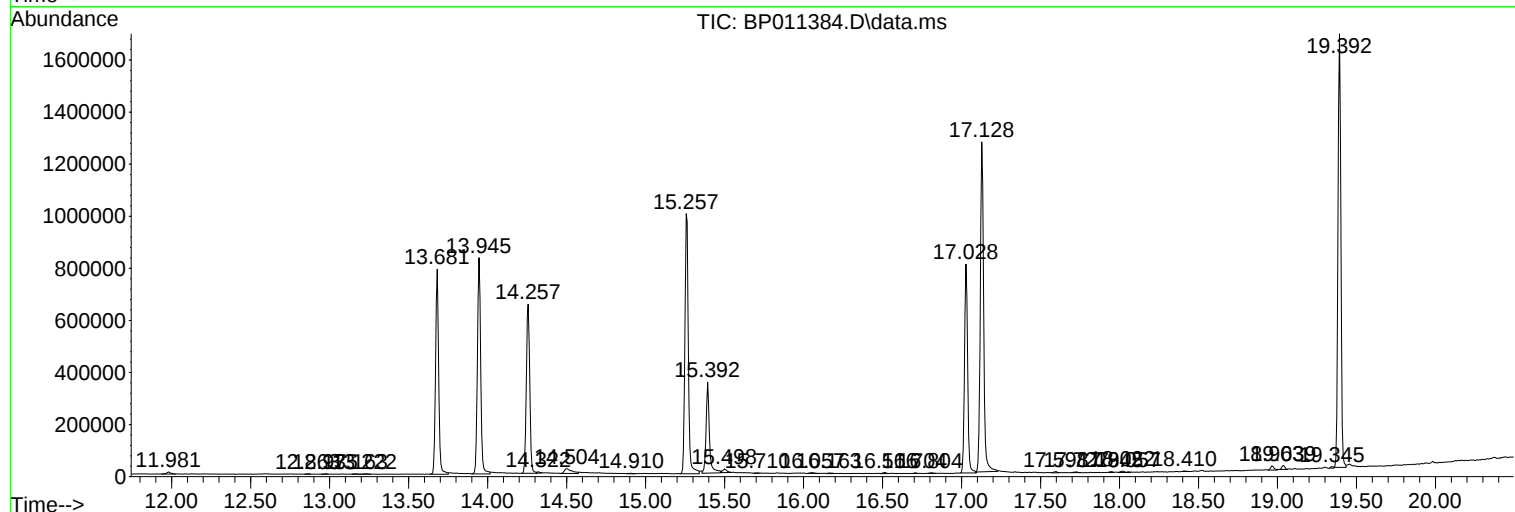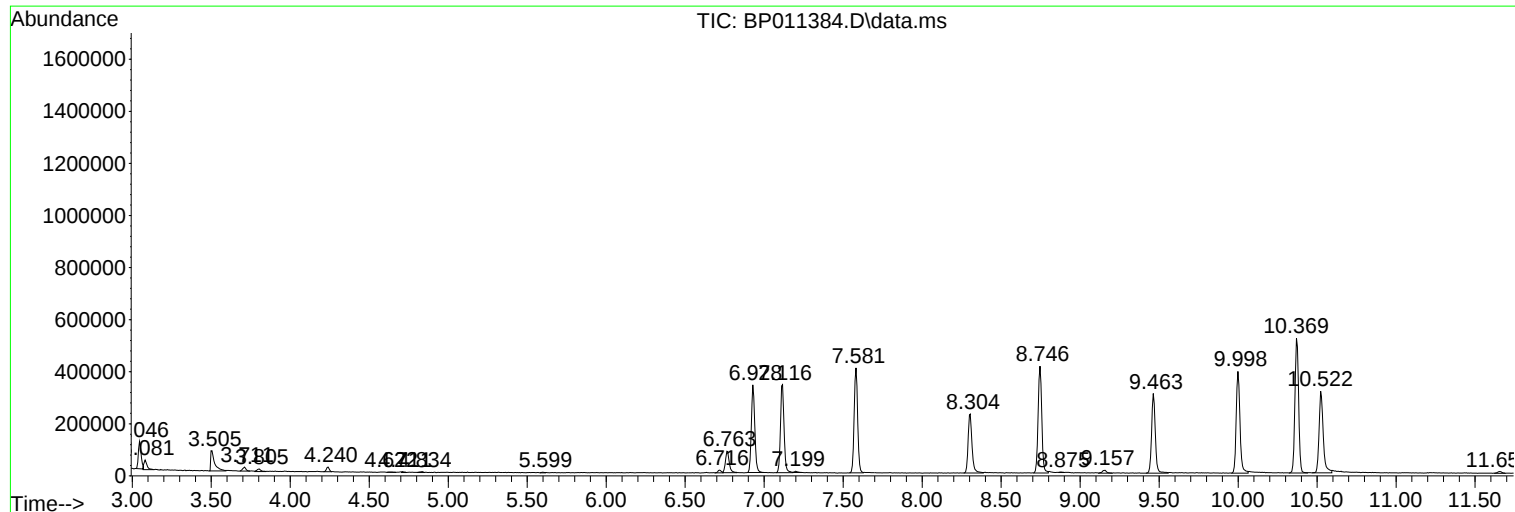

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011384.D
Acq On : 11 Aug 2022 13:18
Operator : CG/JU
Sample : N4128-11
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBT8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011384.D
Acq On : 11 Aug 2022 13:18
Operator : CG/JU
Sample : N4128-11
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBT8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc