

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011385.D
 Acq On : 11 Aug 2022 13:53
 Operator : CG/JU
 Sample : N4128-12
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBT9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011385.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.081	13	16	28	rVB	32022	43795	1.67%	0.180%
2	3.499	84	87	107	rBV	142153	231254	8.81%	0.948%
3	3.711	118	123	127	rBV2	15942	24026	0.92%	0.099%
4	3.799	135	138	143	rVB2	7518	9381	0.36%	0.038%
5	4.240	208	213	220	rVB	23846	32808	1.25%	0.135%
6	4.710	290	293	297	rVB4	3282	3773	0.14%	0.015%
7	4.834	310	314	316	rVB4	3378	3350	0.13%	0.014%
8	6.716	630	634	637	rBV2	11250	15856	0.60%	0.065%
9	6.763	637	642	655	rVB	97178	160064	6.10%	0.656%
10	6.928	664	670	684	rBV	362767	556502	21.20%	2.282%
11	7.116	695	702	713	rBV	364750	591283	22.53%	2.425%
12	7.199	713	716	720	rVB5	4371	6274	0.24%	0.026%
13	7.581	773	781	790	rBV	410715	633172	24.12%	2.596%
14	7.657	790	794	797	rVB6	1971	3022	0.12%	0.012%
15	8.304	896	904	917	rBV	262044	444202	16.92%	1.821%
16	8.746	972	979	987	rBV	454279	725346	27.64%	2.974%
17	8.910	1005	1007	1016	rVB10	2445	4457	0.17%	0.018%
18	9.151	1042	1048	1053	rVB2	14276	21318	0.81%	0.087%
19	9.463	1093	1101	1114	rBV	350871	568109	21.65%	2.330%
20	9.910	1173	1177	1179	rBV5	1674	2750	0.10%	0.011%
21	9.998	1184	1192	1212	rBV	437651	753284	28.70%	3.089%
22	10.369	1247	1255	1267	rBV	521151	870550	33.17%	3.570%
23	10.522	1273	1281	1292	rBV	372210	687477	26.19%	2.819%
24	11.657	1468	1474	1478	rVB3	9082	13657	0.52%	0.056%
25	11.816	1497	1501	1504	rBV6	1996	2874	0.11%	0.012%
26	11.981	1524	1529	1534	rBV4	6895	12782	0.49%	0.052%
27	13.681	1812	1818	1829	rBV	958394	1319407	50.27%	5.410%
28	13.945	1856	1863	1876	rBV	982299	1423157	54.22%	5.836%
29	14.257	1909	1916	1924	rBV	709592	1040866	39.66%	4.268%
30	14.498	1951	1957	1972	rBV3	24277	77667	2.96%	0.318%
31	14.792	2004	2007	2012	rVB7	1985	3327	0.13%	0.014%
32	15.075	2052	2055	2058	rBV3	2070	3108	0.12%	0.013%
33	15.257	2080	2086	2103	rBV	1196563	1839610	70.09%	7.543%
34	15.392	2103	2109	2120	rVV	456260	639933	24.38%	2.624%
35	15.498	2124	2127	2138	rVB3	14514	29081	1.11%	0.119%
36	15.957	2201	2205	2209	rBV6	2122	3002	0.11%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011385.D
 Acq On : 11 Aug 2022 13:53
 Operator : CG/JU
 Sample : N4128-12
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBT9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

37	15.998	2209	2212	2215	rVV5	2844	3632	0.14%	0.015%
38	16.051	2218	2221	2225	rVB6	3195	5055	0.19%	0.021%
39	16.510	2295	2299	2304	rVB4	6409	9281	0.35%	0.038%
40	16.698	2330	2331	2337	rVB6	2656	3990	0.15%	0.016%
41	16.810	2346	2350	2354	rVV6	3777	6885	0.26%	0.028%
42	16.975	2374	2378	2380	rBV4	3385	4045	0.15%	0.017%
43	17.027	2381	2387	2398	rBV	887741	1233915	47.01%	5.060%
44	17.127	2398	2404	2421	rVV2	1535768	2208914	84.16%	9.058%
45	17.592	2480	2483	2488	rVB2	5985	8349	0.32%	0.034%
46	17.727	2500	2506	2509	rBV8	4530	7002	0.27%	0.029%
47	17.945	2540	2543	2547	rBV5	5089	7707	0.29%	0.032%
48	18.016	2552	2555	2562	rVB	7445	10320	0.39%	0.042%
49	18.522	2637	2641	2645	rVB5	5784	6484	0.25%	0.027%
50	18.963	2713	2716	2723	rBV4	18539	26438	1.01%	0.108%
51	19.033	2724	2728	2732	rBV3	17357	25388	0.97%	0.104%
52	19.392	2783	2789	2798	rBV	1982094	2521518	96.07%	10.339%
53	20.892	3040	3044	3051	rBV2	66577	118142	4.50%	0.484%
54	21.157	3085	3089	3098	rBV	1016460	1347355	51.34%	5.525%
55	23.321	3450	3457	3464	rBV2	1435354	2624560	100.00%	10.762%
56	23.468	3476	3482	3494	rVB	730840	1407910	53.64%	5.773%




Sum of corrected areas: 24387414

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011385.D
Acq On : 11 Aug 2022 13:53
Operator : CG/JU
Sample : N4128-12
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBT9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

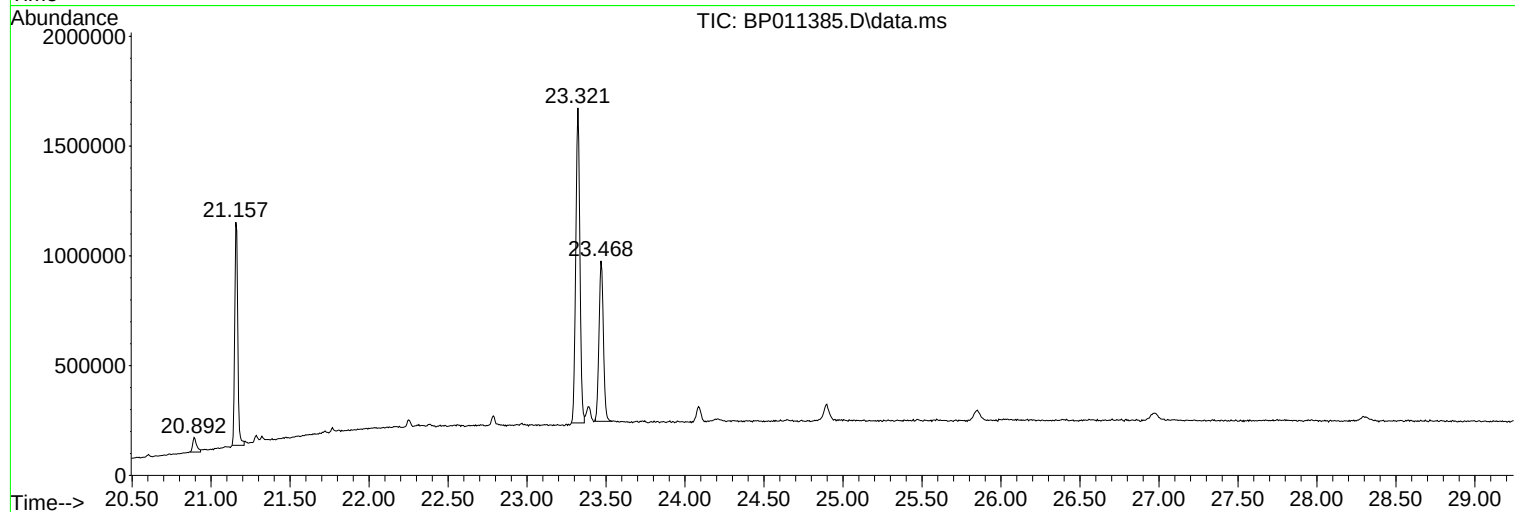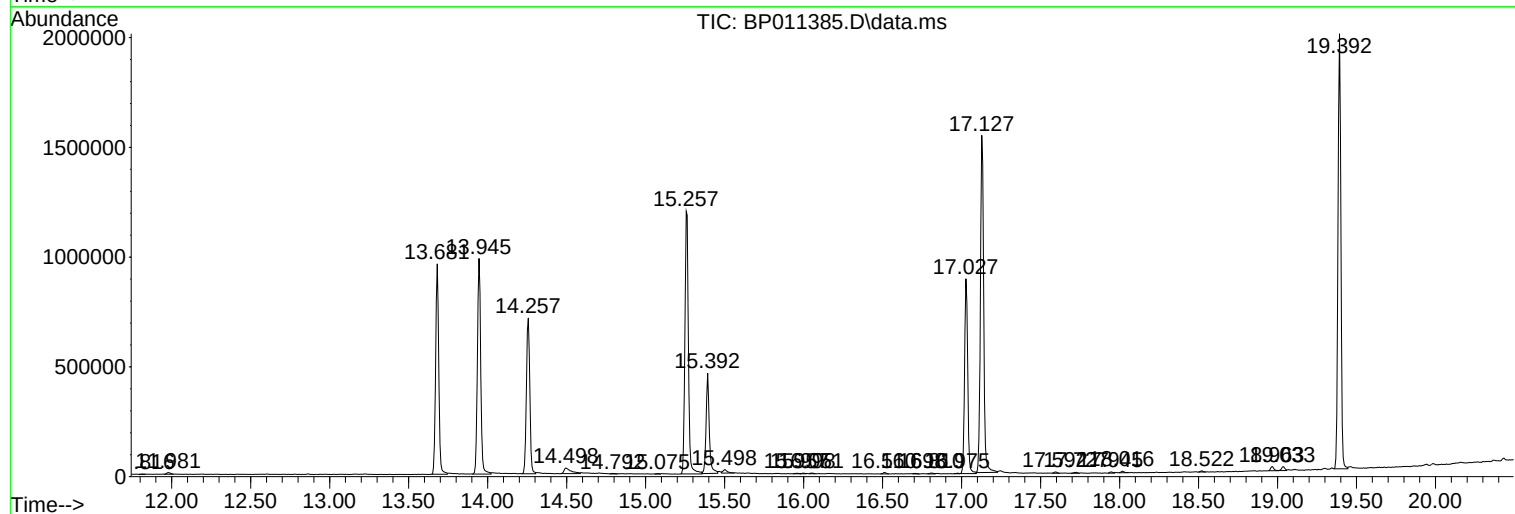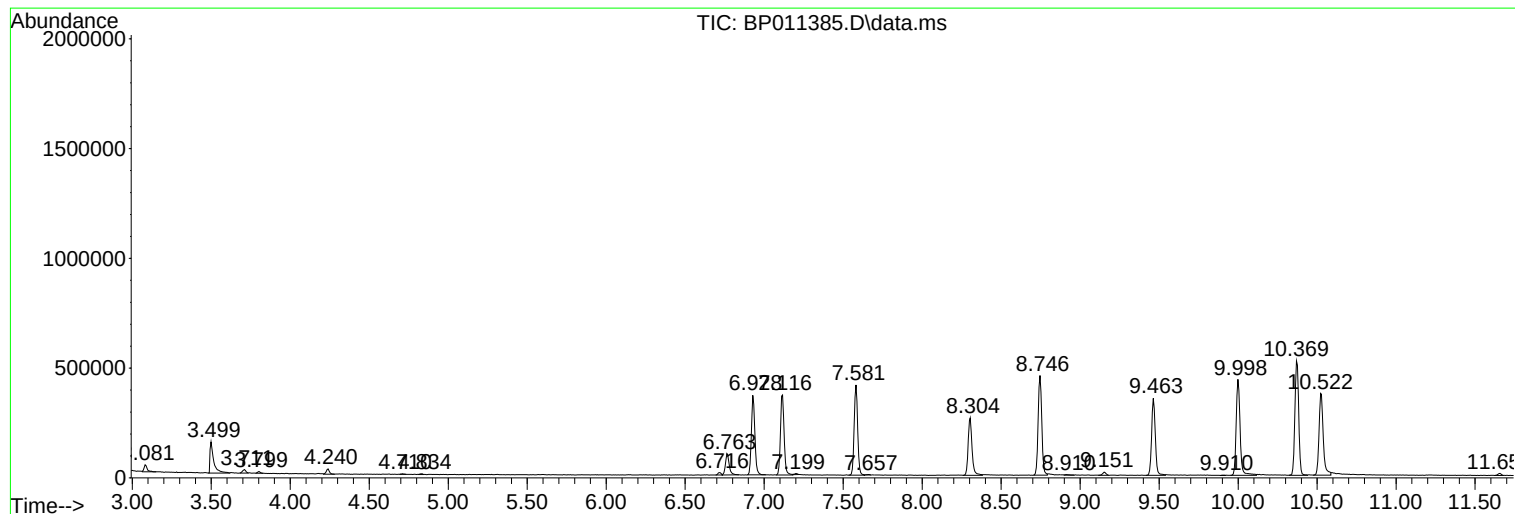

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011385.D
Acq On : 11 Aug 2022 13:53
Operator : CG/JU
Sample : N4128-12
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBT9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011385.D
Acq On : 11 Aug 2022 13:53
Operator : CG/JU
Sample : N4128-12
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBT9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------