

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011386.D
 Acq On : 11 Aug 2022 14:27
 Operator : CG/JU
 Sample : N4128-13
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBX5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011386.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.081	13	16	22	rVB	30908	36063	1.65%	0.169%
2	3.499	85	87	103	rBV	126292	201080	9.21%	0.942%
3	3.711	119	123	127	rVB	13539	16561	0.76%	0.078%
4	3.799	135	138	143	rVB	8185	11513	0.53%	0.054%
5	4.234	208	212	220	rVB	20414	27283	1.25%	0.128%
6	4.711	289	293	295	rBV5	2406	3011	0.14%	0.014%
7	5.234	380	382	387	rVB5	1567	2577	0.12%	0.012%
8	6.563	602	608	609	rBV5	1696	2750	0.13%	0.013%
9	6.622	615	618	622	rBV5	1873	2954	0.14%	0.014%
10	6.716	629	634	637	rBV2	9914	13756	0.63%	0.064%
11	6.763	637	642	654	rVB	84389	138534	6.35%	0.649%
12	6.928	663	670	683	rBV	345788	533246	24.42%	2.498%
13	7.110	695	701	713	rBV	334556	535960	24.55%	2.511%
14	7.199	713	716	720	rVB6	3789	5843	0.27%	0.027%
15	7.581	774	781	790	rBV	395215	608428	27.87%	2.850%
16	7.663	792	795	804	rVB	3351	5730	0.26%	0.027%
17	8.299	897	903	915	rBV	230573	391006	17.91%	1.832%
18	8.746	971	979	988	rBV	421458	675738	30.95%	3.165%
19	9.152	1041	1048	1058	rVB	11551	20946	0.96%	0.098%
20	9.463	1094	1101	1114	rBV	306410	500898	22.94%	2.346%
21	9.999	1184	1192	1205	rBV	401696	668406	30.62%	3.131%
22	10.369	1247	1255	1263	rBV	494377	812594	37.22%	3.807%
23	10.522	1274	1281	1298	rBV	341436	640552	29.34%	3.001%
24	11.651	1467	1473	1478	rBV	7592	12253	0.56%	0.057%
25	11.981	1523	1529	1535	rBV4	7225	14875	0.68%	0.070%
26	12.198	1560	1566	1569	rVB8	1236	2653	0.12%	0.012%
27	12.598	1629	1634	1639	rBV8	2521	4905	0.22%	0.023%
28	12.863	1674	1679	1683	rVB7	2425	3850	0.18%	0.018%
29	13.157	1725	1729	1733	rVB7	1719	3194	0.15%	0.015%
30	13.222	1737	1740	1744	rBV5	1495	2406	0.11%	0.011%
31	13.681	1811	1818	1831	rBV	819775	1155625	52.93%	5.413%
32	13.792	1834	1837	1842	rVB7	4106	7113	0.33%	0.033%
33	13.945	1854	1863	1876	rBV	843881	1247012	57.12%	5.842%
34	14.257	1909	1916	1921	rBV	658602	951297	43.57%	4.456%
35	14.504	1951	1958	1967	rBV2	16657	50820	2.33%	0.238%
36	15.069	2049	2054	2059	rBV7	2481	4755	0.22%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011386.D
 Acq On : 11 Aug 2022 14:27
 Operator : CG/JU
 Sample : N4128-13
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBX5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

37	15.257	2078	2086	2102	rBV	1063562	1596128	73.11%	7.477%
38	15.392	2103	2109	2123	rVV	335160	511600	23.43%	2.397%
39	15.504	2124	2128	2134	rVB4	11756	21785	1.00%	0.102%
40	15.839	2181	2185	2187	rBV5	1671	2523	0.12%	0.012%
41	16.051	2218	2221	2227	rVB7	3694	6575	0.30%	0.031%
42	16.169	2236	2241	2243	rBV6	2141	3345	0.15%	0.016%
43	16.510	2296	2299	2307	rVB3	5411	7765	0.36%	0.036%
44	16.592	2310	2313	2318	rVB7	1567	2302	0.11%	0.011%
45	16.704	2326	2332	2338	rVB7	2126	4751	0.22%	0.022%
46	16.769	2338	2343	2346	rBV7	1125	2302	0.11%	0.011%
47	16.810	2346	2350	2354	rBV7	3454	5307	0.24%	0.025%
48	16.975	2375	2378	2381	rBV5	2213	3284	0.15%	0.015%
49	17.028	2381	2387	2398	rBV	784936	1116389	51.13%	5.230%
50	17.128	2398	2404	2421	rVV	1292988	1864978	85.42%	8.736%
51	17.598	2480	2484	2488	rBV3	5813	8667	0.40%	0.041%
52	17.728	2502	2506	2511	rBV8	3286	5428	0.25%	0.025%
53	18.022	2552	2556	2560	rBV	5641	6101	0.28%	0.029%
54	18.522	2636	2641	2644	rBV6	3923	6370	0.29%	0.030%
55	18.969	2713	2717	2721	rBV3	15152	21422	0.98%	0.100%
56	19.039	2724	2729	2733	rVV	15030	22721	1.04%	0.106%
57	19.339	2778	2780	2783	rBV4	4393	5715	0.26%	0.027%
58	19.392	2783	2789	2804	rVV	1670916	2145996	98.29%	10.053%
59	21.157	3085	3089	3098	rBV	897757	1201997	55.06%	5.631%
60	23.321	3450	3457	3466	rBV2	1172891	2183232	100.00%	10.227%
61	23.468	3476	3482	3493	rVB2	662293	1274280	58.37%	5.969%




Sum of corrected areas: 21347150

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011386.D
Acq On : 11 Aug 2022 14:27
Operator : CG/JU
Sample : N4128-13
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBX5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

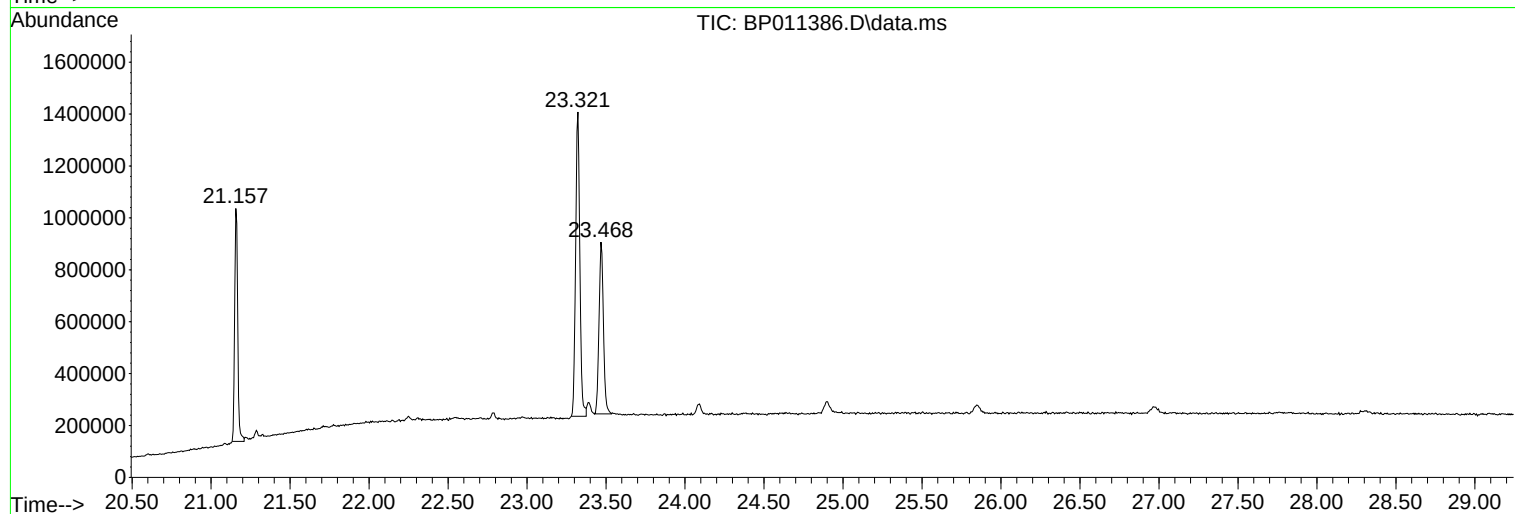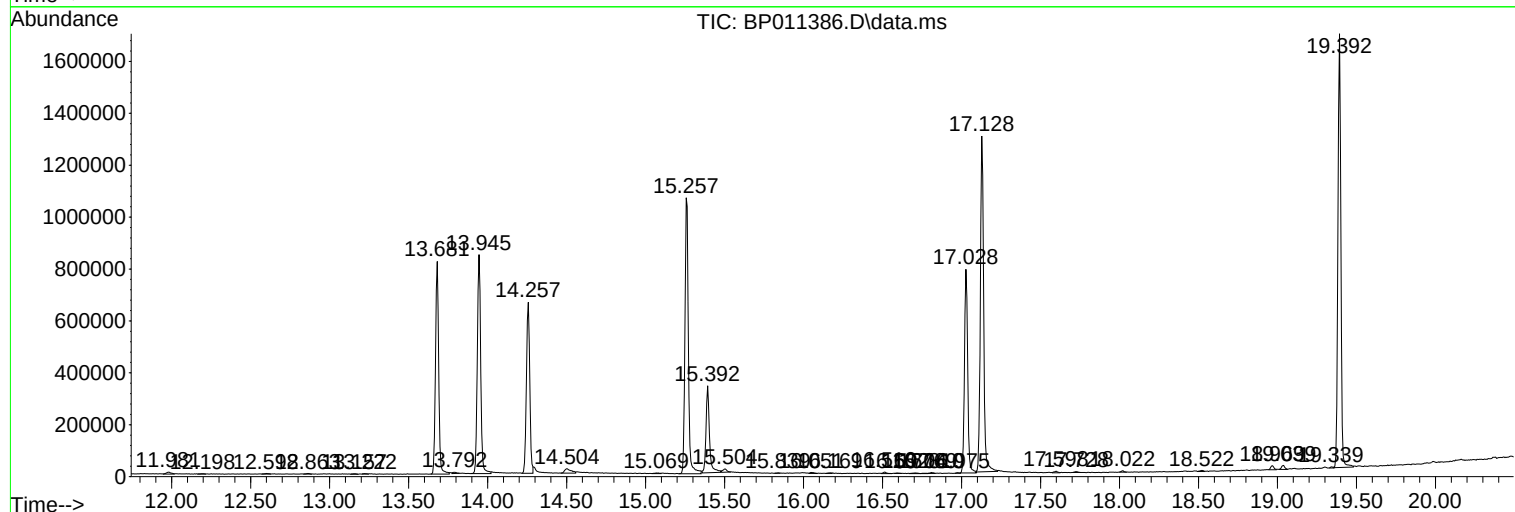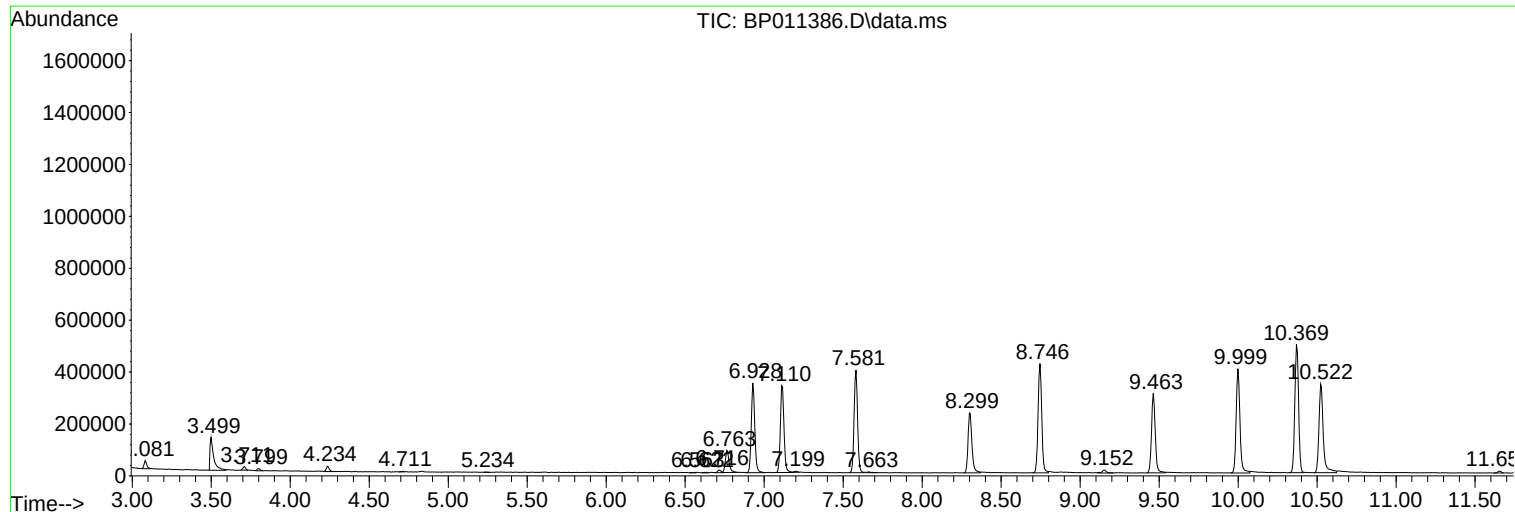

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011386.D
Acq On : 11 Aug 2022 14:27
Operator : CG/JU
Sample : N4128-13
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBX5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011386.D
Acq On : 11 Aug 2022 14:27
Operator : CG/JU
Sample : N4128-13
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBX5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc