

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011387.D
 Acq On : 11 Aug 2022 15:02
 Operator : CG/JU
 Sample : N4128-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBZ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011387.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.081	13	16	22	rVB	26866	32201	1.39%	0.147%
2	3.499	85	87	107	rBV	123166	196047	8.47%	0.895%
3	3.705	118	122	128	rVB	13147	20098	0.87%	0.092%
4	3.799	135	138	144	rVB	8452	11726	0.51%	0.054%
5	4.234	208	212	217	rVB	18046	23362	1.01%	0.107%
6	4.711	290	293	296	rVB4	2707	3755	0.16%	0.017%
7	4.828	310	313	318	rBV7	2579	4085	0.18%	0.019%
8	5.599	441	444	448	rBV5	1952	2385	0.10%	0.011%
9	6.716	628	634	637	rBV2	8001	13161	0.57%	0.060%
10	6.764	637	642	656	rVB	93228	155724	6.72%	0.711%
11	6.928	664	670	688	rVB	326905	505286	21.82%	2.307%
12	7.111	695	701	713	rBV	338306	531864	22.97%	2.428%
13	7.199	713	716	725	rVB8	3847	8369	0.36%	0.038%
14	7.581	774	781	791	rBV	387774	596714	25.77%	2.724%
15	8.299	897	903	918	rBV	240548	415863	17.96%	1.898%
16	8.746	971	979	988	rBV	410645	649724	28.06%	2.966%
17	9.152	1043	1048	1053	rVB2	10822	16785	0.72%	0.077%
18	9.463	1093	1101	1109	rBV	304681	494013	21.33%	2.255%
19	9.999	1183	1192	1205	rBV	392840	661246	28.56%	3.019%
20	10.369	1247	1255	1266	rBV	500416	817173	35.29%	3.730%
21	10.522	1275	1281	1298	rBV	343351	634503	27.40%	2.896%
22	11.657	1468	1474	1480	rBV2	6620	11940	0.52%	0.055%
23	11.981	1524	1529	1537	rBV5	6212	12150	0.52%	0.055%
24	12.657	1641	1644	1649	rVB7	1501	2710	0.12%	0.012%
25	12.863	1675	1679	1684	rBV8	1699	2565	0.11%	0.012%
26	13.163	1724	1730	1735	rBV9	1526	2898	0.13%	0.013%
27	13.234	1735	1742	1747	rVB9	2615	4824	0.21%	0.022%
28	13.681	1811	1818	1832	rBV	819716	1149710	49.65%	5.248%
29	13.769	1832	1833	1840	rVB7	3152	4125	0.18%	0.019%
30	13.946	1855	1863	1880	rBV	851682	1247376	53.87%	5.694%
31	14.257	1909	1916	1925	rBV	674448	975492	42.13%	4.453%
32	14.493	1951	1956	1967	rBV4	21963	65854	2.84%	0.301%
33	15.128	2060	2064	2069	rVB8	2276	3093	0.13%	0.014%
34	15.257	2080	2086	2103	rBV	1029791	1587671	68.56%	7.248%
35	15.393	2103	2109	2121	rVV	398520	575896	24.87%	2.629%
36	15.498	2124	2127	2136	rVB3	12134	24441	1.06%	0.112%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011387.D
 Acq On : 11 Aug 2022 15:02
 Operator : CG/JU
 Sample : N4128-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBZ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

37	15.828	2181	2183	2189	rVB7	1662	2338	0.10%	0.011%
38	15.992	2205	2211	2216	rBV5	5996	11499	0.50%	0.052%
39	16.051	2218	2221	2229	rVB10	3869	7457	0.32%	0.034%
40	16.163	2236	2240	2245	rVB8	2028	2456	0.11%	0.011%
41	16.516	2294	2300	2304	rBV3	5092	7670	0.33%	0.035%
42	16.704	2328	2332	2336	rVB7	1808	2729	0.12%	0.012%
43	16.810	2346	2350	2354	rBV7	2862	4775	0.21%	0.022%
44	16.975	2374	2378	2380	rBV5	2444	3513	0.15%	0.016%
45	17.028	2381	2387	2397	rVV	816897	1163469	50.24%	5.311%
46	17.128	2398	2404	2424	rVV	1367859	1969209	85.04%	8.989%
47	17.551	2474	2476	2480	rVB5	2412	2451	0.11%	0.011%
48	17.598	2480	2484	2487	rBV3	5955	8114	0.35%	0.037%
49	17.722	2503	2505	2513	rVB9	3519	5018	0.22%	0.023%
50	17.945	2541	2543	2549	rVB7	1711	2468	0.11%	0.011%
51	18.416	2621	2623	2628	rVB5	3028	3038	0.13%	0.014%
52	18.522	2637	2641	2646	rBV6	4415	7835	0.34%	0.036%
53	18.969	2712	2717	2722	rBV4	17108	24801	1.07%	0.113%
54	19.033	2724	2728	2733	rBV2	15283	23647	1.02%	0.108%
55	19.345	2778	2781	2783	rBV4	4632	6157	0.27%	0.028%
56	19.392	2783	2789	2798	rBV	1796834	2264307	97.78%	10.336%
57	19.980	2887	2889	2893	rBV5	8449	11122	0.48%	0.051%
58	21.163	3085	3090	3099	rBV	952413	1295560	55.95%	5.914%
59	23.322	3450	3457	3466	rBV2	1214032	2315637	100.00%	10.571%
60	23.469	3476	3482	3493	rVB	647825	1296026	55.97%	5.916%




Sum of corrected areas: 21906125

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011387.D
Acq On : 11 Aug 2022 15:02
Operator : CG/JU
Sample : N4128-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBZ9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

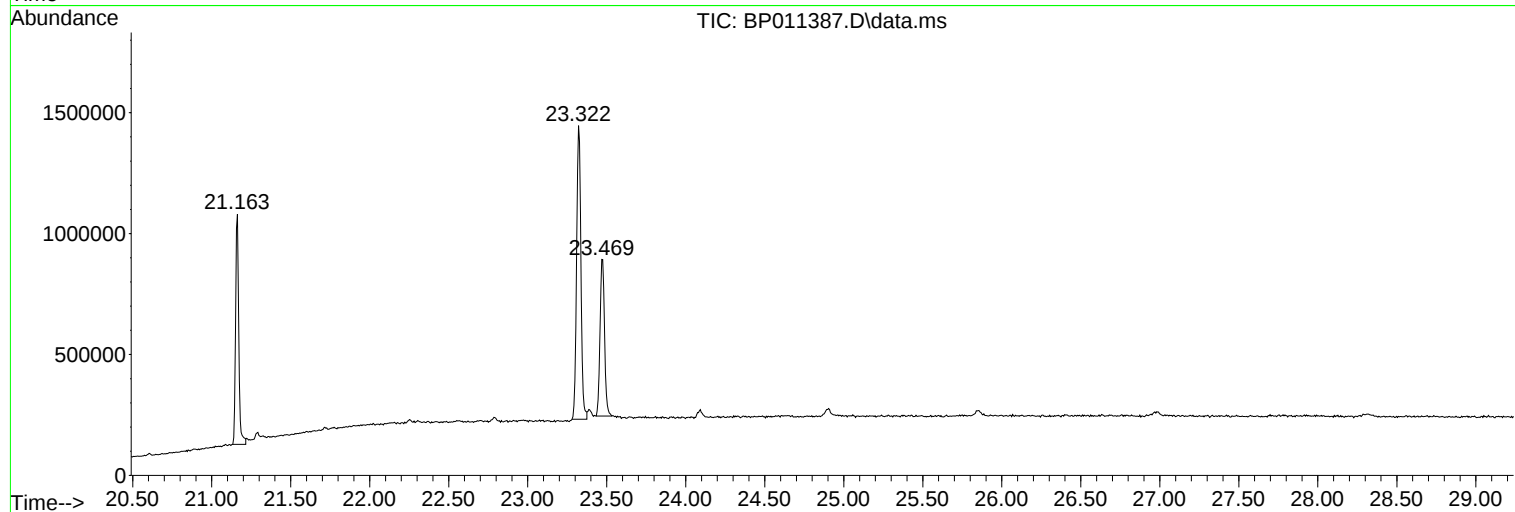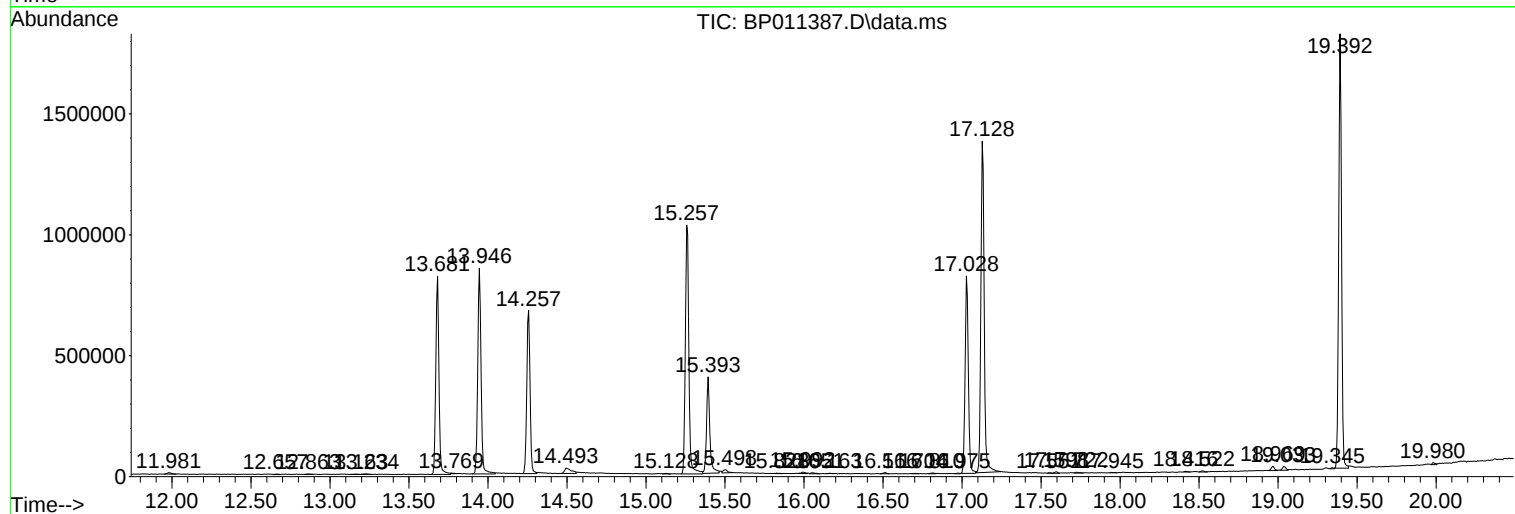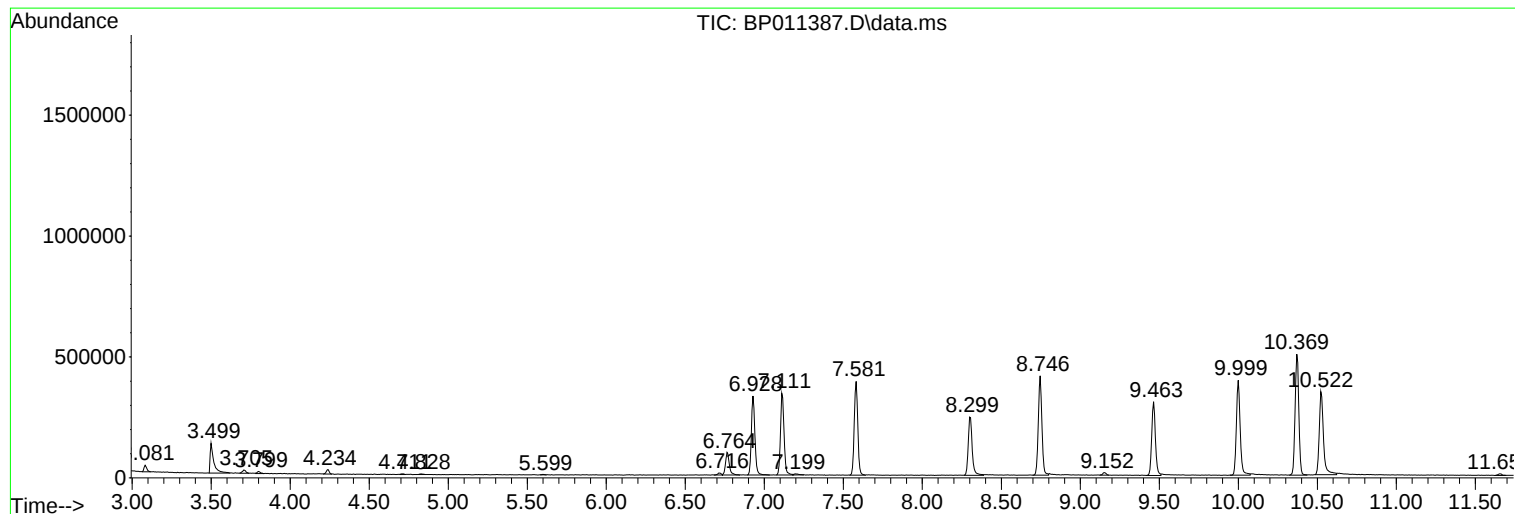

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011387.D
Acq On : 11 Aug 2022 15:02
Operator : CG/JU
Sample : N4128-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBZ9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011387.D
Acq On : 11 Aug 2022 15:02
Operator : CG/JU
Sample : N4128-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBZ9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc