

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011388.D
 Acq On : 11 Aug 2022 15:36
 Operator : CG/JU
 Sample : N4128-16
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGC10

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011388.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.081	13	16	22	rVB	29203	34797	1.29%	0.137%
2	3.499	84	87	100	rBV	92429	145387	5.39%	0.572%
3	3.705	118	122	129	rVB	13937	21406	0.79%	0.084%
4	3.799	134	138	144	rVB2	9836	14045	0.52%	0.055%
5	4.234	209	212	217	rVB	18448	23742	0.88%	0.093%
6	4.711	289	293	296	rBV6	2846	3967	0.15%	0.016%
7	4.834	308	314	317	rVB6	2763	5357	0.20%	0.021%
8	5.605	439	445	450	rBV7	5841	9030	0.33%	0.036%
9	6.628	615	619	623	rBV6	2975	4539	0.17%	0.018%
10	6.716	629	634	637	rVV2	10416	16477	0.61%	0.065%
11	6.763	637	642	653	rVB	89301	150443	5.57%	0.592%
12	6.928	663	670	681	rBV	357693	549988	20.37%	2.163%
13	7.110	694	701	711	rBV	358247	572115	21.19%	2.250%
14	7.199	713	716	727	rVB4	13962	27720	1.03%	0.109%
15	7.581	772	781	790	rBV	423451	656718	24.33%	2.583%
16	8.228	886	891	897	rBV9	3730	7097	0.26%	0.028%
17	8.299	897	903	913	rBV	244678	413378	15.31%	1.626%
18	8.746	972	979	986	rBV	450168	709349	26.28%	2.789%
19	8.804	986	989	998	rVB2	20565	30865	1.14%	0.121%
20	8.875	998	1001	1004	rBV5	3553	5284	0.20%	0.021%
21	9.152	1041	1048	1053	rVB2	11026	20084	0.74%	0.079%
22	9.463	1092	1101	1117	rBV	340035	565134	20.93%	2.222%
23	9.651	1131	1133	1137	rVB5	2533	3149	0.12%	0.012%
24	9.728	1141	1146	1149	rBV6	3496	6668	0.25%	0.026%
25	9.769	1149	1153	1154	rVV4	2914	3048	0.11%	0.012%
26	9.804	1157	1159	1164	rVB6	3537	4640	0.17%	0.018%
27	9.840	1164	1165	1171	rVB5	2791	3358	0.12%	0.013%
28	9.910	1171	1177	1181	rBV8	2910	6094	0.23%	0.024%
29	9.999	1183	1192	1213	rBV	432631	732764	27.14%	2.882%
30	10.369	1247	1255	1271	rVB	550449	936542	34.69%	3.683%
31	10.522	1271	1281	1299	rBV	340595	635280	23.53%	2.498%
32	11.222	1395	1400	1406	rVB9	5217	8636	0.32%	0.034%
33	11.298	1408	1413	1418	rVB6	5313	9715	0.36%	0.038%
34	11.404	1427	1431	1437	rBV5	5050	8118	0.30%	0.032%
35	11.575	1454	1460	1464	rBV9	5127	9457	0.35%	0.037%
36	11.657	1467	1474	1481	rVB	8943	16717	0.62%	0.066%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011388.D
 Acq On : 11 Aug 2022 15:36
 Operator : CG/JU
 Sample : N4128-16
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGC10

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

37	11.816	1496	1501	1509	rVB2	31249	46843	1.74%	0.184%
38	11.940	1517	1522	1524	rBV5	2333	3138	0.12%	0.012%
39	11.981	1524	1529	1533	rVB2	6208	9337	0.35%	0.037%
40	12.051	1539	1541	1545	rVB5	3871	4161	0.15%	0.016%
41	12.304	1581	1584	1590	rVB8	4173	7104	0.26%	0.028%
42	12.463	1602	1611	1615	rBV8	3109	7342	0.27%	0.029%
43	12.510	1615	1619	1625	rVB9	3756	6576	0.24%	0.026%
44	12.569	1625	1629	1633	rBV6	4028	7162	0.27%	0.028%
45	12.640	1636	1641	1650	rVB6	5499	12824	0.48%	0.050%
46	12.728	1652	1656	1662	rBV6	4928	9415	0.35%	0.037%
47	12.787	1662	1666	1671	rVB5	5953	9479	0.35%	0.037%
48	13.081	1707	1716	1722	rVB	39347	57875	2.14%	0.228%
49	13.169	1727	1731	1733	rBV4	2292	3473	0.13%	0.014%
50	13.240	1740	1743	1748	rVB6	4105	6321	0.23%	0.025%
51	13.404	1765	1771	1772	rBV6	3129	4529	0.17%	0.018%
52	13.581	1794	1801	1802	rBV6	1765	3424	0.13%	0.013%
53	13.622	1802	1808	1811	rVV8	3004	5352	0.20%	0.021%
54	13.681	1811	1818	1833	rBV	910005	1295601	47.99%	5.095%
55	13.787	1833	1836	1842	rVB6	6883	9582	0.35%	0.038%
56	13.863	1845	1849	1853	rVB6	3898	5388	0.20%	0.021%
57	13.945	1854	1863	1875	rBV	971649	1391240	51.54%	5.471%
58	14.169	1896	1901	1906	rVB	40310	49738	1.84%	0.196%
59	14.257	1909	1916	1925	rBV	763133	1101255	40.79%	4.331%
60	14.498	1951	1957	1966	rBV4	24086	64940	2.41%	0.255%
61	14.622	1974	1978	1984	rVB9	4997	9836	0.36%	0.039%
62	14.675	1984	1987	1990	rBV5	3833	4249	0.16%	0.017%
63	14.792	2003	2007	2012	rVB4	7151	10025	0.37%	0.039%
64	14.863	2015	2019	2022	rBV5	3974	6452	0.24%	0.025%
65	15.128	2058	2064	2069	rVB	35867	45398	1.68%	0.179%
66	15.257	2078	2086	2100	rBV	1181109	1779102	65.90%	6.996%
67	15.392	2103	2109	2122	rVB	457085	615597	22.80%	2.421%
68	15.504	2124	2128	2131	rBV5	8602	12478	0.46%	0.049%
69	15.634	2148	2150	2156	rVB6	4101	4966	0.18%	0.020%
70	15.692	2157	2160	2164	rVV6	5013	6401	0.24%	0.025%
71	15.751	2166	2170	2175	rVB8	4756	6836	0.25%	0.027%
72	15.834	2180	2184	2188	rBV7	2947	5294	0.20%	0.021%
73	15.951	2201	2204	2207	rBV5	2232	3446	0.13%	0.014%
74	15.998	2208	2212	2220	rBV	37099	60074	2.23%	0.236%
75	16.345	2267	2271	2274	rBV6	3515	5375	0.20%	0.021%
76	16.404	2279	2281	2286	rVB6	4450	5544	0.21%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011388.D
 Acq On : 11 Aug 2022 15:36
 Operator : CG/JU
 Sample : N4128-16
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGC10

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

77	16.469	2287	2292	2294	rBV5	3148	3875	0.14%	0.015%
78	16.516	2297	2300	2303	rVV3	5345	6184	0.23%	0.024%
79	16.804	2344	2349	2353	rBV	35432	47103	1.74%	0.185%
80	16.851	2353	2357	2361	rVV4	11994	18877	0.70%	0.074%
81	17.028	2381	2387	2398	rBV	943161	1328758	49.22%	5.225%
82	17.128	2398	2404	2417	rVV2	1556377	2200633	81.52%	8.654%
83	17.345	2438	2441	2447	rVB8	5149	7849	0.29%	0.031%
84	17.551	2471	2476	2480	rBV	30168	36343	1.35%	0.143%
85	17.592	2481	2483	2488	rVB6	5542	7528	0.28%	0.030%
86	17.728	2502	2506	2511	rVB	24811	31936	1.18%	0.126%
87	17.833	2520	2524	2525	rBV4	2899	3846	0.14%	0.015%
88	17.945	2539	2543	2548	rBV5	10915	16198	0.60%	0.064%
89	18.233	2588	2592	2597	rBV	27916	32078	1.19%	0.126%
90	18.845	2692	2696	2699	rBV2	73762	96691	3.58%	0.380%
91	18.875	2699	2701	2707	rVB2	43064	53464	1.98%	0.210%
92	18.963	2713	2716	2721	rBV3	18556	24636	0.91%	0.097%
93	19.010	2721	2724	2725	rBV2	8738	8753	0.32%	0.034%
94	19.039	2725	2729	2732	rVB	16069	22018	0.82%	0.087%
95	19.392	2783	2789	2798	rBV	2071919	2624640	97.23%	10.321%
96	19.939	2880	2882	2887	rBV4	12164	13286	0.49%	0.052%
97	20.892	3041	3044	3051	rBV3	62994	105333	3.90%	0.414%
98	21.163	3085	3090	3101	rBV	1122396	1486999	55.08%	5.848%
99	23.321	3450	3457	3465	rBV	1427546	2699499	100.00%	10.616%
100	23.474	3476	3483	3491	rVB2	745919	1478564	54.77%	5.814%




Sum of corrected areas: 25429371

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011388.D
Acq On : 11 Aug 2022 15:36
Operator : CG/JU
Sample : N4128-16
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGC10

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

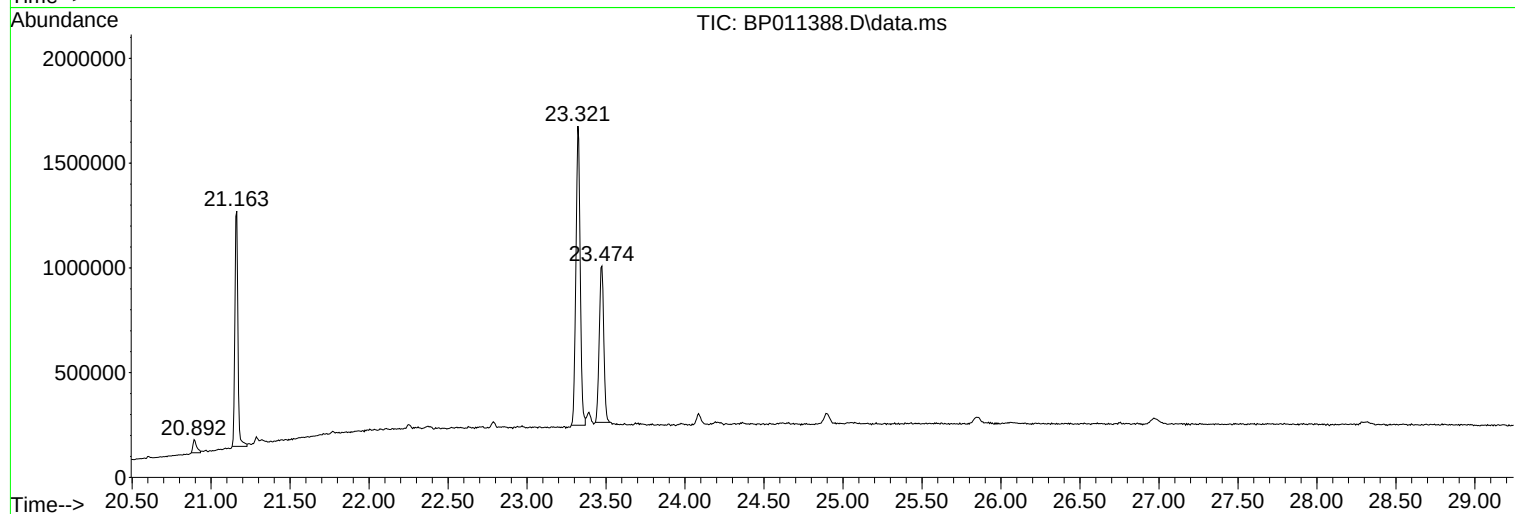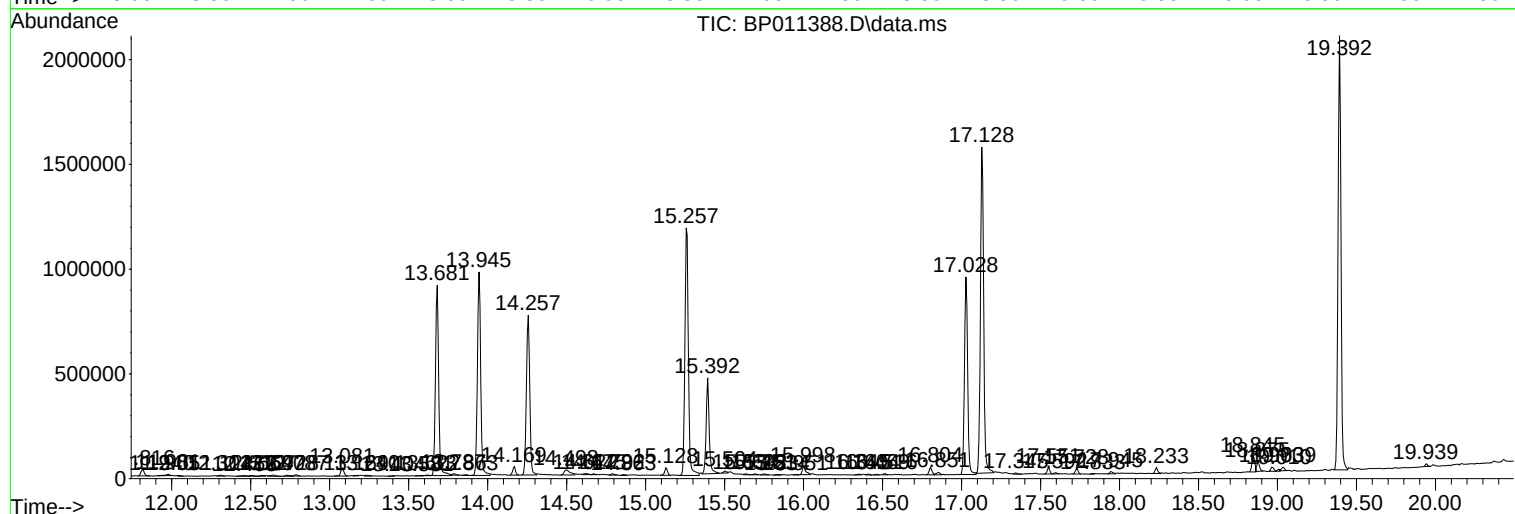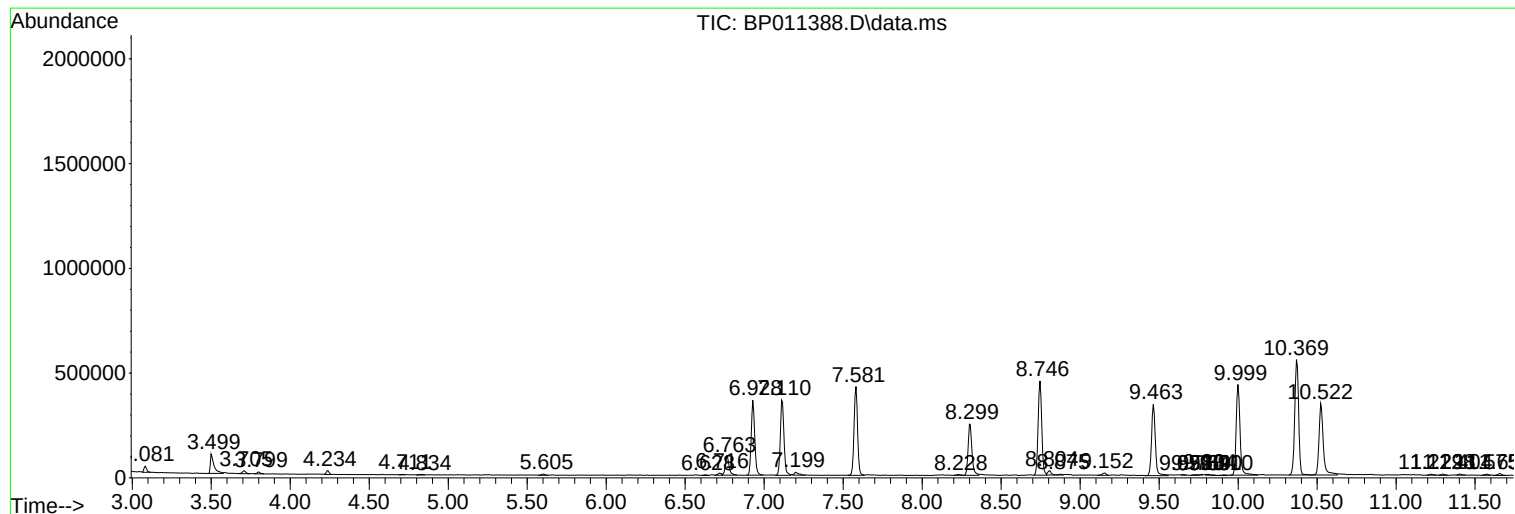

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011388.D
Acq On : 11 Aug 2022 15:36
Operator : CG/JU
Sample : N4128-16
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGC10

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011388.D
Acq On : 11 Aug 2022 15:36
Operator : CG/JU
Sample : N4128-16
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGC10

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc