

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011389.D
 Acq On : 11 Aug 2022 16:11
 Operator : CG/JU
 Sample : N4128-17
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBT3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011389.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.081	12	16	25	rVB	32078	43482	1.85%	0.186%
2	3.499	84	87	106	rBV	96556	160326	6.80%	0.685%
3	3.711	118	123	130	rVB	16265	24334	1.03%	0.104%
4	3.799	135	138	144	rVB	10729	15610	0.66%	0.067%
5	4.240	208	213	219	rVB	22757	33384	1.42%	0.143%
6	4.711	290	293	300	rVB5	2968	4495	0.19%	0.019%
7	4.828	309	313	320	rBV10	3660	6946	0.29%	0.030%
8	5.593	439	443	448	rBV8	2081	4513	0.19%	0.019%
9	6.040	515	519	522	rBV5	1488	2461	0.10%	0.011%
10	6.716	629	634	637	rBV2	11179	16688	0.71%	0.071%
11	6.763	637	642	655	rVB	92989	154571	6.56%	0.661%
12	6.928	664	670	681	rBV	354589	542831	23.04%	2.320%
13	7.110	693	701	713	rBV	357117	572195	24.28%	2.445%
14	7.199	714	716	721	rVB5	4011	5254	0.22%	0.022%
15	7.581	774	781	790	rBV	418600	642295	27.26%	2.745%
16	7.669	792	796	799	rVB6	2015	2774	0.12%	0.012%
17	8.299	896	903	917	rBV2	245603	425882	18.07%	1.820%
18	8.746	971	979	994	rBV	437207	711247	30.18%	3.040%
19	8.875	998	1001	1006	rVV6	3652	5778	0.25%	0.025%
20	9.152	1042	1048	1055	rBV2	14374	22488	0.95%	0.096%
21	9.463	1093	1101	1116	rBV	336624	550358	23.36%	2.352%
22	9.999	1184	1192	1213	rBV	422683	729875	30.97%	3.119%
23	10.369	1246	1255	1264	rBV	549261	887403	37.66%	3.792%
24	10.522	1275	1281	1297	rBV	359833	661049	28.05%	2.825%
25	11.657	1469	1474	1481	rVB3	9672	15527	0.66%	0.066%
26	11.987	1522	1530	1538	rBV3	8074	16856	0.72%	0.072%
27	13.040	1704	1709	1711	rBV6	1580	2664	0.11%	0.011%
28	13.157	1723	1729	1733	rBV8	2132	4074	0.17%	0.017%
29	13.222	1736	1740	1745	rBV7	2674	4057	0.17%	0.017%
30	13.681	1809	1818	1832	rBV	894571	1251682	53.12%	5.349%
31	13.792	1835	1837	1847	rVB10	3053	7448	0.32%	0.032%
32	13.945	1855	1863	1879	rBV	921919	1359579	57.70%	5.810%
33	14.257	1909	1916	1927	rBV	744780	1062116	45.07%	4.539%
34	14.328	1927	1928	1932	rVB4	3353	2974	0.13%	0.013%
35	14.498	1952	1957	1968	rBV4	23776	65187	2.77%	0.279%
36	15.075	2052	2055	2058	rBV5	1745	2460	0.10%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
 Data File : BP011389.D
 Acq On : 11 Aug 2022 16:11
 Operator : CG/JU
 Sample : N4128-17
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGBT3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
 Title : SVOA CALIBRATION

37	15.128	2062	2064	2068	rVB4	2820	3319	0.14%	0.014%
38	15.257	2079	2086	2102	rBV	1158279	1741515	73.90%	7.443%
39	15.392	2103	2109	2124	rVV	427235	605662	25.70%	2.588%
40	15.504	2124	2128	2133	rVB3	13250	22459	0.95%	0.096%
41	15.686	2156	2159	2161	rBV4	1839	2440	0.10%	0.010%
42	15.834	2180	2184	2185	rBV4	1880	2411	0.10%	0.010%
43	15.951	2200	2204	2207	rBV5	2449	4295	0.18%	0.018%
44	15.998	2207	2212	2219	rVV4	7675	16815	0.71%	0.072%
45	16.057	2219	2222	2226	rVB6	3771	5499	0.23%	0.024%
46	16.169	2238	2241	2246	rBV7	2375	4336	0.18%	0.019%
47	16.516	2293	2300	2305	rVB4	6540	11161	0.47%	0.048%
48	16.710	2329	2333	2337	rVB7	1937	3160	0.13%	0.014%
49	16.810	2345	2350	2354	rBV7	4507	7782	0.33%	0.033%
50	17.028	2381	2387	2398	rBV	916302	1254683	53.24%	5.362%
51	17.128	2398	2404	2422	rVV	1413697	2062051	87.51%	8.812%
52	17.333	2436	2439	2446	rVB8	2366	5108	0.22%	0.022%
53	17.598	2480	2484	2490	rVB3	5061	8044	0.34%	0.034%
54	17.728	2502	2506	2510	rVB7	2866	4037	0.17%	0.017%
55	17.945	2540	2543	2547	rBV5	4854	8022	0.34%	0.034%
56	18.016	2553	2555	2561	rVB3	4368	5726	0.24%	0.024%
57	18.410	2619	2622	2627	rBV7	2486	4310	0.18%	0.018%
58	18.522	2638	2641	2647	rVB5	5110	6915	0.29%	0.030%
59	18.963	2712	2716	2721	rBV4	17307	25881	1.10%	0.111%
60	19.039	2725	2729	2734	rVV3	16867	25617	1.09%	0.109%
61	19.392	2783	2789	2797	rBV	1917935	2356487	100.00%	10.071%
62	20.892	3041	3044	3051	rBV3	47073	83595	3.55%	0.357%
63	21.163	3085	3090	3104	rBV	1036843	1393609	59.14%	5.956%
64	23.321	3451	3457	3465	rBV2	1264349	2332540	98.98%	9.968%
65	23.468	3476	3482	3493	rVB2	716942	1371095	58.18%	5.860%




Sum of corrected areas: 23399437

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011389.D
Acq On : 11 Aug 2022 16:11
Operator : CG/JU
Sample : N4128-17
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBT3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

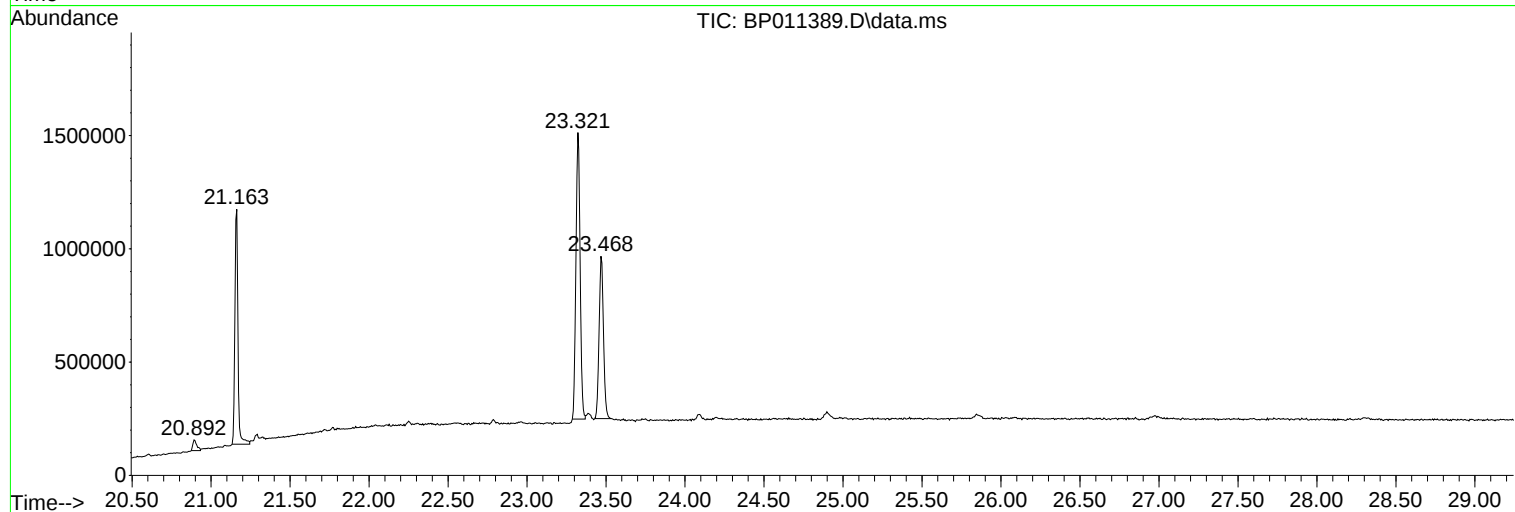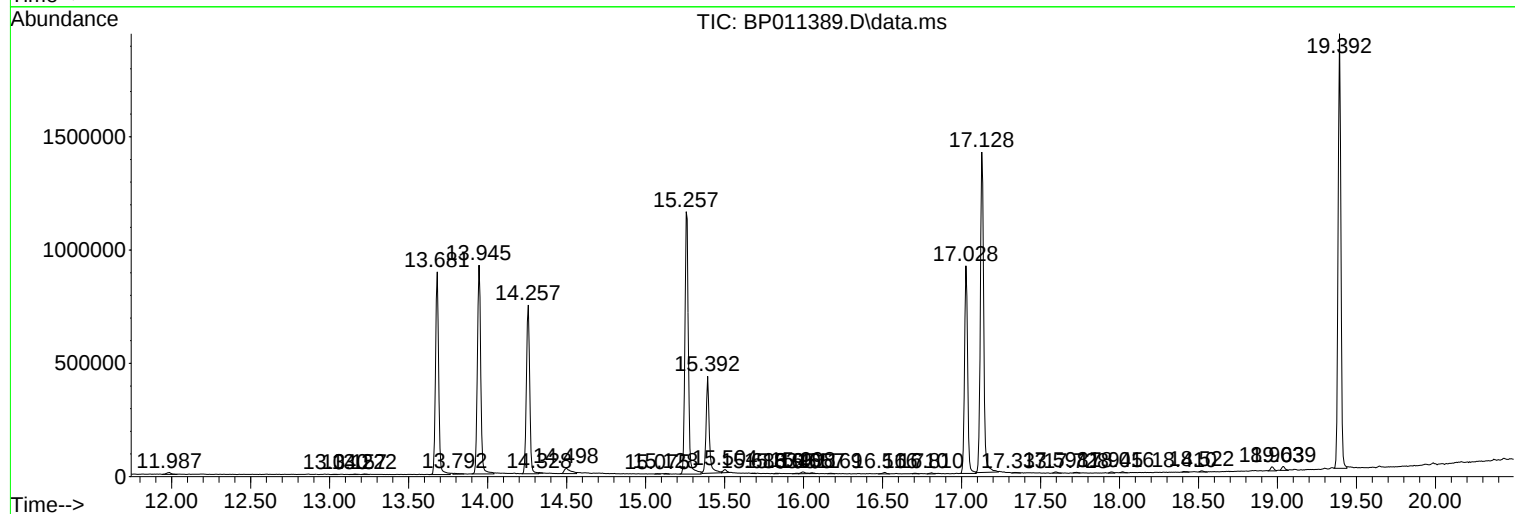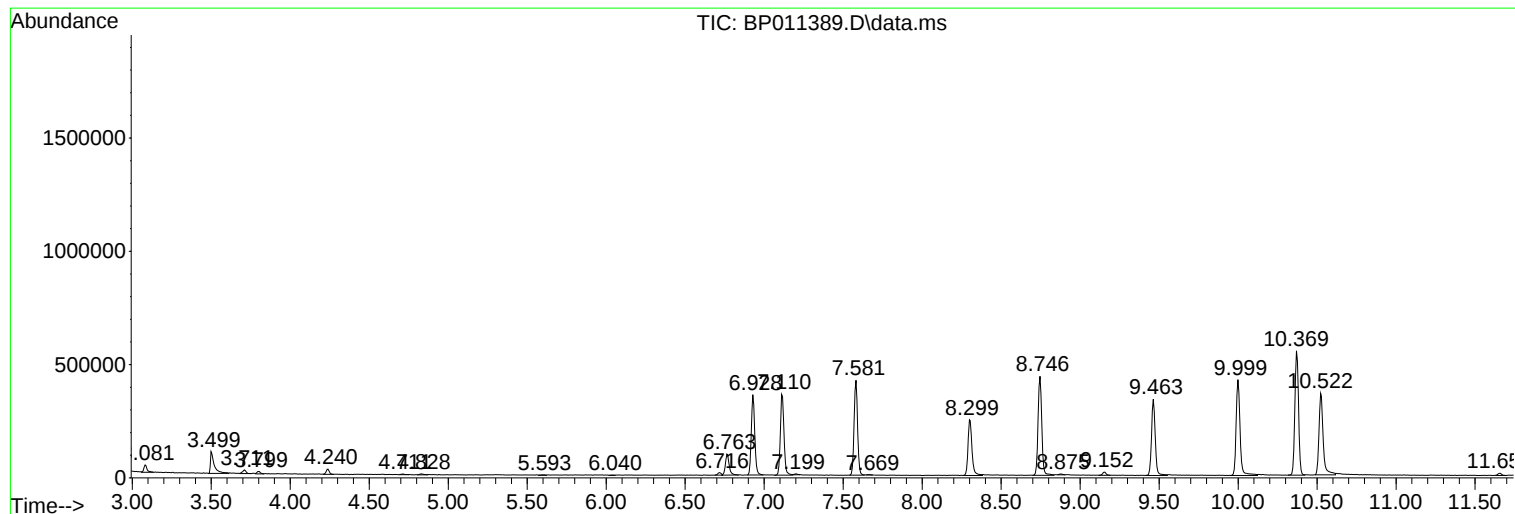

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011389.D
Acq On : 11 Aug 2022 16:11
Operator : CG/JU
Sample : N4128-17
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBT3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081122\
Data File : BP011389.D
Acq On : 11 Aug 2022 16:11
Operator : CG/JU
Sample : N4128-17
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGBT3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP080822.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc